
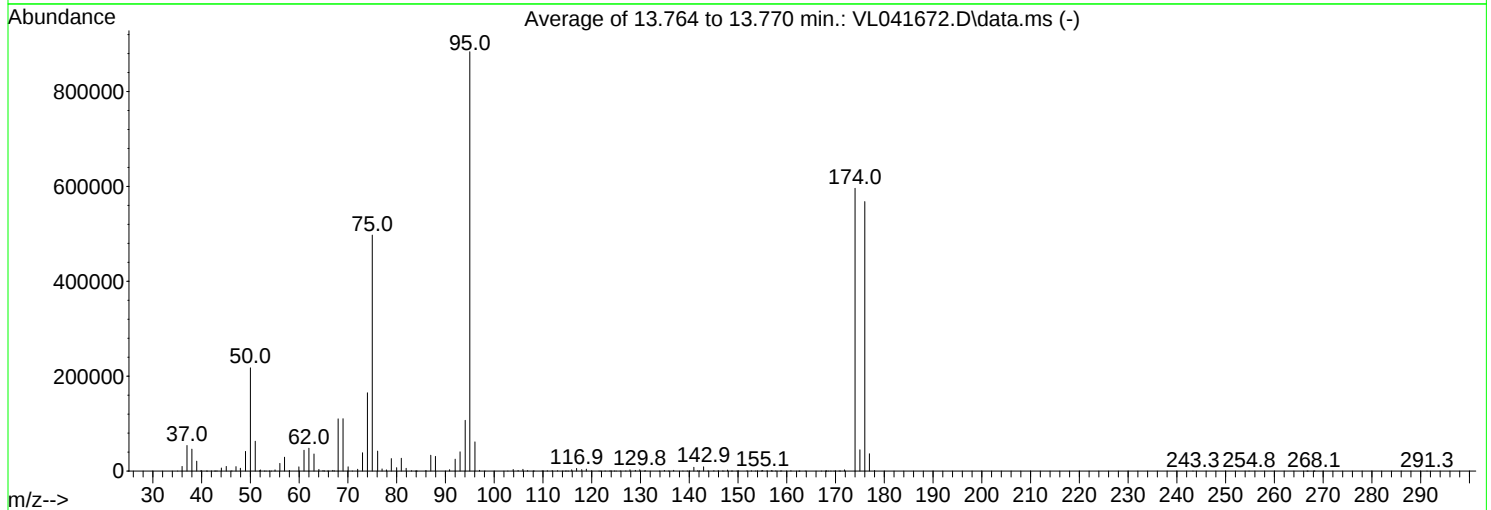


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL110724\
Data File : VL041672.D
Acq On : 7 Nov 2024 8:58
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL110724AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Nov 08 01:01:00 2024

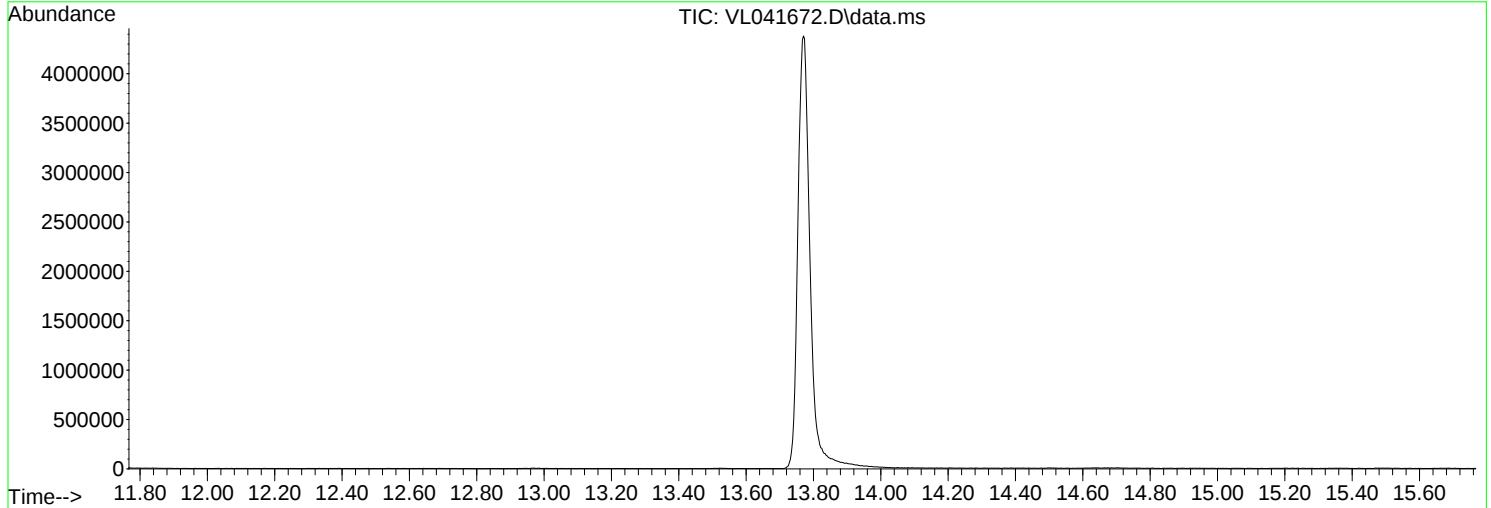

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.6	217600	PASS
75	95	30	66	56.3	497408	PASS
95	95	100	100	100.0	883883	PASS
96	95	5	9	7.0	61491	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.4	595968	PASS
175	174	4	9	7.5	44800	PASS
176	174	93	101	95.3	567979	PASS
177	176	5	9	6.4	36571	PASS

Average of 13.764 to 13.770 min.: VL041672.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	73	42.90	160	52.05	2414	62.00	48165
36.00	9800	43.15	438	52.90	207	63.05	36043
37.00	53912	44.05	6471	53.20	127	64.05	3591
38.00	46298	45.05	9806	53.90	291	64.90	1238
39.00	20824	46.20	540	54.30	110	65.20	527
39.80	346	47.05	9443	55.05	2517	65.85	154
40.00	522	47.95	6008	56.05	16198	66.10	247
41.00	219	49.00	41491	57.00	29283	66.90	1514
41.20	83	50.00	217600	58.00	1270	67.20	860
42.00	89	51.00	62976	59.95	8864	68.00	110088
42.70	136	51.90	858	61.00	43893	69.00	110461

Average of 13.764 to 13.770 min.: VL041672.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
70.05	8980	80.95	27016	94.05	106912	109.85	466
70.90	162	81.95	5922	95.00	883883	110.10	130
72.00	3884	83.05	863	96.05	61491	110.90	823
73.00	38651	83.90	55	97.00	1641	111.90	1050
74.00	165013	84.20	76	98.10	117	113.00	875
75.00	497408	86.00	1307	102.80	238	114.10	70
76.10	42112	87.00	33435	103.90	3328	114.60	206
77.00	4531	87.95	31005	104.90	1372	114.90	345
77.90	2531	90.85	2943	105.90	3759	115.20	89
78.90	26355	92.00	25072	106.85	1024	115.90	2598
80.00	7190	93.00	40613	108.00	52	116.90	5548

Average of 13.764 to 13.770 min.: VL041672.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.95	3063	127.00	433	139.60	382	147.85	2191
118.90	4179	127.85	2804	140.10	233	148.65	246
120.00	357	128.95	1493	140.95	8040	148.90	188
121.50	65	129.85	2901	141.75	896	149.80	171
121.75	128	130.80	371	142.10	442	150.05	609
122.75	374	131.00	858	142.95	9074	151.85	592
123.75	579	133.90	111	143.85	508	152.75	767
124.00	195	134.90	1463	145.05	998	153.65	267
124.65	305	135.80	288	145.95	884	154.00	439
125.00	83	136.80	1606	146.85	428	154.80	660
125.85	285	138.70	276	147.10	214	155.05	1381

Average of 13.764 to 13.770 min.: VL041672.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.95	665	168.20	131	176.95	36571		
156.85	1255	168.60	124	178.00	1029		
157.10	475	169.05	151	243.30	71		
157.75	414	169.70	102	254.80	102		
158.70	330	170.00	84	266.70	53		
158.95	563	170.75	470	268.10	56		
160.85	864	171.00	228	291.30	67		
162.50	60	171.85	2678				
163.80	79	174.00	595968				
167.10	130	175.00	44800				
168.00	53	176.00	567979				

Instrument :

MSVOA_L

ClientSampleId :

BFB