

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	P4699	OrderDate:	11/4/2024 12:02:00 PM
Client:	EarthEfficient LLC	Project:	120-122 Liberty Ave BK
Contact:	Environmental Team	Location:	K21

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
P4699-01	MIXED-DEMO	SOIL	PCB	8082A	11/04/24	11/05/24	11/05/24	11/04/24



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: P4699

Order ID: P4699

Client: EarthEfficient LLC

Project ID: 120-122 Liberty Ave BK

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: **P4699**

Client: **EarthEfficient LLC**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PO107183.D	PIBLK-PO107183.D	Tetrachloro-m-xylene	1	20	22.5	112		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	23.4	117		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	22.1	110		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	22.8	114		70 (60)	130 (140)
I.BLK-PO107686.D	PIBLK-PO107686.D	Tetrachloro-m-xylene	1	20	20.7	104		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	21.3	107		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	21.1	105		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	21.0	105		70 (60)	130 (140)
PB164678BL	PB164678BL	Tetrachloro-m-xylene	1	20	20.9	104		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	21.7	108		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	21.1	106		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	21.4	107		30 (32)	150 (175)
PB164678BS	PB164678BS	Tetrachloro-m-xylene	1	20	21.3	107		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	21.9	109		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	20.2	101		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	21.6	108		30 (32)	150 (175)
I.BLK-PO107701.D	PIBLK-PO107701.D	Tetrachloro-m-xylene	1	20	21.0	105		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	21.0	105		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	21.5	107		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	20.9	105		70 (60)	130 (140)
P4699-01	MIXED-DEMO	Tetrachloro-m-xylene	1	20	22.8	114		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	21.9	110		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	23.2	116		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	22.2	111		30 (32)	150 (175)
P4701-01MS	BP-F3MS	Tetrachloro-m-xylene	1	20	24.7	123		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	21.5	107		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	24.4	122		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	21.9	109		30 (32)	150 (175)
P4701-01MSD	BP-F3MSD	Tetrachloro-m-xylene	1	20	23.5	117		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	21.7	109		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	24.8	124		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	21.7	109		30 (32)	150 (175)
I.BLK-PO107715.D	PIBLK-PO107715.D	Tetrachloro-m-xylene	1	20	21.7	109		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	22.0	110		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	22.0	110		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	23.1	115		70 (60)	130 (140)

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P4699

Client: EarthEfficient LLC

Analytical Method: 8082A

DataFile : PO107706.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	BP-F3MS											
P4701-01MS	AR1016	199	0	236	ug/kg	119				40 (55)	140 (146)	
	AR1260	199	0	215	ug/kg	108				40 (45)	140 (144)	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P4699

Client: EarthEfficient LLC

Analytical Method: 8082A

DataFile : PO107707.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	BP-F3MSD											
P4701-01MSD	AR1016	198.9	0	244	ug/kg	123		3		40 (55)	140 (146)	30 (20)
	AR1260	198.9	0	220	ug/kg	111		3		40 (45)	140 (144)	30 (20)



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: P4699

Client: EarthEfficient LLC

Analytical Method: 8082A Datafile : PO107688.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB164678BS	AR1016	166.6	155	ug/kg	93				40 (71)	140 (120)	
	AR1260	166.6	156	ug/kg	94				40 (65)	140 (130)	

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB164678BL

Lab Name: CHEMTECH

Contract: EART12

Lab Code: CHEM Case No.: P4699

SAS No.: P4699 SDG NO.: P4699

Lab Sample ID: PB164678BL

Lab File ID: PO107687.D

Matrix: (soil/water) Solid

Extraction: (Type) _____

Sulfur Cleanup: (Y/N) N

Date Extracted: 11/05/2024

Date Analyzed (1): 11/05/2024

Date Analyzed (2): 11/05/2024

Time Analyzed (1): 15:00

Time Analyzed (2): 15:00

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB164678BS	PB164678BS	PO107688.D	11/05/2024	11/05/2024
MIXED-DEMO	P4699-01	PO107703.D	11/05/2024	11/05/2024
BP-F3MS	P4701-01MS	PO107706.D	11/05/2024	11/05/2024
BP-F3MSD	P4701-01MSD	PO107707.D	11/05/2024	11/05/2024

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	11/04/24
Project:	120-122 Liberty Ave BK	Date Received:	11/04/24
Client Sample ID:	MIXED-DEMO	SDG No.:	P4699
Lab Sample ID:	P4699-01	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	99.5
Sample Wt/Vol:	30.02	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107703.D	1	11/05/24 08:35	11/05/24 19:53	PB164678

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	3.40	U	3.40	17.1	ug/kg
11104-28-2	Aroclor-1221	6.40	U	6.40	17.1	ug/kg
11141-16-5	Aroclor-1232	3.40	U	3.40	17.1	ug/kg
53469-21-9	Aroclor-1242	3.40	U	3.40	17.1	ug/kg
12672-29-6	Aroclor-1248	7.90	U	7.90	17.1	ug/kg
11097-69-1	Aroclor-1254	2.70	U	2.70	17.1	ug/kg
37324-23-5	Aroclor-1262	4.60	U	4.60	17.1	ug/kg
11100-14-4	Aroclor-1268	3.40	U	3.40	17.1	ug/kg
11096-82-5	Aroclor-1260	2.90	U	2.90	17.1	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	23.2		30 (32) - 150 (144)	116%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.2		30 (32) - 150 (175)	111%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 19:53
 Operator : YP/AJ
 Sample : P4699-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MIXED-DEMO

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:54:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.642	207.4E6	74527027	22.755	23.156
2) SA Decachlor...	10.073	8.639	53836584	60828494	21.944	22.187

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 19:53
Operator : YP/AJ
Sample : P4699-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MIXED-DEMO

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:54:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

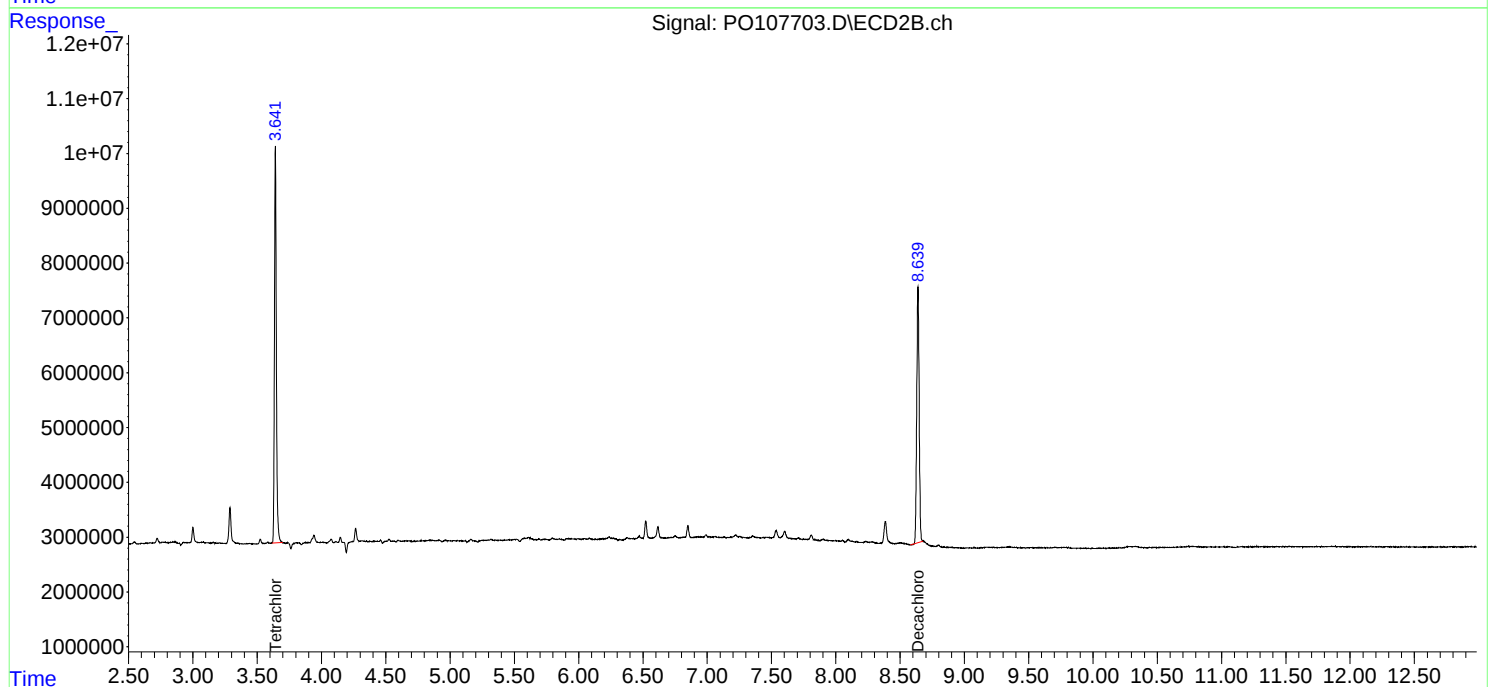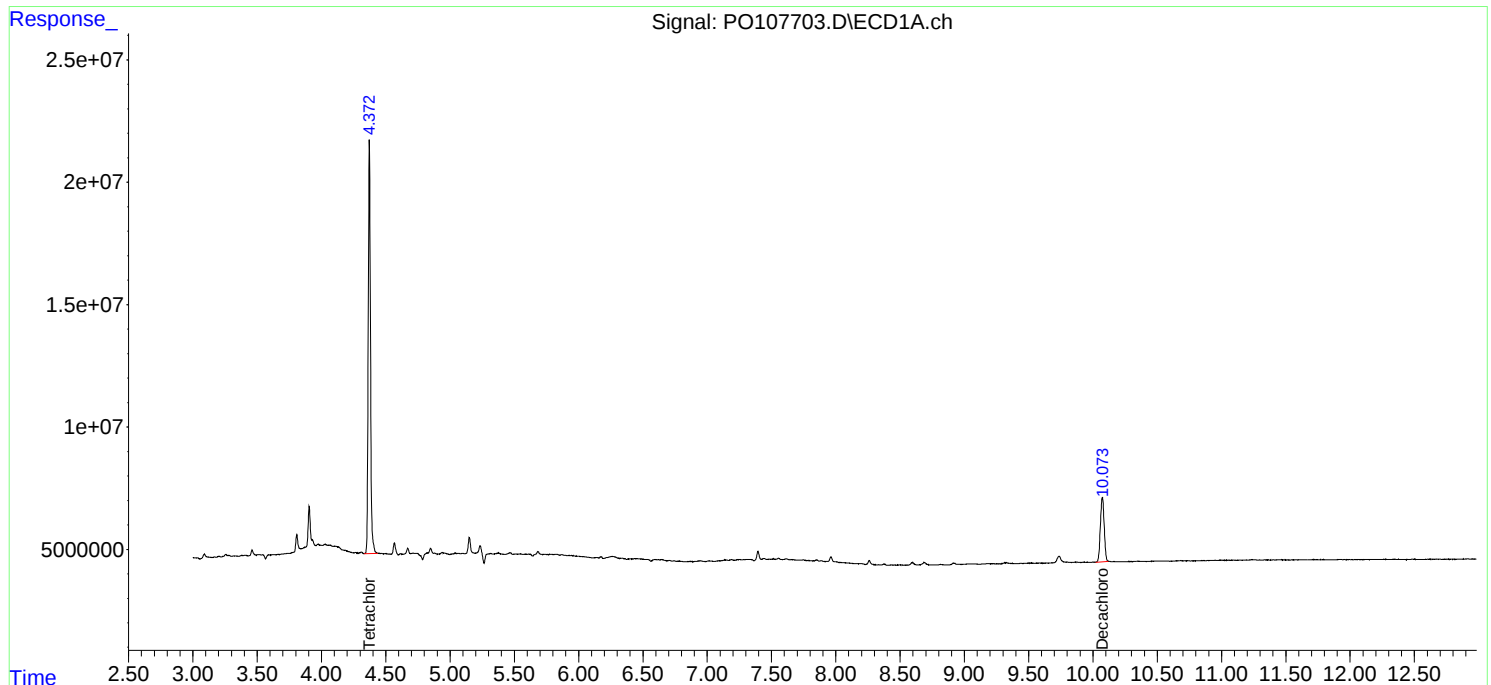


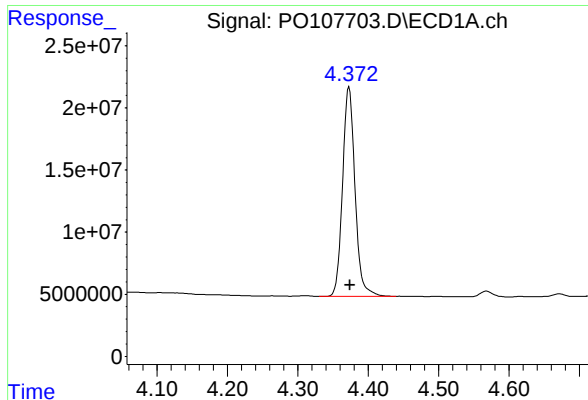

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: -0.001 min
Response: 207384475
Conc: 22.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MIXED-DEMO

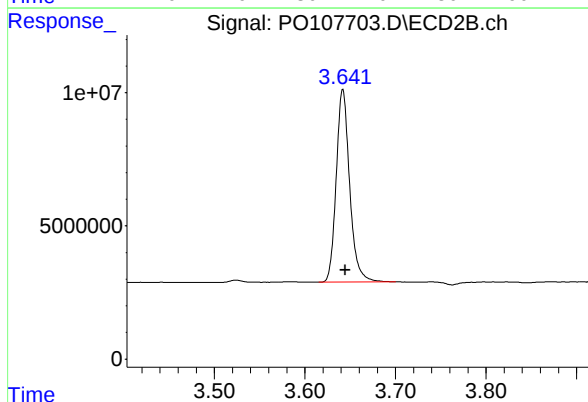


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.003 min
Response: 74527027
Conc: 23.16 ng/ml

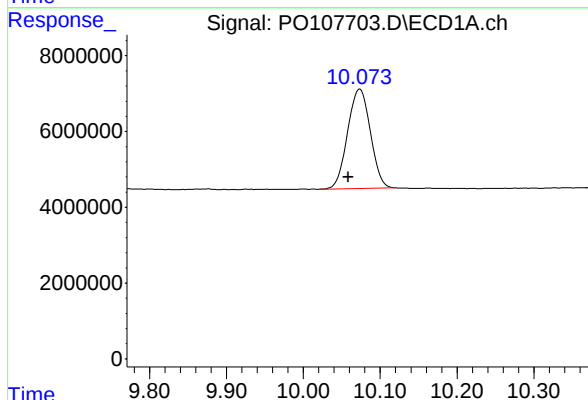

#2 Decachlorobiphenyl

R.T.: 10.073 min
Delta R.T.: 0.015 min
Response: 53836584
Conc: 21.94 ng/ml

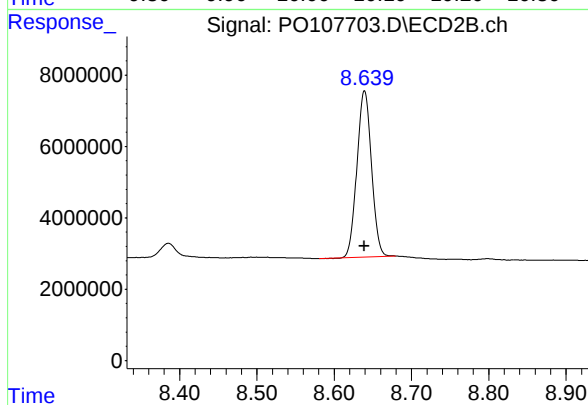

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 60828494
Conc: 22.19 ng/ml



CALIBRATION SUMMARY

RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>EART12</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>P4699</u>	SAS No.:	<u>P4699</u>	SDG NO.:	<u>P4699</u>
Instrument ID:	<u>ECD_O</u>	Calibration Date(s):		<u>10/15/2024</u>	<u>10/16/2024</u>		
		Calibration Times:		<u>18:27</u>	<u>02:36</u>		

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	<u>PO107184.D</u>	RT 750 =	<u>PO107185.D</u>
	RT 500 =	PO107186.D	RT 250 =	PO107187.D
			RT 050 =	PO107188.D

[illegible]

[illegible]

GC Column: ZB-MR2 ID: 0.32 (mm)

[illegible]

RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	8.64	8.64	8.64	8.64	8.64	8.64	8.54	8.74
Tetrachloro-m-xylene	3.65	3.64	3.65	3.64	3.65	3.65	3.55	3.75

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: EART12
Lab Code: CHEM **Case No.:** P4699 **SAS No.:** P4699 **SDG NO.:** P4699
Instrument ID: ECD_O
Calibration Date(s): 10/15/2024 10/16/2024
Calibration Times: 18:27 02:36
GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO107184.D</u>		CF 750 = <u>PO107185.D</u>			
CF 500 = <u>PO107186.D</u>		CF 250 = <u>PO107187.D</u>		CF 050 = <u>PO107188.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	252081604	261702867	271939076	291118488	272229420	269814291 5
Aroclor-1016-2	(2)	373760062	383028583	397887352	419075308	410673320	396884925 5
Aroclor-1016-3	(3)	234678633	244145249	256575754	276405664	244042480	251169556 6
Aroclor-1016-4	(4)	185622493	193848624	202963902	215081552	165543020	192611918 10
Aroclor-1016-5	(5)	176326470	182141932	191487930	203514892	159796500	182653545 9
Aroclor-1260-1	(1)	238480871	246497651	259155974	277220676	271587560	258588546 6
Aroclor-1260-2	(2)	243402558	251747185	264083512	284216460	272650860	263220115 6
Aroclor-1260-3	(3)	167353086	171560129	181491762	195138068	183182660	179745141 6
Aroclor-1260-4	(4)	162125557	166999933	175289716	187582032	185522120	175503872 6
Aroclor-1260-5	(5)	268686175	273623828	283035894	299271412	297351500	284393762 5
Decachlorobiphenyl		2362750210	2427138920	2496479000	2603827440	2376686800	2453376474 4
Tetrachloro-m-xylene		8902656430	9087809293	9285762860	9548006280	8745262400	9113899453 3
Aroclor-1242-1	(1)	207947063	205572916	222208808	238956456	243522880	223641625 8
Aroclor-1242-2	(2)	302439626	299949616	323550412	342804408	348858880	323520588 7
Aroclor-1242-3	(3)	191912697	193178427	209638152	224306728	225847640	208976729 8
Aroclor-1242-4	(4)	150447174	145338196	162797508	173135964	168308740	160005516 7
Aroclor-1242-5	(5)	141009343	143408436	153689098	164623016	179679780	156481935 10
Decachlorobiphenyl		2339420350	2427742867	2492700840	2551827400	2426410200	2447620331 3
Tetrachloro-m-xylene		8860043620	8651743680	9146784160	9504075440	9174828800	9067495140 4
Aroclor-1248-1	(1)	155913014	164800668	175191332	184609772	188867720	173876501 8
Aroclor-1248-2	(2)	222845576	238202488	253637968	270074056	280366620	253025342 9
Aroclor-1248-3	(3)	231904923	246233752	259706092	274388212	266197800	255686156 7
Aroclor-1248-4	(4)	237210289	246633865	260533272	272872732	271860120	257822056 6
Aroclor-1248-5	(5)	236273499	246591072	260733536	276314120	280304600	260043365 7
Decachlorobiphenyl		2339780580	2371533013	2504089680	2566158680	2396701200	2435652631 4
Tetrachloro-m-xylene		8719403610	9119992693	9358904180	9492784200	8995773400	9137371617 3
Aroclor-1254-1	(1)	246822697	256579683	264992242	286189960	289157060	268748328 7
Aroclor-1254-2	(2)	348120894	361641555	373031238	401237980	402995760	377405485 6
Aroclor-1254-3	(3)	336293322	345653409	355909306	378498460	372630440	357796987 5
Aroclor-1254-4	(4)	213138598	220171503	227187688	242530220	244046960	229414994 6
Aroclor-1254-5	(5)	194609638	201069208	205869028	220139672	216546640	207646837 5
Decachlorobiphenyl		2357746210	2401897693	2508594000	2601578200	2359367400	2445836701 4
Tetrachloro-m-xylene		8883763230	9164627320	9184369060	9508828480	8791509400	9106619498 3
Aroclor-1268-1	(1)	351862425	352413819	364622844	381760528	369380480	364008019 3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	313096403	314491445	324862806	339637696	320299560	322477582	3
Aroclor-1268-3	(3)	272236453	272760276	282620036	293538700	275661940	279363481	3
Aroclor-1268-4	(4)	112236308	111261111	114714594	116428084	101458340	111219687	5
Aroclor-1268-5	(5)	836674479	833098204	847063314	864357444	781067560	832452200	4
Decachlorobiphenyl		4074190590	4136234160	4241958160	4399826360	4004084600	4171258774	4
Tetrachloro-m-xylene		9139601460	8935957933	9311606620	9495189880	8951901000	9166851379	3

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: EART12
Lab Code: CHEM **Case No.:** P4699 **SAS No.:** P4699 **SDG NO.:** P4699
Instrument ID: ECD_O
Calibration Date(s): 10/15/2024 10/16/2024
Calibration Times: 18:27 02:36

GC Column: ZB-MR2 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO107184.D</u>		CF 750 = <u>PO107185.D</u>				
CF 500 = <u>PO107186.D</u>		CF 250 = <u>PO107187.D</u>		CF 050 = <u>PO107188.D</u>				
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1	(1)	98519363	99934743	102532802	106601384	108740020	103265662	4
Aroclor-1016-2	(2)	140533795	142751421	144315942	146877552	130360060	140967754	5
Aroclor-1016-3	(3)	75819146	77111448	78799028	81783348	80215260	78745646	3
Aroclor-1016-4	(4)	61532960	63413097	65607722	69564368	70423600	66108349	6
Aroclor-1016-5	(5)	78878086	80970861	83522668	86940988	80356660	82133853	4
Aroclor-1260-1	(1)	150450531	152030172	155131756	161942364	156218200	155154605	3
Aroclor-1260-2	(2)	173752920	181526657	184104290	189736236	151457920	176115605	8
Aroclor-1260-3	(3)	168454604	170292340	172108108	175991544	151894120	167748143	6
Aroclor-1260-4	(4)	143637024	144895129	147115166	150514212	137242140	144680734	3
Aroclor-1260-5	(5)	340738400	339782780	336796716	340391952	289493480	329440666	7
Decachlorobiphenyl		2730622670	2745732653	2784792900	2852828640	2594005000	2741596373	3
Tetrachloro-m-xylene		3312014480	3338472613	3349065240	3230716080	2862214000	3218496483	6
Aroclor-1242-1	(1)	80390662	80447493	83937762	87266896	86674240	83743411	4
Aroclor-1242-2	(2)	114487494	111266404	117741916	120667112	114031640	115638913	3
Aroclor-1242-3	(3)	61817452	60461905	64396992	66865868	63624080	63433259	4
Aroclor-1242-4	(4)	60582529	60636219	64384594	68045260	66598220	64049364	5
Aroclor-1242-5	(5)	73763103	75675432	77215916	80736528	80226620	77523520	4
Decachlorobiphenyl		2686985320	2764418280	2764436780	2798541920	2665265400	2735929540	2
Tetrachloro-m-xylene		3315724680	3241948653	3341198040	3335574400	2920075400	3230904235	6
Aroclor-1248-1	(1)	60218805	63038185	64879120	66667236	62402400	63441149	4
Aroclor-1248-2	(2)	85173308	89108361	93061950	96541480	93540340	91485088	5
Aroclor-1248-3	(3)	89257070	93226611	97377878	100891904	96212540	95393201	5
Aroclor-1248-4	(4)	105934439	110533117	114760412	117772688	111691080	112138347	4
Aroclor-1248-5	(5)	102828085	105359652	109801380	114217964	119140640	110269544	6
Decachlorobiphenyl		2669365810	2682497173	2791873700	2836714480	2679938000	2732077833	3
Tetrachloro-m-xylene		3278417600	3389239440	3425836480	3362184040	2965722400	3284279992	6
Aroclor-1254-1	(1)	159855276	163854537	165548332	171717704	162964860	164788142	3
Aroclor-1254-2	(2)	138468840	142269335	144546922	151325972	148203140	144962842	3
Aroclor-1254-3	(3)	227061110	231385951	232213406	238575248	218867080	229620559	3
Aroclor-1254-4	(4)	128242906	130249965	131325350	135207044	122091880	129423429	4
Aroclor-1254-5	(5)	191904554	195153152	195378104	201188864	171636600	191052255	6
Decachlorobiphenyl		2726927150	2738190720	2773447120	2836815760	2598739800	2734824110	3
Tetrachloro-m-xylene		3347799560	3397335627	3354246660	3362236280	2930639600	3278451545	6
Aroclor-1268-1	(1)	419191400	409991492	413863584	410849472	368955300	404570250	5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	389672996	380096764	383518208	378699872	334345600	373266688	6
Aroclor-1268-3	(3)	345284332	337828173	339535756	338755760	307004380	333681680	5
Aroclor-1268-4	(4)	129107993	127445005	127285362	129260796	113749480	125369727	5
Aroclor-1268-5	(5)	1049237500	1019311260	1017080130	996315476	856840280	987756929	8
Decachlorobiphenyl		4873889790	4739451973	4823511780	4890043960	4430545400	4751488581	4
Tetrachloro-m-xylene		3440286630	3329771373	3416104800	3331345720	2963806400	3296262985	6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Instrument ID: ECD_O Date(s) Analyzed: 10/15/2024 10/16/2024

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	4.57	4.47	4.67	110010000
		2	4.66	4.56	4.76	78836600
		3	4.73	4.63	4.83	234100000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.73	4.63	4.83	195844000
		2	5.26	5.16	5.36	103025000
		3	5.54	5.44	5.64	179001000
		4	5.70	5.60	5.80	90165400
		5	5.80	5.70	5.90	65903200
Aroclor-1262	500	1	7.74	7.64	7.84	245548000
		2	8.28	8.18	8.38	309420000
		3	8.59	8.49	8.69	209196000
		4	8.68	8.58	8.78	163066000
		5	9.32	9.22	9.42	102764000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Instrument ID: ECD_O Date(s) Analyzed: 10/15/2024 10/16/2024

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.86	3.76	3.96	34895600
		2	3.94	3.84	4.04	26624800
		3	4.02	3.92	4.12	81218600
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.02	3.92	4.12	67327000
		2	4.75	4.65	4.85	63205200
		3	4.92	4.82	5.02	34475000
		4	5.00	4.90	5.10	31466000
		5	5.18	5.08	5.28	33083400
Aroclor-1262	500	1	6.76	6.66	6.86	212876000
		2	7.26	7.16	7.36	363332000
		3	7.54	7.44	7.64	137384000
		4	7.61	7.51	7.71	264574000
		5	8.10	8.00	8.20	112833000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 18:27
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:24:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	890.3E6	331.2E6	95.874	98.894
2) SA Decachlor...	10.059	8.639	236.3E6	273.1E6	94.643	98.055
Target Compounds						
3) L1 AR-1016-1	5.521	4.726	252.1E6	98519363	926.978	960.857
4) L1 AR-1016-2	5.544	4.745	373.8E6	140.5E6	939.362	973.793
5) L1 AR-1016-3	5.606	4.921	234.7E6	75819146	914.656	962.184
6) L1 AR-1016-4	5.703	4.962	185.6E6	61532960	914.559	937.892
7) L1 AR-1016-5	5.998	5.175	176.3E6	78878086	920.823	944.391
31) L7 AR-1260-1	7.124	6.207	238.5E6	150.5E6	920.221	969.824
32) L7 AR-1260-2	7.381	6.393	243.4E6	173.8E6	921.688	943.774
33) L7 AR-1260-3	7.743	6.547	167.4E6	168.5E6	922.097	978.772
34) L7 AR-1260-4	7.967	7.018	162.1E6	143.6E6	924.901	976.358
35) L7 AR-1260-5	8.281	7.258	268.7E6	340.7E6	949.301	1011.703



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 18:27
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:24:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

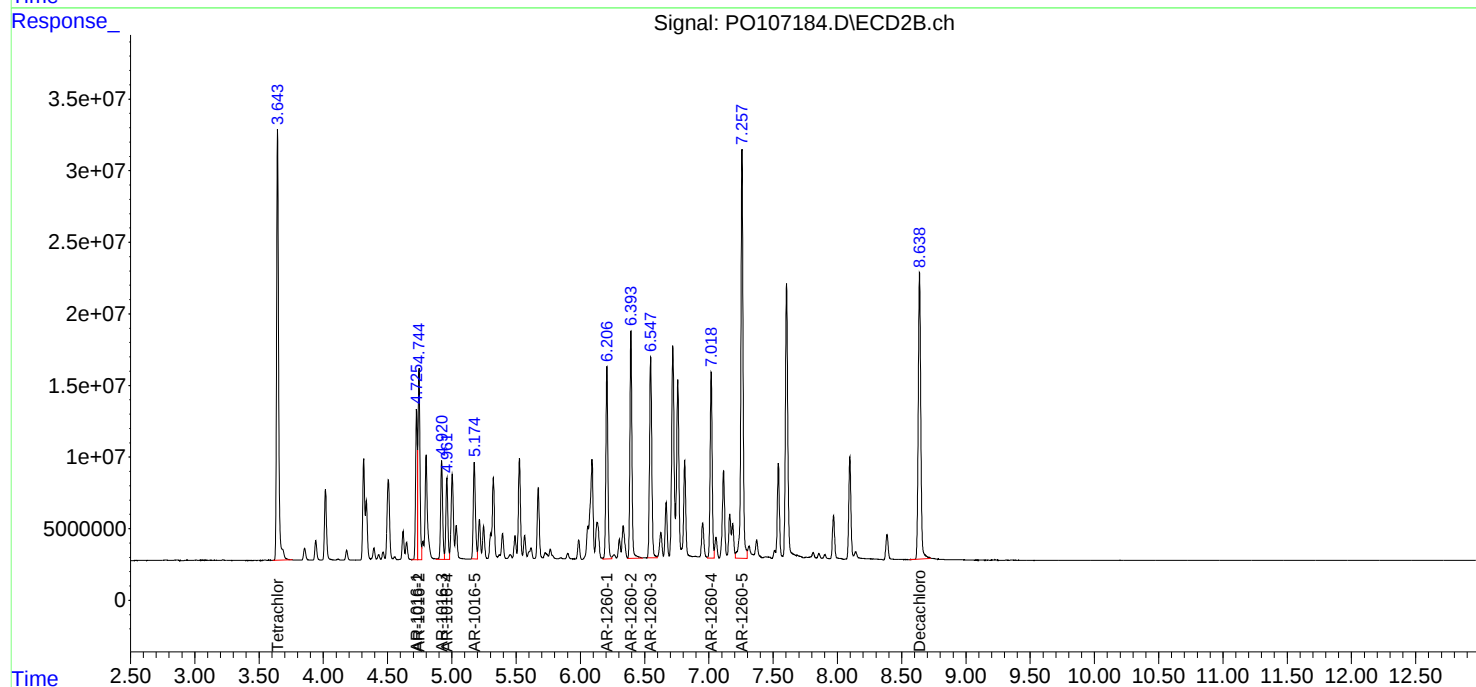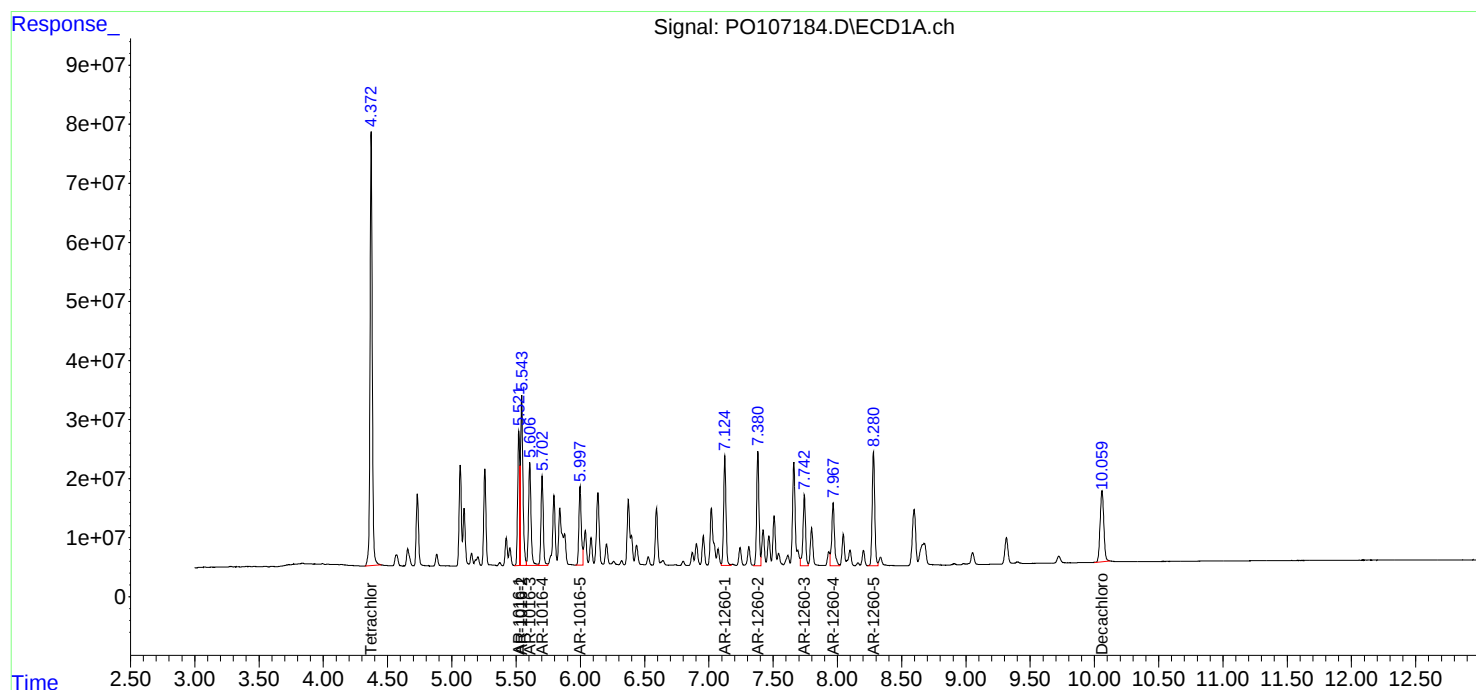

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 18:45
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:24:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.644	681.6E6	250.4E6	73.401	74.763
2) SA Decachlor...	10.059	8.639	182.0E6	205.9E6	72.917	73.948
Target Compounds						
3) L1 AR-1016-1	5.523	4.726	196.3E6	74951057	721.769	730.996
4) L1 AR-1016-2	5.545	4.745	287.3E6	107.1E6	721.992	741.869
5) L1 AR-1016-3	5.607	4.921	183.1E6	57833586	713.664	733.938
6) L1 AR-1016-4	5.704	4.962	145.4E6	47559823	716.317	724.912
7) L1 AR-1016-5	5.999	5.176	136.6E6	60728146	713.395	727.086
31) L7 AR-1260-1	7.125	6.207	184.9E6	114.0E6	713.367	735.005
32) L7 AR-1260-2	7.382	6.394	188.8E6	136.1E6	714.965	739.499
33) L7 AR-1260-3	7.743	6.548	128.7E6	127.7E6	708.958	742.087
34) L7 AR-1260-4	7.968	7.018	125.2E6	108.7E6	714.531	738.682
35) L7 AR-1260-5	8.281	7.258	205.2E6	254.8E6	725.060	756.650



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 18:45
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:24:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

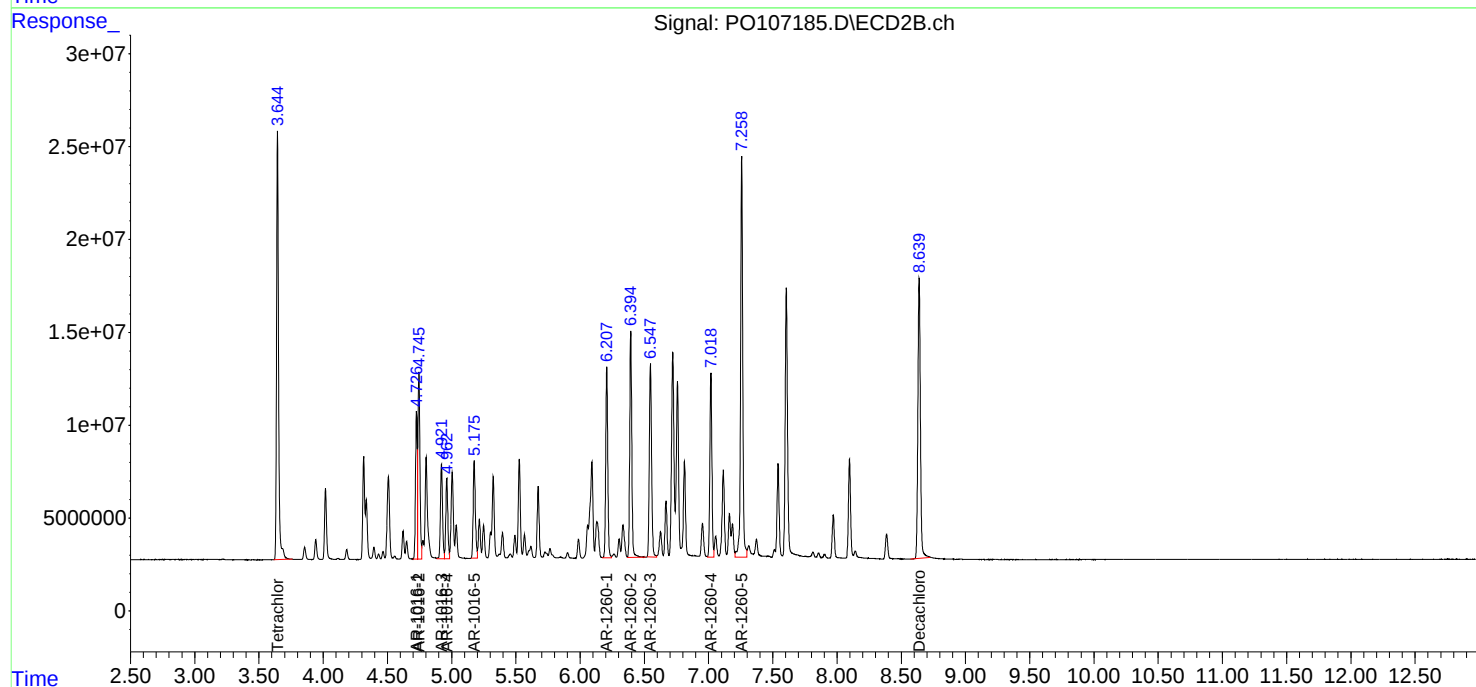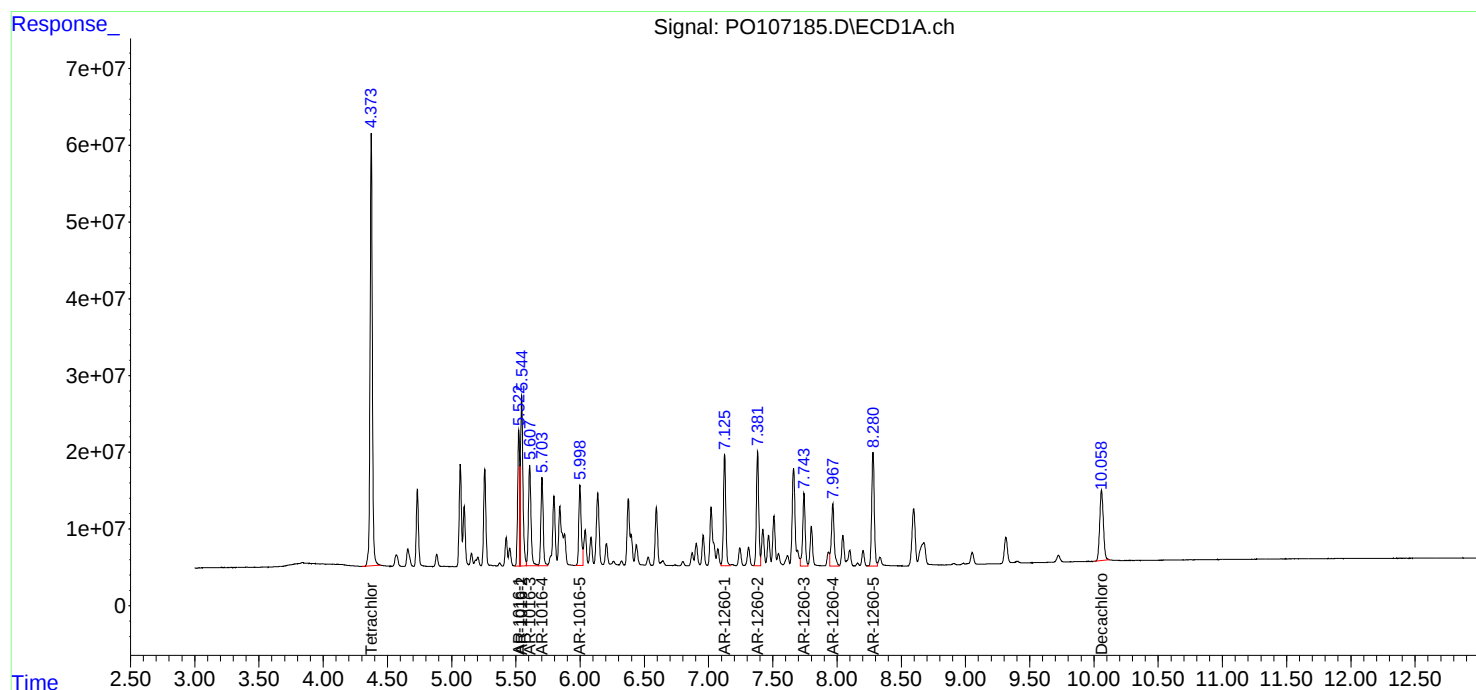

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 19:03
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:25:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.645	464.3E6	167.5E6	50.000	50.000
2) SA Decachlor...	10.058	8.639	124.8E6	139.2E6	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	5.523	4.726	136.0E6	51266401	500.000	500.000
4) L1 AR-1016-2	5.545	4.745	198.9E6	72157971	500.000	500.000
5) L1 AR-1016-3	5.607	4.921	128.3E6	39399514	500.000	500.000
6) L1 AR-1016-4	5.704	4.962	101.5E6	32803861	500.000	500.000
7) L1 AR-1016-5	5.999	5.176	95743965	41761334	500.000	500.000
31) L7 AR-1260-1	7.126	6.207	129.6E6	77565878	500.000	500.000
32) L7 AR-1260-2	7.382	6.394	132.0E6	92052145	500.000	500.000
33) L7 AR-1260-3	7.743	6.548	90745881	86054054	500.000	500.000
34) L7 AR-1260-4	7.968	7.018	87644858	73557583	500.000	500.000
35) L7 AR-1260-5	8.281	7.259	141.5E6	168.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 19:03
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:25:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

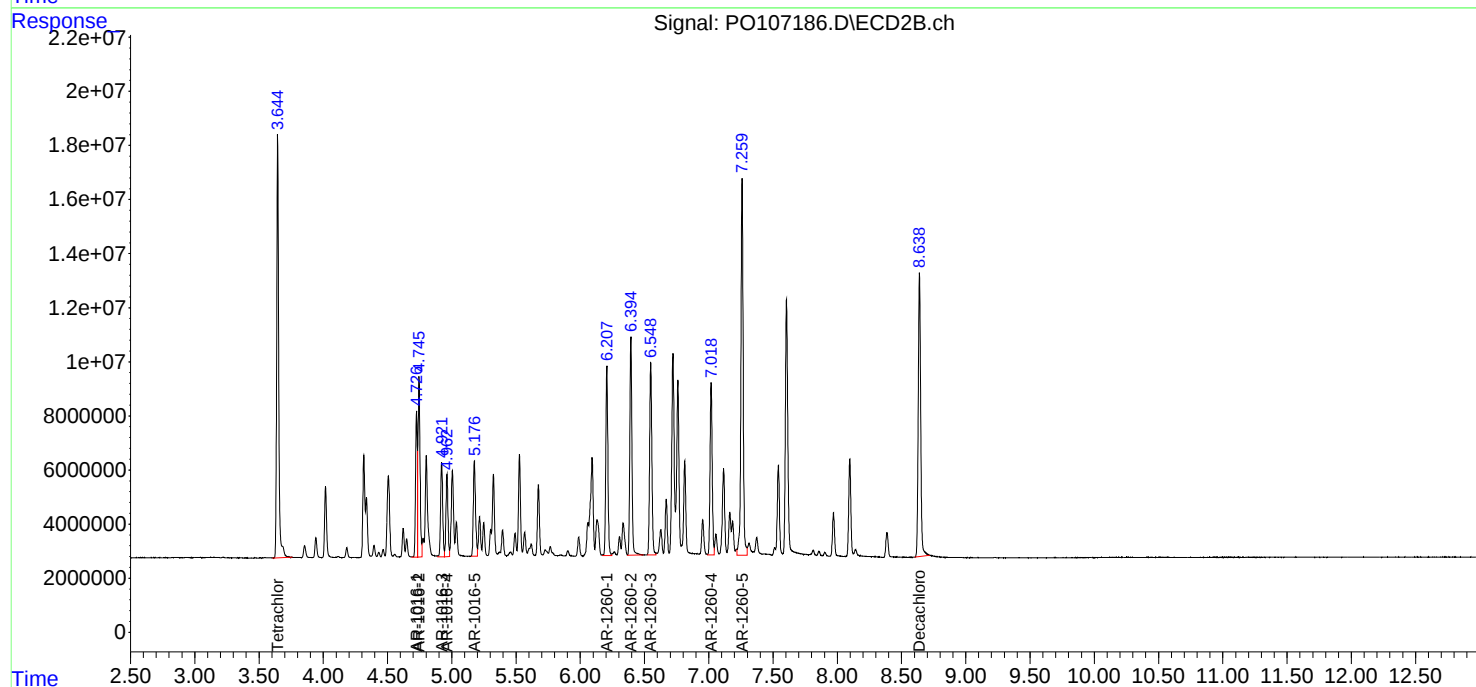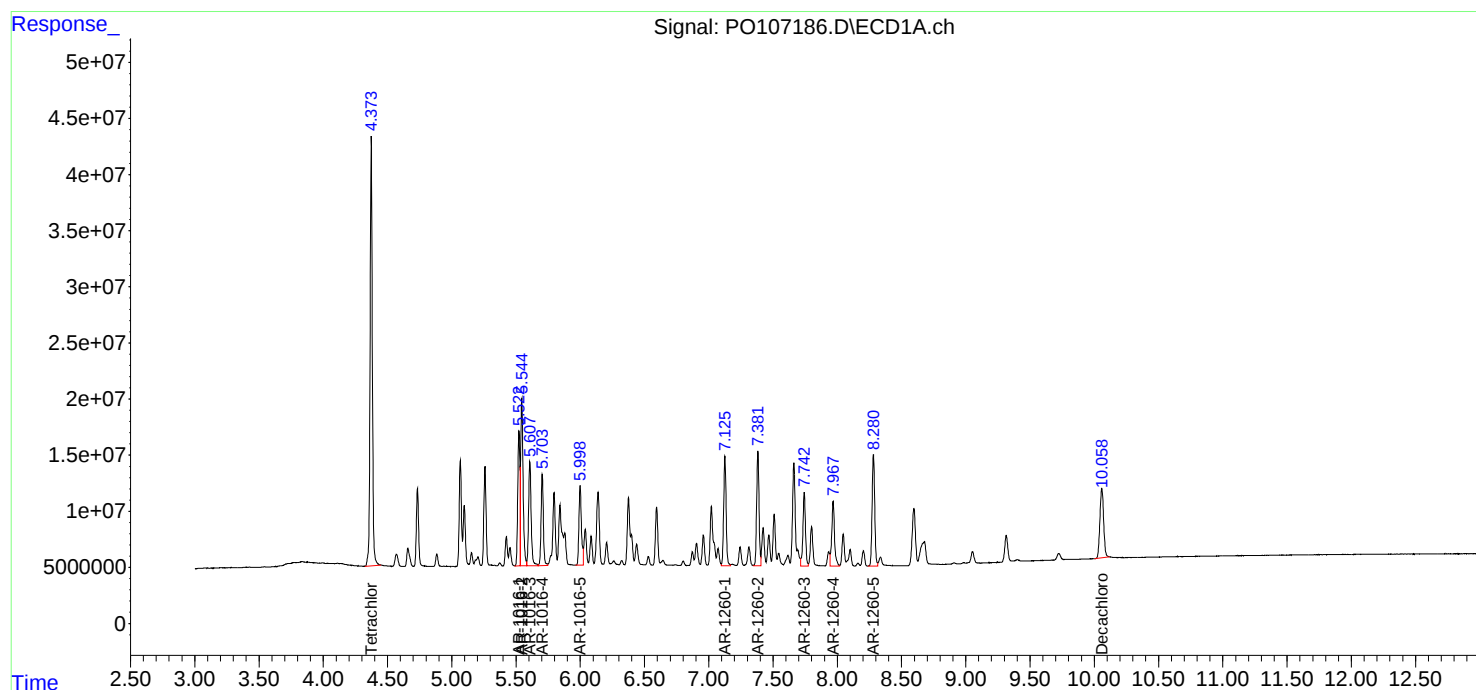

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 19:21
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:25:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	238.7E6	80767902	25.706	24.117
2) SA Decachlor...	10.059	8.640	65095686	71320716	26.075	25.611
Target Compounds						
3) L1 AR-1016-1	5.522	4.727	72779622	26650346	267.632	259.920
4) L1 AR-1016-2	5.544	4.746	104.8E6	36719388	263.313	254.438
5) L1 AR-1016-3	5.606	4.921	69101416	20445837	269.322	259.468
6) L1 AR-1016-4	5.704	4.962	53770388	17391092	264.926	265.077
7) L1 AR-1016-5	5.998	5.176	50878723	21735247	265.702	260.232
31) L7 AR-1260-1	7.124	6.207	69305169	40485591	267.426	260.976
32) L7 AR-1260-2	7.381	6.394	71054115	47434059	269.059	257.648
33) L7 AR-1260-3	7.743	6.548	48784517	43997886	268.797	255.641
34) L7 AR-1260-4	7.966	7.018	46895508	37628553	267.531	255.776
35) L7 AR-1260-5	8.281	7.259	74817853	85097988	264.341	252.669



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 19:21
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:25:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

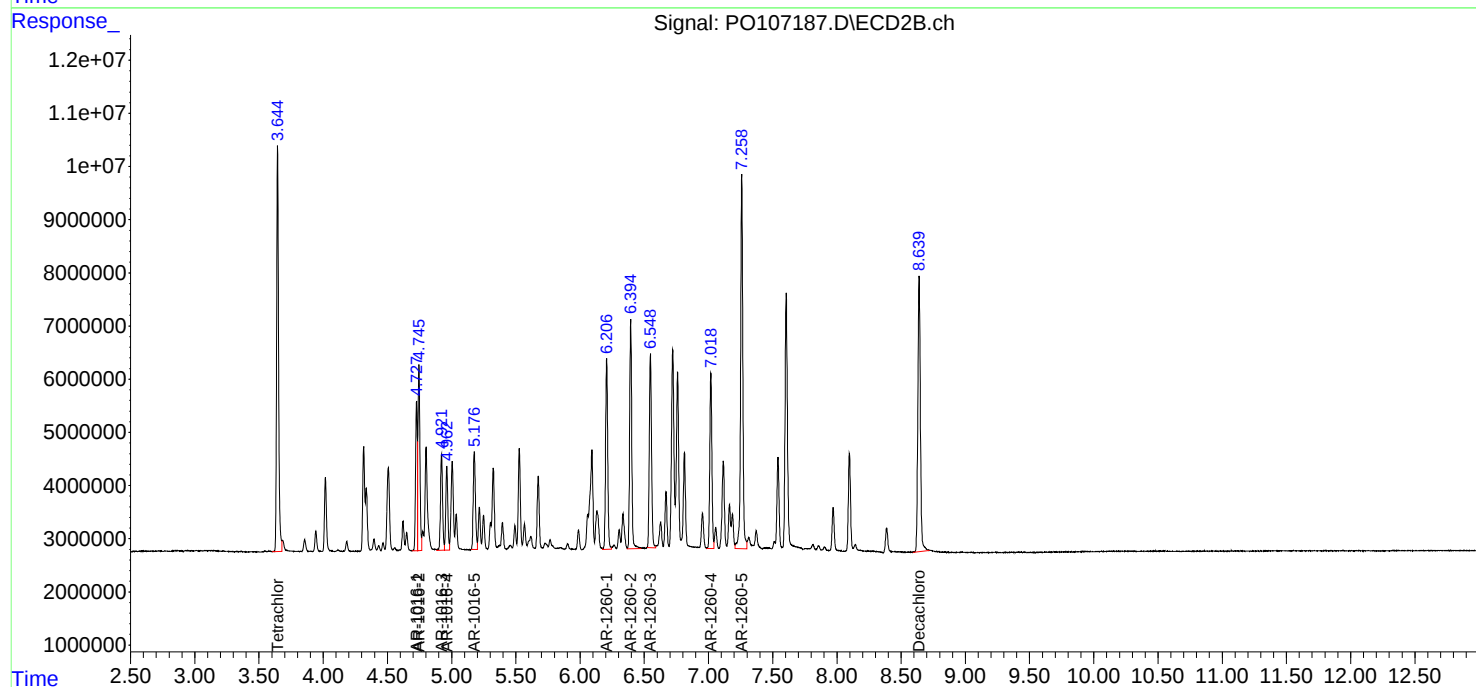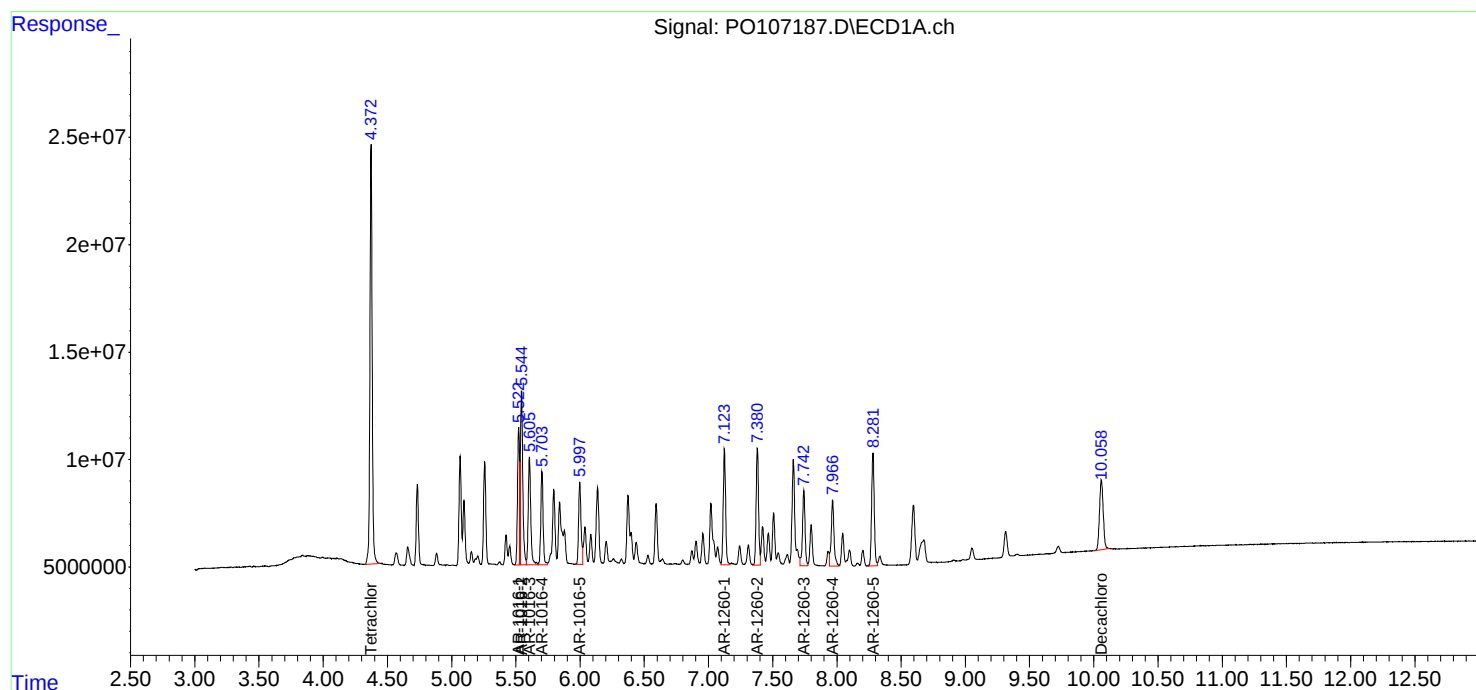

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 19:39
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/16/2024
 Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:26:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.644	43726312	14311070	4.709	4.273
2) SA Decachlor...	10.060	8.639	11883434	12970025	4.760	4.657m
Target Compounds						
3) L1 AR-1016-1	5.523	4.727	13611471	5437001	50.053	53.027
4) L1 AR-1016-2	5.544	4.745	20533666	6518003	51.607	45.165
5) L1 AR-1016-3	5.607	4.922	12202124	4010763	47.558	50.899
6) L1 AR-1016-4	5.704	4.963	8277151	3521180	40.781	53.670 #
7) L1 AR-1016-5	5.999	5.176	7989825	4017833	41.725	48.105
31) L7 AR-1260-1	7.125	6.207	13579378	7810910	52.398	50.350m
32) L7 AR-1260-2	7.380	6.395	13632543	7572896	51.622m	41.134m
33) L7 AR-1260-3	7.743	6.548	9159133	7594706	50.466m	44.128m
34) L7 AR-1260-4	7.967	7.019	9276106	6862107	52.919	46.644m
35) L7 AR-1260-5	8.280	7.258	14867575	14474674	52.529m	42.977m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 19:39
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:26:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

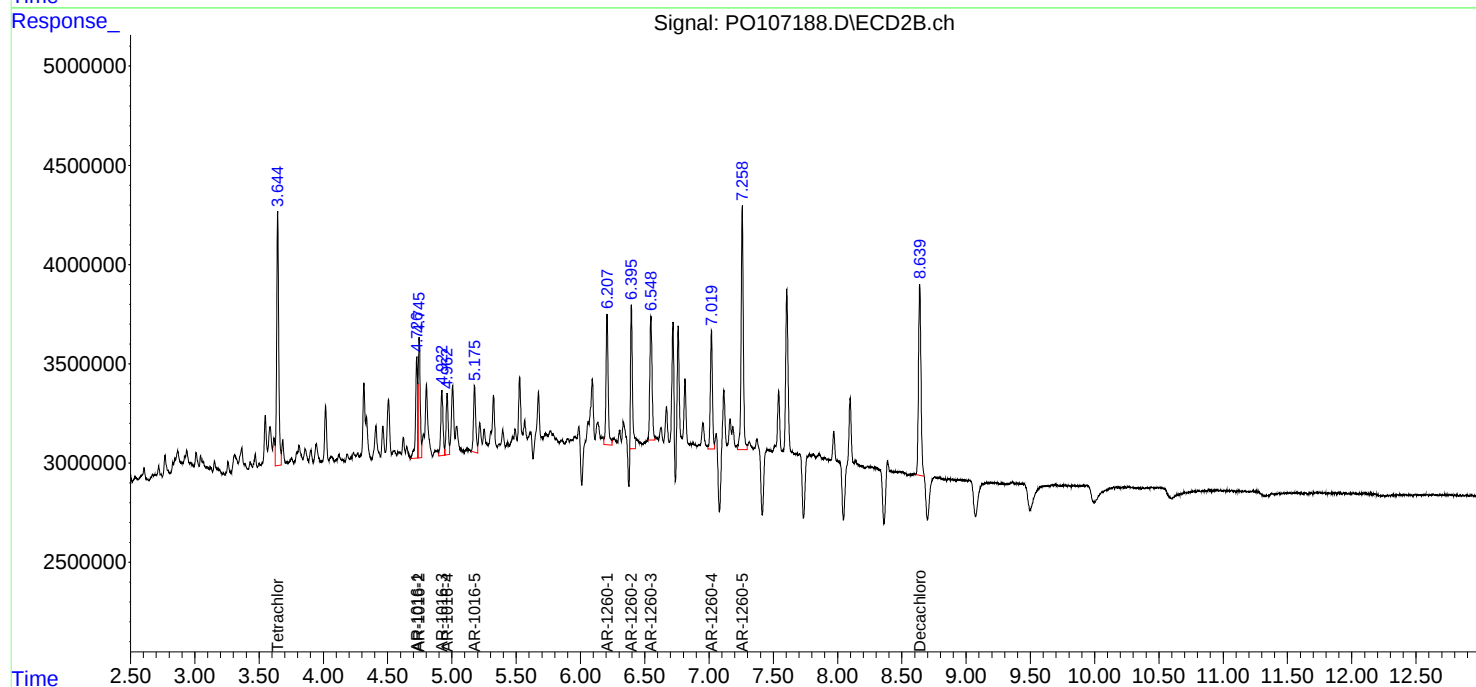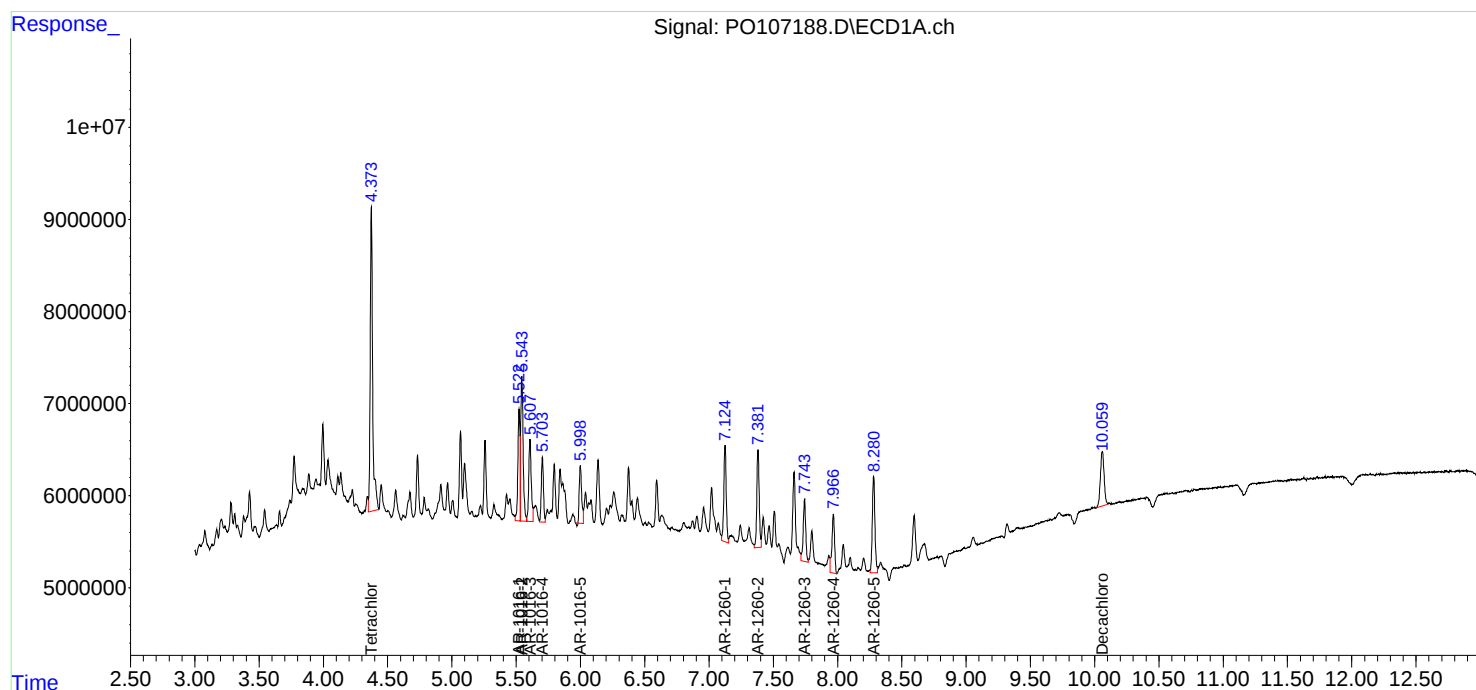

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 19:57
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:41:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:40:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	449.1E6	154.1E6	50.000	50.000
2) SA Decachlor...	10.060	8.639	121.6E6	134.8E6	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.573	3.856	55004944	17447760	500.000	500.000
9) L2 AR-1221-2	4.658	3.942	39418330	13312448	500.000	500.000
10) L2 AR-1221-3	4.733	4.018	117.0E6	40609299	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 19:57
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:41:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:40:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

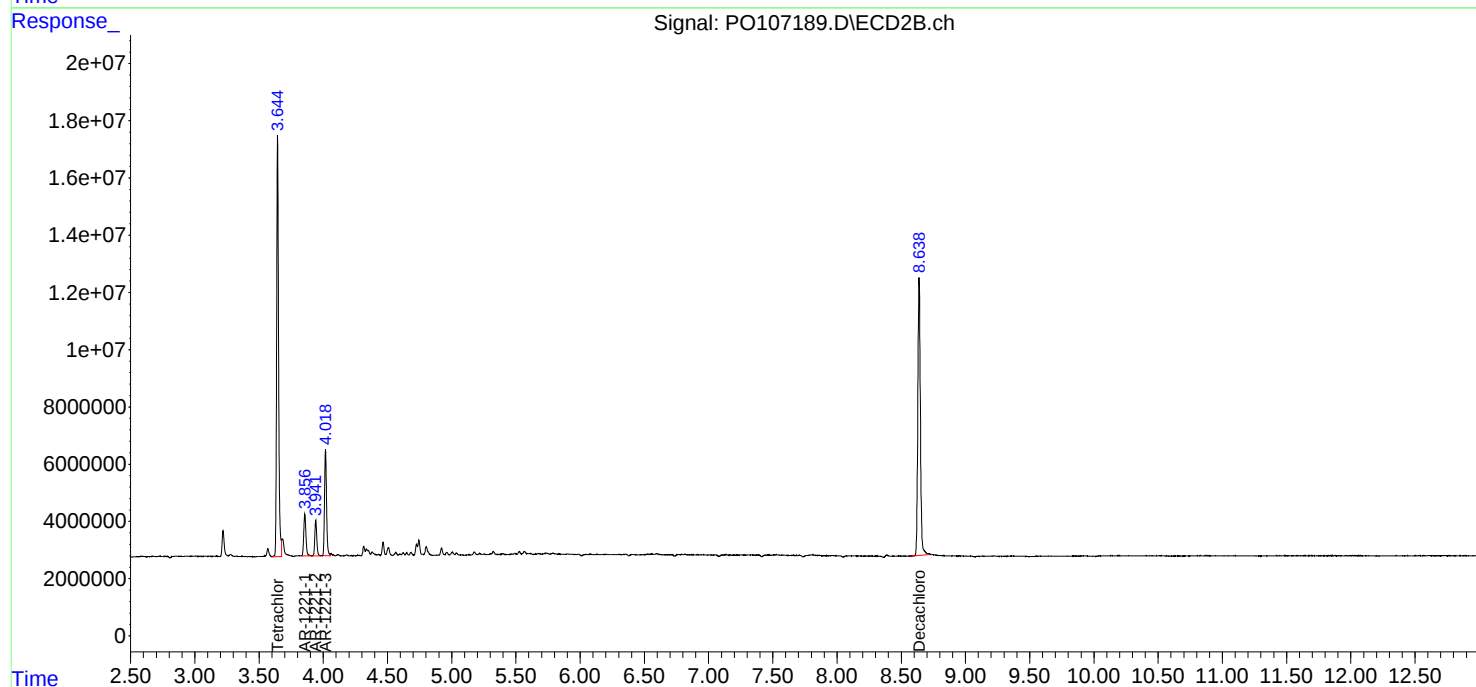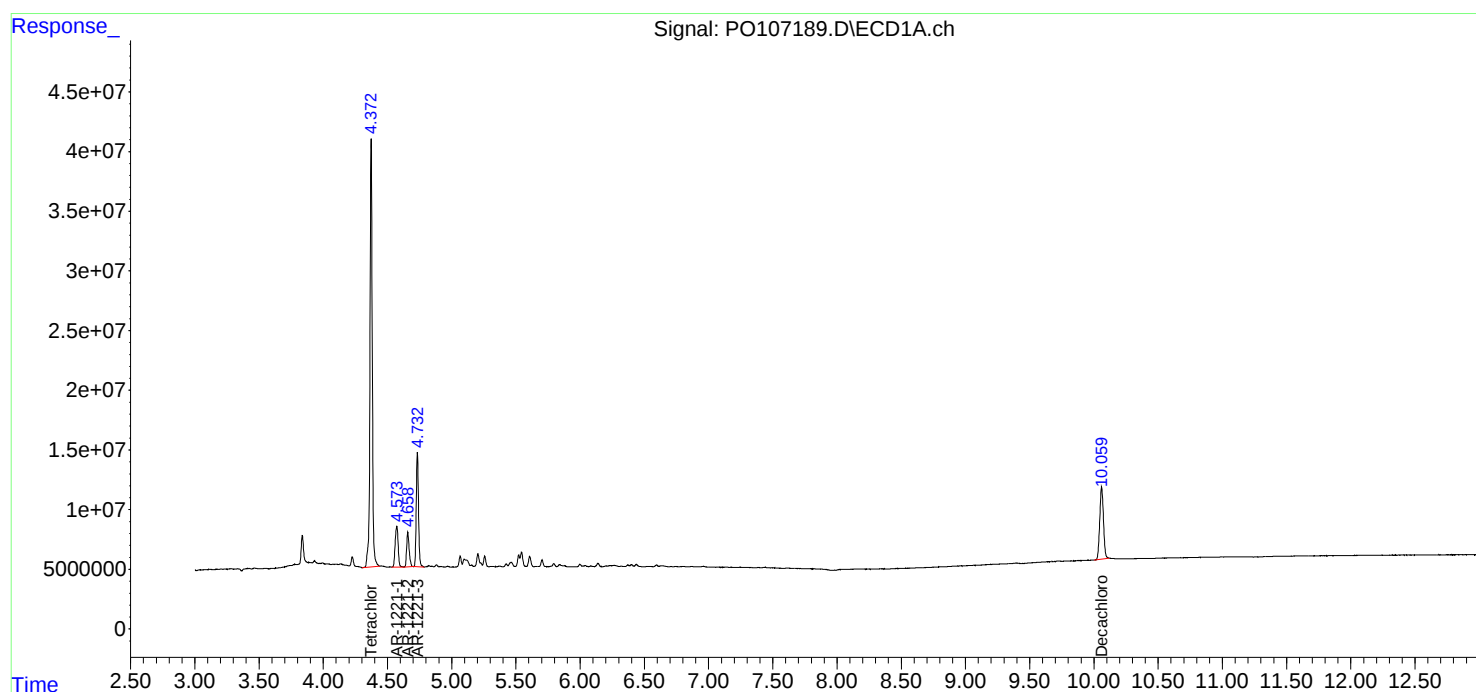

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 20:15
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:46:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:45:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	454.2E6	157.5E6	50.000	50.000
2) SA Decachlor...	10.059	8.639	121.6E6	135.6E6	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.733	4.017	97921824	33663502	500.000	500.000
12) L3 AR-1232-2	5.258	4.745	51512576	31602645	500.000	500.000
13) L3 AR-1232-3	5.544	4.921	89500289	17237464	500.000	500.000
14) L3 AR-1232-4	5.704	5.004	45082743	15732978	500.000	500.000
15) L3 AR-1232-5	5.796	5.176	32951614	16541659	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 20:15
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:46:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:45:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

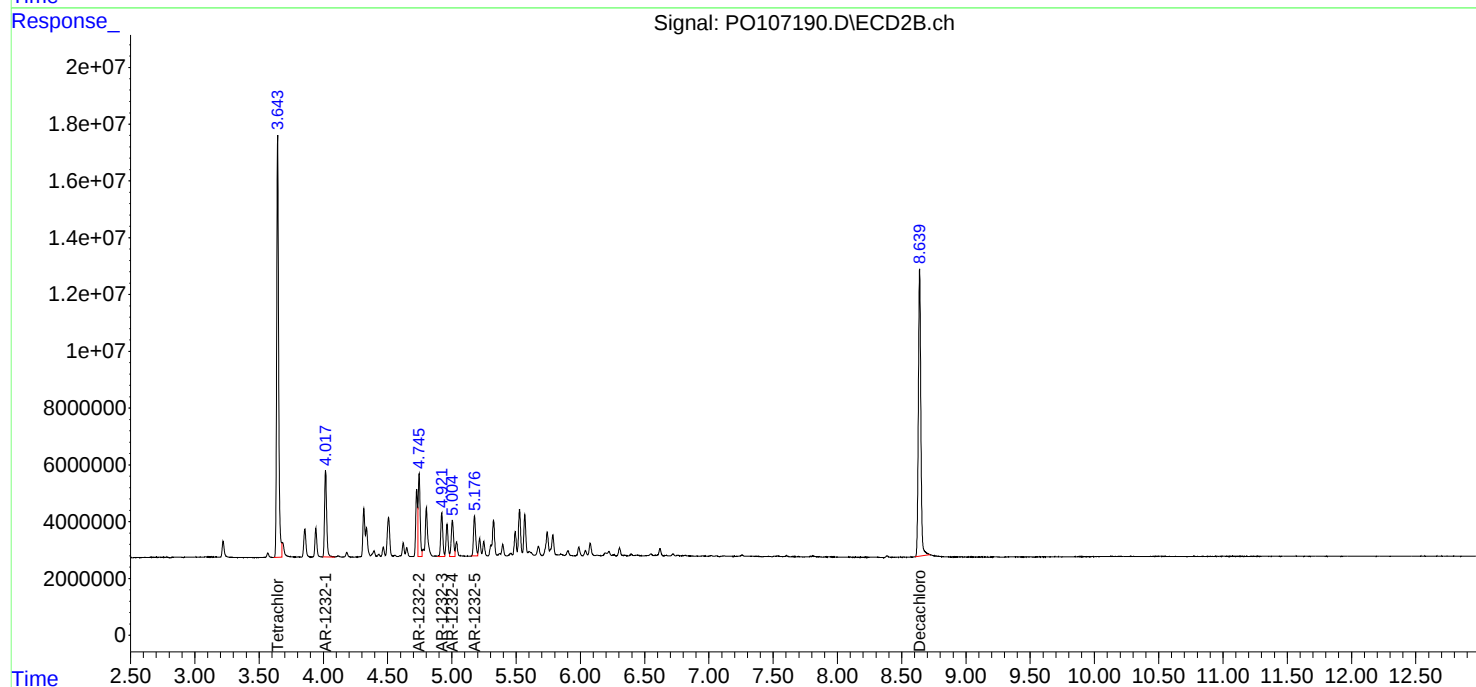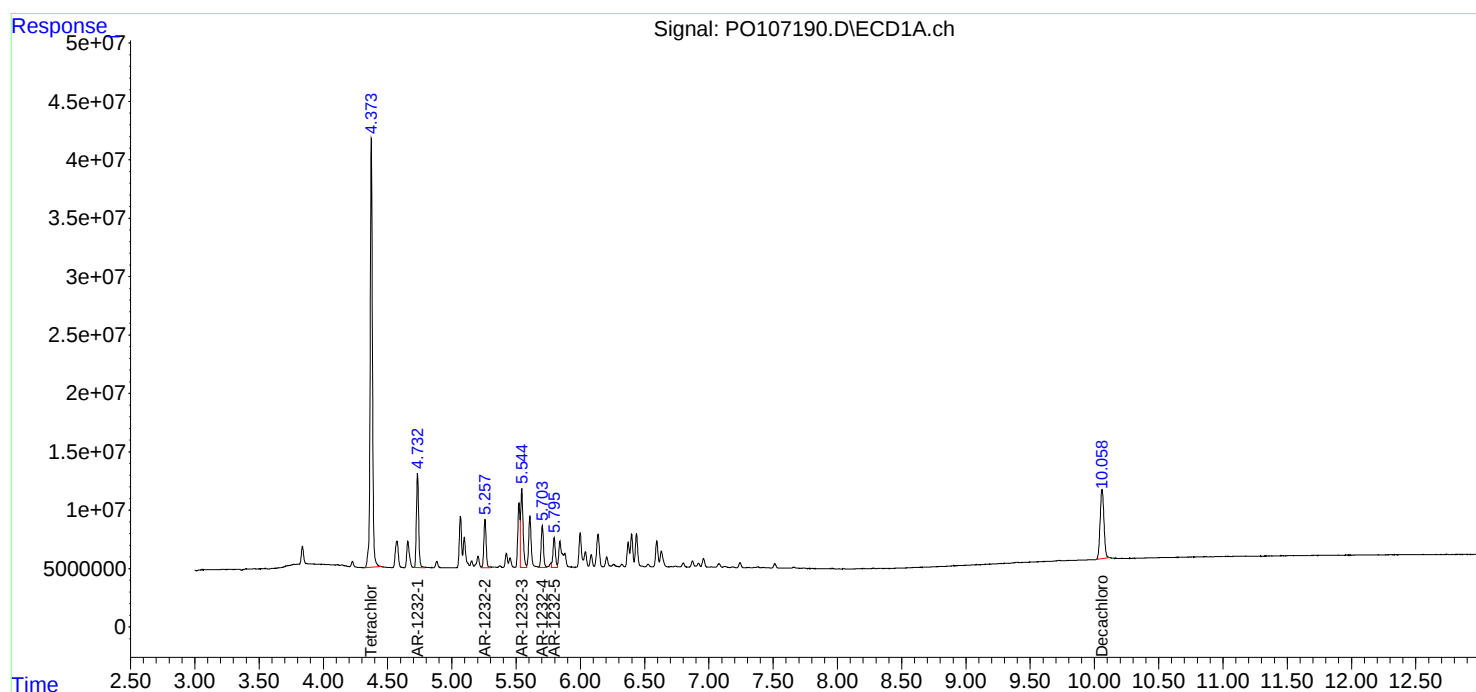

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 20:34
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:49:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	886.0E6	331.6E6	96.865	99.238
2) SA Decachlor...	10.061	8.638	233.9E6	268.7E6	93.851	97.198
Target Compounds						
16) L4 AR-1242-1	5.522	4.726	207.9E6	80390662	935.818	957.741
17) L4 AR-1242-2	5.545	4.745	302.4E6	114.5E6	934.753	972.360
18) L4 AR-1242-3	5.607	4.921	191.9E6	61817452	915.447	959.943
19) L4 AR-1242-4	5.704	5.004	150.4E6	60582529	924.137	940.948
20) L4 AR-1242-5	6.437	5.526	141.0E6	73763103	917.497	955.284



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 20:34
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:49:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

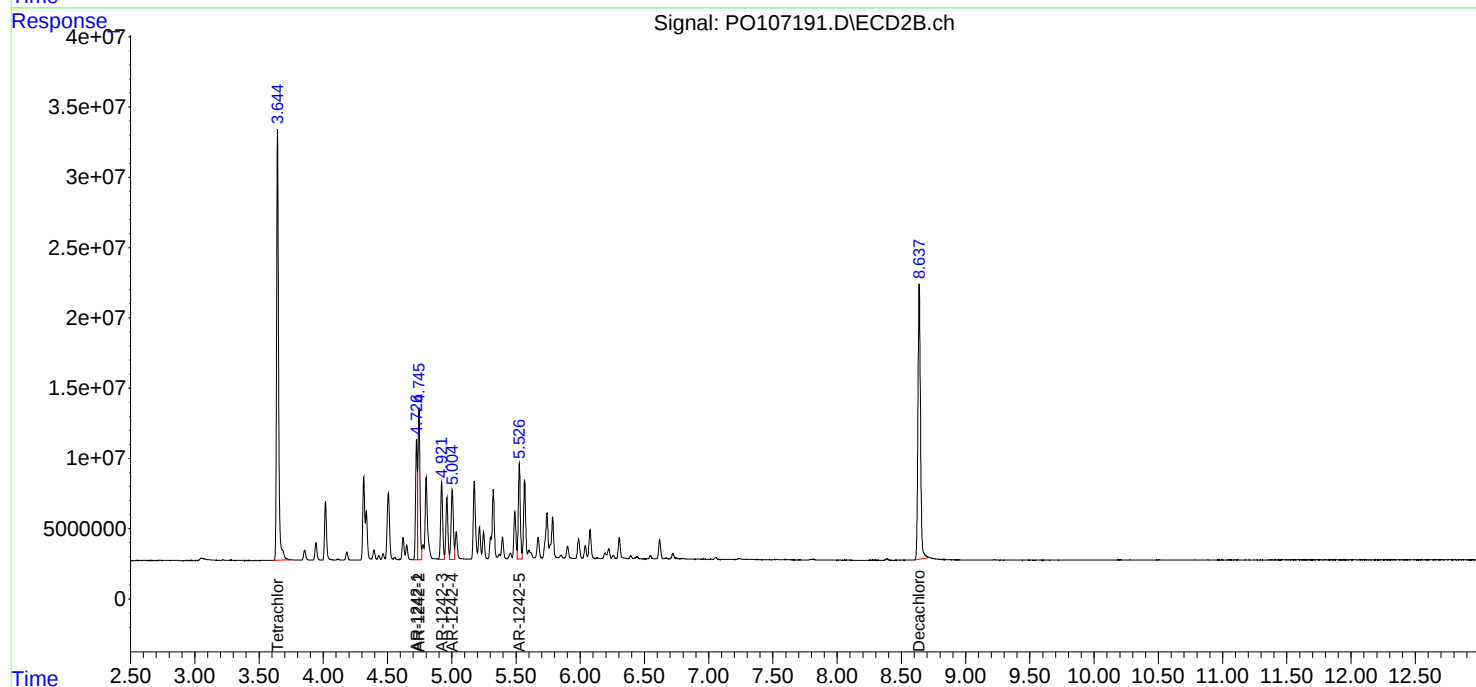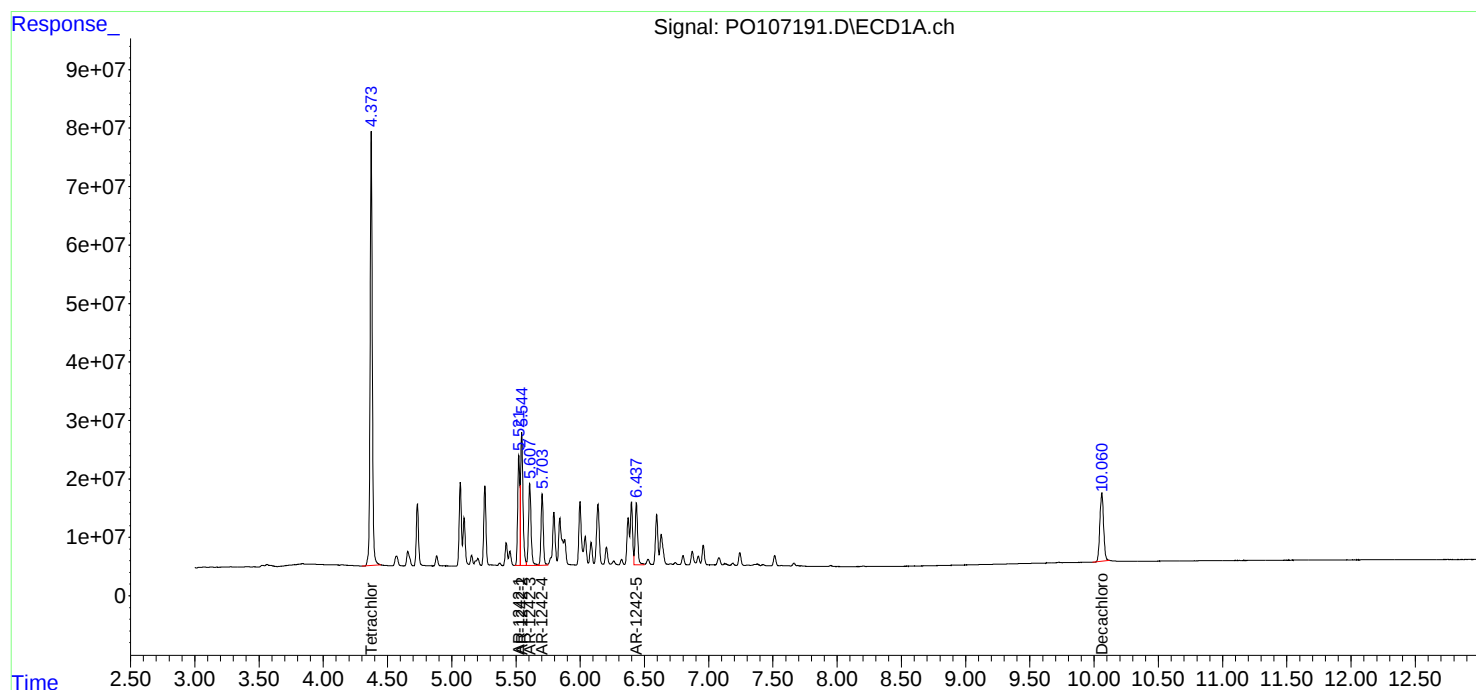

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 20:52
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:49:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	648.9E6	243.1E6	70.941	72.772
2) SA Decachlor...	10.059	8.639	182.1E6	207.3E6	73.046	74.999
Target Compounds						
16) L4 AR-1242-1	5.521	4.726	154.2E6	60335620	693.850	718.814
17) L4 AR-1242-2	5.544	4.746	225.0E6	83449803	695.293	708.752
18) L4 AR-1242-3	5.606	4.922	144.9E6	45346429	691.114	704.170
19) L4 AR-1242-4	5.703	5.005	109.0E6	45477164	669.566	706.336
20) L4 AR-1242-5	6.437	5.526	107.6E6	56756574	699.831	735.037



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 20:52
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:49:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

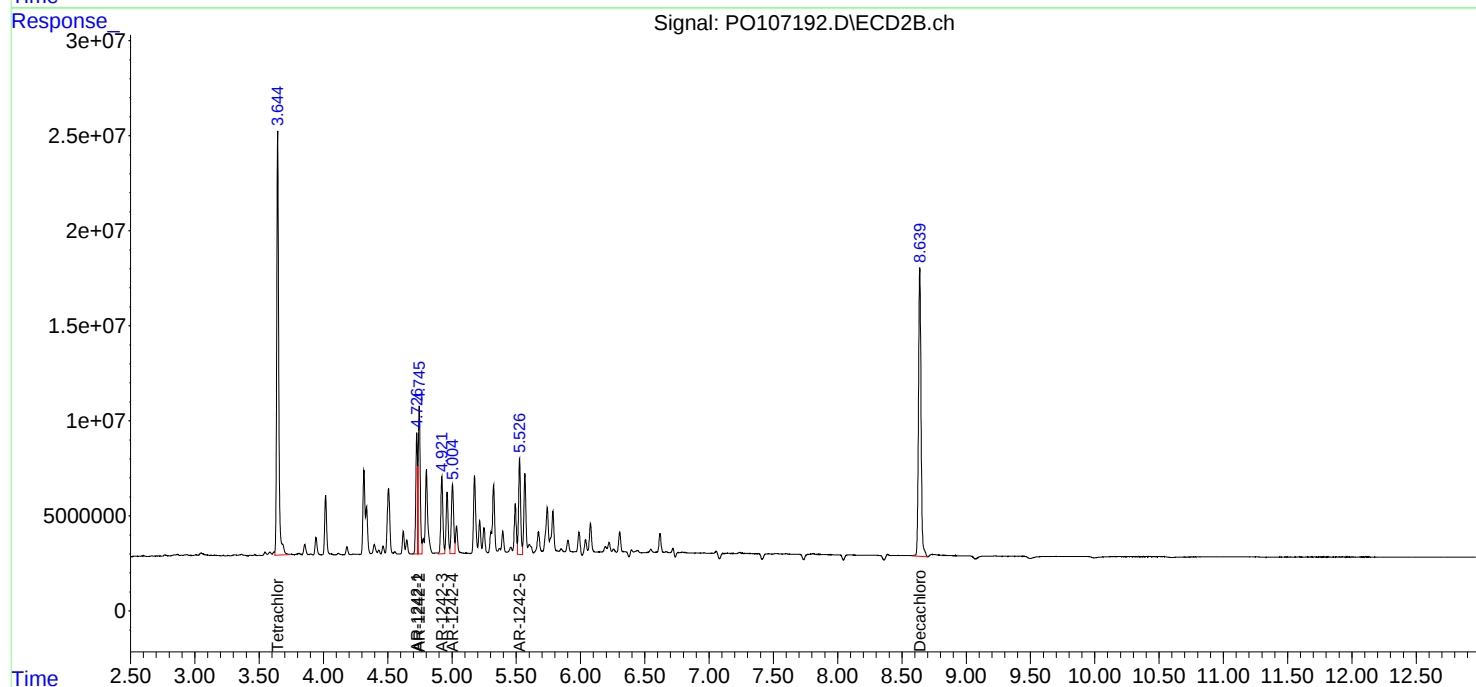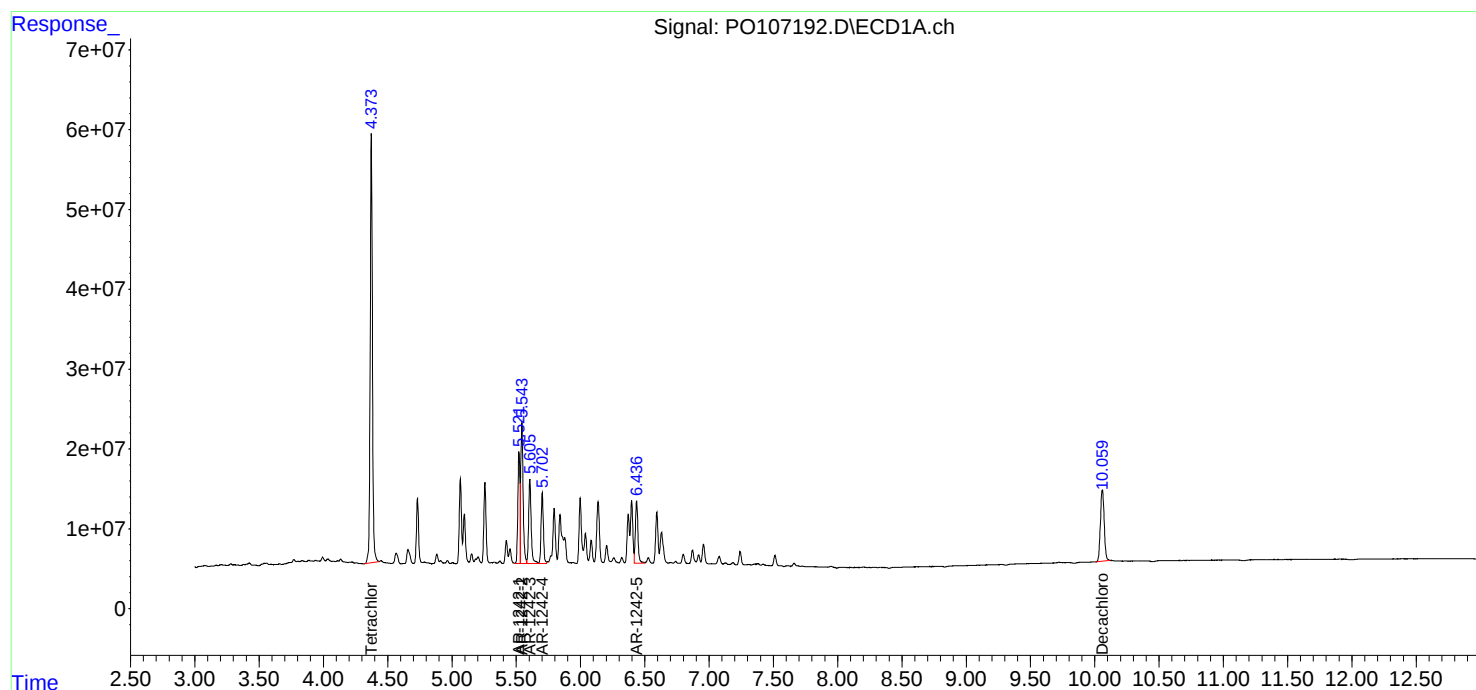

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 21:10
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:50:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	457.3E6	167.1E6	50.000	50.000
2) SA Decachlor...	10.057	8.639	124.6E6	138.2E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	5.522	4.726	111.1E6	41968881	500.000	500.000
17) L4 AR-1242-2	5.544	4.745	161.8E6	58870958	500.000	500.000
18) L4 AR-1242-3	5.607	4.922	104.8E6	32198496	500.000	500.000
19) L4 AR-1242-4	5.703	5.004	81398754	32192297	500.000	500.000
20) L4 AR-1242-5	6.437	5.526	76844549	38607958	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 21:10
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:50:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

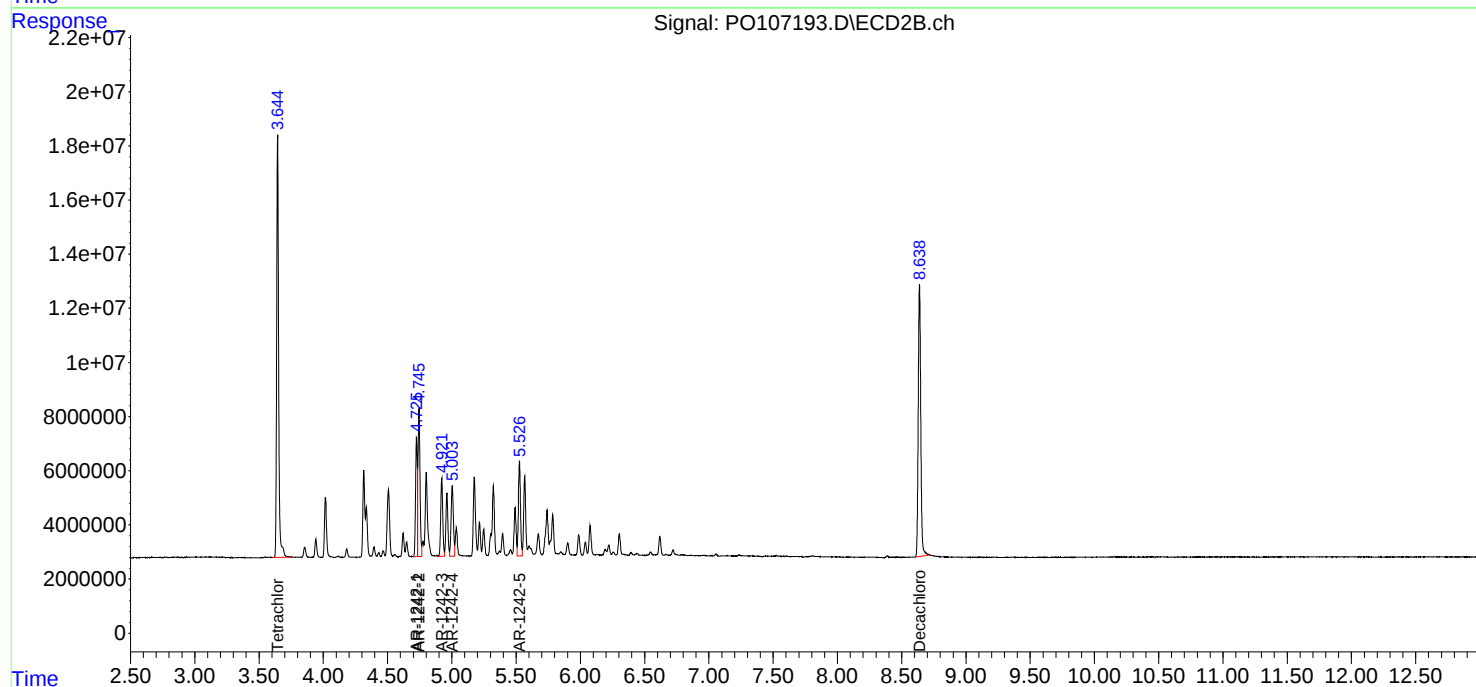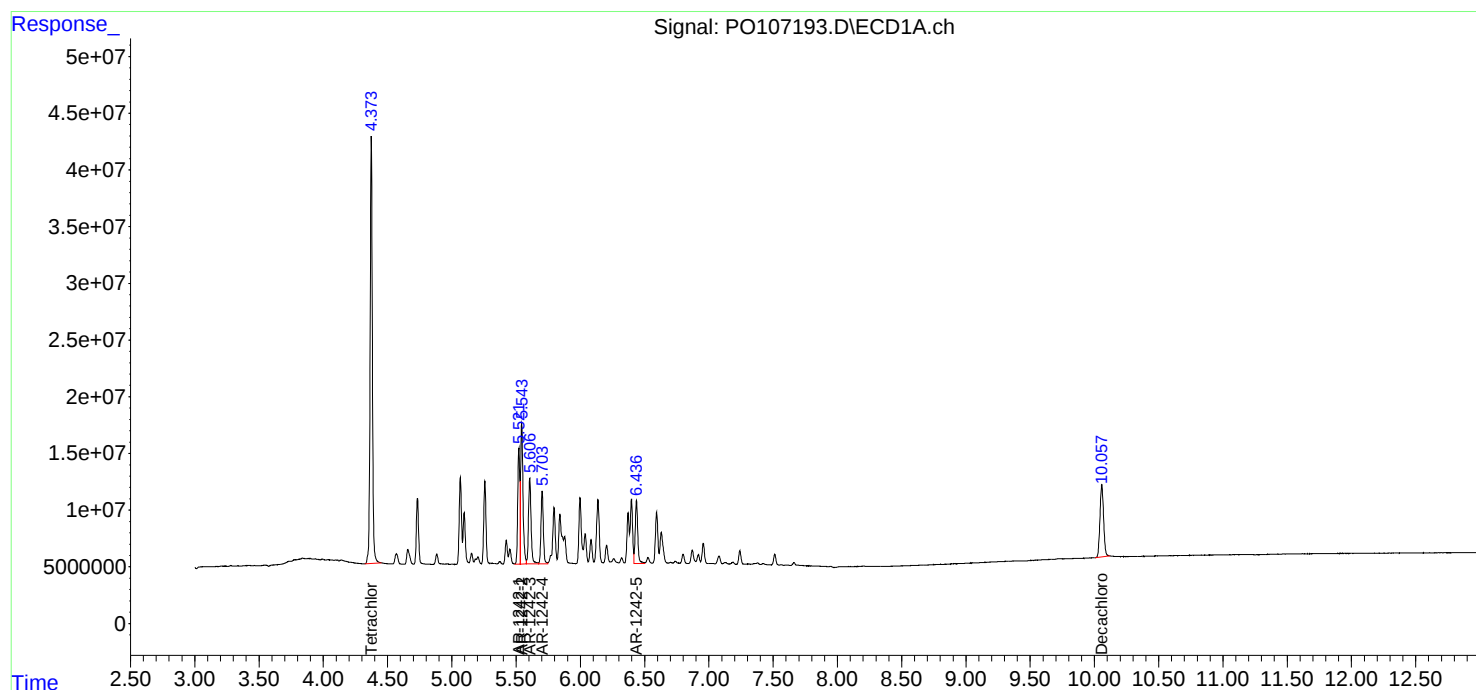

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 21:28
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:50:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	237.6E6	83389360	25.977	24.958
2) SA Decachlor...	10.057	8.639	63795685	69963548	25.593	25.308
Target Compounds						
16) L4 AR-1242-1	5.522	4.727	59739114	21816724	268.842	259.915
17) L4 AR-1242-2	5.544	4.746	85701102	30166778	264.877	256.211
18) L4 AR-1242-3	5.607	4.922	56076682	16716467	267.493	259.585
19) L4 AR-1242-4	5.703	5.005	43283991	17011315	265.876	264.214
20) L4 AR-1242-5	6.437	5.526	41155754	20184132	267.786	261.399



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 21:28
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:50:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

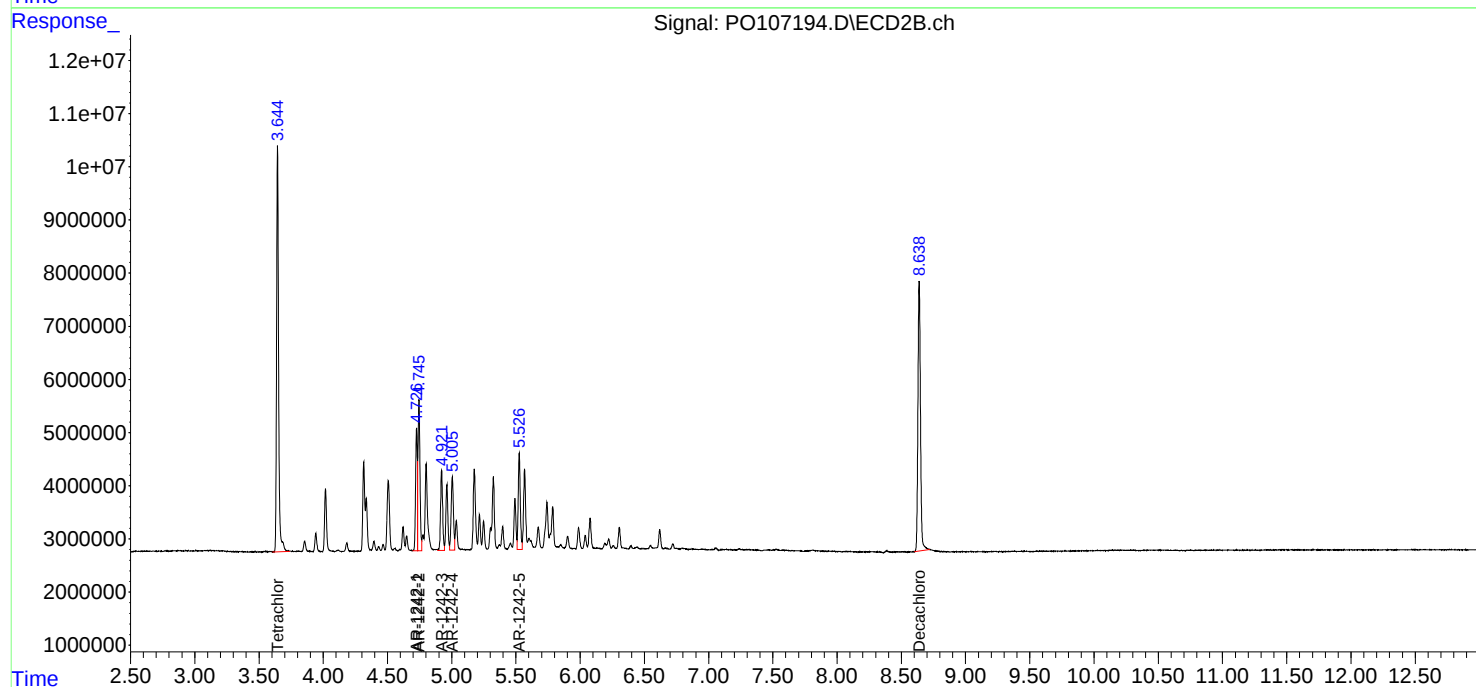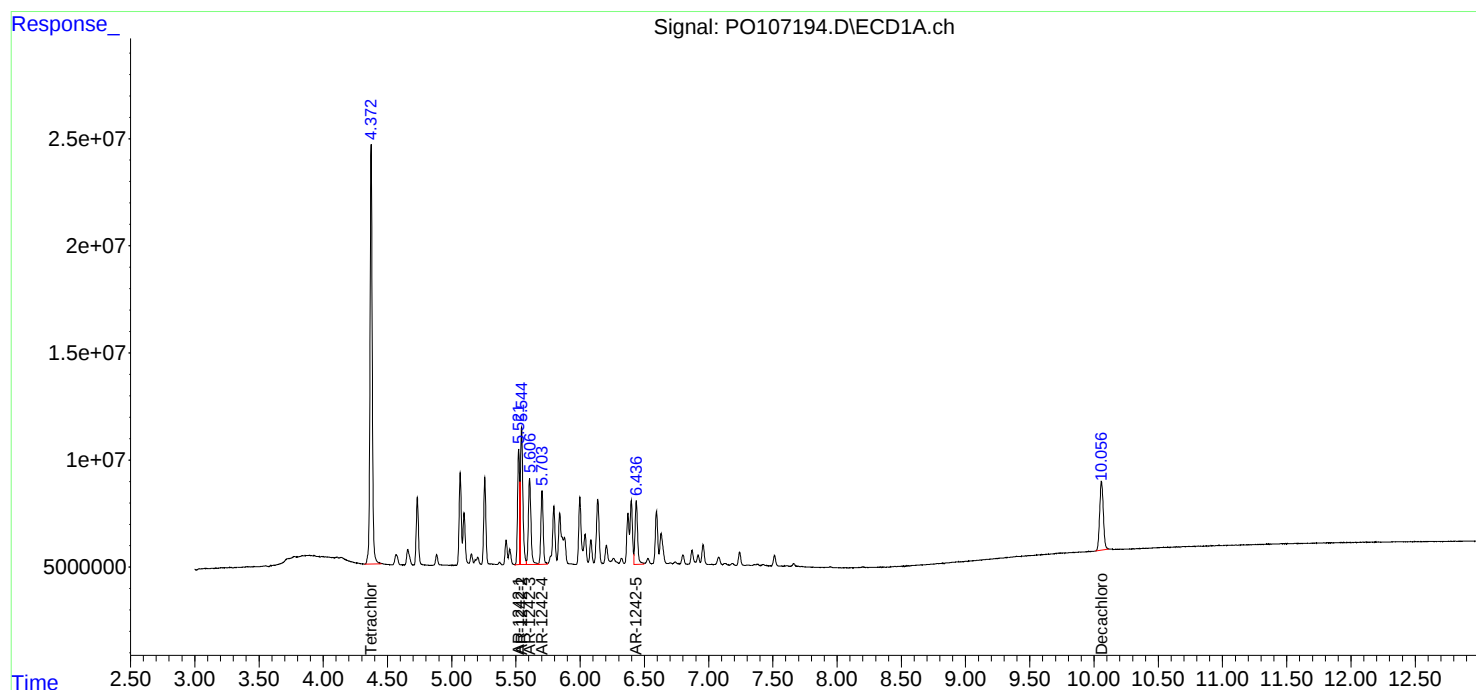

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 21:46
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:51:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	45874144	14600377	5.015	4.370
2) SA Decachlor...	10.055	8.638	12132051	13326327	4.867	4.821
Target Compounds						
16) L4 AR-1242-1	5.521	4.726	12176144	4333712	54.796	51.630
17) L4 AR-1242-2	5.544	4.745	17442944	5701582	53.911	48.424
18) L4 AR-1242-3	5.606	4.921	11292382	3181204	53.866	49.400
19) L4 AR-1242-4	5.703	5.004	8415437	3329911	51.693	51.719
20) L4 AR-1242-5	6.437	5.526	8983989	4011331	58.456	51.950



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 21:46
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:51:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

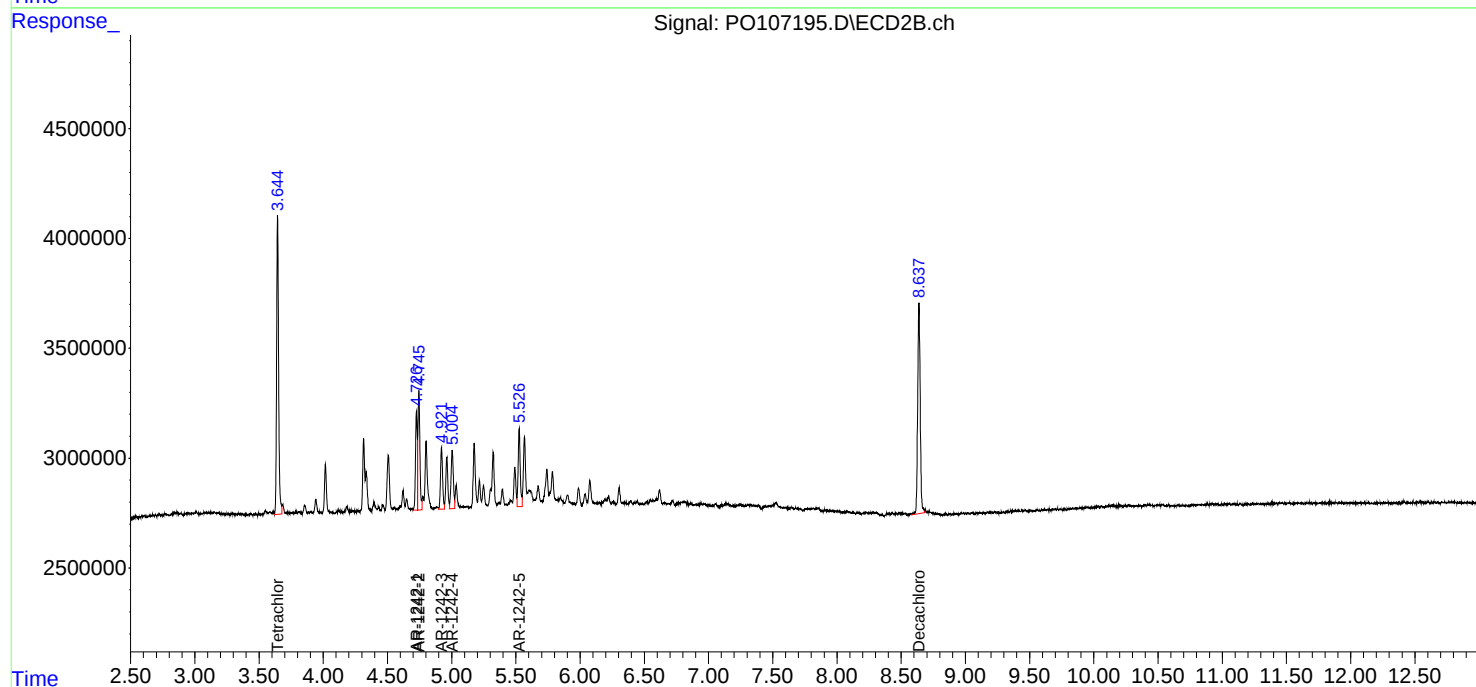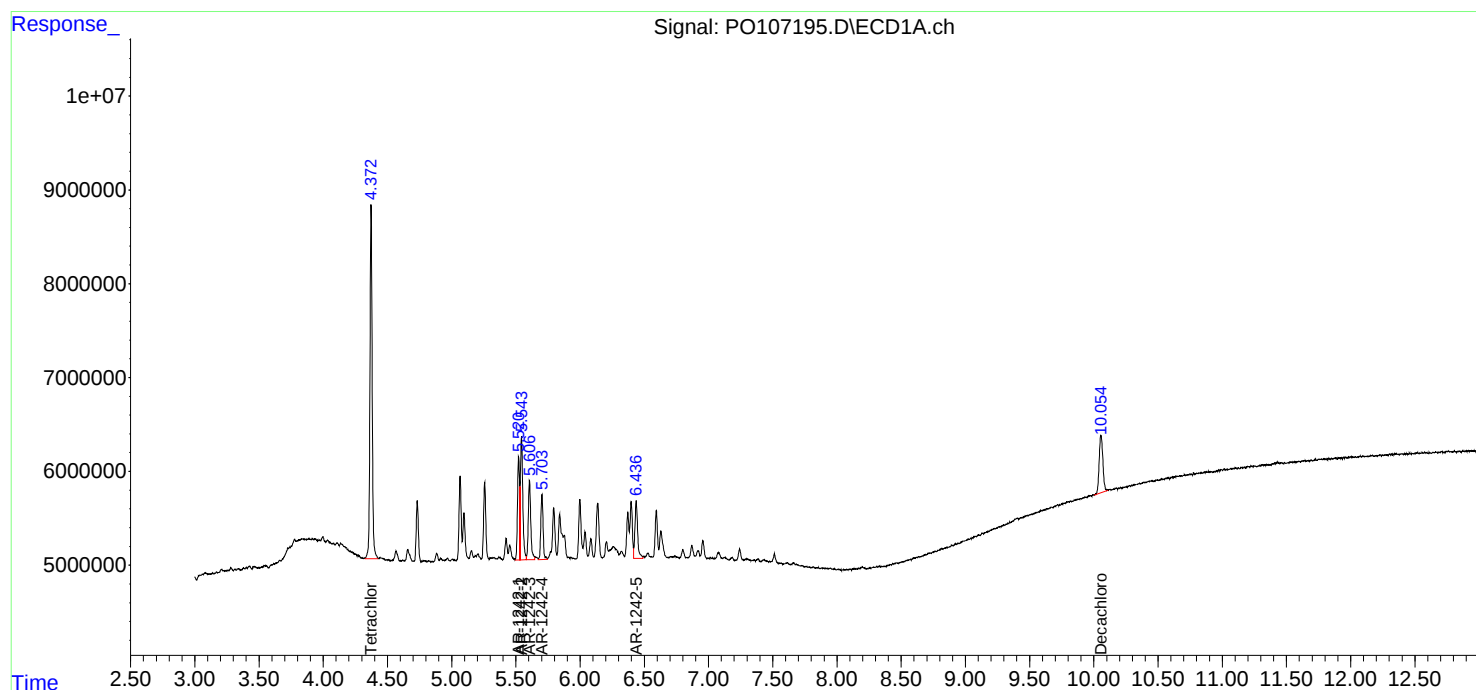

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 22:04
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:08:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	871.9E6	327.8E6	93.167	95.697
2) SA Decachlor...	10.057	8.638	234.0E6	266.9E6	93.438	95.612
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	155.9E6	60218805	889.958	928.169
22) L5 AR-1248-2	5.795	4.962	222.8E6	85173308	878.597	915.232
23) L5 AR-1248-3	5.997	5.004	231.9E6	89257070	892.951	916.605
24) L5 AR-1248-4	6.398	5.176	237.2E6	105.9E6	910.480	923.092
25) L5 AR-1248-5	6.437	5.567	236.3E6	102.8E6	906.188	936.492



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 22:04
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:08:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

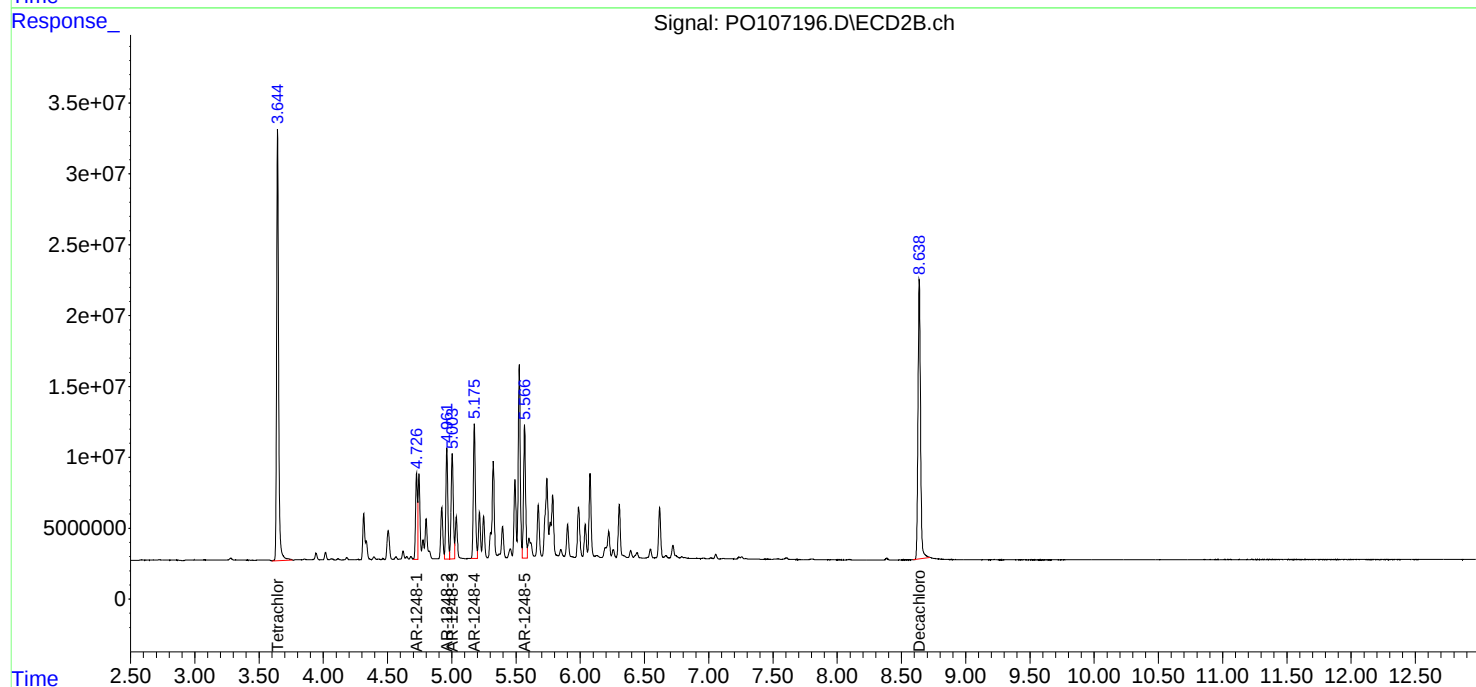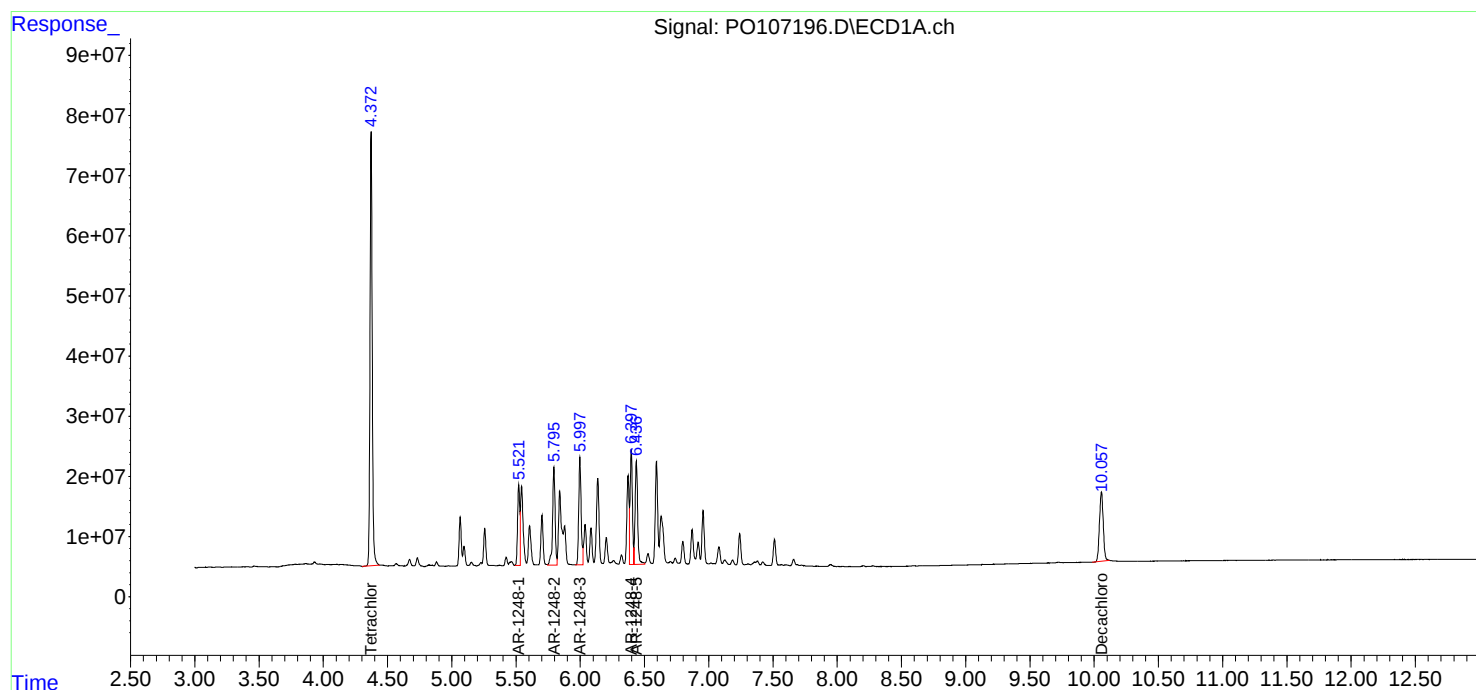

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 22:22
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:09:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	684.0E6	254.2E6	73.085	74.199
2) SA Decachlor...	10.056	8.638	177.9E6	201.2E6	71.030	72.062
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	123.6E6	47278639	705.517	728.719
22) L5 AR-1248-2	5.795	4.962	178.7E6	66831271	704.358	718.137
23) L5 AR-1248-3	5.997	5.004	184.7E6	69919958	711.094	718.027
24) L5 AR-1248-4	6.398	5.176	185.0E6	82899838	709.988	722.373
25) L5 AR-1248-5	6.437	5.568	184.9E6	79019739	709.319	719.661



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 22:22
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:09:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

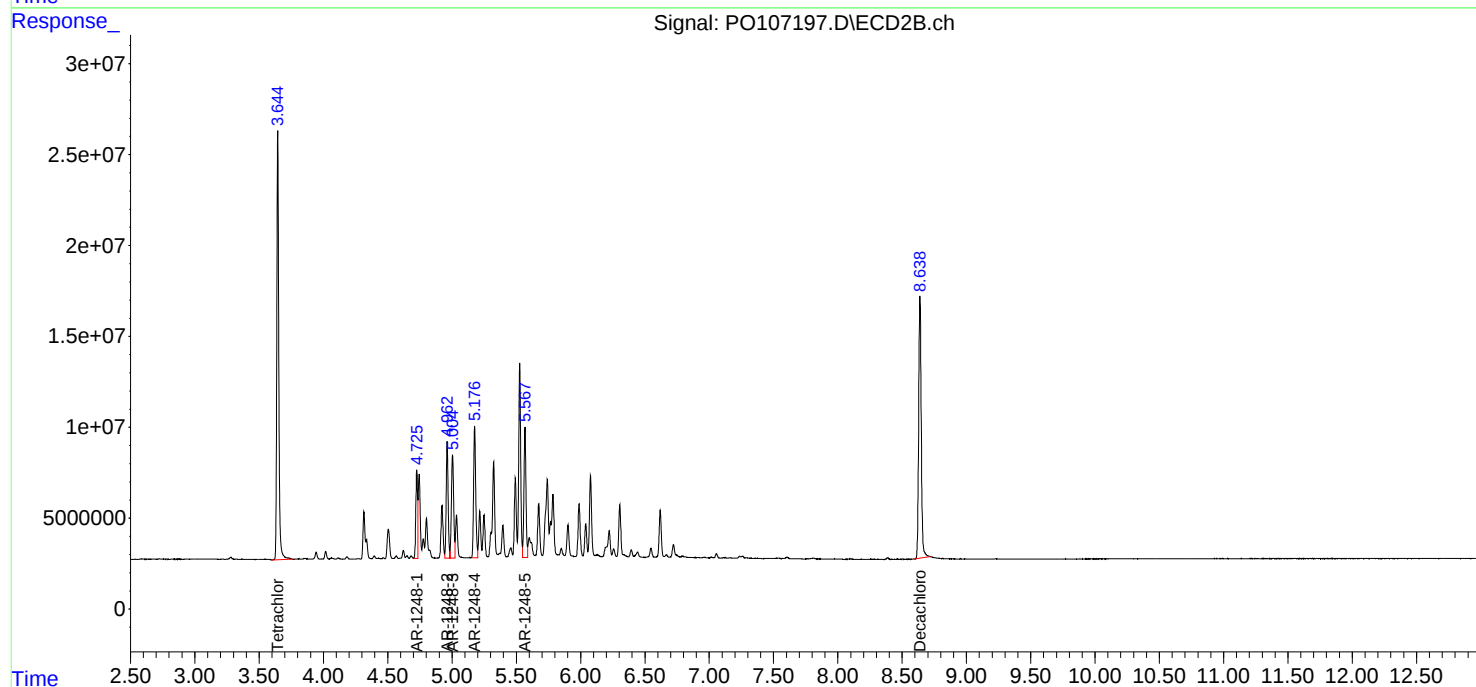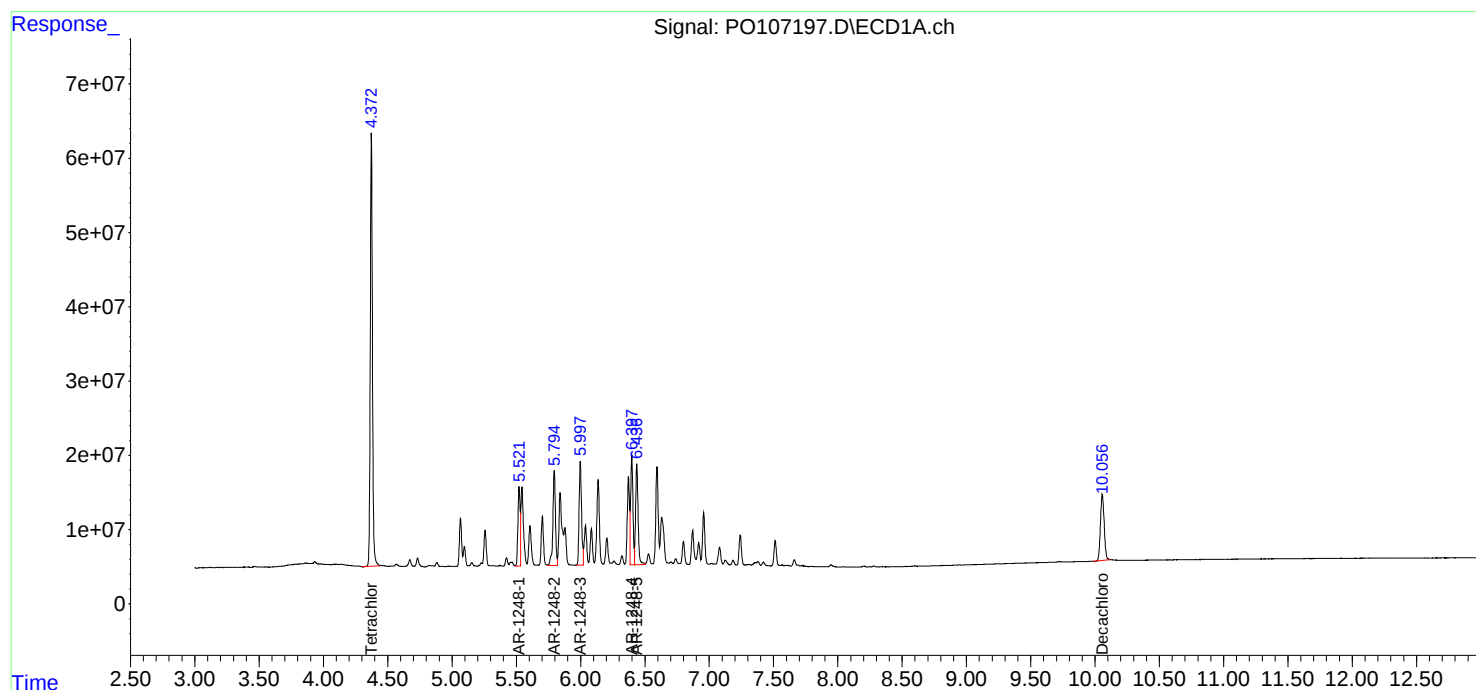

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 22:41
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:09:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	467.9E6	171.3E6	50.000	50.000
2) SA Decachlor...	10.058	8.638	125.2E6	139.6E6	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	87595666	32439560	500.000	500.000
22) L5 AR-1248-2	5.795	4.962	126.8E6	46530975	500.000	500.000
23) L5 AR-1248-3	5.998	5.004	129.9E6	48688939	500.000	500.000
24) L5 AR-1248-4	6.398	5.176	130.3E6	57380206	500.000	500.000
25) L5 AR-1248-5	6.437	5.567	130.4E6	54900690	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 22:41
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:09:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

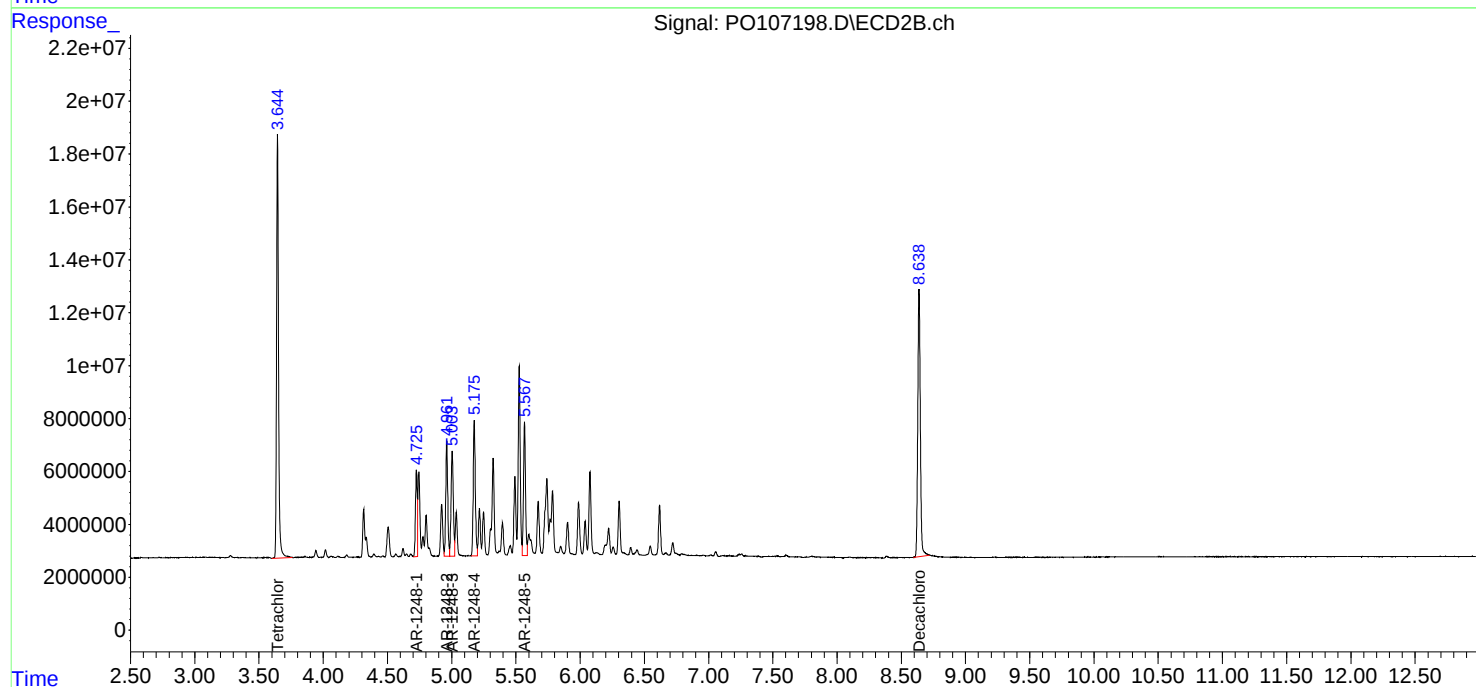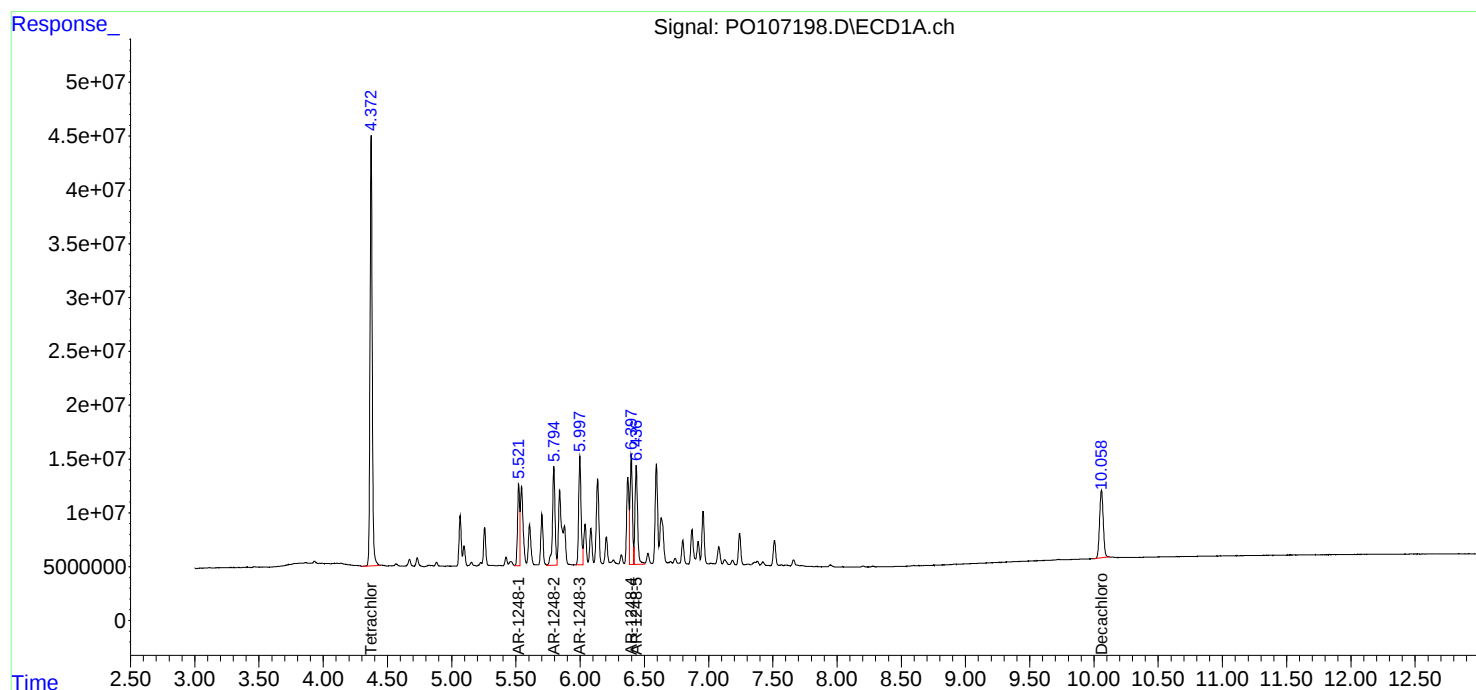

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 22:59
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:09:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	237.3E6	84054601	25.358	24.535
2) SA Decachlor...	10.056	8.639	64153967	70917862	25.620	25.402
Target Compounds						
21) L5 AR-1248-1	5.522	4.725	46152443	16666809	263.440	256.890
22) L5 AR-1248-2	5.796	4.962	67518514	24135370	266.200	259.347
23) L5 AR-1248-3	5.998	5.003	68597053	25222976	264.133	259.022
24) L5 AR-1248-4	6.399	5.175	68218183	29443172	261.841	256.562
25) L5 AR-1248-5	6.437	5.567	69078530	28554491	264.939	260.056



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 22:59
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:09:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

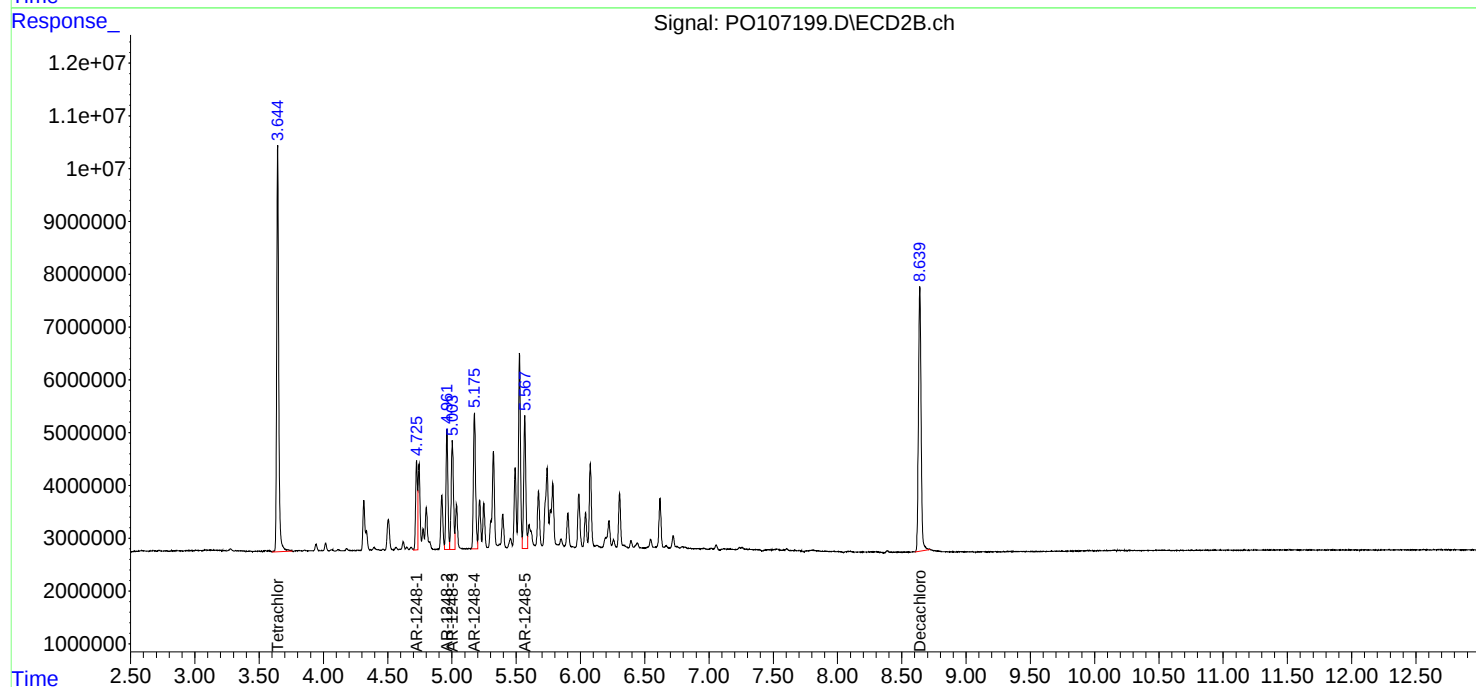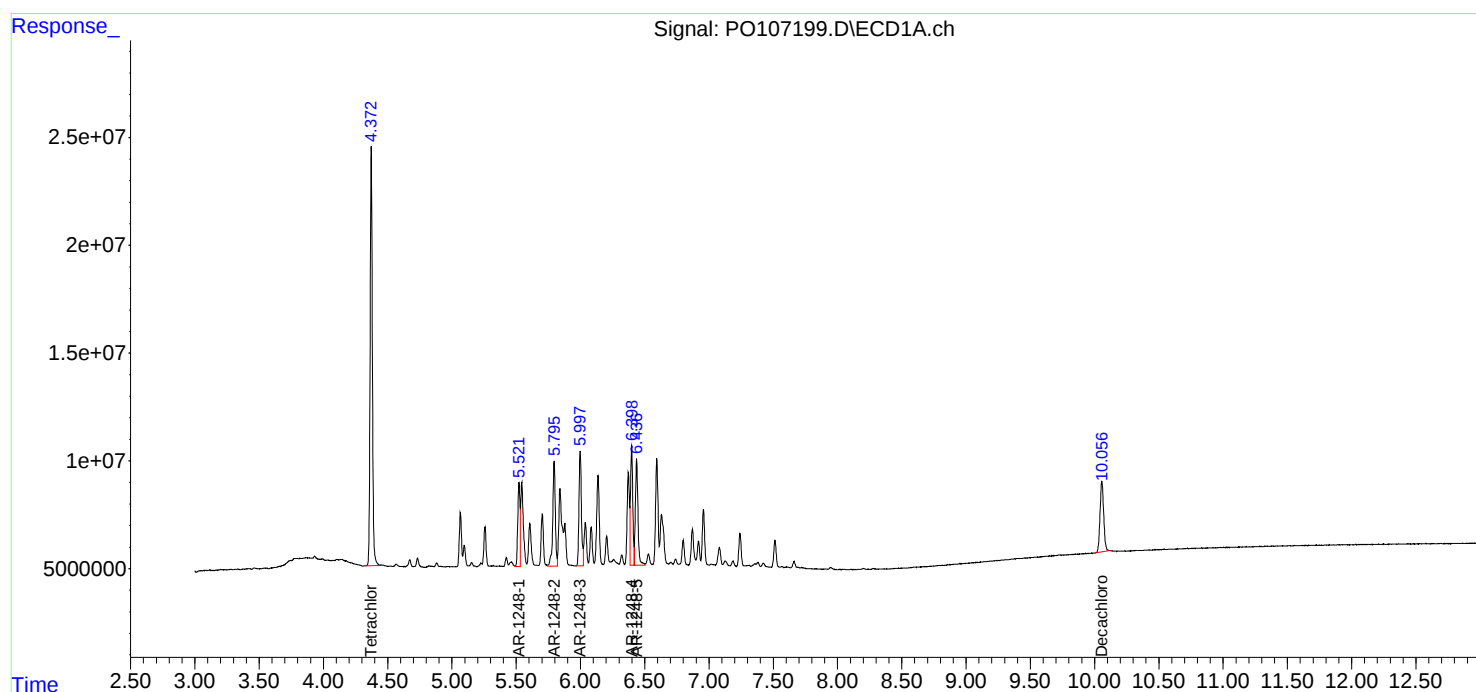

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 23:17
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:10:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	44978867	14828612	4.806	4.328
2) SA Decachlor...	10.057	8.638	11983506	13399690	4.786	4.800
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	9443386	3120120	53.903	48.091
22) L5 AR-1248-2	5.795	4.962	14018331	4677017	55.269	50.257
23) L5 AR-1248-3	5.997	5.004	13309890	4810627	51.250	49.402
24) L5 AR-1248-4	6.398	5.176	13593006	5584554	52.174	48.663
25) L5 AR-1248-5	6.436	5.567	14015230	5957032	53.753	54.253



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 23:17
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:10:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

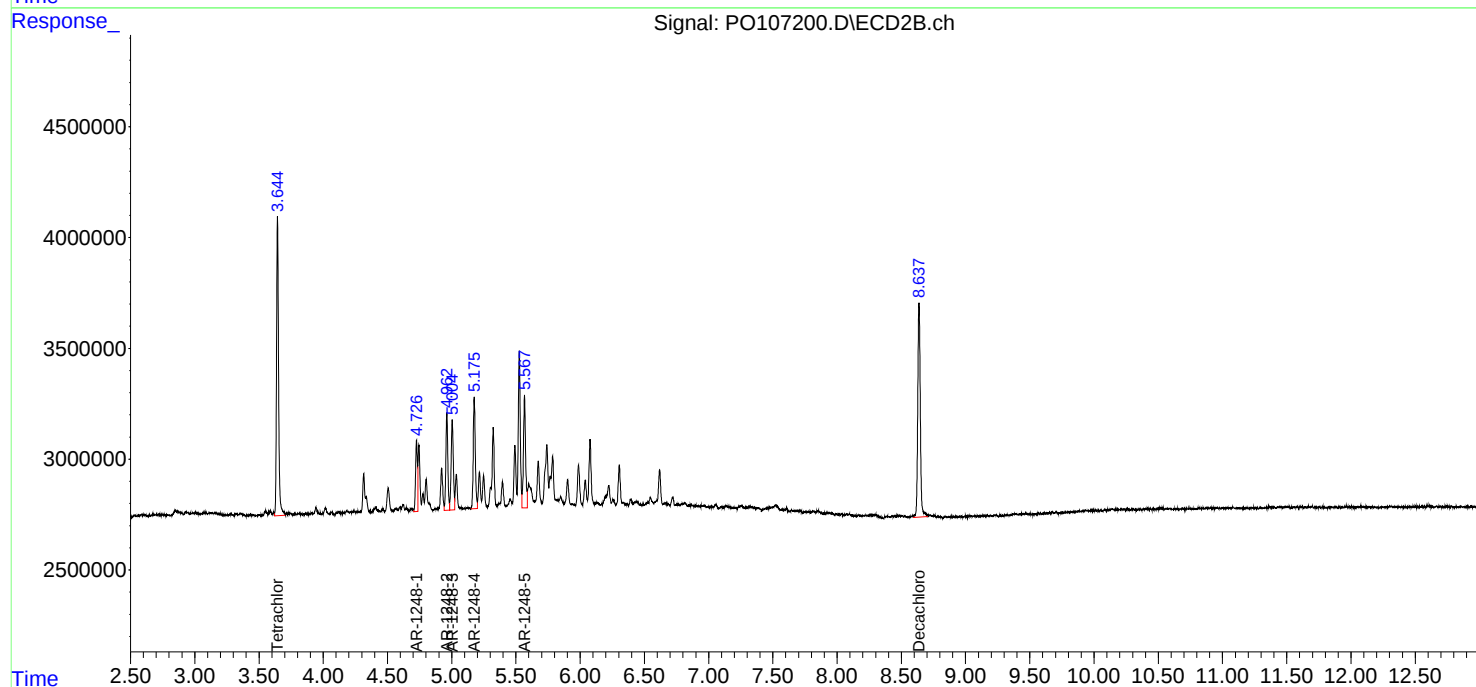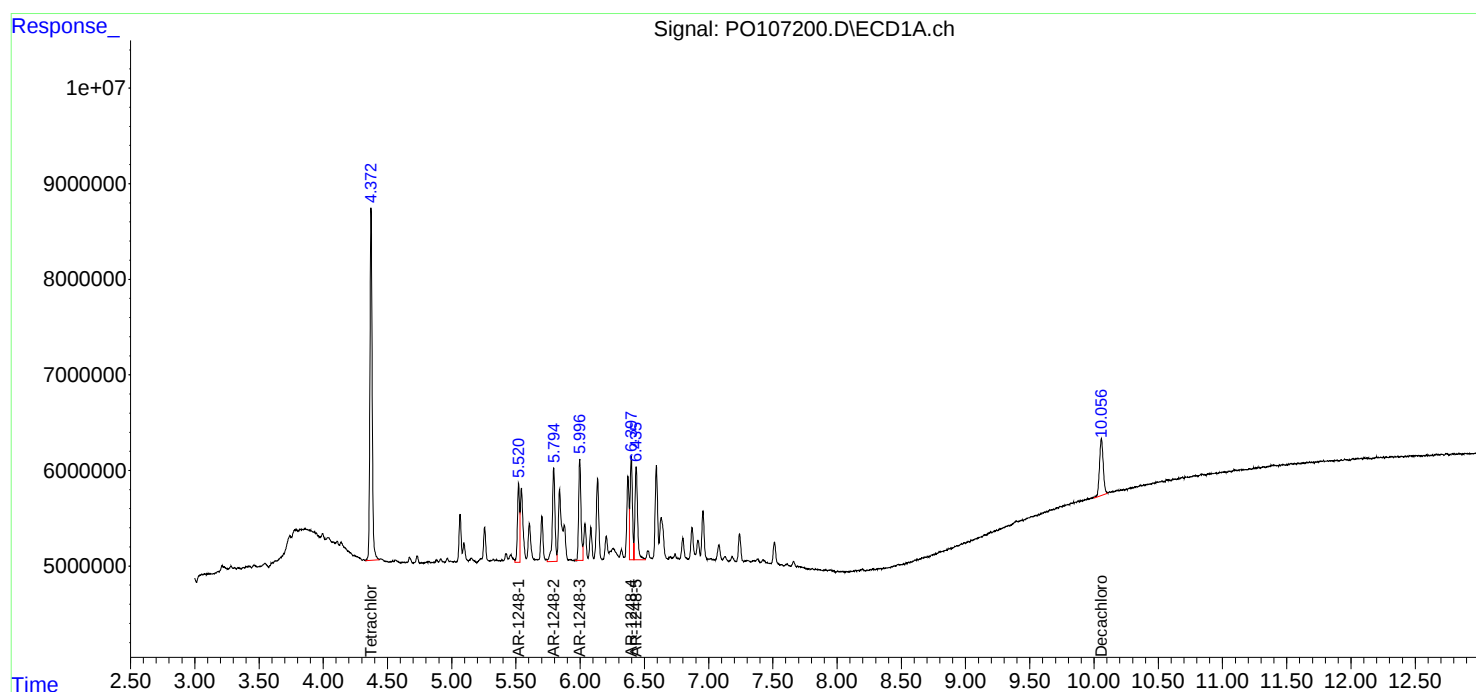

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 23:35
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:21:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	888.4E6	334.8E6	96.727	99.808
2) SA Decachlor...	10.058	8.638	235.8E6	272.7E6	93.987	98.323
Target Compounds						
26) L6 AR-1254-1	6.374	5.526	246.8E6	159.9E6	931.434	965.611
27) L6 AR-1254-2	6.593	5.674	348.1E6	138.5E6	933.222	957.951
28) L6 AR-1254-3	6.957	6.077	336.3E6	227.1E6	944.885	977.812
29) L6 AR-1254-4	7.242	6.304	213.1E6	128.2E6	938.161	976.528
30) L6 AR-1254-5	7.663	6.721	194.6E6	191.9E6	945.308	982.221



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 23:35
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:21:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

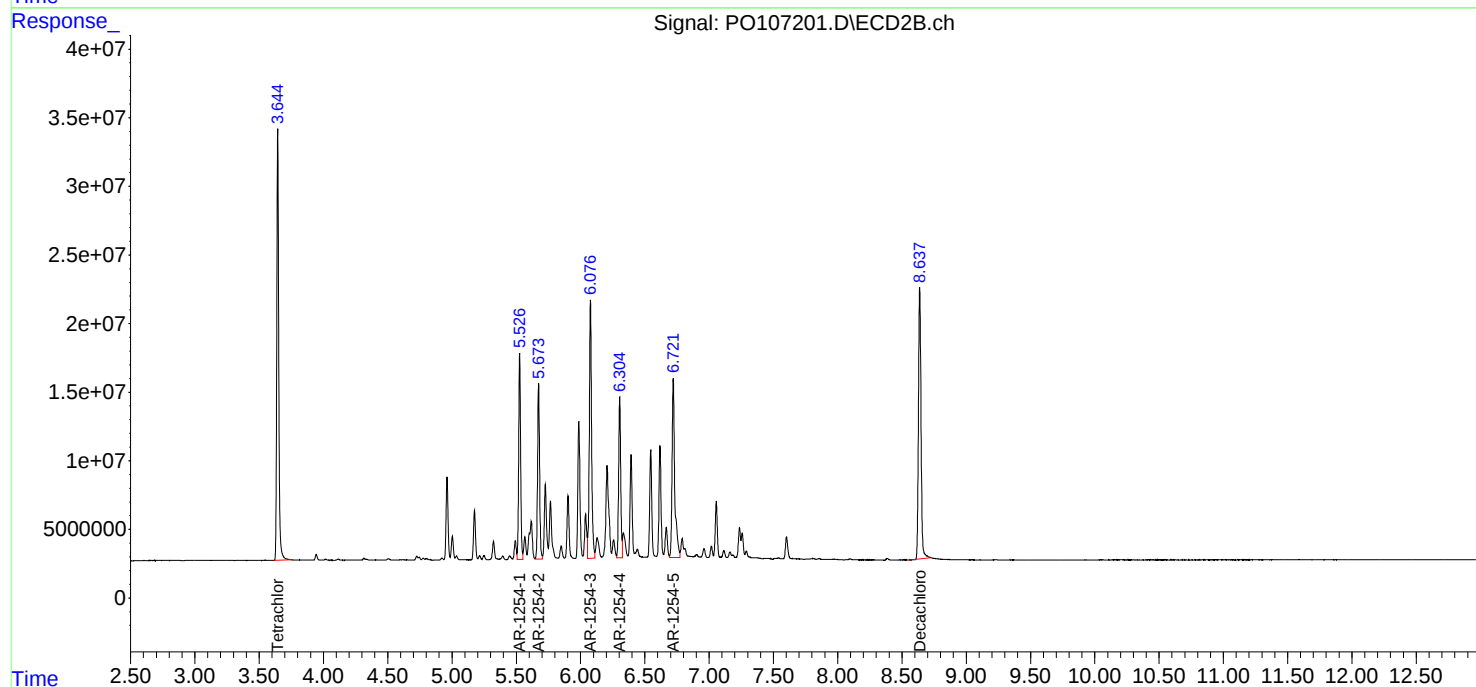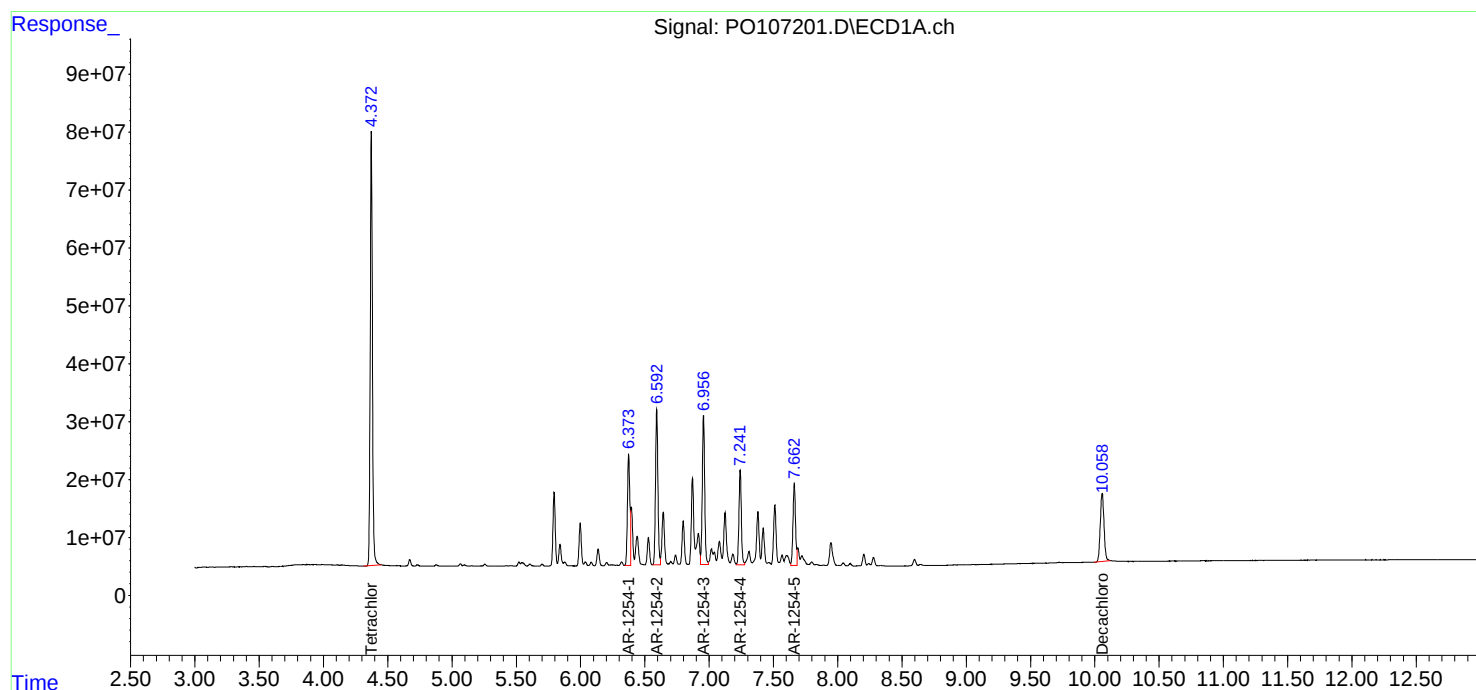

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 23:53
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:22:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	687.3E6	254.8E6	74.839	75.963
2) SA Decachlor...	10.058	8.638	180.1E6	205.4E6	71.810	74.047
Target Compounds						
26) L6 AR-1254-1	6.374	5.526	192.4E6	122.9E6	726.190	742.326
27) L6 AR-1254-2	6.593	5.673	271.2E6	106.7E6	727.100	738.182
28) L6 AR-1254-3	6.957	6.076	259.2E6	173.5E6	728.388	747.327
29) L6 AR-1254-4	7.241	6.303	165.1E6	97687474	726.838	743.858
30) L6 AR-1254-5	7.662	6.721	150.8E6	146.4E6	732.514	749.136



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 23:53
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:22:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

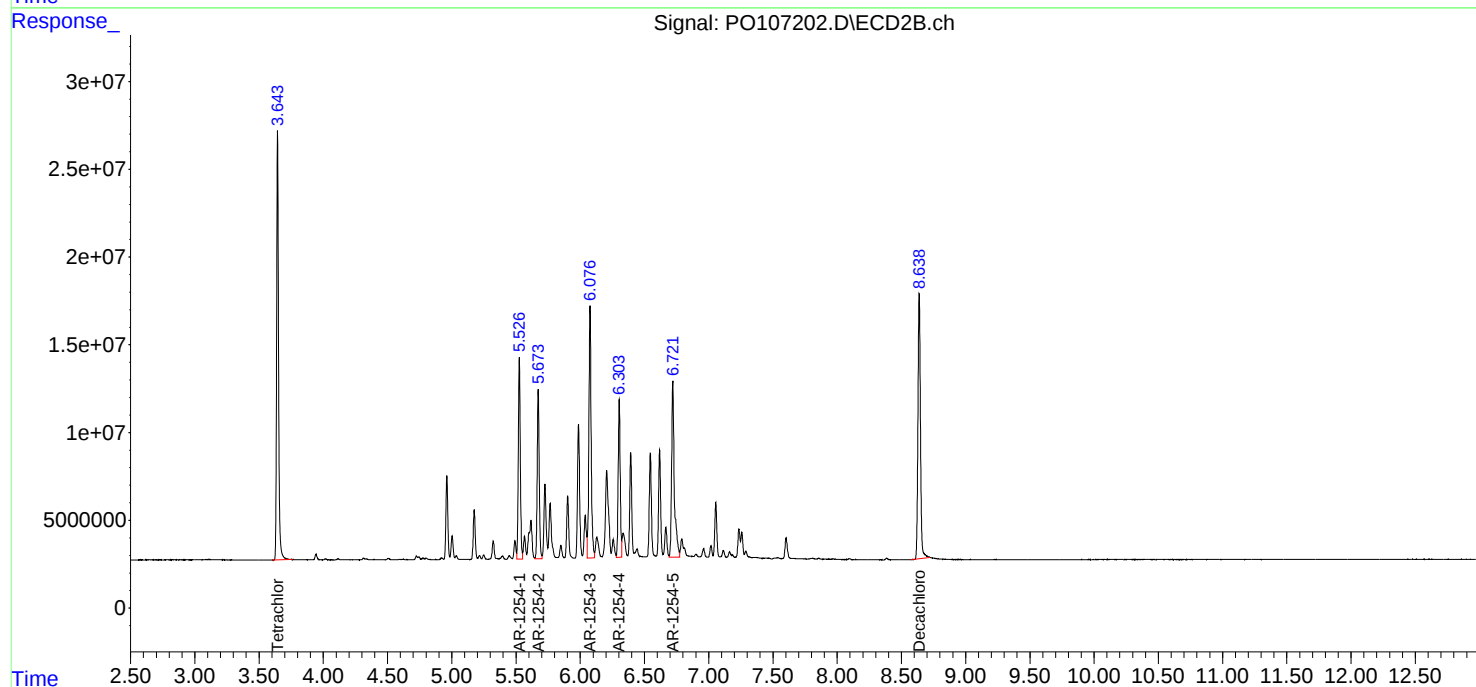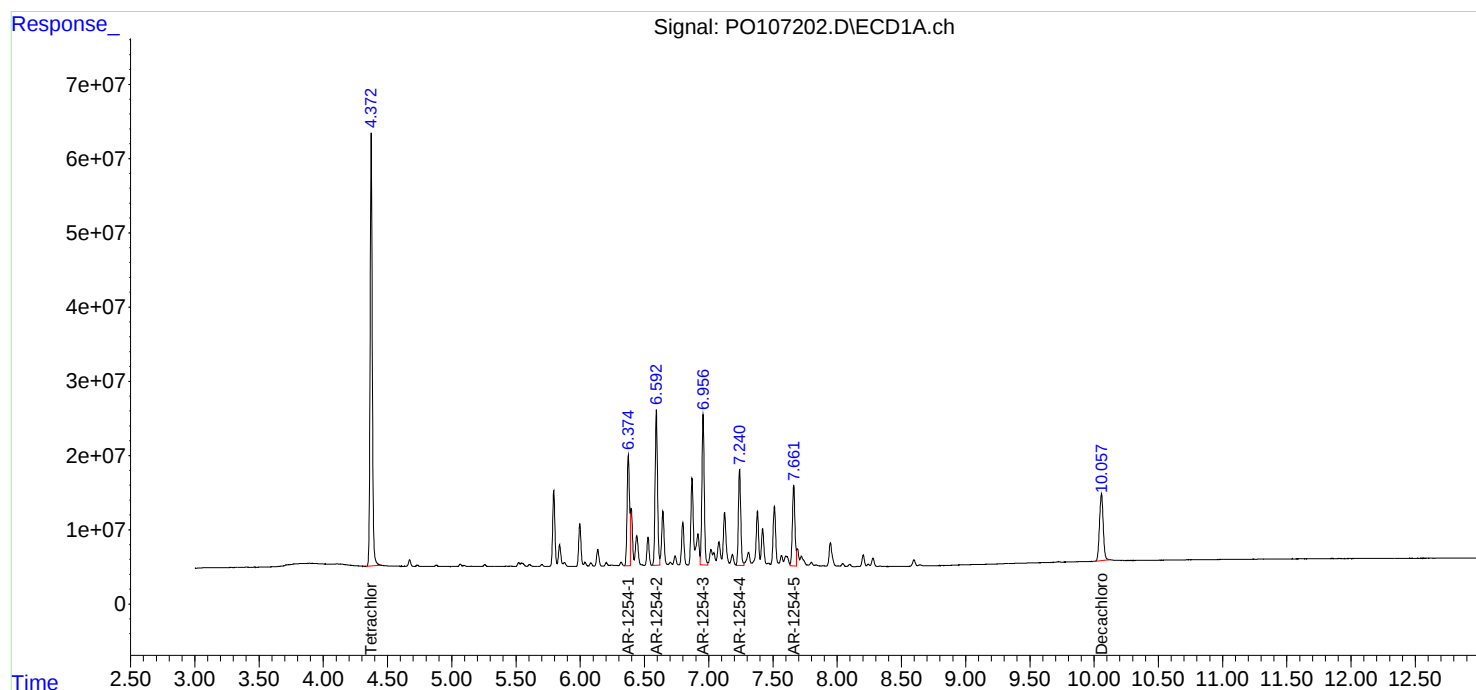

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 00:11
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:22:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	459.2E6	167.7E6	50.000	50.000
2) SA Decachlor...	10.059	8.637	125.4E6	138.7E6	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	6.375	5.526	132.5E6	82774166	500.000	500.000
27) L6 AR-1254-2	6.593	5.673	186.5E6	72273461	500.000	500.000
28) L6 AR-1254-3	6.957	6.077	178.0E6	116.1E6	500.000	500.000
29) L6 AR-1254-4	7.241	6.304	113.6E6	65662675	500.000	500.000
30) L6 AR-1254-5	7.662	6.721	102.9E6	97689052	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 00:11
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:22:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

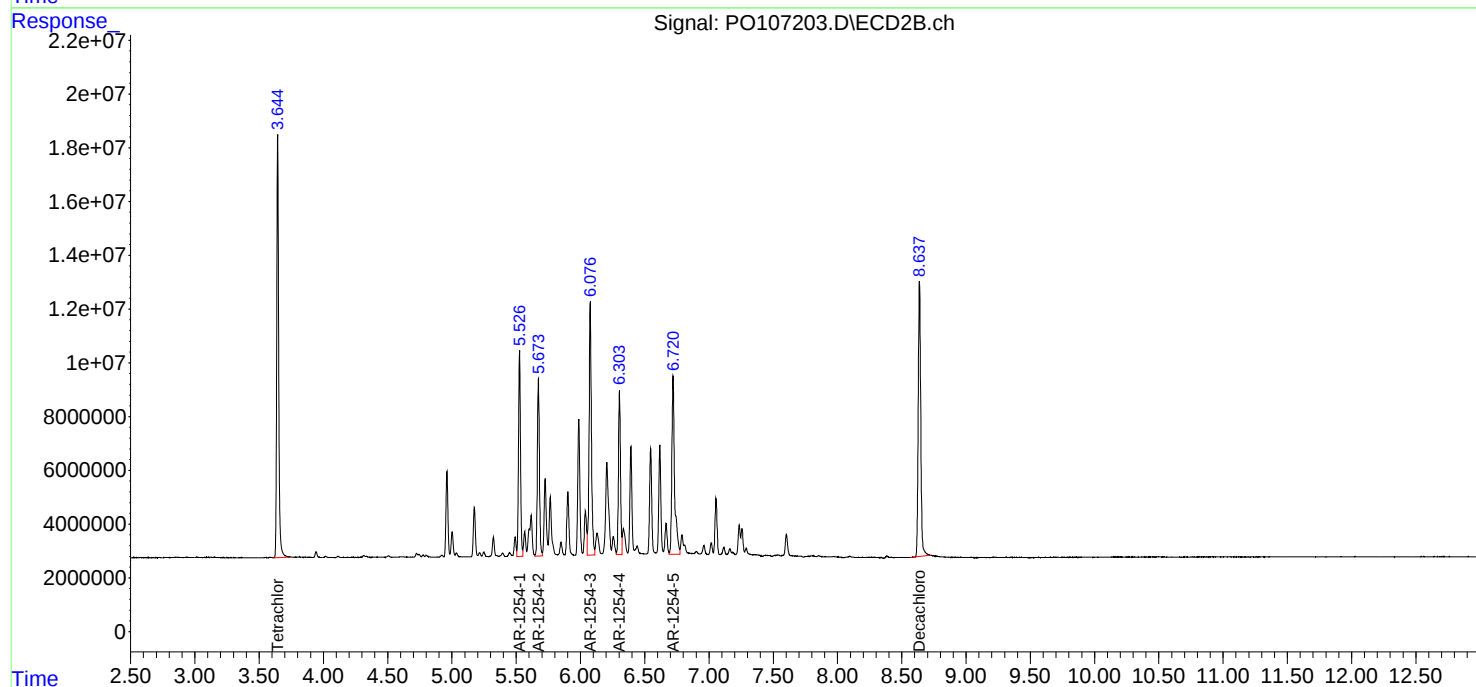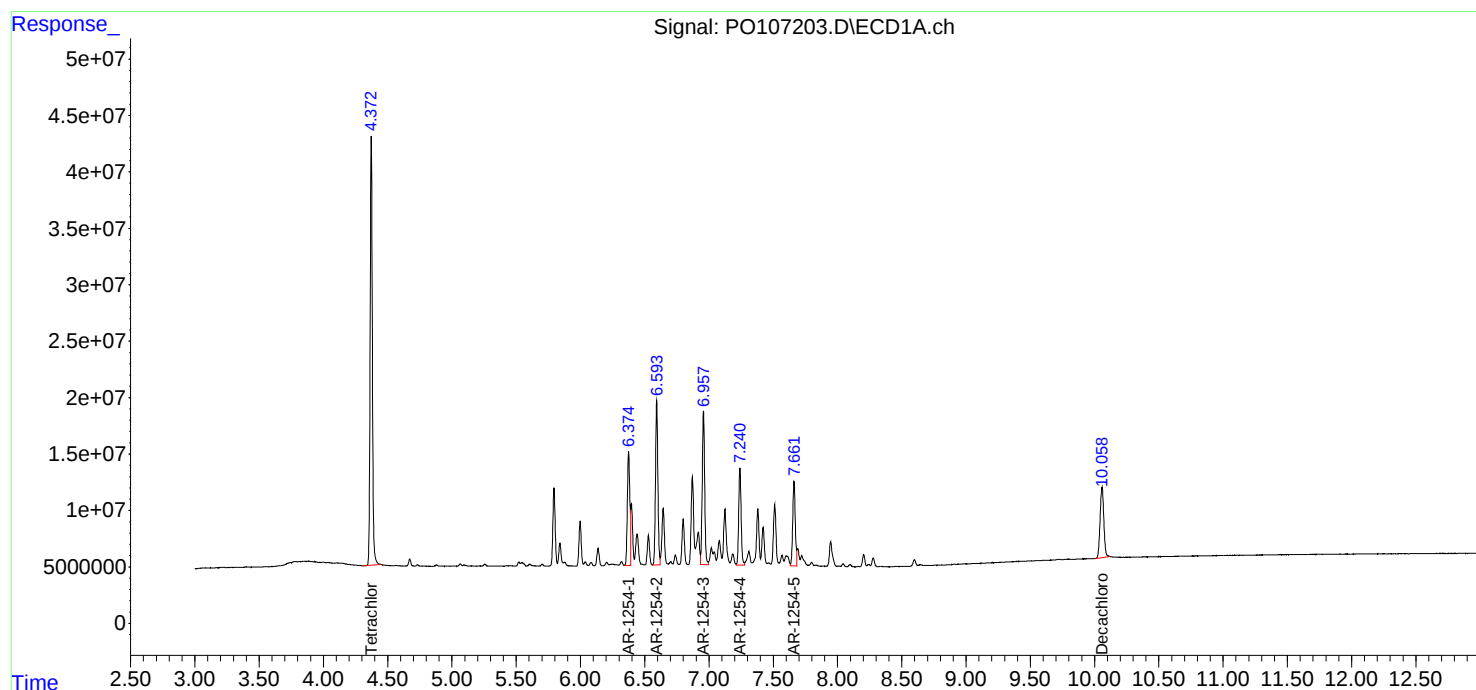

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 00:29
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:23:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	237.7E6	84055907	25.883	25.060
2) SA Decachlor...	10.058	8.638	65039455	70920394	25.927	25.571
Target Compounds						
26) L6 AR-1254-1	6.374	5.527	71547490	42929426	269.998	259.317
27) L6 AR-1254-2	6.593	5.674	100.3E6	37831493	268.904	261.725
28) L6 AR-1254-3	6.956	6.078	94624615	59643812	265.867	256.849
29) L6 AR-1254-4	7.241	6.305	60632555	33801761	266.883	257.389
30) L6 AR-1254-5	7.662	6.721	55034918	50297216	267.330	257.435



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 00:29
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:23:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

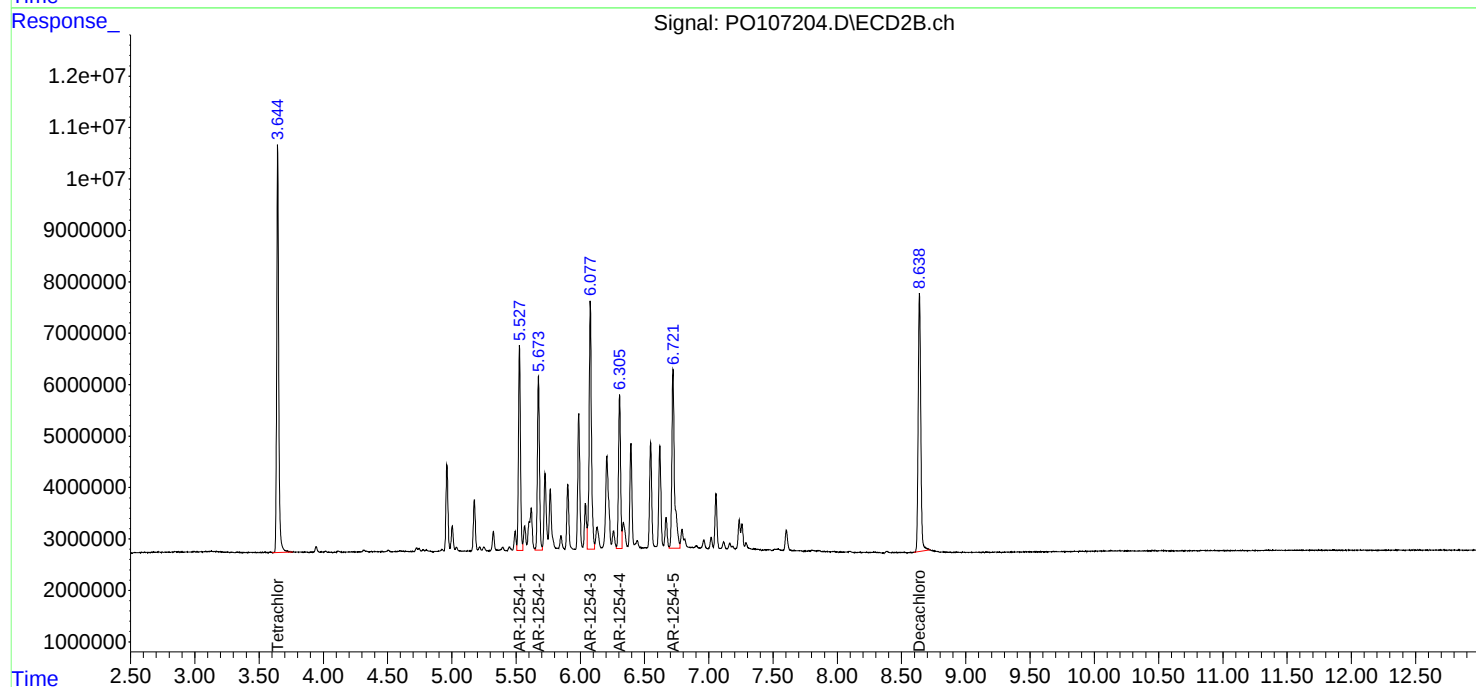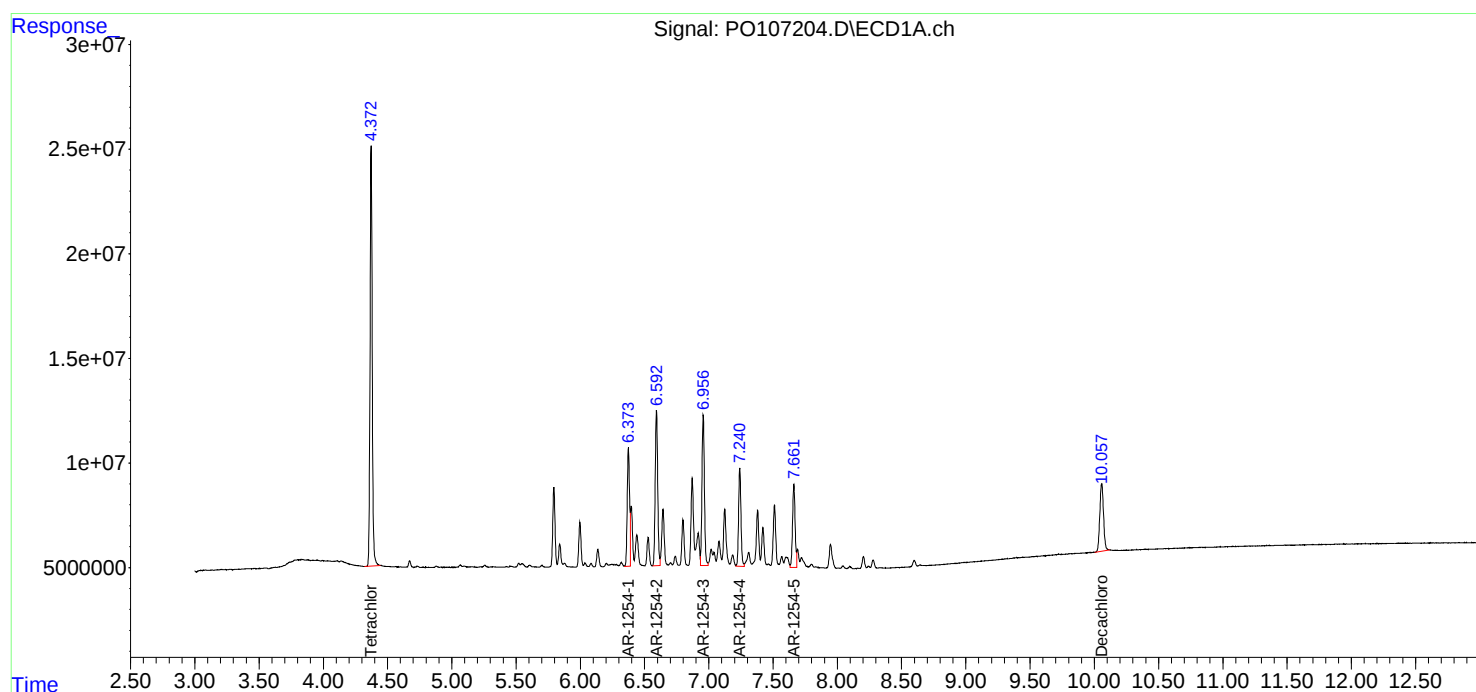

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 00:47
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:23:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	43957547	14653198	4.786	4.369
2) SA Decachlor...	10.057	8.638	11796837	12993699	4.703	4.685
Target Compounds						
26) L6 AR-1254-1	6.375	5.527	14457853	8148243	54.560	49.220
27) L6 AR-1254-2	6.593	5.674	20149788	7410157	54.016	51.265
28) L6 AR-1254-3	6.956	6.077	18631522	10943354	52.349	47.126
29) L6 AR-1254-4	7.241	6.304	12202348	6104594	53.710	46.485
30) L6 AR-1254-5	7.662	6.721	10827332	8581830	52.593	43.924



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 00:47
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:23:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

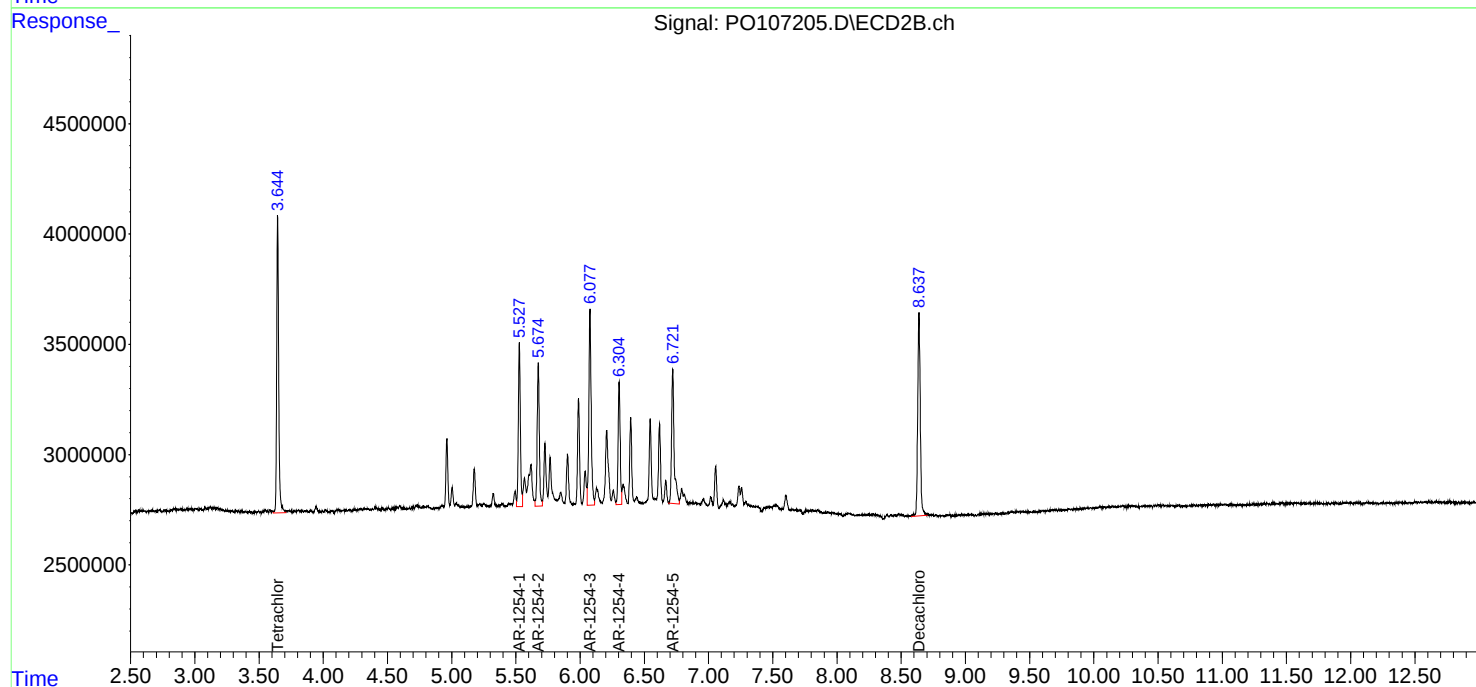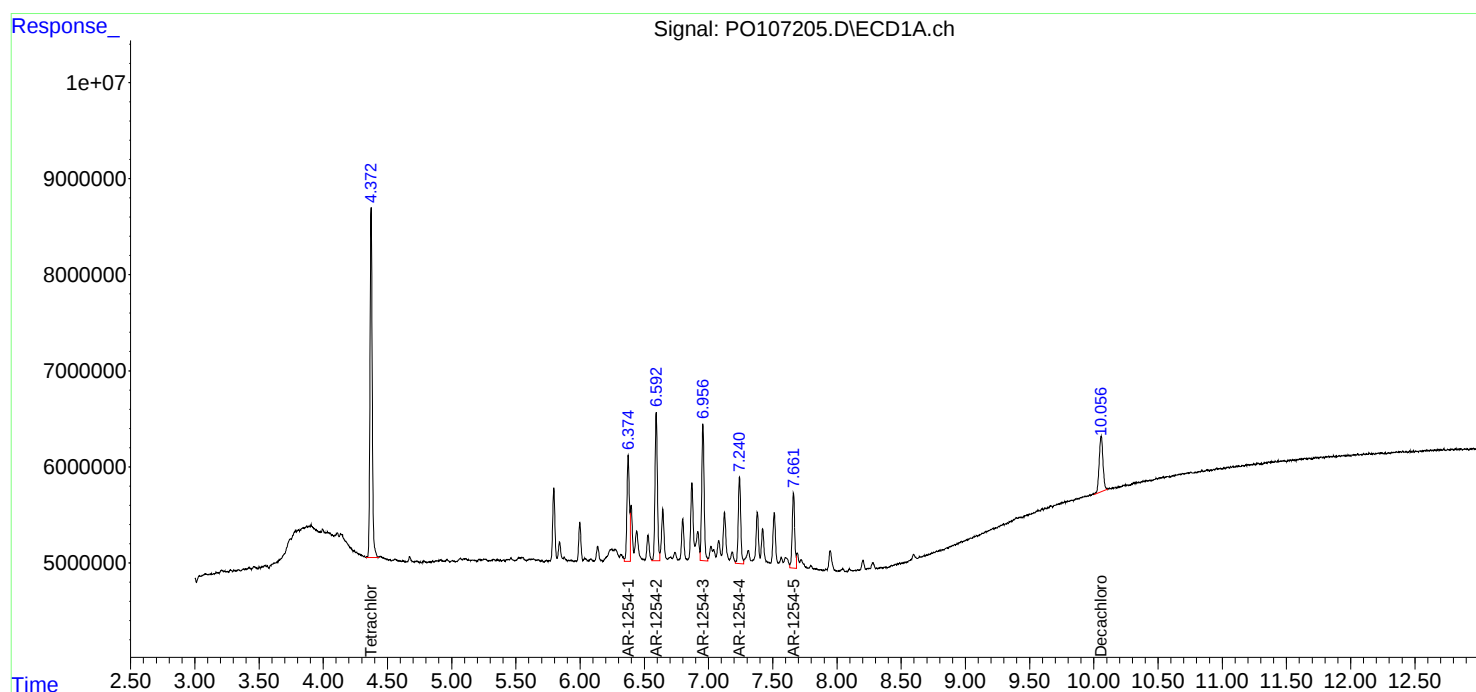

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 01:05
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:32:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:31:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	446.6E6	163.0E6	50.000	50.000
2) SA Decachlor...	10.059	8.638	123.1E6	135.8E6	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	7.742	6.759	122.8E6	106.4E6	500.000	500.000
37) L8 AR-1262-2	8.279	7.258	154.7E6	181.7E6	500.000	500.000
38) L8 AR-1262-3	8.592	7.541	104.6E6	68691960	500.000	500.000
39) L8 AR-1262-4	8.677	7.605	81533074	132.3E6	500.000	500.000
40) L8 AR-1262-5	9.315	8.096	51381891	56416259	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 01:05
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:32:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:31:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

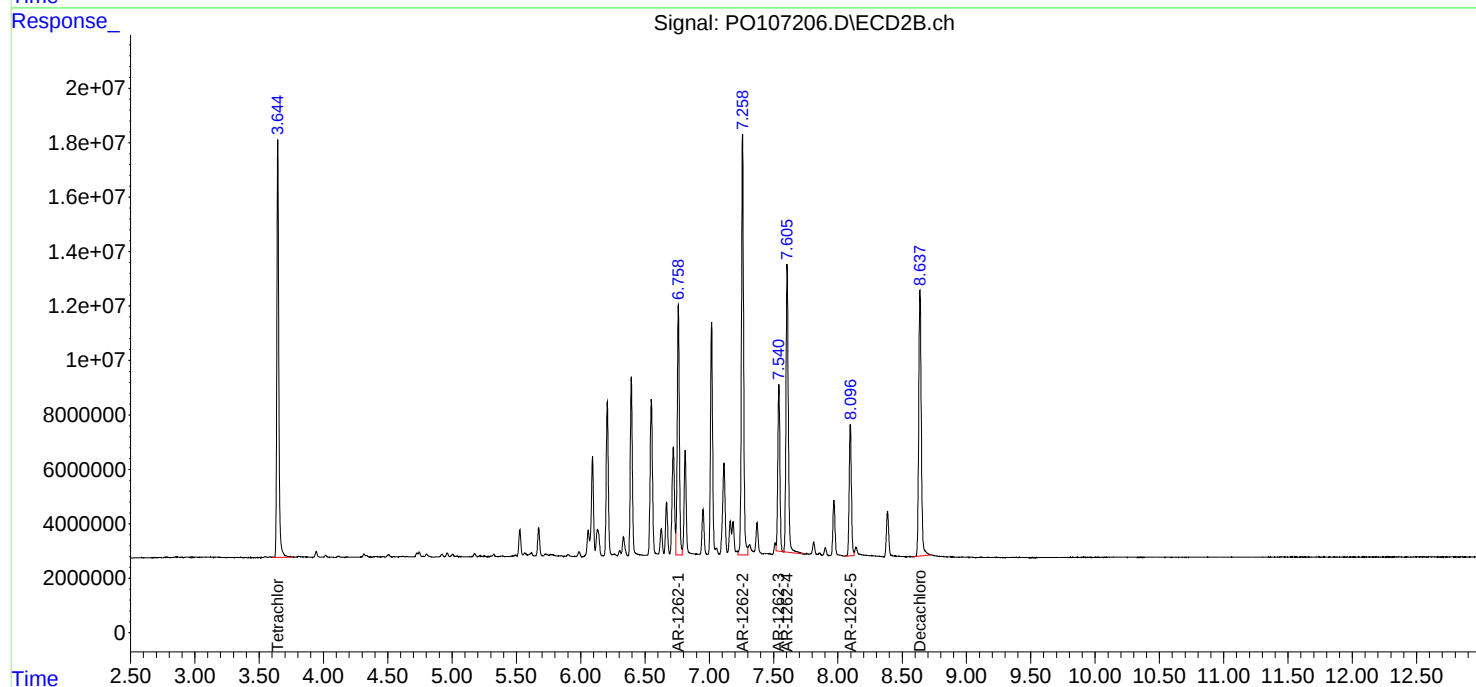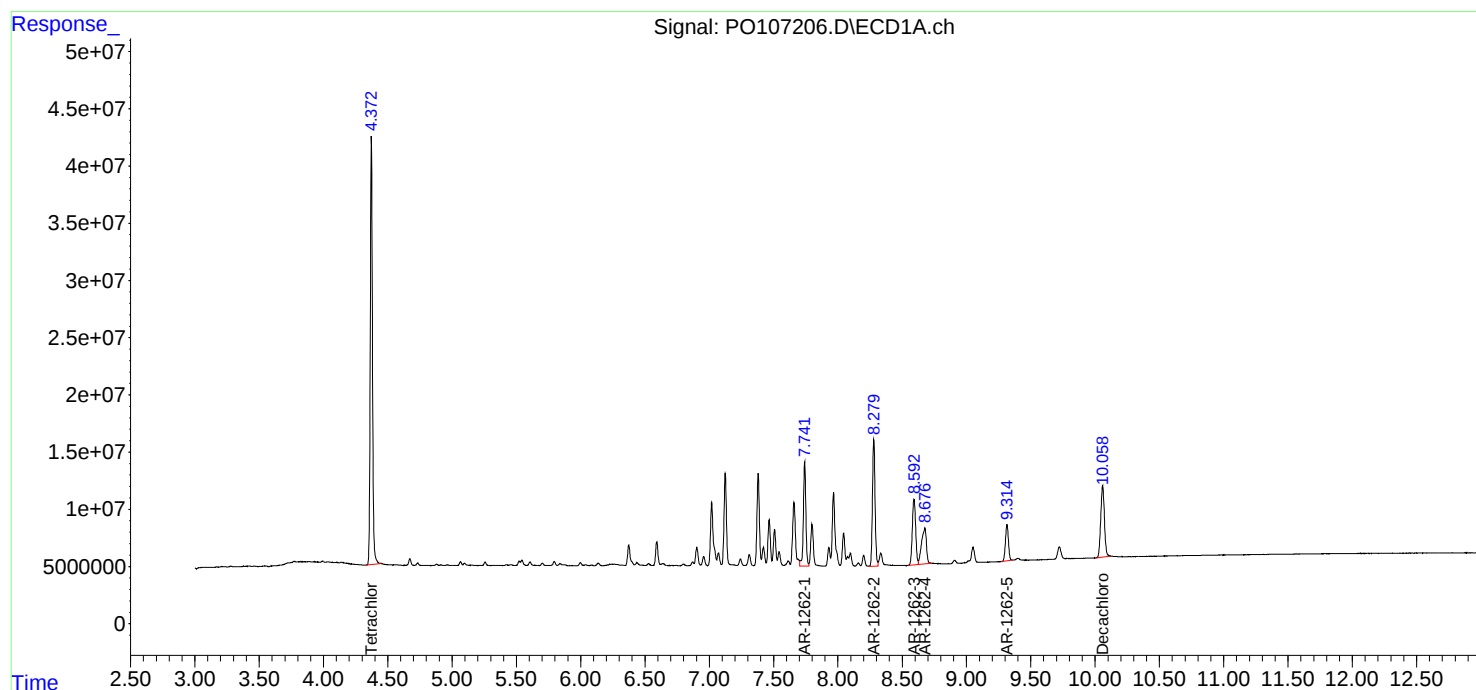

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 01:23
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:40:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	914.0E6	344.0E6	98.153	100.708
2) SA Decachlor...	10.057	8.639	407.4E6	487.4E6	96.045	101.044
Target Compounds						
41) L9 AR-1268-1	8.587	7.541	351.9E6	419.2E6	965.004	1012.873
42) L9 AR-1268-2	8.679	7.606	313.1E6	389.7E6	963.780	1016.048
43) L9 AR-1268-3	8.907	7.812	272.2E6	345.3E6	963.260	1016.931
44) L9 AR-1268-4	9.313	8.097	112.2E6	129.1E6	978.396	1014.319
45) L9 AR-1268-5	9.721	8.386	836.7E6	1049.2E6	987.735	1031.617



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 01:23
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:40:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

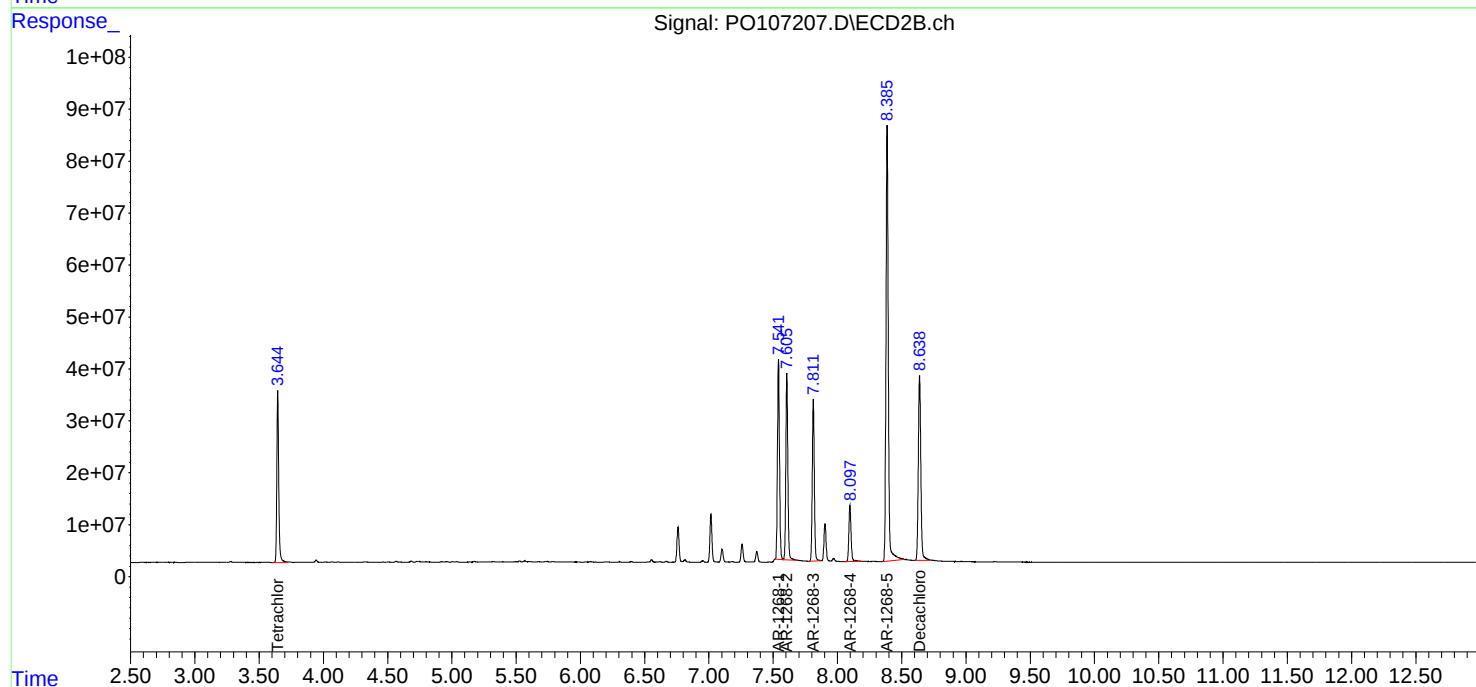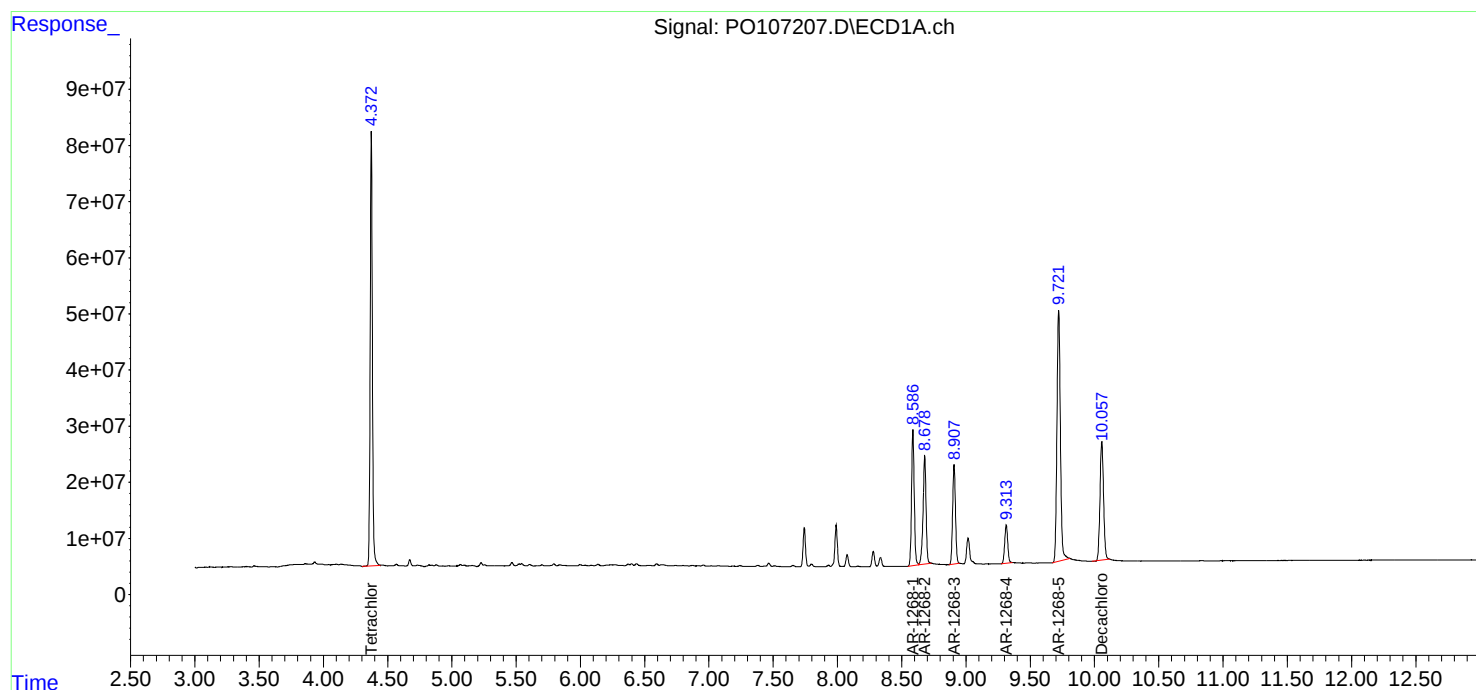

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 01:41
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:40:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	670.2E6	249.7E6	71.974	73.105
2) SA Decachlor...	10.058	8.638	310.2E6	355.5E6	73.131	73.693
Target Compounds						
41) L9 AR-1268-1	8.587	7.541	264.3E6	307.5E6	724.887	742.983
42) L9 AR-1268-2	8.678	7.605	235.9E6	285.1E6	726.056	743.309
43) L9 AR-1268-3	8.908	7.812	204.6E6	253.4E6	723.835	746.228
44) L9 AR-1268-4	9.312	8.096	83445833	95583754	727.421	750.941
45) L9 AR-1268-5	9.722	8.386	624.8E6	764.5E6	737.635	751.645



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 01:41
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:40:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

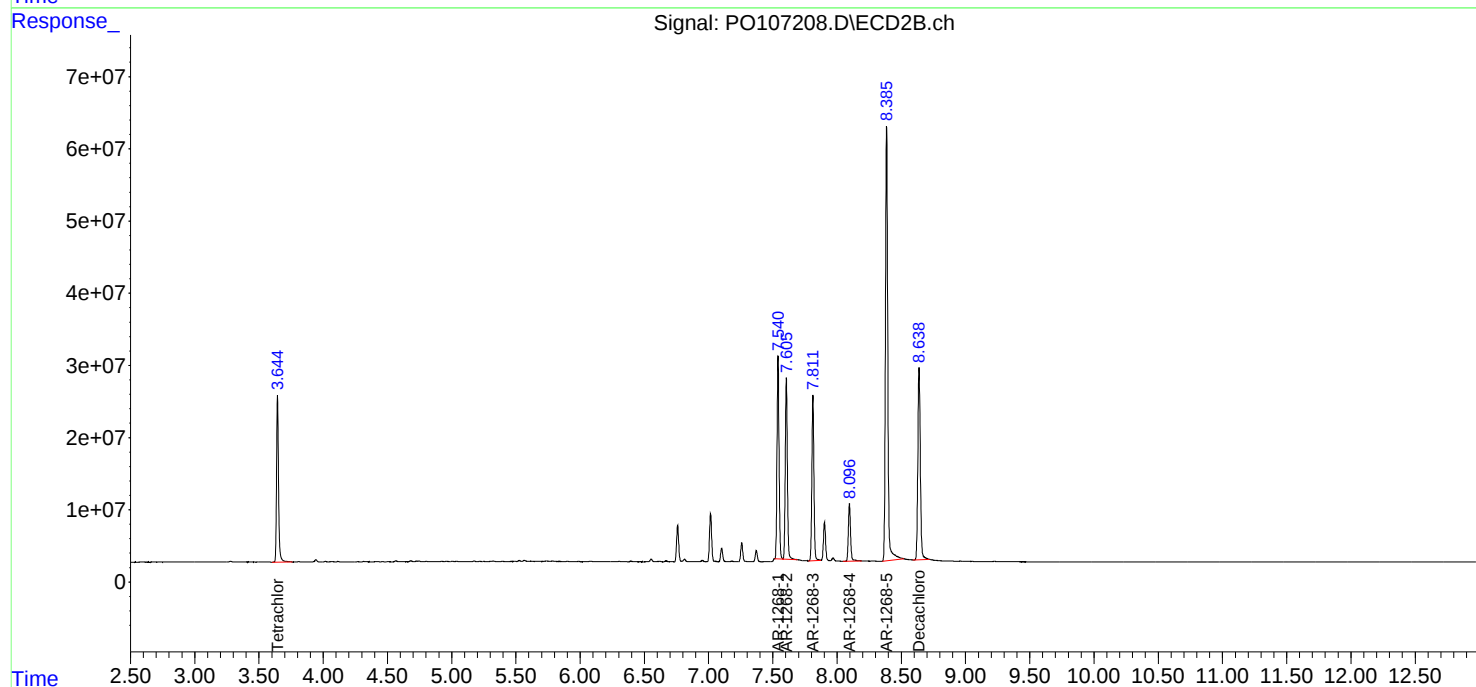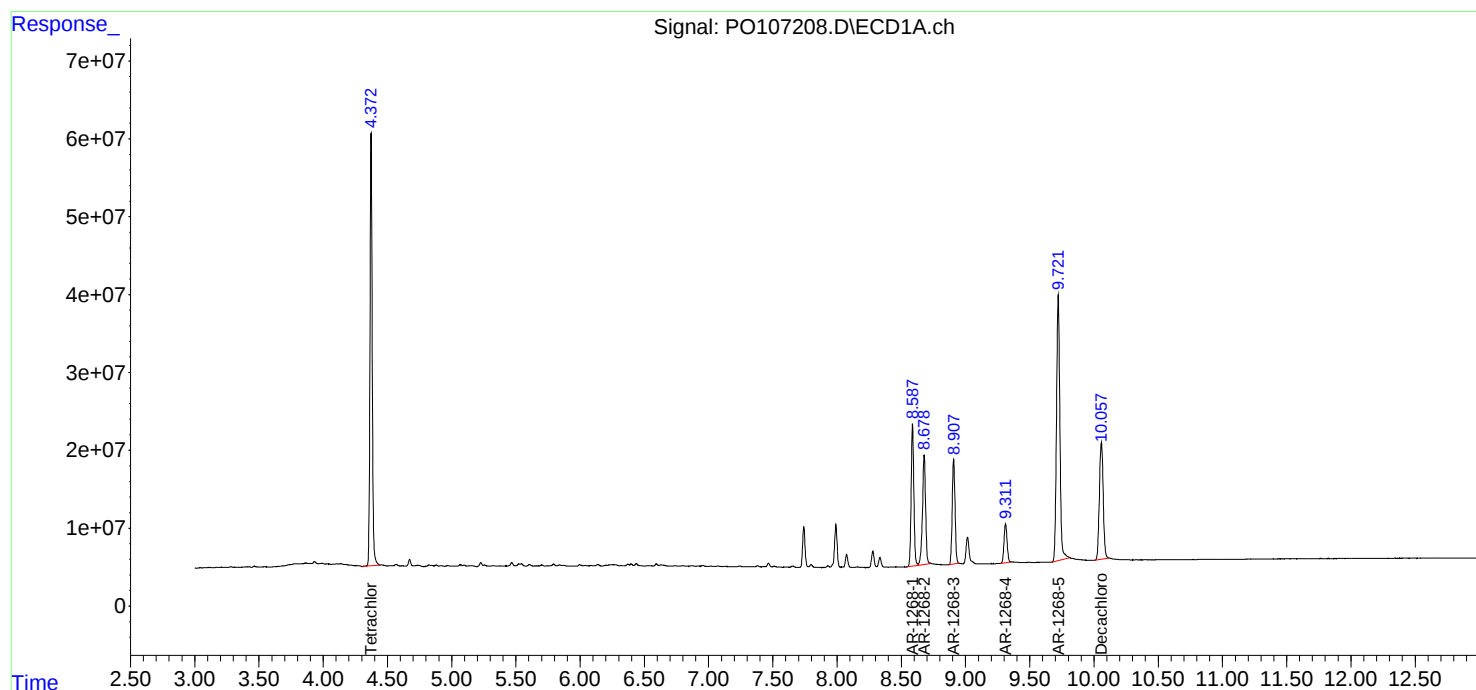

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 01:59
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:40:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	465.6E6	170.8E6	50.000	50.000
2) SA Decachlor...	10.057	8.637	212.1E6	241.2E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	8.587	7.541	182.3E6	206.9E6	500.000	500.000
42) L9 AR-1268-2	8.678	7.605	162.4E6	191.8E6	500.000	500.000
43) L9 AR-1268-3	8.907	7.811	141.3E6	169.8E6	500.000	500.000
44) L9 AR-1268-4	9.312	8.096	57357297	63642681	500.000	500.000
45) L9 AR-1268-5	9.721	8.385	423.5E6	508.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 01:59
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:40:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

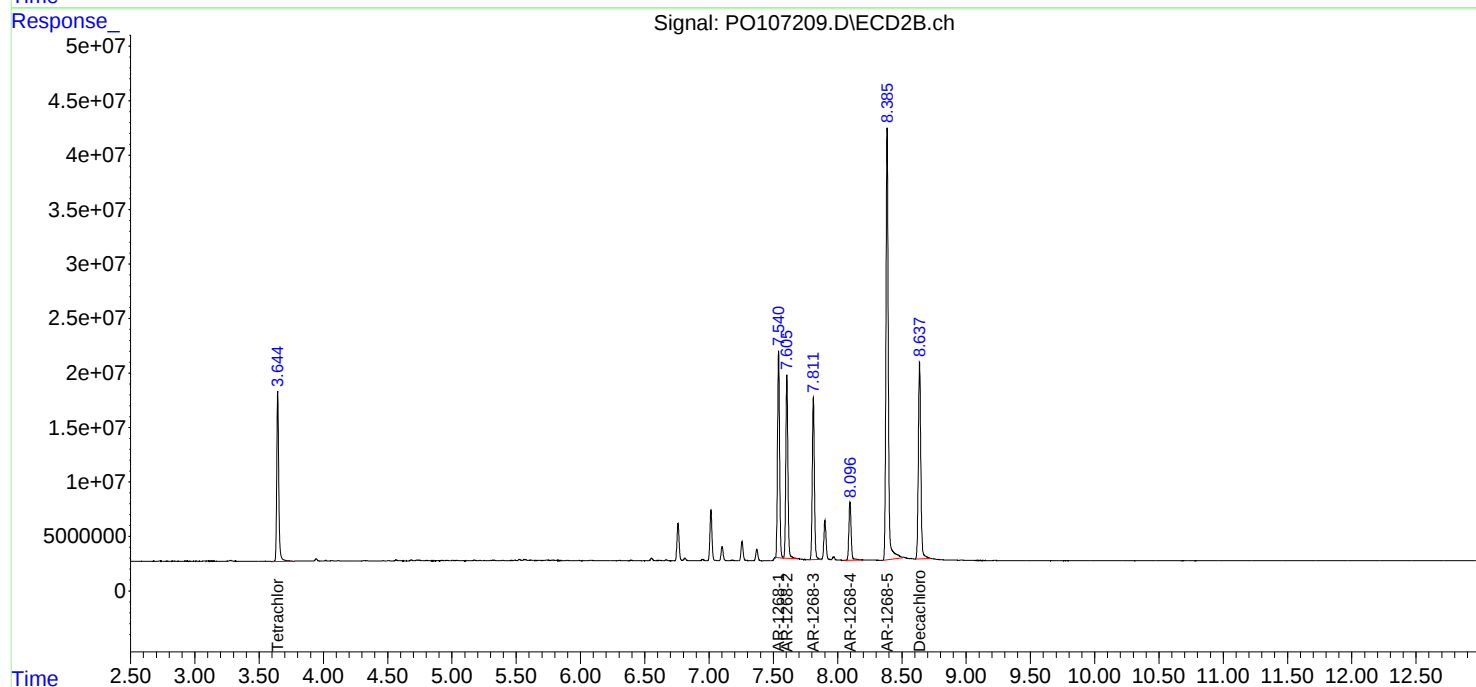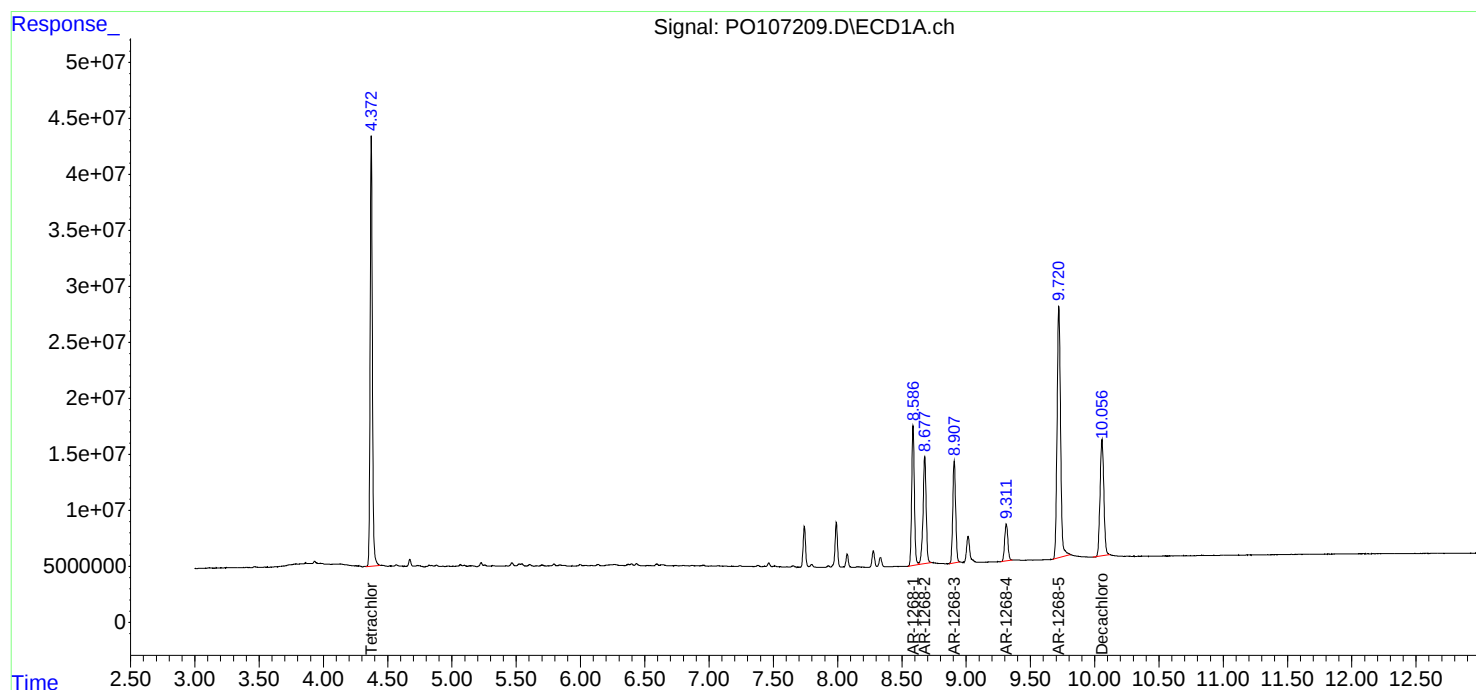

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 02:18
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:21:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	237.4E6	83283643	25.493	24.380
2) SA Decachlor...	10.058	8.638	110.0E6	122.3E6	25.930	25.345
Target Compounds						
41) L9 AR-1268-1	8.588	7.541	95440132	102.7E6	261.750	248.179
42) L9 AR-1268-2	8.679	7.606	84909424	94674968	261.370	246.859
43) L9 AR-1268-3	8.908	7.812	73384675	84688940	259.658	249.426
44) L9 AR-1268-4	9.314	8.097	29107021	32315199	253.734	253.880
45) L9 AR-1268-5	9.721	8.386	216.1E6	249.1E6	255.104	244.896



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 02:18
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:21:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

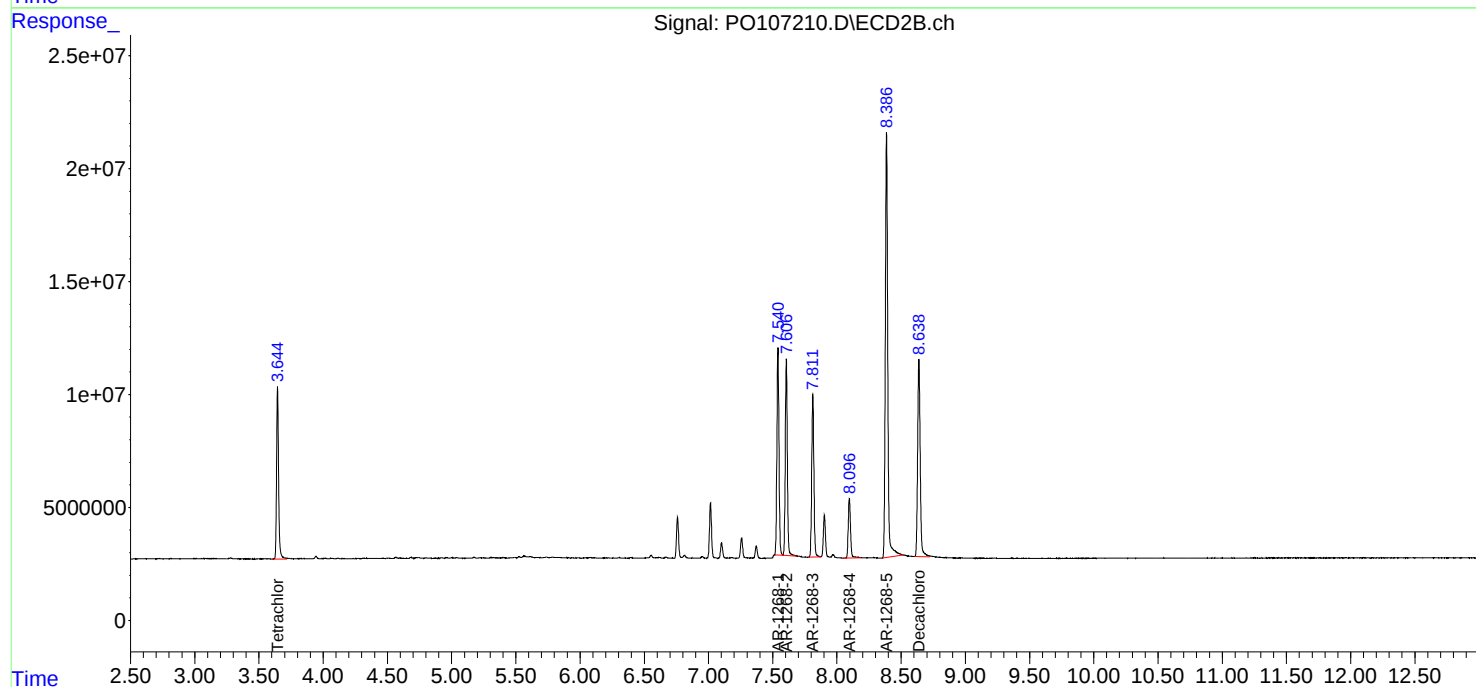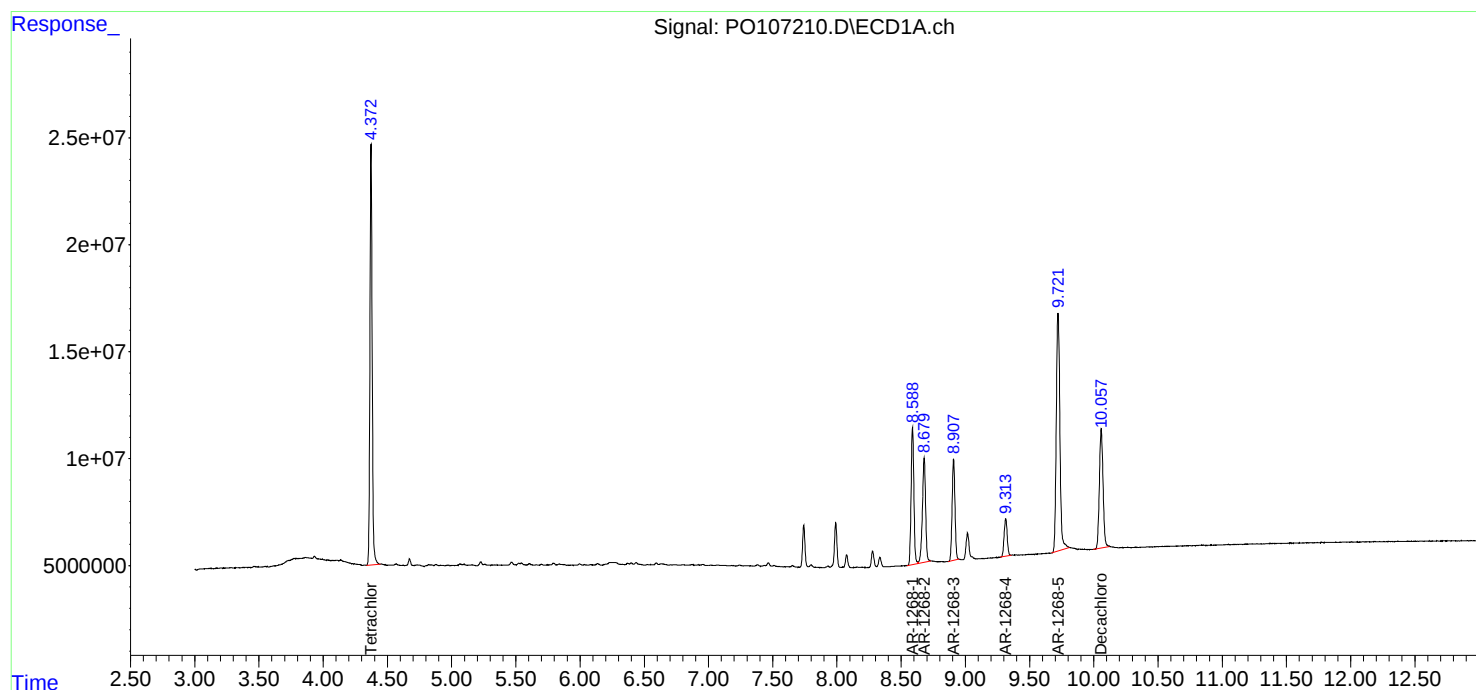

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 02:36
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/16/2024
 Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:22:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	44759505	14819032	4.807	4.338
2) SA Decachlor...	10.056	8.638	20020423	22152727	4.720	4.593
Target Compounds						
41) L9 AR-1268-1	8.587	7.541	18469024	18447765	50.652m	44.575
42) L9 AR-1268-2	8.679	7.606	16014978	16717280	49.298	43.589
43) L9 AR-1268-3	8.908	7.811	13783097	15350219	48.769	45.209
44) L9 AR-1268-4	9.314	8.097	5072917	5687474	44.222	44.683
45) L9 AR-1268-5	9.723	8.385	39053378	42842014	46.104	42.123

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 02:36
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:22:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

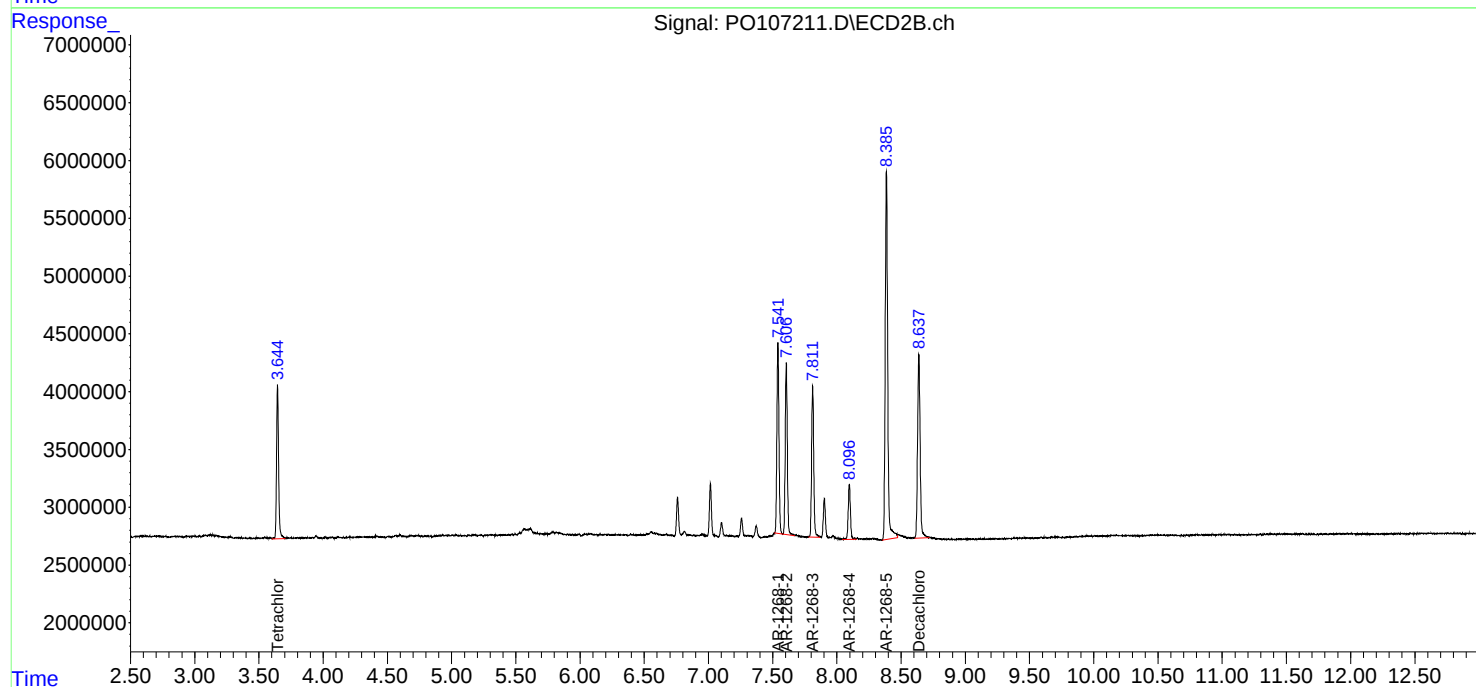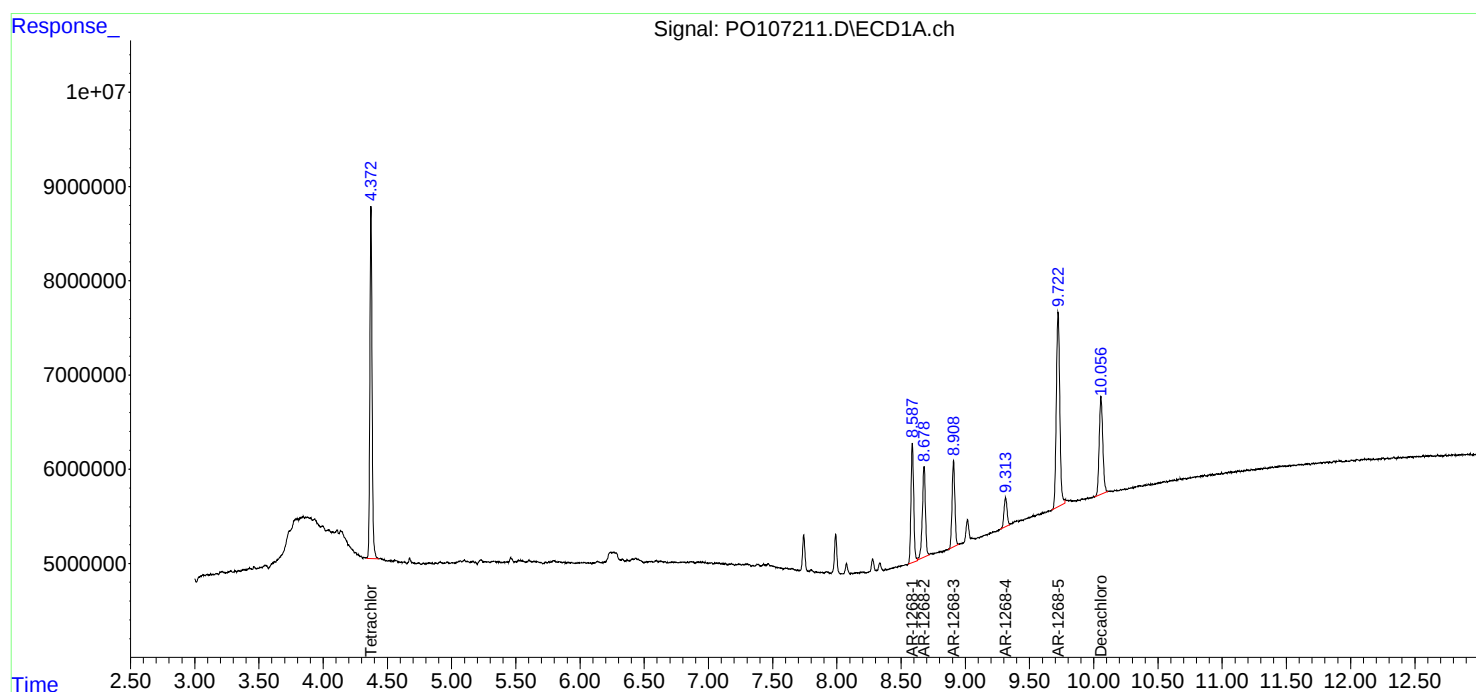

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 02:54
 Operator : YP/AJ
 Sample : P0101524ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:33:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:32:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	465.3E6	164.4E6	51.058	51.086
2) SA Decachlor...	10.056	8.638	123.9E6	136.1E6	50.497	49.626
Target Compounds						
3) L1 AR-1016-1	5.521	4.726	134.9E6	51843655	500.111	502.042
4) L1 AR-1016-2	5.543	4.745	197.8E6	72270469	498.259	512.674
5) L1 AR-1016-3	5.606	4.920	128.2E6	39765886	510.233	504.992
6) L1 AR-1016-4	5.702	4.962	100.3E6	33242228	520.863	502.845
7) L1 AR-1016-5	5.997	5.175	96027789	42039253	525.737	511.838
31) L7 AR-1260-1	7.123	6.207	127.8E6	78048903	494.246	503.040
32) L7 AR-1260-2	7.380	6.394	129.5E6	92023271	492.099	522.516
33) L7 AR-1260-3	7.741	6.547	88394667	86099269	491.778	513.265
34) L7 AR-1260-4	7.966	7.018	84877632	73152631	483.623	505.614
35) L7 AR-1260-5	8.279	7.258	138.1E6	168.0E6	485.508	510.033



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 02:54
Operator : YP/AJ
Sample : PO101524ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:33:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:32:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

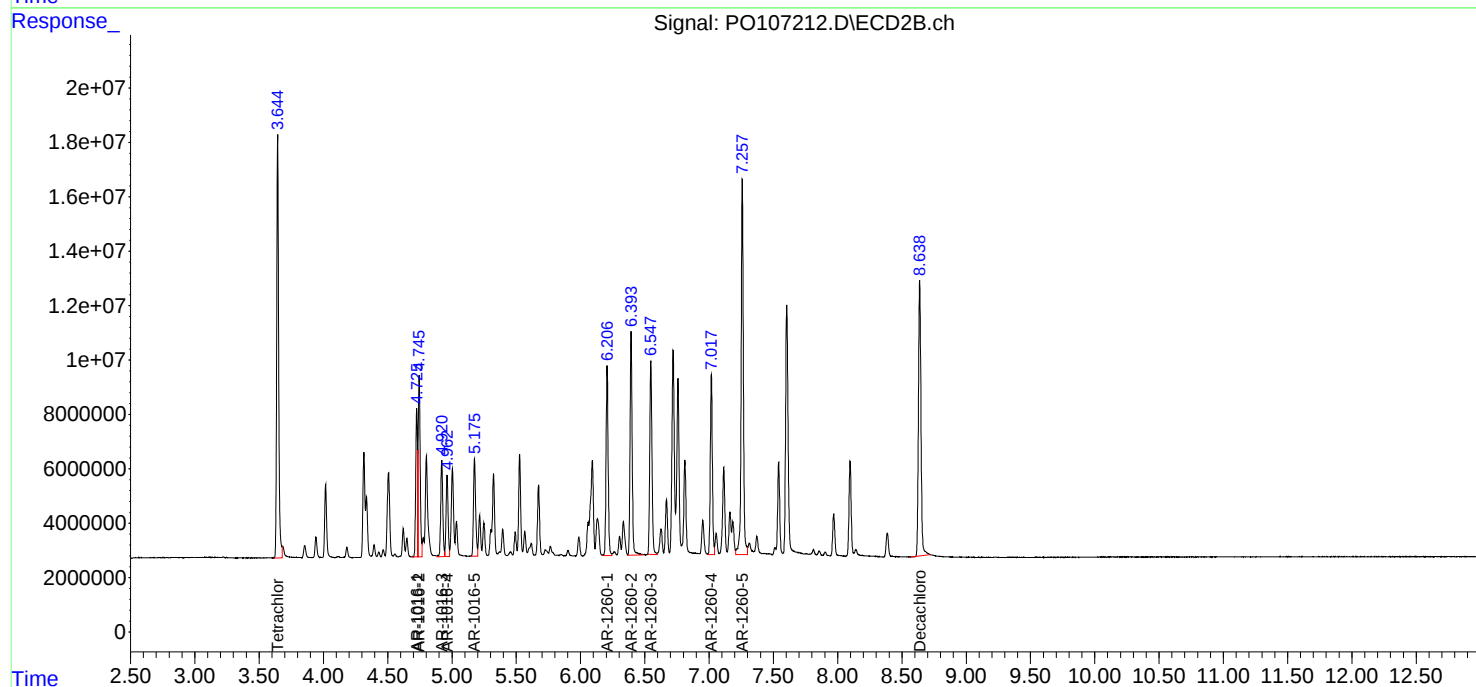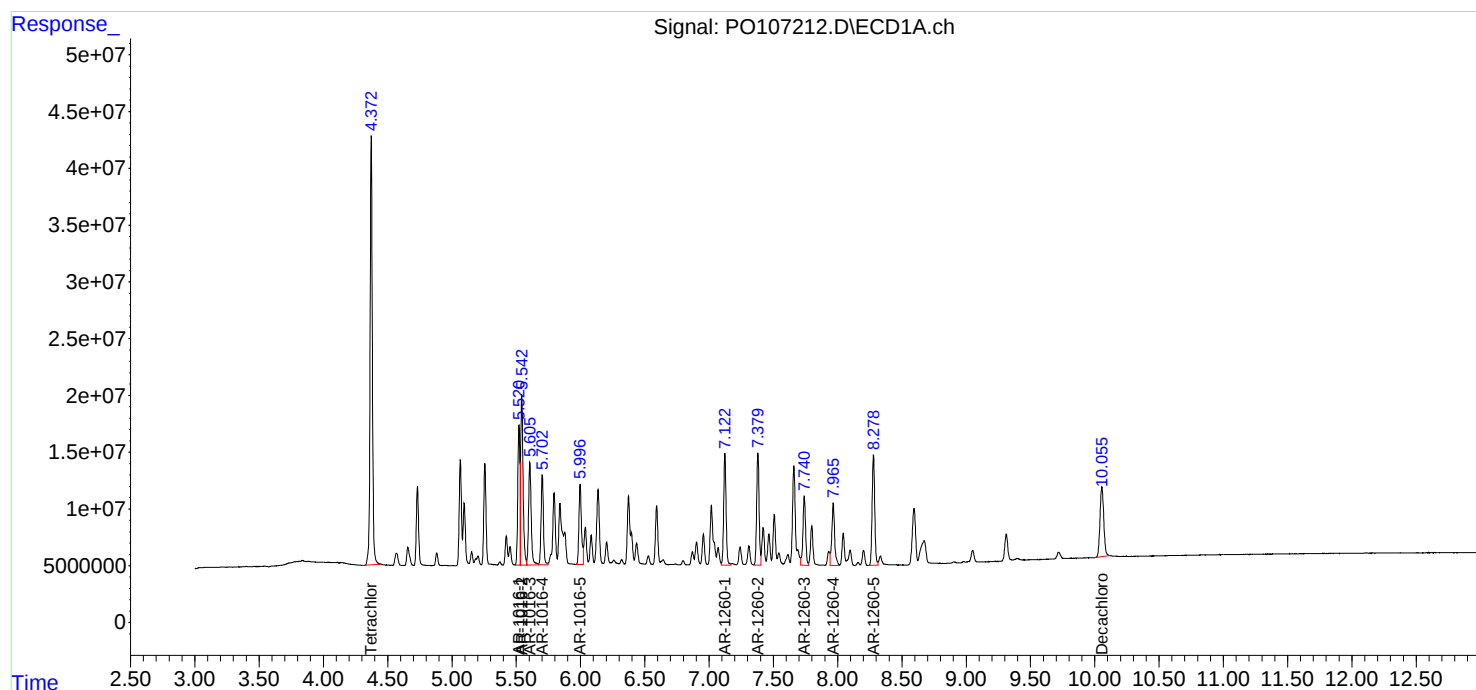

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 03:12
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:37:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:36:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	462.5E6	169.0E6	51.003	52.312
2) SA Decachlor...	10.058	8.637	124.4E6	137.6E6	50.838	50.298
Target Compounds						
16) L4 AR-1242-1	5.522	4.726	112.5E6	42391283	503.251	506.204
17) L4 AR-1242-2	5.544	4.745	161.7E6	59212746	499.677	512.049
18) L4 AR-1242-3	5.606	4.921	104.8E6	32647360	501.419	514.673
19) L4 AR-1242-4	5.703	5.004	80827975	32698937	505.157	510.527
20) L4 AR-1242-5	6.436	5.526	77500840	39282831	495.270	506.721



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 03:12
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:37:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:36:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

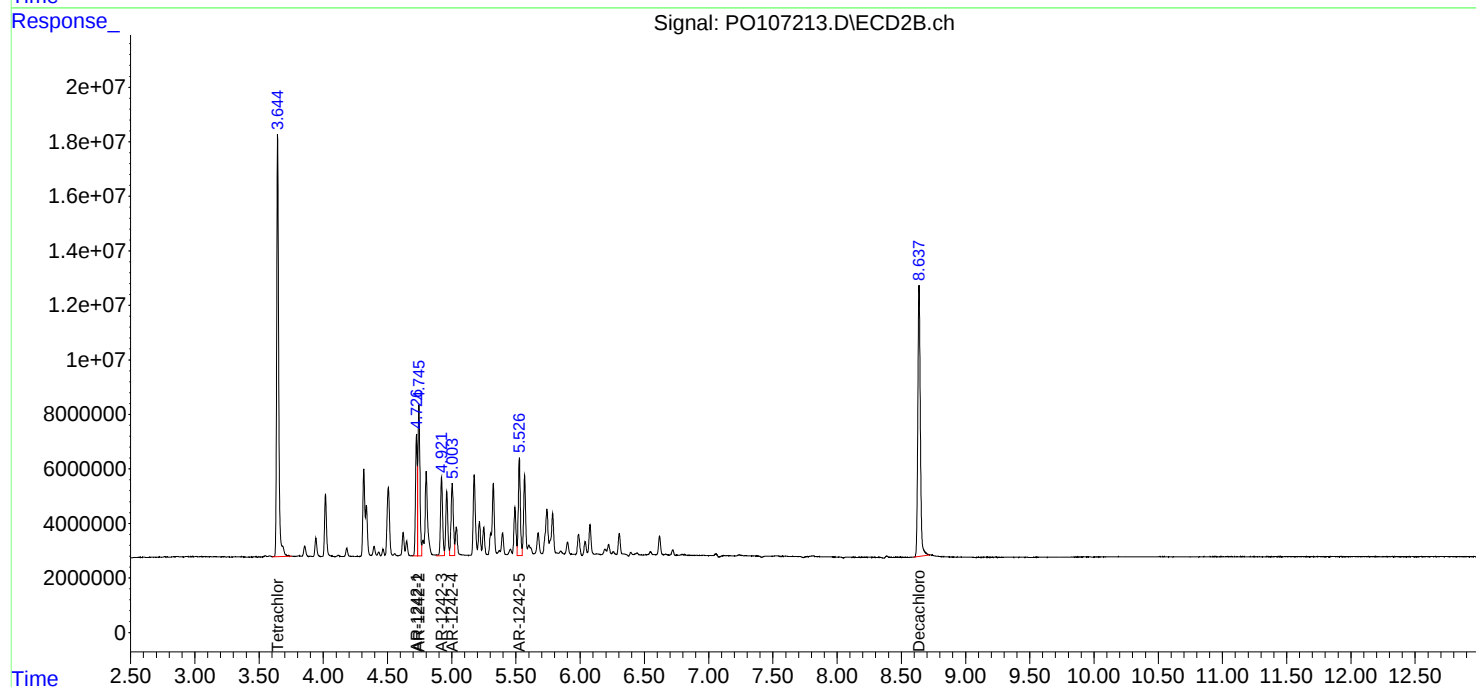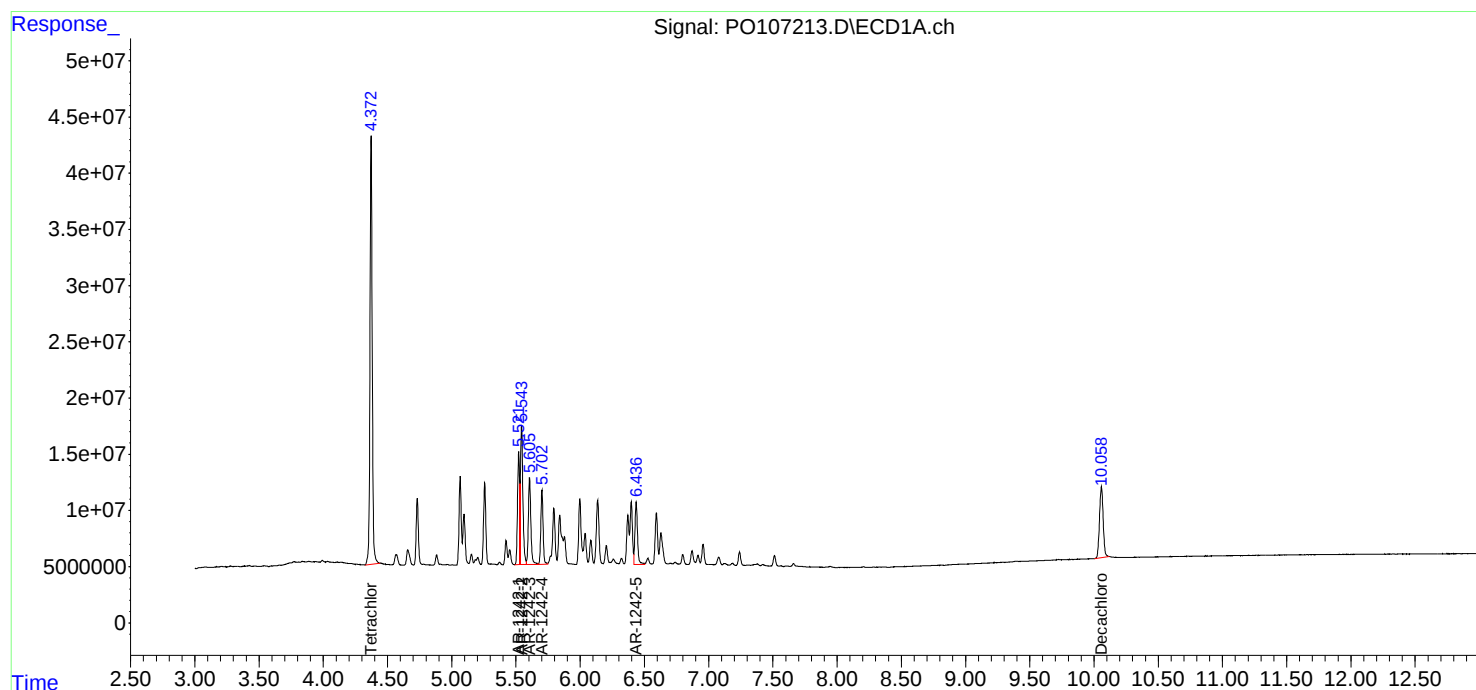

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
 Data File : PO107214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 03:30
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:41:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:40:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	468.2E6	171.8E6	51.242	52.316
2) SA Decachlor...	10.056	8.637	126.4E6	139.3E6	51.882	50.991
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	87306267	32470217	502.117	511.816
22) L5 AR-1248-2	5.794	4.962	126.0E6	46450269	498.018	507.736
23) L5 AR-1248-3	5.997	5.004	130.0E6	48736000	508.271	510.896
24) L5 AR-1248-4	6.397	5.175	129.0E6	57212370	500.494	510.195
25) L5 AR-1248-5	6.436	5.567	130.2E6	54714064	500.737	496.185



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 03:30
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:41:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:40:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

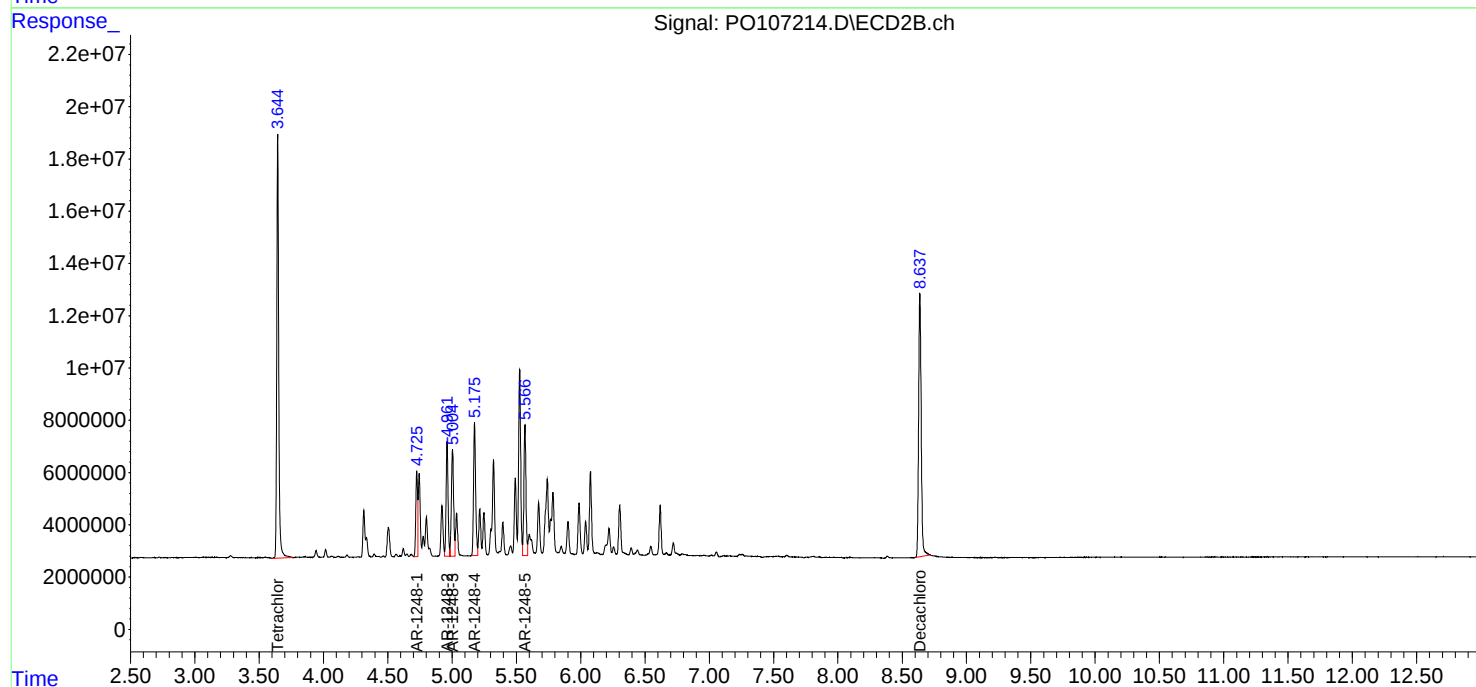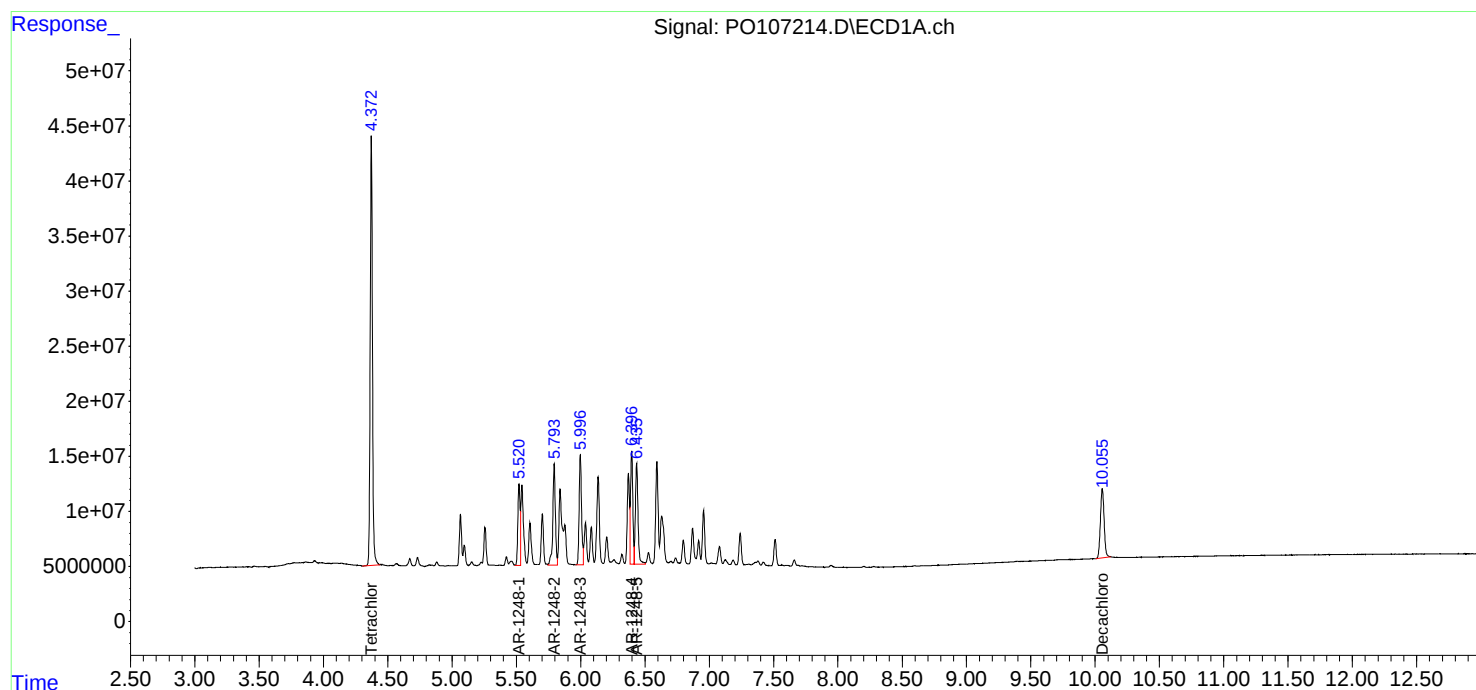

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 03:48
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:44:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:44:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	461.3E6	168.2E6	50.657	51.320
2) SA Decachlor...	10.057	8.638	125.1E6	138.4E6	51.131	50.597
Target Compounds						
26) L6 AR-1254-1	6.374	5.527	132.5E6	83096071	492.928	504.260
27) L6 AR-1254-2	6.592	5.673	186.6E6	72524753	494.424	500.299
28) L6 AR-1254-3	6.956	6.077	177.6E6	116.6E6	496.443	508.012
29) L6 AR-1254-4	7.242	6.304	112.6E6	65655140	490.851	507.289
30) L6 AR-1254-5	7.661	6.722	102.5E6	98535916	493.779	515.754



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 03:48
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:44:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:44:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

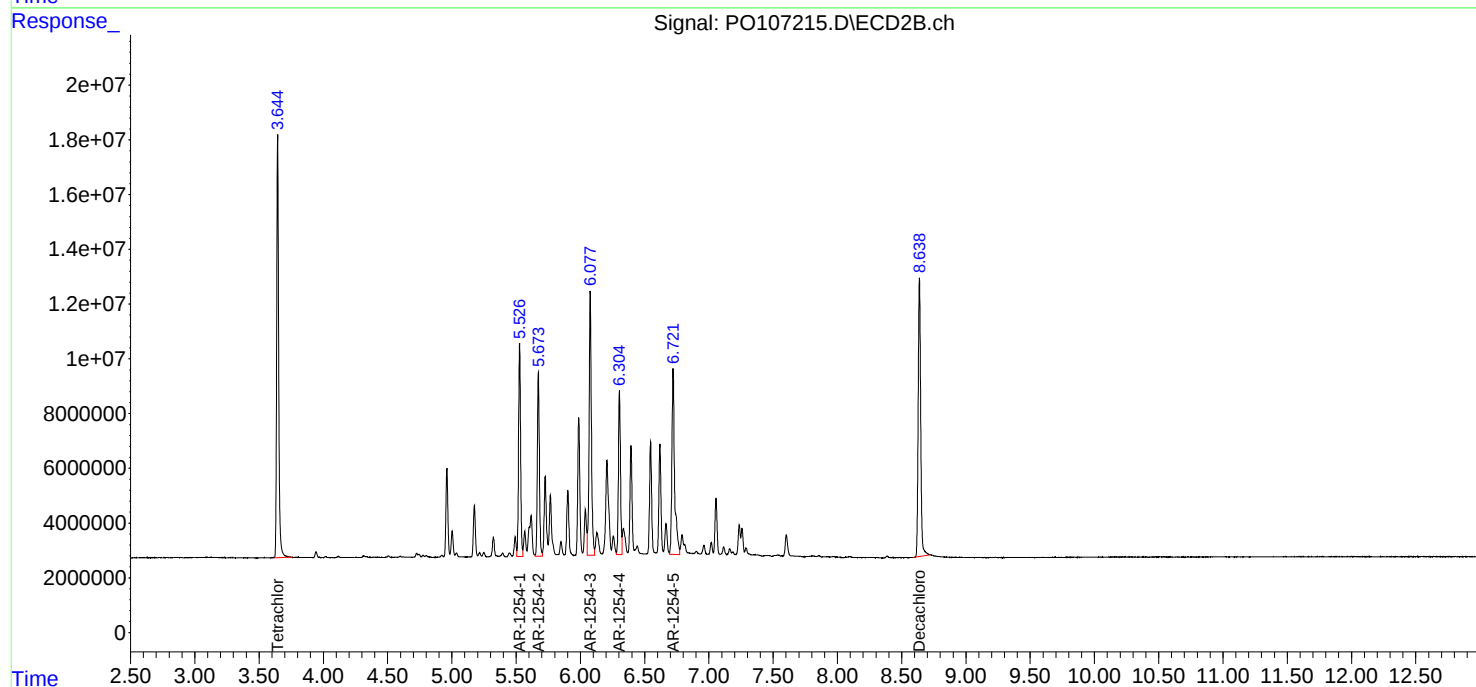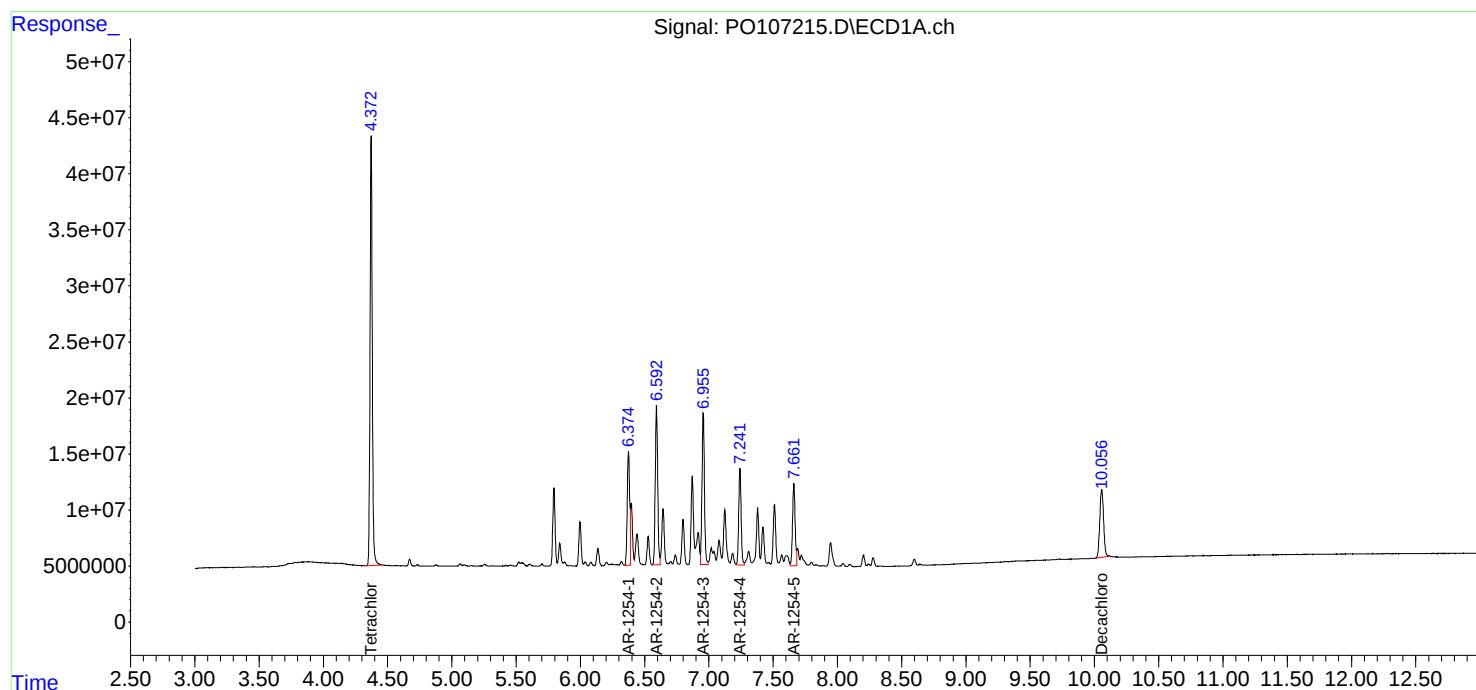

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 04:06
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:22:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	461.5E6	169.8E6	49.559	49.696
2) SA Decachlor...	10.057	8.638	214.2E6	240.5E6	50.485	49.870
Target Compounds						
41) L9 AR-1268-1	8.588	7.541	182.7E6	207.4E6	501.152	501.118
42) L9 AR-1268-2	8.678	7.606	163.0E6	192.3E6	501.726	501.439
43) L9 AR-1268-3	8.907	7.812	141.7E6	170.9E6	501.280	503.353
44) L9 AR-1268-4	9.313	8.096	57558867	64279608	501.757	505.004
45) L9 AR-1268-5	9.721	8.385	423.5E6	510.6E6	499.926	501.994



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 04:06
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524AR1268

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:22:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

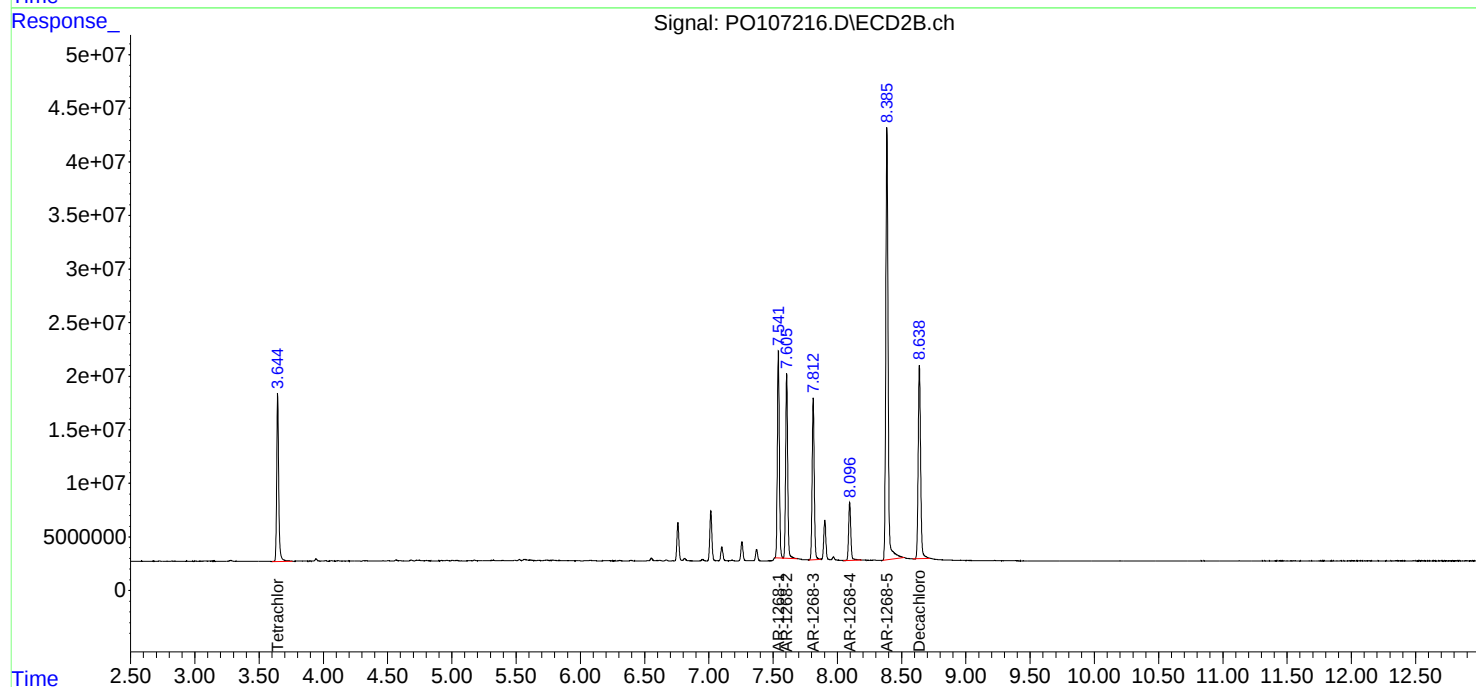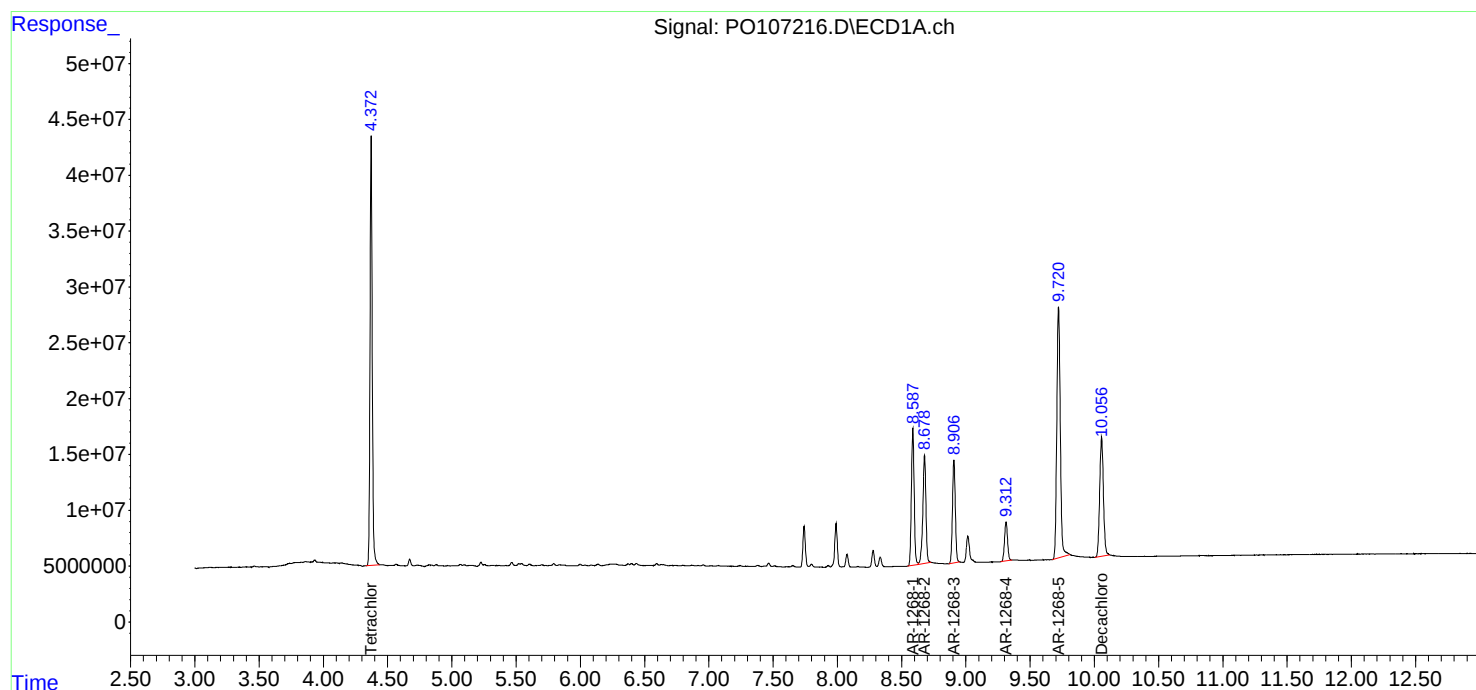



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Continuing Calib Date: 11/05/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 13:01 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.52	5.52	5.42	5.62	0.00
Aroclor-1016-2	(2)	5.54	5.55	5.45	5.65	0.01
Aroclor-1016-3	(3)	5.61	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.70	5.70	5.60	5.80	0.00
Aroclor-1016-5	(5)	6.00	6.00	5.90	6.10	0.00
Aroclor-1260-1	(1)	7.13	7.13	7.03	7.23	0.00
Aroclor-1260-2	(2)	7.38	7.38	7.28	7.48	0.00
Aroclor-1260-3	(3)	7.75	7.74	7.64	7.84	-0.01
Aroclor-1260-4	(4)	7.97	7.97	7.87	8.07	0.00
Aroclor-1260-5	(5)	8.29	8.28	8.18	8.38	-0.01
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.07	10.06	9.96	10.16	-0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Continuing Calib Date: 11/05/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 13:01 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.73	4.63	4.83	0.01
Aroclor-1016-2	(2)	4.74	4.75	4.65	4.85	0.01
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.17	5.18	5.08	5.28	0.01
Aroclor-1260-1	(1)	6.20	6.21	6.11	6.31	0.01
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.55	6.45	6.65	0.01
Aroclor-1260-4	(4)	7.02	7.02	6.92	7.12	0.01
Aroclor-1260-5	(5)	7.26	7.26	7.16	7.36	0.00
Tetrachloro-m-xylene		3.64	3.65	3.55	3.75	0.01
Decachlorobiphenyl		8.64	8.64	8.54	8.74	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL01 Date Analyzed: 11/05/2024

Lab Sample No.: AR1660CCC500 Data File : PO107682.D Time Analyzed: 13:01

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.522	5.423	5.623	496.940	500.000	-0.6
Aroclor-1016-2	5.544	5.445	5.645	490.020	500.000	-2.0
Aroclor-1016-3	5.607	5.507	5.707	482.070	500.000	-3.6
Aroclor-1016-4	5.704	5.604	5.804	497.190	500.000	-0.6
Aroclor-1016-5	5.999	5.899	6.099	491.380	500.000	-1.7
Aroclor-1260-1	7.128	7.026	7.226	479.190	500.000	-4.2
Aroclor-1260-2	7.384	7.282	7.482	525.610	500.000	5.1
Aroclor-1260-3	7.748	7.643	7.843	518.430	500.000	3.7
Aroclor-1260-4	7.972	7.868	8.068	541.150	500.000	8.2
Aroclor-1260-5	8.287	8.181	8.381	533.350	500.000	6.7
Decachlorobiphenyl	10.071	9.958	10.158	48.700	50.000	-2.6
Tetrachloro-m-xylene	4.371	4.274	4.474	49.030	50.000	-1.9



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL01 Date Analyzed: 11/05/2024

Lab Sample No.: AR1660CCC500 Data File : PO107682.D Time Analyzed: 13:01

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.723	4.626	4.826	536.740	500.000	7.3
Aroclor-1016-2	4.742	4.645	4.845	546.450	500.000	9.3
Aroclor-1016-3	4.918	4.821	5.021	521.460	500.000	4.3
Aroclor-1016-4	4.959	4.862	5.062	474.530	500.000	-5.1
Aroclor-1016-5	5.173	5.076	5.276	525.150	500.000	5.0
Aroclor-1260-1	6.204	6.107	6.307	492.350	500.000	-1.5
Aroclor-1260-2	6.391	6.294	6.494	507.430	500.000	1.5
Aroclor-1260-3	6.544	6.448	6.648	492.680	500.000	-1.5
Aroclor-1260-4	7.015	6.918	7.118	465.830	500.000	-6.8
Aroclor-1260-5	7.256	7.159	7.359	492.690	500.000	-1.5
Decachlorobiphenyl	8.636	8.539	8.739	47.340	50.000	-5.3
Tetrachloro-m-xylene	3.642	3.545	3.745	55.510	50.000	11.0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 13:01
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:43:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	446.9E6	178.7E6	49.034	55.510
2) SA Decachlor...	10.071	8.636	119.5E6	129.8E6	48.698	47.343
Target Compounds						
3) L1 AR-1016-1	5.522	4.723	134.1E6	55427318	496.937	536.745
4) L1 AR-1016-2	5.544	4.742	194.5E6	77032255	490.018	546.453
5) L1 AR-1016-3	5.607	4.918	121.1E6	41062755	482.072	521.461
6) L1 AR-1016-4	5.704	4.959	95764445	31370237	497.189	474.528
7) L1 AR-1016-5	5.999	5.173	89751554	43132865	491.376	525.153
31) L7 AR-1260-1	7.128	6.204	123.9E6	76390741	479.188	492.352
32) L7 AR-1260-2	7.384	6.391	138.4E6	89366514	525.609	507.431
33) L7 AR-1260-3	7.748	6.544	93184594	82646440	518.426	492.682
34) L7 AR-1260-4	7.972	7.015	94974133	67396734	541.151	465.831
35) L7 AR-1260-5	8.287	7.256	151.7E6	162.3E6	533.349	492.692



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 13:01
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:43:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

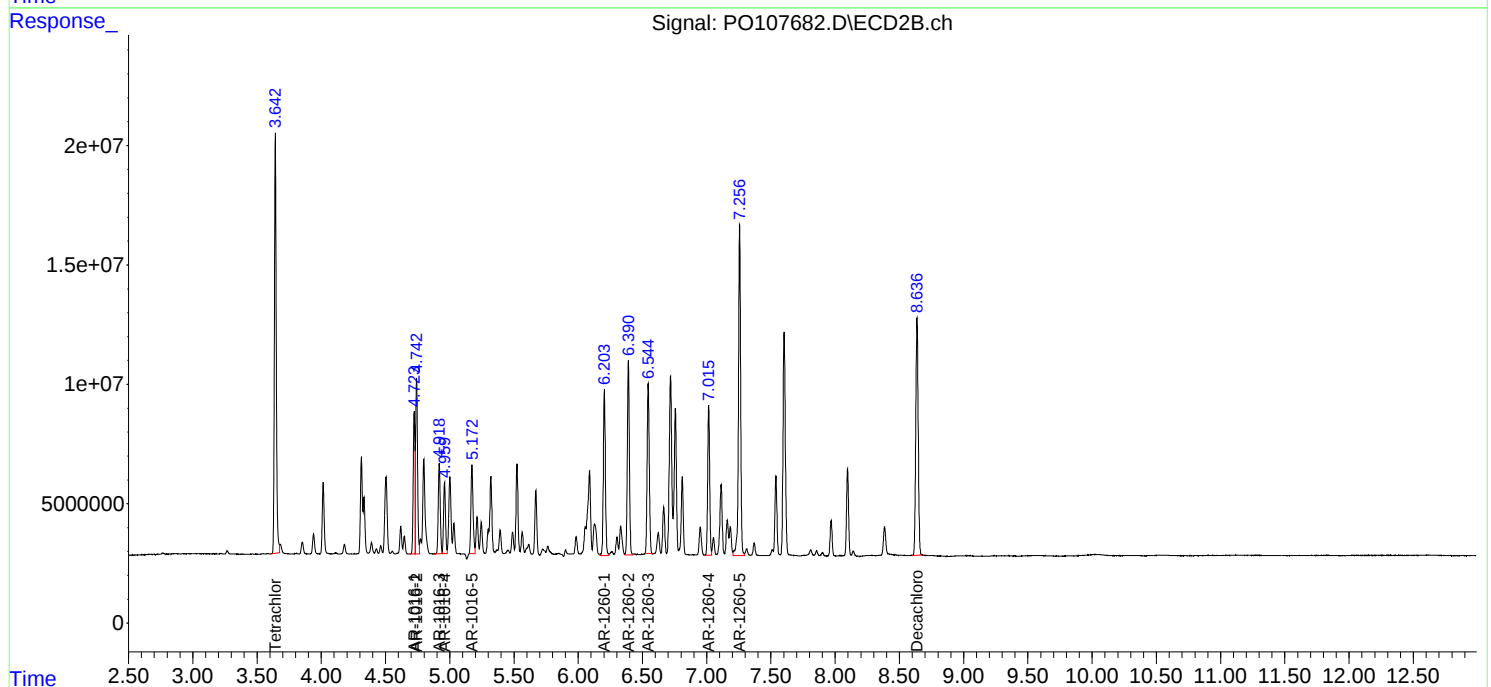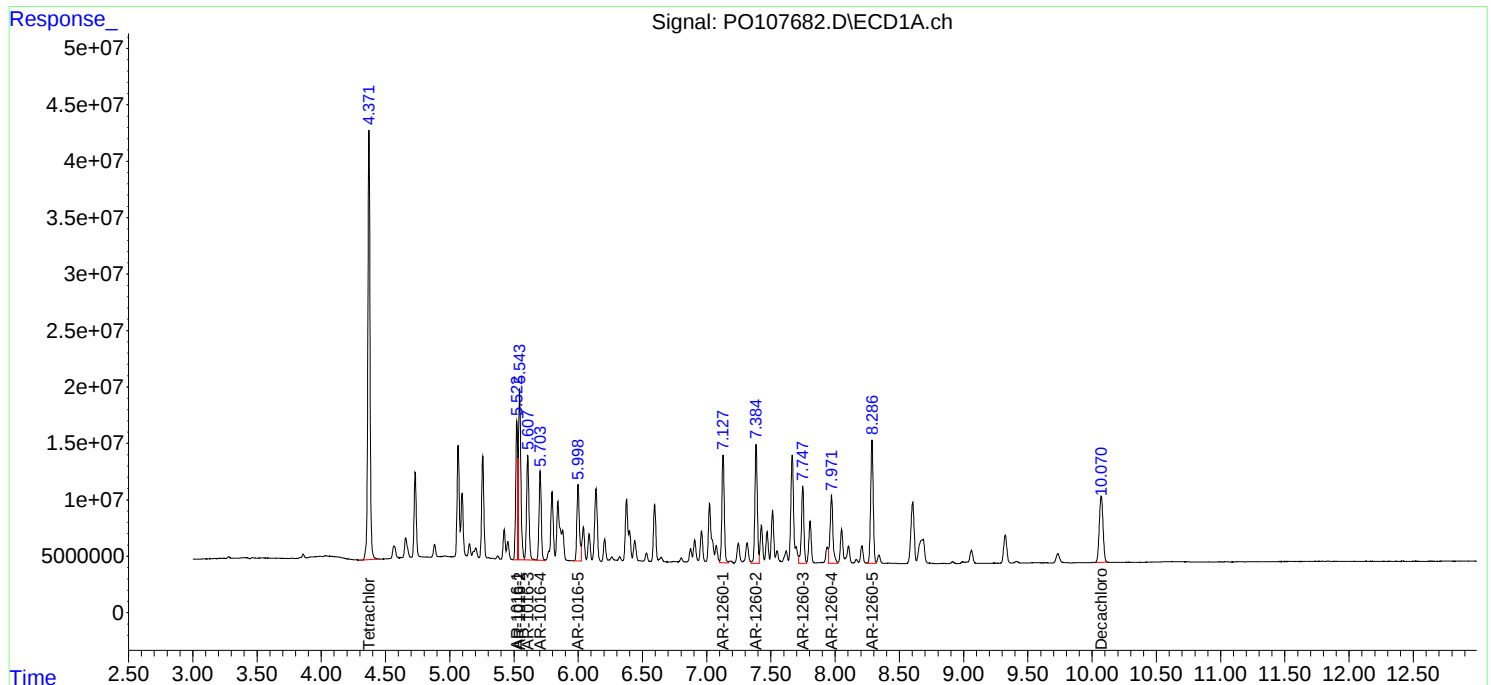



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Continuing Calib Date: 11/05/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 18:14 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.52	5.52	5.42	5.62	0.00
Aroclor-1016-2	(2)	5.54	5.55	5.45	5.65	0.01
Aroclor-1016-3	(3)	5.61	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.70	5.70	5.60	5.80	0.00
Aroclor-1016-5	(5)	6.00	6.00	5.90	6.10	0.00
Aroclor-1260-1	(1)	7.13	7.13	7.03	7.23	0.00
Aroclor-1260-2	(2)	7.38	7.38	7.28	7.48	0.00
Aroclor-1260-3	(3)	7.75	7.74	7.64	7.84	-0.01
Aroclor-1260-4	(4)	7.97	7.97	7.87	8.07	0.00
Aroclor-1260-5	(5)	8.29	8.28	8.18	8.38	0.00
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.07	10.06	9.96	10.16	-0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Continuing Calib Date: 11/05/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 18:14 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.73	4.63	4.83	0.01
Aroclor-1016-2	(2)	4.74	4.75	4.65	4.85	0.01
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.17	5.18	5.08	5.28	0.01
Aroclor-1260-1	(1)	6.20	6.21	6.11	6.31	0.01
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.55	6.55	6.45	6.65	0.00
Aroclor-1260-4	(4)	7.02	7.02	6.92	7.12	0.01
Aroclor-1260-5	(5)	7.26	7.26	7.16	7.36	0.00
Tetrachloro-m-xylene		3.64	3.65	3.55	3.75	0.01
Decachlorobiphenyl		8.64	8.64	8.54	8.74	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL02 Date Analyzed: 11/05/2024

Lab Sample No.: AR1660CCC500 Data File : PO107697.D Time Analyzed: 18:14

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.521	5.423	5.623	522.470	500.000	4.5
Aroclor-1016-2	5.543	5.445	5.645	507.430	500.000	1.5
Aroclor-1016-3	5.606	5.507	5.707	503.820	500.000	0.8
Aroclor-1016-4	5.703	5.604	5.804	525.210	500.000	5.0
Aroclor-1016-5	5.998	5.899	6.099	515.260	500.000	3.1
Aroclor-1260-1	7.126	7.026	7.226	513.720	500.000	2.7
Aroclor-1260-2	7.384	7.282	7.482	520.670	500.000	4.1
Aroclor-1260-3	7.746	7.643	7.843	528.800	500.000	5.8
Aroclor-1260-4	7.971	7.868	8.068	552.130	500.000	10.4
Aroclor-1260-5	8.285	8.181	8.381	543.660	500.000	8.7
Decachlorobiphenyl	10.070	9.958	10.158	48.260	50.000	-3.5
Tetrachloro-m-xylene	4.371	4.274	4.474	55.650	50.000	11.3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL02 Date Analyzed: 11/05/2024

Lab Sample No.: AR1660CCC500 Data File : PO107697.D Time Analyzed: 18:14

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.722	4.626	4.826	575.760	500.000	15.2
Aroclor-1016-2	4.742	4.645	4.845	589.770	500.000	18.0
Aroclor-1016-3	4.918	4.821	5.021	567.830	500.000	13.6
Aroclor-1016-4	4.959	4.862	5.062	515.120	500.000	3.0
Aroclor-1016-5	5.173	5.076	5.276	560.050	500.000	12.0
Aroclor-1260-1	6.203	6.107	6.307	556.200	500.000	11.2
Aroclor-1260-2	6.391	6.294	6.494	575.150	500.000	15.0
Aroclor-1260-3	6.545	6.448	6.648	536.310	500.000	7.3
Aroclor-1260-4	7.015	6.918	7.118	525.040	500.000	5.0
Aroclor-1260-5	7.256	7.159	7.359	545.390	500.000	9.1
Decachlorobiphenyl	8.636	8.539	8.739	48.340	50.000	-3.3
Tetrachloro-m-xylene	3.642	3.545	3.745	57.920	50.000	15.8

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 18:14
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:51:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	507.2E6	186.4E6	55.650	57.915
2) SA Decachlor...	10.070	8.636	118.4E6	132.5E6	48.263	48.337
Target Compounds						
3) L1 AR-1016-1	5.521	4.722	141.0E6	59456019	522.471	575.758
4) L1 AR-1016-2	5.543	4.742	201.4E6	83138802	507.431	589.772
5) L1 AR-1016-3	5.606	4.918	126.5E6	44714125	503.817	567.830
6) L1 AR-1016-4	5.703	4.959	101.2E6	34053745	525.213	515.120
7) L1 AR-1016-5	5.998	5.173	94114916	45999260	515.265	560.052
31) L7 AR-1260-1	7.126	6.203	132.8E6	86297640	513.719	556.204
32) L7 AR-1260-2	7.384	6.391	137.1E6	101.3E6	520.669	575.149
33) L7 AR-1260-3	7.746	6.545	95049980	89964539	528.804	536.307
34) L7 AR-1260-4	7.971	7.015	96900298	75962759	552.126	525.037
35) L7 AR-1260-5	8.285	7.256	154.6E6	179.7E6	543.663	545.393



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 18:14
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:51:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

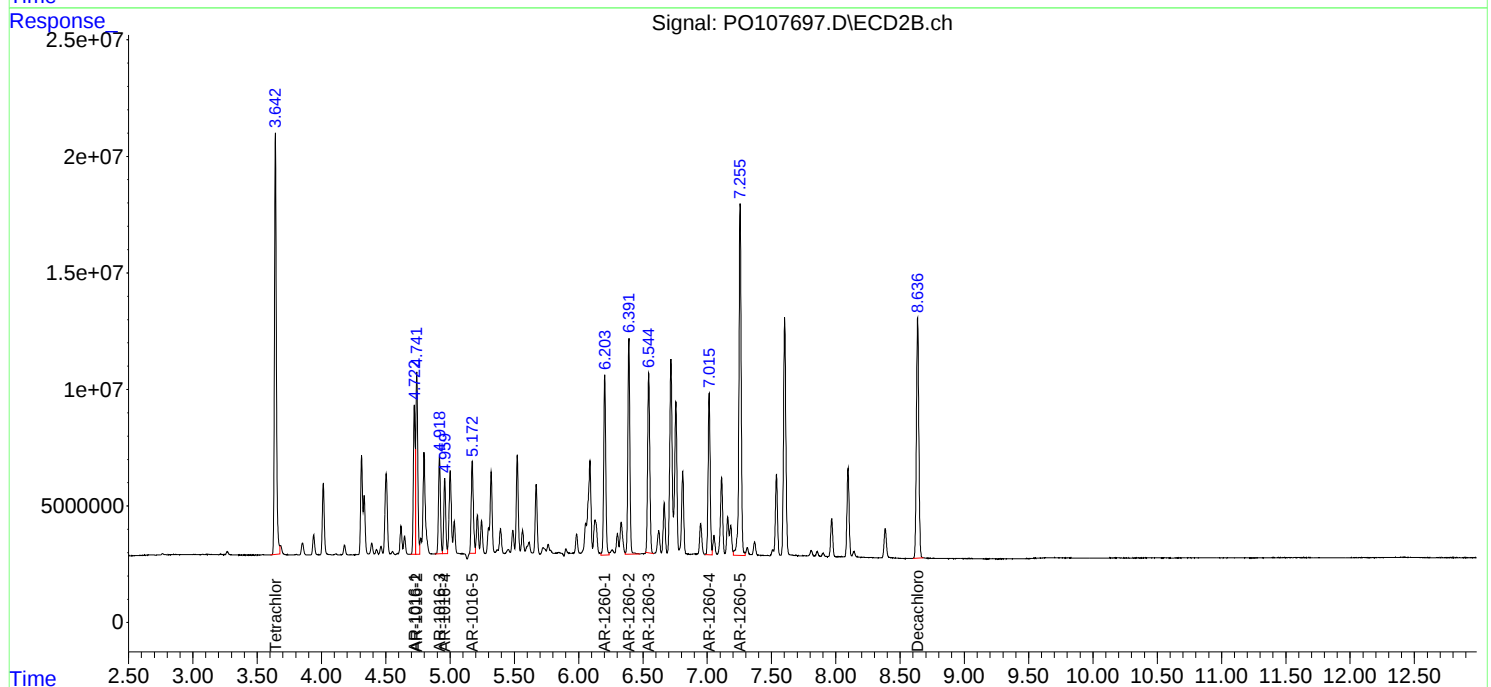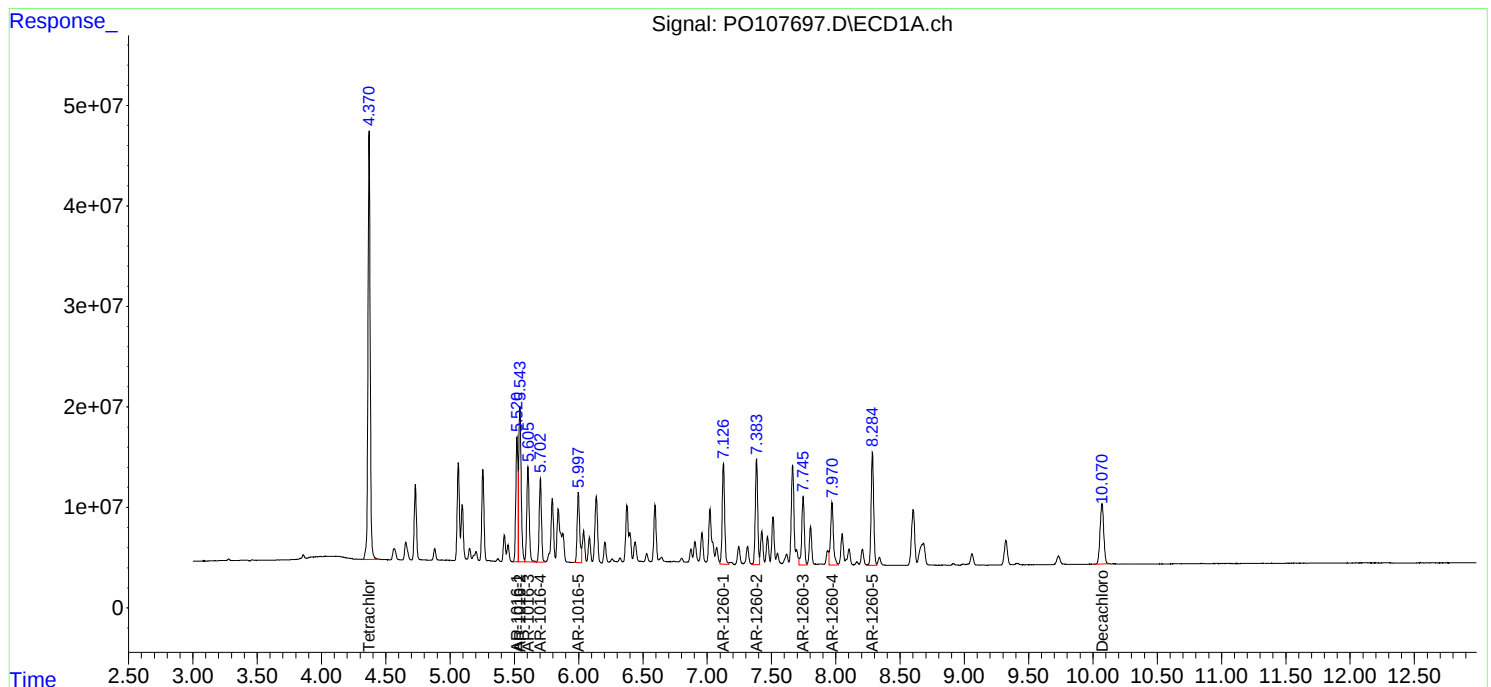



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Continuing Calib Date: 11/05/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 22:34 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.52	5.52	5.42	5.62	0.00
Aroclor-1016-2	(2)	5.54	5.55	5.45	5.65	0.01
Aroclor-1016-3	(3)	5.61	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.70	5.70	5.60	5.80	0.00
Aroclor-1016-5	(5)	6.00	6.00	5.90	6.10	0.00
Aroclor-1260-1	(1)	7.13	7.13	7.03	7.23	0.00
Aroclor-1260-2	(2)	7.39	7.38	7.28	7.48	-0.01
Aroclor-1260-3	(3)	7.75	7.74	7.64	7.84	-0.01
Aroclor-1260-4	(4)	7.97	7.97	7.87	8.07	0.00
Aroclor-1260-5	(5)	8.29	8.28	8.18	8.38	-0.01
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.07	10.06	9.96	10.16	-0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Continuing Calib Date: 11/05/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 22:34 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.73	4.63	4.83	0.01
Aroclor-1016-2	(2)	4.74	4.75	4.65	4.85	0.01
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.17	5.18	5.08	5.28	0.01
Aroclor-1260-1	(1)	6.20	6.21	6.11	6.31	0.01
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.55	6.55	6.45	6.65	0.00
Aroclor-1260-4	(4)	7.02	7.02	6.92	7.12	0.01
Aroclor-1260-5	(5)	7.26	7.26	7.16	7.36	0.00
Tetrachloro-m-xylene		3.64	3.65	3.55	3.75	0.01
Decachlorobiphenyl		8.64	8.64	8.54	8.74	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL03 Date Analyzed: 11/05/2024

Lab Sample No.: AR1660CCC500 Data File : PO107711.D Time Analyzed: 22:34

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.522	5.423	5.623	540.930	500.000	8.2
Aroclor-1016-2	5.544	5.445	5.645	536.510	500.000	7.3
Aroclor-1016-3	5.607	5.507	5.707	524.620	500.000	4.9
Aroclor-1016-4	5.704	5.604	5.804	546.140	500.000	9.2
Aroclor-1016-5	5.998	5.899	6.099	539.380	500.000	7.9
Aroclor-1260-1	7.128	7.026	7.226	530.520	500.000	6.1
Aroclor-1260-2	7.385	7.282	7.482	550.560	500.000	10.1
Aroclor-1260-3	7.747	7.643	7.843	552.230	500.000	10.4
Aroclor-1260-4	7.973	7.868	8.068	570.140	500.000	14.0
Aroclor-1260-5	8.286	8.181	8.381	566.790	500.000	13.4
Decachlorobiphenyl	10.071	9.958	10.158	50.590	50.000	1.2
Tetrachloro-m-xylene	4.371	4.274	4.474	55.110	50.000	10.2



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL03 Date Analyzed: 11/05/2024

Lab Sample No.: AR1660CCC500 Data File : PO107711.D Time Analyzed: 22:34

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.723	4.626	4.826	571.620	500.000	14.3
Aroclor-1016-2	4.742	4.645	4.845	590.130	500.000	18.0
Aroclor-1016-3	4.918	4.821	5.021	564.280	500.000	12.9
Aroclor-1016-4	4.959	4.862	5.062	505.500	500.000	1.1
Aroclor-1016-5	5.172	5.076	5.276	557.810	500.000	11.6
Aroclor-1260-1	6.203	6.107	6.307	555.170	500.000	11.0
Aroclor-1260-2	6.391	6.294	6.494	582.330	500.000	16.5
Aroclor-1260-3	6.545	6.448	6.648	547.050	500.000	9.4
Aroclor-1260-4	7.015	6.918	7.118	535.770	500.000	7.2
Aroclor-1260-5	7.257	7.159	7.359	569.080	500.000	13.8
Decachlorobiphenyl	8.637	8.539	8.739	54.680	50.000	9.4
Tetrachloro-m-xylene	3.642	3.545	3.745	58.830	50.000	17.7

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 22:34
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 01:00:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	502.3E6	189.4E6	55.110	58.832
2) SA Decachlor...	10.071	8.637	124.1E6	149.9E6	50.588	54.681
Target Compounds						
3) L1 AR-1016-1	5.522	4.723	146.0E6	59028386	540.932	571.617
4) L1 AR-1016-2	5.544	4.742	212.9E6	83189832	536.506	590.134
5) L1 AR-1016-3	5.607	4.918	131.8E6	44434382	524.618	564.277
6) L1 AR-1016-4	5.704	4.959	105.2E6	33417478	546.137	505.496
7) L1 AR-1016-5	5.998	5.172	98519687	45815342	539.380	557.813
31) L7 AR-1260-1	7.128	6.203	137.2E6	86137365	530.516	555.171
32) L7 AR-1260-2	7.385	6.391	144.9E6	102.6E6	550.560	582.327
33) L7 AR-1260-3	7.747	6.545	99260327	91766044	552.228	547.047
34) L7 AR-1260-4	7.973	7.015	100.1E6	77515492	570.138	535.769
35) L7 AR-1260-5	8.286	7.257	161.2E6	187.5E6	566.791	569.081



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 22:34
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 01:00:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

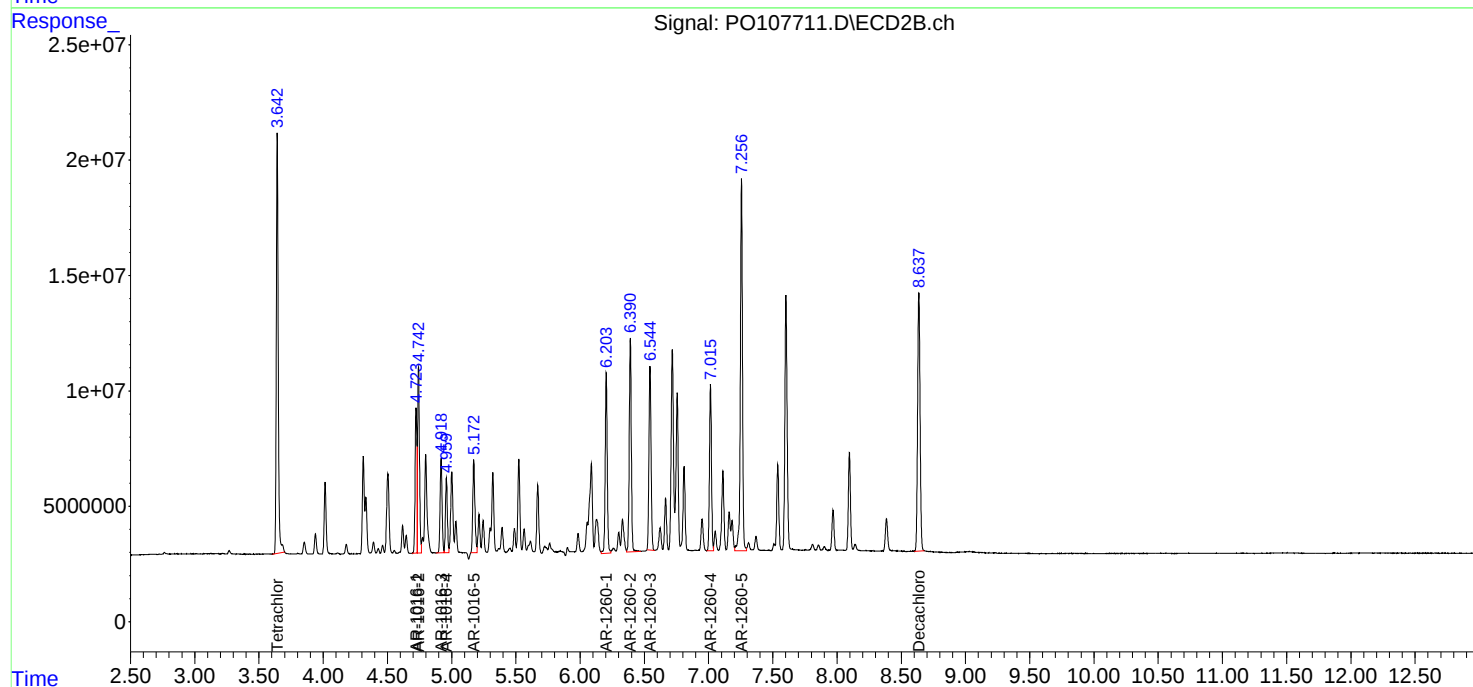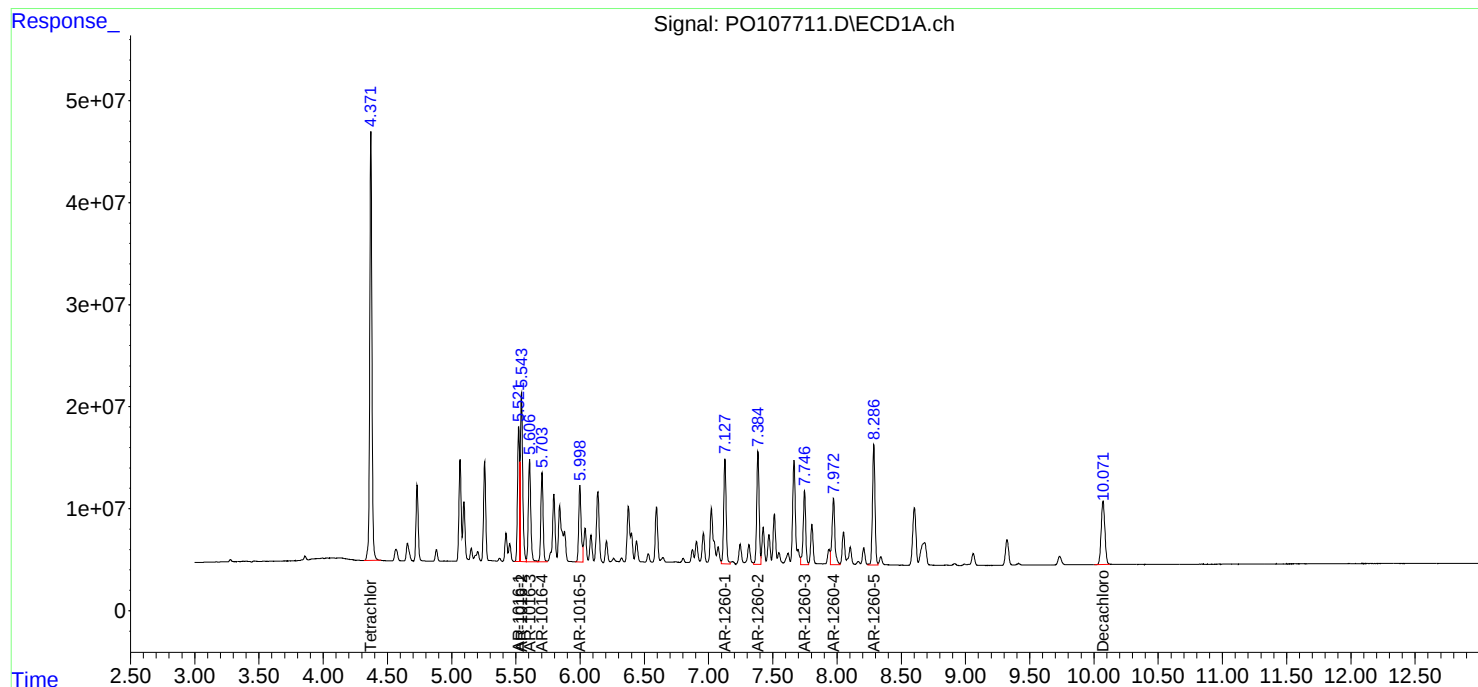

Analytical Sequence

Client: EarthEfficient LLC

SDG No.: P4699

Project: 120-122 Liberty Ave BK

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 10/15/2024

10/15/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	10/15/2024	18:08	PO107183.D	10.06	4.37
AR1660ICC1000	AR1660ICC1000	10/15/2024	18:27	PO107184.D	10.06	4.37
AR1660ICC750	AR1660ICC750	10/15/2024	18:45	PO107185.D	10.06	4.37
AR1660ICC500	AR1660ICC500	10/15/2024	19:03	PO107186.D	10.06	4.37
AR1660ICC250	AR1660ICC250	10/15/2024	19:21	PO107187.D	10.06	4.37
AR1660ICC050	AR1660ICC050	10/15/2024	19:39	PO107188.D	10.06	4.37
AR1221ICC500	AR1221ICC500	10/15/2024	19:57	PO107189.D	10.06	4.37
AR1232ICC500	AR1232ICC500	10/15/2024	20:15	PO107190.D	10.06	4.37
AR1242ICC1000	AR1242ICC1000	10/15/2024	20:34	PO107191.D	10.06	4.37
AR1242ICC750	AR1242ICC750	10/15/2024	20:52	PO107192.D	10.06	4.37
AR1242ICC500	AR1242ICC500	10/15/2024	21:10	PO107193.D	10.06	4.37
AR1242ICC250	AR1242ICC250	10/15/2024	21:28	PO107194.D	10.06	4.37
AR1242ICC050	AR1242ICC050	10/15/2024	21:46	PO107195.D	10.06	4.37
AR1248ICC1000	AR1248ICC1000	10/15/2024	22:04	PO107196.D	10.06	4.37
AR1248ICC750	AR1248ICC750	10/15/2024	22:22	PO107197.D	10.06	4.37
AR1248ICC500	AR1248ICC500	10/15/2024	22:41	PO107198.D	10.06	4.37
AR1248ICC250	AR1248ICC250	10/15/2024	22:59	PO107199.D	10.06	4.37
AR1248ICC050	AR1248ICC050	10/15/2024	23:17	PO107200.D	10.06	4.37
AR1254ICC1000	AR1254ICC1000	10/15/2024	23:35	PO107201.D	10.06	4.37
AR1254ICC750	AR1254ICC750	10/15/2024	23:53	PO107202.D	10.06	4.37
AR1254ICC500	AR1254ICC500	10/16/2024	00:11	PO107203.D	10.06	4.37
AR1254ICC250	AR1254ICC250	10/16/2024	00:29	PO107204.D	10.06	4.37
AR1254ICC050	AR1254ICC050	10/16/2024	00:47	PO107205.D	10.06	4.37
AR1262ICC500	AR1262ICC500	10/16/2024	01:05	PO107206.D	10.06	4.37
AR1268ICC1000	AR1268ICC1000	10/16/2024	01:23	PO107207.D	10.06	4.37
AR1268ICC750	AR1268ICC750	10/16/2024	01:41	PO107208.D	10.06	4.37
AR1268ICC500	AR1268ICC500	10/16/2024	01:59	PO107209.D	10.06	4.37
AR1268ICC250	AR1268ICC250	10/16/2024	02:18	PO107210.D	10.06	4.37
AR1268ICC050	AR1268ICC050	10/16/2024	02:36	PO107211.D	10.06	4.37
AR1660CCC500	AR1660CCC500	11/05/2024	13:01	PO107682.D	10.07	4.37
IBLK	IBLK	11/05/2024	14:09	PO107686.D	10.07	4.37
PB164678BL	PB164678BL	11/05/2024	15:00	PO107687.D	10.07	4.37
PB164678BS	PB164678BS	11/05/2024	15:16	PO107688.D	10.07	4.37
AR1660CCC500	AR1660CCC500	11/05/2024	18:14	PO107697.D	10.07	4.37
IBLK	IBLK	11/05/2024	19:20	PO107701.D	10.07	4.37
MIXED-DEMO	P4699-01	11/05/2024	19:53	PO107703.D	10.07	4.37
BP-F3MS	P4701-01MS	11/05/2024	20:43	PO107706.D	10.07	4.37
BP-F3MSD	P4701-01MSD	11/05/2024	20:59	PO107707.D	10.07	4.37
AR1660CCC500	AR1660CCC500	11/05/2024	22:34	PO107711.D	10.07	4.37
IBLK	IBLK	11/05/2024	23:42	PO107715.D	10.07	4.37

Analytical Sequence

Client: EarthEfficient LLC

SDG No.: P4699

Project: 120-122 Liberty Ave BK

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 10/15/2024

10/15/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	10/15/2024	18:08	PO107183.D	8.64	3.64
AR1660ICC1000	AR1660ICC1000	10/15/2024	18:27	PO107184.D	8.64	3.64
AR1660ICC750	AR1660ICC750	10/15/2024	18:45	PO107185.D	8.64	3.64
AR1660ICC500	AR1660ICC500	10/15/2024	19:03	PO107186.D	8.64	3.65
AR1660ICC250	AR1660ICC250	10/15/2024	19:21	PO107187.D	8.64	3.64
AR1660ICC050	AR1660ICC050	10/15/2024	19:39	PO107188.D	8.64	3.64
AR1221ICC500	AR1221ICC500	10/15/2024	19:57	PO107189.D	8.64	3.64
AR1232ICC500	AR1232ICC500	10/15/2024	20:15	PO107190.D	8.64	3.64
AR1242ICC1000	AR1242ICC1000	10/15/2024	20:34	PO107191.D	8.64	3.64
AR1242ICC750	AR1242ICC750	10/15/2024	20:52	PO107192.D	8.64	3.64
AR1242ICC500	AR1242ICC500	10/15/2024	21:10	PO107193.D	8.64	3.64
AR1242ICC250	AR1242ICC250	10/15/2024	21:28	PO107194.D	8.64	3.65
AR1242ICC050	AR1242ICC050	10/15/2024	21:46	PO107195.D	8.64	3.64
AR1248ICC1000	AR1248ICC1000	10/15/2024	22:04	PO107196.D	8.64	3.64
AR1248ICC750	AR1248ICC750	10/15/2024	22:22	PO107197.D	8.64	3.64
AR1248ICC500	AR1248ICC500	10/15/2024	22:41	PO107198.D	8.64	3.64
AR1248ICC250	AR1248ICC250	10/15/2024	22:59	PO107199.D	8.64	3.64
AR1248ICC050	AR1248ICC050	10/15/2024	23:17	PO107200.D	8.64	3.64
AR1254ICC1000	AR1254ICC1000	10/15/2024	23:35	PO107201.D	8.64	3.65
AR1254ICC750	AR1254ICC750	10/15/2024	23:53	PO107202.D	8.64	3.64
AR1254ICC500	AR1254ICC500	10/16/2024	00:11	PO107203.D	8.64	3.64
AR1254ICC250	AR1254ICC250	10/16/2024	00:29	PO107204.D	8.64	3.64
AR1254ICC050	AR1254ICC050	10/16/2024	00:47	PO107205.D	8.64	3.65
AR1262ICC500	AR1262ICC500	10/16/2024	01:05	PO107206.D	8.64	3.64
AR1268ICC1000	AR1268ICC1000	10/16/2024	01:23	PO107207.D	8.64	3.65
AR1268ICC750	AR1268ICC750	10/16/2024	01:41	PO107208.D	8.64	3.64
AR1268ICC500	AR1268ICC500	10/16/2024	01:59	PO107209.D	8.64	3.65
AR1268ICC250	AR1268ICC250	10/16/2024	02:18	PO107210.D	8.64	3.64
AR1268ICC050	AR1268ICC050	10/16/2024	02:36	PO107211.D	8.64	3.65
AR1660CCC500	AR1660CCC500	11/05/2024	13:01	PO107682.D	8.64	3.64
IBLK	IBLK	11/05/2024	14:09	PO107686.D	8.64	3.64
PB164678BL	PB164678BL	11/05/2024	15:00	PO107687.D	8.64	3.64
PB164678BS	PB164678BS	11/05/2024	15:16	PO107688.D	8.64	3.64
AR1660CCC500	AR1660CCC500	11/05/2024	18:14	PO107697.D	8.64	3.64
IBLK	IBLK	11/05/2024	19:20	PO107701.D	8.64	3.64
MIXED-DEMO	P4699-01	11/05/2024	19:53	PO107703.D	8.64	3.64
BP-F3MS	P4701-01MS	11/05/2024	20:43	PO107706.D	8.64	3.64
BP-F3MSD	P4701-01MSD	11/05/2024	20:59	PO107707.D	8.64	3.64
AR1660CCC500	AR1660CCC500	11/05/2024	22:34	PO107711.D	8.64	3.64
IBLK	IBLK	11/05/2024	23:42	PO107715.D	8.64	3.64

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB164678BS

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Lab Sample ID: PB164678BS Date(s) Analyzed: 11/05/2024 11/05/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO107688.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.523	5.473	5.573	159	155	0
COLUMN 1	2	5.544	5.494	5.594	154		
	3	5.607	5.557	5.657	152		
	4	5.704	5.654	5.754	157		
	5	5.999	5.949	6.049	153		
	1	4.723	4.673	4.773	160		
COLUMN 2	2	4.742	4.692	4.792	163	155	
	3	4.918	4.868	4.968	157		
	4	4.959	4.909	5.009	143		
	5	5.173	5.123	5.223	151		
Aroclor-1260	1	7.128	7.078	7.178	167	156	1.29
COLUMN 1	2	7.385	7.335	7.435	170		
	3	7.747	7.697	7.797	140		
	4	7.972	7.922	8.022	156		
	5	8.287	8.237	8.337	148		
	1	6.202	6.152	6.252	158	154	
COLUMN 2	2	6.39	6.34	6.44	167		
	3	6.543	6.493	6.593	163		
	4	7.014	6.964	7.064	138		
	5	7.255	7.205	7.305	145		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

BP-F3MS

Contract: EART12

Lab Code: CHEM

Case No.: P4699

SAS No.: P4699

SDG NO.: P4699

Lab Sample ID: P4701-01MS

Date(s) Analyzed: 11/05/2024

11/05/2024

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO107706.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.523	5.473	5.573	226	222	6.11
COLUMN 1	2	5.546	5.496	5.596	222		
	3	5.609	5.559	5.659	213		
	4	5.705	5.655	5.755	229		
	5	6.001	5.951	6.051	221		
	1	4.723	4.673	4.773	245		
COLUMN 2	2	4.742	4.692	4.792	255	236	
	3	4.918	4.868	4.968	241		
	4	4.959	4.909	5.009	214		
	5	5.173	5.123	5.223	223		
Aroclor-1260	1	7.13	7.08	7.18	214	211	1.88
COLUMN 1	2	7.386	7.336	7.436	218		
	3	7.749	7.699	7.799	194		
	4	7.973	7.923	8.023	222		
	5	8.288	8.238	8.338	208		
	1	6.204	6.154	6.254	219	215	
COLUMN 2	2	6.391	6.341	6.441	240		
	3	6.544	6.494	6.594	228		
	4	7.015	6.965	7.065	191		
	5	7.256	7.206	7.306	197		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

BP-F3MSD

Contract: EART12

Lab Code: CHEM Case No.: P4699 SAS No.: P4699 SDG NO.: P4699

Lab Sample ID: P4701-01MSD Date(s) Analyzed: 11/05/2024 11/05/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO107707.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.522	5.472	5.572	243	238	2.49
COLUMN 1	2	5.544	5.494	5.594	237		
	3	5.607	5.557	5.657	228		
	4	5.703	5.653	5.753	248		
	5	5.998	5.948	6.048	231		
	1	4.723	4.673	4.773	254		
COLUMN 2	2	4.741	4.691	4.791	261	244	
	3	4.917	4.867	4.967	249		
	4	4.959	4.909	5.009	222		
	5	5.172	5.122	5.222	231		
Aroclor-1260	1	7.128	7.078	7.178	213	217	1.37
COLUMN 1	2	7.385	7.335	7.435	226		
	3	7.747	7.697	7.797	202		
	4	7.972	7.922	8.022	230		
	5	8.287	8.237	8.337	212		
	1	6.203	6.153	6.253	229	220	
COLUMN 2	2	6.39	6.34	6.44	236		
	3	6.544	6.494	6.594	225		
	4	7.015	6.965	7.065	202		
	5	7.256	7.206	7.306	210		



QC SAMPLE DATA

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	
Project:	120-122 Liberty Ave BK	Date Received:	
Client Sample ID:	PB164678BL	SDG No.:	P4699
Lab Sample ID:	PB164678BL	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	100 Decanted:
Sample Wt/Vol:	30.03 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107687.D	1	11/05/24 08:35	11/05/24 15:00	PB164678

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	3.40	U	3.40	17.0	ug/kg
11104-28-2	Aroclor-1221	6.40	U	6.40	17.0	ug/kg
11141-16-5	Aroclor-1232	3.40	U	3.40	17.0	ug/kg
53469-21-9	Aroclor-1242	3.40	U	3.40	17.0	ug/kg
12672-29-6	Aroclor-1248	7.90	U	7.90	17.0	ug/kg
11097-69-1	Aroclor-1254	2.70	U	2.70	17.0	ug/kg
37324-23-5	Aroclor-1262	4.60	U	4.60	17.0	ug/kg
11100-14-4	Aroclor-1268	3.40	U	3.40	17.0	ug/kg
11096-82-5	Aroclor-1260	2.90	U	2.90	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.1		30 (32) - 150 (144)	106%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.7		30 (32) - 150 (175)	108%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 15:00
 Operator : YP/AJ
 Sample : PB164678BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB164678BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:45:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.642	190.3E6	67905156	20.880	21.098
2) SA Decachlor...	10.074	8.637	53210309	58731987	21.689	21.423

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 15:00
Operator : YP/AJ
Sample : PB164678BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB164678BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:45:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

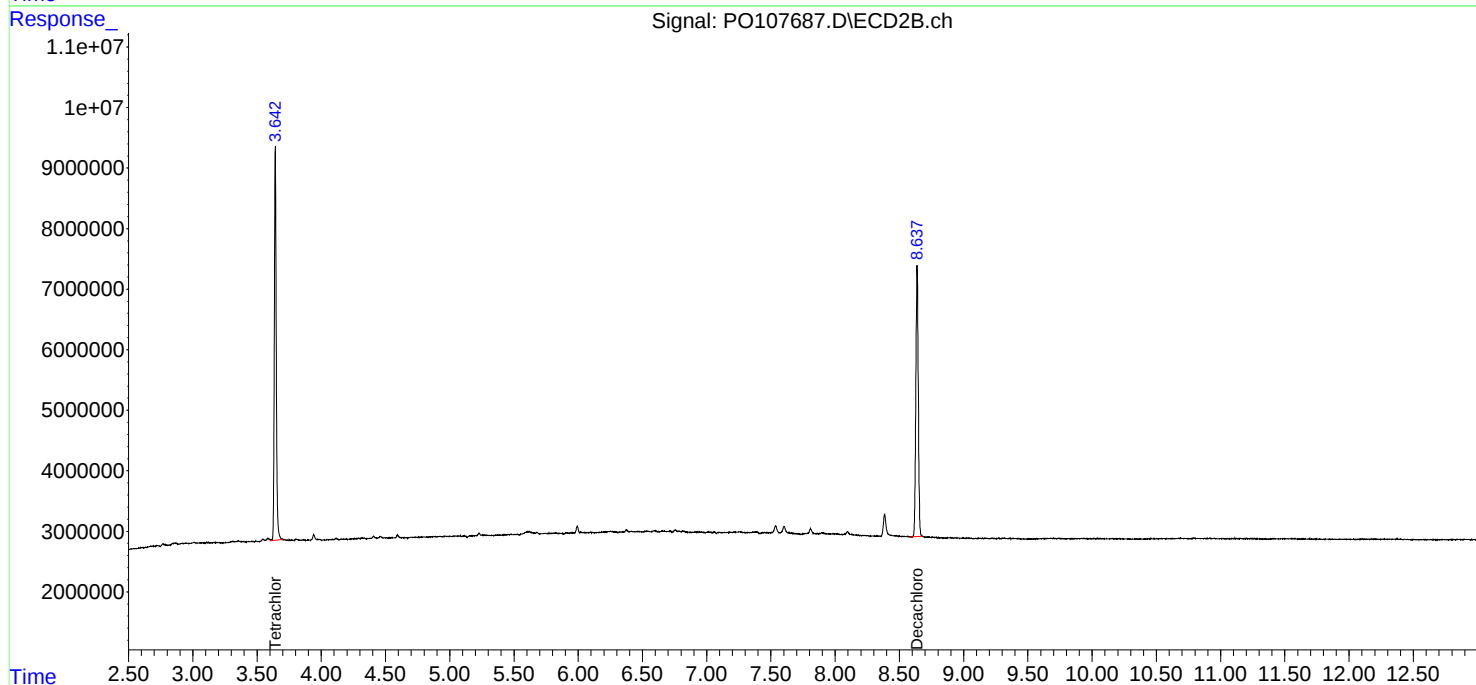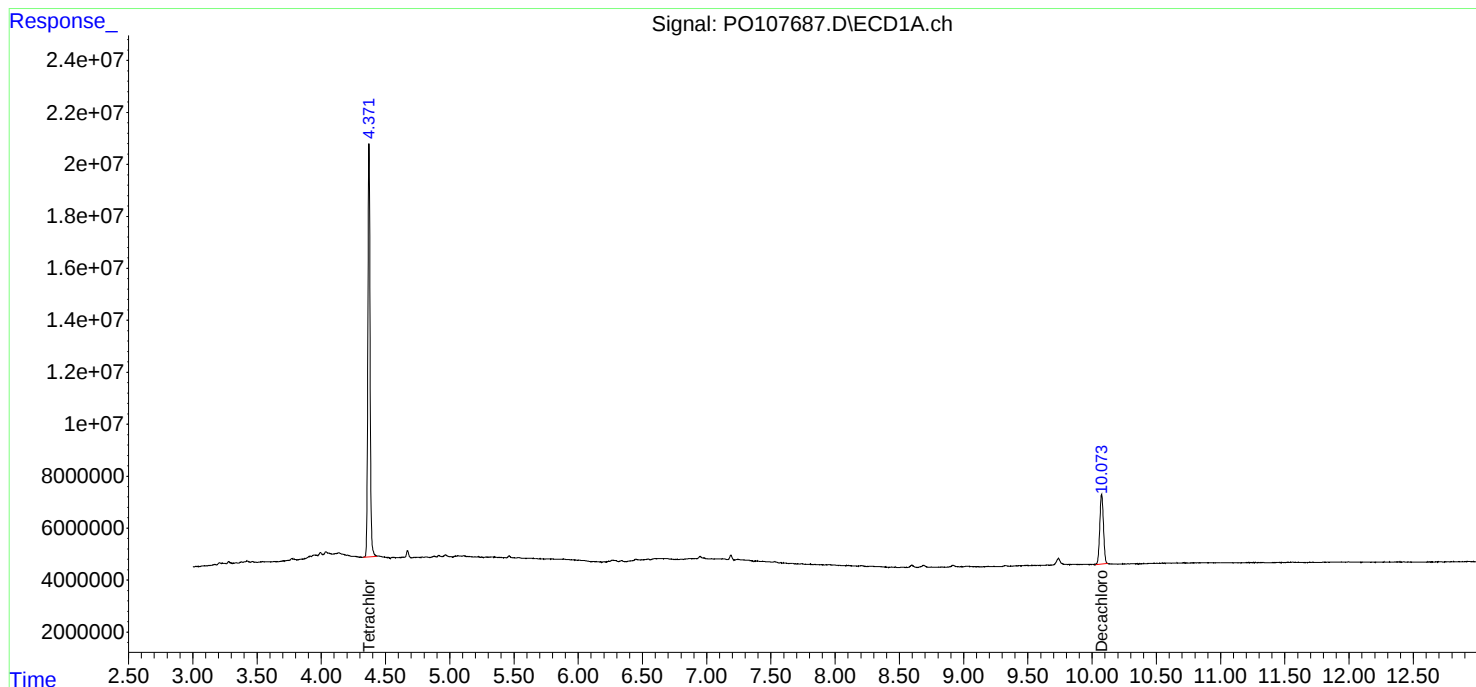


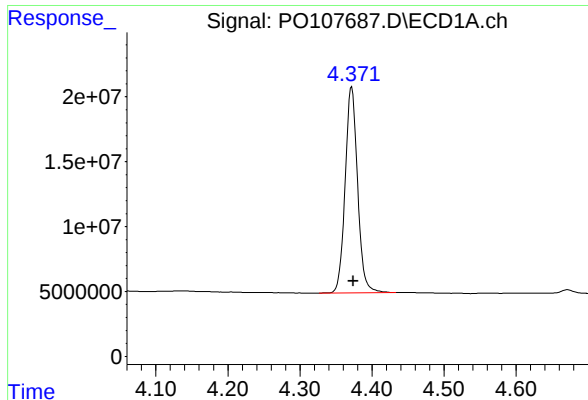

#1 Tetrachloro-m-xylene


R.T.: 4.372 min
Delta R.T.: -0.002 min
Response: 190297832
Conc: 20.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB164678BL

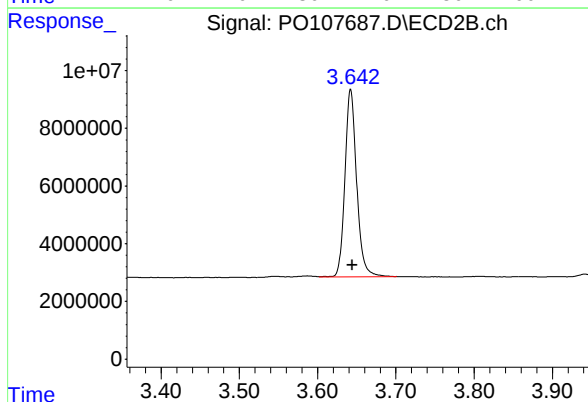


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.002 min
Response: 67905156
Conc: 21.10 ng/ml

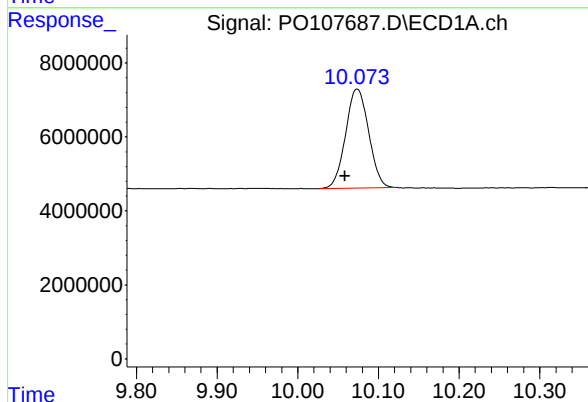

#2 Decachlorobiphenyl

R.T.: 10.074 min
Delta R.T.: 0.016 min
Response: 53210309
Conc: 21.69 ng/ml

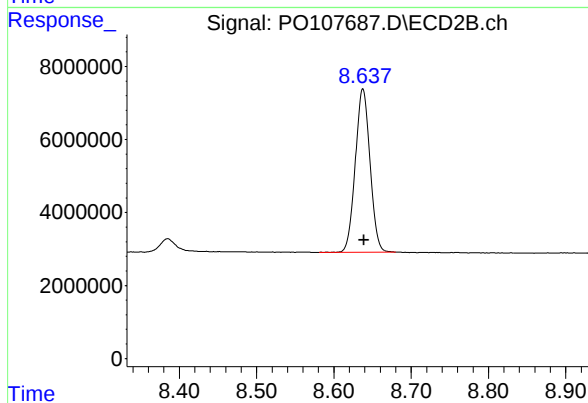

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.001 min
Response: 58731987
Conc: 21.42 ng/ml

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	10/15/24
Project:	120-122 Liberty Ave BK	Date Received:	10/15/24
Client Sample ID:	PIBLK-PO107183.D	SDG No.:	P4699
Lab Sample ID:	I.BLK-PO107183.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107183.D	1		10/15/24	po101524

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.1		70 (60) - 130 (140)	110%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.8		70 (60) - 130 (140)	114%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
 Data File : PO107183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 18:08
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:56:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:53:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	204.9E6	71065652	22.480	22.080
2) SA Decachlor...	10.057	8.638	57445703	62504934	23.415	22.799

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 18:08
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:56:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:53:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

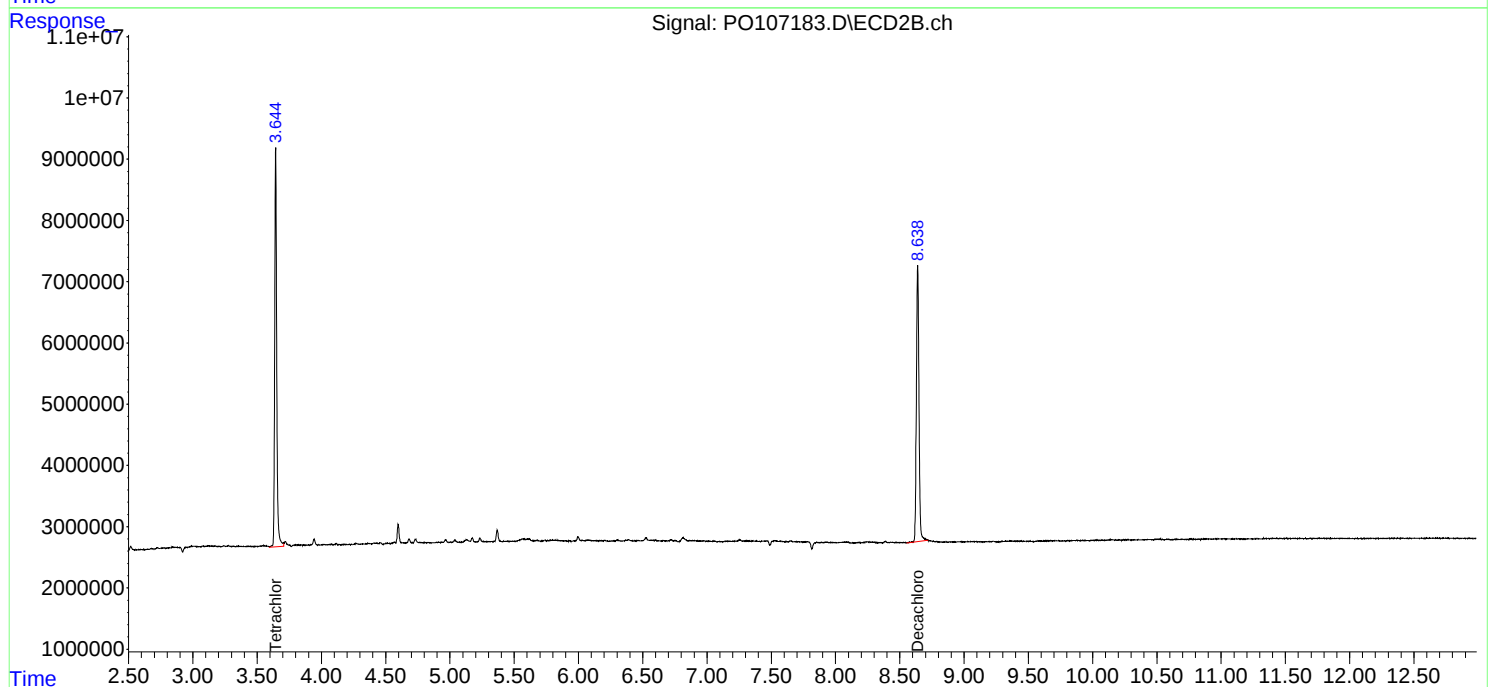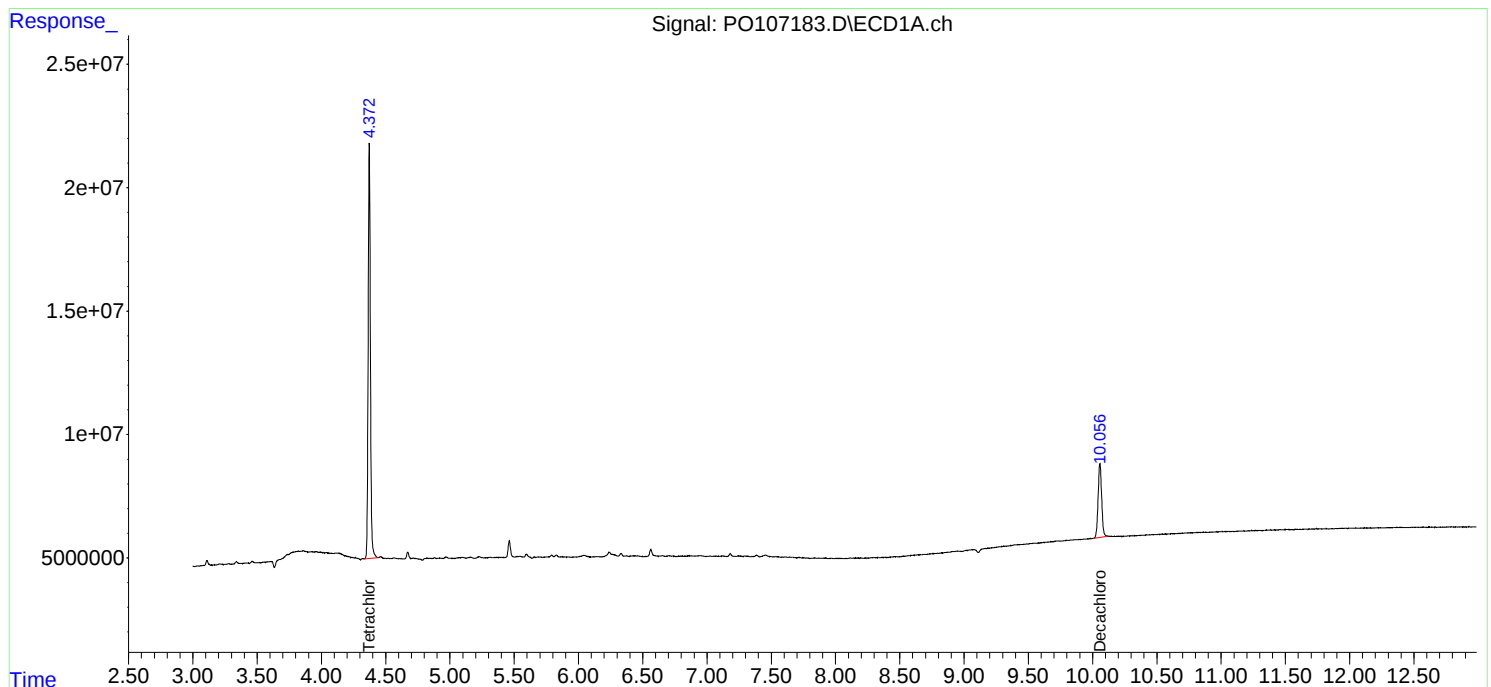


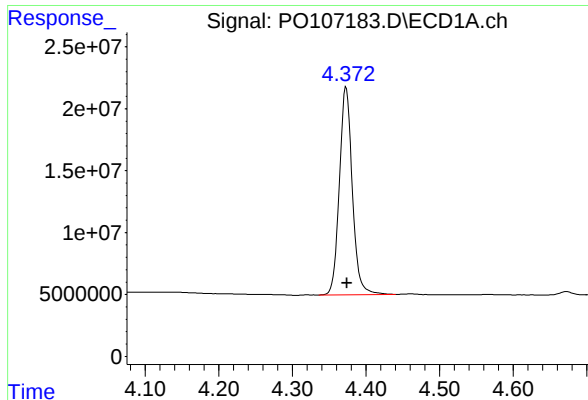

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: -0.001 min
Response: 204884980
Conc: 22.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

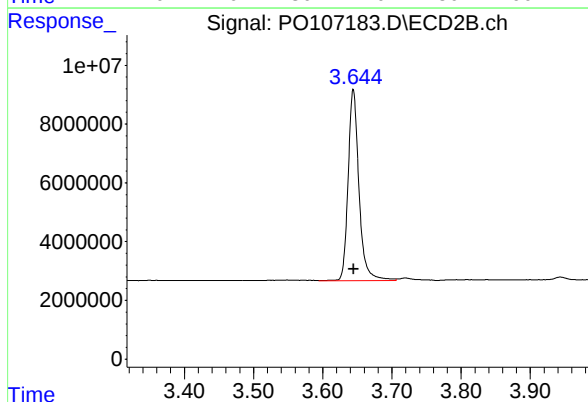


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.000 min
Response: 71065652
Conc: 22.08 ng/ml

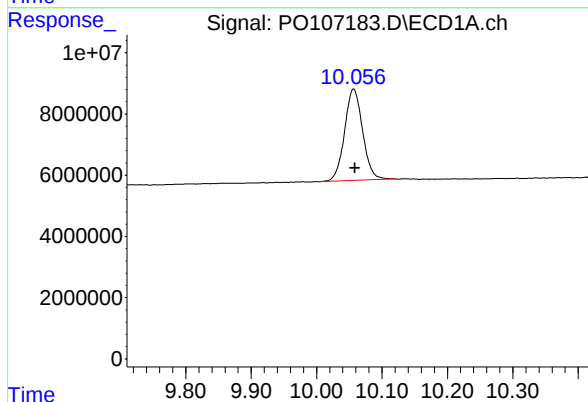

#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: -0.002 min
Response: 57445703
Conc: 23.41 ng/ml

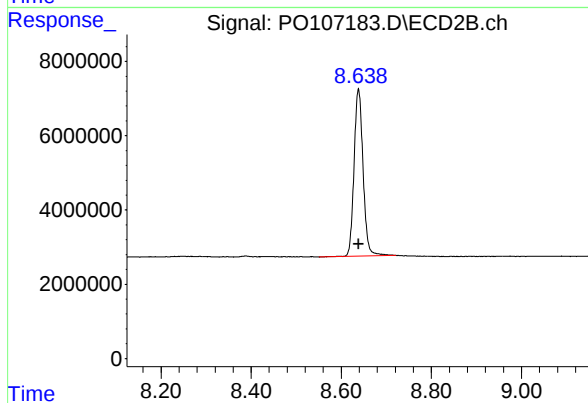

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 62504934
Conc: 22.80 ng/ml

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	11/05/24
Project:	120-122 Liberty Ave BK	Date Received:	11/05/24
Client Sample ID:	PIBLK-PO107686.D	SDG No.:	P4699
Lab Sample ID:	I.BLK-PO107686.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107686.D	1		11/05/24	PO110524

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.7		70 (60) - 130 (140)	104%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.0		70 (60) - 130 (140)	105%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 14:09
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:45:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.641	189.0E6	67752087	20.739	21.051
2) SA Decachlor...	10.073	8.637	52290962	57563026	21.314	20.996

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 14:09
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:45:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

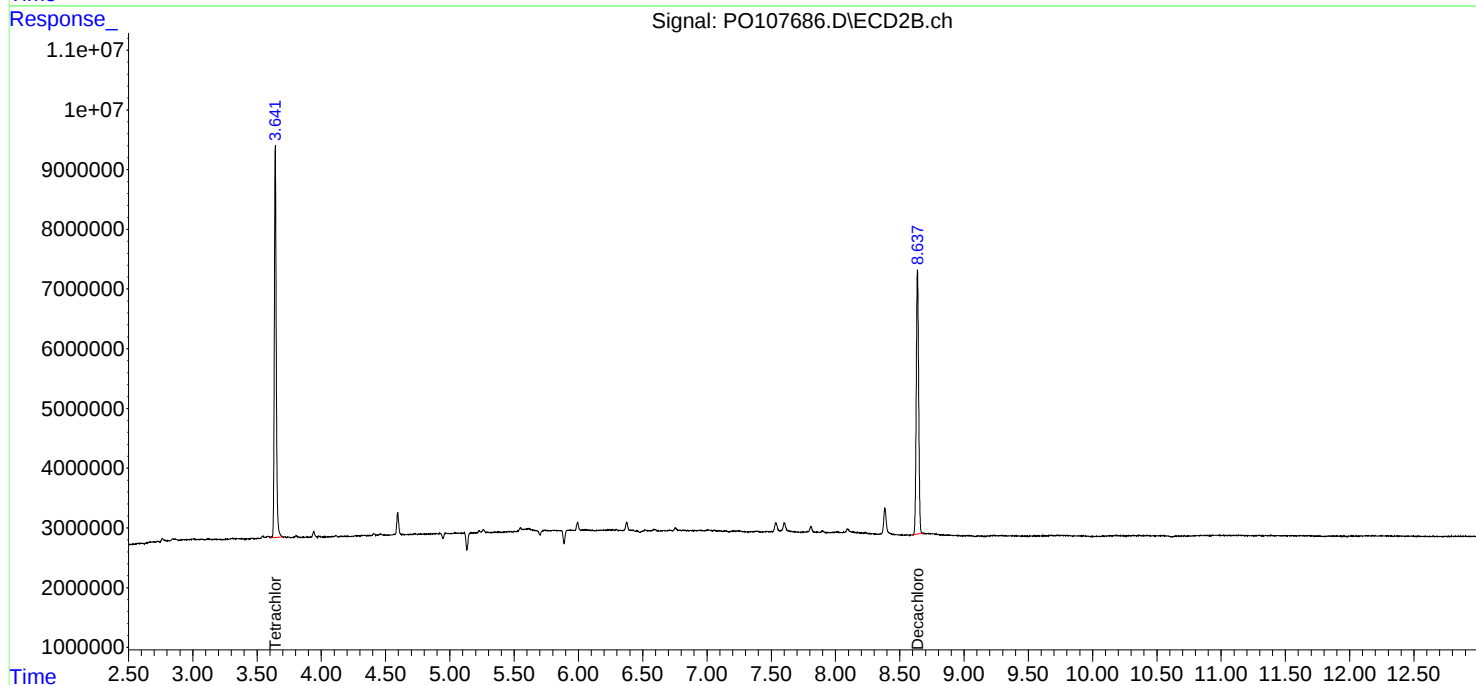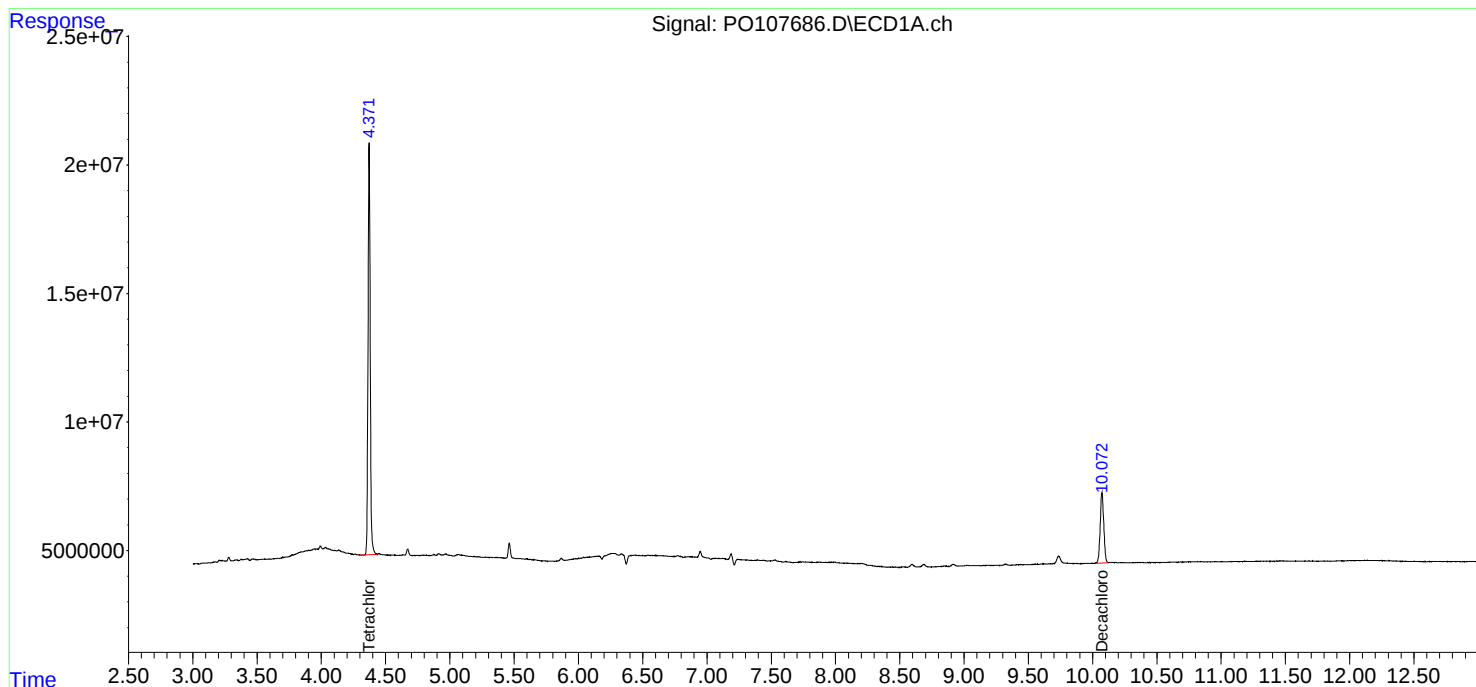


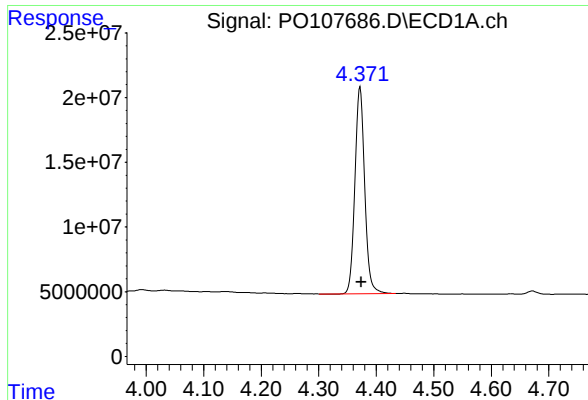

#1 Tetrachloro-m-xylene


R.T.: 4.372 min
Delta R.T.: -0.002 min
Response: 189015024
Conc: 20.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

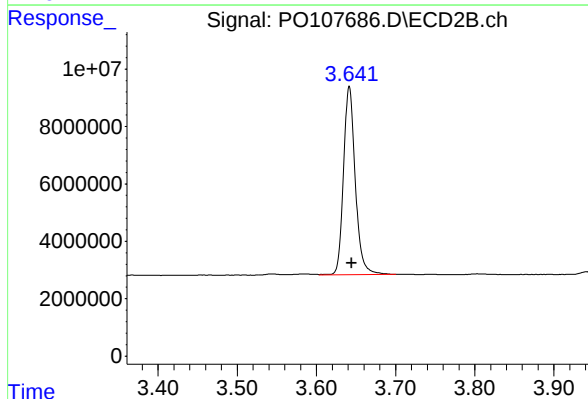


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: -0.003 min
Response: 67752087
Conc: 21.05 ng/ml

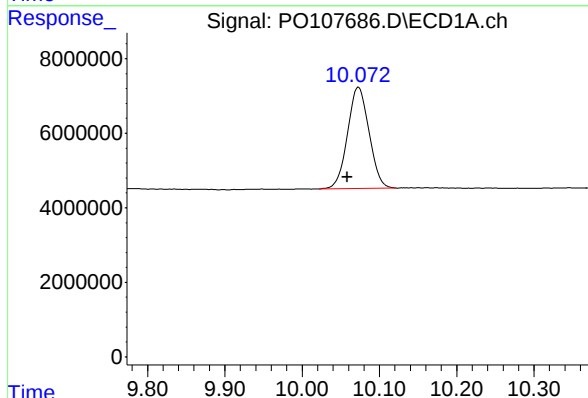

#2 Decachlorobiphenyl

R.T.: 10.073 min
Delta R.T.: 0.014 min
Response: 52290962
Conc: 21.31 ng/ml

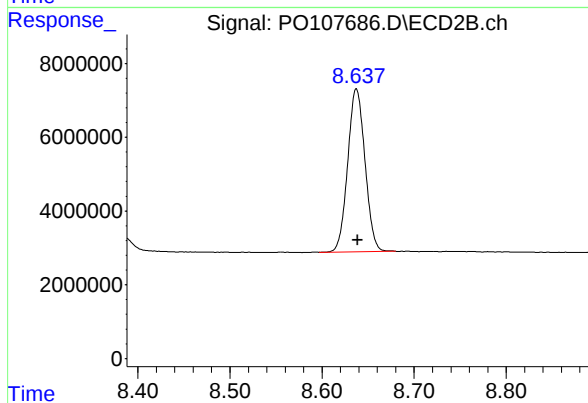

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.001 min
Response: 57563026
Conc: 21.00 ng/ml

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	11/05/24
Project:	120-122 Liberty Ave BK	Date Received:	11/05/24
Client Sample ID:	PIBLK-PO107701.D	SDG No.:	P4699
Lab Sample ID:	I.BLK-PO107701.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107701.D	1		11/05/24	PO110524

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.0		70 (60) - 130 (140)	105%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.9		70 (60) - 130 (140)	105%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 19:20
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:53:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.642	191.1E6	69154593	20.973	21.487
2) SA Decachlor...	10.071	8.637	51599060	57354344	21.032	20.920

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 19:20
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:53:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

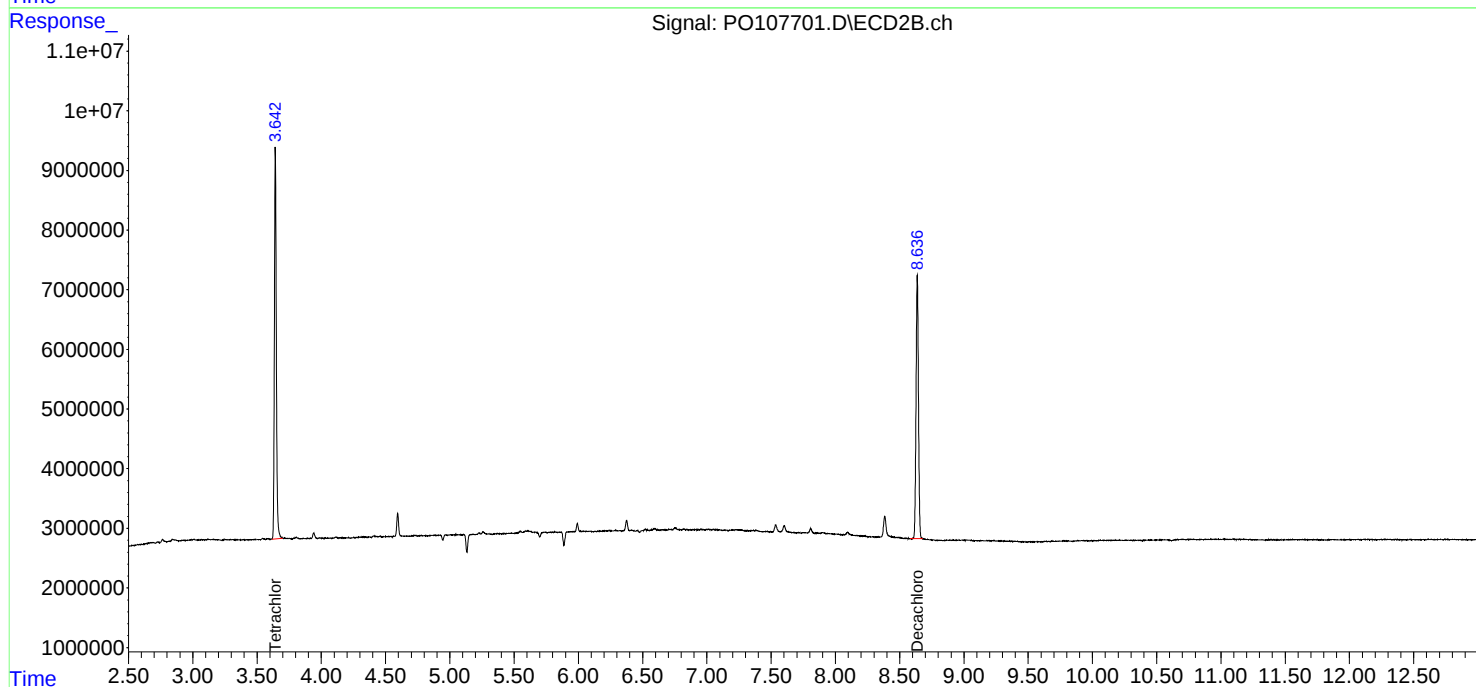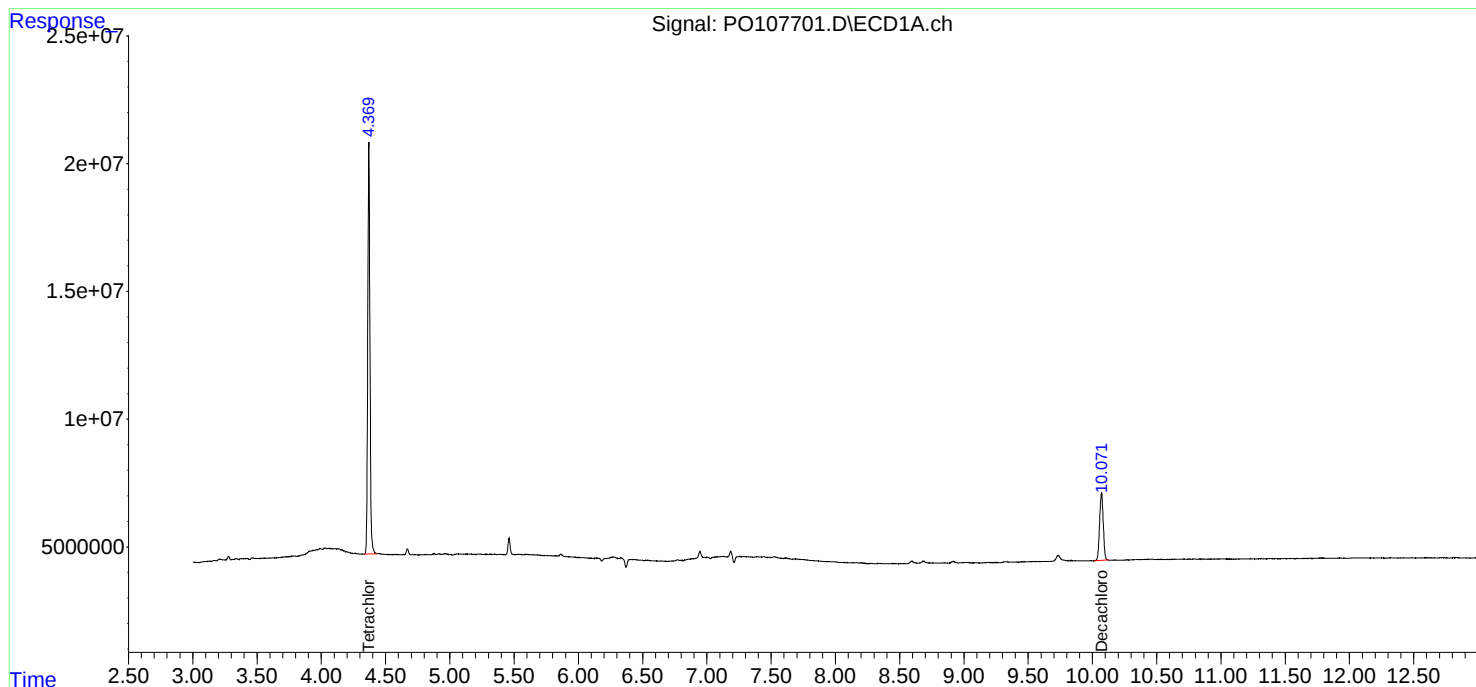


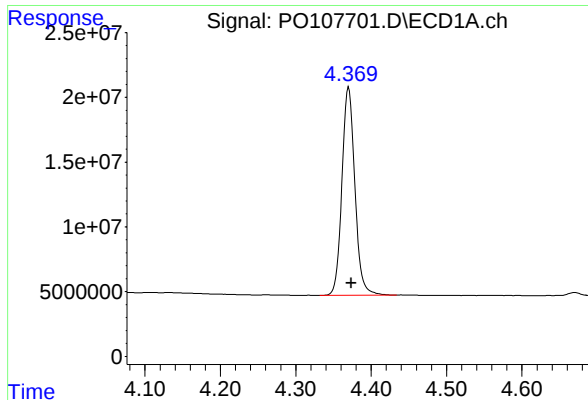

#1 Tetrachloro-m-xylene


R.T.: 4.370 min
Delta R.T.: -0.004 min
Response: 191143896
Conc: 20.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

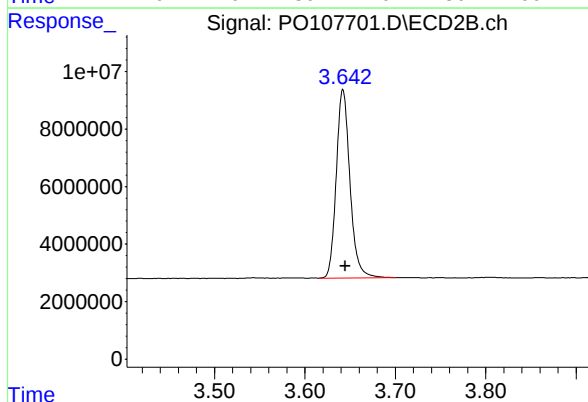


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.002 min
Response: 69154593
Conc: 21.49 ng/ml

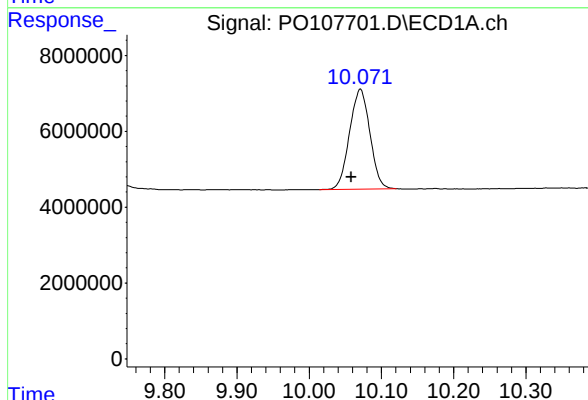

#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: 0.013 min
Response: 51599060
Conc: 21.03 ng/ml

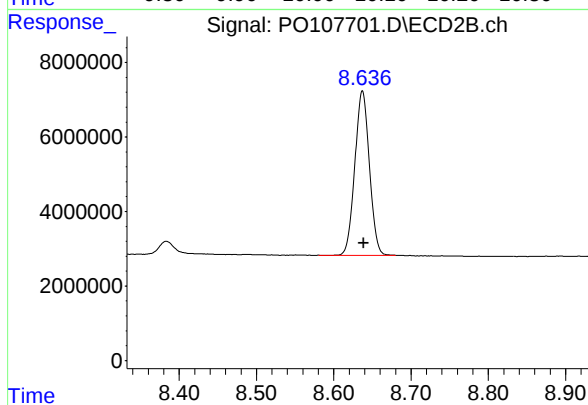

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.002 min
Response: 57354344
Conc: 20.92 ng/ml

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	11/05/24
Project:	120-122 Liberty Ave BK	Date Received:	11/05/24
Client Sample ID:	PIBLK-PO107715.D	SDG No.:	P4699
Lab Sample ID:	I.BLK-PO107715.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107715.D	1		11/05/24	PO110524

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.7		70 (60) - 130 (140)	109%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.0		70 (60) - 130 (140)	110%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 23:42
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 01:02:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.642	198.2E6	70716092	21.742	21.972
2) SA Decachlor...	10.074	8.638	54072498	63243261	22.040	23.068

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 23:42
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 01:02:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

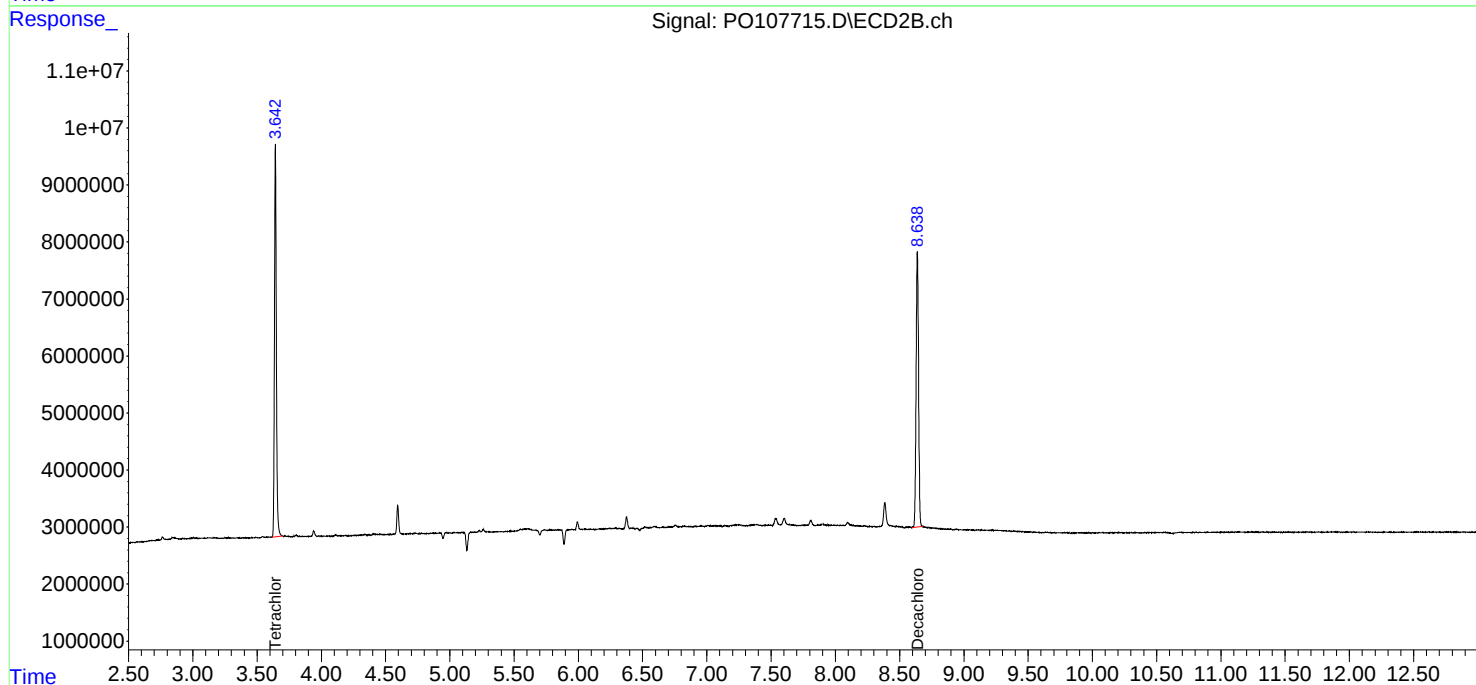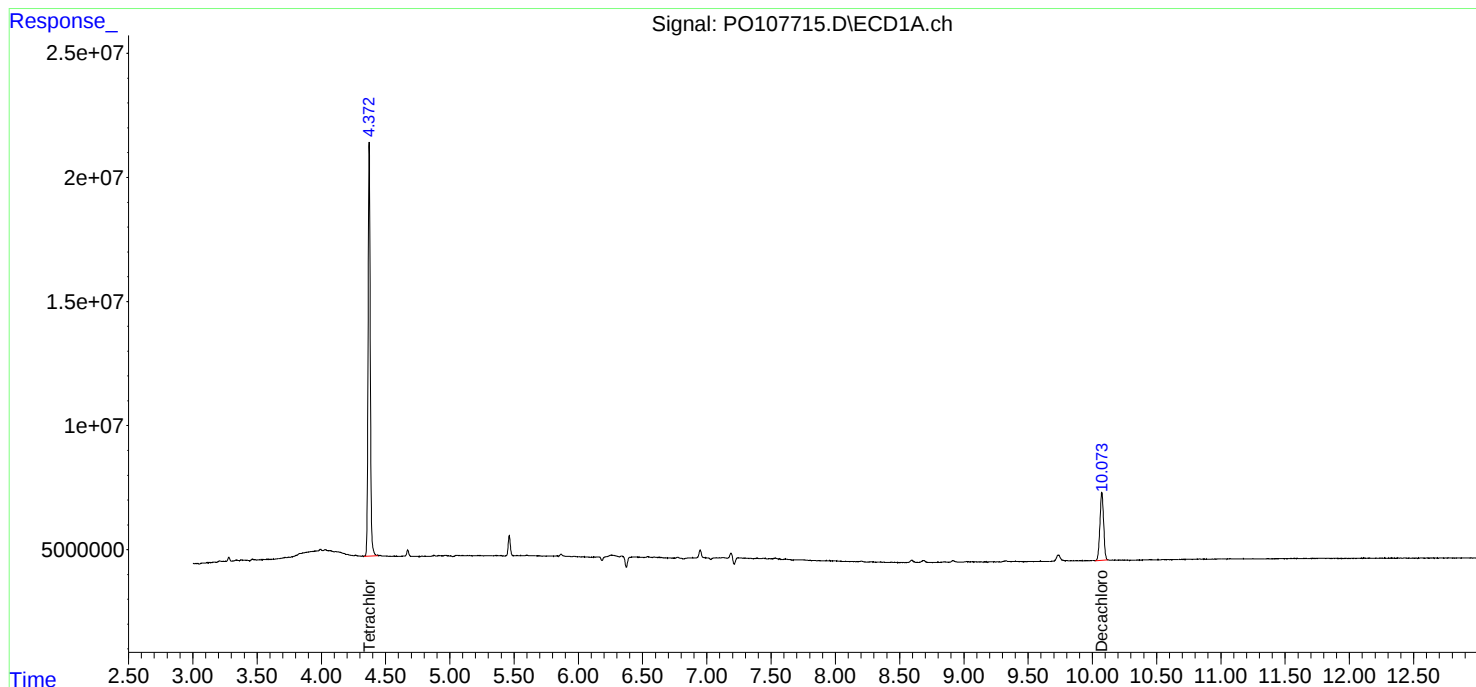


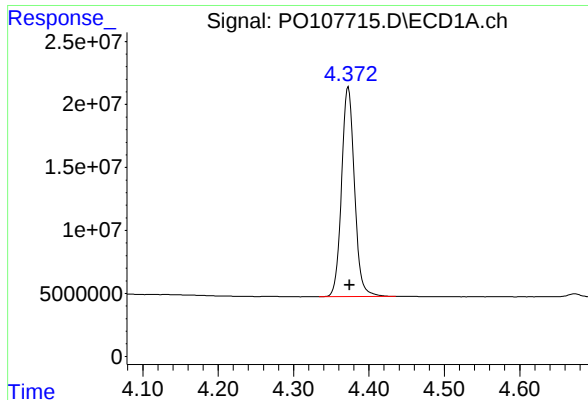

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: -0.001 min
Response: 198158885
Conc: 21.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

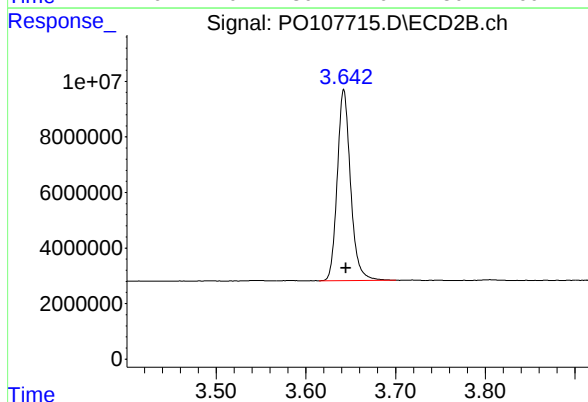


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.002 min
Response: 70716092
Conc: 21.97 ng/ml

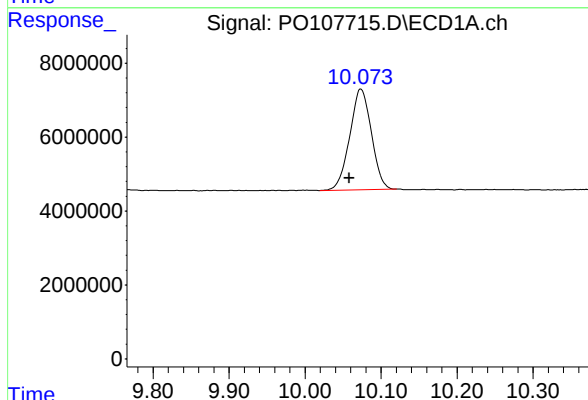

#2 Decachlorobiphenyl

R.T.: 10.074 min
Delta R.T.: 0.015 min
Response: 54072498
Conc: 22.04 ng/ml

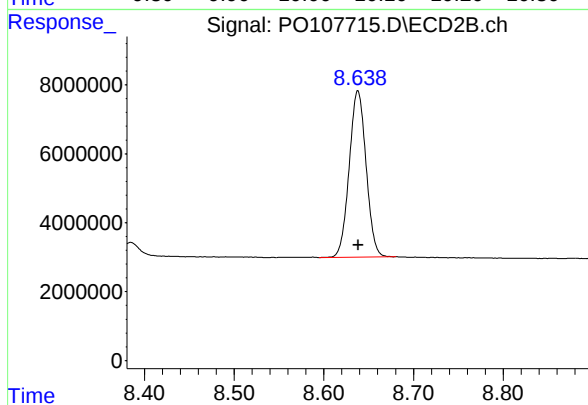

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 63243261
Conc: 23.07 ng/ml

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	
Project:	120-122 Liberty Ave BK	Date Received:	
Client Sample ID:	PB164678BS	SDG No.:	P4699
Lab Sample ID:	PB164678BS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	100
Sample Wt/Vol:	30.01	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107688.D	1	11/05/24 08:35	11/05/24 15:16	PB164678

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	155		3.40	17.0	ug/kg
11104-28-2	Aroclor-1221	6.40	U	6.40	17.0	ug/kg
11141-16-5	Aroclor-1232	3.40	U	3.40	17.0	ug/kg
53469-21-9	Aroclor-1242	3.40	U	3.40	17.0	ug/kg
12672-29-6	Aroclor-1248	7.90	U	7.90	17.0	ug/kg
11097-69-1	Aroclor-1254	2.70	U	2.70	17.0	ug/kg
37324-23-5	Aroclor-1262	4.60	U	4.60	17.0	ug/kg
11100-14-4	Aroclor-1268	3.40	U	3.40	17.0	ug/kg
11096-82-5	Aroclor-1260	156		2.90	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.3		30 (32) - 150 (144)	107%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.9		30 (32) - 150 (175)	109%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 15:16
 Operator : YP/AJ
 Sample : PB164678BS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB164678BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:46:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.643	194.3E6	65152758	21.325	20.243
2) SA Decachlor...	10.071	8.636	53624821	59167262	21.858	21.581
Target Compounds						
3) L1 AR-1016-1	5.523	4.723	128.5E6	49534534	476.416	479.681
4) L1 AR-1016-2	5.544	4.742	184.0E6	68809838	463.637	488.125
5) L1 AR-1016-3	5.607	4.918	114.5E6	37068941	455.739	470.743
6) L1 AR-1016-4	5.704	4.959	91029031	28459100	472.603	430.492
7) L1 AR-1016-5	5.999	5.173	83652574	37260018	457.985	453.650
31) L7 AR-1260-1	7.128	6.202	129.2E6	73581512	499.797	474.246
32) L7 AR-1260-2	7.385	6.390	134.5E6	88364076	510.877	501.739
33) L7 AR-1260-3	7.747	6.543	75580135	82085088	420.485	489.335
34) L7 AR-1260-4	7.972	7.014	81977780	60130738	467.100	415.610
35) L7 AR-1260-5	8.287	7.255	126.3E6	143.0E6	444.055	433.917



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 15:16
Operator : YP/AJ
Sample : PB164678BS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB164678BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:46:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

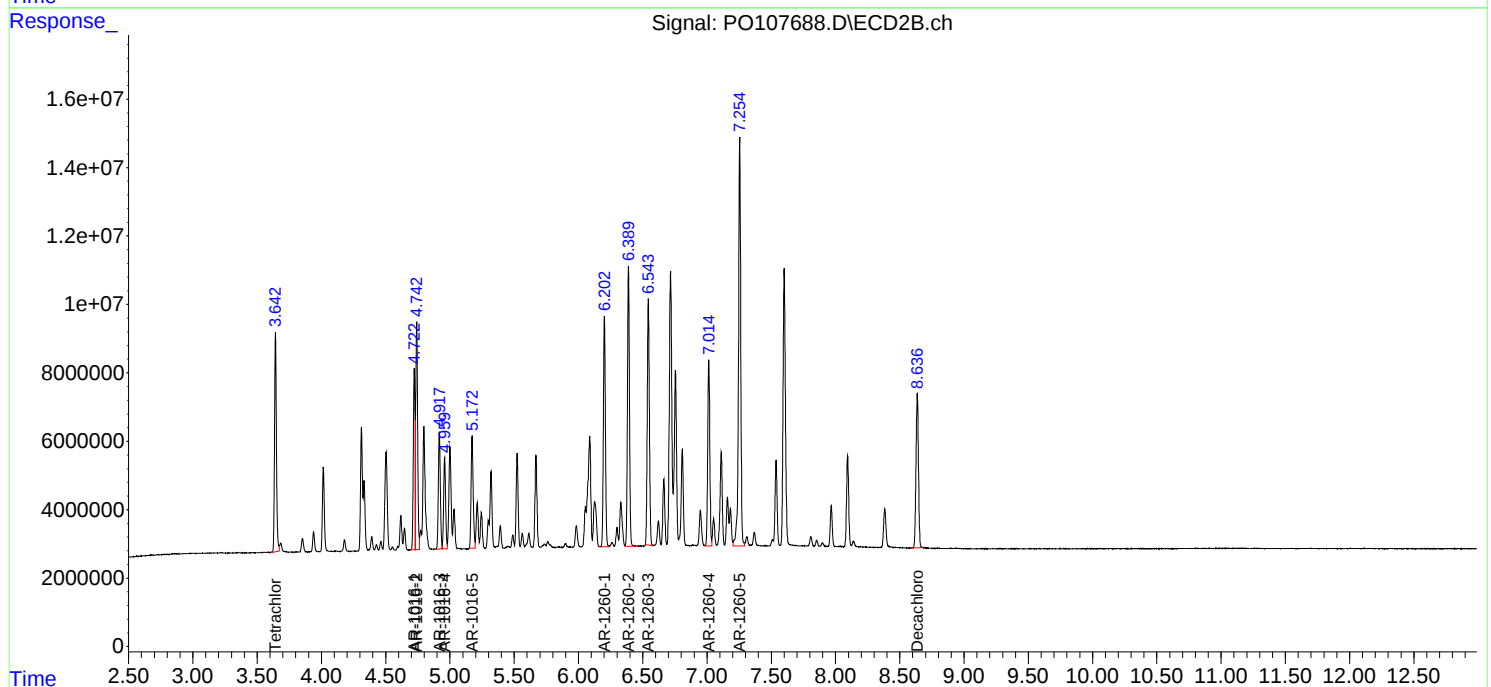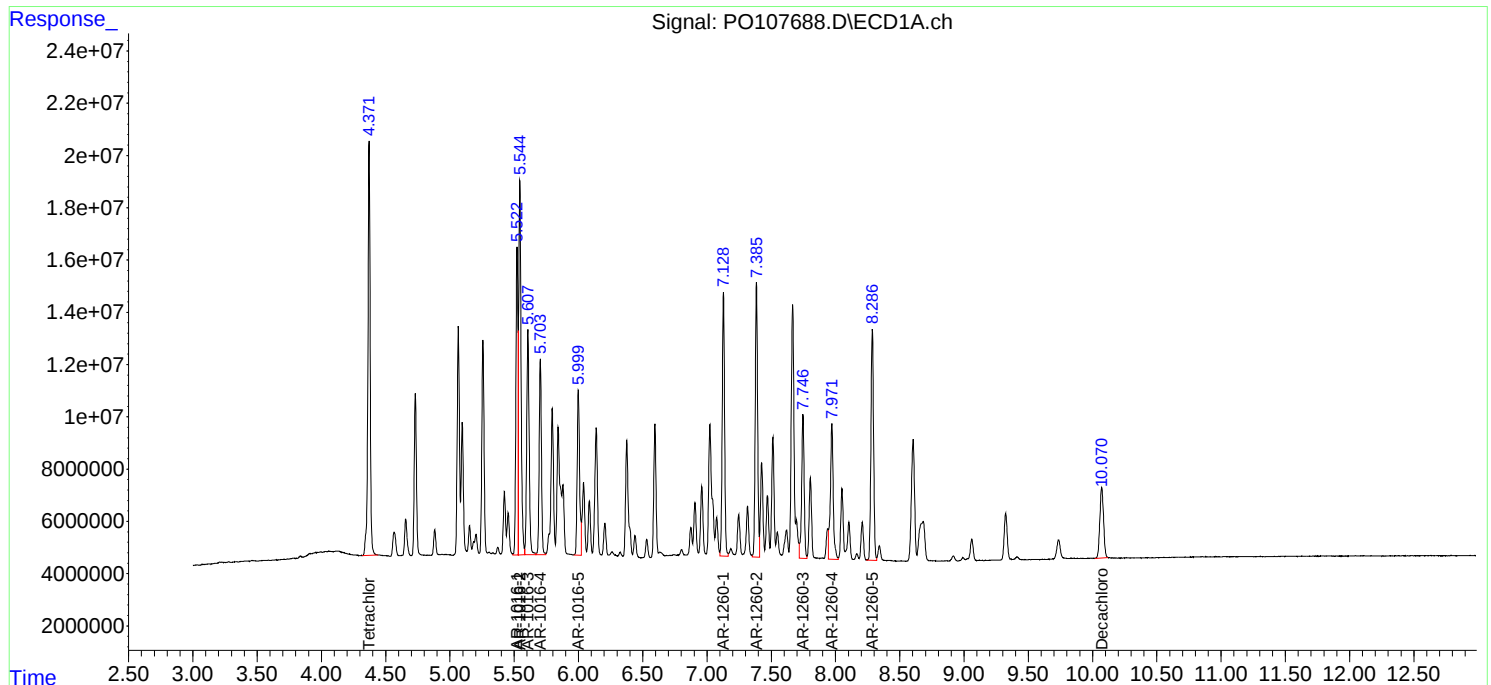

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	11/04/24
Project:	120-122 Liberty Ave BK	Date Received:	11/04/24
Client Sample ID:	BP-F3MS	SDG No.:	P4699
Lab Sample ID:	P4701-01MS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	83.7
Sample Wt/Vol:	30.02	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107706.D	1	11/05/24 08:35	11/05/24 20:43	PB164678

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	236		4.00	20.3	ug/kg
11104-28-2	Aroclor-1221	7.70	U	7.70	20.3	ug/kg
11141-16-5	Aroclor-1232	4.10	U	4.10	20.3	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	20.3	ug/kg
12672-29-6	Aroclor-1248	9.40	U	9.40	20.3	ug/kg
11097-69-1	Aroclor-1254	3.30	U	3.30	20.3	ug/kg
37324-23-5	Aroclor-1262	5.50	U	5.50	20.3	ug/kg
11100-14-4	Aroclor-1268	4.10	U	4.10	20.3	ug/kg
11096-82-5	Aroclor-1260	215		3.50	20.3	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	24.7		30 (32) - 150 (144)	123%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.9		30 (32) - 150 (175)	109%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 20:43
 Operator : YP/AJ
 Sample : P4701-01MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

BP-F3MS

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/06/2024

Supervised By :Ankita Jodhani 11/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:57:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.642	224.8E6	78371995	24.670	24.350
2) SA Decachlor...	10.072	8.637	52676649	59900443	21.471	21.849
Target Compounds						
3) L1 AR-1016-1	5.523	4.723	153.5E6	63543574	568.835	615.341
4) L1 AR-1016-2	5.546	4.742	221.5E6	90216821	557.983	639.982
5) L1 AR-1016-3	5.609	4.918	134.6E6	47771285	536.007	606.653
6) L1 AR-1016-4	5.705	4.959	110.8E6	35528000	575.301	537.421
7) L1 AR-1016-5	6.001	5.173	101.5E6	45989455	555.837	559.933
31) L7 AR-1260-1	7.130	6.204	139.2E6	85240865	538.410	549.393
32) L7 AR-1260-2	7.386	6.391	144.3E6	106.2E6	548.345	602.966
33) L7 AR-1260-3	7.749	6.544	87546421	95945976	487.059	571.964
34) L7 AR-1260-4	7.973	7.015	97949819	69532457	558.106m	480.592
35) L7 AR-1260-5	8.288	7.256	148.3E6	163.0E6	521.622	494.745

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 20:43
Operator : YP/AJ
Sample : P4701-01MS
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BP-F3MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/06/2024
Supervised By :Ankita Jodhani 11/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:57:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

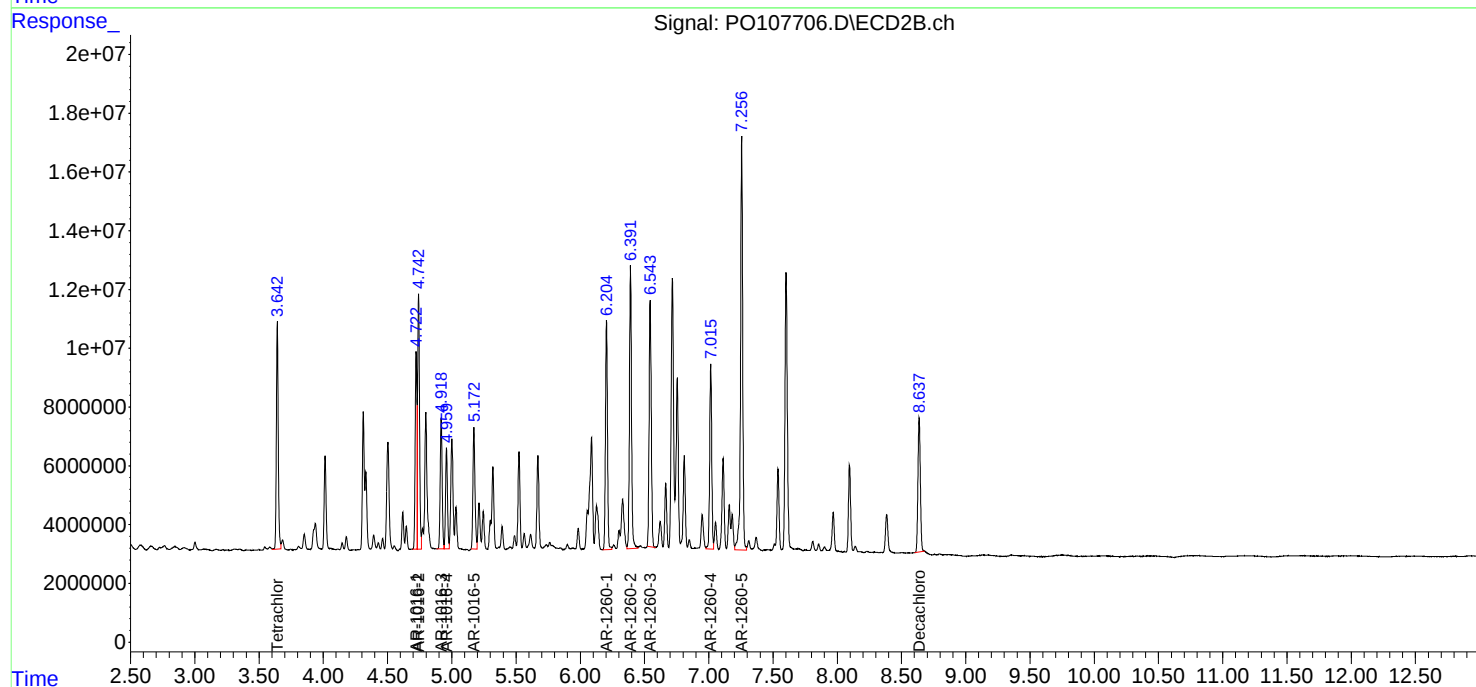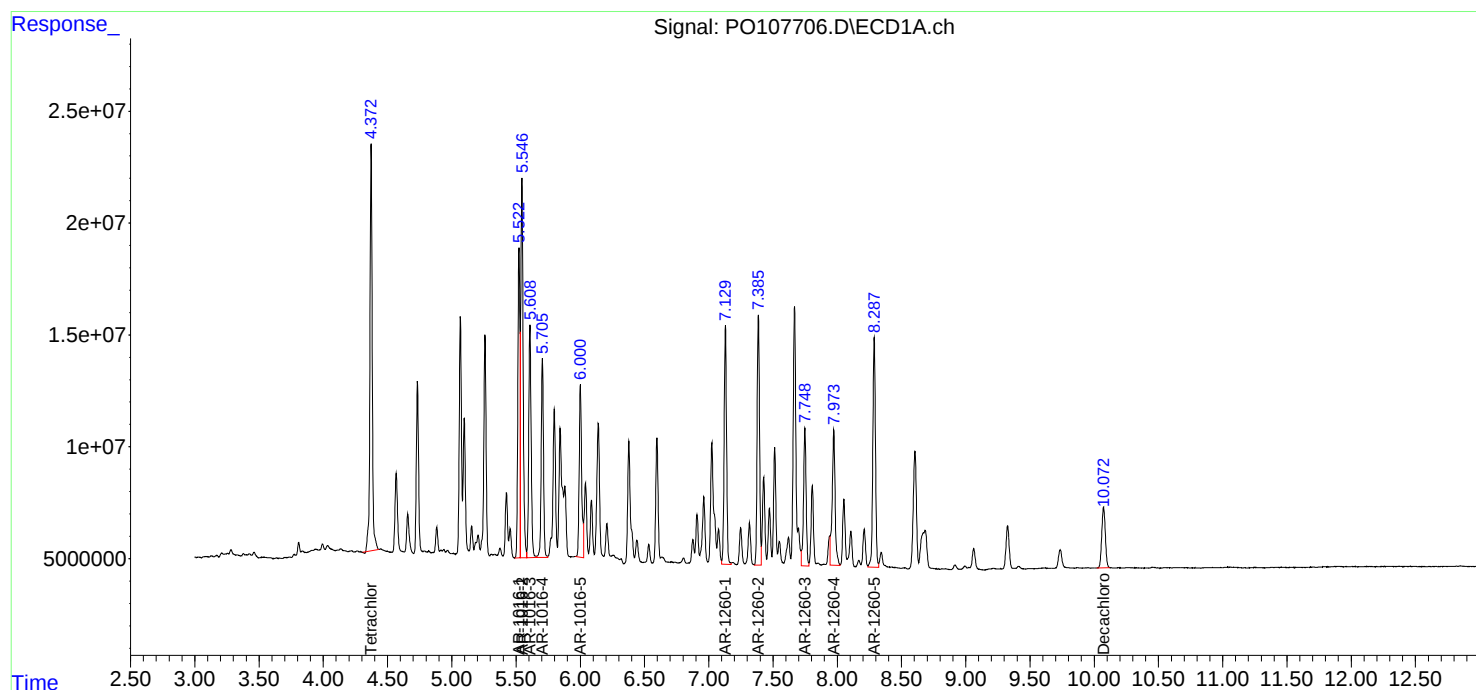

Report of Analysis

Client:	EarthEfficient LLC	Date Collected:	11/04/24
Project:	120-122 Liberty Ave BK	Date Received:	11/04/24
Client Sample ID:	BP-F3MSD	SDG No.:	P4699
Lab Sample ID:	P4701-01MSD	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	83.7
Sample Wt/Vol:	30.04	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107707.D	1	11/05/24 08:35	11/05/24 20:59	PB164678

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	244		4.00	20.3	ug/kg
11104-28-2	Aroclor-1221	7.60	U	7.60	20.3	ug/kg
11141-16-5	Aroclor-1232	4.10	U	4.10	20.3	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	20.3	ug/kg
12672-29-6	Aroclor-1248	9.40	U	9.40	20.3	ug/kg
11097-69-1	Aroclor-1254	3.30	U	3.30	20.3	ug/kg
37324-23-5	Aroclor-1262	5.50	U	5.50	20.3	ug/kg
11100-14-4	Aroclor-1268	4.10	U	4.10	20.3	ug/kg
11096-82-5	Aroclor-1260	220		3.50	20.3	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	24.8		30 (32) - 150 (144)	124%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.7		30 (32) - 150 (175)	109%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
 Data File : PO107707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2024 20:59
 Operator : YP/AJ
 Sample : P4701-01MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

BP-F3MSD

Manual Integrations**APPROVED**

Reviewed By :Yogesh Patel 11/06/2024

Supervised By :Ankita Jodhani 11/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:57:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	214.0E6	79768989	23.480	24.785
2) SA Decachlor...	10.071	8.637	53283533	59484206	21.718	21.697
Target Compounds						
3) L1 AR-1016-1	5.522	4.723	165.2E6	66045470	612.139	639.569
4) L1 AR-1016-2	5.544	4.741	236.7E6	92671351	596.504	657.394
5) L1 AR-1016-3	5.607	4.917	144.2E6	49352025	574.174	626.727
6) L1 AR-1016-4	5.703	4.959	120.1E6	36877141	623.494	557.829
7) L1 AR-1016-5	5.998	5.172	105.9E6	47673979	579.573	580.443
31) L7 AR-1260-1	7.128	6.203	138.5E6	89349183	535.697	575.872
32) L7 AR-1260-2	7.385	6.390	149.7E6	104.4E6	568.550	592.668
33) L7 AR-1260-3	7.747	6.544	91145675	94986236	507.083	566.243
34) L7 AR-1260-4	7.972	7.015	101.7E6	73304045	579.359m	506.661
35) L7 AR-1260-5	8.287	7.256	151.5E6	174.1E6	532.794	528.615

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110524\
Data File : PO107707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2024 20:59
Operator : YP/AJ
Sample : P4701-01MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

BP-F3MSD

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 11/06/2024

Supervised By :Ankita Jodhani 11/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:57:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

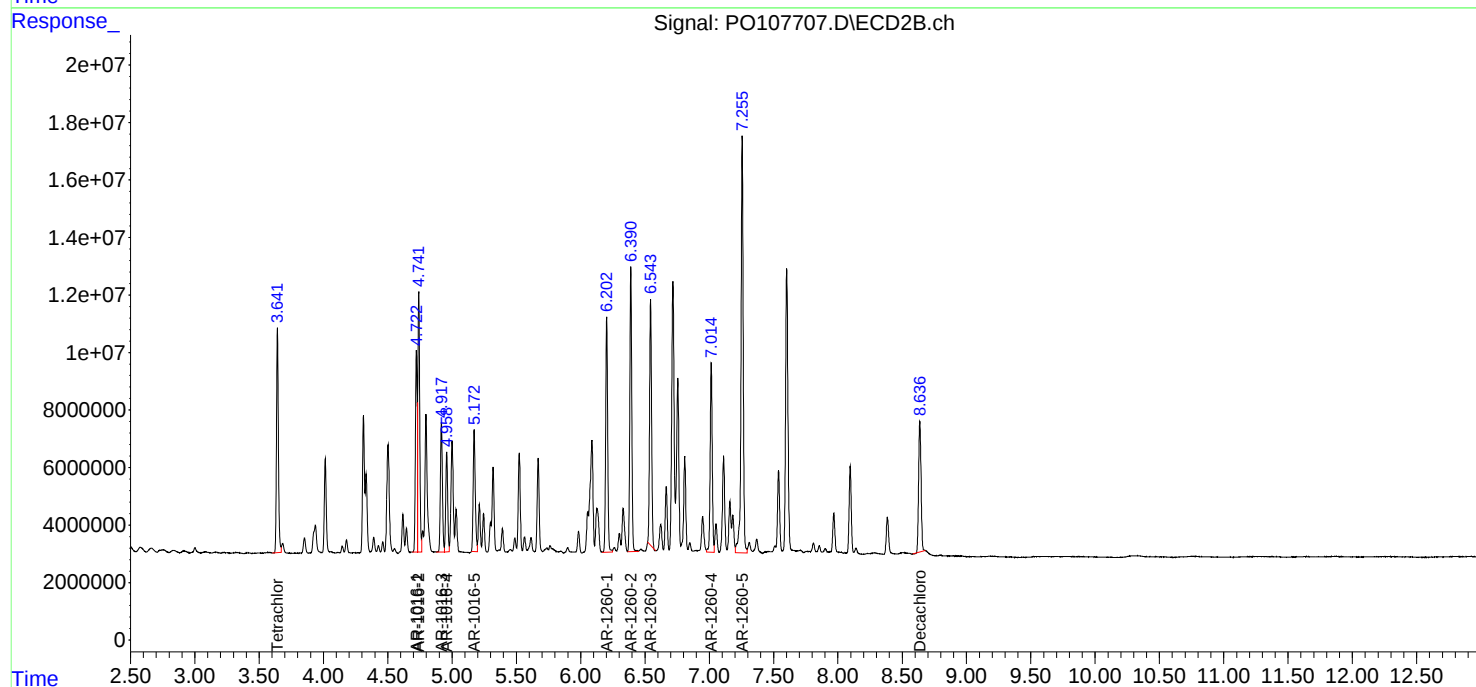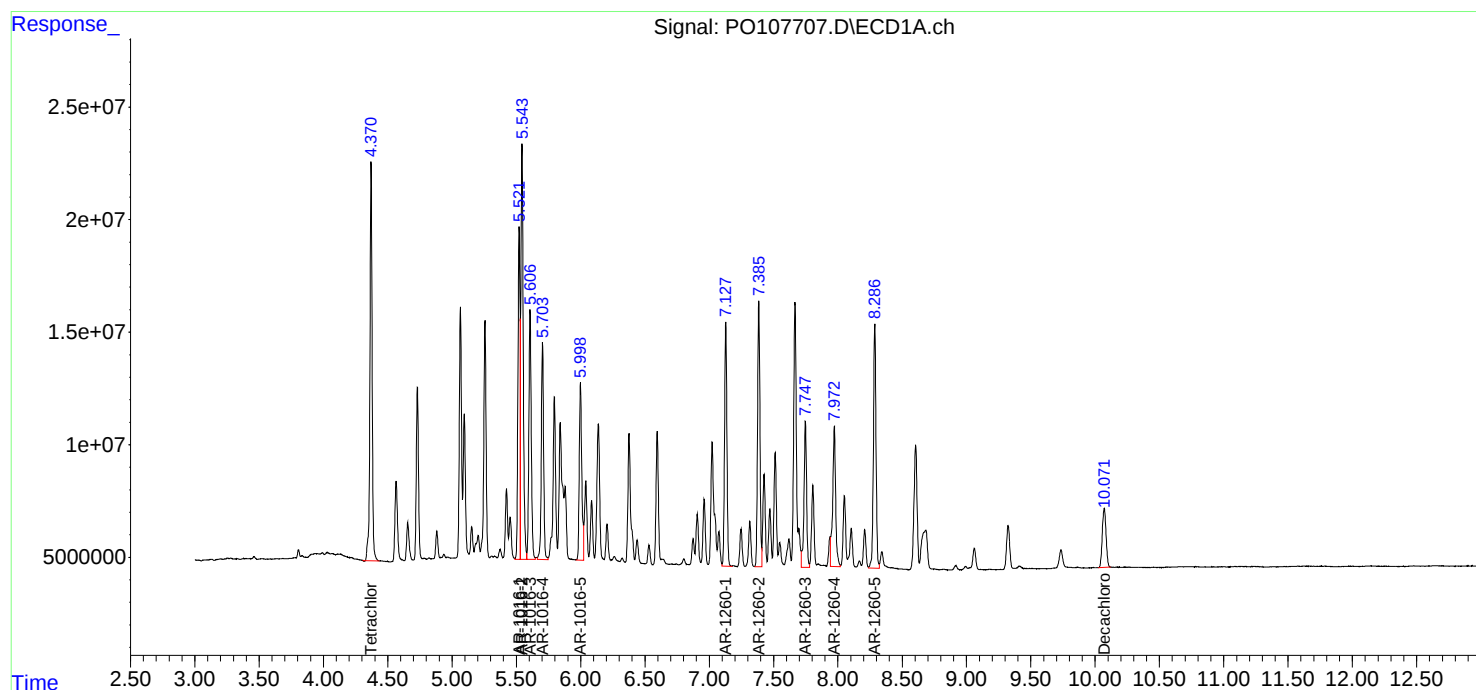

Manual Integration Report

Sequence:	po101524	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC050	PO107188.D	AR-1260-1 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-2 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-3	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-3 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-4 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-5	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-5 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	Decachlorobiphenyl #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1268ICC050	PO107211.D	AR-1268-1	yogesh	10/16/2024 8:49:03 AM	Ankita	10/16/2024 9:57:36	Peak Integrated by Software

Manual Integration Report

Sequence:	PO110524	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254CCC500	PO107677.D	AR-1254-2 #2	yogesh	11/6/2024 9:28:08 AM	Ankita	11/6/2024 9:43:56	Peak Integrated by Software
AR1254CCC500	PO107677.D	AR-1254-5	yogesh	11/6/2024 9:28:08 AM	Ankita	11/6/2024 9:43:56	Peak Integrated by Software
AR1254CCC500	PO107685.D	AR-1254-2 #2	yogesh	11/6/2024 9:28:10 AM	Ankita	11/6/2024 9:43:59	Peak Integrated by Software
AR1254CCC500	PO107700.D	AR-1254-2 #2	yogesh	11/6/2024 9:28:26 AM	Ankita	11/6/2024 9:44:23	Peak Integrated by Software
P4701-01MS	PO107706.D	AR-1260-4	yogesh	11/6/2024 9:28:32 AM	Ankita	11/6/2024 9:45:31	Peak Integrated by Software
P4701-01MSD	PO107707.D	AR-1260-4	yogesh	11/6/2024 9:28:33 AM	Ankita	11/6/2024 9:45:32	Peak Integrated by Software
AR1254CCC500	PO107714.D	AR-1254-2 #2	yogesh	11/6/2024 9:28:38 AM	Ankita	11/6/2024 9:45:49	Peak Integrated by Software
AR1254CCC500	PO107723.D	AR-1254-2 #2	yogesh	11/6/2024 9:28:58 AM	Ankita	11/6/2024 9:45:56	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO107180.D	15 Oct 2024 13:05	YP/AJ	Ok
2	AR1660CCC500	PO107181.D	15 Oct 2024 13:23	YP/AJ	Not Ok
3	HEXANE	PO107182.D	15 Oct 2024 17:50	YP/AJ	Ok
4	I.BLK	PO107183.D	15 Oct 2024 18:08	YP/AJ	Ok
5	AR1660ICC1000	PO107184.D	15 Oct 2024 18:27	YP/AJ	Ok
6	AR1660ICC750	PO107185.D	15 Oct 2024 18:45	YP/AJ	Ok
7	AR1660ICC500	PO107186.D	15 Oct 2024 19:03	YP/AJ	Ok
8	AR1660ICC250	PO107187.D	15 Oct 2024 19:21	YP/AJ	Ok
9	AR1660ICC050	PO107188.D	15 Oct 2024 19:39	YP/AJ	Ok,M
10	AR1221ICC500	PO107189.D	15 Oct 2024 19:57	YP/AJ	Ok
11	AR1232ICC500	PO107190.D	15 Oct 2024 20:15	YP/AJ	Ok
12	AR1242ICC1000	PO107191.D	15 Oct 2024 20:34	YP/AJ	Ok
13	AR1242ICC750	PO107192.D	15 Oct 2024 20:52	YP/AJ	Ok
14	AR1242ICC500	PO107193.D	15 Oct 2024 21:10	YP/AJ	Ok
15	AR1242ICC250	PO107194.D	15 Oct 2024 21:28	YP/AJ	Ok
16	AR1242ICC050	PO107195.D	15 Oct 2024 21:46	YP/AJ	Ok
17	AR1248ICC1000	PO107196.D	15 Oct 2024 22:04	YP/AJ	Ok
18	AR1248ICC750	PO107197.D	15 Oct 2024 22:22	YP/AJ	Ok
19	AR1248ICC500	PO107198.D	15 Oct 2024 22:41	YP/AJ	Ok
20	AR1248ICC250	PO107199.D	15 Oct 2024 22:59	YP/AJ	Ok
21	AR1248ICC050	PO107200.D	15 Oct 2024 23:17	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC1000	PO107201.D	15 Oct 2024 23:35	YP/AJ	Ok
23	AR1254ICC750	PO107202.D	15 Oct 2024 23:53	YP/AJ	Ok
24	AR1254ICC500	PO107203.D	16 Oct 2024 00:11	YP/AJ	Ok
25	AR1254ICC250	PO107204.D	16 Oct 2024 00:29	YP/AJ	Ok
26	AR1254ICC050	PO107205.D	16 Oct 2024 00:47	YP/AJ	Ok
27	AR1262ICC500	PO107206.D	16 Oct 2024 01:05	YP/AJ	Ok
28	AR1268ICC1000	PO107207.D	16 Oct 2024 01:23	YP/AJ	Ok
29	AR1268ICC750	PO107208.D	16 Oct 2024 01:41	YP/AJ	Ok
30	AR1268ICC500	PO107209.D	16 Oct 2024 01:59	YP/AJ	Ok
31	AR1268ICC250	PO107210.D	16 Oct 2024 02:18	YP/AJ	Ok
32	AR1268ICC050	PO107211.D	16 Oct 2024 02:36	YP/AJ	Ok,M
33	PO101524ICV500	PO107212.D	16 Oct 2024 02:54	YP/AJ	Ok
34	AR1242ICV500	PO107213.D	16 Oct 2024 03:12	YP/AJ	Ok
35	AR1248ICV500	PO107214.D	16 Oct 2024 03:30	YP/AJ	Ok
36	AR1254ICV500	PO107215.D	16 Oct 2024 03:48	YP/AJ	Ok
37	AR1268ICV500	PO107216.D	16 Oct 2024 04:06	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110524

Review By	yogesh	Review On	11/6/2024 9:29:20 AM
Supervise By	Ankita	Supervise On	11/6/2024 9:46:53 AM
SubDirectory	PO110524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775 PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773 PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO107673.D	05 Nov 2024 09:02	YP/AJ	Ok
2	AR1660CCC500	PO107674.D	05 Nov 2024 09:19	YP/AJ	Ok
3	AR1242CCC500	PO107675.D	05 Nov 2024 10:16	YP/AJ	Ok
4	AR1248CCC500	PO107676.D	05 Nov 2024 10:32	YP/AJ	Ok
5	AR1254CCC500	PO107677.D	05 Nov 2024 10:49	YP/AJ	Ok,M
6	I.BLK	PO107678.D	05 Nov 2024 11:06	YP/AJ	Ok
7	PB144677BL	PO107679.D	05 Nov 2024 11:43	YP/AJ	Ok
8	PB144677BS	PO107680.D	05 Nov 2024 11:59	YP/AJ	Ok
9	P4677-01	PO107681.D	05 Nov 2024 12:15	YP/AJ	Ok,M
10	AR1660CCC500	PO107682.D	05 Nov 2024 13:01	YP/AJ	Ok
11	AR1242CCC500	PO107683.D	05 Nov 2024 13:18	YP/AJ	Ok
12	AR1248CCC500	PO107684.D	05 Nov 2024 13:35	YP/AJ	Ok
13	AR1254CCC500	PO107685.D	05 Nov 2024 13:52	YP/AJ	Ok,M
14	I.BLK	PO107686.D	05 Nov 2024 14:09	YP/AJ	Ok
15	PB164678BL	PO107687.D	05 Nov 2024 15:00	YP/AJ	Ok
16	PB164678BS	PO107688.D	05 Nov 2024 15:16	YP/AJ	Ok
17	P4682-01	PO107689.D	05 Nov 2024 15:33	YP/AJ	Ok,M
18	P4684-01	PO107690.D	05 Nov 2024 15:49	YP/AJ	Ok,M
19	P4685-01	PO107691.D	05 Nov 2024 16:06	YP/AJ	Ok,M
20	P4693-01	PO107692.D	05 Nov 2024 16:23	YP/AJ	Ok,M
21	P4693-05	PO107693.D	05 Nov 2024 16:39	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110524

Review By	yogesh	Review On	11/6/2024 9:29:20 AM
Supervise By	Ankita	Supervise On	11/6/2024 9:46:53 AM
SubDirectory	PO110524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	P4694-01	PO107694.D	05 Nov 2024 16:55	YP/AJ	Ok,M
23	P4694-05	PO107695.D	05 Nov 2024 17:12	YP/AJ	Ok,M
24	P4695-01	PO107696.D	05 Nov 2024 17:28	YP/AJ	Ok,M
25	AR1660CCC500	PO107697.D	05 Nov 2024 18:14	YP/AJ	Ok
26	AR1242CCC500	PO107698.D	05 Nov 2024 18:31	YP/AJ	Ok
27	AR1248CCC500	PO107699.D	05 Nov 2024 18:48	YP/AJ	Ok
28	AR1254CCC500	PO107700.D	05 Nov 2024 19:04	YP/AJ	Ok,M
29	I.BLK	PO107701.D	05 Nov 2024 19:20	YP/AJ	Ok
30	P4697-01	PO107702.D	05 Nov 2024 19:36	YP/AJ	Ok,M
31	P4699-01	PO107703.D	05 Nov 2024 19:53	YP/AJ	Ok
32	P4700-01	PO107704.D	05 Nov 2024 20:10	YP/AJ	Ok,M
33	P4701-01	PO107705.D	05 Nov 2024 20:26	YP/AJ	Ok
34	P4701-01MS	PO107706.D	05 Nov 2024 20:43	YP/AJ	Ok,M
35	P4701-01MSD	PO107707.D	05 Nov 2024 20:59	YP/AJ	Ok,M
36	P4701-05	PO107708.D	05 Nov 2024 21:15	YP/AJ	Ok
37	P4711-01	PO107709.D	05 Nov 2024 21:31	YP/AJ	Ok,M
38	P4711-06	PO107710.D	05 Nov 2024 21:48	YP/AJ	Ok,M
39	AR1660CCC500	PO107711.D	05 Nov 2024 22:34	YP/AJ	Ok
40	AR1242CCC500	PO107712.D	05 Nov 2024 22:51	YP/AJ	Ok
41	AR1248CCC500	PO107713.D	05 Nov 2024 23:07	YP/AJ	Ok
42	AR1254CCC500	PO107714.D	05 Nov 2024 23:25	YP/AJ	Ok,M
43	I.BLK	PO107715.D	05 Nov 2024 23:42	YP/AJ	Ok
44	P4705-01	PO107716.D	05 Nov 2024 23:58	YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110524

Review By	yogesh	Review On	11/6/2024 9:29:20 AM
Supervise By	Ankita	Supervise On	11/6/2024 9:46:53 AM
SubDirectory	PO110524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

45	P4703-02	PO107717.D	06 Nov 2024 00:14	YP/AJ	Ok,M
46	P4703-03	PO107718.D	06 Nov 2024 00:30	YP/AJ	Ok,M
47	P4703-01	PO107719.D	06 Nov 2024 00:47	YP/AJ	Ok,M
48	AR1660CCC500	PO107720.D	06 Nov 2024 02:03	YP/AJ	Ok
49	AR1242CCC500	PO107721.D	06 Nov 2024 02:19	YP/AJ	Ok
50	AR1248CCC500	PO107722.D	06 Nov 2024 02:35	YP/AJ	Ok
51	AR1254CCC500	PO107723.D	06 Nov 2024 02:51	YP/AJ	Ok,M
52	I.BLK	PO107724.D	06 Nov 2024 03:08	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO107180.D	15 Oct 2024 13:05		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO107181.D	15 Oct 2024 13:23	need ICAL	YP/AJ	Not Ok
3	HEXANE	HEXANE	PO107182.D	15 Oct 2024 17:50		YP/AJ	Ok
4	I.BLK	I.BLK	PO107183.D	15 Oct 2024 18:08		YP/AJ	Ok
5	AR1660ICC1000	AR1660ICC1000	PO107184.D	15 Oct 2024 18:27		YP/AJ	Ok
6	AR1660ICC750	AR1660ICC750	PO107185.D	15 Oct 2024 18:45		YP/AJ	Ok
7	AR1660ICC500	AR1660ICC500	PO107186.D	15 Oct 2024 19:03		YP/AJ	Ok
8	AR1660ICC250	AR1660ICC250	PO107187.D	15 Oct 2024 19:21		YP/AJ	Ok
9	AR1660ICC050	AR1660ICC050	PO107188.D	15 Oct 2024 19:39		YP/AJ	Ok,M
10	AR1221ICC500	AR1221ICC500	PO107189.D	15 Oct 2024 19:57		YP/AJ	Ok
11	AR1232ICC500	AR1232ICC500	PO107190.D	15 Oct 2024 20:15		YP/AJ	Ok
12	AR1242ICC1000	AR1242ICC1000	PO107191.D	15 Oct 2024 20:34		YP/AJ	Ok
13	AR1242ICC750	AR1242ICC750	PO107192.D	15 Oct 2024 20:52		YP/AJ	Ok
14	AR1242ICC500	AR1242ICC500	PO107193.D	15 Oct 2024 21:10		YP/AJ	Ok
15	AR1242ICC250	AR1242ICC250	PO107194.D	15 Oct 2024 21:28		YP/AJ	Ok
16	AR1242ICC050	AR1242ICC050	PO107195.D	15 Oct 2024 21:46		YP/AJ	Ok
17	AR1248ICC1000	AR1248ICC1000	PO107196.D	15 Oct 2024 22:04		YP/AJ	Ok
18	AR1248ICC750	AR1248ICC750	PO107197.D	15 Oct 2024 22:22		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775 PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773 PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248ICC500	AR1248ICC500	PO107198.D	15 Oct 2024 22:41		YP/AJ	Ok
20	AR1248ICC250	AR1248ICC250	PO107199.D	15 Oct 2024 22:59		YP/AJ	Ok
21	AR1248ICC050	AR1248ICC050	PO107200.D	15 Oct 2024 23:17		YP/AJ	Ok
22	AR1254ICC1000	AR1254ICC1000	PO107201.D	15 Oct 2024 23:35		YP/AJ	Ok
23	AR1254ICC750	AR1254ICC750	PO107202.D	15 Oct 2024 23:53		YP/AJ	Ok
24	AR1254ICC500	AR1254ICC500	PO107203.D	16 Oct 2024 00:11		YP/AJ	Ok
25	AR1254ICC250	AR1254ICC250	PO107204.D	16 Oct 2024 00:29		YP/AJ	Ok
26	AR1254ICC050	AR1254ICC050	PO107205.D	16 Oct 2024 00:47		YP/AJ	Ok
27	AR1262ICC500	AR1262ICC500	PO107206.D	16 Oct 2024 01:05		YP/AJ	Ok
28	AR1268ICC1000	AR1268ICC1000	PO107207.D	16 Oct 2024 01:23		YP/AJ	Ok
29	AR1268ICC750	AR1268ICC750	PO107208.D	16 Oct 2024 01:41		YP/AJ	Ok
30	AR1268ICC500	AR1268ICC500	PO107209.D	16 Oct 2024 01:59		YP/AJ	Ok
31	AR1268ICC250	AR1268ICC250	PO107210.D	16 Oct 2024 02:18		YP/AJ	Ok
32	AR1268ICC050	AR1268ICC050	PO107211.D	16 Oct 2024 02:36		YP/AJ	Ok,M
33	PO101524ICV500	ICVPO101524	PO107212.D	16 Oct 2024 02:54		YP/AJ	Ok
34	AR1242ICV500	ICVPO101524AR1242	PO107213.D	16 Oct 2024 03:12		YP/AJ	Ok
35	AR1248ICV500	ICVPO101524AR1248	PO107214.D	16 Oct 2024 03:30		YP/AJ	Ok
36	AR1254ICV500	ICVPO101524AR1254	PO107215.D	16 Oct 2024 03:48		YP/AJ	Ok
37	AR1268ICV500	ICVPO101524AR1268	PO107216.D	16 Oct 2024 04:06		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110524

Review By	yogesh	Review On	11/6/2024 9:29:20 AM
Supervise By	Ankita	Supervise On	11/6/2024 9:46:53 AM
SubDirectory	PO110524	HP Acquire Method	HP Processing Method PO101524

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO107673.D	05 Nov 2024 09:02		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO107674.D	05 Nov 2024 09:19		YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO107675.D	05 Nov 2024 10:16		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO107676.D	05 Nov 2024 10:32		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO107677.D	05 Nov 2024 10:49		YP/AJ	Ok,M
6	I.BLK	I.BLK	PO107678.D	05 Nov 2024 11:06		YP/AJ	Ok
7	PB144677BL	PB144677BL	PO107679.D	05 Nov 2024 11:43		YP/AJ	Ok
8	PB144677BS	PB144677BS	PO107680.D	05 Nov 2024 11:59		YP/AJ	Ok
9	P4677-01	2410-6346	PO107681.D	05 Nov 2024 12:15		YP/AJ	Ok,M
10	AR1660CCC500	AR1660CCC500	PO107682.D	05 Nov 2024 13:01		YP/AJ	Ok
11	AR1242CCC500	AR1242CCC500	PO107683.D	05 Nov 2024 13:18		YP/AJ	Ok
12	AR1248CCC500	AR1248CCC500	PO107684.D	05 Nov 2024 13:35		YP/AJ	Ok
13	AR1254CCC500	AR1254CCC500	PO107685.D	05 Nov 2024 13:52		YP/AJ	Ok,M
14	I.BLK	I.BLK	PO107686.D	05 Nov 2024 14:09		YP/AJ	Ok
15	PB164678BL	PB164678BL	PO107687.D	05 Nov 2024 15:00		YP/AJ	Ok
16	PB164678BS	PB164678BS	PO107688.D	05 Nov 2024 15:16		YP/AJ	Ok
17	P4682-01	BELL-SHOP-RAGS	PO107689.D	05 Nov 2024 15:33		YP/AJ	Ok,M
18	P4684-01	MECHANIC-ST-SWEE	PO107690.D	05 Nov 2024 15:49	AR1260 Hit	YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110524

Review By	yogesh	Review On	11/6/2024 9:29:20 AM
Supervise By	Ankita	Supervise On	11/6/2024 9:46:53 AM
SubDirectory	PO110524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775 PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773 PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		

19	P4685-01	OK-01-11012024	PO107691.D	05 Nov 2024 16:06		YP/AJ	Ok,M
20	P4693-01	BP-G5-WC	PO107692.D	05 Nov 2024 16:23		YP/AJ	Ok,M
21	P4693-05	BP-G4-WC	PO107693.D	05 Nov 2024 16:39		YP/AJ	Ok
22	P4694-01	Z-03A	PO107694.D	05 Nov 2024 16:55		YP/AJ	Ok,M
23	P4694-05	Z-04	PO107695.D	05 Nov 2024 17:12		YP/AJ	Ok,M
24	P4695-01	Z-01	PO107696.D	05 Nov 2024 17:28		YP/AJ	Ok,M
25	AR1660CCC500	AR1660CCC500	PO107697.D	05 Nov 2024 18:14		YP/AJ	Ok
26	AR1242CCC500	AR1242CCC500	PO107698.D	05 Nov 2024 18:31		YP/AJ	Ok
27	AR1248CCC500	AR1248CCC500	PO107699.D	05 Nov 2024 18:48		YP/AJ	Ok
28	AR1254CCC500	AR1254CCC500	PO107700.D	05 Nov 2024 19:04		YP/AJ	Ok,M
29	I.BLK	I.BLK	PO107701.D	05 Nov 2024 19:20		YP/AJ	Ok
30	P4697-01	TP-1	PO107702.D	05 Nov 2024 19:36		YP/AJ	Ok,M
31	P4699-01	MIXED-DEMO	PO107703.D	05 Nov 2024 19:53		YP/AJ	Ok
32	P4700-01	MH-8	PO107704.D	05 Nov 2024 20:10		YP/AJ	Ok,M
33	P4701-01	BP-F3	PO107705.D	05 Nov 2024 20:26		YP/AJ	Ok
34	P4701-01MS	BP-F3MS	PO107706.D	05 Nov 2024 20:43		YP/AJ	Ok,M
35	P4701-01MSD	BP-F3MSD	PO107707.D	05 Nov 2024 20:59		YP/AJ	Ok,M
36	P4701-05	BP-F4	PO107708.D	05 Nov 2024 21:15		YP/AJ	Ok
37	P4711-01	CF-613-COMP-16	PO107709.D	05 Nov 2024 21:31		YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110524

Review By	yogesh	Review On	11/6/2024 9:29:20 AM
Supervise By	Ankita	Supervise On	11/6/2024 9:46:53 AM
SubDirectory	PO110524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	P4711-06	CF-613-COMP-17	PO107710.D	05 Nov 2024 21:48		YP/AJ	Ok,M
39	AR1660CCC500	AR1660CCC500	PO107711.D	05 Nov 2024 22:34		YP/AJ	Ok
40	AR1242CCC500	AR1242CCC500	PO107712.D	05 Nov 2024 22:51		YP/AJ	Ok
41	AR1248CCC500	AR1248CCC500	PO107713.D	05 Nov 2024 23:07		YP/AJ	Ok
42	AR1254CCC500	AR1254CCC500	PO107714.D	05 Nov 2024 23:25		YP/AJ	Ok,M
43	I.BLK	I.BLK	PO107715.D	05 Nov 2024 23:42		YP/AJ	Ok
44	P4705-01	1024	PO107716.D	05 Nov 2024 23:58	TCMX low in 2nd column,	YP/AJ	Ok,M
45	P4703-02	0910	PO107717.D	06 Nov 2024 00:14	DCB high in 1st column	YP/AJ	Ok,M
46	P4703-03	1008	PO107718.D	06 Nov 2024 00:30		YP/AJ	Ok,M
47	P4703-01	S0-1	PO107719.D	06 Nov 2024 00:47		YP/AJ	Ok,M
48	AR1660CCC500	AR1660CCC500	PO107720.D	06 Nov 2024 02:03		YP/AJ	Ok
49	AR1242CCC500	AR1242CCC500	PO107721.D	06 Nov 2024 02:19		YP/AJ	Ok
50	AR1248CCC500	AR1248CCC500	PO107722.D	06 Nov 2024 02:35		YP/AJ	Ok
51	AR1254CCC500	AR1254CCC500	PO107723.D	06 Nov 2024 02:51		YP/AJ	Ok,M
52	I.BLK	I.BLK	PO107724.D	06 Nov 2024 03:08		YP/AJ	Ok

M : Manual Integration

PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 11/5/2024

OVENTEMP IN Celsius(°C): 107
Time IN: 17:20
In Date: 11/04/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 103
Time OUT: 08:18
Out Date: 11/05/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB133273

Lab ID	Client SampleID	Dish #	Dish Wt (g) (A)	Sample Wt (g)	Dish + Sample Wt (g) (B)	Dish+Dry Sample Wt (g) (C)	% Solid	Comments
P4682-01	BELL-SHOP-RAGS	1	1.00	1.00	2.00	2.00	100.0	debris- rags
P4683-01	GHA605R-1-1	2	1.00	1.00	2.00	2.00	100.0	oilc
P4683-02	GHA605R-1-2	3	1.00	1.00	2.00	2.00	100.0	oilc
P4684-01	MECHANIC-ST-SWEEPINGS	4	1.14	8.39	9.53	8.03	82.1	
P4685-01	OK-01-11012024	5	1.15	8.44	9.59	9.26	96.1	
P4685-02	OK-02-11012024-E2	6	1.13	8.70	9.83	9.4	95.1	
P4686-01	GCP52	26	1.15	8.82	9.97	8.56	84.0	
P4686-02	GCP52MS	27	1.15	8.82	9.97	8.56	84.0	
P4686-03	GCP52MSD	28	1.15	8.82	9.97	8.56	84.0	
P4686-04	GCP53	29	1.13	8.46	9.59	8.19	83.5	
P4686-05	GCP54	30	1.00	1.00	2.00	2.00	100.0	P.T. SAMPLE
P4692-01	TAPLPR-SED02-103124-00-T2	7	1.16	8.50	9.66	8.17	82.5	
P4692-02	TAPLPR-SED01-103124-00-T2	8	1.15	8.59	9.74	8.05	80.3	
P4693-01	BP-G5-WC	9	1.13	8.84	9.97	8.73	86.0	
P4693-02	BP-G5-WC-EPH	10	1.14	8.83	9.97	8.6	84.5	
P4693-03	BP-G5-WC-VOC	11	1.12	8.71	9.83	8.71	87.1	
P4693-05	BP-G4-WC	12	1.13	8.70	9.83	8.84	88.6	
P4693-06	BP-G4-WC-EPH	13	1.15	8.44	9.59	8.13	82.7	
P4693-07	BP-G4-WC-VOC	14	1.15	8.84	9.99	9.53	94.8	
P4694-01	Z-03A	15	1.18	8.44	9.62	8.85	90.9	
P4694-02	Z-03A-EPH	16	1.12	8.66	9.78	8.95	90.4	
P4694-03	Z-03A-VOC	17	1.19	8.52	9.71	8.86	90.0	
P4694-05	Z-04	18	1.14	8.60	9.74	8.8	89.1	
P4694-06	Z-04-EPH	19	1.15	8.63	9.78	8.81	88.8	
P4694-07	Z-04-VOC	20	1.18	8.64	9.82	9.02	90.7	
P4695-01	Z-01	21	1.15	8.44	9.59	8.34	85.2	
P4695-02	Z-01-EPH	22	1.15	8.57	9.72	8.67	87.7	

PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 11/5/2024

OVENTEMP IN Celsius(°C): 107
Time IN: 17:20
In Date: 11/04/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 103
Time OUT: 08:18
Out Date: 11/05/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB133273

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
P4695-03	Z-01-VOC	23	1.18	8.73	9.91	8.74	86.6	
P4697-01	TP-1	24	1.15	8.70	9.85	8.83	88.3	
P4697-02	TP-1	25	1.14	8.68	9.82	9.04	91.0	
P4699-01	MIXED-DEMO	31	1.18	8.76	9.94	9.9	99.5	
P4700-01	MH-8	32	1.15	8.67	9.82	9.06	91.2	
P4700-02	MH-8-EPH	33	1.16	8.51	9.67	8.87	90.6	
P4700-03	MH-8-VOC	34	1.18	8.57	9.75	8.79	88.8	
P4701-01	BP-F3	35	1.11	8.78	9.89	8.46	83.7	
P4701-02	BP-F3-EPH	36	1.15	8.84	9.99	8.43	82.4	
P4701-03	BP-F3-VOC	37	1.15	8.67	9.82	8.06	79.7	
P4701-05	BP-F4	38	1.19	8.52	9.71	8.56	86.5	
P4701-06	BP-F4-EPH	39	1.19	8.67	9.86	8.86	88.5	
P4701-07	BP-F4-VOC	40	1.15	8.56	9.71	8.64	87.5	
P4703-01	S0-1	41	1.00	1.00	2.00	2.00	100.0	oil sample
P4703-02	0910	42	1.00	1.00	2.00	2.00	100.0	debris
P4703-03	1008	43	1.15	8.46	9.61	9.34	96.8	
P4705-01	1024	44	1.00	1.00	2.00	2.00	100.0	debris
P4711-01	CF-613-COMP-16	45	1.16	8.50	9.66	9.2	94.6	
P4711-02	CF-613-VOC-16	46	1.18	8.66	9.84	9.43	95.3	
P4711-03	CF-613-46	47	1.18	8.50	9.68	9.21	94.5	
P4711-04	CF-613-47	48	1.18	8.45	9.63	9.1	93.7	
P4711-06	CF-613-COMP-17	49	1.15	8.52	9.67	9.02	92.4	
P4711-07	CF-613-VOC-17	50	1.16	8.80	9.96	9.32	92.7	
P4711-08	CF-613-48	51	1.15	8.71	9.86	9.17	92.1	
P4711-09	CF-613-49	52	1.16	8.76	9.92	9.41	94.2	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

132273

WorkList Name : %1-110424

WorkList ID : 185070

Department : Wet-Chemistry

Date : 11-04-2024 08:01:17

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P4682-01	BELL-SHOP-RAGS	Solid	Percent Solids	Cool 4 deg C	PSEG03	L13	11/01/2024	Chemtech -SO
P4683-01	GHA605R-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L13	11/01/2024	Chemtech -SO
P4683-02	GHA605R-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L13	11/01/2024	Chemtech -SO
P4684-01	MECHANIC-ST-SWEEPINGS	Solid	Percent Solids	Cool 4 deg C	PSEG03	L13	11/01/2024	Chemtech -SO
P4685-01	OK-01-11012024	Solid	Percent Solids	Cool 4 deg C	PSEG05	L13	11/01/2024	Chemtech -SO
P4685-02	OK-02-11012024-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L13	11/01/2024	Chemtech -SO
P4686-01	GCP52	Solid	Percent Solids	Cool 4 deg C	USEP04	A11	10/29/2024	Chemtech -SO
P4686-02	GCP52MS	Solid	Percent Solids	Cool 4 deg C	USEP04	A11	10/29/2024	Chemtech -SO
P4686-03	GCP52MSD	Solid	Percent Solids	Cool 4 deg C	USEP04	A11	10/29/2024	Chemtech -SO
P4686-04	GCP53	Solid	Percent Solids	Cool 4 deg C	USEP04	A11	10/30/2024	Chemtech -SO
P4686-05	GCP54	Solid	Percent Solids	Cool 4 deg C	USEP04	A11	10/30/2024	Chemtech -SO
P4692-01	TAPLPR-SED02-103124-00-T2	Solid	Percent Solids	Cool 4 deg C	WEST04	L21	10/31/2024	Chemtech -SO
P4692-02	TAPLPR-SED01-103124-00-T2	Solid	Percent Solids	Cool 4 deg C	WEST04	L21	10/31/2024	Chemtech -SO
P4693-01	BP-G5-WC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/02/2024	Chemtech -SO
P4693-02	BP-G5-WC-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/02/2024	Chemtech -SO
P4693-03	BP-G5-WC-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/02/2024	Chemtech -SO
P4693-05	BP-G4-WC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/02/2024	Chemtech -SO
P4693-06	BP-G4-WC-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/02/2024	Chemtech -SO
P4693-07	BP-G4-WC-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/02/2024	Chemtech -SO
P4694-01	Z-03A	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/03/2024	Chemtech -SO
P4694-02	Z-03A-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/03/2024	Chemtech -SO

Date/Time 11/04/24 15:35
 Raw Sample Received by: SP GOC
 Raw Sample Relinquished by: SP GOC
 Date/Time 11/04/24 17:30
 Raw Sample Received by: SP GOC
 Raw Sample Relinquished by: SP GOC

WORKLIST(Hardcopy Internal Chain)

WorkList Name : %1-110424

WorkList ID : 185070

Department : Wet-Chemistry

Date : 11-04-2024 08:01:17

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P4694-03	Z-03A-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/03/2024	Chemtech -SO
P4694-05	Z-04	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/03/2024	Chemtech -SO
P4694-06	Z-04-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/03/2024	Chemtech -SO
P4694-07	Z-04-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/03/2024	Chemtech -SO
P4695-01	Z-01	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/03/2024	Chemtech -SO
P4695-02	Z-01-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/01/2024	Chemtech -SO
P4695-03	Z-01-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/01/2024	Chemtech -SO
P4697-01	TP-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/01/2024	Chemtech -SO
P4697-02	TP-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L23	11/04/2024	Chemtech -SO
P4699-01	MIXED-DEMO	Solid	Percent Solids	Cool 4 deg C	PSEG03	L23	11/04/2024	Chemtech -SO
P4700-01	MH-8	Solid	Percent Solids	Cool 4 deg C	EART12	K21	11/04/2024	Chemtech -SO
P4700-02	MH-8-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/04/2024	Chemtech -SO
P4700-03	MH-8-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/04/2024	Chemtech -SO
P4701-01	BP-F3	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	11/04/2024	Chemtech -SO
P4701-02	BP-F3-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	K23	11/04/2024	Chemtech -SO
P4701-03	BP-F3-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	K23	11/04/2024	Chemtech -SO
P4701-05	BP-F4	Solid	Percent Solids	Cool 4 deg C	PSEG03	K23	11/04/2024	Chemtech -SO
P4701-06	BP-F4-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	K23	11/04/2024	Chemtech -SO
P4701-07	BP-F4-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	K23	11/04/2024	Chemtech -SO
P4703-01	S0-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	K23	11/04/2024	Chemtech -SO
P4703-02	0910	Solid	Percent Solids	Cool 4 deg C	PSEG03	L23	11/04/2024	Chemtech -SO

Date/Time 11/04/24 15:35

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: [Signature]

Date/Time 11/04/24

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

VB 133273

WorkList Name : %1-110424 WorkList ID : 185070 Department : Wet-Chemistry Date : 11-04-2024 08:01:17

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P4703-03	1008	Solid	Percent Solids	Cool 4 deg C	PSEG03	L23	11/04/2024	Chemtech -SO
P4705-01	1024	Solid	Percent Solids	Cool 4 deg C	PSEG03	L23	11/04/2024	Chemtech -SO
P4711-01	CF-613-COMP-16	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	11/04/2024	Chemtech -SO
P4711-02	CF-613-VOC-16	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	11/04/2024	Chemtech -SO
P4711-03	CF-613-46	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	11/04/2024	Chemtech -SO
P4711-04	CF-613-47	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	11/04/2024	Chemtech -SO
P4711-06	CF-613-COMP-17	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	11/04/2024	Chemtech -SO
P4711-07	CF-613-VOC-17	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	11/04/2024	Chemtech -SO
P4711-08	CF-613-48	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	11/04/2024	Chemtech -SO
P4711-09	CF-613-49	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	11/04/2024	Chemtech -SO

Date/Time 11/04/24 15:35
 Raw Sample Received by: SO
 Raw Sample Relinquished by: CP

Date/Time 11/04/24 17:30
 Raw Sample Received by: CP
 Raw Sample Relinquished by: SO

SOP ID: M3541-ASE Extraction-14

Clean Up SOP #: Acid Cleanup

Extraction Start Date : 11/05/2024

Matrix : Solid

Extraction Start Time : 08:35

Weigh By: RJ

Extraction By: RJ

Extraction End Date : 11/05/2024

Balance check: RJ

Filter By: RJ

Extraction End Time : 11:50

Balance ID: EX-SC-2

pH Meter ID: N/A

Concentration By: RS

pH Strip Lot#: N/A

Hood ID: 3,7

Supervisor By : rajesh

Extraction Method: ☐ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP23640
Surrogate	1.0ML	200 PPB	PP23858
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2539
Baked Na2SO4	N/A	EP2556
Hexane	N/A	E3819
Sand	N/A	E2865
H2SO4 1:1	N/A	EP2548
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40BTS721. P4682-01.P4703-01,02, P4705-01 Limited volume used as samples are Oil & Oily debries

KD Bath ID: N/A

Envap ID: NEVAP-02

KD Bath Temperature: N/A

Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
11/5/24	Rp (Ext Lab)	R. Pesti/PCB Lab
11:55	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-14

Concentration Date: 11/05/2024

Sample ID	Client Sample ID	Test	g/mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB164678BL	ABLK678	PCB	30.03	N/A	ritesh	RUPESH	10			U1-1
PB164678BS	ALCS678	PCB	30.01	N/A	ritesh	RUPESH	10			2
P4682-01	BELL-SHOP-RAGS	PCB	5.03	N/A	ritesh	RUPESH	10	D	Oily Debris	3
P4684-01	MECHANIC-ST-SWEEPING S	PCB	30.09	N/A	ritesh	RUPESH	10	B		4
P4685-01	OK-01-11012024	PCB	30.05	N/A	ritesh	RUPESH	10	D		5
P4693-01	BP-G5-WC	PCB	30.07	N/A	ritesh	RUPESH	10	D		6
P4693-05	BP-G4-WC	PCB	30.02	N/A	ritesh	RUPESH	10	D		U5-1
P4694-01	Z-03A	PCB	30.08	N/A	ritesh	RUPESH	10	D		2
P4694-05	Z-04	PCB	30.10	N/A	ritesh	RUPESH	10	D		3
P4695-01	Z-01	PCB	30.03	N/A	ritesh	RUPESH	10	E		4
P4697-01	TP-1	PCB	30.09	N/A	ritesh	RUPESH	10	D		5
P4699-01	MIXED-DEMO	PCB	30.02	N/A	ritesh	RUPESH	10			6
P4700-01	MH-8	PCB	30.04	N/A	ritesh	RUPESH	10	D		U6-1
P4701-01	BP-F3	PCB	30.08	N/A	ritesh	RUPESH	10	D		2
P4701-01MS	BP-F3MS	PCB	30.02	N/A	ritesh	RUPESH	10	D		3
P4701-01MS D	BP-F3MSD	PCB	30.04	N/A	ritesh	RUPESH	10	D		4
P4701-05	BP-F4	PCB	30.09	N/A	ritesh	RUPESH	10	D		5
P4703-01	S0-1	PCB	1.05	N/A	ritesh	RUPESH	10	B	Oil	
P4703-02	0910	PCB	5.09	N/A	ritesh	RUPESH	10	B	Oily Debris	6
P4703-03	1008	PCB	30.05	N/A	ritesh	RUPESH	10	B	S.Partical	U7-1
P4705-01	1024	PCB	5.04	N/A	ritesh	RUPESH	10	D	Oily Debris	2
P4711-01	CF-613-COMP-16	PCB	30.04	N/A	ritesh	RUPESH	10	D		3
P4711-06	CF-613-COMP-17	PCB	30.09	N/A	ritesh	RUPESH	10	D		4

* Extracts relinquished on the same date as received.

WORKLIST(Hardcopy Internal Chain)

WorkList Name : P4684

WorkList ID : 185129

Department : Extraction

Date : 11-05-2024 08:28:04

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P4682-01	BELL-SHOP-RAGS	Solid	PCB	Cool 4 deg C	PSEG03	L13	11/01/2024	8082A
P4684-01	MECHANIC-ST-SWEEPINGS	Solid	PCB	Cool 4 deg C	PSEG03	L13	11/01/2024	8082A
P4685-01	OK-01-11012024	Solid	PCB	Cool 4 deg C	PSEG05	L13	11/01/2024	8082A
P4693-01	BP-G5-WC	Solid	PCB	Cool 4 deg C	PSEG03	L21	11/02/2024	8082A
P4693-05	BP-G4-WC	Solid	PCB	Cool 4 deg C	PSEG03	L21	11/02/2024	8082A
P4694-01	Z-03A	Solid	PCB	Cool 4 deg C	PSEG03	L21	11/03/2024	8082A
P4694-05	Z-04	Solid	PCB	Cool 4 deg C	PSEG03	L21	11/03/2024	8082A
P4695-01	Z-01	Solid	PCB	Cool 4 deg C	PSEG03	L21	11/01/2024	8082A
P4697-01	TP-1	Solid	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4699-01	MIXED-DEMO	Solid	PCB	Cool 4 deg C	EART12	K21	11/04/2024	8082A
P4700-01	MH-8	Solid	PCB	Cool 4 deg C	PSEG03	L21	11/04/2024	8082A
P4701-01	BP-F3	Solid	PCB	Cool 4 deg C	PSEG03	K23	11/04/2024	8082A
P4701-05	BP-F4	Solid	PCB	Cool 4 deg C	PSEG03	K23	11/04/2024	8082A
P4703-01	S0-1	Solid	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4703-02	0910	Solid	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4703-03	1008	Solid	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4705-01	1024	Solid	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4711-01	CF-613-COMP-16	Solid	PCB	Cool 4 deg C	PSEG03	K51	11/04/2024	8082A
P4711-06	CF-613-COMP-17	Solid	PCB	Cool 4 deg C	PSEG03	K51	11/04/2024	8082A

Date/Time

Raw Sample Received by:

Raw Sample Relinquished by:

Date/Time 11/5/24 8:05
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

Prep Standard - Chemical Standard Summary

Order ID : P4699

Test : PCB

Prepbatch ID : PB164678,

Sequence ID/Qc Batch ID: PO110524,

Standard ID :

EP2539,EP2548,EP2556,PP23640,PP23733,PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775,PP23776,PP23777,PP23778,PP23779,PP23780,PP23781,PP23782,PP23783,PP23784,PP23785,PP23786,PP23787,PP23788,PP23789,PP23790,PP23858

Chemical ID :

E2865,E3551,E3788,E3792,E3793,E3804,E3805,E3815,E3819,M5178,P10483,P10500,P11507,P11512,P11581,P11587,P11590,P11597,P12698,P12929,P12934,P12946,P12947,P12957,P13033,P13350,P13351,P13372,W3112,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2539	09/17/2024	03/11/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 09/17/2024

FROM 4000.00000ml of E3792 + 4000.00000ml of E3793 = Final Quantity: 8000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2548	10/16/2024	04/16/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 10/16/2024

FROM 1000.00000ml of W3112 + 4000.00000ml of M5178 = Final Quantity: 2000.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2556	11/03/2024	01/03/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 11/03/2024
<u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP23640	09/09/2024	01/12/2025	Ankita Jodhani	None	None	Yogesh Patel 09/10/2024
<u>FROM</u>	0.50000ml of P12946 + 99.50000ml of E3788 = Final Quantity: 100.000 ml							

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP23733	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13350 + 9.00000ml of E3805 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP23735	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10483 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP23736	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23735 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP23737	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP23738	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23735 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP23739	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23737 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP23740	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11581 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP23741	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23740 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP23742	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP23743	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23740 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP23744	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23742 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP23745	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11587 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP23747	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23745 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP23748	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP23749	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23745 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP23750	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23748 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP23751	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12929 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP23752	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23751 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP23753	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP23754	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23751 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP23755	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23753 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP23756	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12934 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP23757	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23756 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP23758	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP23759	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23756 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP23760	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23758 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP23761	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11590 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP23762	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23761 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP23763	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP23764	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23761 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP23765	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23763 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP23766	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10500 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP23767	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23766 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP23768	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP23769	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23766 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP23770	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23768 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP23771	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11597 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP23772	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23771 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP23773	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP23774	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23771 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP23775	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23773 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP23776	10/03/2024	04/01/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12947 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP23777	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 98.50000ml of E3805 + 0.50000ml of PP23733 + 1.00000ml of PP23776 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP23778	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23777 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP23779	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13372 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3790	AR1221 500 PPB ICV(AGILENT)	PP23780	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23779 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP23781	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12698 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP23782	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P11507 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP23783	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23781 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP23784	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23782 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP23785	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11512 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP23786	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23785 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP23787	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12957 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP23788	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23787 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP23789	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P13033 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP23790	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23789 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP23858	10/14/2024	04/04/2025	Abdul Mirza	None	None	Ankita Jodhani
10/14/2024								
<u>FROM</u> 1.00000ml of P13351 + 999.00000ml of E3815 = Final Quantity: 1000.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	01/03/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	23H1462005	04/23/2025	08/13/2024 / Rajesh	08/13/2024 / Rajesh	E3788

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/11/2025	09/12/2024 / Rajesh	09/11/2024 / Rajesh	E3792

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	03/11/2025	09/12/2024 / Rajesh	09/11/2024 / Rajesh	E3793

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/30/2025	09/30/2024 / Rajesh	09/25/2024 / Rajesh	E3805

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	04/04/2025	10/04/2024 / Rajesh	10/04/2024 / Rajesh	E3815

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	04/15/2025	10/15/2024 / Rajesh	10/09/2024 / Rajesh	E3819

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	03/29/2026	05/25/2022 / william	04/05/2022 / william	M5178

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0163157	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Abdul	P10483

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0167722	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Ankita	P10500

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11507

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006626997	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11512

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0175456	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11581

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0173309	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11587

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0175403	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11590

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0181782	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11597

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	04/03/2025	10/03/2024 / Ankita	08/07/2023 / Ankita	P12698

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12929

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12934

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	01/12/2025	07/12/2024 / Abdul	12/20/2023 / Yogesh	P12946

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12947

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Aroclor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	90165 / Aroclor 1262	112322	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P13033

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/03/2025	10/03/2024 / Ankita	04/22/2024 / Abdul	P13350

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/14/2025	10/14/2024 / Abdul	04/22/2024 / Abdul	P13351

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	04/03/2025	10/03/2024 / Ankita	05/02/2024 / Ankita	P13372

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1


Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865

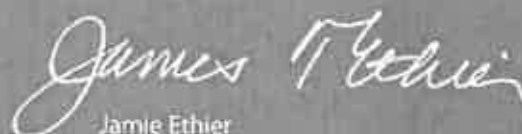
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03
Batch No.: 23H1462005
Manufactured Date: 2023-07-26
Expiration Date: 2026-07-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 8/13/24

E 3788

Ken Koehnlein
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 09/11/24

E 3192

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
CMOS

avantor™



Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

>>> Continued on page 2 >>>

Recd. by RP on 9/11/24

E3793

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use
Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC

Michelle Bales
Sr. Manager, Quality Assurance

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 9/25/24

E 3805

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 24H1462005
Manufactured Date: 2024-05-24
Expiration Date: 2027-05-24
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3815

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 10/09/24

E 3819

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700
Page 1 of 1

Hydrochloric Acid, 36.5–38.0%
 BAKER INSTRA-ANALYZED® Reagent
 For Trace Metal Analysis



Material No.: 9530-33
 Batch No.: 0000281827
 Manufactured Date: 2021/03/30
 Retest Date: 2026/03/29
 Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
 Avantor Performance Materials, LLC
 100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 Lot No.: A0163157
Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2026 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1016 CAS # 12674-11-2 (Lot 04) Purity ----%	1,007.0 µg/mL	+/- 5.8683 µg/mL Gravimetric +/- 31.9082 µg/mL Unstressed +/- 41.6868 µg/mL Stressed
2	Aroclor 1260 CAS # 11096-82-5 (Lot 07) Purity ----%	1,008.0 µg/mL	+/- 5.8741 µg/mL Gravimetric +/- 31.9399 µg/mL Unstressed +/- 41.7282 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 10476

P 10480

AR
02/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

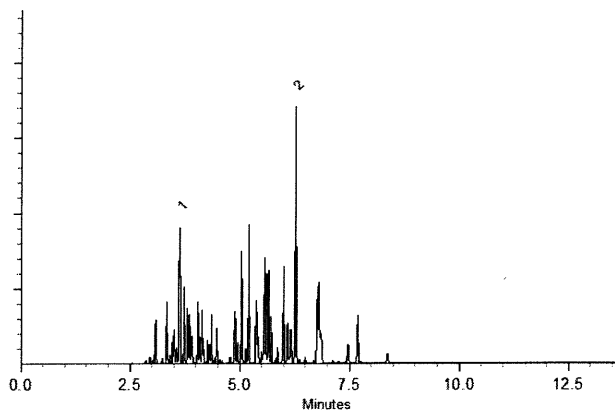

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 03-Aug-2020

Balance: B442140311

Justine Albertson - Operations Tech-ARM QC

Date Passed: 05-Aug-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32409 Lot No.: A0167722
Description : Aroclor® 1262 Standard
Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : April 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1262	1,004.0 µg/mL	+/- 5.9635 µg/mL Gravimetric
	CAS # 37324-23-5 (Lot 10849100)		+/- 31.8340 µg/mL Unstressed
	Purity ----%		+/- 41.5787 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P10496
↓
P10500

AJ
09/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

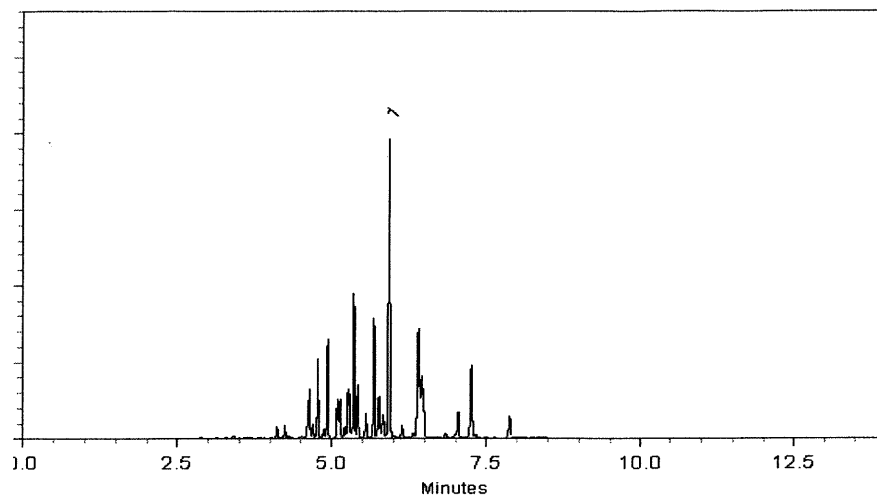

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 03-Jan-2021


Balance: B707717271

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 05-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
Aroclor 1242	100.4	± 0.5 µg/mL		053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11503
↓
P11507A7
02/21/22

Page: 1 of 2

CSD-QA-015.1

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2


www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1248 Standard

Lot Number: 0006626997

Product Number: PP-342-1

Lot Issue Date: 17-Aug-2021

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 30-Sep-2025

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1248	100.3	± 0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.


P11508

↓
P11512

AJ

2/21/22

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 Lot No.: A0175456
Description : Aroclor® 1221 Standard
Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1221	1,002.0 µg/mL	+/- 5.9516 µg/mL Gravimetric
	CAS # 11104-28-2 (Lot 10210500)		+/- 31.7706 µg/mL Unstressed
	Purity ----%		+/- 41.4958 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11578
↓
P 11582 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

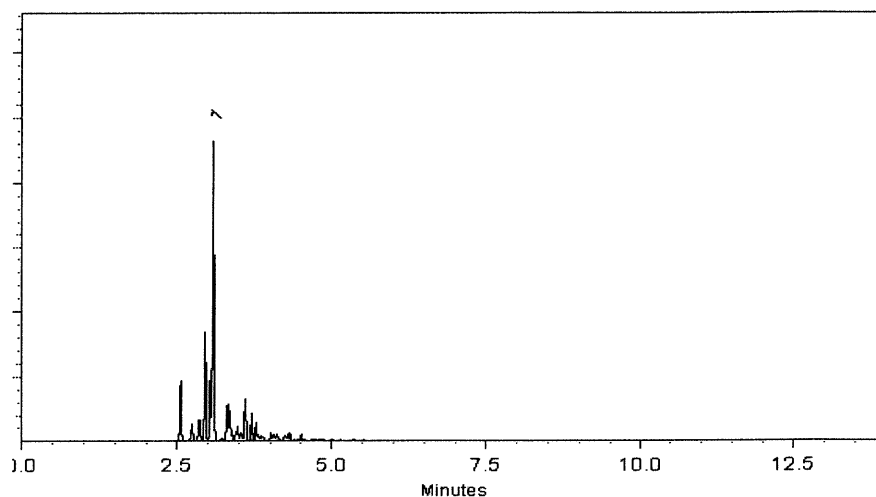

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 16-Aug-2021 Balance: B442140311

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 18-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11578
↓
P11582 / (S)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008 Lot No.: A0173309
Description : Aroclor® 1232 Standard
Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : September 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1232	1,001.0 µg/mL	+/- 5.9456 µg/mL Gravimetric
	CAS # 11141-16-5 (Lot 15665-01)		+/- 31.7389 µg/mL Unstressed
	Purity ----%		+/- 41.4544 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11583
↓
P11587 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

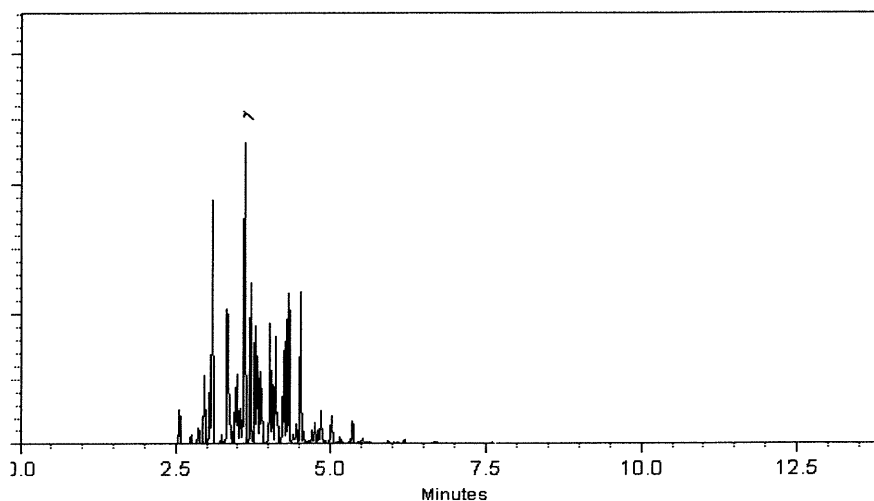

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 13-Jun-2021 **Balance:** B442140311

Alexis Shelow
Alexis Shelow - Operations Tech I

Date Passed: 16-Jun-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11583
↓
P11587 (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 Lot No.: A0175403
Description : Aroclor® 1254 Standard
Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1254 CAS # 11097-69-1 (Lot 124-191-B) Purity ----%	1,000.7 µg/mL	+/- 5.9437 µg/mL Gravimetric +/- 31.7284 µg/mL Unstressed +/- 41.4406 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11588
↓
P11592 / (S)

AR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

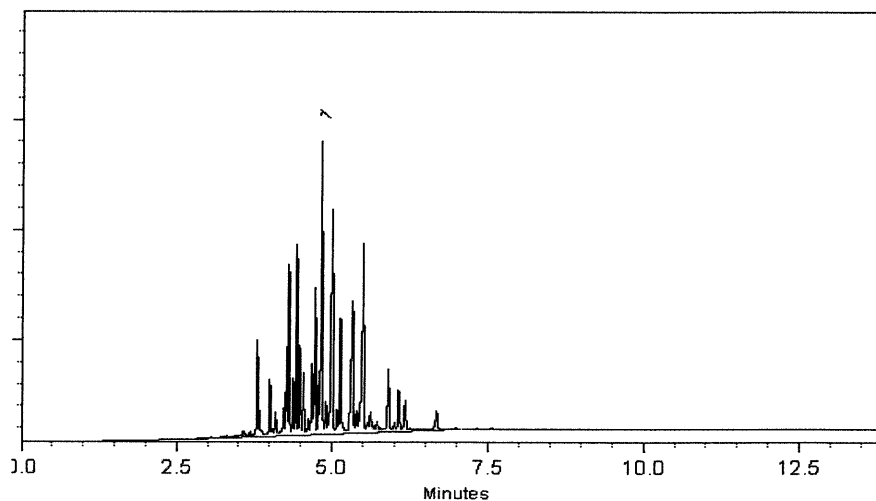

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cathleen Soltis

Cathleen Soltis - Mix Technician

Date Mixed: 15-Aug-2021

Balance: 1128360905

Alexis Shelow

Alexis Shelow - Operations Tech I

Date Passed: 17-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11588
↓
P11592 / (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410 **Lot No.:** A0181782

Description : Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : May 31, 2028 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1268	1,001.4 µg/mL	+/- 5.9480 µg/mL Gravimetric
	CAS # 11100-14-4 (Lot 10947000)		+/- 31.7516 µg/mL Unstressed
	Purity ----%		+/- 41.4710 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11593
↓
P 11597
⑤

UAR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

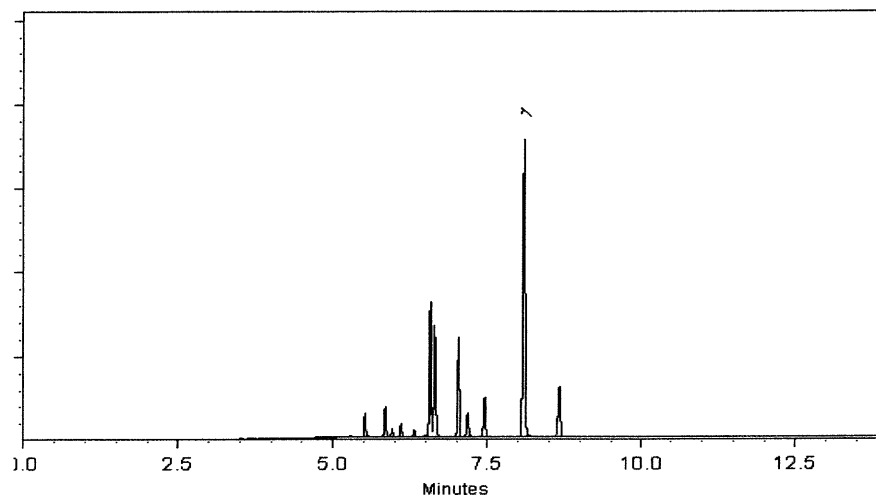

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope Riglin - Operations Tech I

Date Mixed: 14-Feb-2022

Balance: 1128360905

Clara Windle - Operations Technician I

Date Passed: 17-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 11593 / (5)
↓
P 11597
[Signature]
04/30/2022



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration ($\mu\text{g/mL}$): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton

Weight(s) shown below were combined and diluted to (mL): **100.0**

5E-05 Balance Uncertainty

0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier

Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness

Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min


Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min

Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)

Rate = 8°C/min, Total run time = 35 min

Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1

Standard injection = 1.5 μL , Range=3

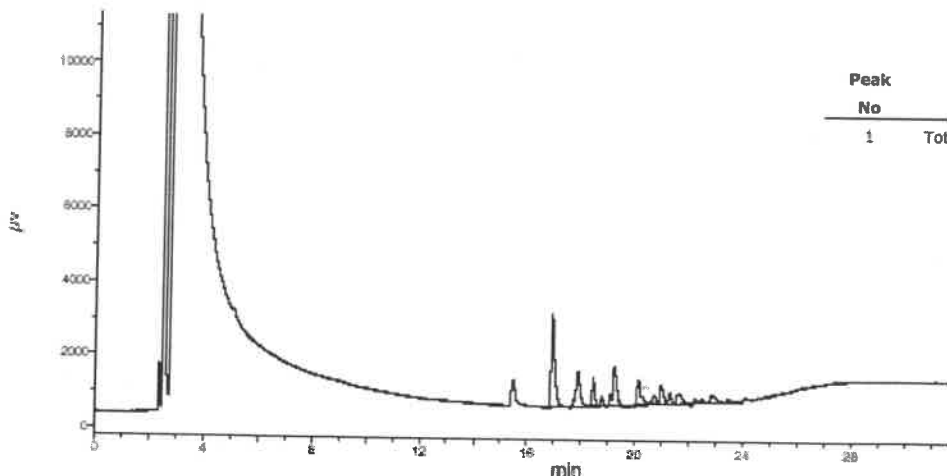



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32009 **Lot No.:** A0203672

Description: Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

p12928

→

p12932

AJ

12/27/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

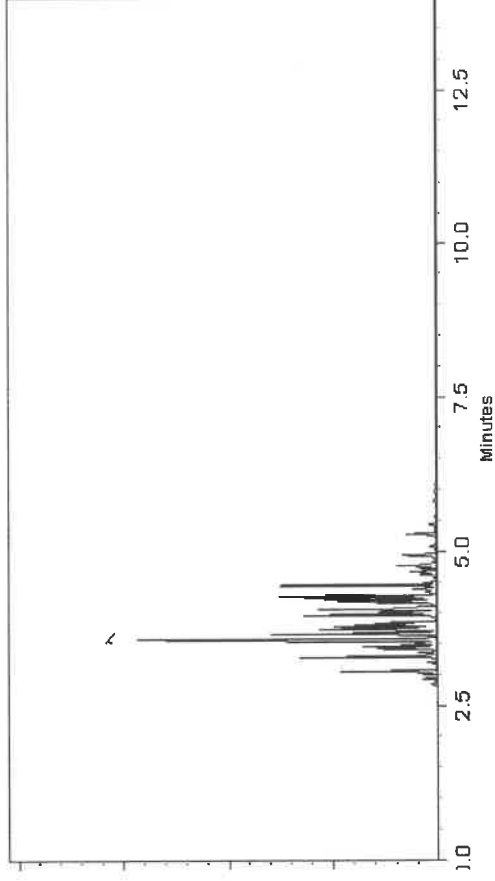

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boothamer - Operations Technician I

Date Mixed: 26-Oct-2023 Balance Serial # B442140311

Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010 **Lot No.:** A0202803

Description: Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P1219697
P1219697
AF
12/10/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 µg/mL	+/- 55.5850

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

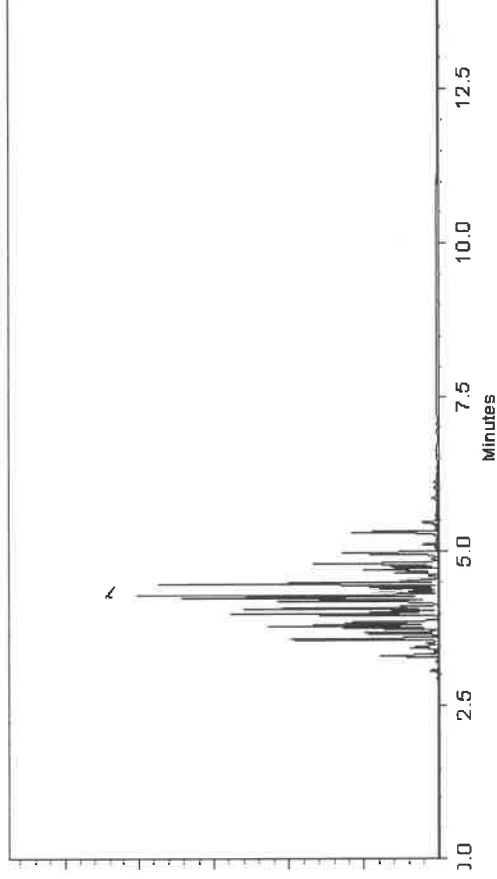

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 03-Oct-2023

Balance Serial # 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Solvent(s):
Hexane

Lot#
273615

Lot Number:
022023

Formulated By:
Benson Chan

DATE
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Reviewed By:
Pedro L. Rentas

DATE
022023

Expiration Date:
Ambient (20 °C)

Expanded
Uncertainty

SDS Information
(Solvent Safety Info. On Attached pg.)

Recommended Storage:
Nominal Concentration (µg/mL):
200.0

Purity

OSHA PEL (TWA)
LD50

NIST Test ID#:
6UTB

Balance Uncertainty
0.010

Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL):

5E-05


0.010

PR2946 718
↓
12/20/23
P12955

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

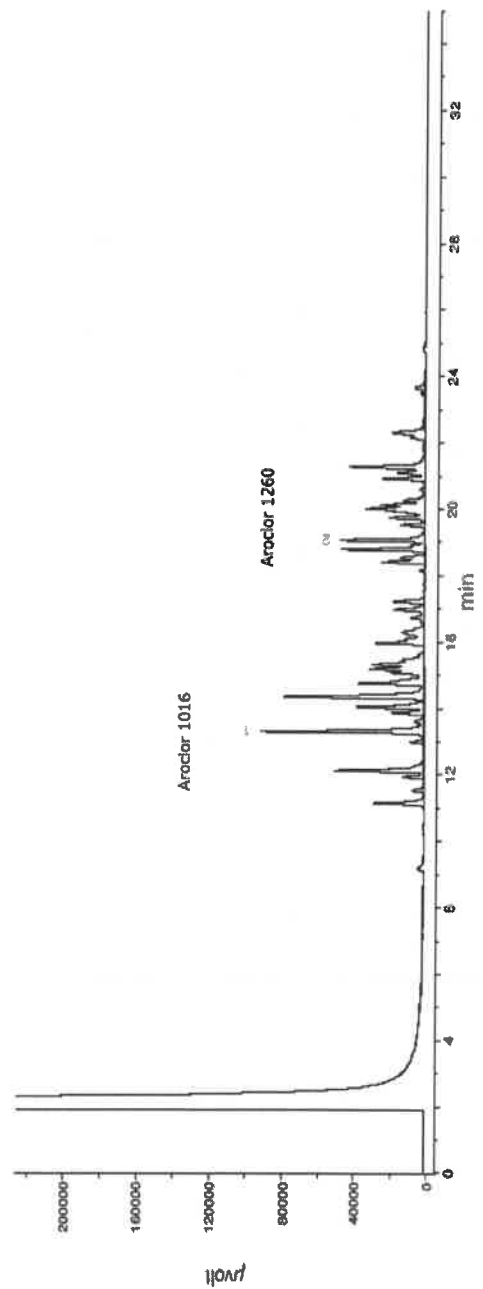



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty


Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

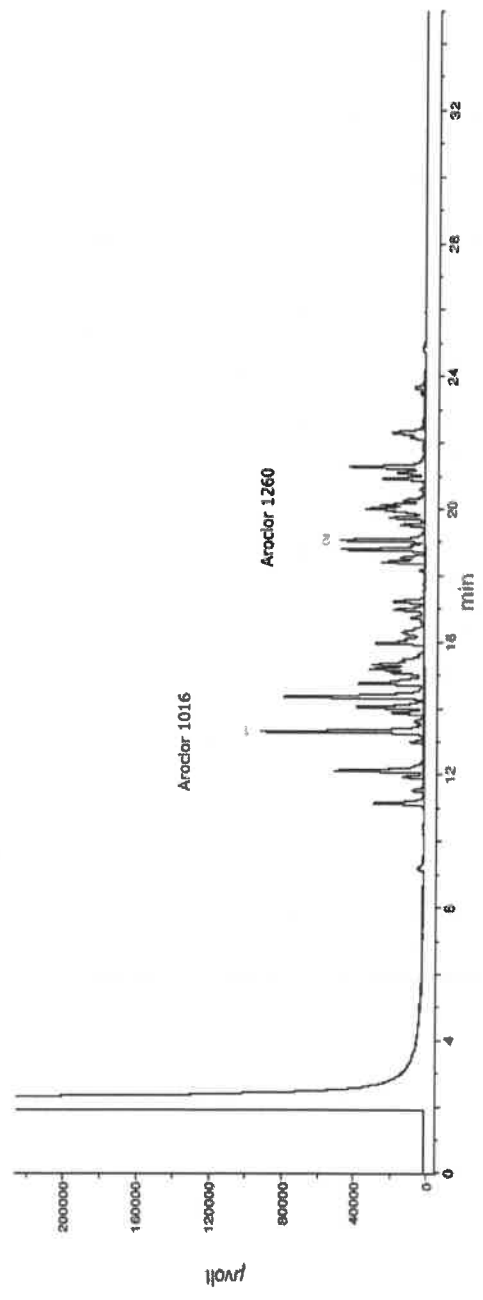



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Solvent(s): Iso-octane

Lot# 82227

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

Balance Uncertainty 5E-05

Flask Uncertainty 0.003

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE


P12956 / Y.P.
12/18/23
P12957

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Initial Uncertainty	Pipette (mL)	Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
											(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA) LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	1003.3	100.1	1.8	11097-69-1	0.5mg/m3 (skin)	or-rat 1295mg/kg		

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 280 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

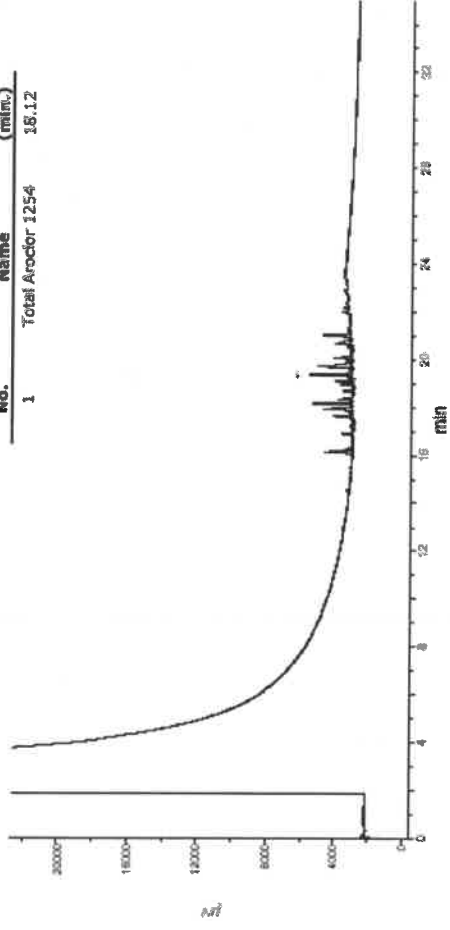



CERTIFIED WEIGHT REPORT

Part Number: **90165**

Lot Number: 11232

Description:

Solvent(s): **Loth**

Hexane 273615

Expiration Date: 11233

Recommended Storage: Ambient (20 °C)

Nominal Concentration ($\mu\text{g/mL}$):

NIST Test ID#:

Weight(s) shown below were combined and diluted to (mL):

5E-05	Balance Uncertainty
0.005	Flask Uncertainty

Formulated By:		112322
	Prashant Chauhan	DATE
Reviewed By:		112322
	Pedro L. Romias	DATE

By:  Pedro L. Rentas

112322

SDS information

**Expanded
Uncertainty
SDS Information
(Solvent Safety Info. On Attached pg.)**


(+/-) (µg/mL)	CAS#	OSHA PEL (TWA)
---------------	------	----------------

1050

Compound	RM#	Lot Number	Nominal	Purity	Uncertainty	Target	Actual	Actual	Uncertainty	(Solvent Safety Info. On Attached pg.)		
			Conc (ug/mL)	(%)	Purity	Weight (g)	Weight (g)	Conc(ug/mL)	(+/-) (ug/mL)	CAS#	OSHA PEL (TWA)	LDSO
1. Atoclor 1262	444	W-130-05	1000	100	0.2	0.05003	0.05016	1002.7	4.5	37324-23-5	N/A	ori-rel 11300mg/kg

Method GC/MSD-7.M: Column/(30 m X 0.25 mm ID X 0.25 μ m film thickness) Temp 1 = 150°C (0 min.), Temp 2 = 290°C (12.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C.

TIC: [B8B1]P70444-2.D

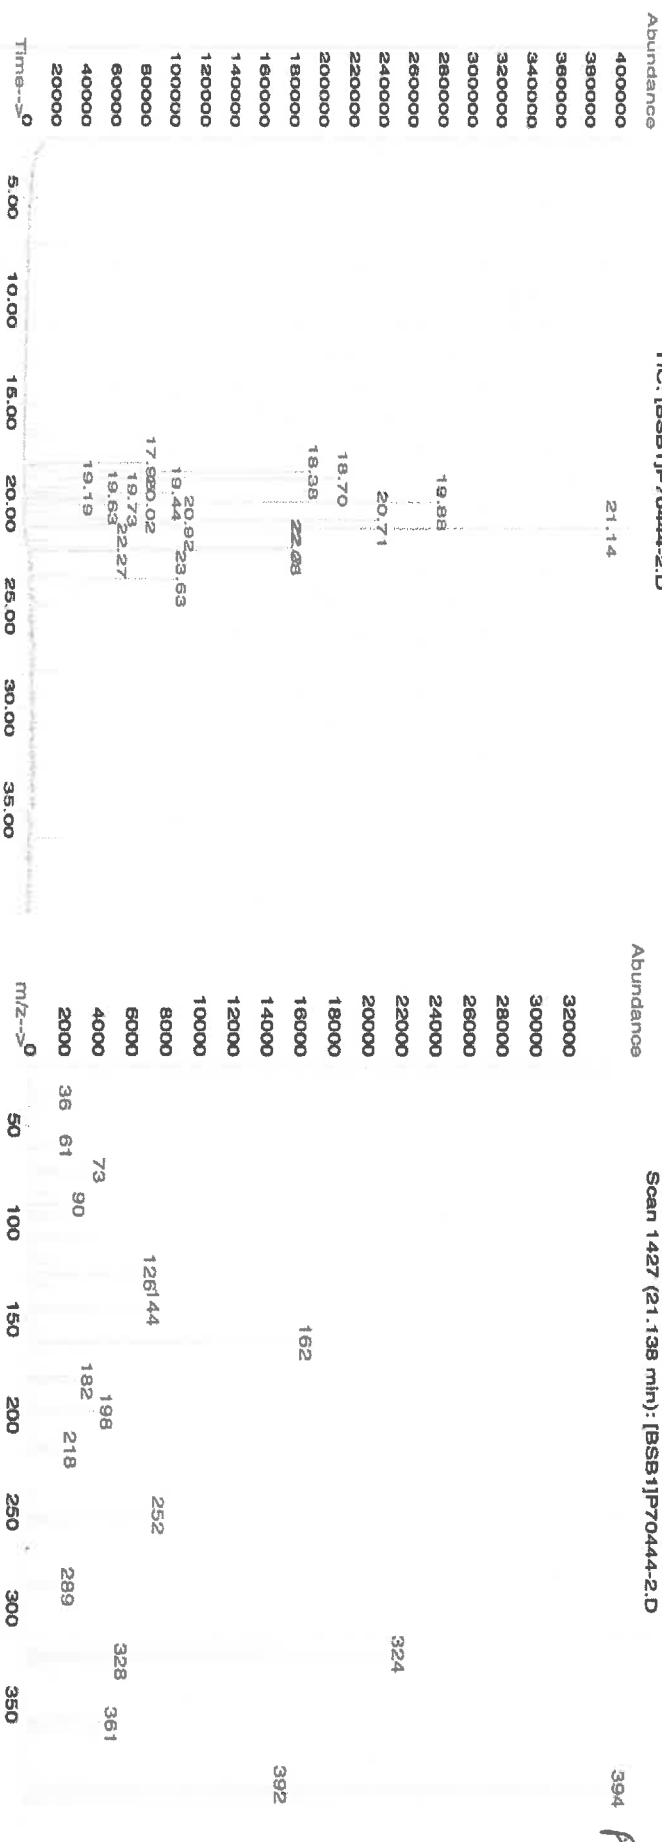

- The certified value/the concentration calculated from gravimetric and volumetric measurements unless otherwise stated
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.

- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.

* Uncertainty Reference: Laylor, B.N. and Kuyul, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 20, "P90165 L112322 [1000µg/mL in hexane]"

Run Length: 35.00 min, 21000 points at 10 points/second.
Created: Thu, Dec 8, 2022 at 2:31:02 AM.
Sampled: Sequence "120722-GC3M1", Method "GC3-M1".
Analyzed using Method "GC3-M1".

Comments

GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3

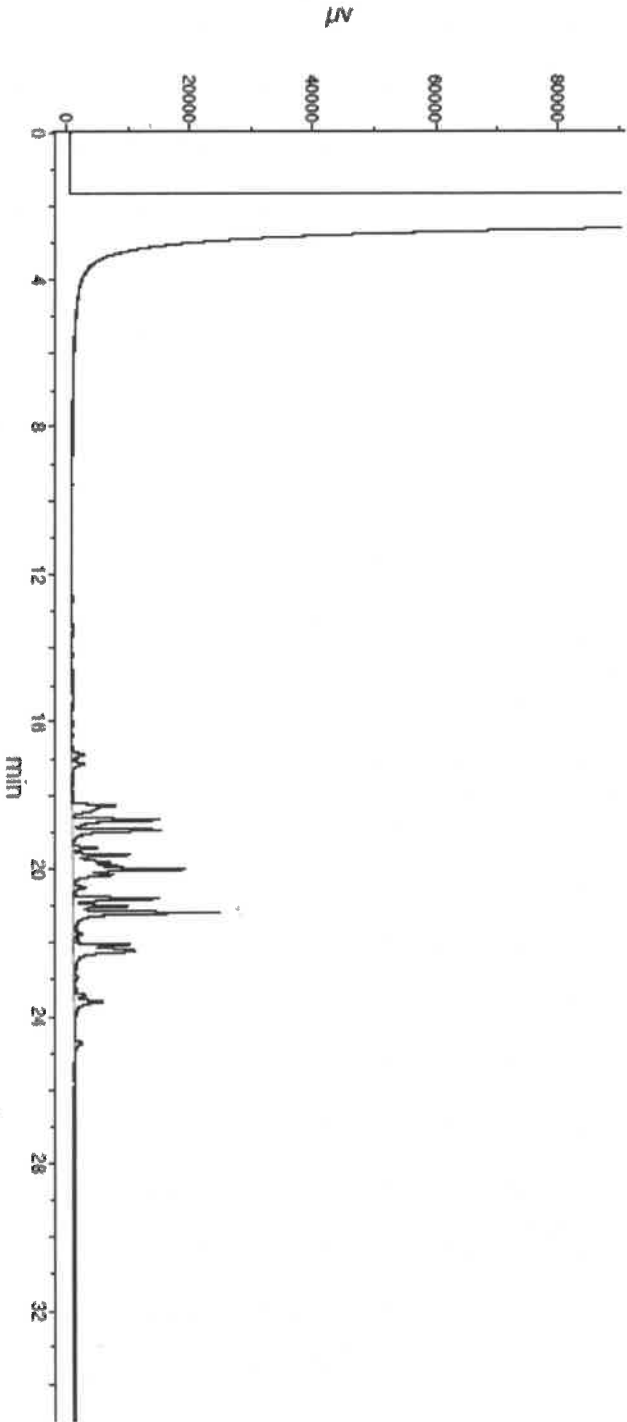



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

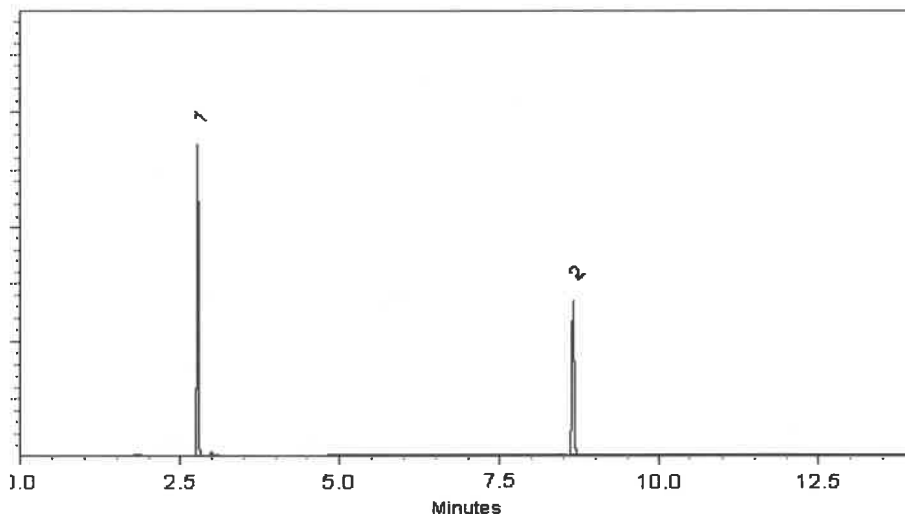


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
BAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

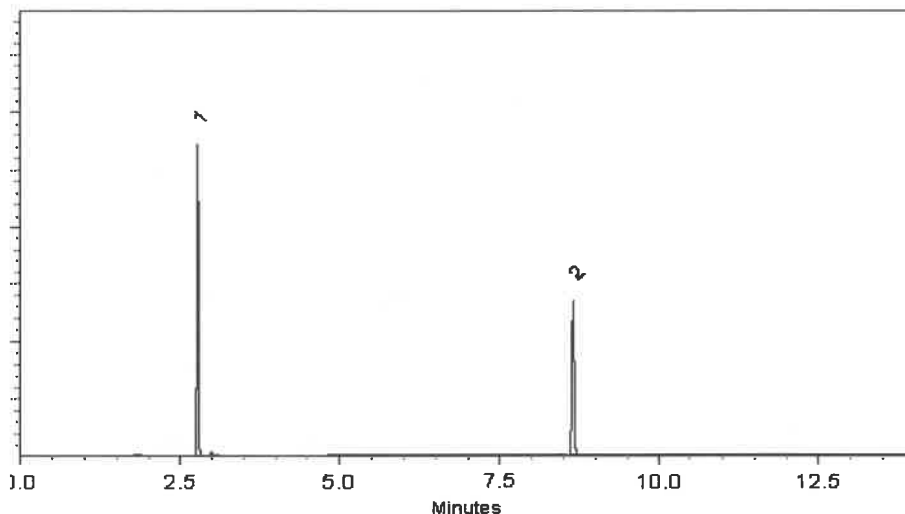


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10

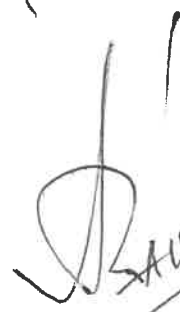
SAUF
04/25/2025



ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name: Aroclor 1221 Standard
Product Number: PP-292-1
Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006783205
Lot Issue Date: 20-Feb-2024
Expiration Date: 31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ±	0.5 µg/mL	011104-28-2	NT01017

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342
AJ
05106124
P13343

Page: 1 of 2

CSD-QA-015.2

ISO 17025

Cert No. AT-1937


250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



SHIPPING DOCUMENTS



CHAIN OF CUSTODY RECORD

284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 Fax (908) 789-8922
www.chemtech.net

Chemtech Project Number	P4699
COC Number	

CLIENT INFORMATION			PROJECT INFORMATION				BILLING INFORMATION												
Report to be sent to:			PROJECT NAME: 120 122 Liberty Ave BK				BILL TO: EarthEfficient PO#												
COMPANY: EarthEfficient			PROJECT #:		LOCATION: 120 122 Liberty Ave		ADDRESS: 30 W Main St												
ADDRESS: 30 W Main St			PROJECT MANAGER: Ryan Casserly		Brooklyn, NY		CITY: Riverhead STATE: NY ZIP: 11901												
CITY: Riverhead STATE: NY ZIP: 11901			E-MAIL: envteam@earthefficient.com				ATTENTION: Pia Tague - pia@earthefficient.com												
ATTENTION: Env Team - envteam@earthefficient.com			PHONE: (631) 209-4245		FAX:		PHONE: (631) 209-4245												
PHONE: (631) 209-4245 FAX:			DATA DELIVERABLE INFORMATION				ANALYSIS												
FAX (RUSH) ⁵ DAYS*			☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data) ☐ Level 2 (Results + QC) ☒ NJ Reduced ☐ US EPA CLP ☐ Level 3 (Results + QC + Raw Data) ☐ NYS ASP A ☐ NYS ASP B ☐ EDD FORMAT ☐ Other				1 total lead (6010) 2 PCBs (8082) 3 4 5 6 7 8 9												
HARDCOPY (DATA PACKAGE): ⁵ DAYS*							PRESERVATIVES												
EDD: ⁵ DAYS*							COMMENTS												
*TO BE APPROVED BY CHEMTECH							<-- Specify Preservatives												
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS							A-HCl D-NaOH B-HNO3 E-ICE C-H2SO4 F-OTHER												
CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles												
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9			
1.	Mixed Demo	S	✓		11/4/21	10:00AM	1	✓	✓										
2.																			
3.																			
4.																			
5.																			
6.																			
7.																			
8.																			
9.																			
10.																			
SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE PROSESSION INCLUDING COURIER DELIVERY																			
RELINQUISHED BY SAMPLER		DATE/TIME	RECEIVED BY		Conditions of bottles or collars at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP 4.2°C														
1. [Signature]		11/4/21	1. [Signature]		Comments:														
RELINQUISHED BY		DATE/TIME	RECEIVED BY																
2.			2.																
RELINQUISHED BY		DATE/TIME	RECEIVED FOR LAB BY		CLIENT: ☐ Hand Delivered ☐ Other: _____ CHEMTECH: ☐ Picked Up														
3.			3.		Shipment Complete ☐ YES ☐ NO														

10/2021

WHITE - CHEMTECH COPY FOR RETURN TO CLIENT

YELLOW - CHEMTECH COPY

PINK - SAMPLER COPY



284 Sheffield Street, Mountainside NJ 07092 (908)-789-8900 Fax : 908 789 8922

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488