
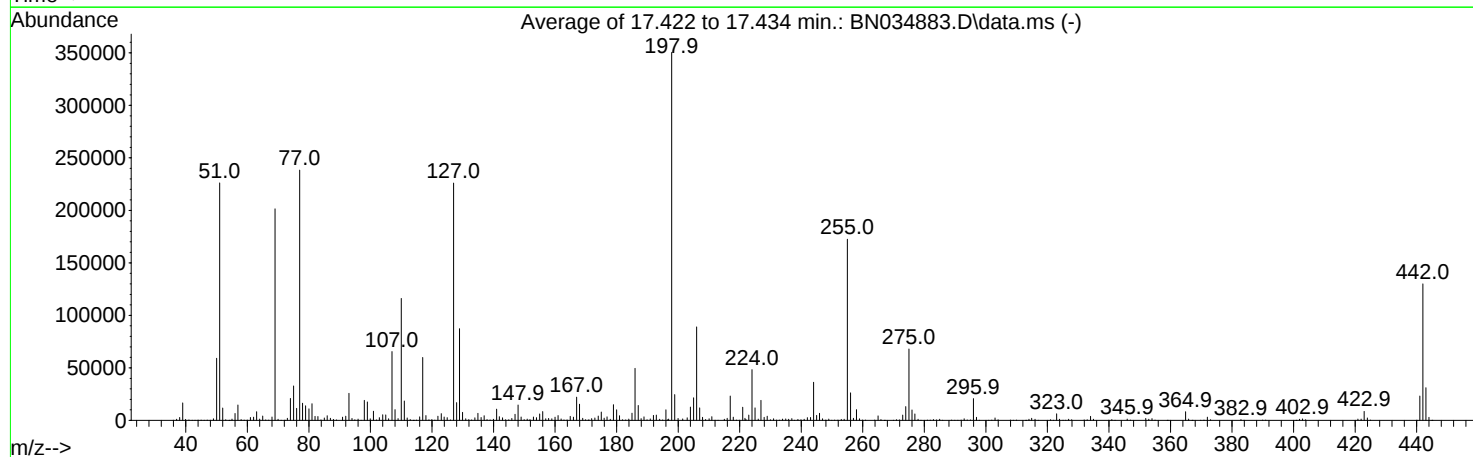


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110724\
Data File : BN034883.D
Acq On : 07 Nov 2024 08:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 15:02:36 2024

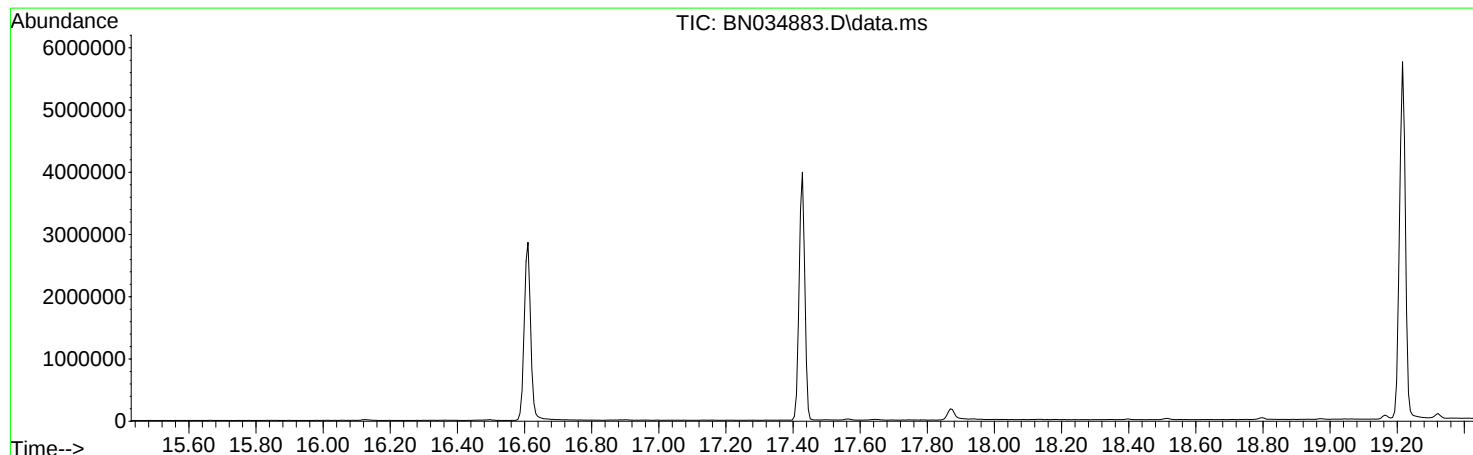




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.6	226187	PASS
68	69	0.00	2	1.6	3175	PASS
69	198	0.00	100	57.5	201387	PASS
70	69	0.00	2	0.6	1113	PASS
127	198	10	80	64.5	225920	PASS
197	198	0.00	2	0.3	1194	PASS
198	198	100	100	100.0	350336	PASS
199	198	5	9	7.0	24557	PASS
275	198	10	60	19.4	67965	PASS
365	198	1	100	2.3	8198	PASS
441	198	0.01	100	6.6	23149	PASS
442	442	50	100	100.0	130005	PASS
443	442	15	24	24.0	31165	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110724\
Data File : BN034883.D
Acq On : 07 Nov 2024 08:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 08 05:30:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:30:33 2024
Response via : Initial Calibration

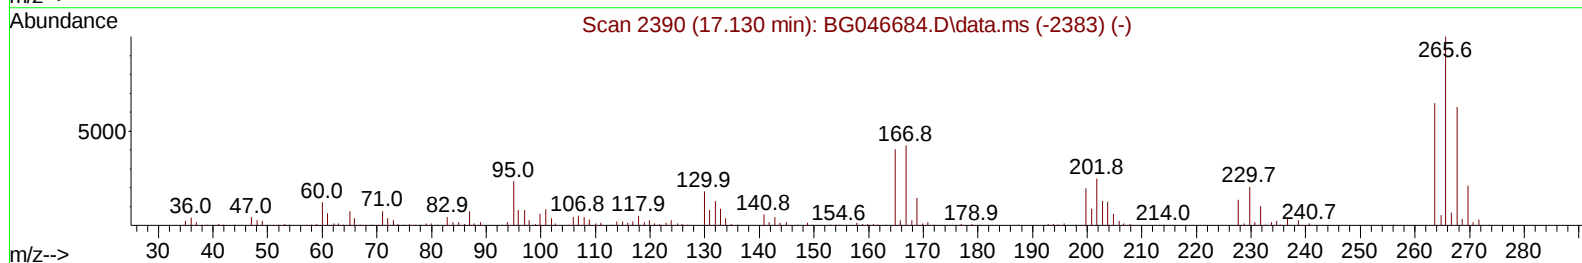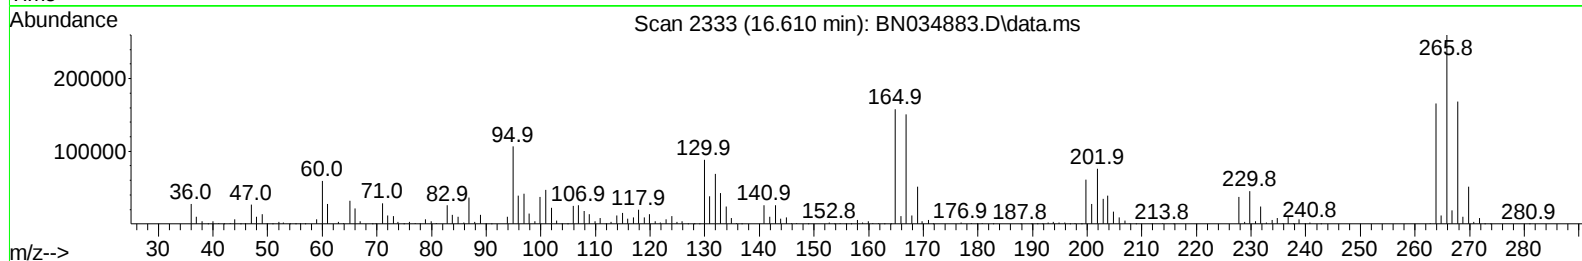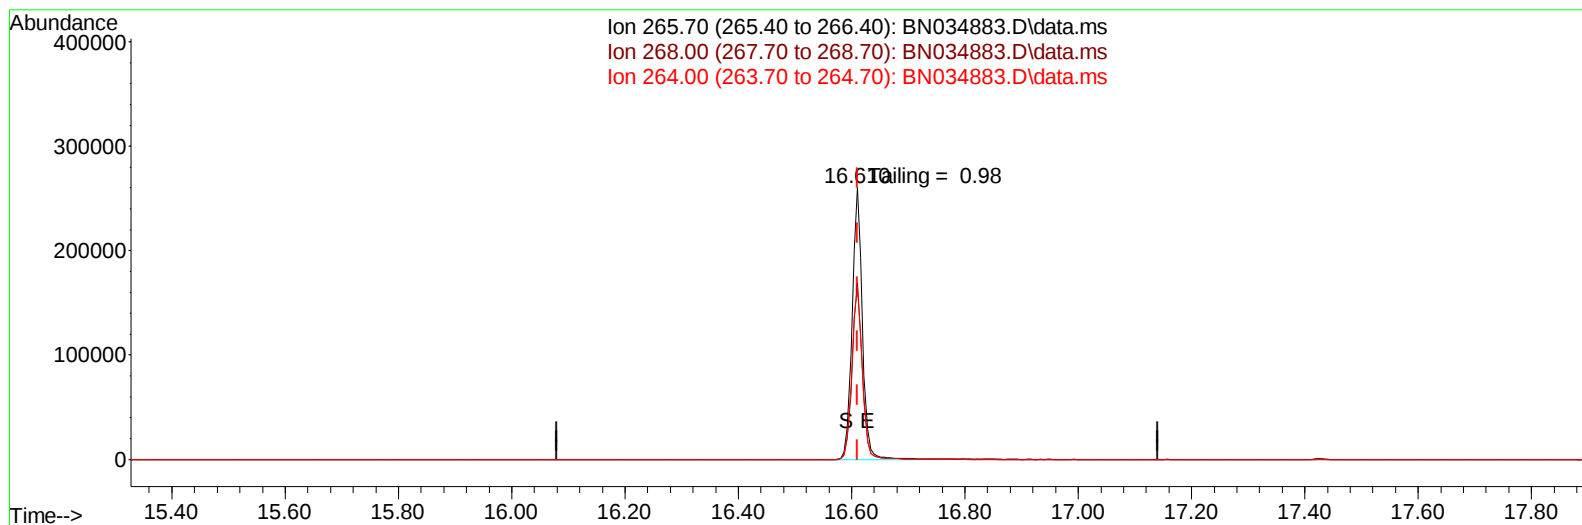

TIC: BN034883.D\data.ms

(70) Pentachlorophenol (C)

16.610min (0.000) 18769.66 ng




response 330393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.93
264.00	61.60	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110724\
Data File : BN034883.D
Acq On : 07 Nov 2024 08:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 08 05:30:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:30:33 2024
Response via : Initial Calibration

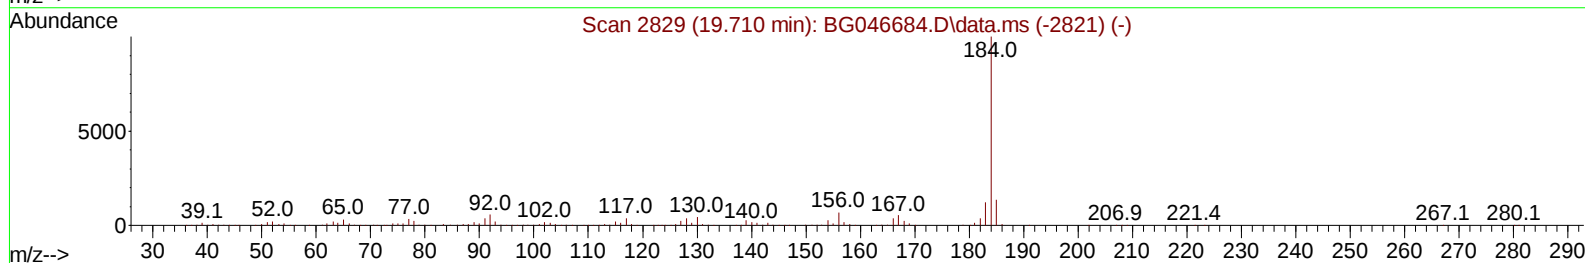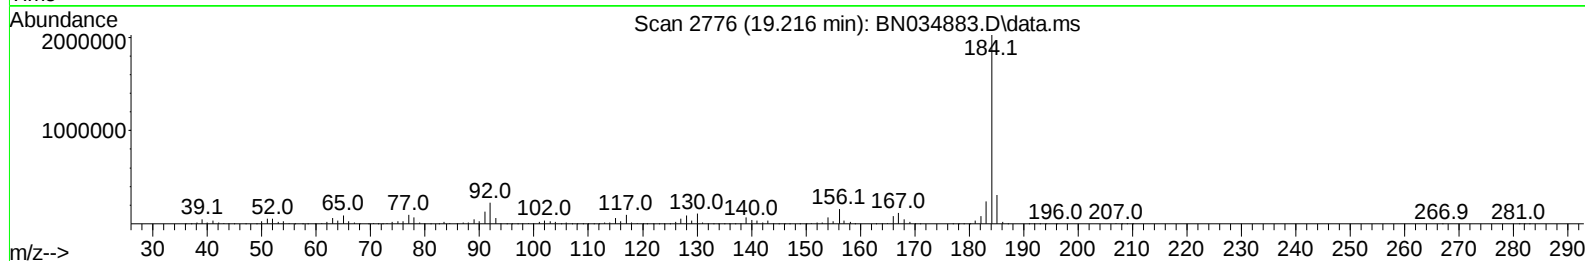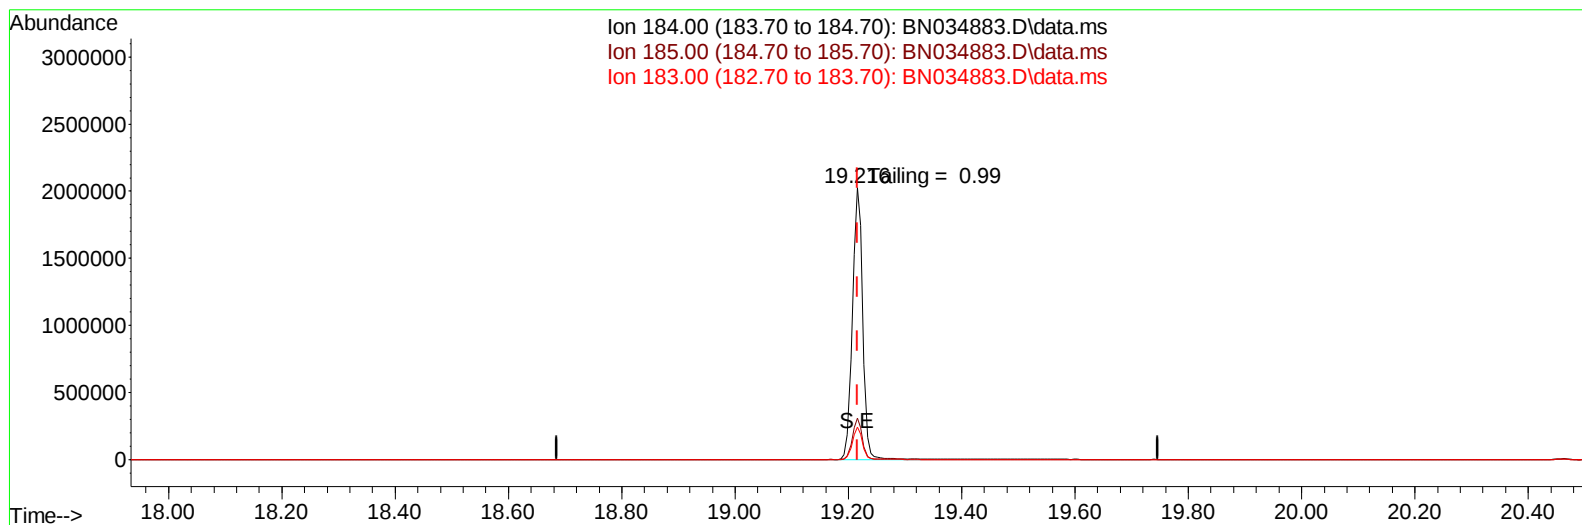

TIC: BN034883.D\data.ms

(77) Benzidine

19.216min (0.000) 0.00 ng

response 2581167

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.29
183.00	13.20	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2024	BNA_N	<u>BN034883.D</u>
Compound Name	Response	Retention Time
DDT	1134074	20.463
DDD	9937	20.069
DDE	132	19.504
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10069	1144143	0.88

Instrument :
BNA_N
ClientSampleId :
DFTPP