
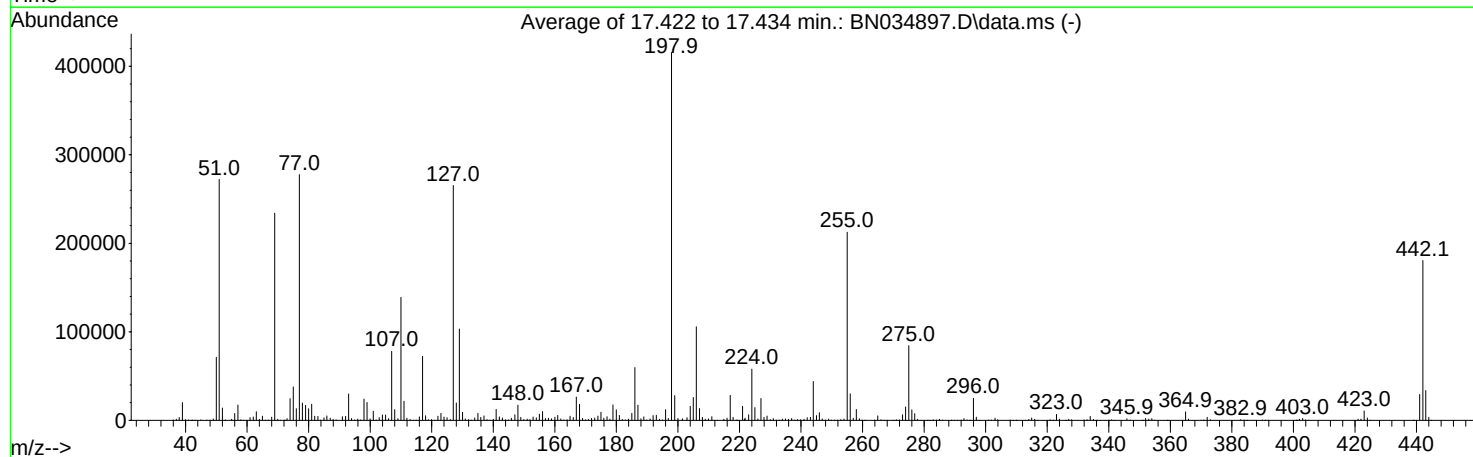


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110824\
Data File : BN034897.D
Acq On : 08 Nov 2024 07:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 15:02:36 2024

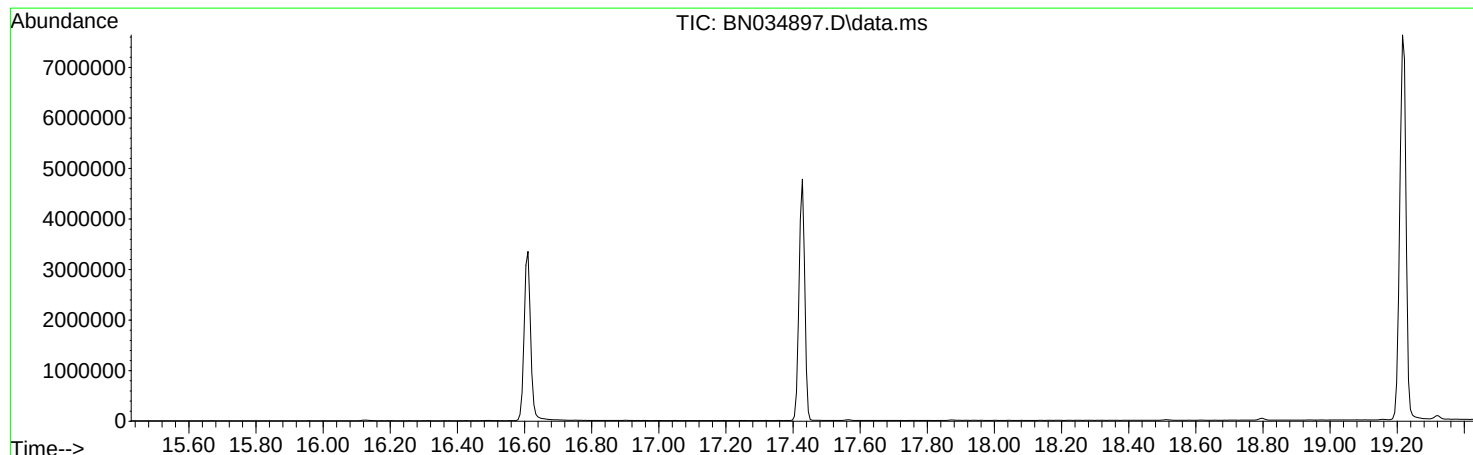

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.5	272195	PASS
68	69	0.00	2	1.6	3690	PASS
69	198	0.00	100	56.3	234112	PASS
70	69	0.00	2	0.5	1192	PASS
127	198	10	80	63.8	265344	PASS
197	198	0.00	2	0.5	2163	PASS
198	198	100	100	100.0	415616	PASS
199	198	5	9	6.7	28043	PASS
275	198	10	60	20.3	84464	PASS
365	198	1	100	2.3	9568	PASS
441	198	0.01	100	7.0	29224	PASS
442	442	50	100	100.0	180587	PASS
443	442	15	24	18.6	33651	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/8/2024	BNA_N	<u>BN034897.D</u>
Compound Name	Response	Retention Time
DDT	1384783	20.457
DDD	13389	20.069
DDE	195	19.51
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13584	1398367	0.97

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110824\
Data File : BN034897.D
Acq On : 08 Nov 2024 07:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 09 04:05:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 04:05:27 2024
Response via : Initial Calibration

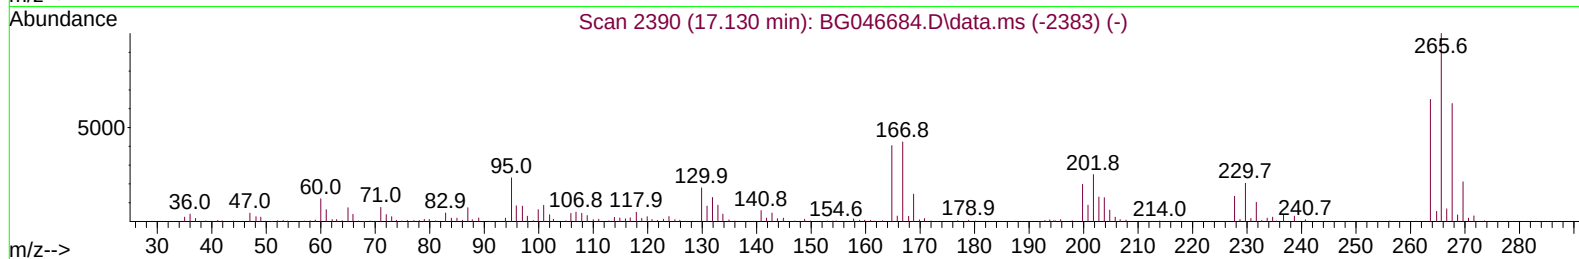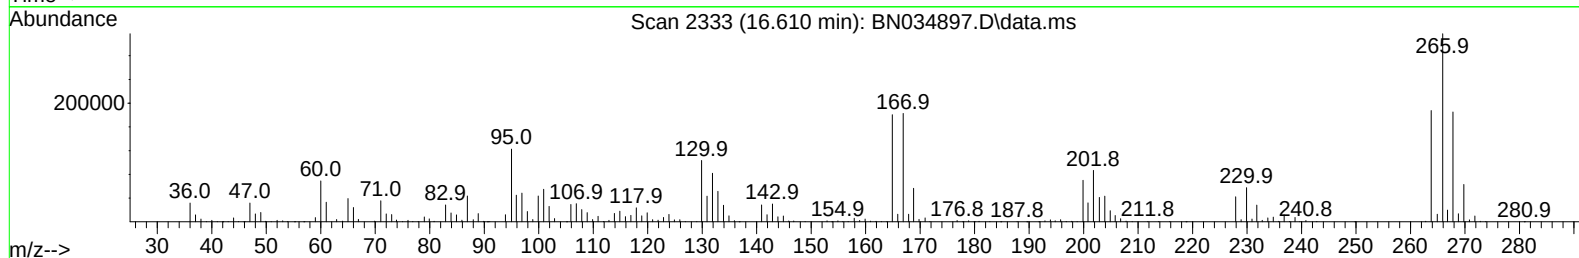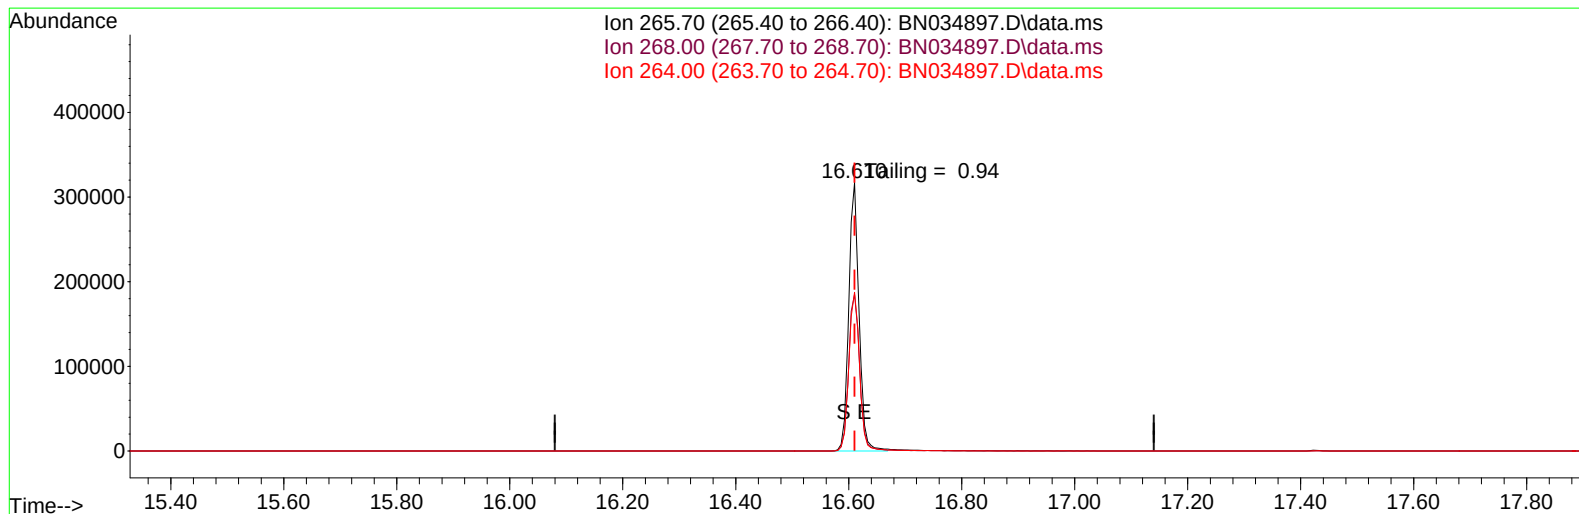

TIC: BN034897.D\data.ms

(70) Pentachlorophenol (C)

16.610min (0.000) 20617.49 ng




response 407091

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.38
264.00	61.60	59.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110824\
Data File : BN034897.D
Acq On : 08 Nov 2024 07:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 09 04:05:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 04:05:27 2024
Response via : Initial Calibration

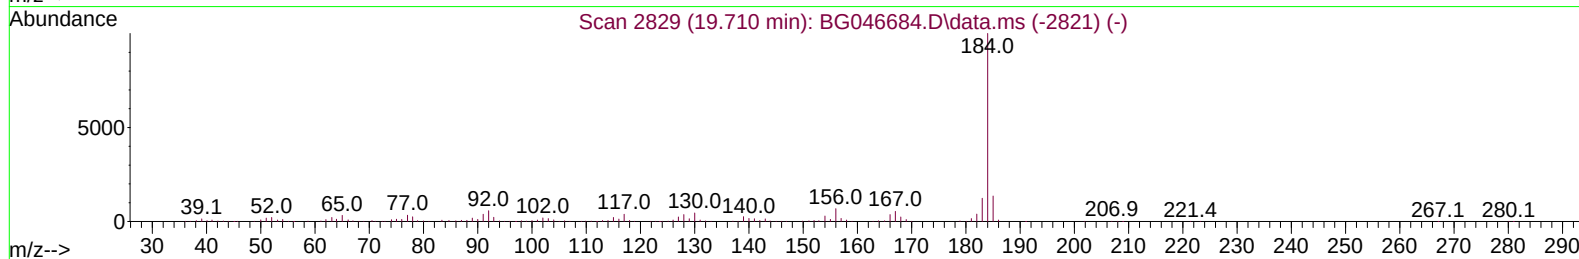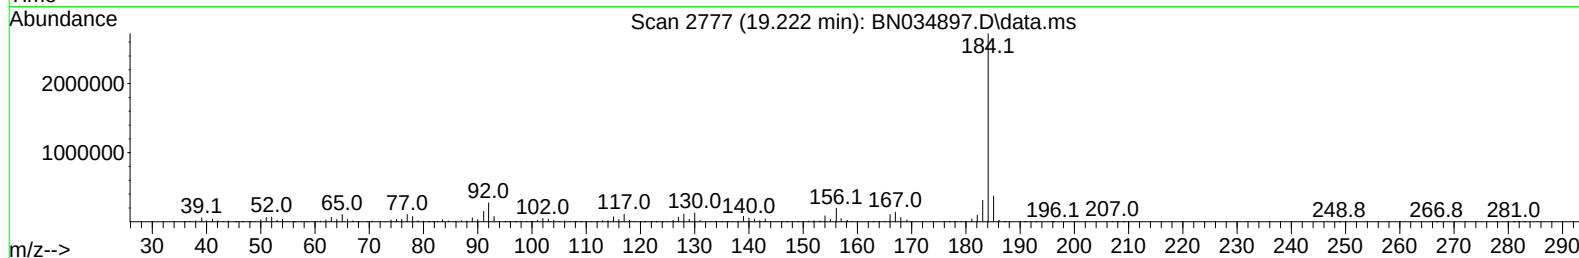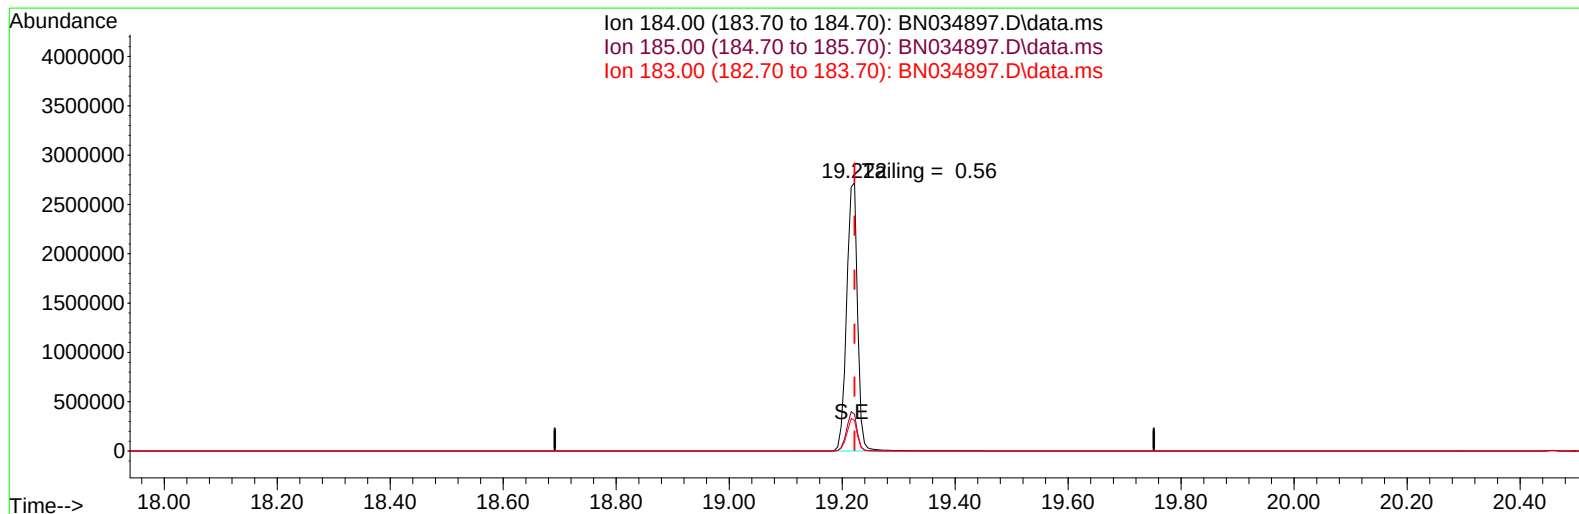

TIC: BN034897.D\data.ms

(77) Benzidine

19.222min (0.000) 0.00 ng

response 3642384

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	11.43
0.00	0.00	0.00