

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	P4718	OrderDate:	11/5/2024 1:31:00 PM
Client:	Portal Partners Tri-Venture	Project:	Amtrak Sawtooth Bridges 2024
Contact:	Joseph Krupansky	Location:	L21,VOA Ref. #2 Soil,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
P4718-01	WB-307-SB01	SOIL	PCB	8082A	11/04/24	11/06/24	11/06/24	11/05/24
P4718-02	WB-307-SB02	SOIL	PCB	8082A	11/04/24	11/06/24	11/06/24	11/05/24
P4718-04	WB-307-SW	WATER	PCB	8082A	11/04/24	11/06/24	11/06/24	11/05/24



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: P4718

Order ID: P4718

Client: Portal Partners Tri-Venture

Project ID: Amtrak Sawtooth Bridges 2024

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: **P4718**

Client: **Portal Partners Tri-Venture**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PO107183.D	PIBLK-PO107183.D	Tetrachloro-m-xylene	1	20	22.5	112		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	23.4	117		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	22.1	110		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	22.8	114		70 (60)	130 (140)
I.BLK-PO107730.D	PIBLK-PO107730.D	Tetrachloro-m-xylene	1	20	19.9	100		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	21.1	105		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.2	101		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	22.2	111		70 (60)	130 (140)
PB164700BL	PB164700BL	Tetrachloro-m-xylene	1	20	21.5	108		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	22.9	114		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	21.5	108		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	24.1	121		30 (32)	150 (175)
PB164700BS	PB164700BS	Tetrachloro-m-xylene	1	20	21.6	108		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	22.5	112		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	20.3	101		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	23.5	117		30 (32)	150 (175)
P4706-01MS	TR-04-110424MS	Tetrachloro-m-xylene	1	20	16.1	81		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	17.9	89		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	16.6	83		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	14.7	74		30 (32)	150 (175)
P4706-01MSD	TR-04-110424MSD	Tetrachloro-m-xylene	1	20	15.4	77		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	17.2	86		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	16.4	82		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	13.8	69		30 (32)	150 (175)
P4718-01	WB-307-SB01	Tetrachloro-m-xylene	1	20	14.9	75		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	13.1	66		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	18.5	93		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	11.0	55		30 (32)	150 (175)
I.BLK-PO107745.D	PIBLK-PO107745.D	Tetrachloro-m-xylene	1	20	19.2	96		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	18.8	94		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.0	100		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	18.1	91		70 (60)	130 (140)
PB164704BL	PB164704BL	Tetrachloro-m-xylene	1	20	19.0	95		30 (10)	150 (157)
		Decachlorobiphenyl	1	20	19.0	95		30 (10)	150 (173)
		Tetrachloro-m-xylene	2	20	19.8	99		30 (10)	150 (157)
		Decachlorobiphenyl	2	20	18.4	92		30 (10)	150 (173)
PB164704BS	PB164704BS	Tetrachloro-m-xylene	1	20	18.7	93		30 (10)	150 (157)
		Decachlorobiphenyl	1	20	18.8	94		30 (10)	150 (173)
		Tetrachloro-m-xylene	2	20	18.7	93		30 (10)	150 (157)
		Decachlorobiphenyl	2	20	18.5	92		30 (10)	150 (173)
PB164704BSD	PB164704BSD	Tetrachloro-m-xylene	1	20	19.6	98		30 (10)	150 (157)

() = LABORATORY INHOUSE LIMIT

Surrogate Summary

SDG No.: **P4718**

Client: **Portal Partners Tri-Venture**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
PB164704BSD	PB164704BSD	Decachlorobiphenyl	1	20	19.5	98		30 (10)	150 (173)
		Tetrachloro-m-xylene	2	20	19.3	97		30 (10)	150 (157)
P4718-04	WB-307-SW	Decachlorobiphenyl	2	20	19.3	97		30 (10)	150 (173)
		Tetrachloro-m-xylene	1	20	18.2	91		30 (10)	150 (157)
		Decachlorobiphenyl	1	20	17.6	88		30 (10)	150 (173)
		Tetrachloro-m-xylene	2	20	18.9	94		30 (10)	150 (157)
		Decachlorobiphenyl	2	20	18.8	94		30 (10)	150 (173)
		Tetrachloro-m-xylene	1	20	20.1	101		70 (60)	130 (140)
I.BLK-PO107760.D	PIBLK-PO107760.D	Decachlorobiphenyl	1	20	20.2	101		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.6	103		70 (60)	130 (140)
P4718-02	WB-307-SB02	Decachlorobiphenyl	2	20	22.6	113		70 (60)	130 (140)
		Tetrachloro-m-xylene	1	20	20.7	104		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	19.0	95		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	21.2	106		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	21.0	105		30 (32)	150 (175)
		Tetrachloro-m-xylene	1	20	20.6	103		70 (60)	130 (140)
I.BLK-PO107767.D	PIBLK-PO107767.D	Decachlorobiphenyl	1	20	21.1	106		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.7	104		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	22.6	113		70 (60)	130 (140)
		Tetrachloro-m-xylene	1	20	20.7	104		70 (60)	130 (140)

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P4718

Client: Portal Partners Tri-Venture

Analytical Method: 8082A

DataFile : PO107736.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	TR-04-110424MS											
P4706-01MS	AR1016	178.1	0	143	ug/kg	80				40 (55)	140 (146)	
	AR1260	178.1	0	142	ug/kg	80				40 (45)	140 (144)	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P4718

Client: Portal Partners Tri-Venture

Analytical Method: 8082A

DataFile : PO107737.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	TR-04-110424MSD											
P4706-01MSD	AR1016	178	0	139	ug/kg	78		3		40 (55)	140 (146)	30 (20)
	AR1260	178	0	135	ug/kg	76		5		40 (45)	140 (144)	30 (20)



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: P4718

Client: Portal Partners Tri-Venture

Analytical Method: **8082A** **Datafile :** PO107732.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD	Limits		RPD
								Qual	Low	High	
PB164700BS	AR1016	166.5	163	ug/kg	98				40 (71)	140 (120)	
	AR1260	166.5	168	ug/kg	101				40 (65)	140 (130)	



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: P4718

Client: Portal Partners Tri-Venture

Analytical Method: 8082A Datafile : PO107747.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB164704BS	AR1016	5	4.20	ug/L	84				40 (61)	140 (112)	
	AR1260	5	4.30	ug/L	86				40 (66)	140 (113)	



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: P4718

Client: Portal Partners Tri-Venture

Analytical Method: 8082A Datafile : PO107748.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD	Limits		RPD
								Qual	Low	High	
PB164704BSD	AR1016	5	4.50	ug/L	90	7			40 (61)	140 (112)	20 (20)
	AR1260	5	4.50	ug/L	90	5			40 (66)	140 (113)	20 (20)

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB164700BL

Lab Name: CHEMTECH

Contract: PORT06

Lab Code: CHEM Case No.: P4718

SAS No.: P4718 SDG NO.: P4718

Lab Sample ID: PB164700BL

Lab File ID: PO107731.D

Matrix: (soil/water) Solid

Extraction: (Type) _____

Sulfur Cleanup: (Y/N) N

Date Extracted: 11/06/2024

Date Analyzed (1): 11/06/2024

Date Analyzed (2): 11/06/2024

Time Analyzed (1): 13:10

Time Analyzed (2): 13:10

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB164700BS	PB164700BS	PO107732.D	11/06/2024	11/06/2024
TR-04-110424MS	P4706-01MS	PO107736.D	11/06/2024	11/06/2024
TR-04-110424MSD	P4706-01MSD	PO107737.D	11/06/2024	11/06/2024
WB-307-SB01	P4718-01	PO107740.D	11/06/2024	11/06/2024
WB-307-SB02	P4718-02	PO107761.D	11/06/2024	11/06/2024

COMMENTS: _____

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB164704BL

Lab Name: CHEMTECH

Contract: PORT06

Lab Code: CHEM Case No.: P4718

SAS No.: P4718 SDG NO.: P4718

Lab Sample ID: PB164704BL

Lab File ID: PO107746.D

Matrix: (soil/water) WATER

Extraction: (Type) _____

Sulfur Cleanup: (Y/N) N

Date Extracted: 11/06/2024

Date Analyzed (1): 11/06/2024

Date Analyzed (2): 11/06/2024

Time Analyzed (1): 18:15

Time Analyzed (2): 18:15

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB164704BS	PB164704BS	PO107747.D	11/06/2024	11/06/2024
PB164704BSD	PB164704BSD	PO107748.D	11/06/2024	11/06/2024
WB-307-SW	P4718-04	PO107755.D	11/06/2024	11/06/2024

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/04/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/05/24
Client Sample ID:	WB-307-SB01	SDG No.:	P4718
Lab Sample ID:	P4718-01	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	78
Sample Wt/Vol:	30.06	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107740.D	1	11/06/24 09:10	11/06/24 15:35	PB164700

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.30	U	4.30	21.8	ug/kg
11104-28-2	Aroclor-1221	8.20	U	8.20	21.8	ug/kg
11141-16-5	Aroclor-1232	4.40	U	4.40	21.8	ug/kg
53469-21-9	Aroclor-1242	4.30	U	4.30	21.8	ug/kg
12672-29-6	Aroclor-1248	10.1	U	10.1	21.8	ug/kg
11097-69-1	Aroclor-1254	3.50	U	3.50	21.8	ug/kg
37324-23-5	Aroclor-1262	5.80	U	5.80	21.8	ug/kg
11100-14-4	Aroclor-1268	4.40	U	4.40	21.8	ug/kg
11096-82-5	Aroclor-1260	3.70	U	3.70	21.8	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.5		30 (32) - 150 (144)	93%	SPK: 20
2051-24-3	Decachlorobiphenyl	13.1		30 (32) - 150 (175)	66%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107740.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 15:35
 Operator : YP/AJ
 Sample : P4718-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WB-307-SB01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:38:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.643	136.2E6	59626457	14.945	18.526
2) SA Decachlor...	10.076	8.639	32165255	30200030	13.111	11.015

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107740.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 15:35
Operator : YP/AJ
Sample : P4718-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WB-307-SB01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:38:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

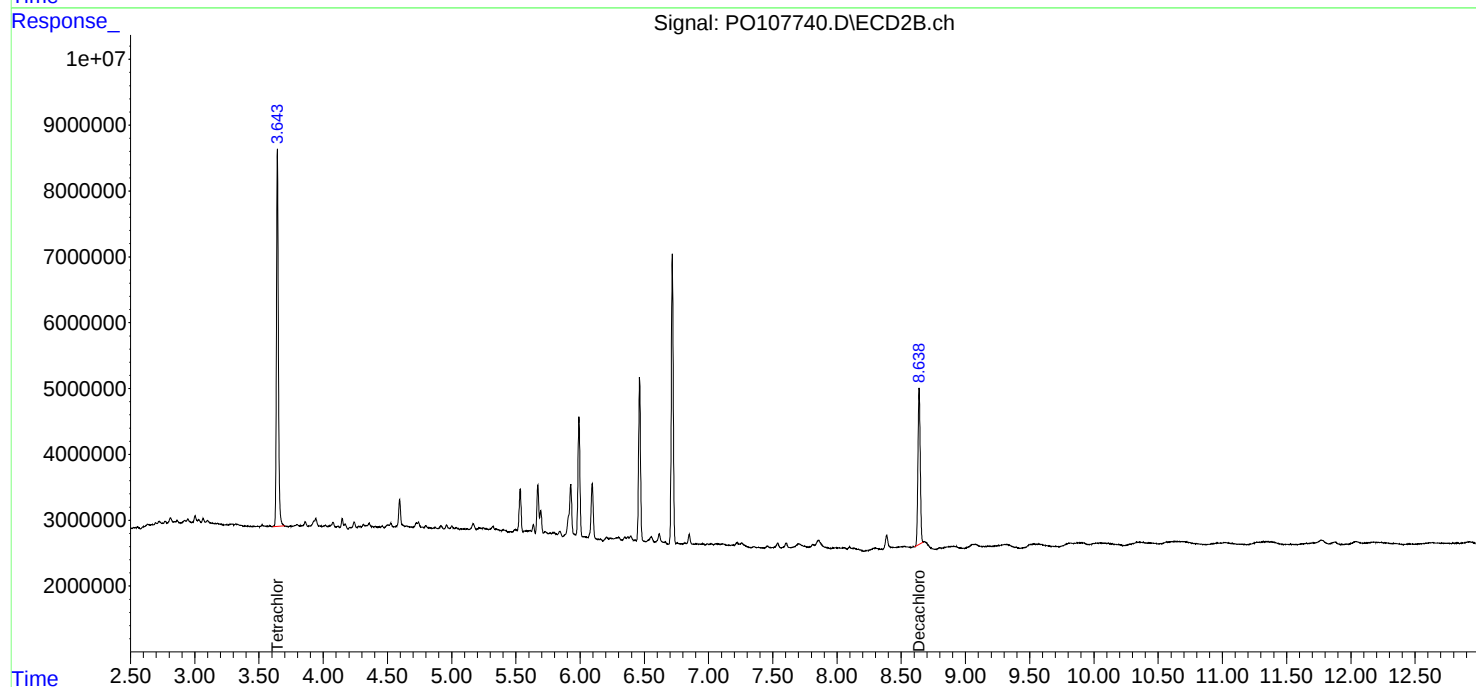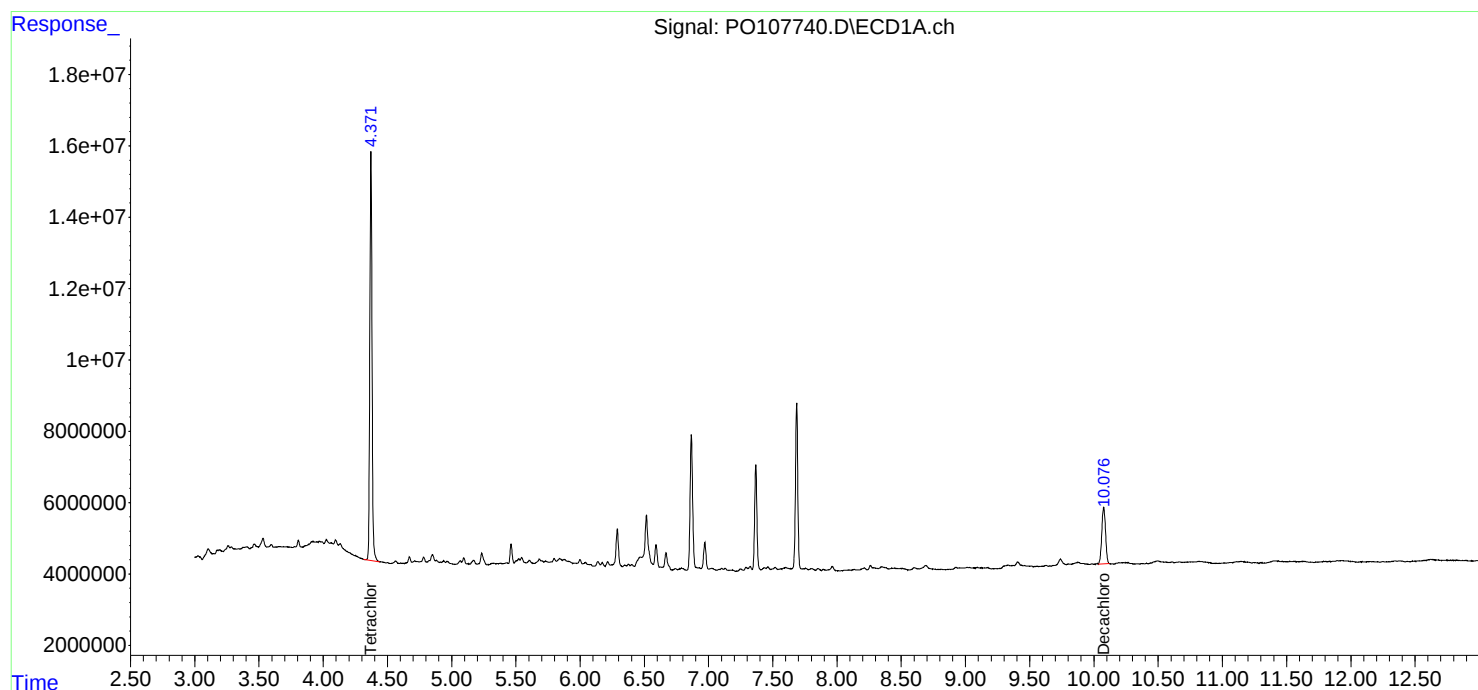


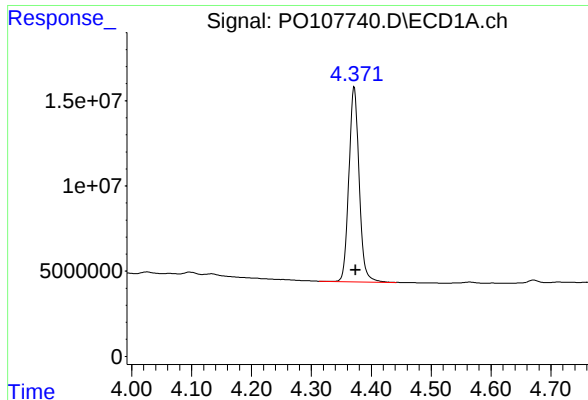

#1 Tetrachloro-m-xylene


R.T.: 4.372 min
Delta R.T.: -0.002 min
Response: 136204161
Conc: 14.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
WB-307-SB01

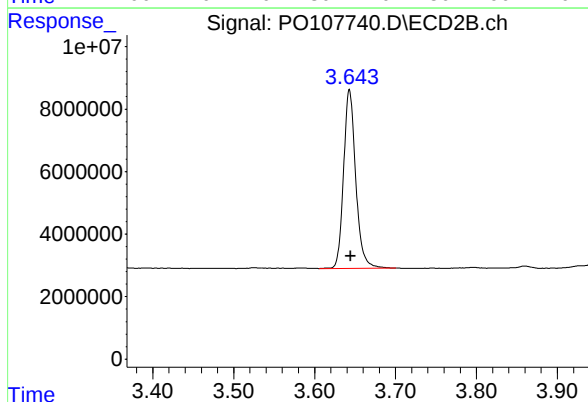


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.002 min
Response: 59626457
Conc: 18.53 ng/ml

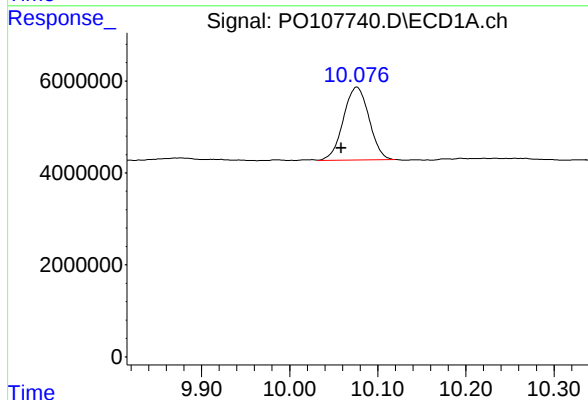

#2 Decachlorobiphenyl

R.T.: 10.076 min
Delta R.T.: 0.018 min
Response: 32165255
Conc: 13.11 ng/ml

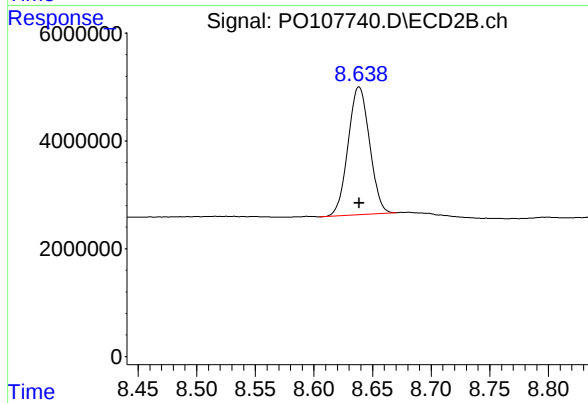

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 30200030
Conc: 11.02 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/04/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/05/24
Client Sample ID:	WB-307-SB02	SDG No.:	P4718
Lab Sample ID:	P4718-02	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	77.6
Sample Wt/Vol:	30.03	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107761.D	1	11/06/24 09:10	11/06/24 23:02	PB164700

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.40	U	4.40	21.9	ug/kg
11104-28-2	Aroclor-1221	8.30	U	8.30	21.9	ug/kg
11141-16-5	Aroclor-1232	4.40	U	4.40	21.9	ug/kg
53469-21-9	Aroclor-1242	4.40	U	4.40	21.9	ug/kg
12672-29-6	Aroclor-1248	10.2	U	10.2	21.9	ug/kg
11097-69-1	Aroclor-1254	3.50	U	3.50	21.9	ug/kg
37324-23-5	Aroclor-1262	5.90	U	5.90	21.9	ug/kg
11100-14-4	Aroclor-1268	4.40	U	4.40	21.9	ug/kg
11096-82-5	Aroclor-1260	3.70	U	3.70	21.9	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.2		30 (32) - 150 (144)	106%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.0		30 (32) - 150 (175)	105%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 23:02
 Operator : YP/AJ
 Sample : P4718-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WB-307-SB02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:51:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.642	188.9E6	68344143	20.728	21.235
2) SA Decachlor...	10.075	8.639	46538403	57577942	18.969	21.002

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 23:02
Operator : YP/AJ
Sample : P4718-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WB-307-SB02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:51:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

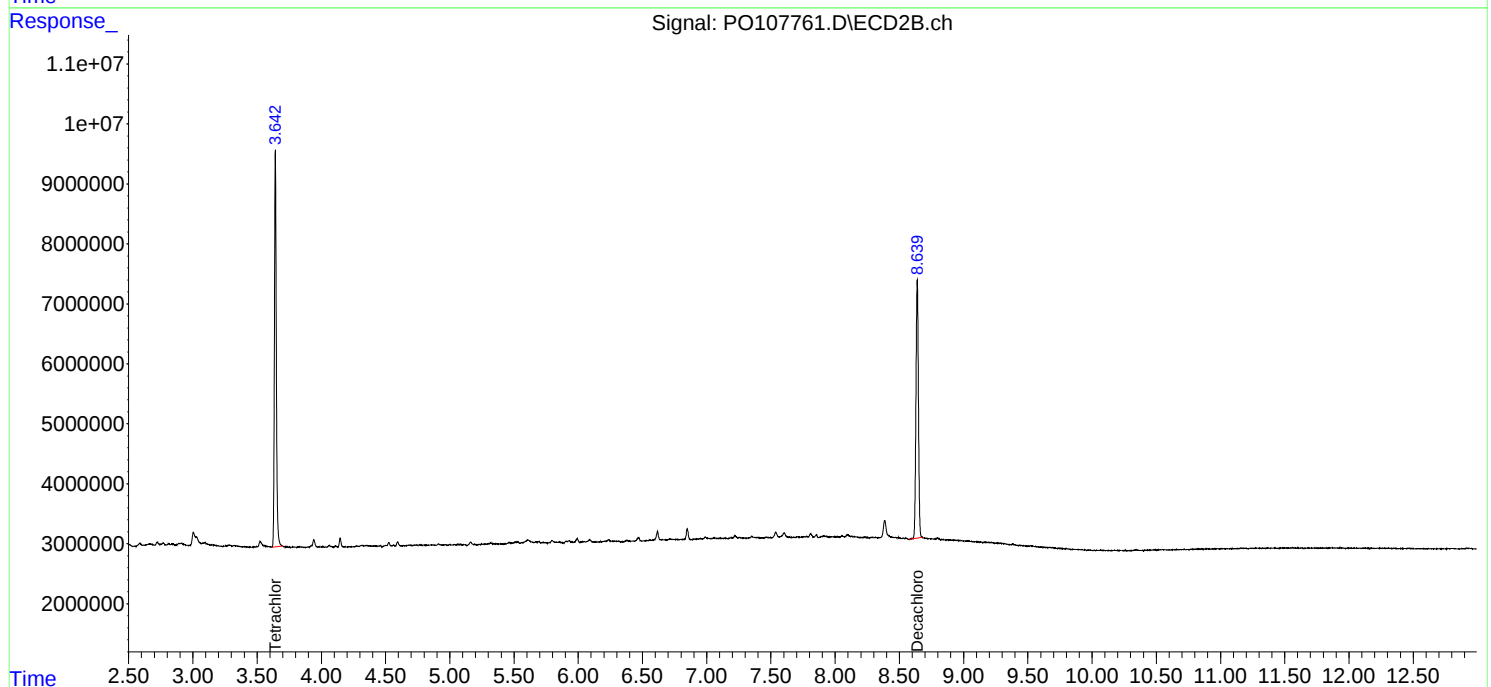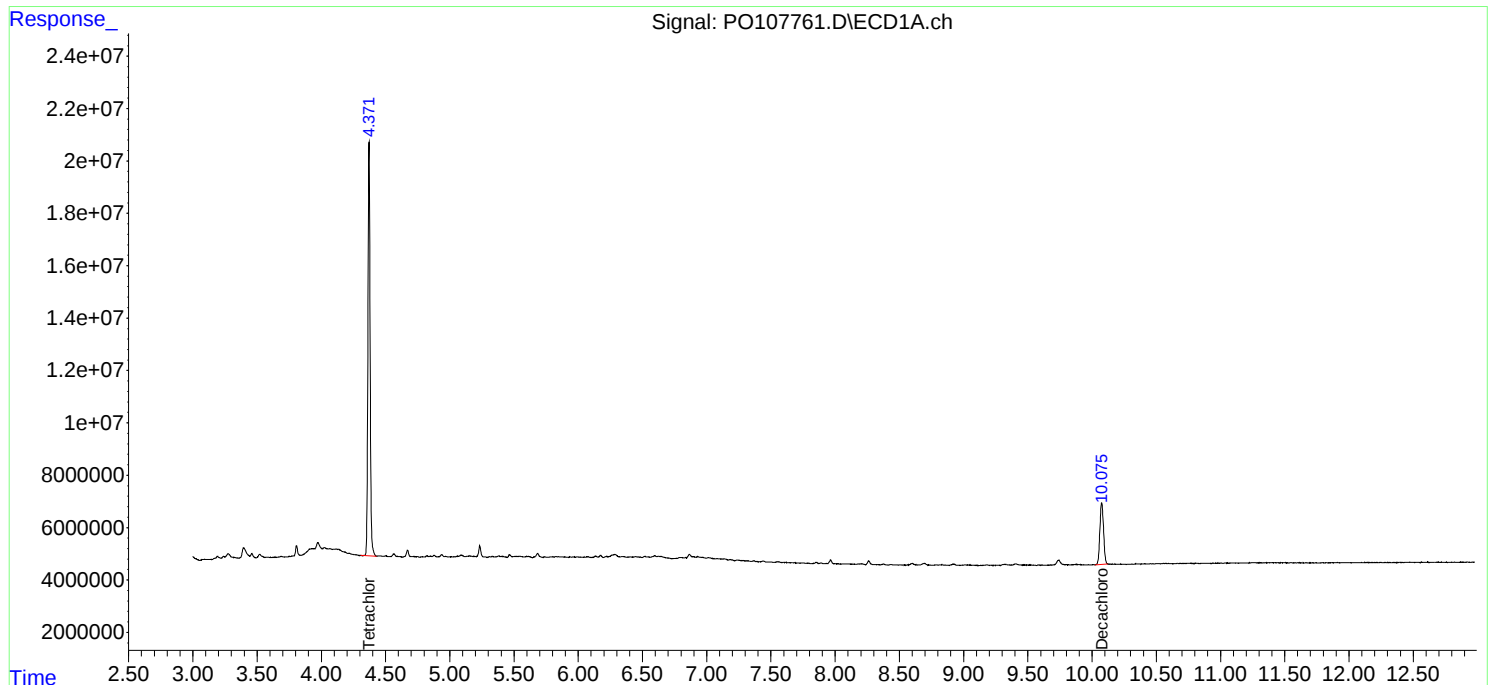


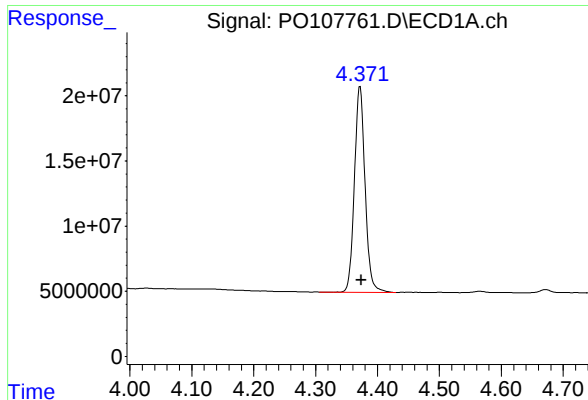

#1 Tetrachloro-m-xylene


R.T.: 4.372 min
Delta R.T.: -0.002 min
Response: 188913124
Conc: 20.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
WB-307-SB02

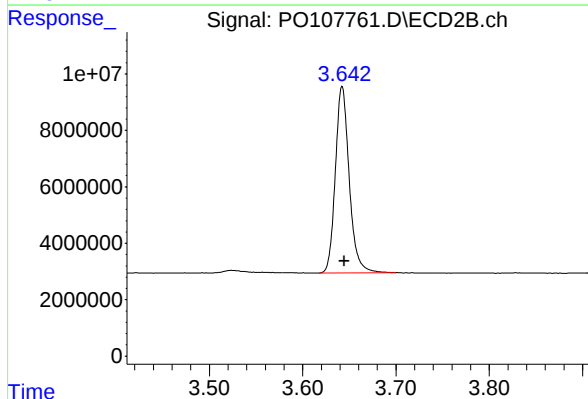


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.002 min
Response: 68344143
Conc: 21.23 ng/ml

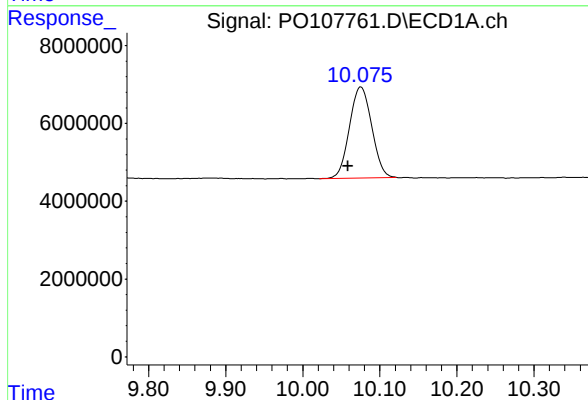

#2 Decachlorobiphenyl

R.T.: 10.075 min
Delta R.T.: 0.017 min
Response: 46538403
Conc: 18.97 ng/ml

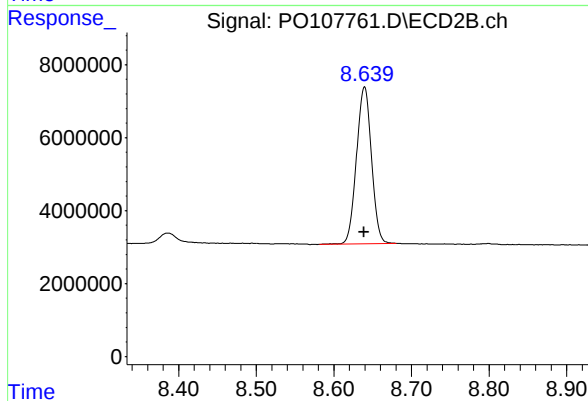

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 57577942
Conc: 21.00 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/04/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/05/24
Client Sample ID:	WB-307-SW	SDG No.:	P4718
Lab Sample ID:	P4718-04	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	450	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	3510C	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107755.D	1	11/06/24 08:25	11/06/24 20:41	PB164704

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.17	U	0.17	0.56	ug/L
11104-28-2	Aroclor-1221	0.26	U	0.26	0.56	ug/L
11141-16-5	Aroclor-1232	0.41	U	0.41	0.56	ug/L
53469-21-9	Aroclor-1242	0.18	U	0.18	0.56	ug/L
12672-29-6	Aroclor-1248	0.13	U	0.13	0.56	ug/L
11097-69-1	Aroclor-1254	0.12	U	0.12	0.56	ug/L
37324-23-5	Aroclor-1262	0.16	U	0.16	0.56	ug/L
11100-14-4	Aroclor-1268	0.13	U	0.13	0.56	ug/L
11096-82-5	Aroclor-1260	0.17	U	0.17	0.56	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.9		30 (10) - 150 (157)	94%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.8		30 (10) - 150 (173)	94%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 20:41
 Operator : YP/AJ
 Sample : P4718-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WB-307-SW

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:47:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.643	165.7E6	60741855	18.177	18.873
2) SA Decachlor...	10.075	8.639	43125108	51403974	17.578	18.750

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 20:41
Operator : YP/AJ
Sample : P4718-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WB-307-SW

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:47:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

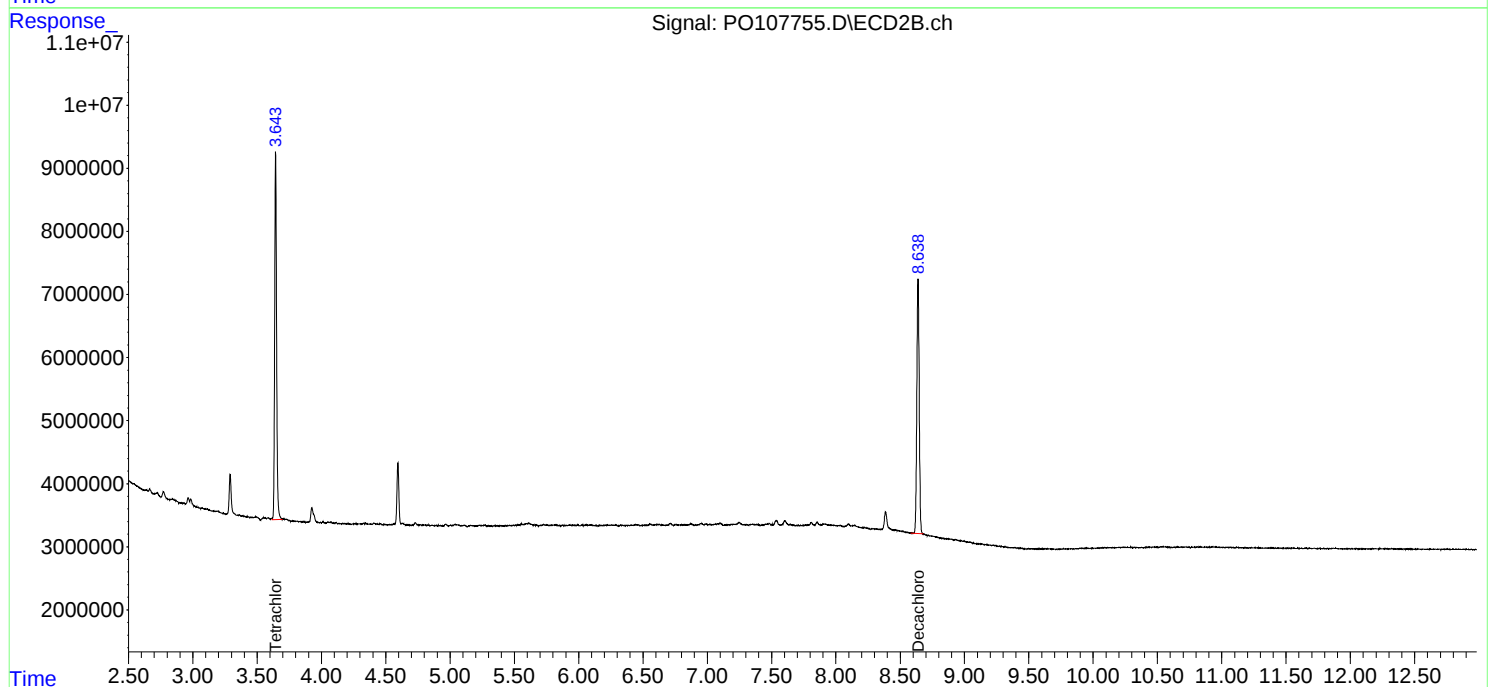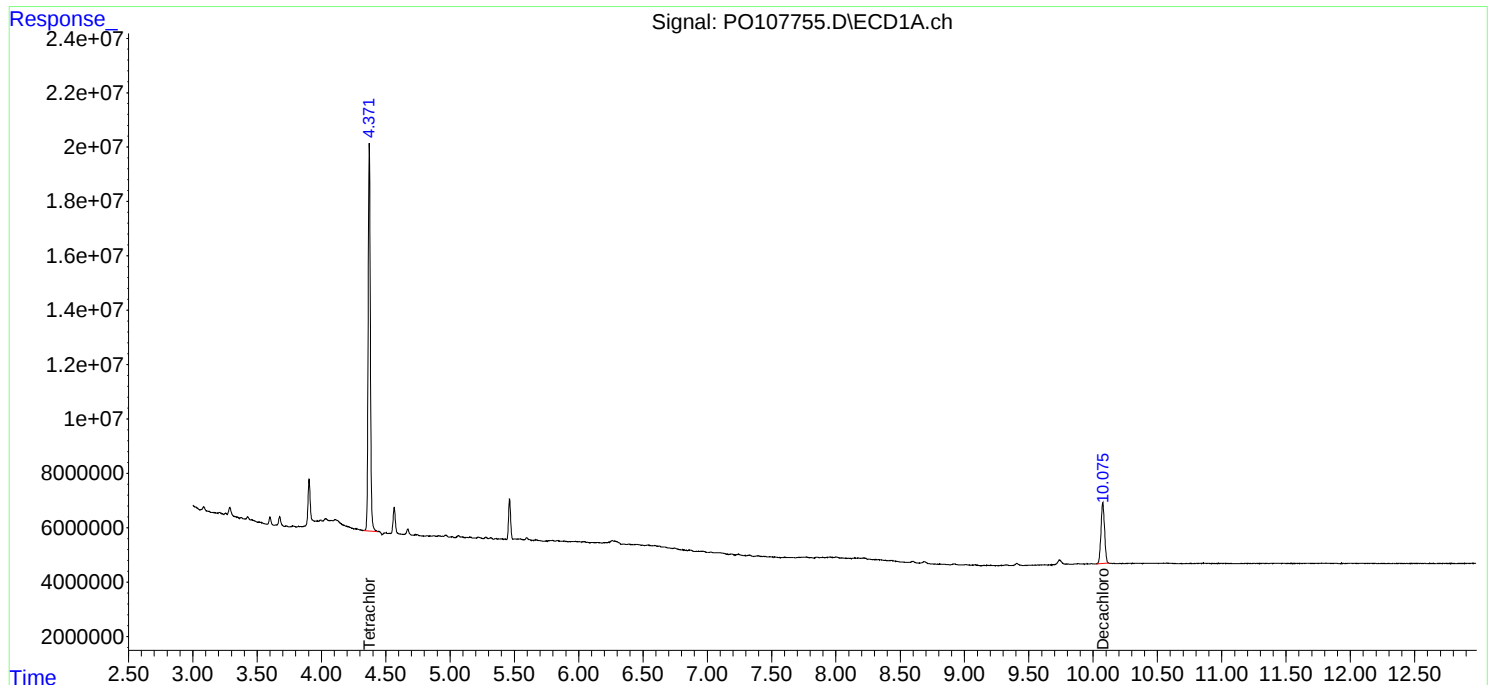


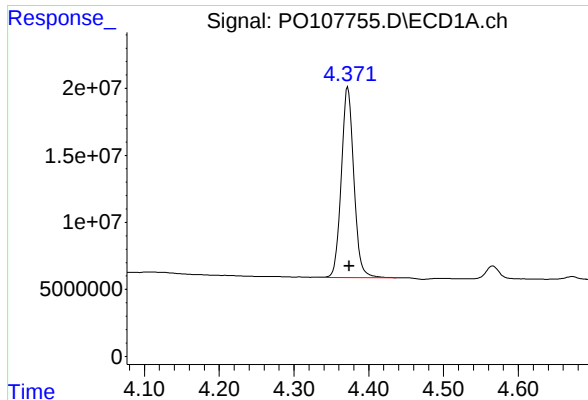

#1 Tetrachloro-m-xylene


R.T.: 4.372 min
Delta R.T.: -0.002 min
Response: 165666421
Conc: 18.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
WB-307-SW

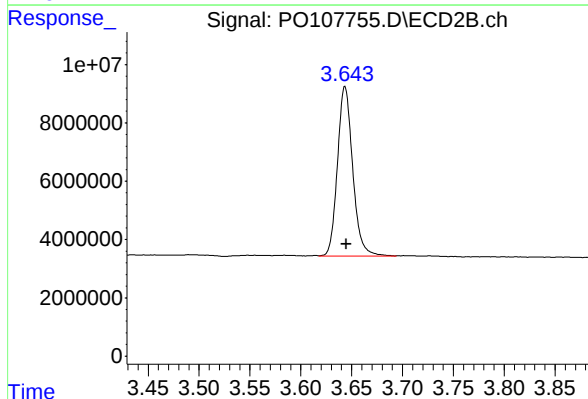


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.001 min
Response: 60741855
Conc: 18.87 ng/ml

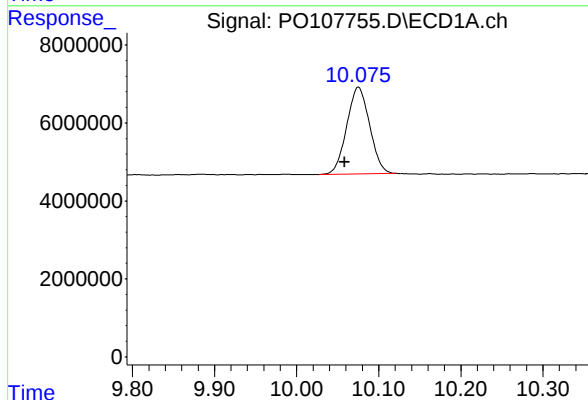

#2 Decachlorobiphenyl

R.T.: 10.075 min
Delta R.T.: 0.017 min
Response: 43125108
Conc: 17.58 ng/ml

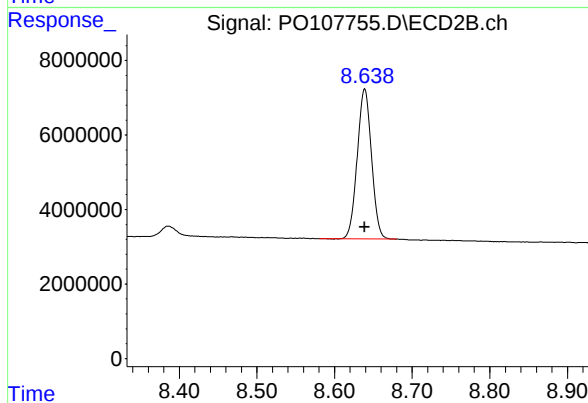

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 51403974
Conc: 18.75 ng/ml



CALIBRATION SUMMARY

RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>PORT06</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>P4718</u>	SAS No.:	<u>P4718</u>	SDG NO.:	<u>P4718</u>
Instrument ID:	<u>ECD_O</u>	Calibration Date(s):		<u>10/15/2024</u>	<u>10/16/2024</u>		
		Calibration Times:		<u>18:27</u>	<u>02:36</u>		

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	<u>PO107184.D</u>	RT 750 =	<u>PO107185.D</u>
	RT 500 =	PO107186.D	RT 250 =	PO107187.D
			RT 050 =	PO107188.D

[illegible]

[illegible]

GC Column: ZB-MR2 ID: 0.32 (mm)

[illegible]

RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	8.64	8.64	8.64	8.64	8.64	8.64	8.54	8.74
Tetrachloro-m-xylene	3.65	3.64	3.65	3.64	3.65	3.65	3.55	3.75

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: PORT06
Lab Code: CHEM **Case No.:** P4718 **SAS No.:** P4718 **SDG NO.:** P4718
Instrument ID: ECD_O
Calibration Date(s): 10/15/2024 10/16/2024
Calibration Times: 18:27 02:36

GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO107184.D</u>		CF 750 = <u>PO107185.D</u>			
CF 500 = <u>PO107186.D</u>		CF 250 = <u>PO107187.D</u>		CF 050 = <u>PO107188.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	252081604	261702867	271939076	291118488	272229420	269814291 5
Aroclor-1016-2	(2)	373760062	383028583	397887352	419075308	410673320	396884925 5
Aroclor-1016-3	(3)	234678633	244145249	256575754	276405664	244042480	251169556 6
Aroclor-1016-4	(4)	185622493	193848624	202963902	215081552	165543020	192611918 10
Aroclor-1016-5	(5)	176326470	182141932	191487930	203514892	159796500	182653545 9
Aroclor-1260-1	(1)	238480871	246497651	259155974	277220676	271587560	258588546 6
Aroclor-1260-2	(2)	243402558	251747185	264083512	284216460	272650860	263220115 6
Aroclor-1260-3	(3)	167353086	171560129	181491762	195138068	183182660	179745141 6
Aroclor-1260-4	(4)	162125557	166999933	175289716	187582032	185522120	175503872 6
Aroclor-1260-5	(5)	268686175	273623828	283035894	299271412	297351500	284393762 5
Decachlorobiphenyl		2362750210	2427138920	2496479000	2603827440	2376686800	2453376474 4
Tetrachloro-m-xylene		8902656430	9087809293	9285762860	9548006280	8745262400	9113899453 3
Aroclor-1242-1	(1)	207947063	205572916	222208808	238956456	243522880	223641625 8
Aroclor-1242-2	(2)	302439626	299949616	323550412	342804408	348858880	323520588 7
Aroclor-1242-3	(3)	191912697	193178427	209638152	224306728	225847640	208976729 8
Aroclor-1242-4	(4)	150447174	145338196	162797508	173135964	168308740	160005516 7
Aroclor-1242-5	(5)	141009343	143408436	153689098	164623016	179679780	156481935 10
Decachlorobiphenyl		2339420350	2427742867	2492700840	2551827400	2426410200	2447620331 3
Tetrachloro-m-xylene		8860043620	8651743680	9146784160	9504075440	9174828800	9067495140 4
Aroclor-1248-1	(1)	155913014	164800668	175191332	184609772	188867720	173876501 8
Aroclor-1248-2	(2)	222845576	238202488	253637968	270074056	280366620	253025342 9
Aroclor-1248-3	(3)	231904923	246233752	259706092	274388212	266197800	255686156 7
Aroclor-1248-4	(4)	237210289	246633865	260533272	272872732	271860120	257822056 6
Aroclor-1248-5	(5)	236273499	246591072	260733536	276314120	280304600	260043365 7
Decachlorobiphenyl		2339780580	2371533013	2504089680	2566158680	2396701200	2435652631 4
Tetrachloro-m-xylene		8719403610	9119992693	9358904180	9492784200	8995773400	9137371617 3
Aroclor-1254-1	(1)	246822697	256579683	264992242	286189960	289157060	268748328 7
Aroclor-1254-2	(2)	348120894	361641555	373031238	401237980	402995760	377405485 6
Aroclor-1254-3	(3)	336293322	345653409	355909306	378498460	372630440	357796987 5
Aroclor-1254-4	(4)	213138598	220171503	227187688	242530220	244046960	229414994 6
Aroclor-1254-5	(5)	194609638	201069208	205869028	220139672	216546640	207646837 5
Decachlorobiphenyl		2357746210	2401897693	2508594000	2601578200	2359367400	2445836701 4
Tetrachloro-m-xylene		8883763230	9164627320	9184369060	9508828480	8791509400	9106619498 3
Aroclor-1268-1	(1)	351862425	352413819	364622844	381760528	369380480	364008019 3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	313096403	314491445	324862806	339637696	320299560	322477582	3
Aroclor-1268-3	(3)	272236453	272760276	282620036	293538700	275661940	279363481	3
Aroclor-1268-4	(4)	112236308	111261111	114714594	116428084	101458340	111219687	5
Aroclor-1268-5	(5)	836674479	833098204	847063314	864357444	781067560	832452200	4
Decachlorobiphenyl		4074190590	4136234160	4241958160	4399826360	4004084600	4171258774	4
Tetrachloro-m-xylene		9139601460	8935957933	9311606620	9495189880	8951901000	9166851379	3

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: PORT06
Lab Code: CHEM **Case No.:** P4718 **SAS No.:** P4718 **SDG NO.:** P4718
Instrument ID: ECD_O
Calibration Date(s): 10/15/2024 10/16/2024
Calibration Times: 18:27 02:36
GC Column: ZB-MR2 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO107184.D</u>		CF 750 = <u>PO107185.D</u>				
CF 500 = <u>PO107186.D</u>		CF 250 = <u>PO107187.D</u>		CF 050 = <u>PO107188.D</u>				
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1	(1)	98519363	99934743	102532802	106601384	108740020	103265662	4
Aroclor-1016-2	(2)	140533795	142751421	144315942	146877552	130360060	140967754	5
Aroclor-1016-3	(3)	75819146	77111448	78799028	81783348	80215260	78745646	3
Aroclor-1016-4	(4)	61532960	63413097	65607722	69564368	70423600	66108349	6
Aroclor-1016-5	(5)	78878086	80970861	83522668	86940988	80356660	82133853	4
Aroclor-1260-1	(1)	150450531	152030172	155131756	161942364	156218200	155154605	3
Aroclor-1260-2	(2)	173752920	181526657	184104290	189736236	151457920	176115605	8
Aroclor-1260-3	(3)	168454604	170292340	172108108	175991544	151894120	167748143	6
Aroclor-1260-4	(4)	143637024	144895129	147115166	150514212	137242140	144680734	3
Aroclor-1260-5	(5)	340738400	339782780	336796716	340391952	289493480	329440666	7
Decachlorobiphenyl		2730622670	2745732653	2784792900	2852828640	2594005000	2741596373	3
Tetrachloro-m-xylene		3312014480	3338472613	3349065240	3230716080	2862214000	3218496483	6
Aroclor-1242-1	(1)	80390662	80447493	83937762	87266896	86674240	83743411	4
Aroclor-1242-2	(2)	114487494	111266404	117741916	120667112	114031640	115638913	3
Aroclor-1242-3	(3)	61817452	60461905	64396992	66865868	63624080	63433259	4
Aroclor-1242-4	(4)	60582529	60636219	64384594	68045260	66598220	64049364	5
Aroclor-1242-5	(5)	73763103	75675432	77215916	80736528	80226620	77523520	4
Decachlorobiphenyl		2686985320	2764418280	2764436780	2798541920	2665265400	2735929540	2
Tetrachloro-m-xylene		3315724680	3241948653	3341198040	3335574400	2920075400	3230904235	6
Aroclor-1248-1	(1)	60218805	63038185	64879120	66667236	62402400	63441149	4
Aroclor-1248-2	(2)	85173308	89108361	93061950	96541480	93540340	91485088	5
Aroclor-1248-3	(3)	89257070	93226611	97377878	100891904	96212540	95393201	5
Aroclor-1248-4	(4)	105934439	110533117	114760412	117772688	111691080	112138347	4
Aroclor-1248-5	(5)	102828085	105359652	109801380	114217964	119140640	110269544	6
Decachlorobiphenyl		2669365810	2682497173	2791873700	2836714480	2679938000	2732077833	3
Tetrachloro-m-xylene		3278417600	3389239440	3425836480	3362184040	2965722400	3284279992	6
Aroclor-1254-1	(1)	159855276	163854537	165548332	171717704	162964860	164788142	3
Aroclor-1254-2	(2)	138468840	142269335	144546922	151325972	148203140	144962842	3
Aroclor-1254-3	(3)	227061110	231385951	232213406	238575248	218867080	229620559	3
Aroclor-1254-4	(4)	128242906	130249965	131325350	135207044	122091880	129423429	4
Aroclor-1254-5	(5)	191904554	195153152	195378104	201188864	171636600	191052255	6
Decachlorobiphenyl		2726927150	2738190720	2773447120	2836815760	2598739800	2734824110	3
Tetrachloro-m-xylene		3347799560	3397335627	3354246660	3362236280	2930639600	3278451545	6
Aroclor-1268-1	(1)	419191400	409991492	413863584	410849472	368955300	404570250	5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	389672996	380096764	383518208	378699872	334345600	373266688	6
Aroclor-1268-3	(3)	345284332	337828173	339535756	338755760	307004380	333681680	5
Aroclor-1268-4	(4)	129107993	127445005	127285362	129260796	113749480	125369727	5
Aroclor-1268-5	(5)	1049237500	1019311260	1017080130	996315476	856840280	987756929	8
Decachlorobiphenyl		4873889790	4739451973	4823511780	4890043960	4430545400	4751488581	4
Tetrachloro-m-xylene		3440286630	3329771373	3416104800	3331345720	2963806400	3296262985	6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Instrument ID: ECD_O Date(s) Analyzed: 10/15/2024 10/16/2024

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	4.57	4.47	4.67	110010000
		2	4.66	4.56	4.76	78836600
		3	4.73	4.63	4.83	234100000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.73	4.63	4.83	195844000
		2	5.26	5.16	5.36	103025000
		3	5.54	5.44	5.64	179001000
		4	5.70	5.60	5.80	90165400
		5	5.80	5.70	5.90	65903200
Aroclor-1262	500	1	7.74	7.64	7.84	245548000
		2	8.28	8.18	8.38	309420000
		3	8.59	8.49	8.69	209196000
		4	8.68	8.58	8.78	163066000
		5	9.32	9.22	9.42	102764000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Instrument ID: ECD_O Date(s) Analyzed: 10/15/2024 10/16/2024

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.86	3.76	3.96	34895600
		2	3.94	3.84	4.04	26624800
		3	4.02	3.92	4.12	81218600
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.02	3.92	4.12	67327000
		2	4.75	4.65	4.85	63205200
		3	4.92	4.82	5.02	34475000
		4	5.00	4.90	5.10	31466000
		5	5.18	5.08	5.28	33083400
Aroclor-1262	500	1	6.76	6.66	6.86	212876000
		2	7.26	7.16	7.36	363332000
		3	7.54	7.44	7.64	137384000
		4	7.61	7.51	7.71	264574000
		5	8.10	8.00	8.20	112833000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 18:27
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:24:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	890.3E6	331.2E6	95.874	98.894
2) SA Decachlor...	10.059	8.639	236.3E6	273.1E6	94.643	98.055
Target Compounds						
3) L1 AR-1016-1	5.521	4.726	252.1E6	98519363	926.978	960.857
4) L1 AR-1016-2	5.544	4.745	373.8E6	140.5E6	939.362	973.793
5) L1 AR-1016-3	5.606	4.921	234.7E6	75819146	914.656	962.184
6) L1 AR-1016-4	5.703	4.962	185.6E6	61532960	914.559	937.892
7) L1 AR-1016-5	5.998	5.175	176.3E6	78878086	920.823	944.391
31) L7 AR-1260-1	7.124	6.207	238.5E6	150.5E6	920.221	969.824
32) L7 AR-1260-2	7.381	6.393	243.4E6	173.8E6	921.688	943.774
33) L7 AR-1260-3	7.743	6.547	167.4E6	168.5E6	922.097	978.772
34) L7 AR-1260-4	7.967	7.018	162.1E6	143.6E6	924.901	976.358
35) L7 AR-1260-5	8.281	7.258	268.7E6	340.7E6	949.301	1011.703



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 18:27
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:24:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

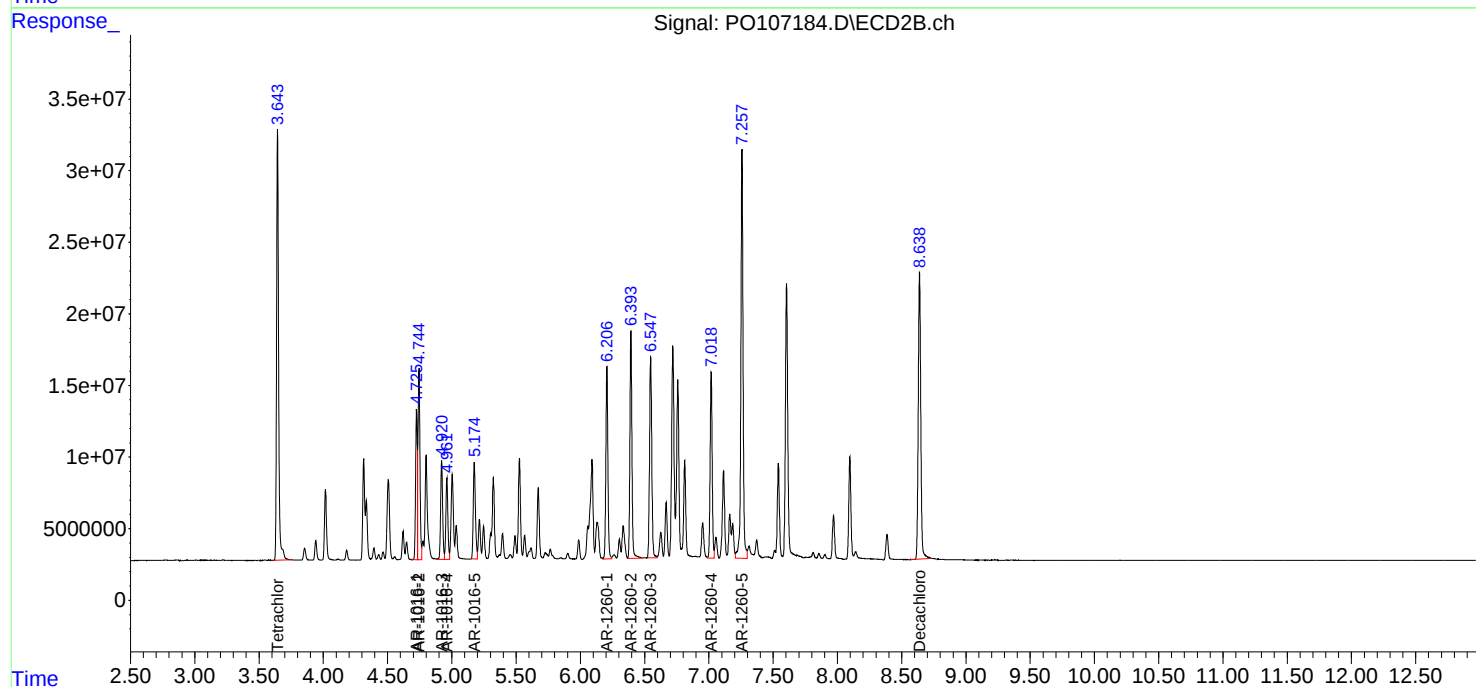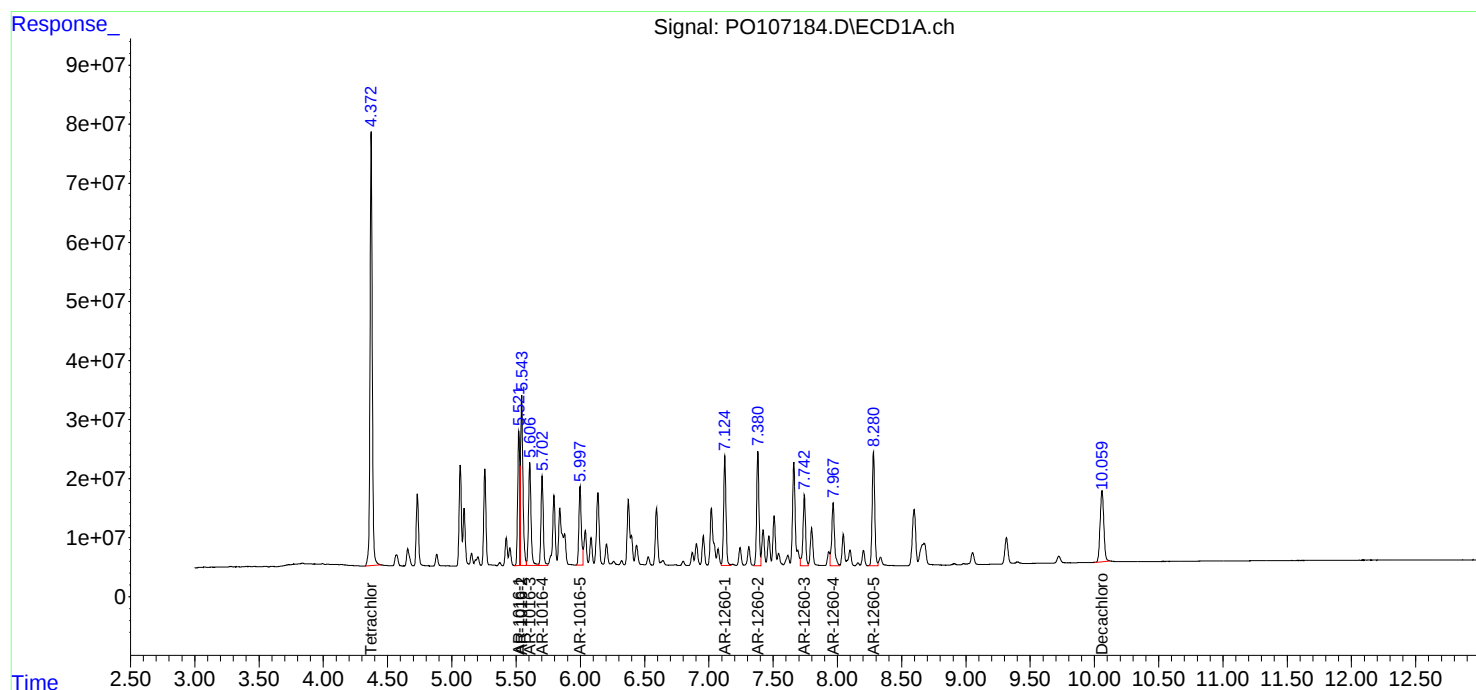

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 18:45
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:24:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.644	681.6E6	250.4E6	73.401	74.763
2) SA Decachlor...	10.059	8.639	182.0E6	205.9E6	72.917	73.948
Target Compounds						
3) L1 AR-1016-1	5.523	4.726	196.3E6	74951057	721.769	730.996
4) L1 AR-1016-2	5.545	4.745	287.3E6	107.1E6	721.992	741.869
5) L1 AR-1016-3	5.607	4.921	183.1E6	57833586	713.664	733.938
6) L1 AR-1016-4	5.704	4.962	145.4E6	47559823	716.317	724.912
7) L1 AR-1016-5	5.999	5.176	136.6E6	60728146	713.395	727.086
31) L7 AR-1260-1	7.125	6.207	184.9E6	114.0E6	713.367	735.005
32) L7 AR-1260-2	7.382	6.394	188.8E6	136.1E6	714.965	739.499
33) L7 AR-1260-3	7.743	6.548	128.7E6	127.7E6	708.958	742.087
34) L7 AR-1260-4	7.968	7.018	125.2E6	108.7E6	714.531	738.682
35) L7 AR-1260-5	8.281	7.258	205.2E6	254.8E6	725.060	756.650



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 18:45
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:24:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

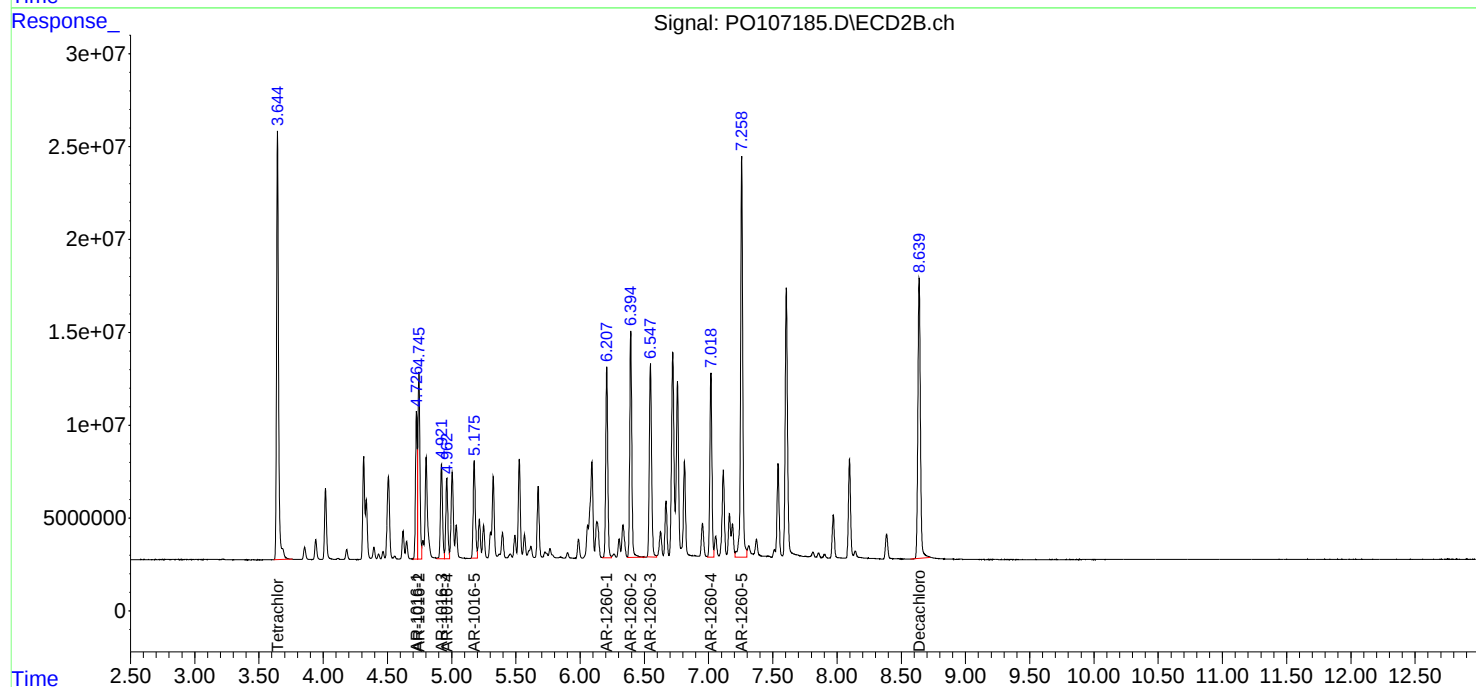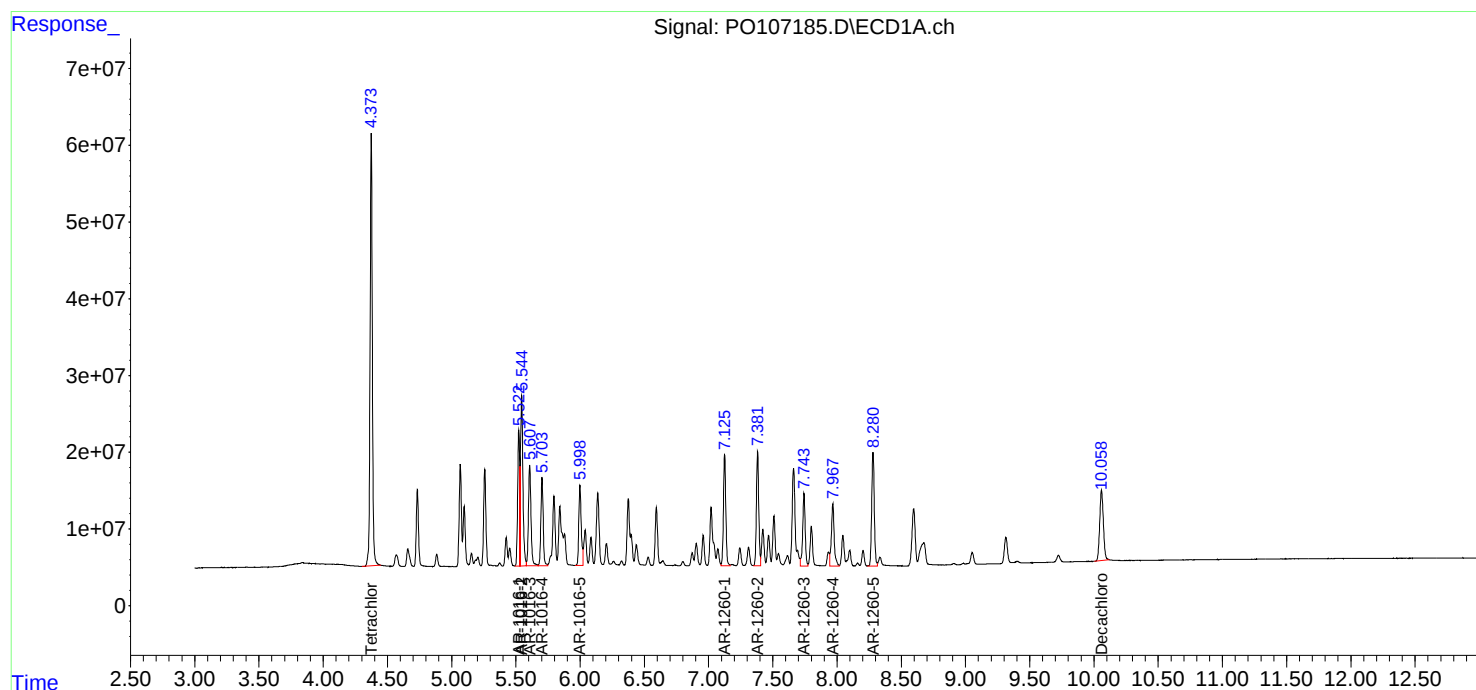

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 19:03
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:25:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.645	464.3E6	167.5E6	50.000	50.000
2) SA Decachlor...	10.058	8.639	124.8E6	139.2E6	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	5.523	4.726	136.0E6	51266401	500.000	500.000
4) L1 AR-1016-2	5.545	4.745	198.9E6	72157971	500.000	500.000
5) L1 AR-1016-3	5.607	4.921	128.3E6	39399514	500.000	500.000
6) L1 AR-1016-4	5.704	4.962	101.5E6	32803861	500.000	500.000
7) L1 AR-1016-5	5.999	5.176	95743965	41761334	500.000	500.000
31) L7 AR-1260-1	7.126	6.207	129.6E6	77565878	500.000	500.000
32) L7 AR-1260-2	7.382	6.394	132.0E6	92052145	500.000	500.000
33) L7 AR-1260-3	7.743	6.548	90745881	86054054	500.000	500.000
34) L7 AR-1260-4	7.968	7.018	87644858	73557583	500.000	500.000
35) L7 AR-1260-5	8.281	7.259	141.5E6	168.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 19:03
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:25:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

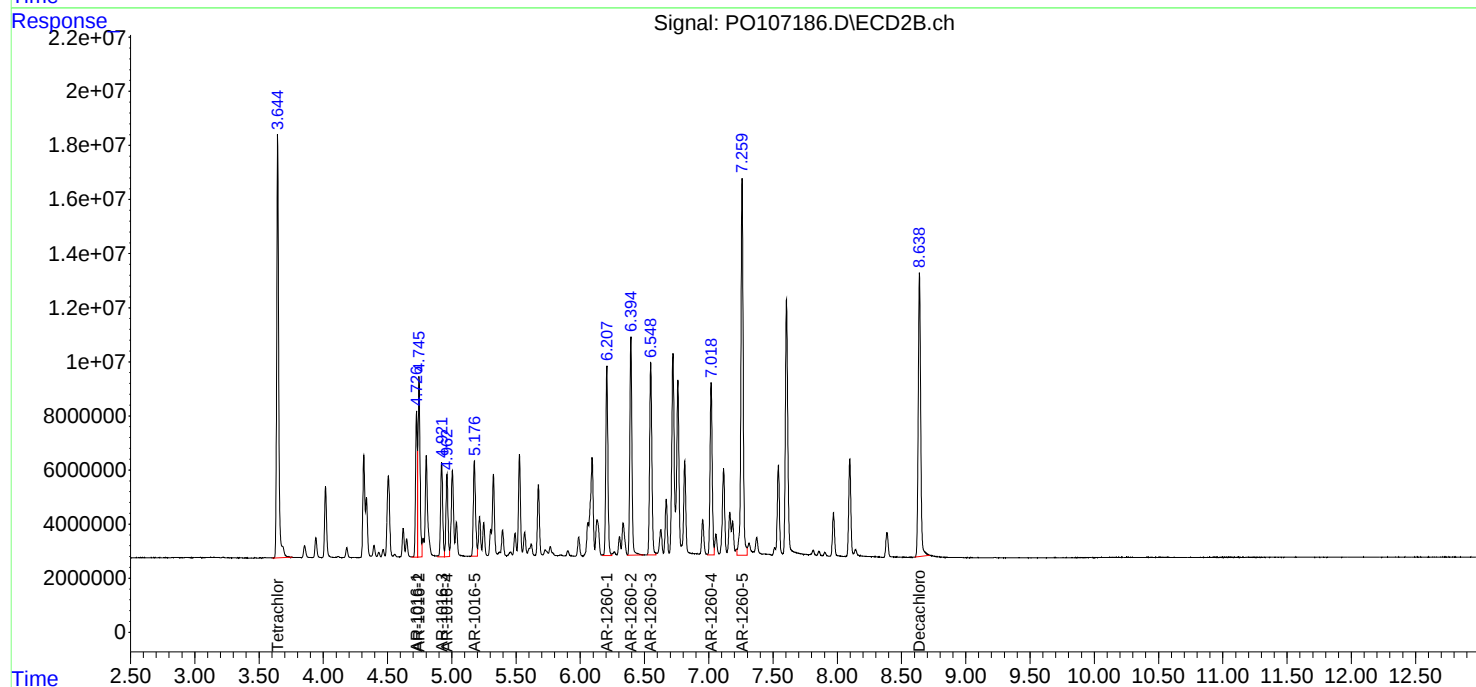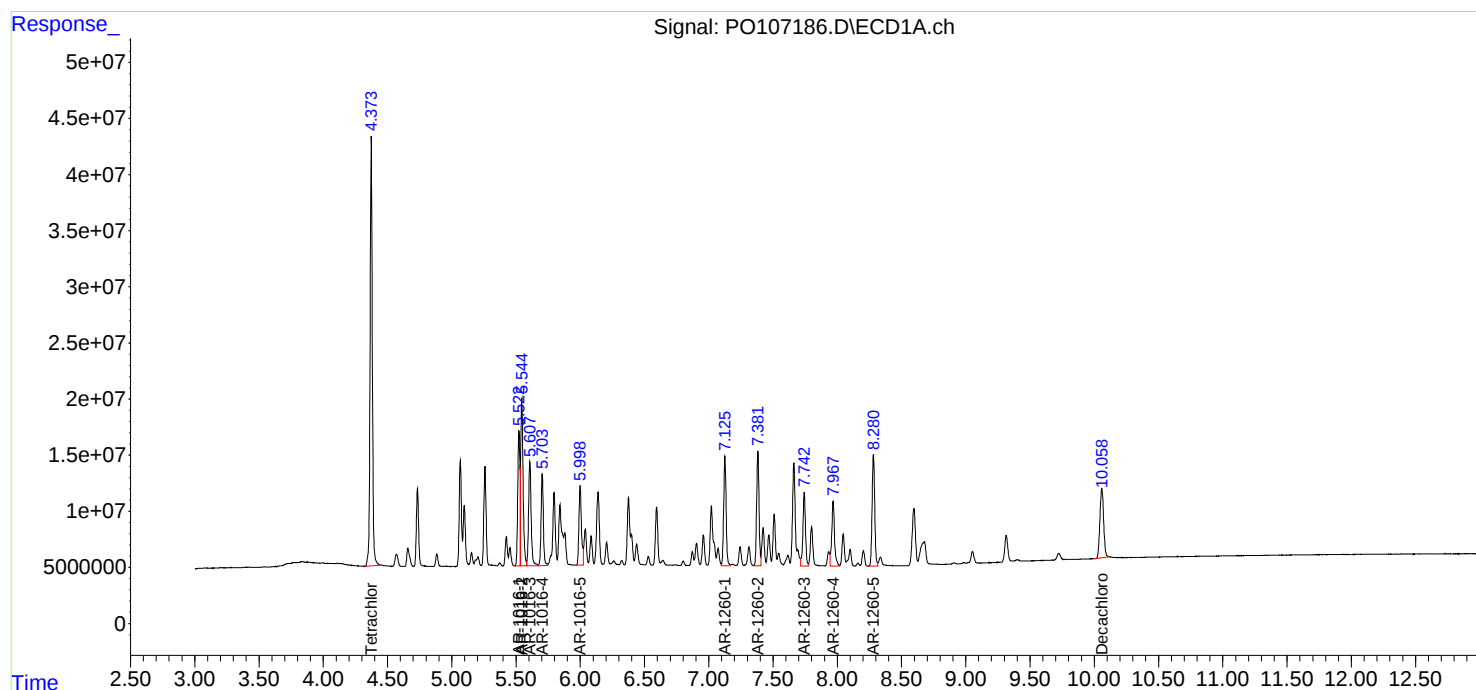

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 19:21
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:25:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	238.7E6	80767902	25.706	24.117
2) SA Decachlor...	10.059	8.640	65095686	71320716	26.075	25.611
Target Compounds						
3) L1 AR-1016-1	5.522	4.727	72779622	26650346	267.632	259.920
4) L1 AR-1016-2	5.544	4.746	104.8E6	36719388	263.313	254.438
5) L1 AR-1016-3	5.606	4.921	69101416	20445837	269.322	259.468
6) L1 AR-1016-4	5.704	4.962	53770388	17391092	264.926	265.077
7) L1 AR-1016-5	5.998	5.176	50878723	21735247	265.702	260.232
31) L7 AR-1260-1	7.124	6.207	69305169	40485591	267.426	260.976
32) L7 AR-1260-2	7.381	6.394	71054115	47434059	269.059	257.648
33) L7 AR-1260-3	7.743	6.548	48784517	43997886	268.797	255.641
34) L7 AR-1260-4	7.966	7.018	46895508	37628553	267.531	255.776
35) L7 AR-1260-5	8.281	7.259	74817853	85097988	264.341	252.669



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 19:21
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:25:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

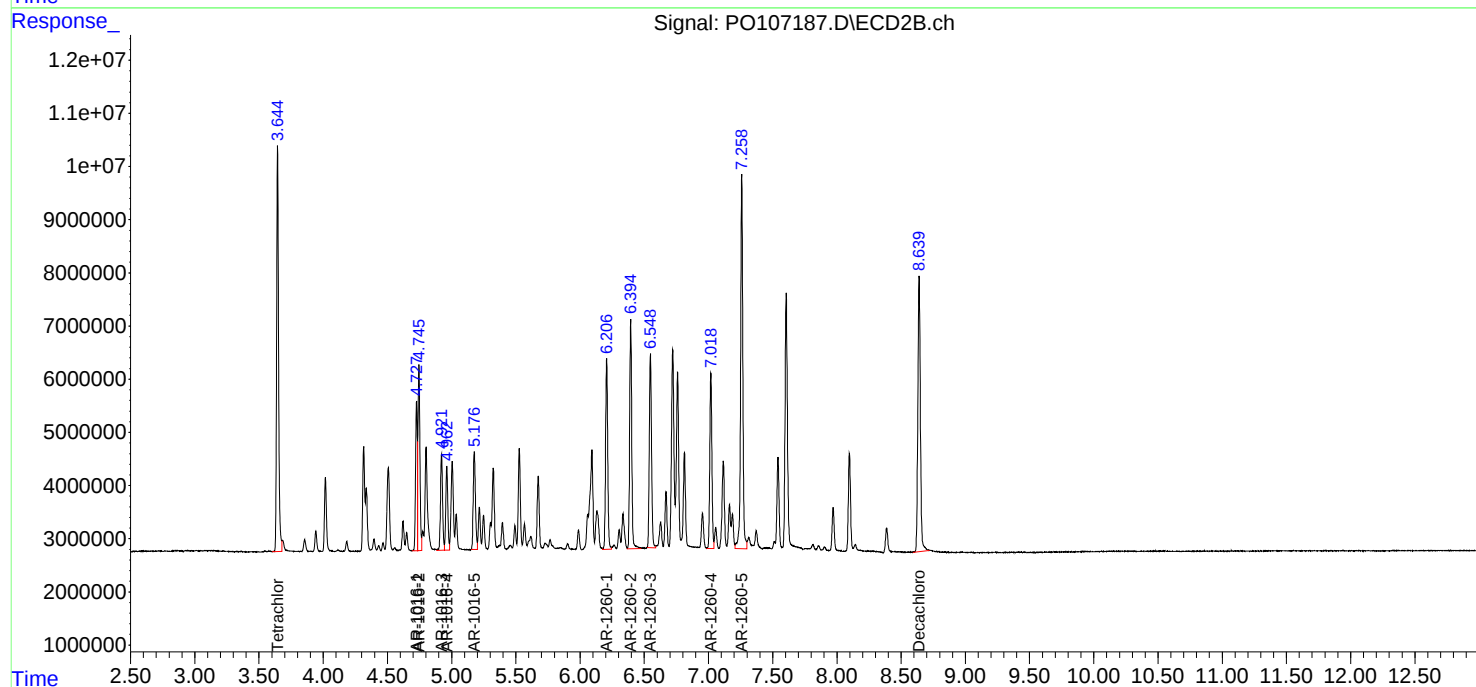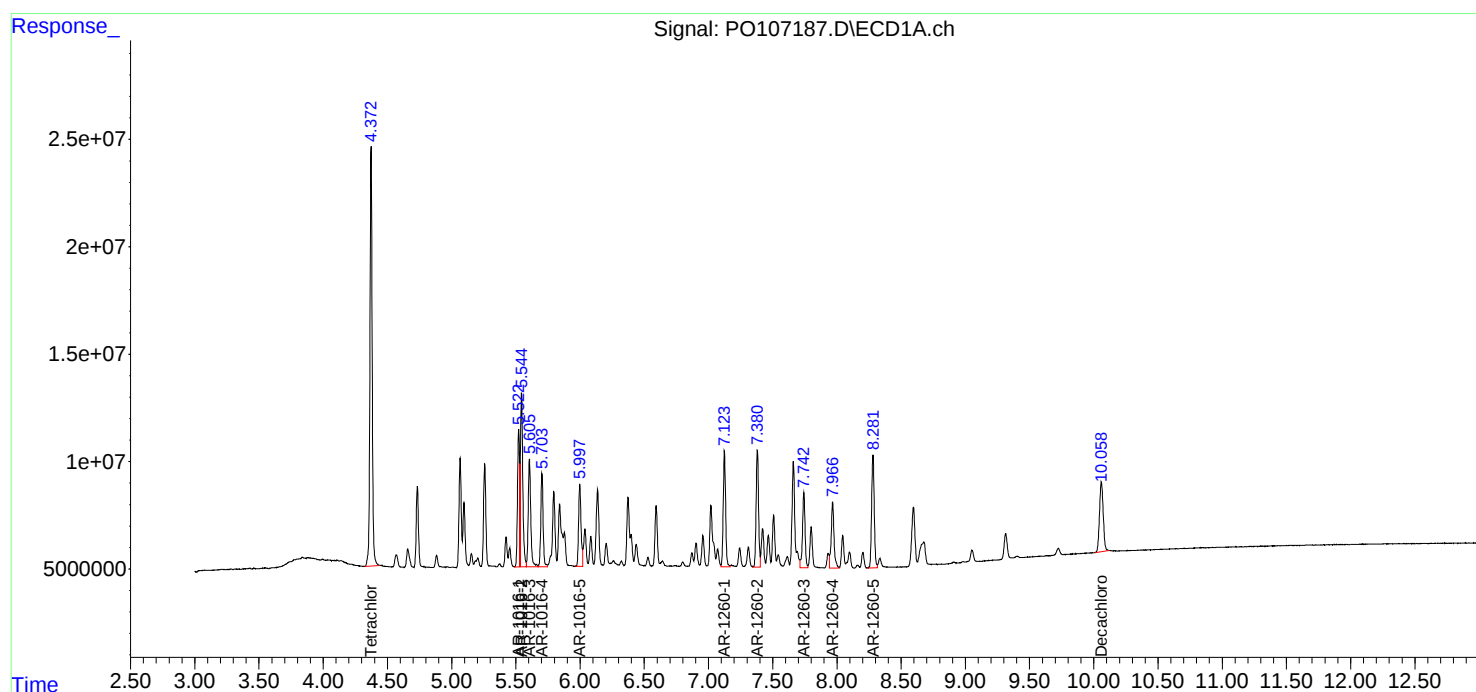

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 19:39
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/16/2024
 Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:26:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:21:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.644	43726312	14311070	4.709	4.273
2) SA Decachlor...	10.060	8.639	11883434	12970025	4.760	4.657m
Target Compounds						
3) L1 AR-1016-1	5.523	4.727	13611471	5437001	50.053	53.027
4) L1 AR-1016-2	5.544	4.745	20533666	6518003	51.607	45.165
5) L1 AR-1016-3	5.607	4.922	12202124	4010763	47.558	50.899
6) L1 AR-1016-4	5.704	4.963	8277151	3521180	40.781	53.670 #
7) L1 AR-1016-5	5.999	5.176	7989825	4017833	41.725	48.105
31) L7 AR-1260-1	7.125	6.207	13579378	7810910	52.398	50.350m
32) L7 AR-1260-2	7.380	6.395	13632543	7572896	51.622m	41.134m
33) L7 AR-1260-3	7.743	6.548	9159133	7594706	50.466m	44.128m
34) L7 AR-1260-4	7.967	7.019	9276106	6862107	52.919	46.644m
35) L7 AR-1260-5	8.280	7.258	14867575	14474674	52.529m	42.977m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 19:39
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:26:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:21:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

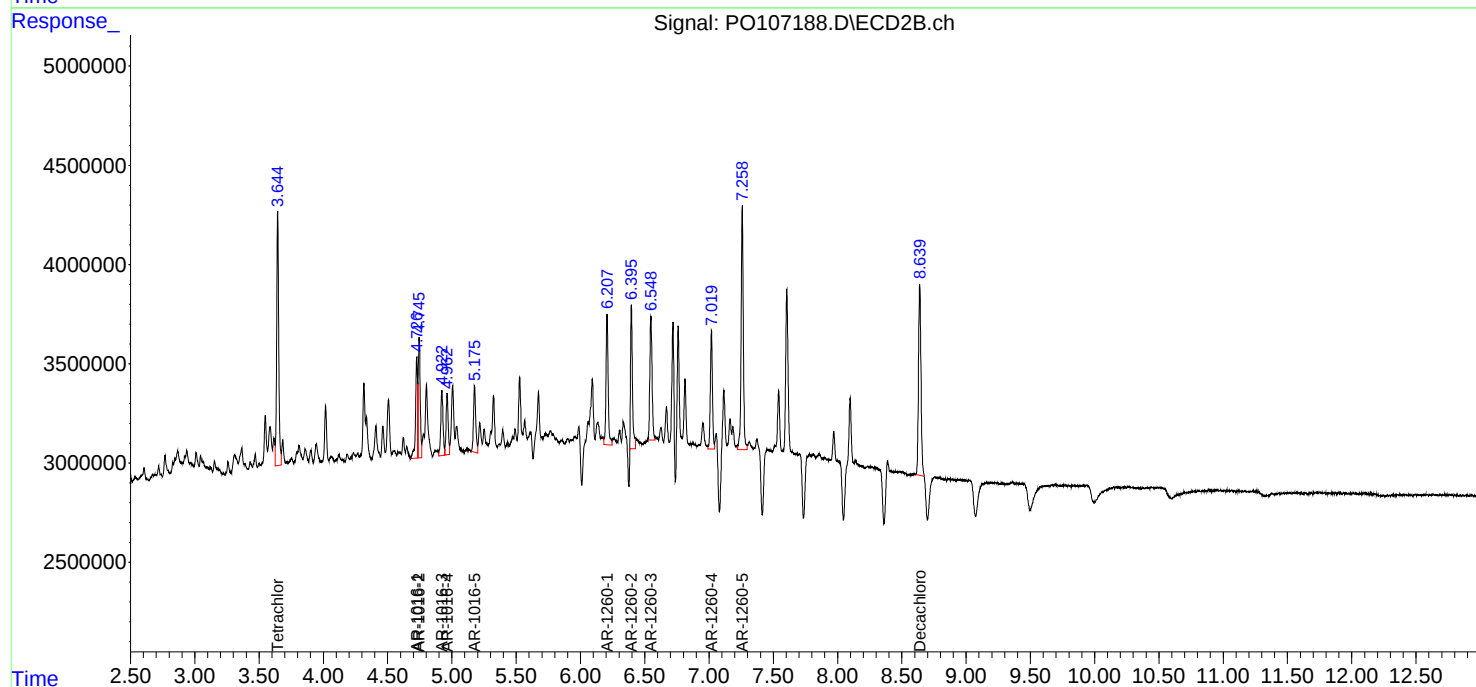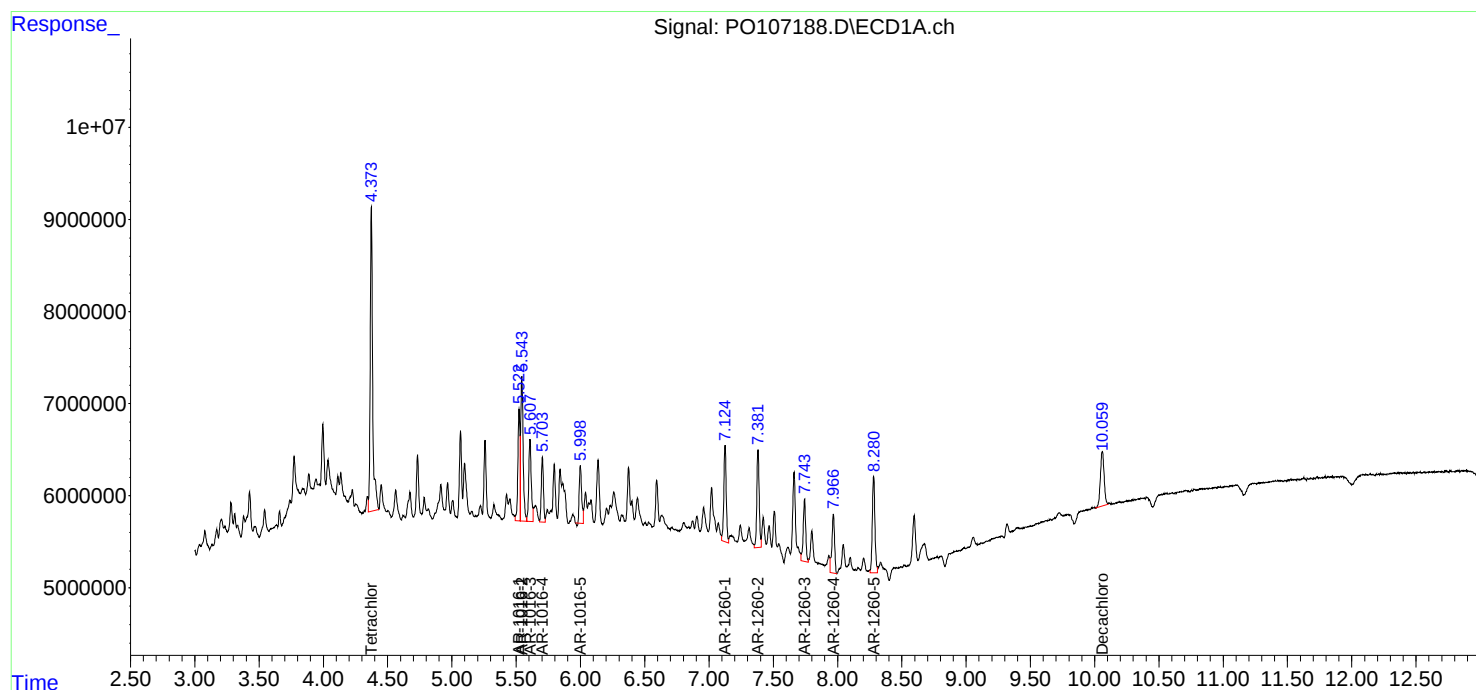

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 19:57
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:41:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:40:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	449.1E6	154.1E6	50.000	50.000
2) SA Decachlor...	10.060	8.639	121.6E6	134.8E6	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.573	3.856	55004944	17447760	500.000	500.000
9) L2 AR-1221-2	4.658	3.942	39418330	13312448	500.000	500.000
10) L2 AR-1221-3	4.733	4.018	117.0E6	40609299	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 19:57
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:41:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:40:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

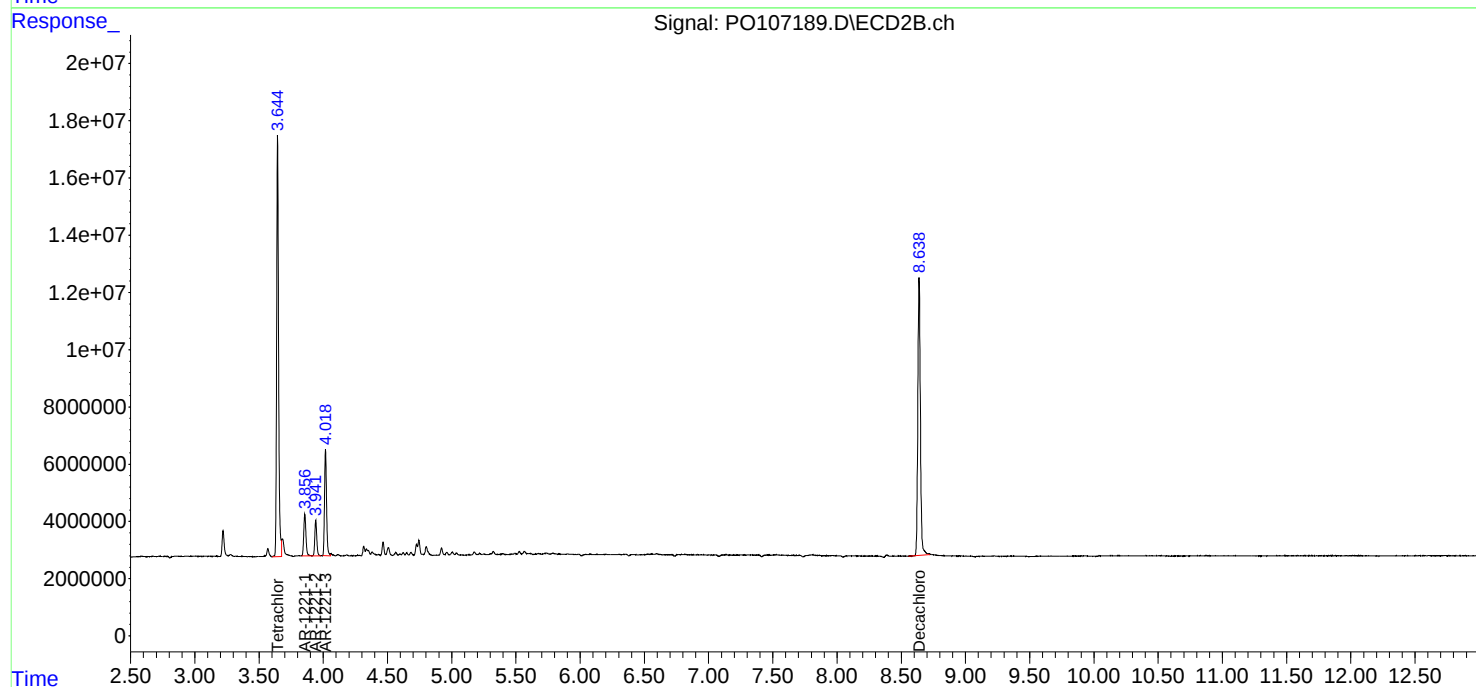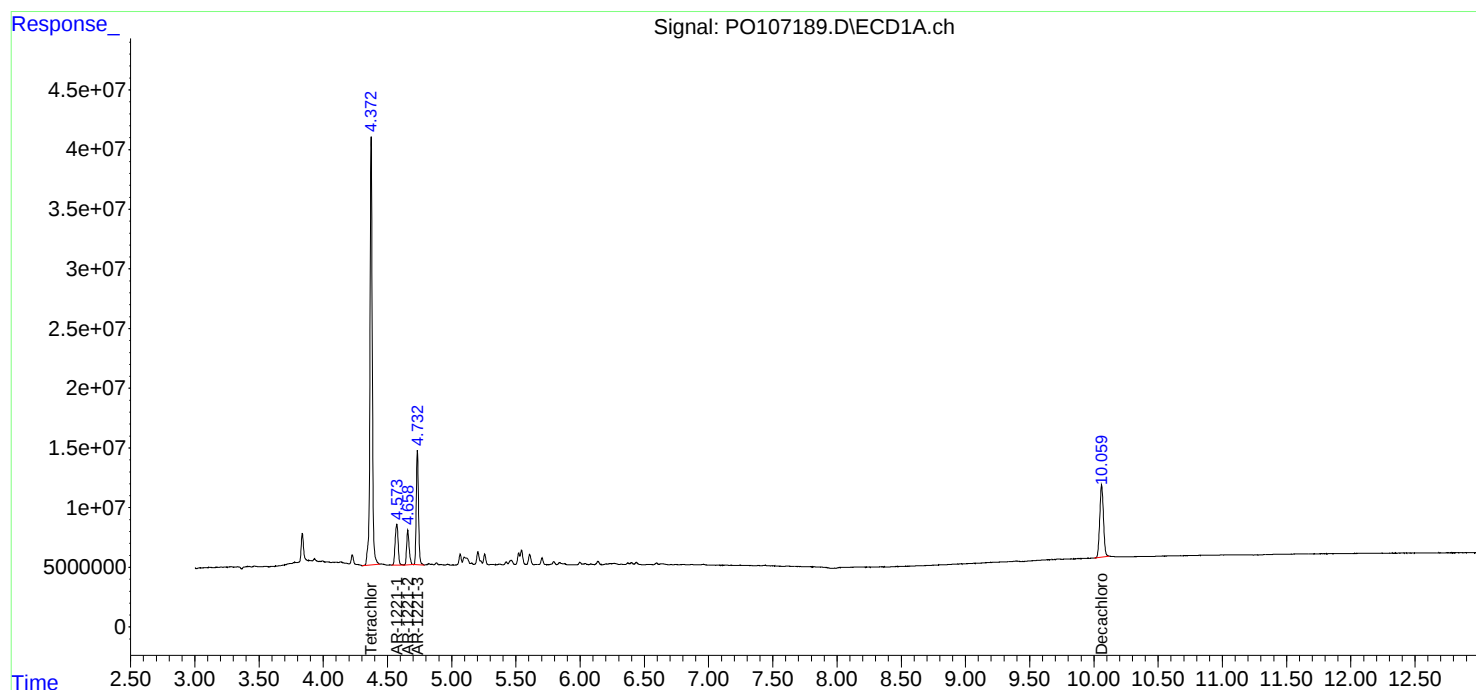

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 20:15
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:46:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:45:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	454.2E6	157.5E6	50.000	50.000
2) SA Decachlor...	10.059	8.639	121.6E6	135.6E6	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.733	4.017	97921824	33663502	500.000	500.000
12) L3 AR-1232-2	5.258	4.745	51512576	31602645	500.000	500.000
13) L3 AR-1232-3	5.544	4.921	89500289	17237464	500.000	500.000
14) L3 AR-1232-4	5.704	5.004	45082743	15732978	500.000	500.000
15) L3 AR-1232-5	5.796	5.176	32951614	16541659	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 20:15
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:46:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:45:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

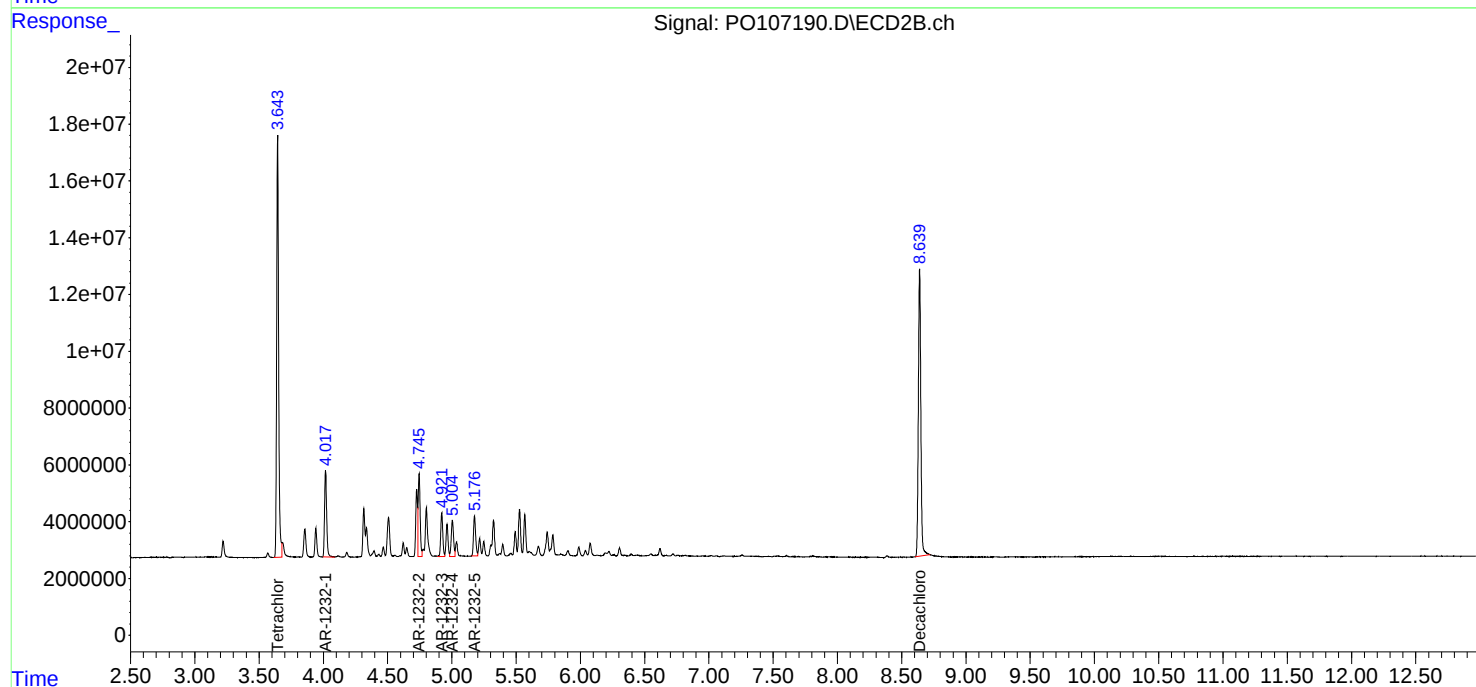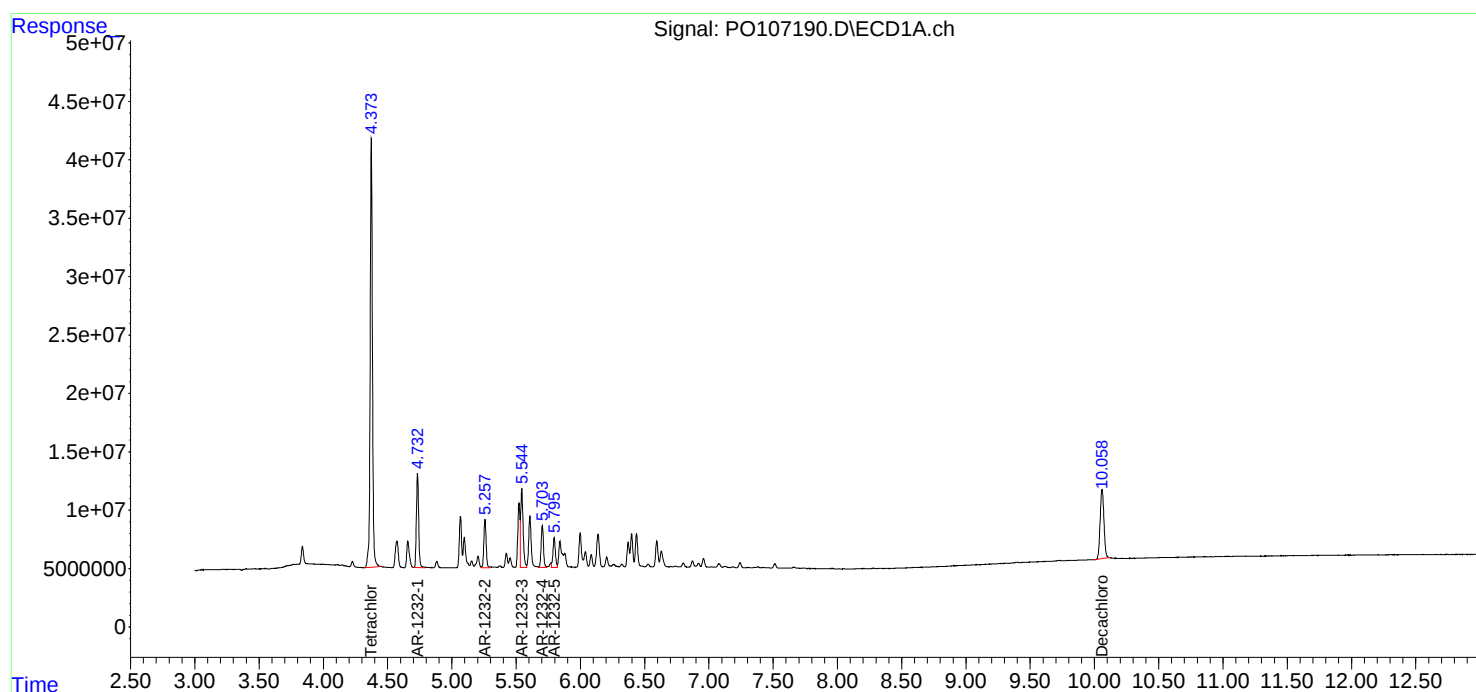

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 20:34
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:49:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	886.0E6	331.6E6	96.865	99.238
2) SA Decachlor...	10.061	8.638	233.9E6	268.7E6	93.851	97.198
Target Compounds						
16) L4 AR-1242-1	5.522	4.726	207.9E6	80390662	935.818	957.741
17) L4 AR-1242-2	5.545	4.745	302.4E6	114.5E6	934.753	972.360
18) L4 AR-1242-3	5.607	4.921	191.9E6	61817452	915.447	959.943
19) L4 AR-1242-4	5.704	5.004	150.4E6	60582529	924.137	940.948
20) L4 AR-1242-5	6.437	5.526	141.0E6	73763103	917.497	955.284



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 20:34
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:49:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

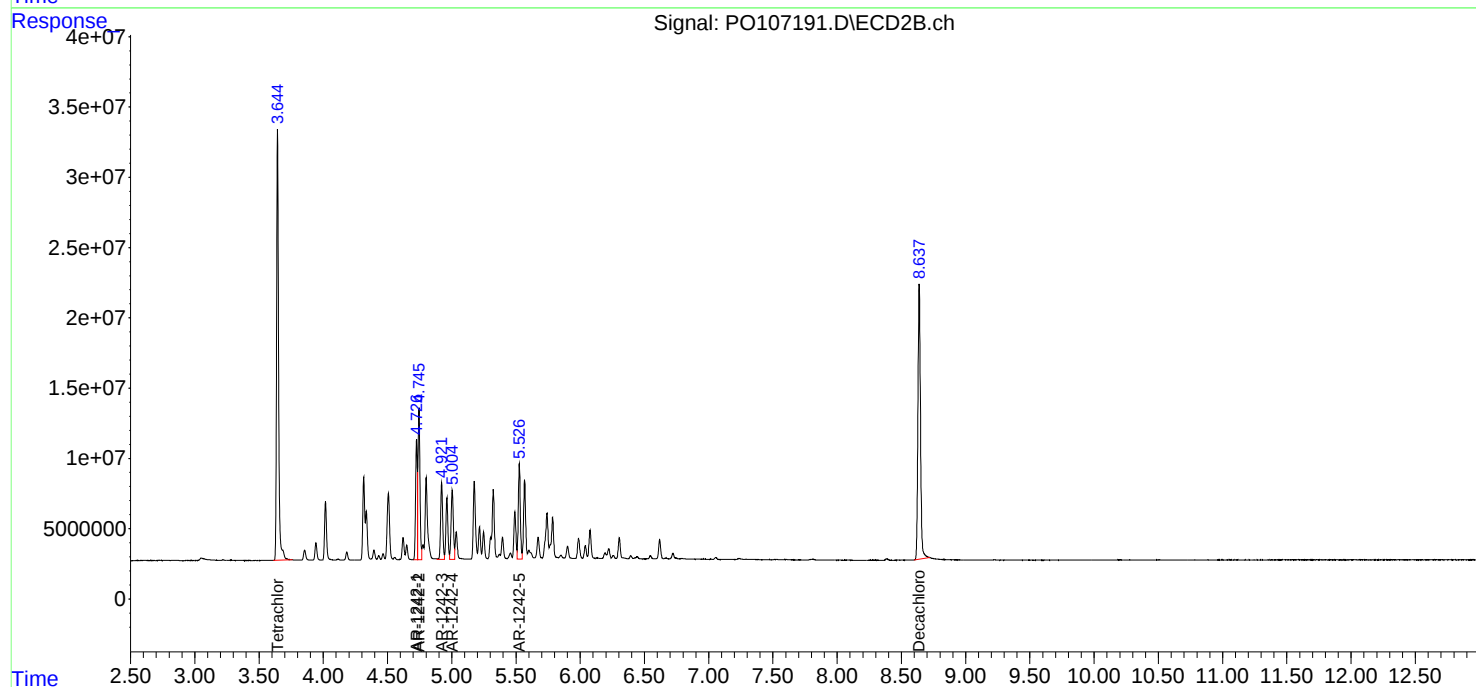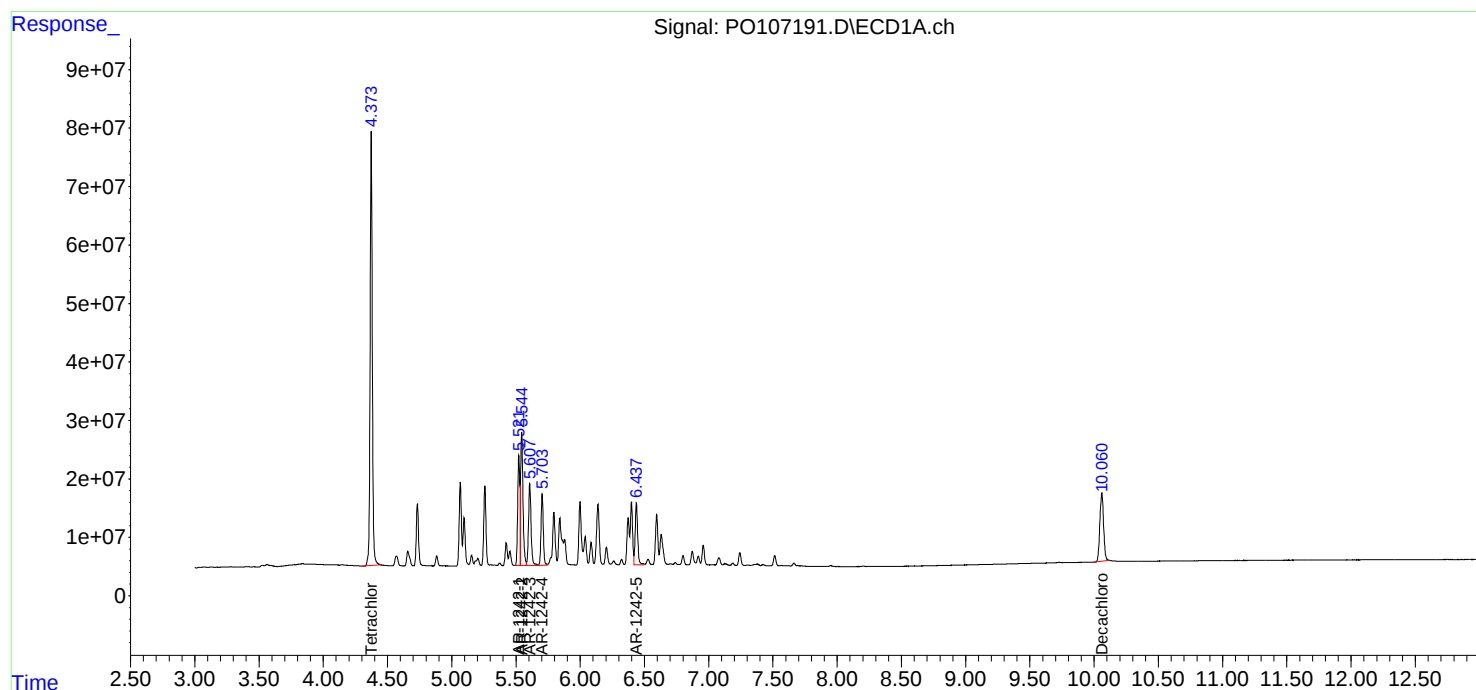

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 20:52
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:49:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	648.9E6	243.1E6	70.941	72.772
2) SA Decachlor...	10.059	8.639	182.1E6	207.3E6	73.046	74.999
Target Compounds						
16) L4 AR-1242-1	5.521	4.726	154.2E6	60335620	693.850	718.814
17) L4 AR-1242-2	5.544	4.746	225.0E6	83449803	695.293	708.752
18) L4 AR-1242-3	5.606	4.922	144.9E6	45346429	691.114	704.170
19) L4 AR-1242-4	5.703	5.005	109.0E6	45477164	669.566	706.336
20) L4 AR-1242-5	6.437	5.526	107.6E6	56756574	699.831	735.037



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 20:52
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:49:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

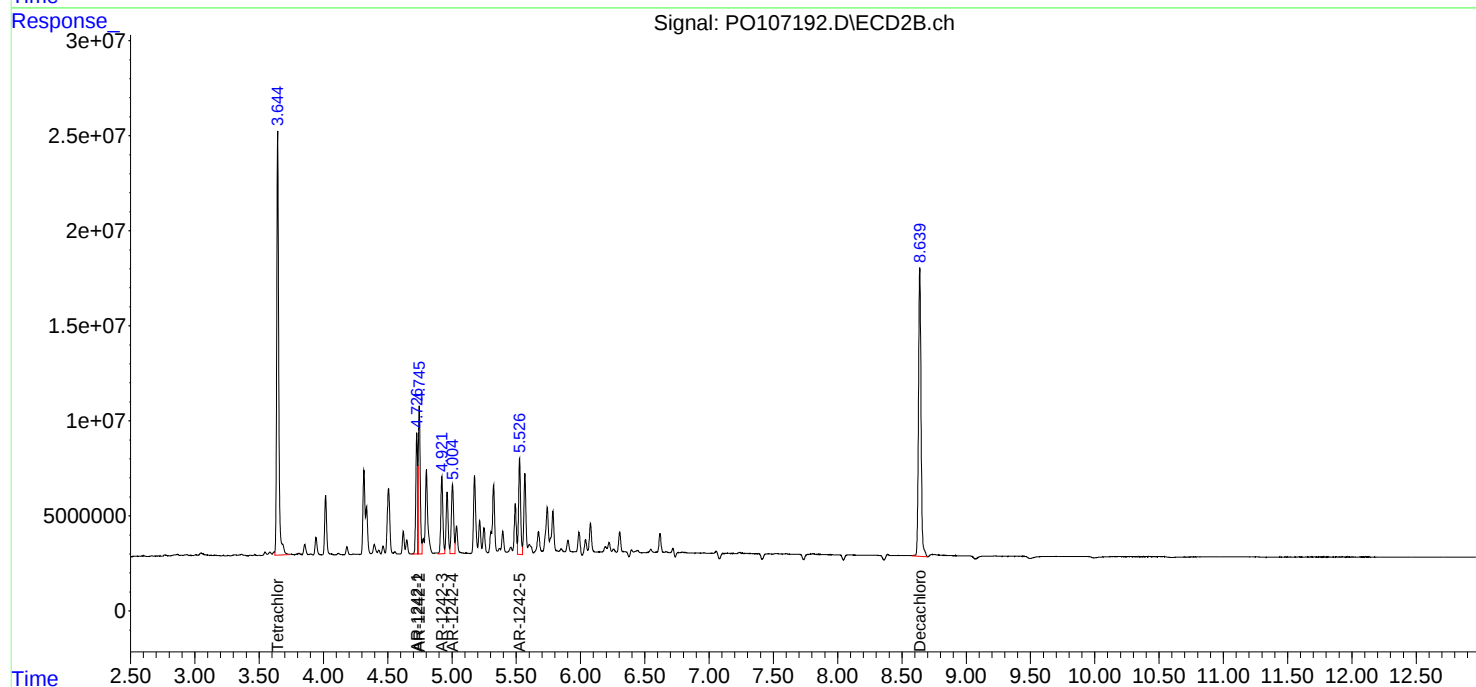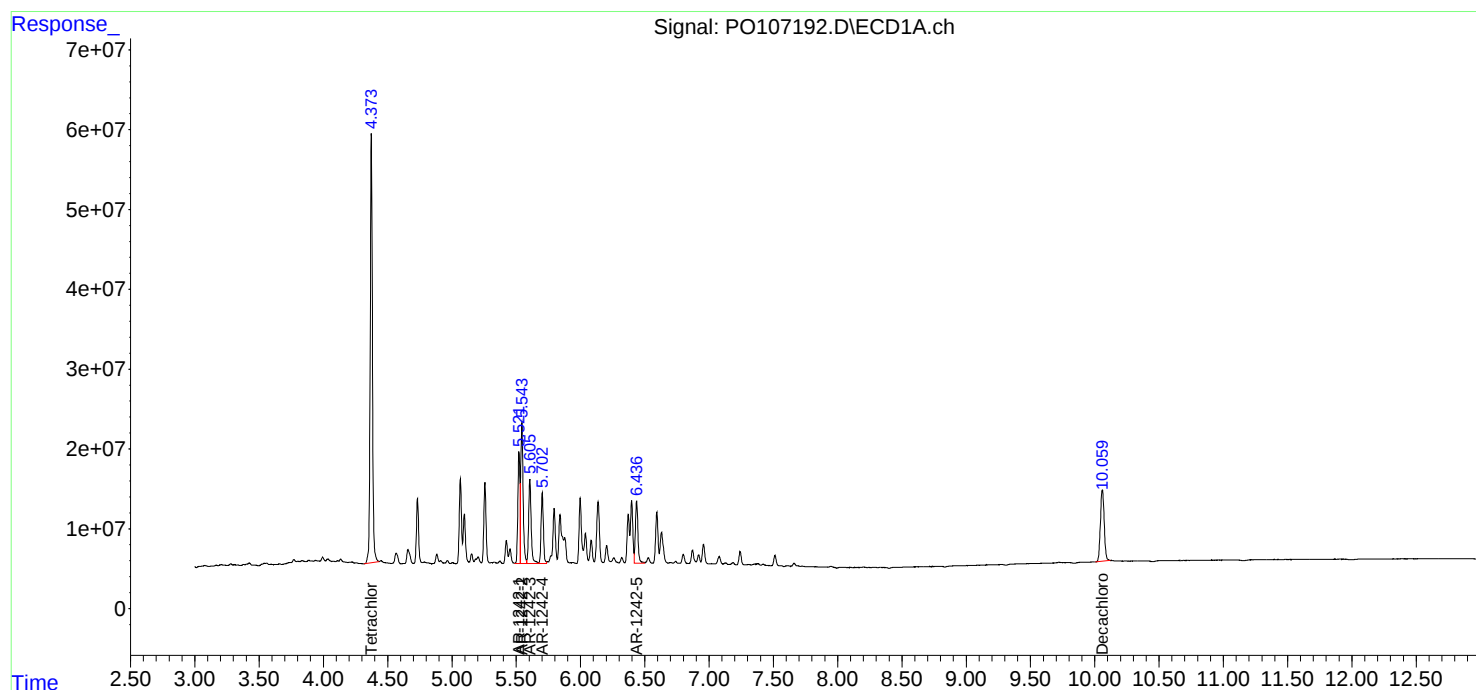

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 21:10
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:50:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	457.3E6	167.1E6	50.000	50.000
2) SA Decachlor...	10.057	8.639	124.6E6	138.2E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	5.522	4.726	111.1E6	41968881	500.000	500.000
17) L4 AR-1242-2	5.544	4.745	161.8E6	58870958	500.000	500.000
18) L4 AR-1242-3	5.607	4.922	104.8E6	32198496	500.000	500.000
19) L4 AR-1242-4	5.703	5.004	81398754	32192297	500.000	500.000
20) L4 AR-1242-5	6.437	5.526	76844549	38607958	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 21:10
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:50:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

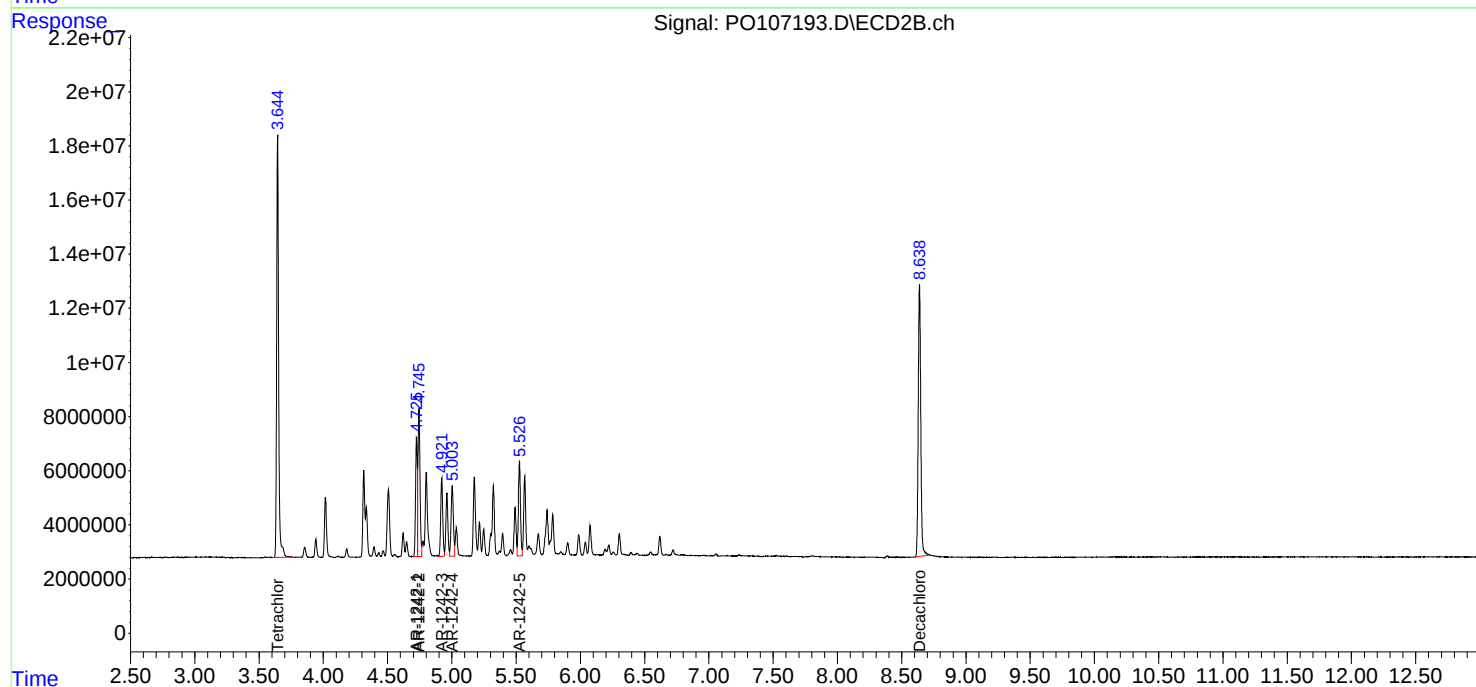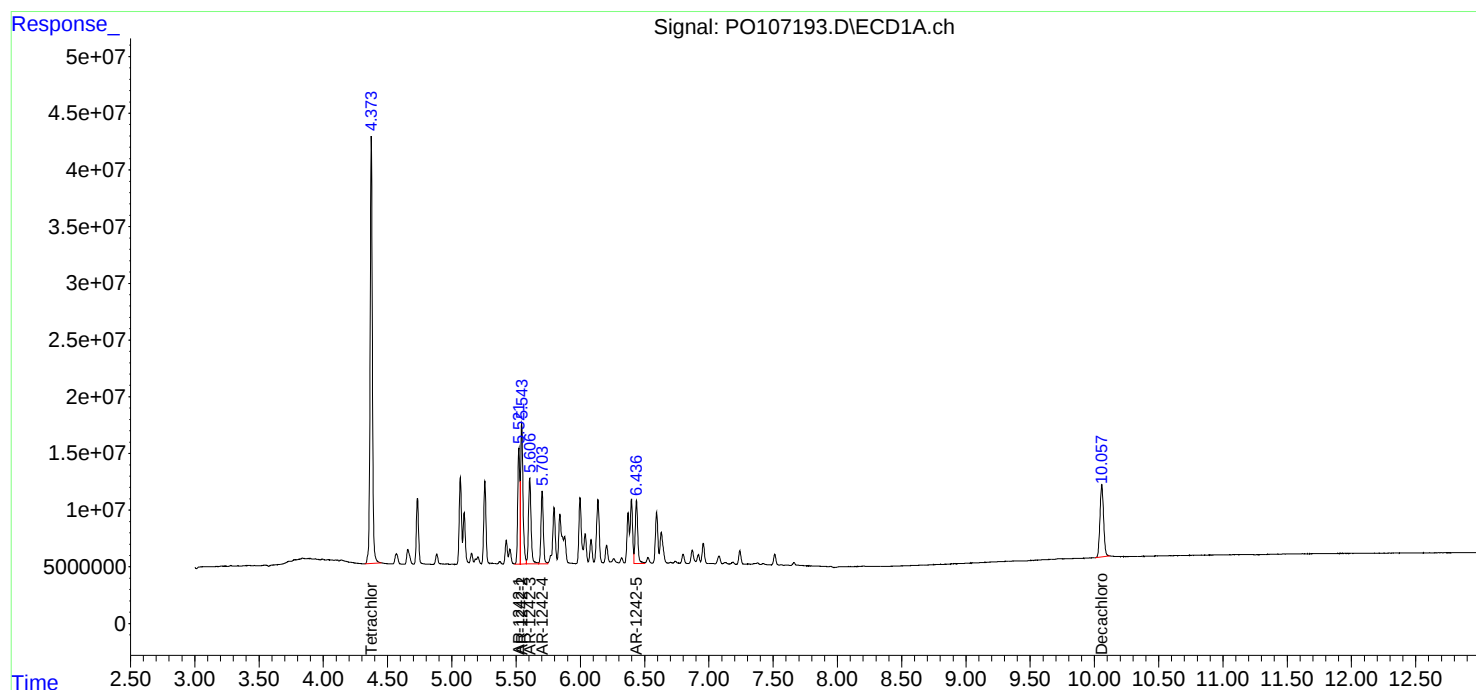

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 21:28
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:50:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	237.6E6	83389360	25.977	24.958
2) SA Decachlor...	10.057	8.639	63795685	69963548	25.593	25.308
Target Compounds						
16) L4 AR-1242-1	5.522	4.727	59739114	21816724	268.842	259.915
17) L4 AR-1242-2	5.544	4.746	85701102	30166778	264.877	256.211
18) L4 AR-1242-3	5.607	4.922	56076682	16716467	267.493	259.585
19) L4 AR-1242-4	5.703	5.005	43283991	17011315	265.876	264.214
20) L4 AR-1242-5	6.437	5.526	41155754	20184132	267.786	261.399



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 21:28
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:50:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

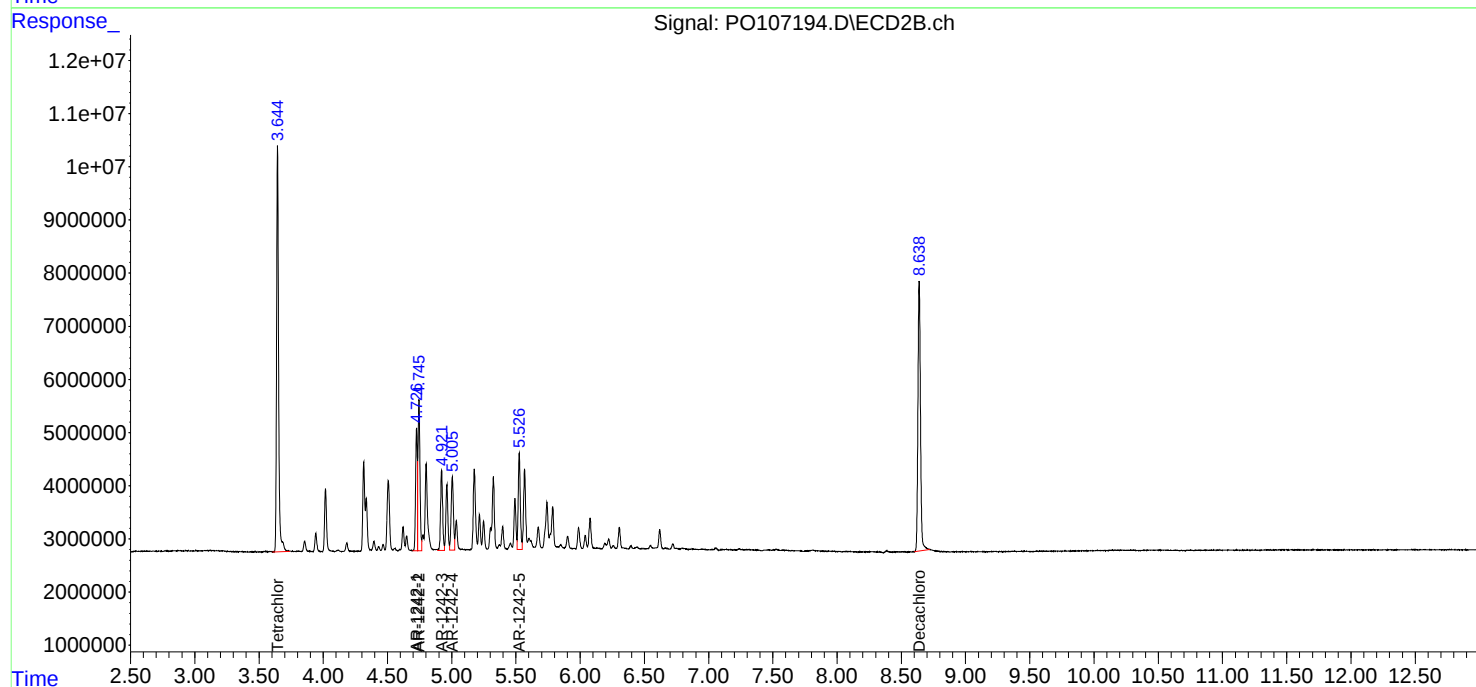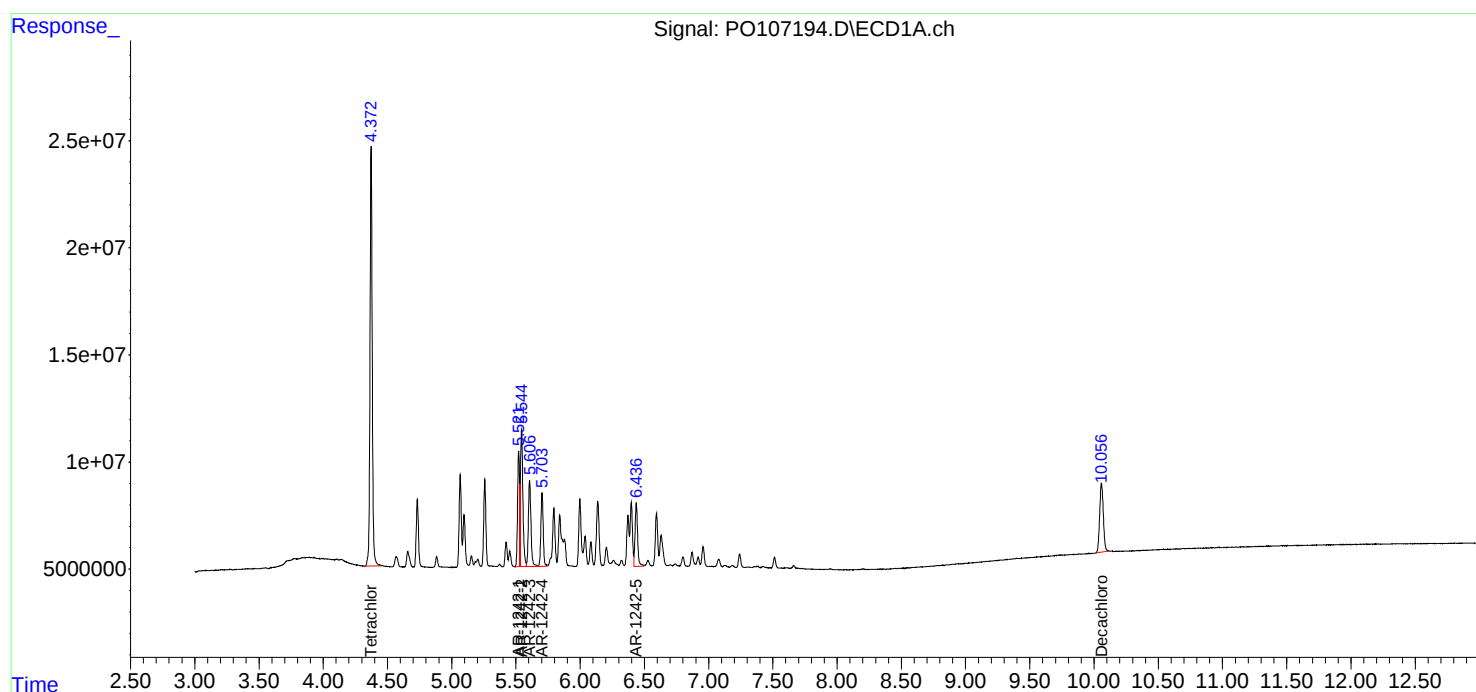

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 21:46
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:51:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 01:48:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	45874144	14600377	5.015	4.370
2) SA Decachlor...	10.055	8.638	12132051	13326327	4.867	4.821
Target Compounds						
16) L4 AR-1242-1	5.521	4.726	12176144	4333712	54.796	51.630
17) L4 AR-1242-2	5.544	4.745	17442944	5701582	53.911	48.424
18) L4 AR-1242-3	5.606	4.921	11292382	3181204	53.866	49.400
19) L4 AR-1242-4	5.703	5.004	8415437	3329911	51.693	51.719
20) L4 AR-1242-5	6.437	5.526	8983989	4011331	58.456	51.950



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 21:46
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:51:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 01:48:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

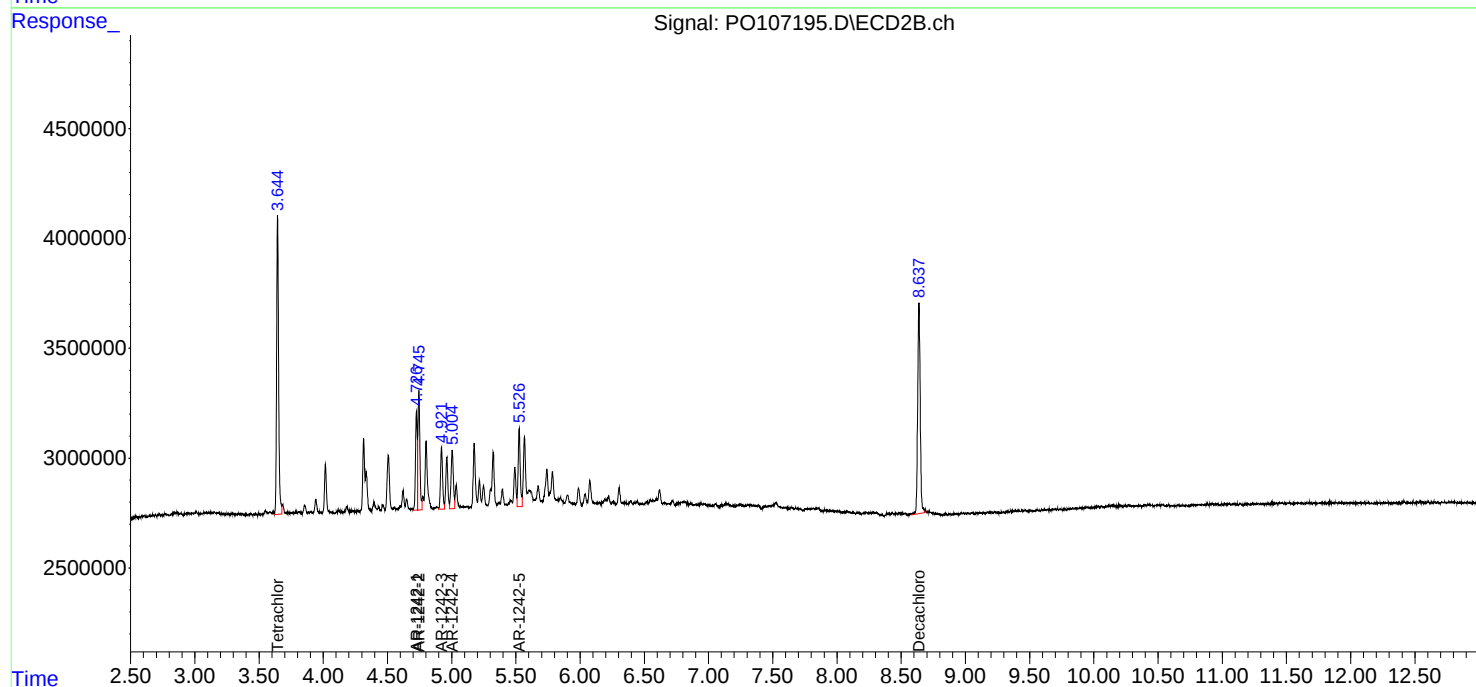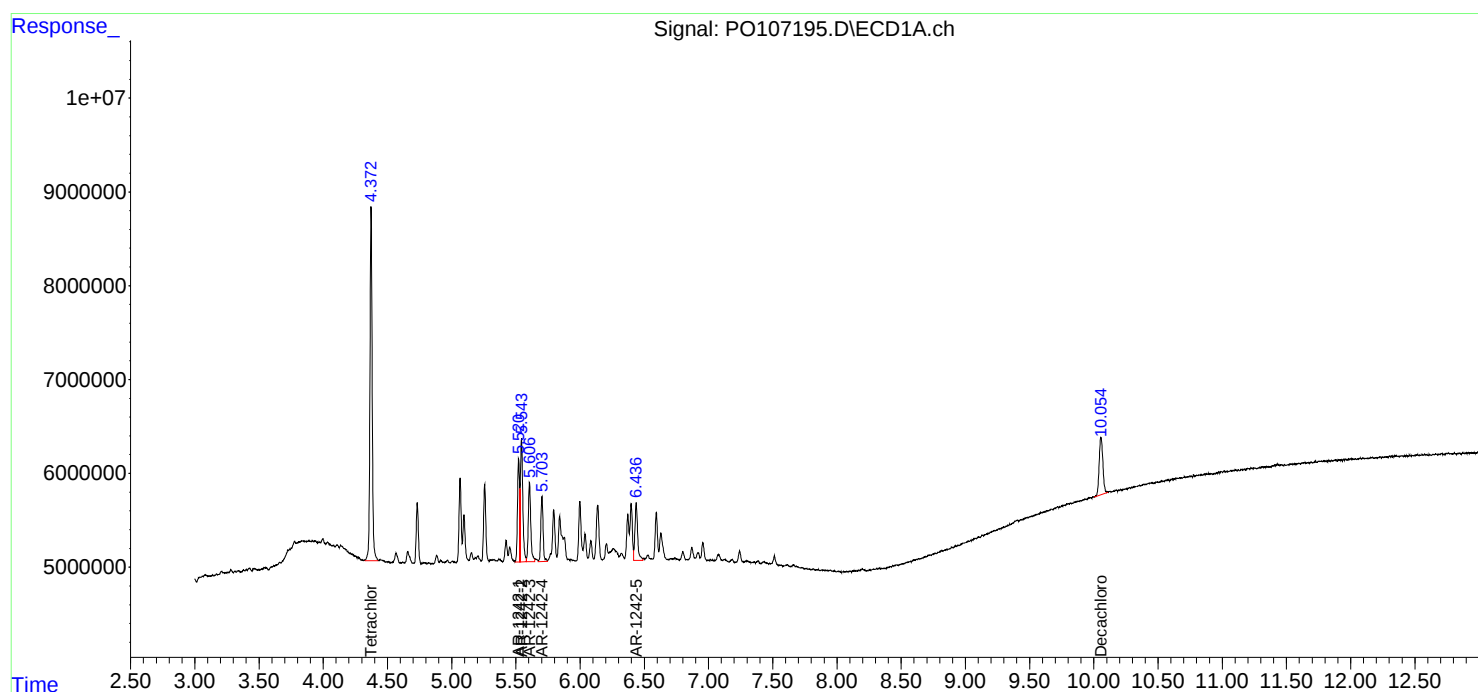

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 22:04
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:08:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	871.9E6	327.8E6	93.167	95.697
2) SA Decachlor...	10.057	8.638	234.0E6	266.9E6	93.438	95.612
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	155.9E6	60218805	889.958	928.169
22) L5 AR-1248-2	5.795	4.962	222.8E6	85173308	878.597	915.232
23) L5 AR-1248-3	5.997	5.004	231.9E6	89257070	892.951	916.605
24) L5 AR-1248-4	6.398	5.176	237.2E6	105.9E6	910.480	923.092
25) L5 AR-1248-5	6.437	5.567	236.3E6	102.8E6	906.188	936.492



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 22:04
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:08:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

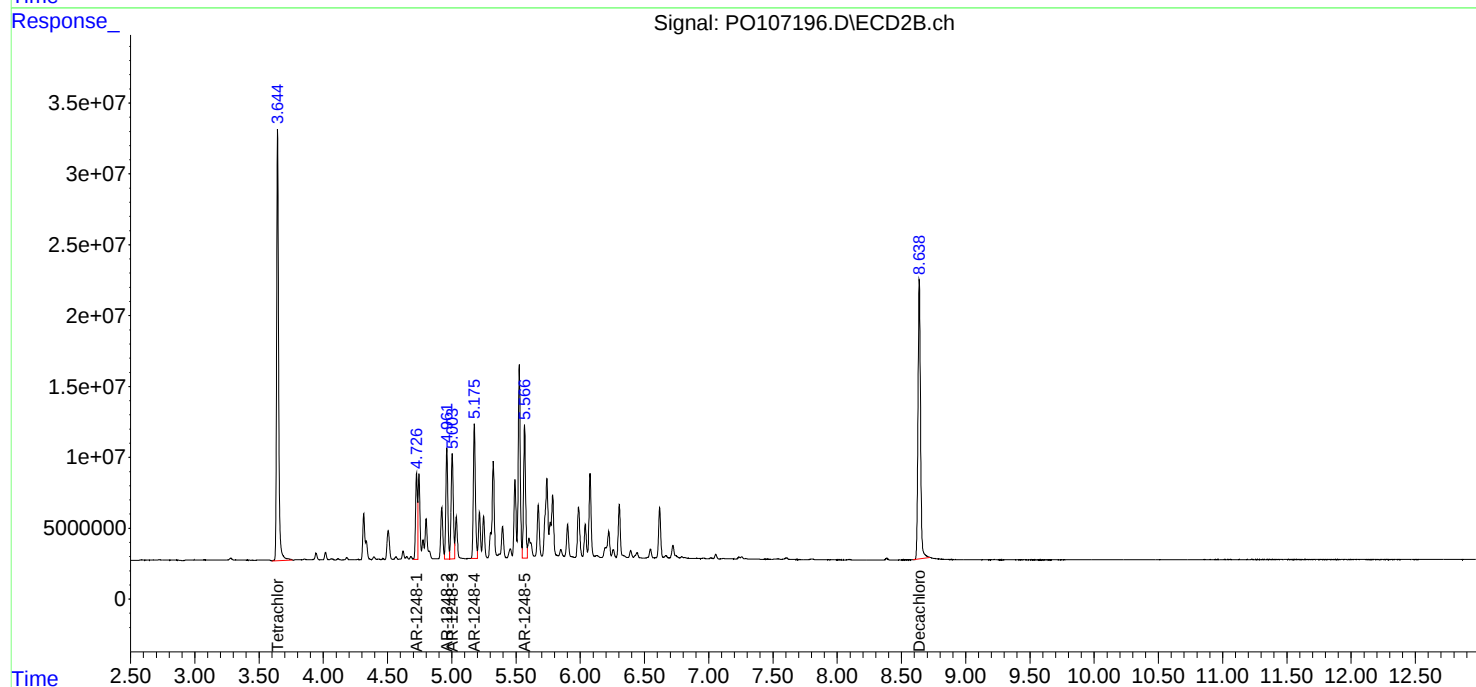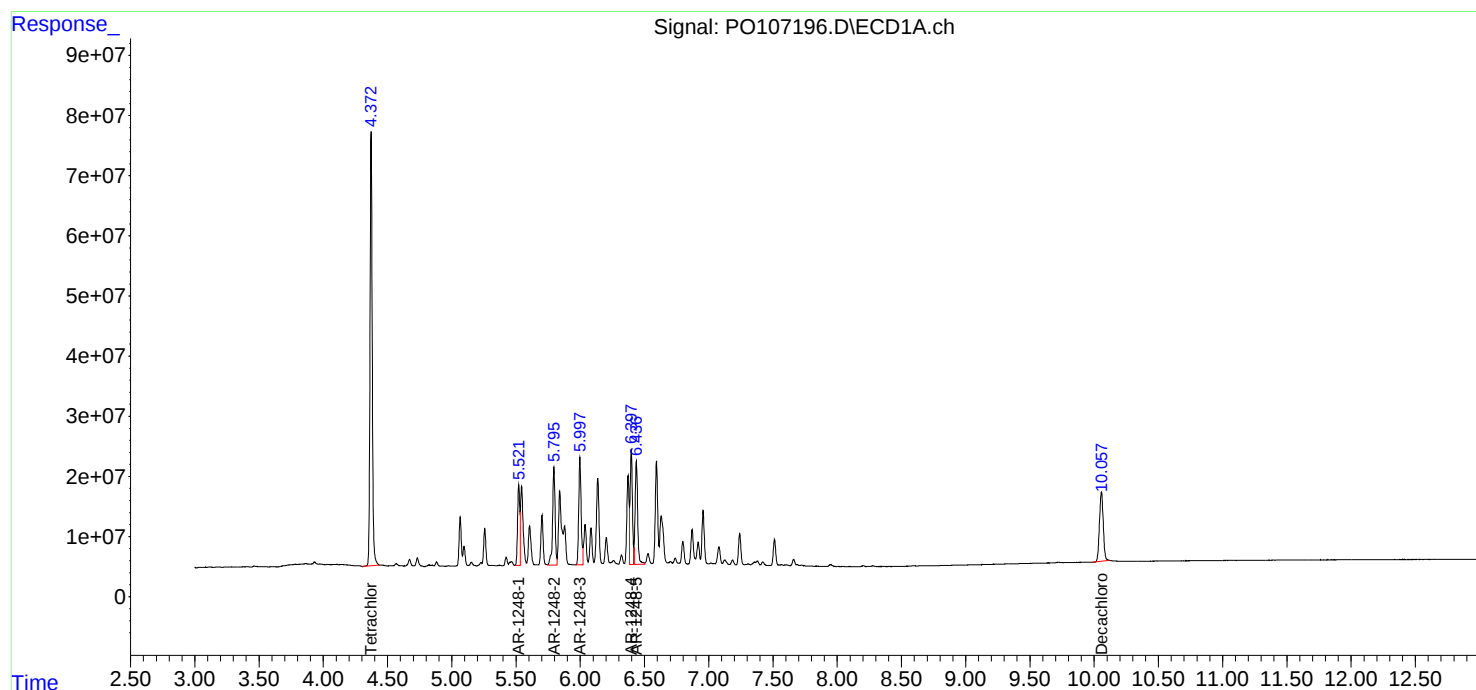

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 22:22
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:09:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	684.0E6	254.2E6	73.085	74.199
2) SA Decachlor...	10.056	8.638	177.9E6	201.2E6	71.030	72.062
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	123.6E6	47278639	705.517	728.719
22) L5 AR-1248-2	5.795	4.962	178.7E6	66831271	704.358	718.137
23) L5 AR-1248-3	5.997	5.004	184.7E6	69919958	711.094	718.027
24) L5 AR-1248-4	6.398	5.176	185.0E6	82899838	709.988	722.373
25) L5 AR-1248-5	6.437	5.568	184.9E6	79019739	709.319	719.661



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 22:22
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:09:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

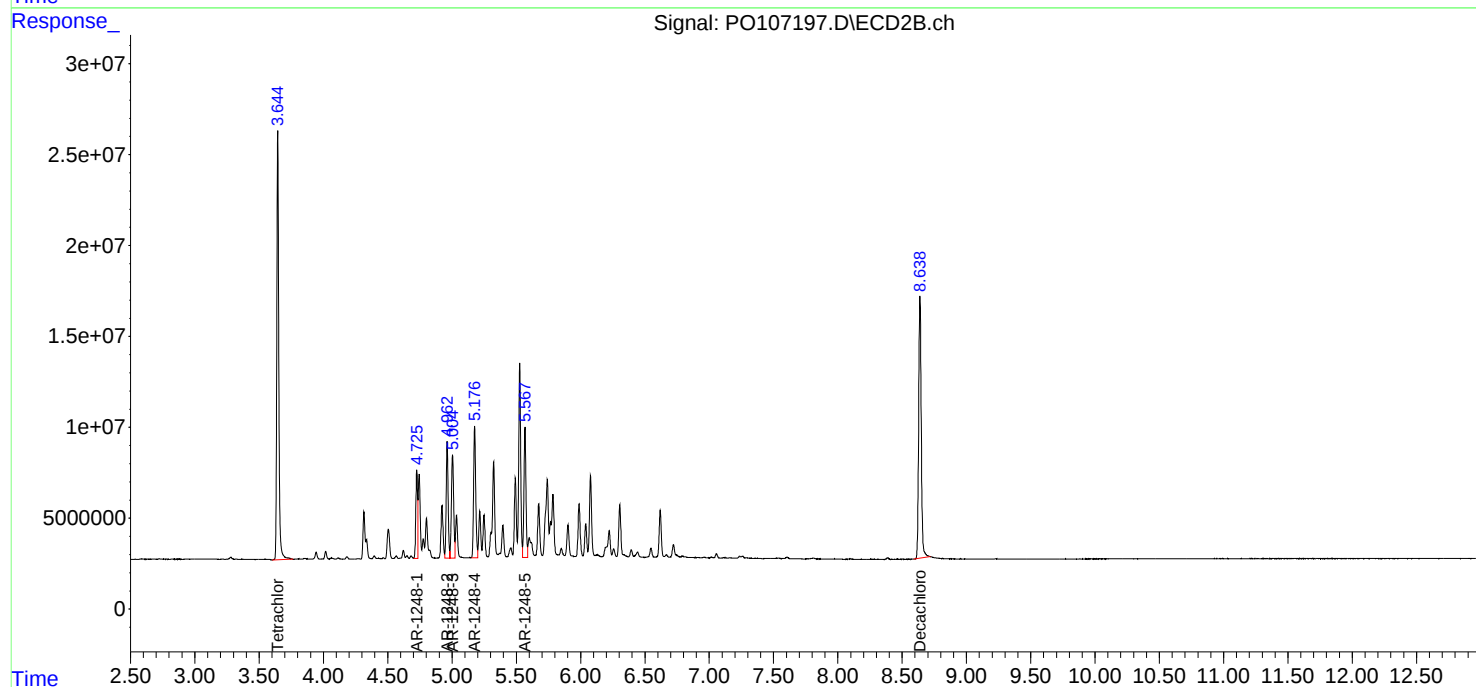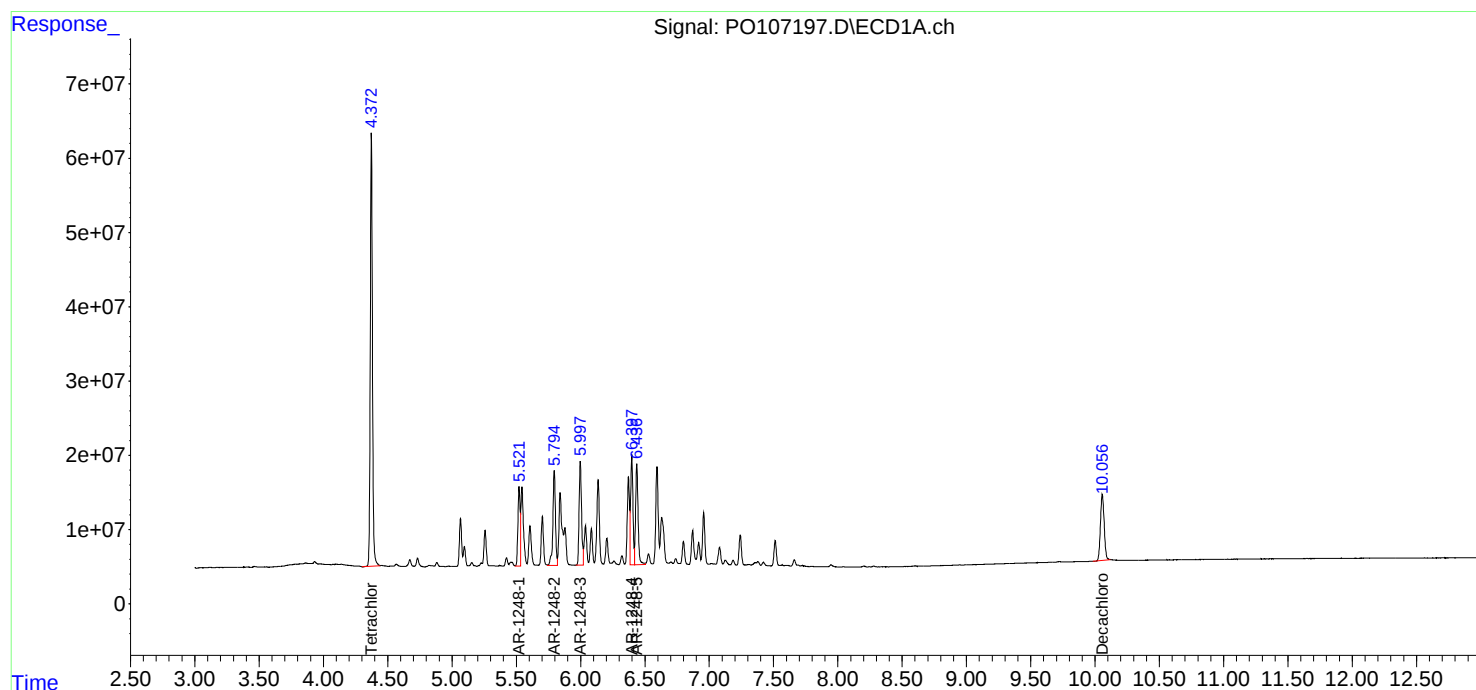

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 22:41
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:09:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	467.9E6	171.3E6	50.000	50.000
2) SA Decachlor...	10.058	8.638	125.2E6	139.6E6	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	87595666	32439560	500.000	500.000
22) L5 AR-1248-2	5.795	4.962	126.8E6	46530975	500.000	500.000
23) L5 AR-1248-3	5.998	5.004	129.9E6	48688939	500.000	500.000
24) L5 AR-1248-4	6.398	5.176	130.3E6	57380206	500.000	500.000
25) L5 AR-1248-5	6.437	5.567	130.4E6	54900690	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 22:41
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:09:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

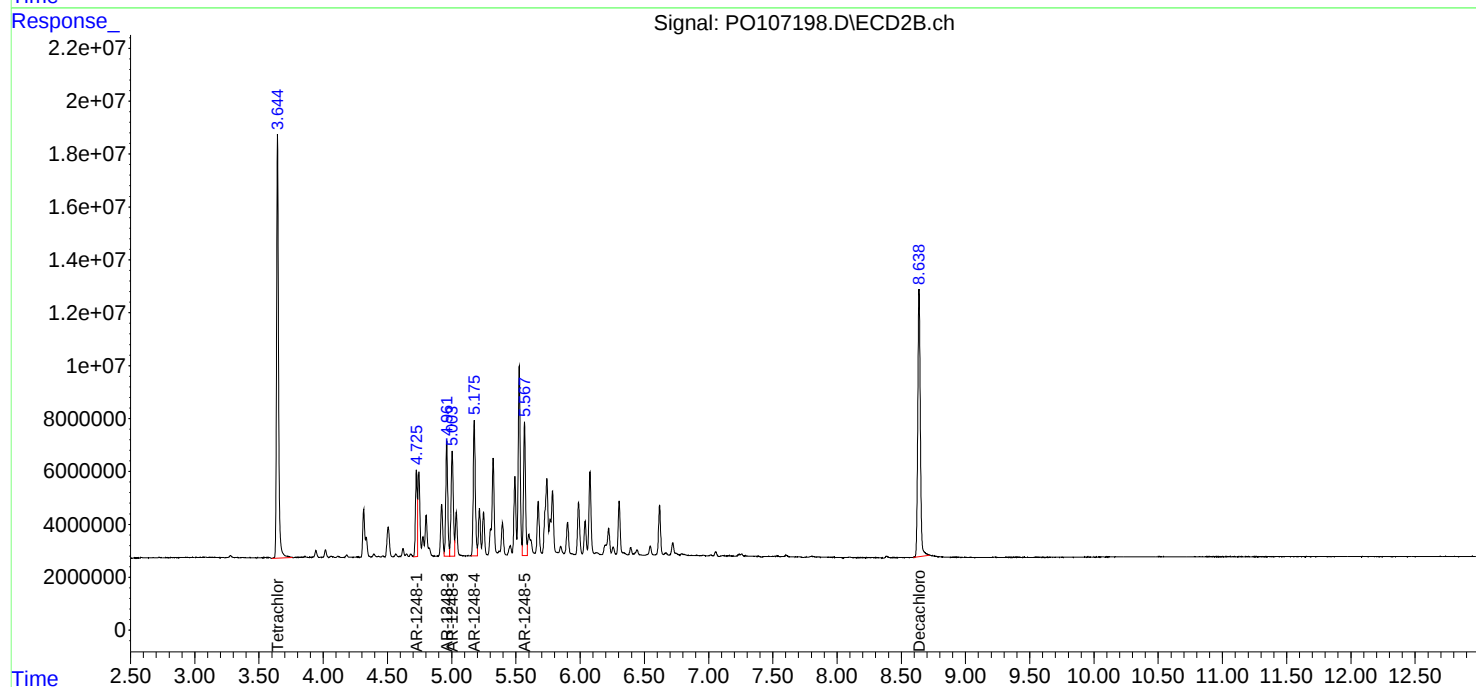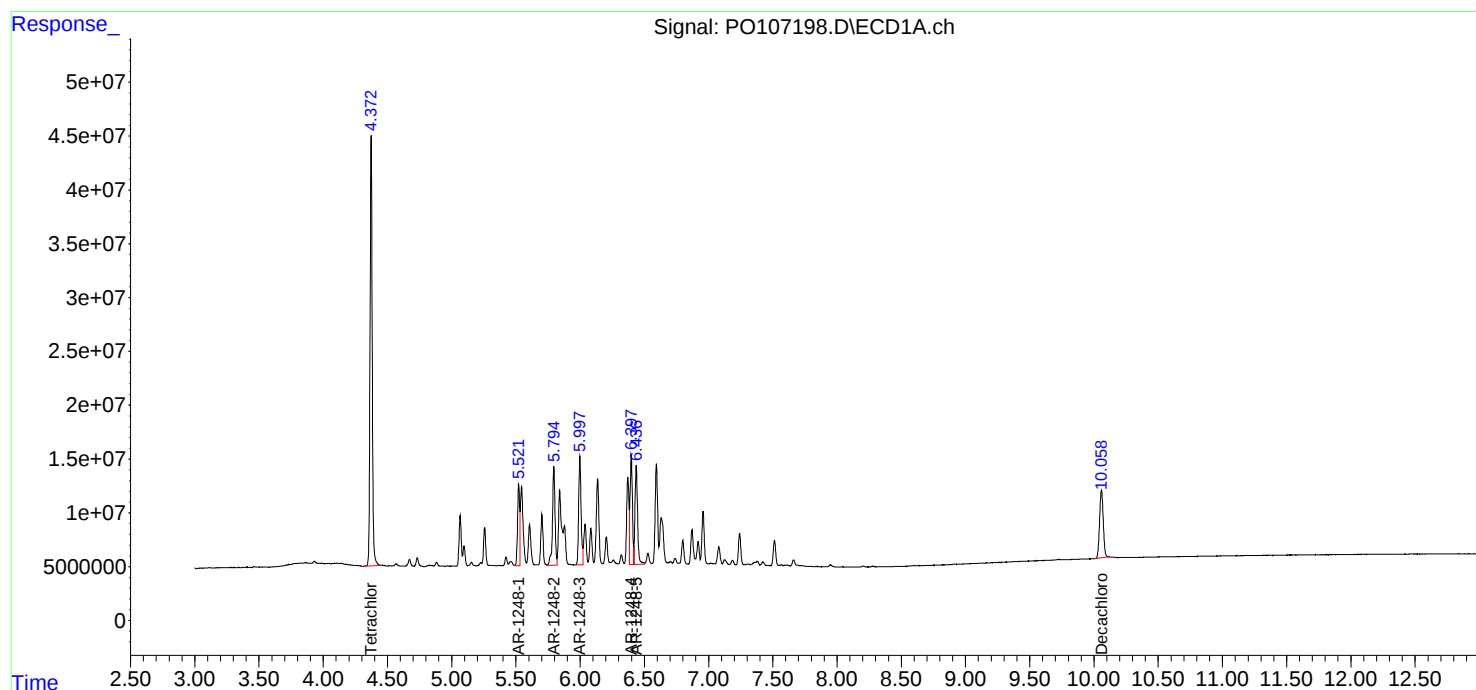

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 22:59
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:09:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	237.3E6	84054601	25.358	24.535
2) SA Decachlor...	10.056	8.639	64153967	70917862	25.620	25.402
Target Compounds						
21) L5 AR-1248-1	5.522	4.725	46152443	16666809	263.440	256.890
22) L5 AR-1248-2	5.796	4.962	67518514	24135370	266.200	259.347
23) L5 AR-1248-3	5.998	5.003	68597053	25222976	264.133	259.022
24) L5 AR-1248-4	6.399	5.175	68218183	29443172	261.841	256.562
25) L5 AR-1248-5	6.437	5.567	69078530	28554491	264.939	260.056



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 22:59
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:09:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

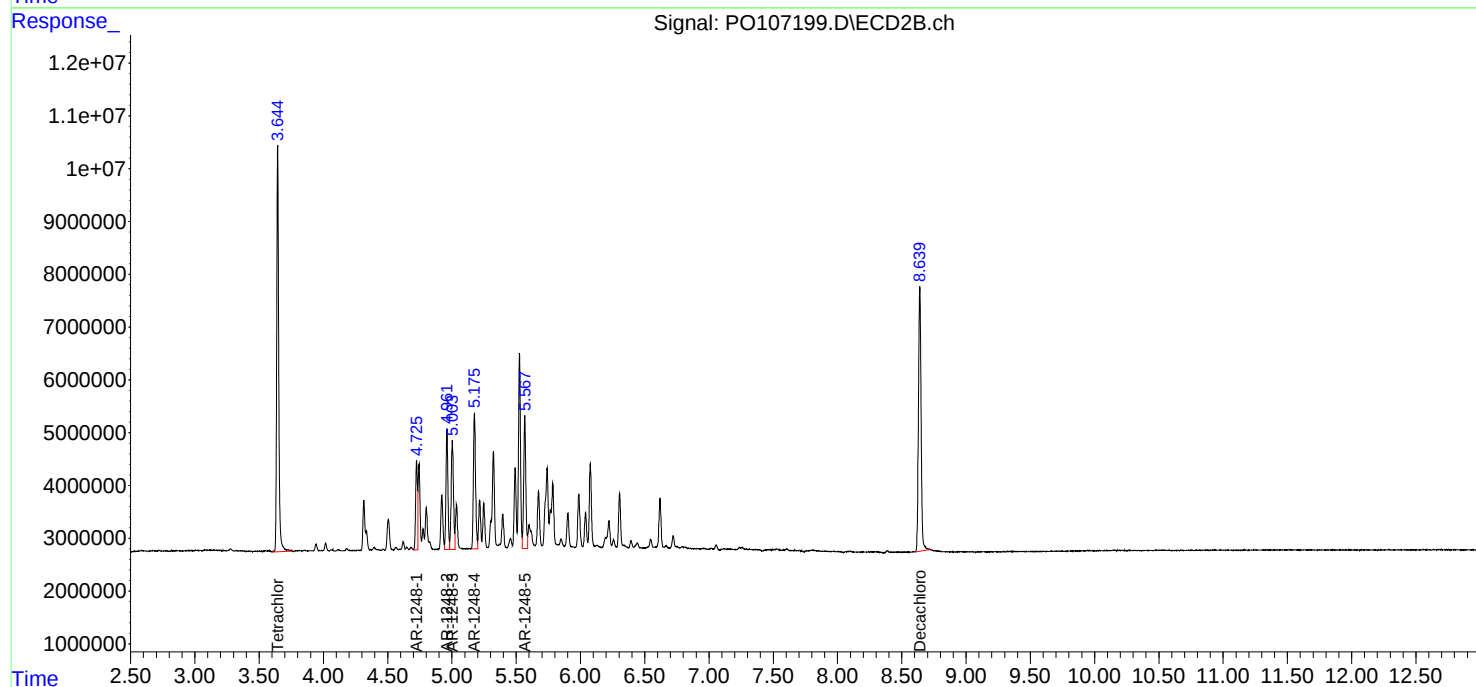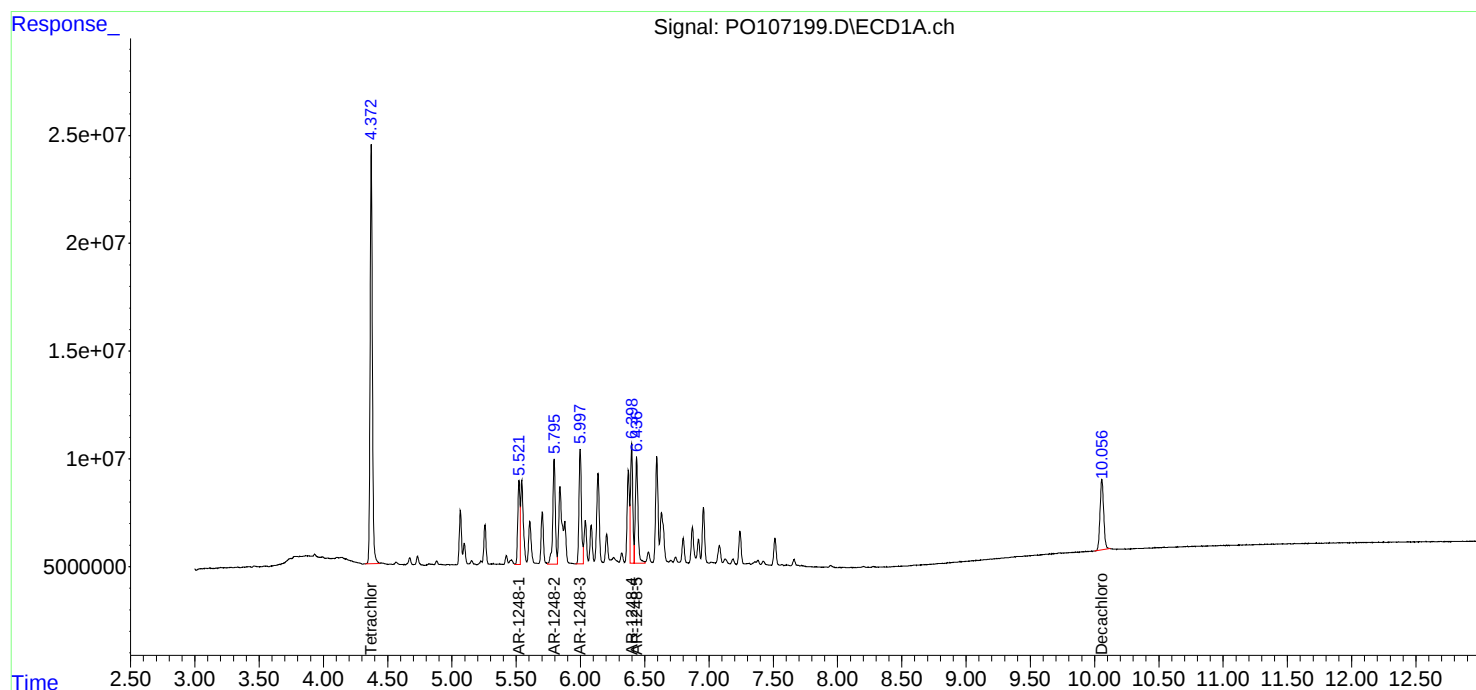

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 23:17
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:10:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:08:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	44978867	14828612	4.806	4.328
2) SA Decachlor...	10.057	8.638	11983506	13399690	4.786	4.800
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	9443386	3120120	53.903	48.091
22) L5 AR-1248-2	5.795	4.962	14018331	4677017	55.269	50.257
23) L5 AR-1248-3	5.997	5.004	13309890	4810627	51.250	49.402
24) L5 AR-1248-4	6.398	5.176	13593006	5584554	52.174	48.663
25) L5 AR-1248-5	6.436	5.567	14015230	5957032	53.753	54.253



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 23:17
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:10:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:08:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

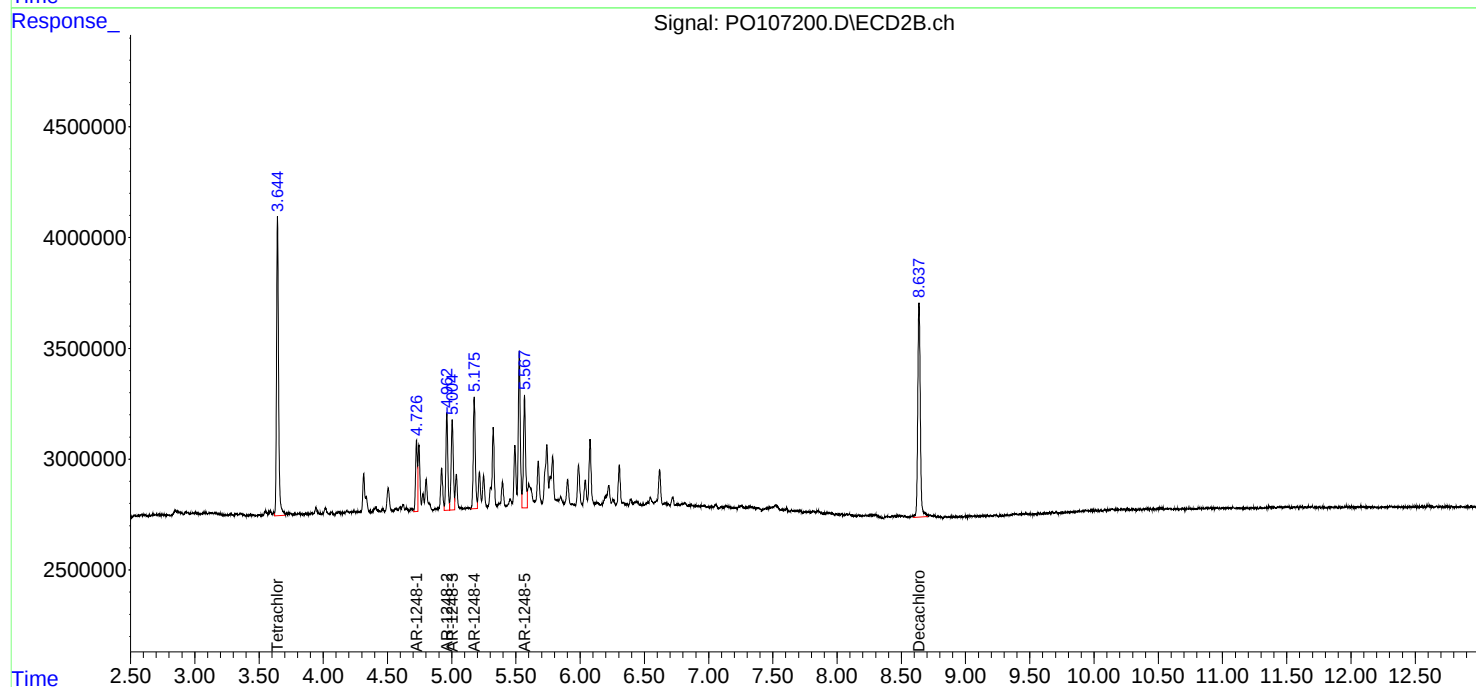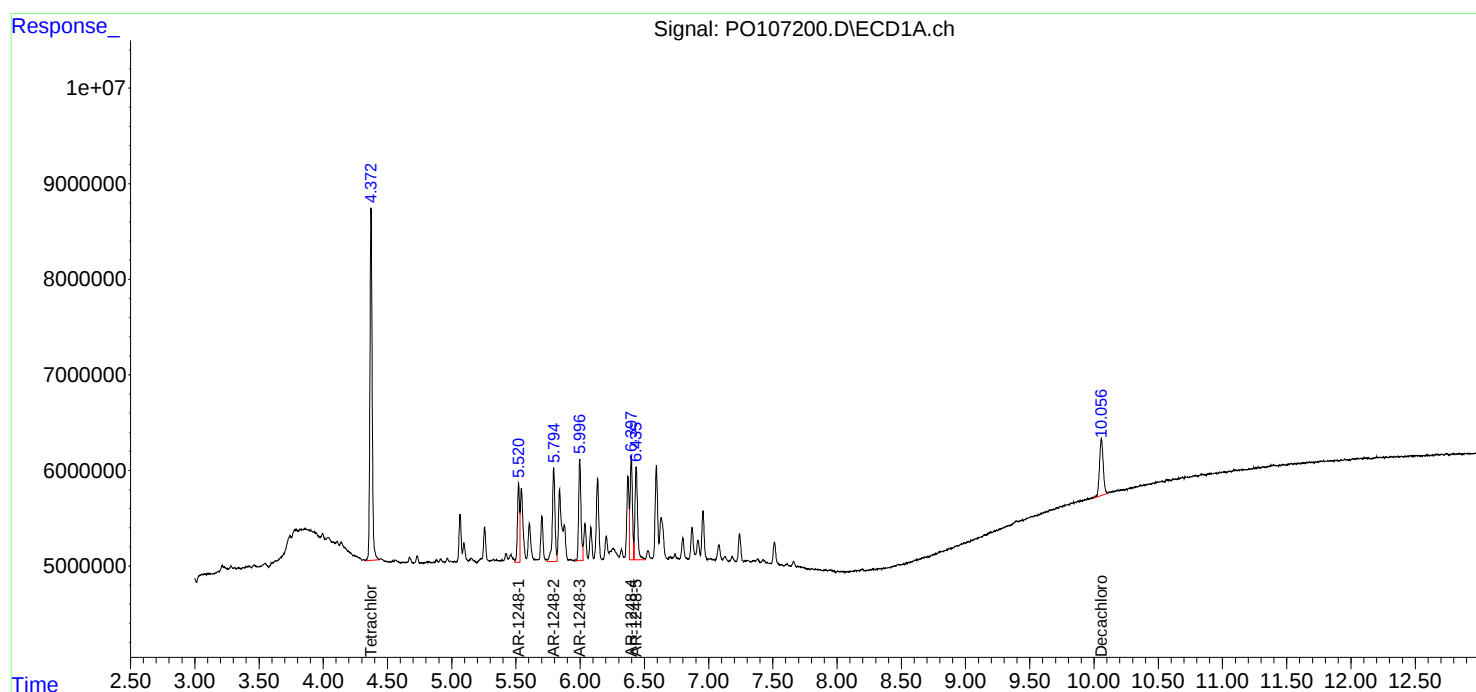

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 23:35
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:21:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	888.4E6	334.8E6	96.727	99.808
2) SA Decachlor...	10.058	8.638	235.8E6	272.7E6	93.987	98.323
Target Compounds						
26) L6 AR-1254-1	6.374	5.526	246.8E6	159.9E6	931.434	965.611
27) L6 AR-1254-2	6.593	5.674	348.1E6	138.5E6	933.222	957.951
28) L6 AR-1254-3	6.957	6.077	336.3E6	227.1E6	944.885	977.812
29) L6 AR-1254-4	7.242	6.304	213.1E6	128.2E6	938.161	976.528
30) L6 AR-1254-5	7.663	6.721	194.6E6	191.9E6	945.308	982.221



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 23:35
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:21:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

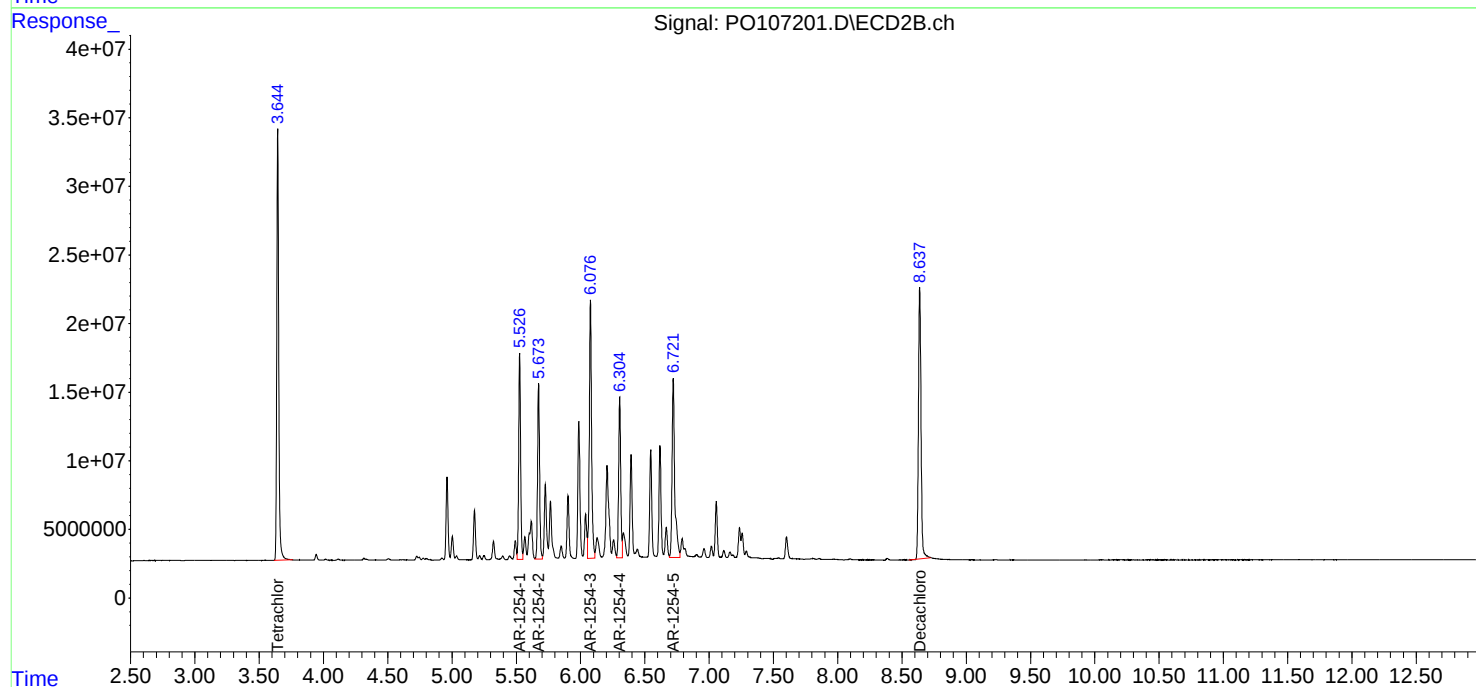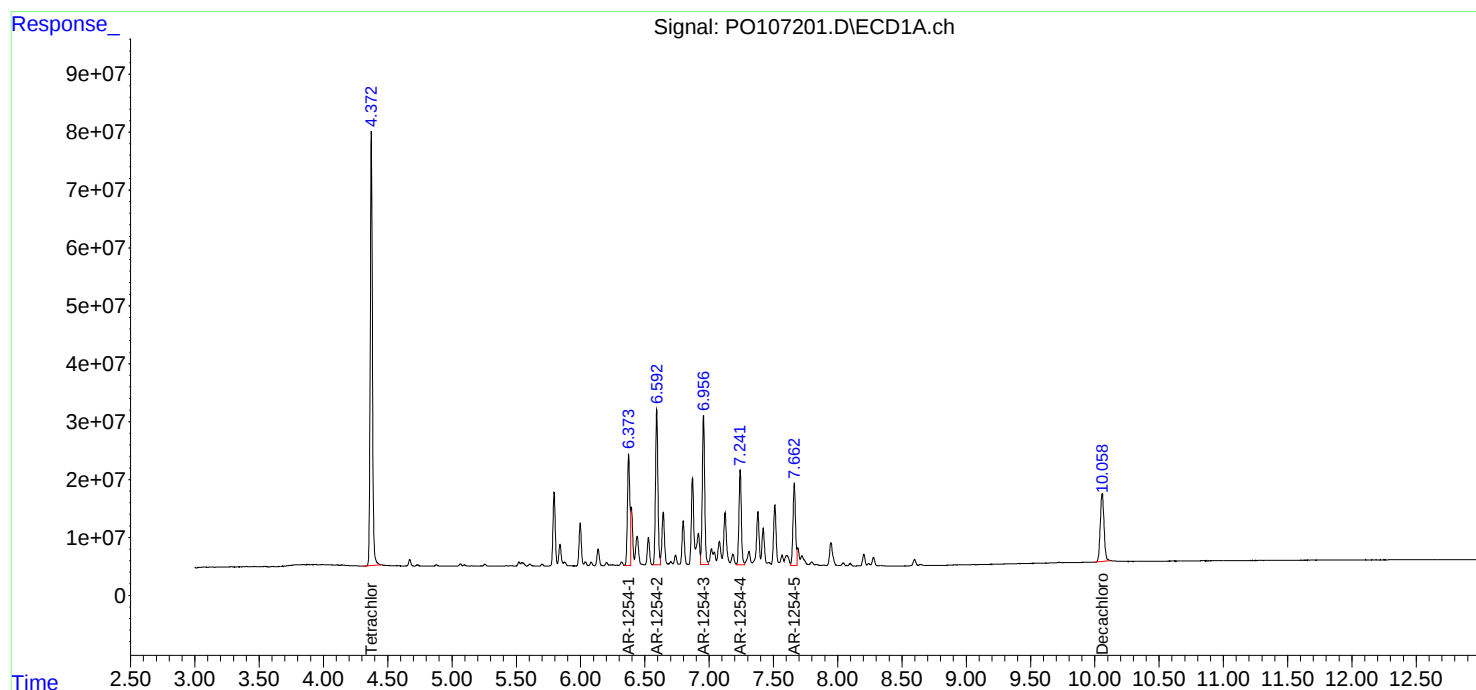

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 23:53
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:22:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	687.3E6	254.8E6	74.839	75.963
2) SA Decachlor...	10.058	8.638	180.1E6	205.4E6	71.810	74.047
Target Compounds						
26) L6 AR-1254-1	6.374	5.526	192.4E6	122.9E6	726.190	742.326
27) L6 AR-1254-2	6.593	5.673	271.2E6	106.7E6	727.100	738.182
28) L6 AR-1254-3	6.957	6.076	259.2E6	173.5E6	728.388	747.327
29) L6 AR-1254-4	7.241	6.303	165.1E6	97687474	726.838	743.858
30) L6 AR-1254-5	7.662	6.721	150.8E6	146.4E6	732.514	749.136



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 23:53
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:22:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

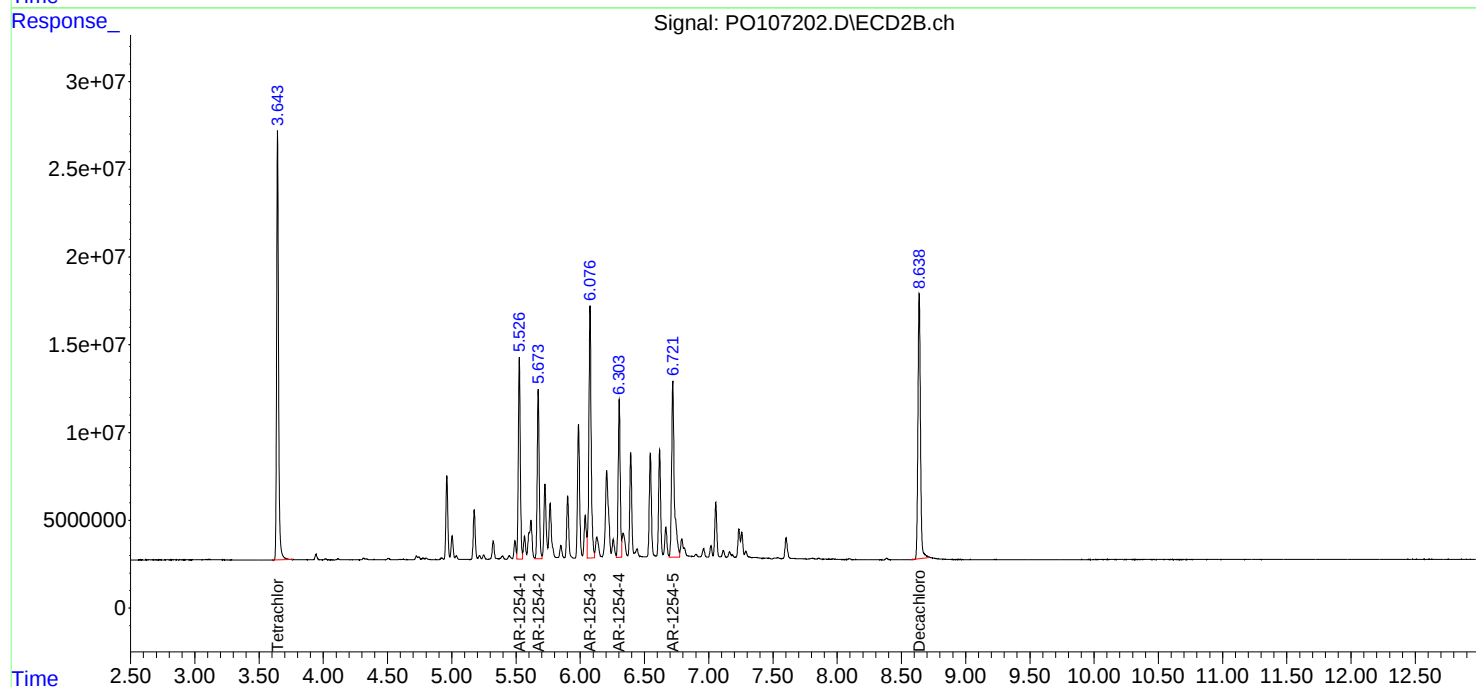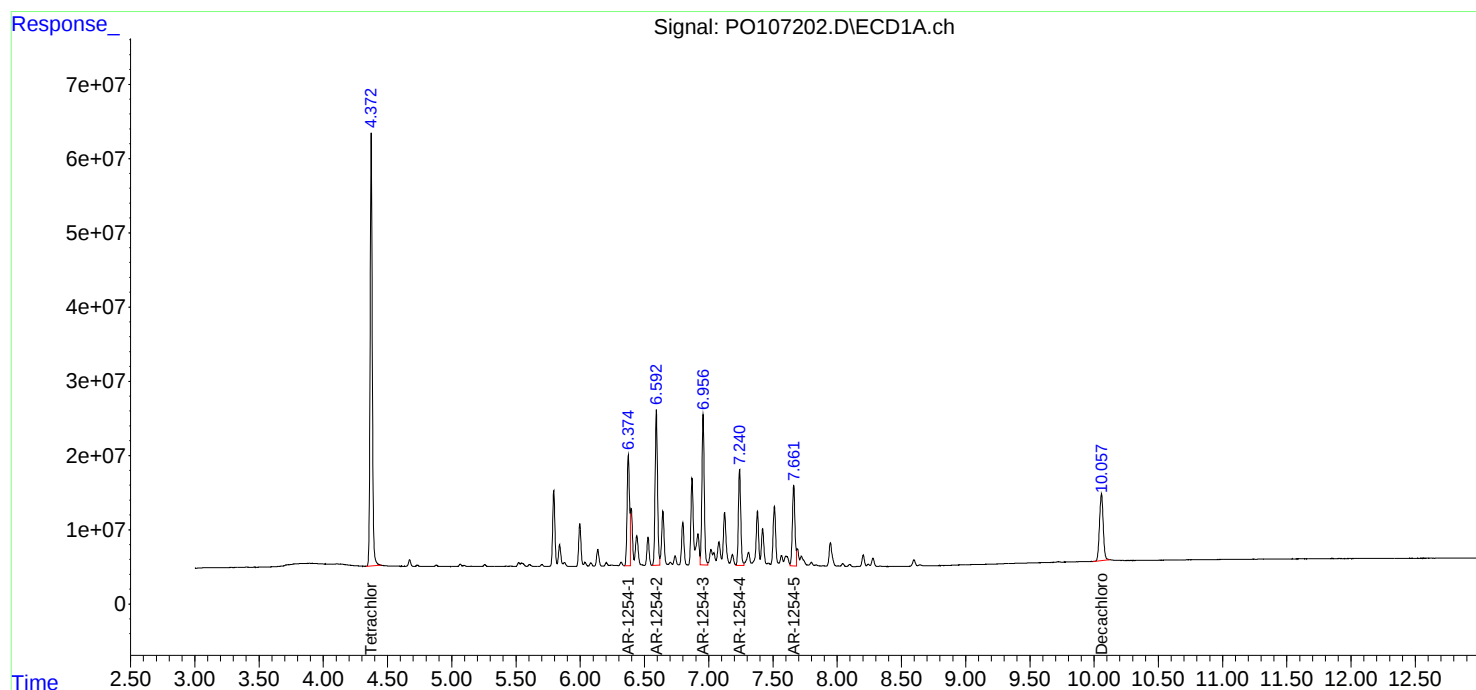

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 00:11
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:22:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	459.2E6	167.7E6	50.000	50.000
2) SA Decachlor...	10.059	8.637	125.4E6	138.7E6	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	6.375	5.526	132.5E6	82774166	500.000	500.000
27) L6 AR-1254-2	6.593	5.673	186.5E6	72273461	500.000	500.000
28) L6 AR-1254-3	6.957	6.077	178.0E6	116.1E6	500.000	500.000
29) L6 AR-1254-4	7.241	6.304	113.6E6	65662675	500.000	500.000
30) L6 AR-1254-5	7.662	6.721	102.9E6	97689052	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 00:11
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:22:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

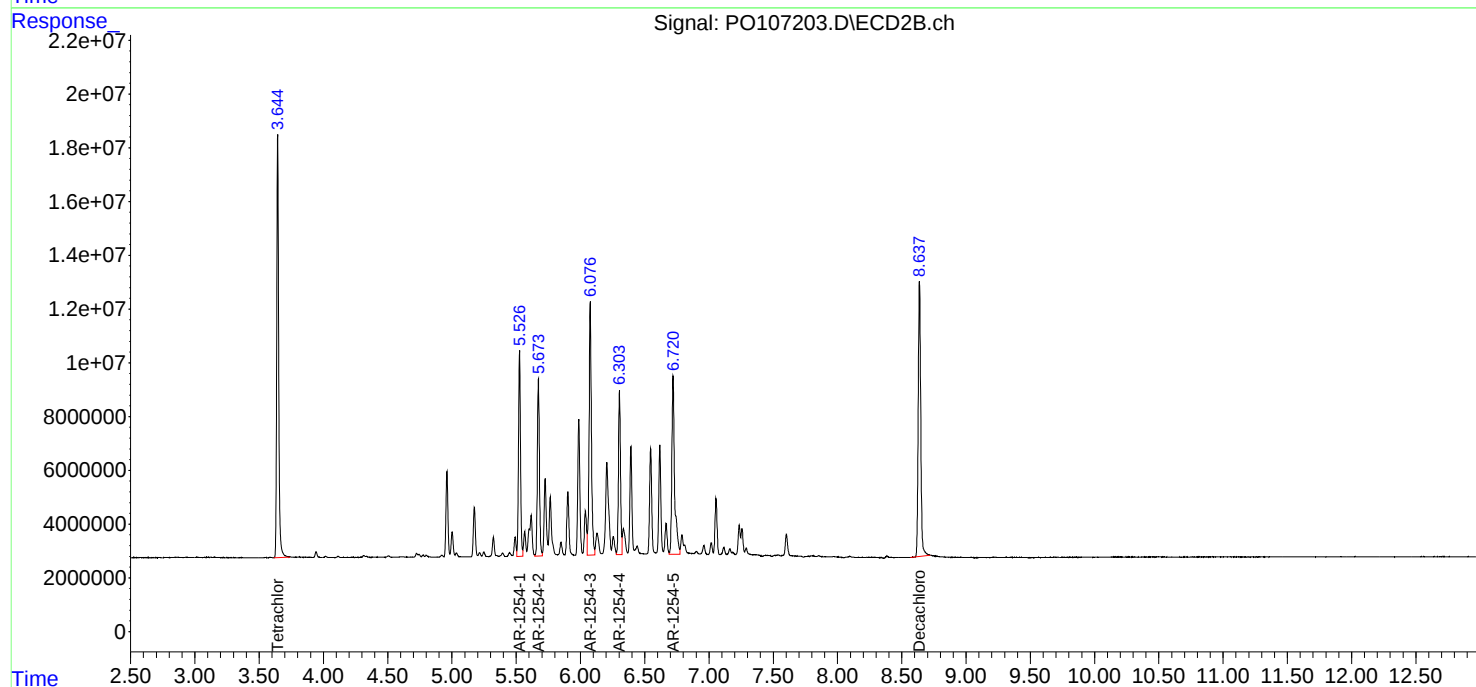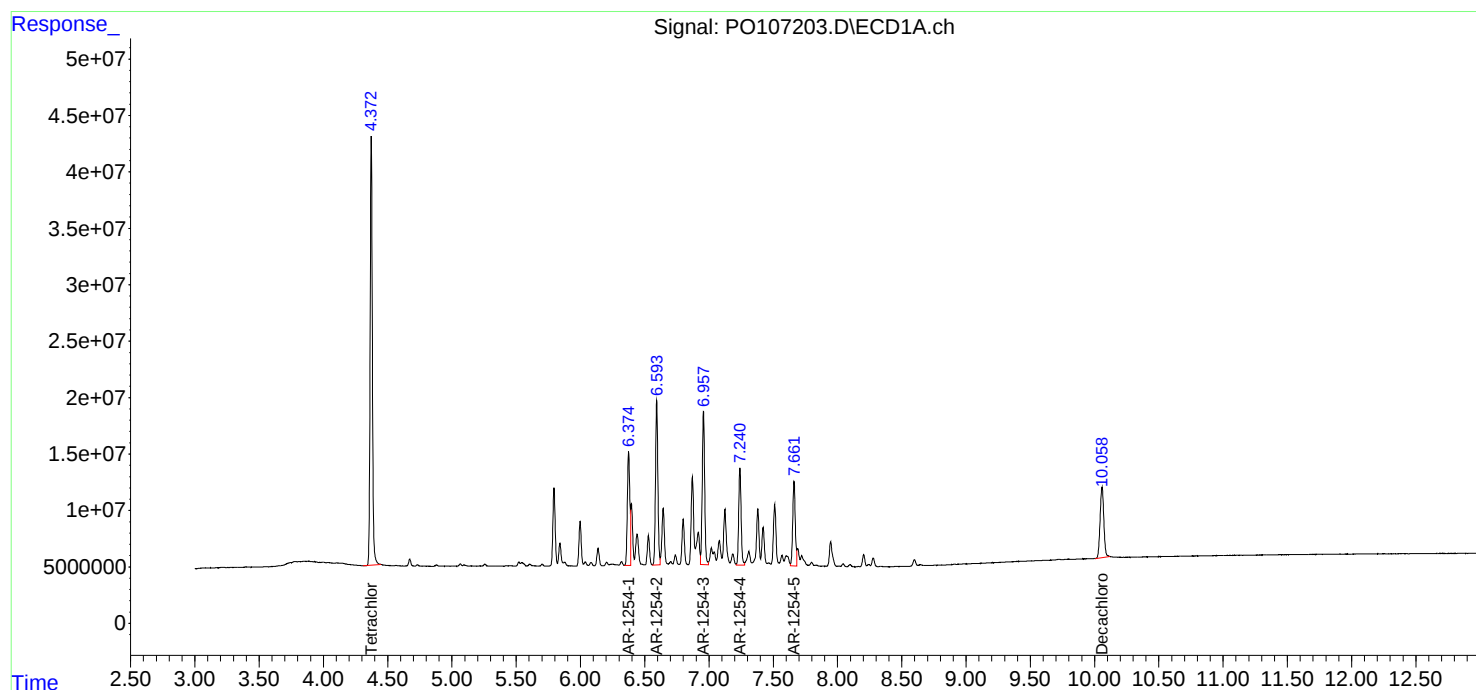

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 00:29
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:23:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	237.7E6	84055907	25.883	25.060
2) SA Decachlor...	10.058	8.638	65039455	70920394	25.927	25.571
Target Compounds						
26) L6 AR-1254-1	6.374	5.527	71547490	42929426	269.998	259.317
27) L6 AR-1254-2	6.593	5.674	100.3E6	37831493	268.904	261.725
28) L6 AR-1254-3	6.956	6.078	94624615	59643812	265.867	256.849
29) L6 AR-1254-4	7.241	6.305	60632555	33801761	266.883	257.389
30) L6 AR-1254-5	7.662	6.721	55034918	50297216	267.330	257.435



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 00:29
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:23:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

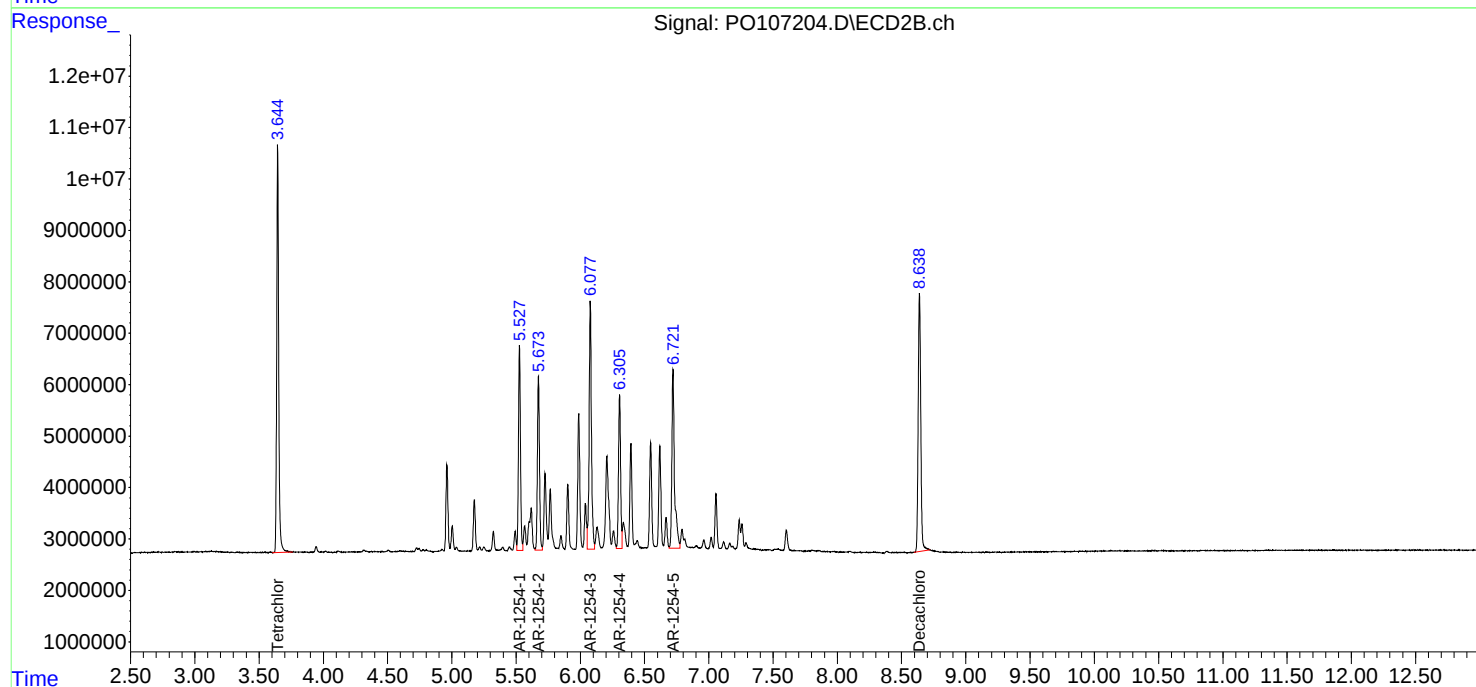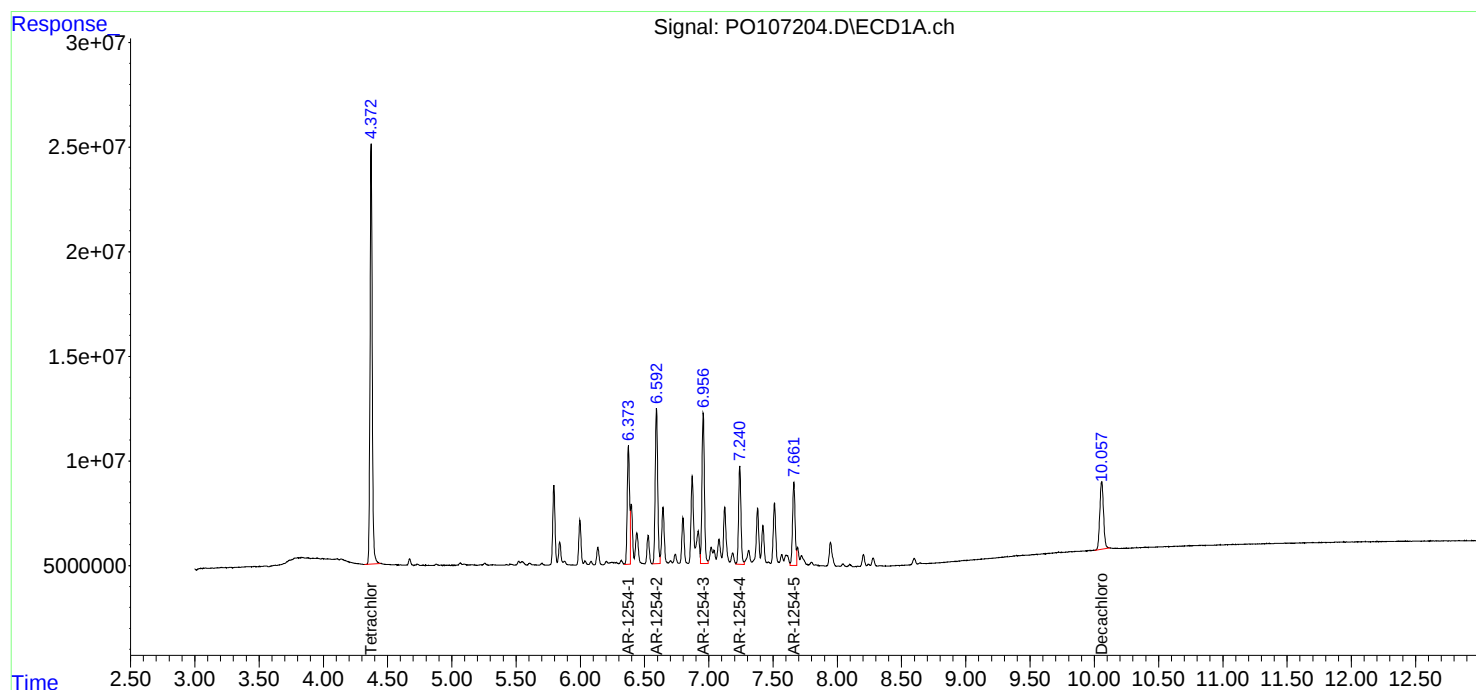

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 00:47
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:23:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:21:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	43957547	14653198	4.786	4.369
2) SA Decachlor...	10.057	8.638	11796837	12993699	4.703	4.685
Target Compounds						
26) L6 AR-1254-1	6.375	5.527	14457853	8148243	54.560	49.220
27) L6 AR-1254-2	6.593	5.674	20149788	7410157	54.016	51.265
28) L6 AR-1254-3	6.956	6.077	18631522	10943354	52.349	47.126
29) L6 AR-1254-4	7.241	6.304	12202348	6104594	53.710	46.485
30) L6 AR-1254-5	7.662	6.721	10827332	8581830	52.593	43.924



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 00:47
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:23:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:21:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

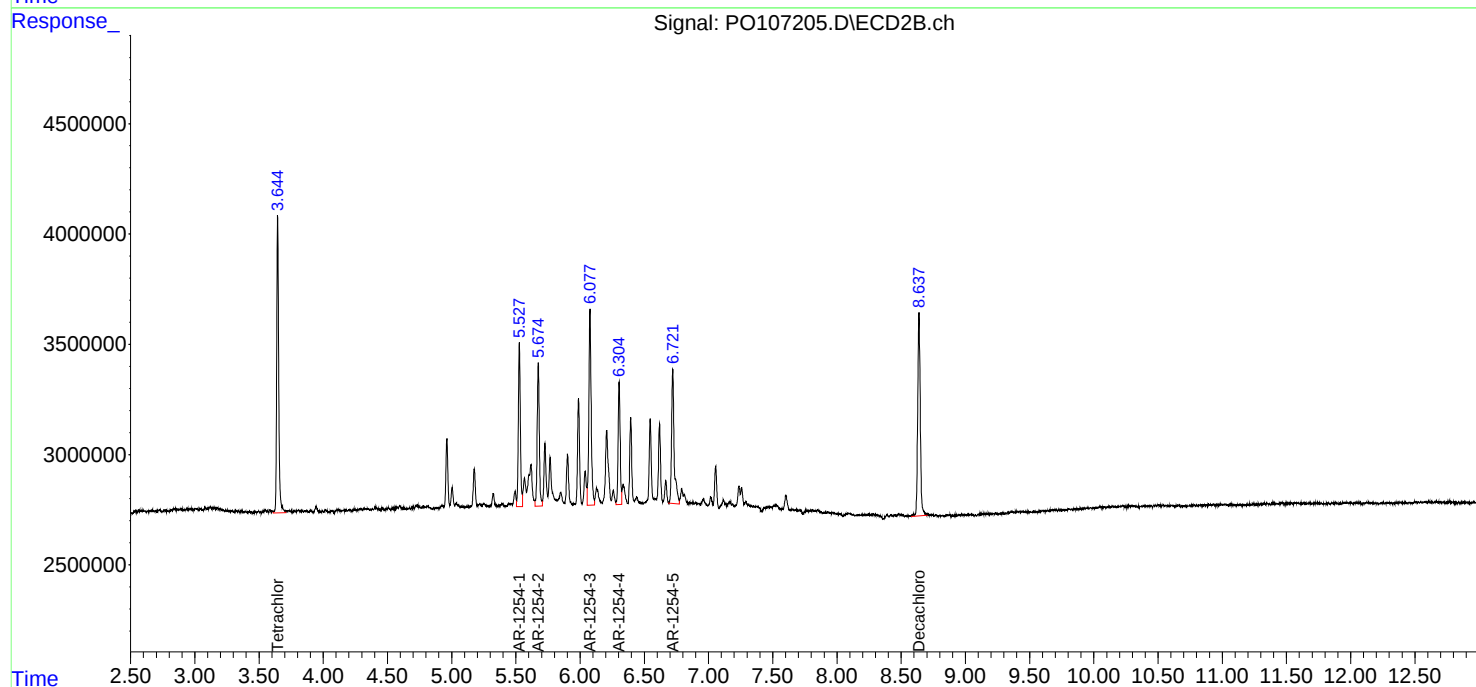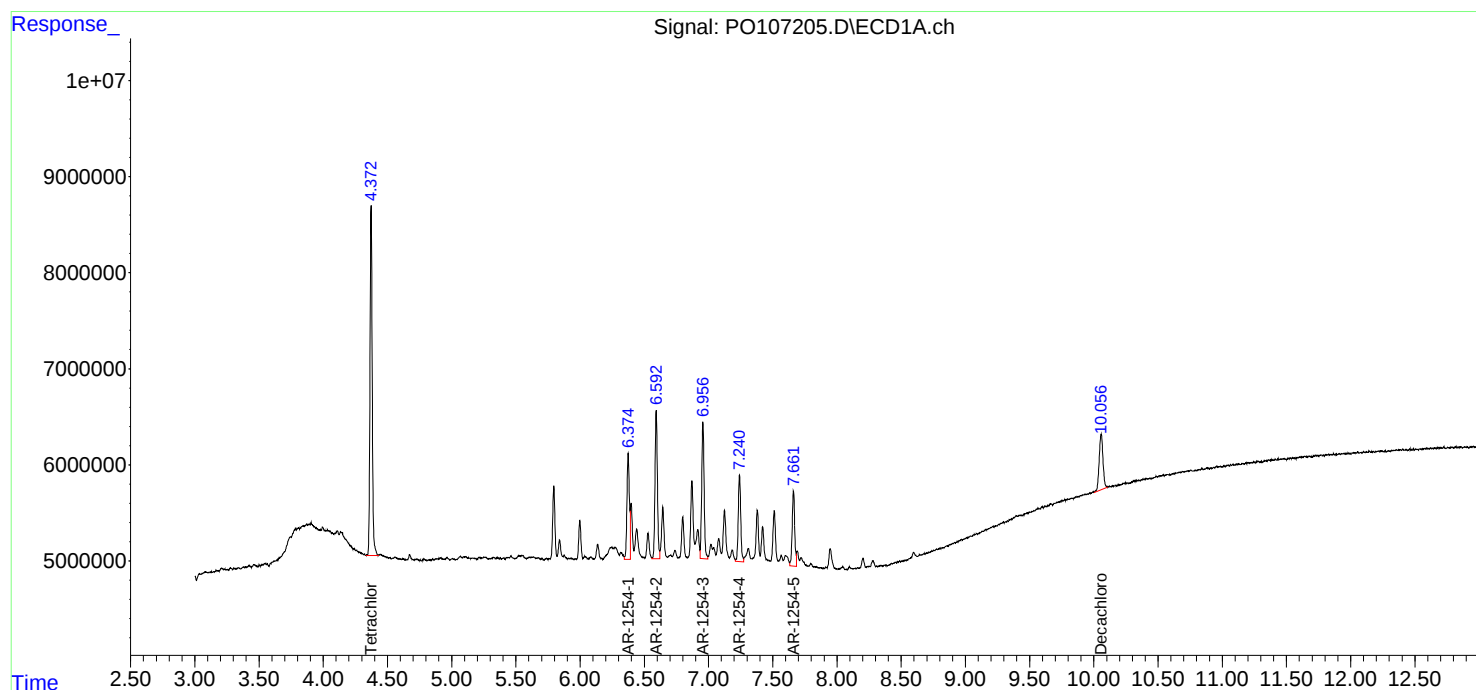

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 01:05
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:32:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:31:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	446.6E6	163.0E6	50.000	50.000
2) SA Decachlor...	10.059	8.638	123.1E6	135.8E6	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	7.742	6.759	122.8E6	106.4E6	500.000	500.000
37) L8 AR-1262-2	8.279	7.258	154.7E6	181.7E6	500.000	500.000
38) L8 AR-1262-3	8.592	7.541	104.6E6	68691960	500.000	500.000
39) L8 AR-1262-4	8.677	7.605	81533074	132.3E6	500.000	500.000
40) L8 AR-1262-5	9.315	8.096	51381891	56416259	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 01:05
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:32:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:31:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

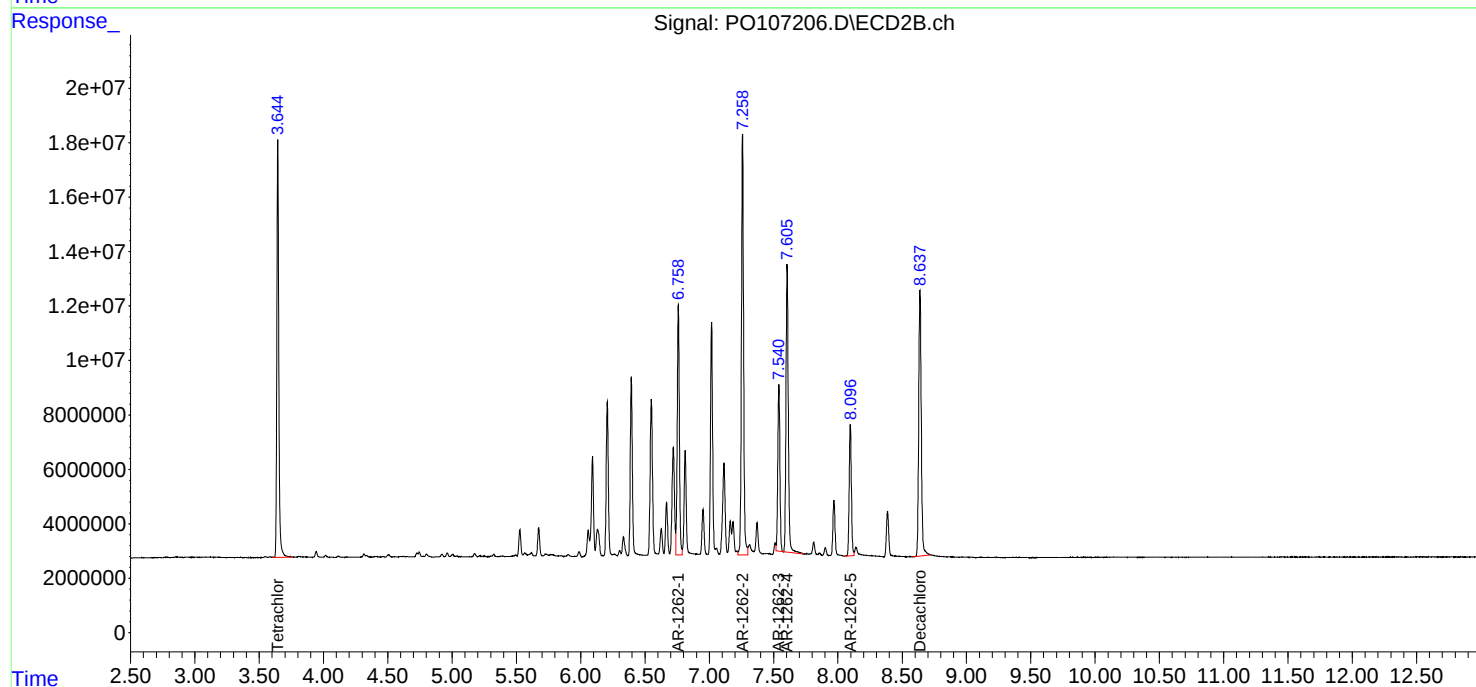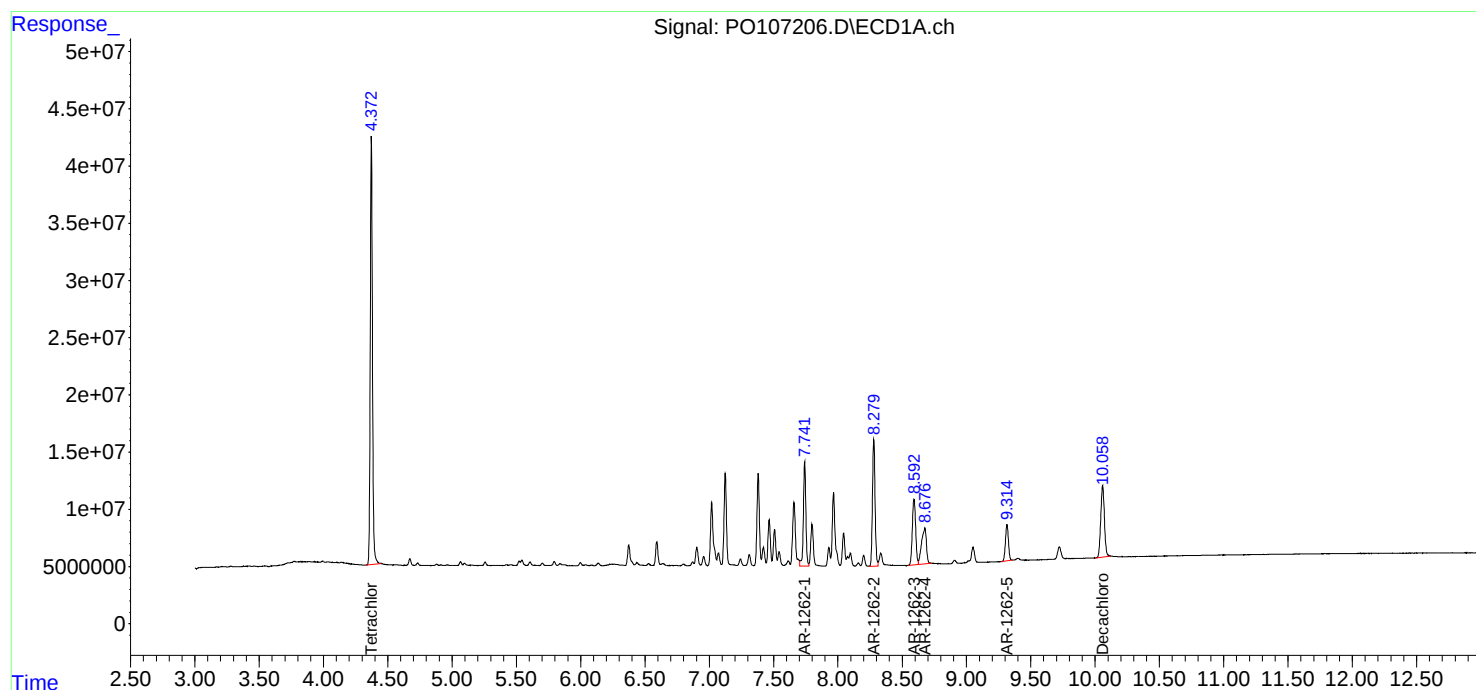

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 01:23
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:40:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	914.0E6	344.0E6	98.153	100.708
2) SA Decachlor...	10.057	8.639	407.4E6	487.4E6	96.045	101.044
Target Compounds						
41) L9 AR-1268-1	8.587	7.541	351.9E6	419.2E6	965.004	1012.873
42) L9 AR-1268-2	8.679	7.606	313.1E6	389.7E6	963.780	1016.048
43) L9 AR-1268-3	8.907	7.812	272.2E6	345.3E6	963.260	1016.931
44) L9 AR-1268-4	9.313	8.097	112.2E6	129.1E6	978.396	1014.319
45) L9 AR-1268-5	9.721	8.386	836.7E6	1049.2E6	987.735	1031.617



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 01:23
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:40:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

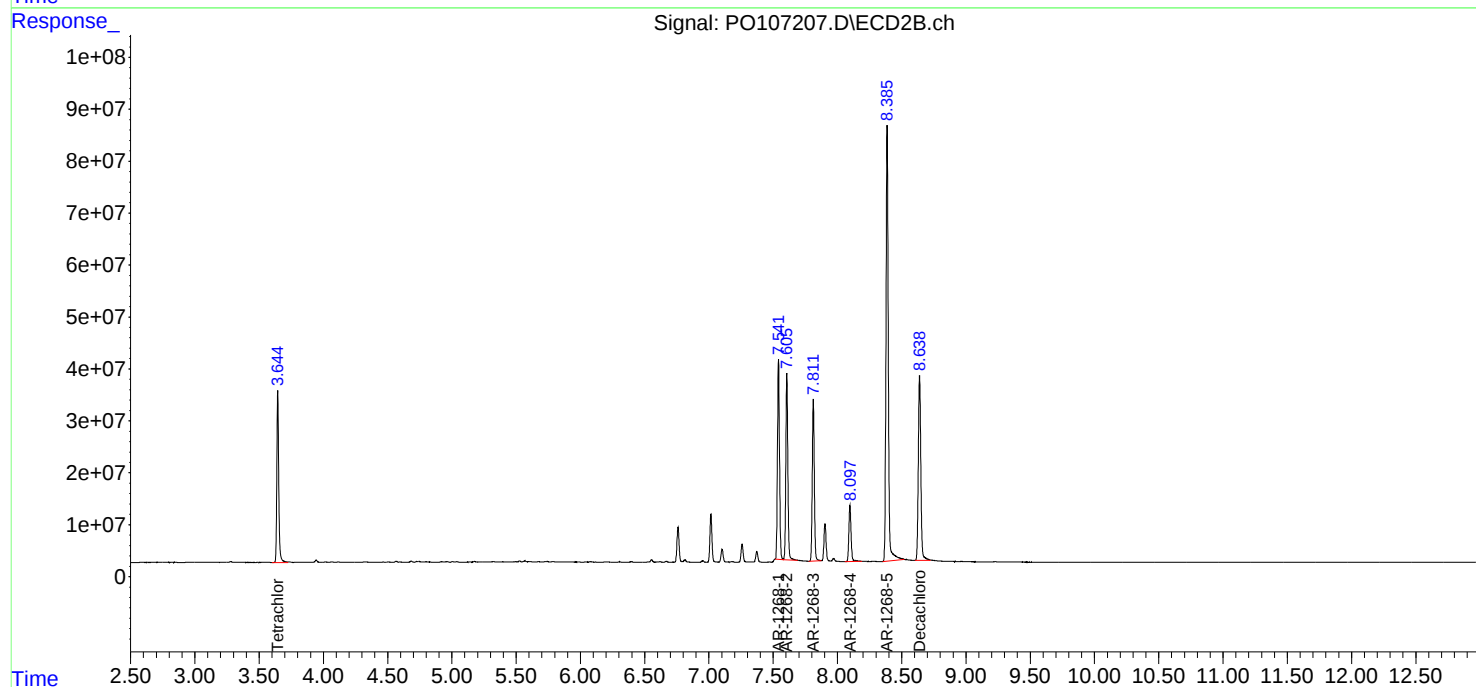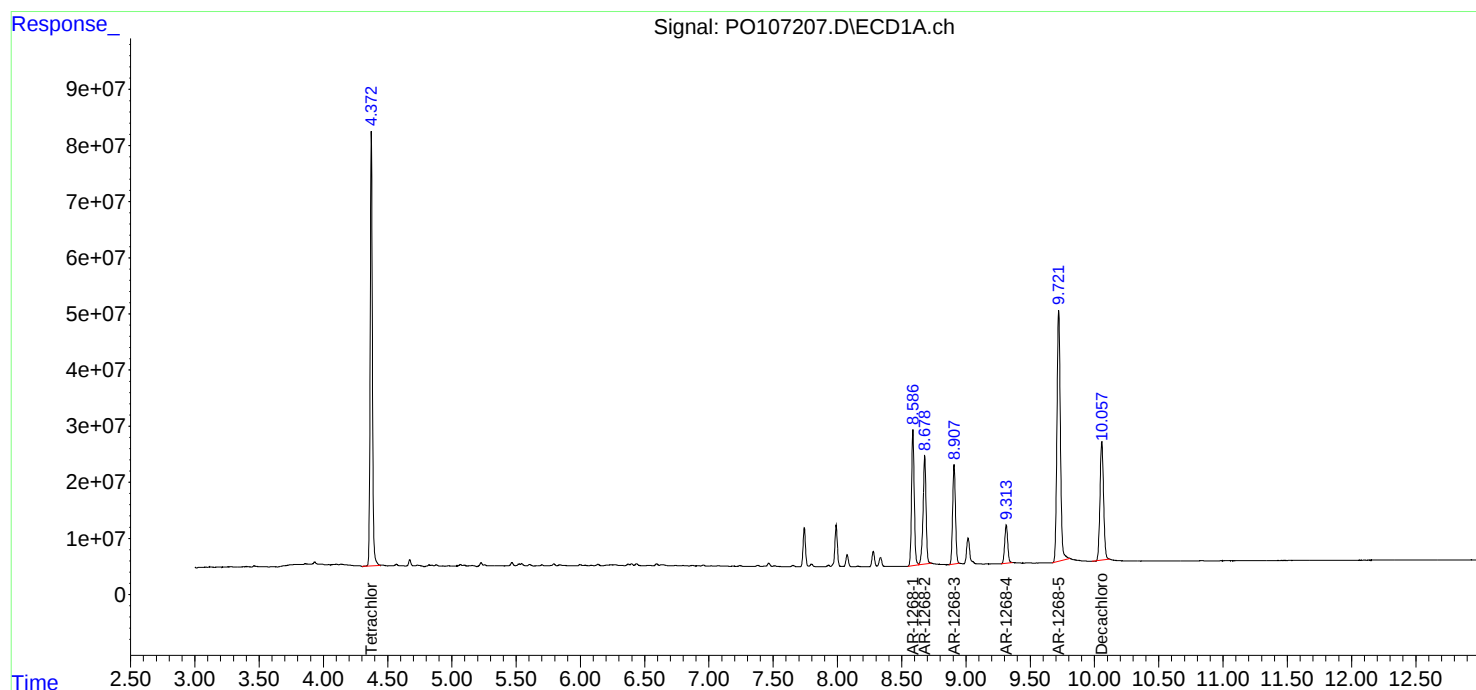

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 01:41
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:40:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	670.2E6	249.7E6	71.974	73.105
2) SA Decachlor...	10.058	8.638	310.2E6	355.5E6	73.131	73.693
Target Compounds						
41) L9 AR-1268-1	8.587	7.541	264.3E6	307.5E6	724.887	742.983
42) L9 AR-1268-2	8.678	7.605	235.9E6	285.1E6	726.056	743.309
43) L9 AR-1268-3	8.908	7.812	204.6E6	253.4E6	723.835	746.228
44) L9 AR-1268-4	9.312	8.096	83445833	95583754	727.421	750.941
45) L9 AR-1268-5	9.722	8.386	624.8E6	764.5E6	737.635	751.645



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 01:41
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:40:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

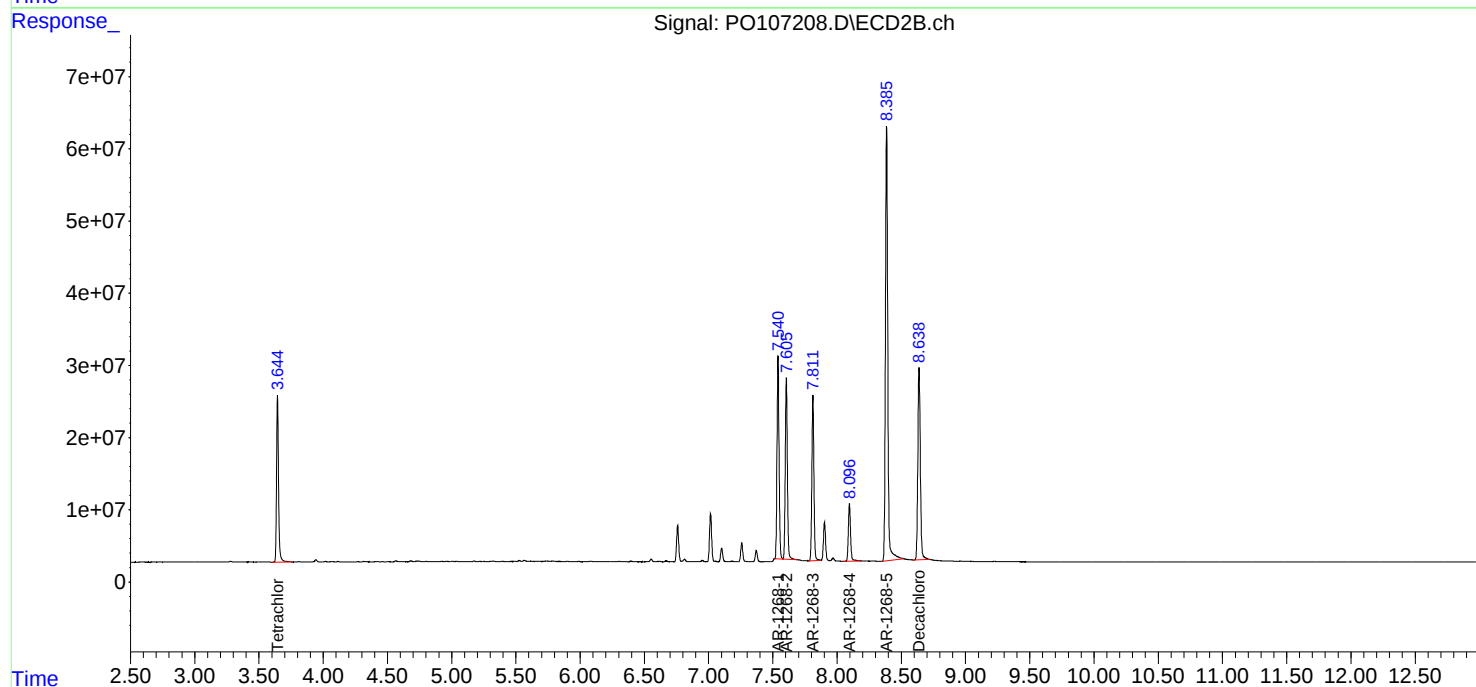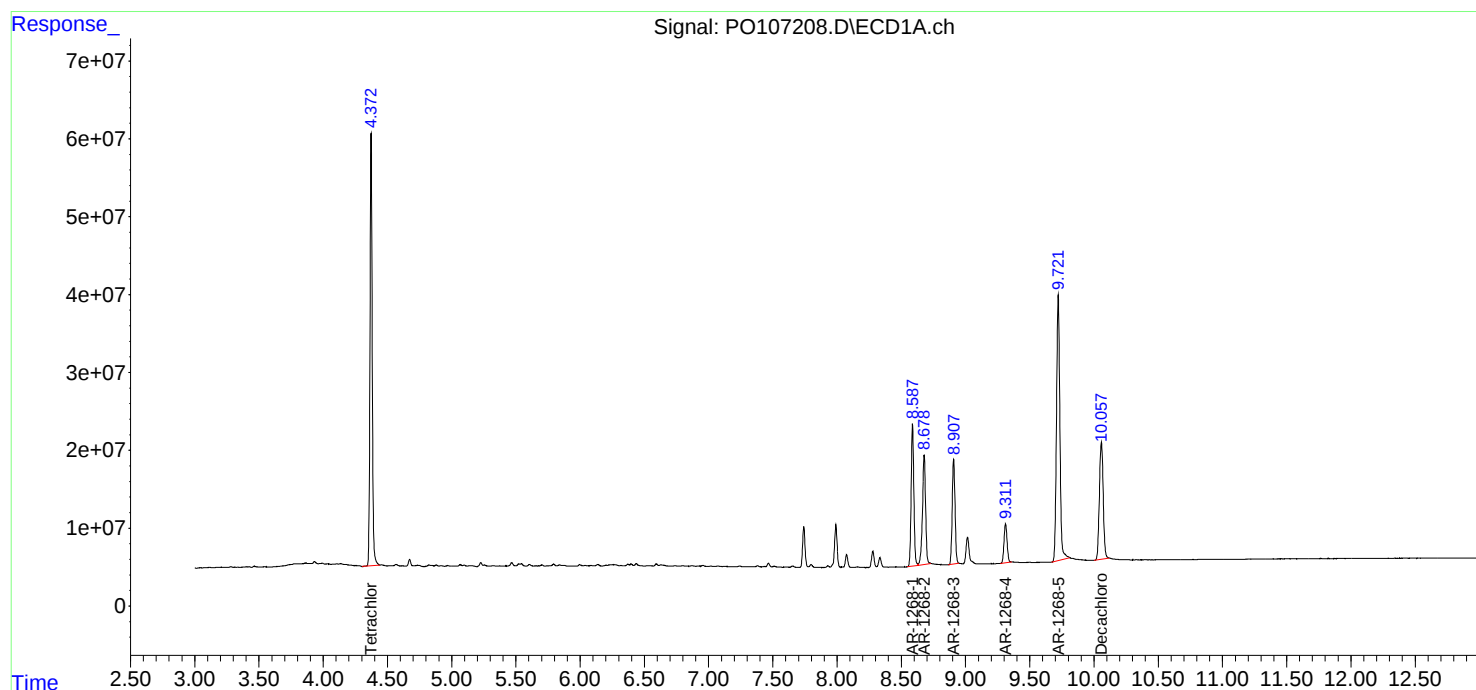

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 01:59
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 02:40:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	465.6E6	170.8E6	50.000	50.000
2) SA Decachlor...	10.057	8.637	212.1E6	241.2E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	8.587	7.541	182.3E6	206.9E6	500.000	500.000
42) L9 AR-1268-2	8.678	7.605	162.4E6	191.8E6	500.000	500.000
43) L9 AR-1268-3	8.907	7.811	141.3E6	169.8E6	500.000	500.000
44) L9 AR-1268-4	9.312	8.096	57357297	63642681	500.000	500.000
45) L9 AR-1268-5	9.721	8.385	423.5E6	508.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 01:59
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 02:40:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

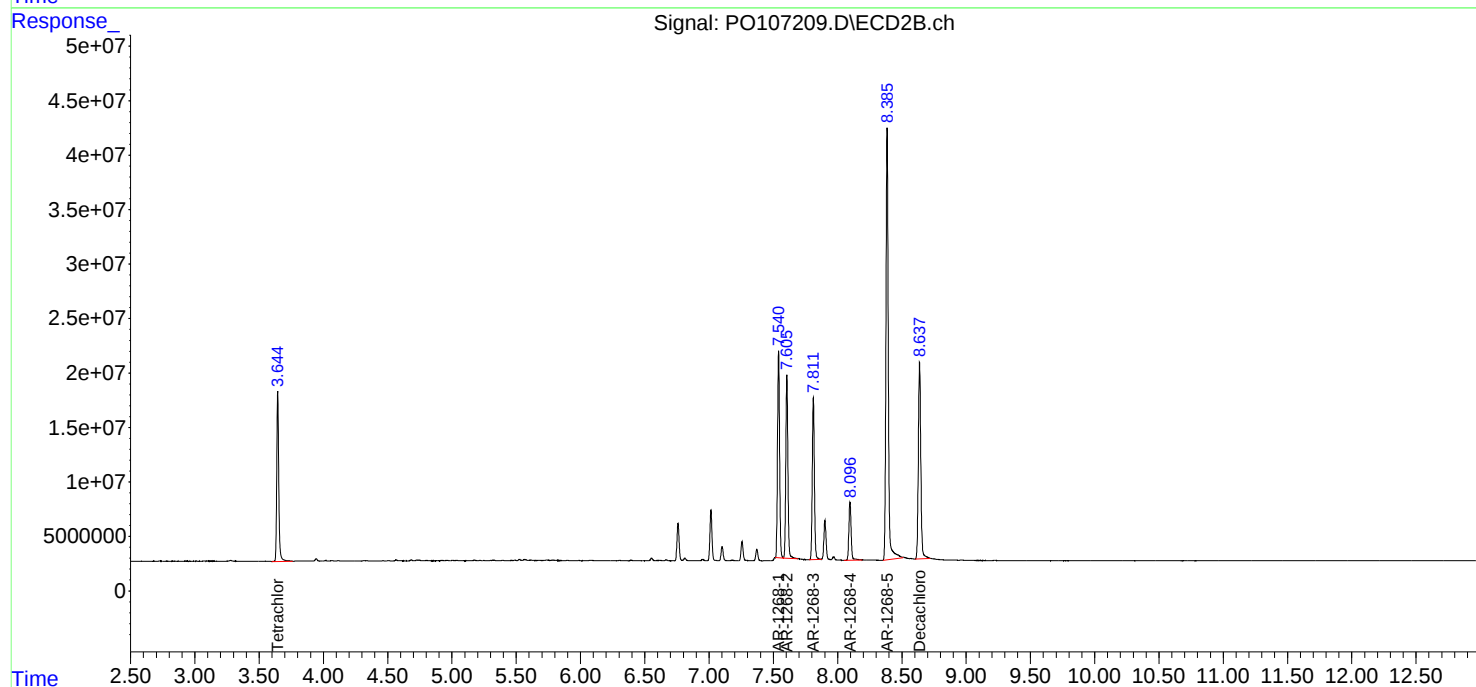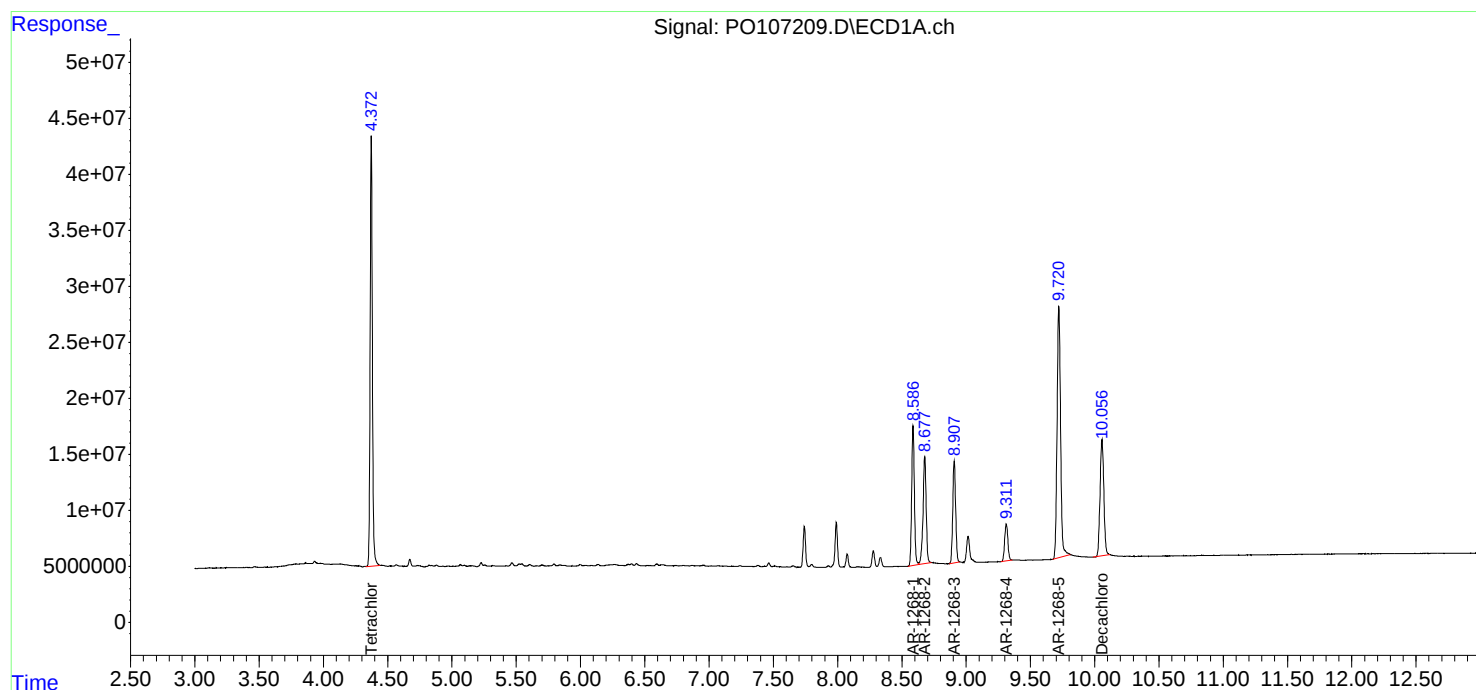

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 02:18
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:21:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	237.4E6	83283643	25.493	24.380
2) SA Decachlor...	10.058	8.638	110.0E6	122.3E6	25.930	25.345
Target Compounds						
41) L9 AR-1268-1	8.588	7.541	95440132	102.7E6	261.750	248.179
42) L9 AR-1268-2	8.679	7.606	84909424	94674968	261.370	246.859
43) L9 AR-1268-3	8.908	7.812	73384675	84688940	259.658	249.426
44) L9 AR-1268-4	9.314	8.097	29107021	32315199	253.734	253.880
45) L9 AR-1268-5	9.721	8.386	216.1E6	249.1E6	255.104	244.896



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 02:18
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:21:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

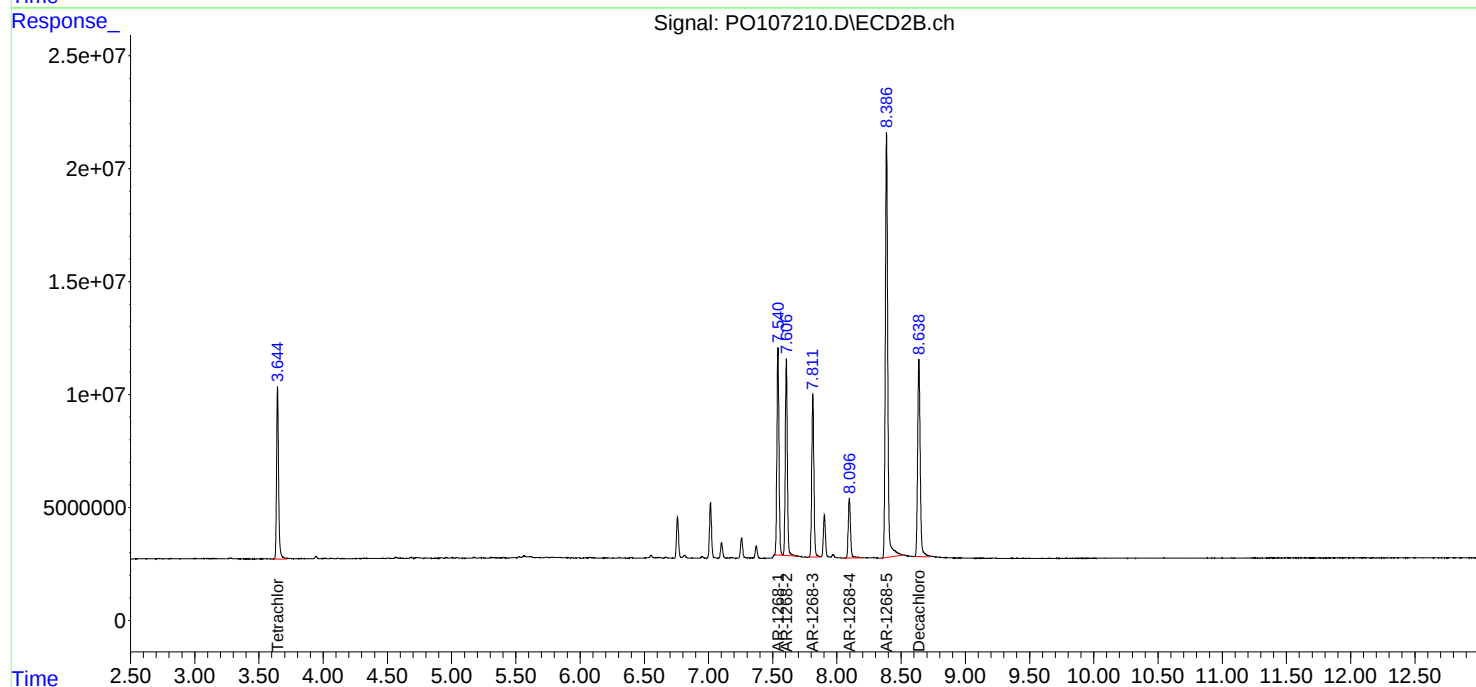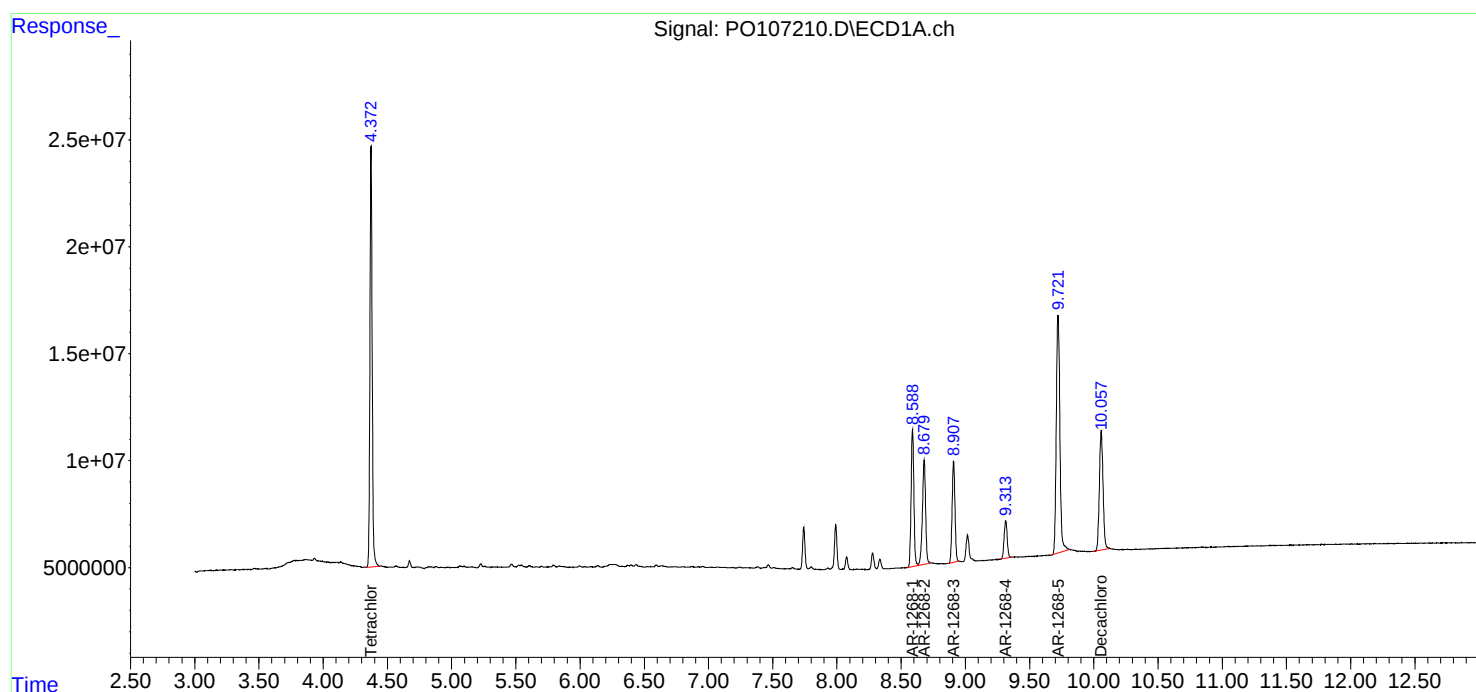

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 02:36
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/16/2024
 Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:22:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.645	44759505	14819032	4.807	4.338
2) SA Decachlor...	10.056	8.638	20020423	22152727	4.720	4.593
Target Compounds						
41) L9 AR-1268-1	8.587	7.541	18469024	18447765	50.652m	44.575
42) L9 AR-1268-2	8.679	7.606	16014978	16717280	49.298	43.589
43) L9 AR-1268-3	8.908	7.811	13783097	15350219	48.769	45.209
44) L9 AR-1268-4	9.314	8.097	5072917	5687474	44.222	44.683
45) L9 AR-1268-5	9.723	8.385	39053378	42842014	46.104	42.123

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 02:36
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2024
Supervised By :Ankita Jodhani 10/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:22:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

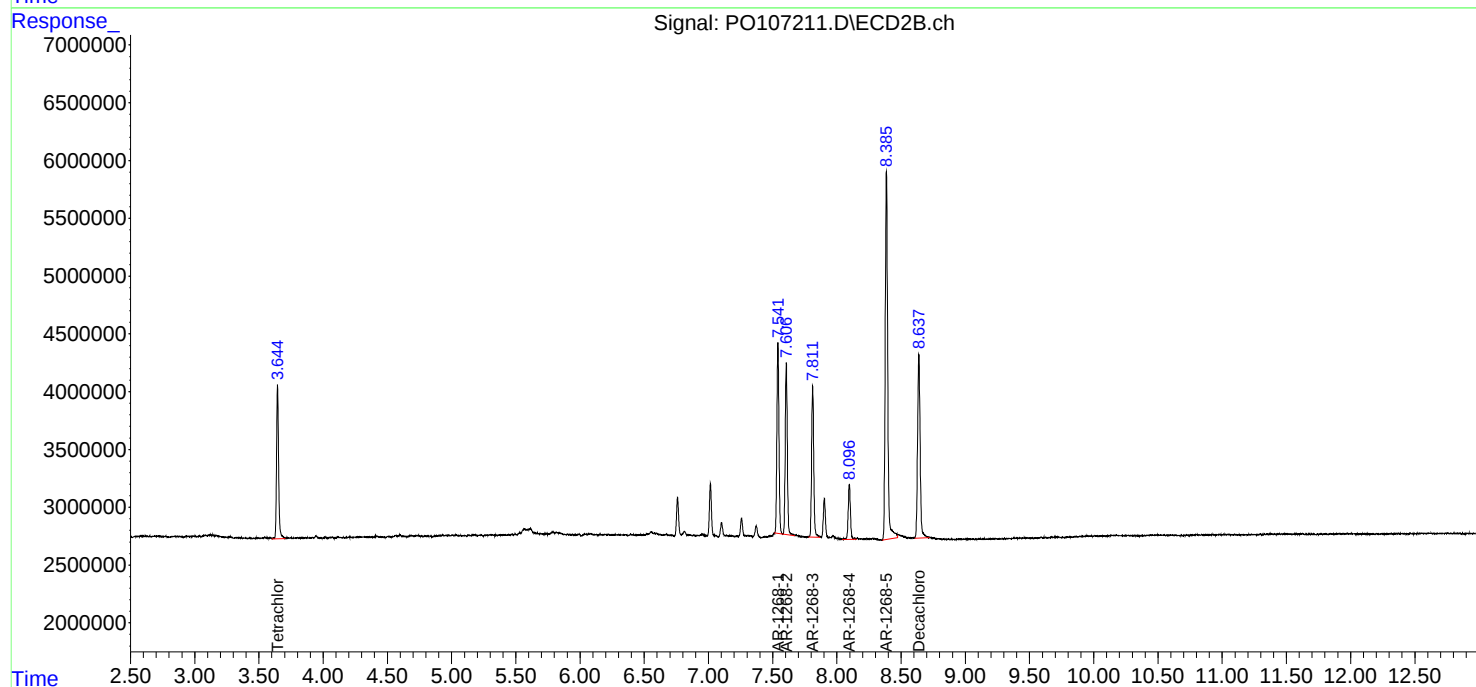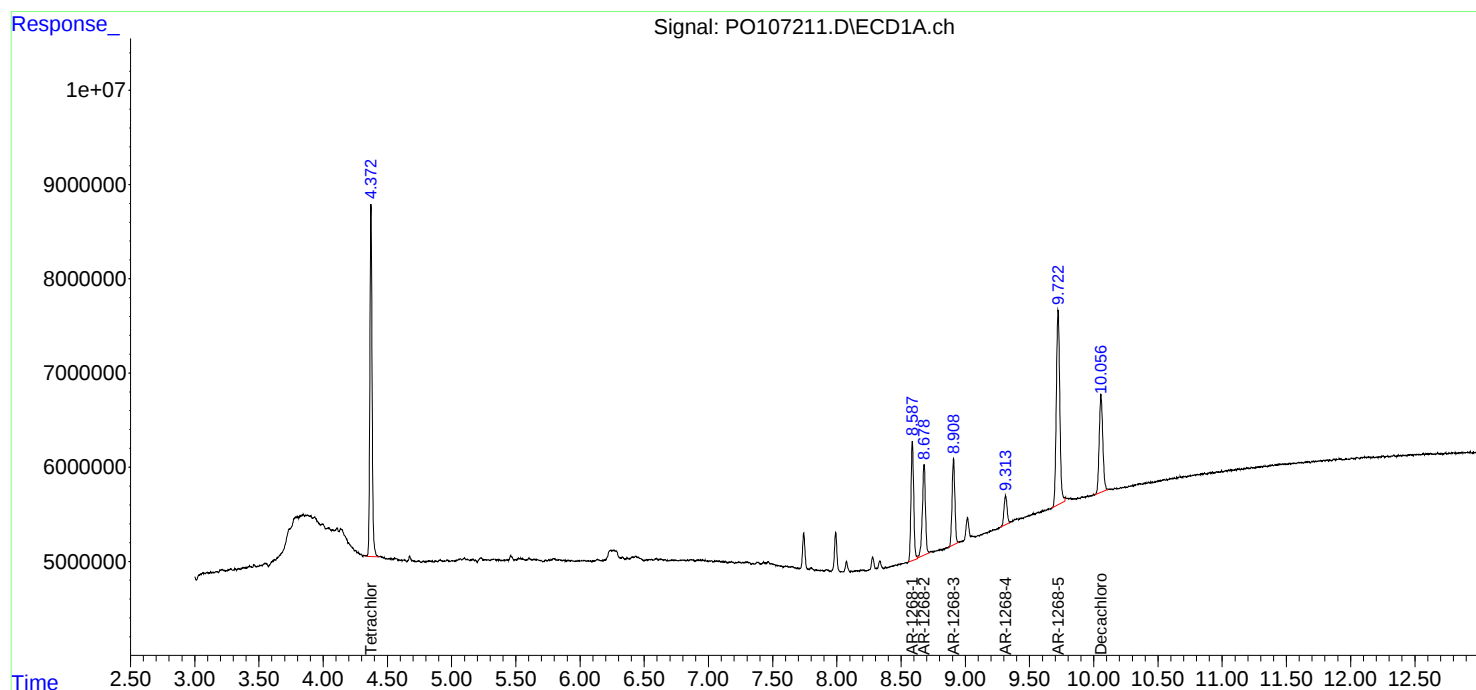

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 02:54
 Operator : YP/AJ
 Sample : P0101524ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:33:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:32:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	465.3E6	164.4E6	51.058	51.086
2) SA Decachlor...	10.056	8.638	123.9E6	136.1E6	50.497	49.626
Target Compounds						
3) L1 AR-1016-1	5.521	4.726	134.9E6	51843655	500.111	502.042
4) L1 AR-1016-2	5.543	4.745	197.8E6	72270469	498.259	512.674
5) L1 AR-1016-3	5.606	4.920	128.2E6	39765886	510.233	504.992
6) L1 AR-1016-4	5.702	4.962	100.3E6	33242228	520.863	502.845
7) L1 AR-1016-5	5.997	5.175	96027789	42039253	525.737	511.838
31) L7 AR-1260-1	7.123	6.207	127.8E6	78048903	494.246	503.040
32) L7 AR-1260-2	7.380	6.394	129.5E6	92023271	492.099	522.516
33) L7 AR-1260-3	7.741	6.547	88394667	86099269	491.778	513.265
34) L7 AR-1260-4	7.966	7.018	84877632	73152631	483.623	505.614
35) L7 AR-1260-5	8.279	7.258	138.1E6	168.0E6	485.508	510.033



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 02:54
Operator : YP/AJ
Sample : PO101524ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:33:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:32:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

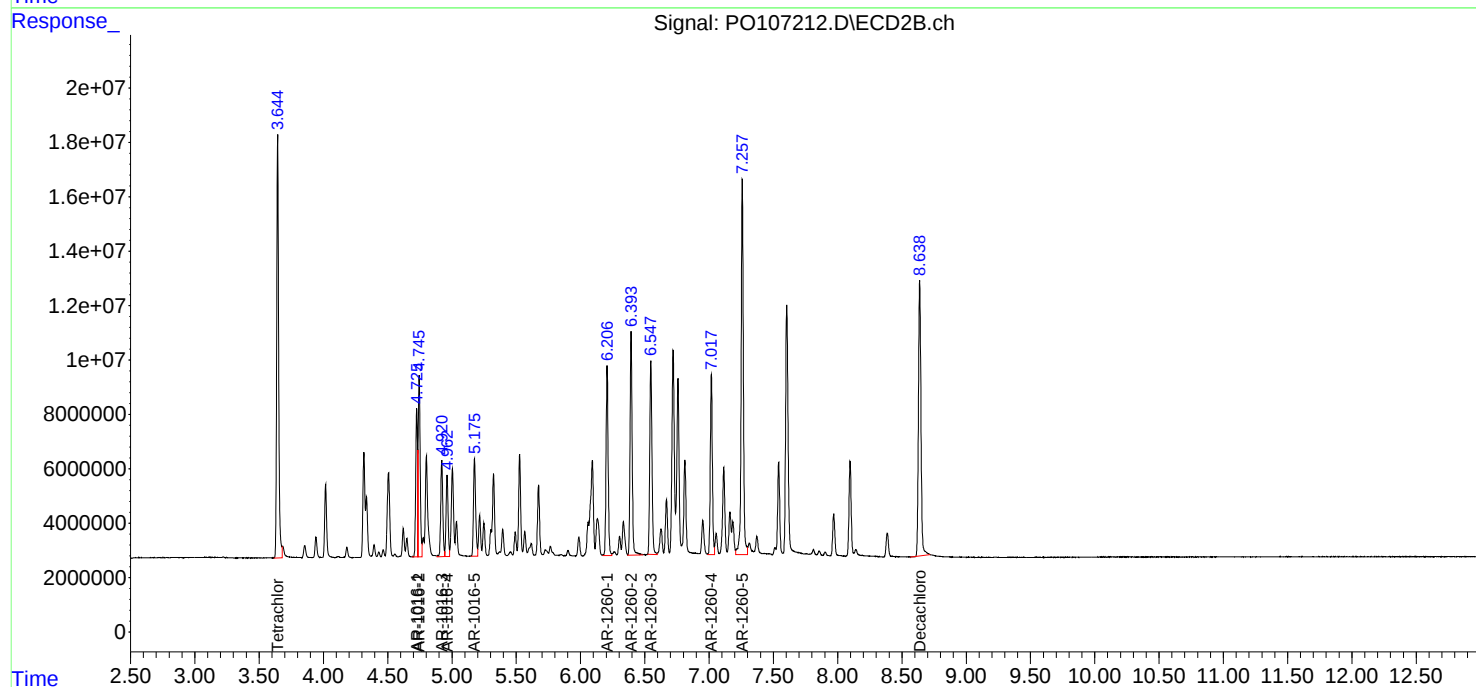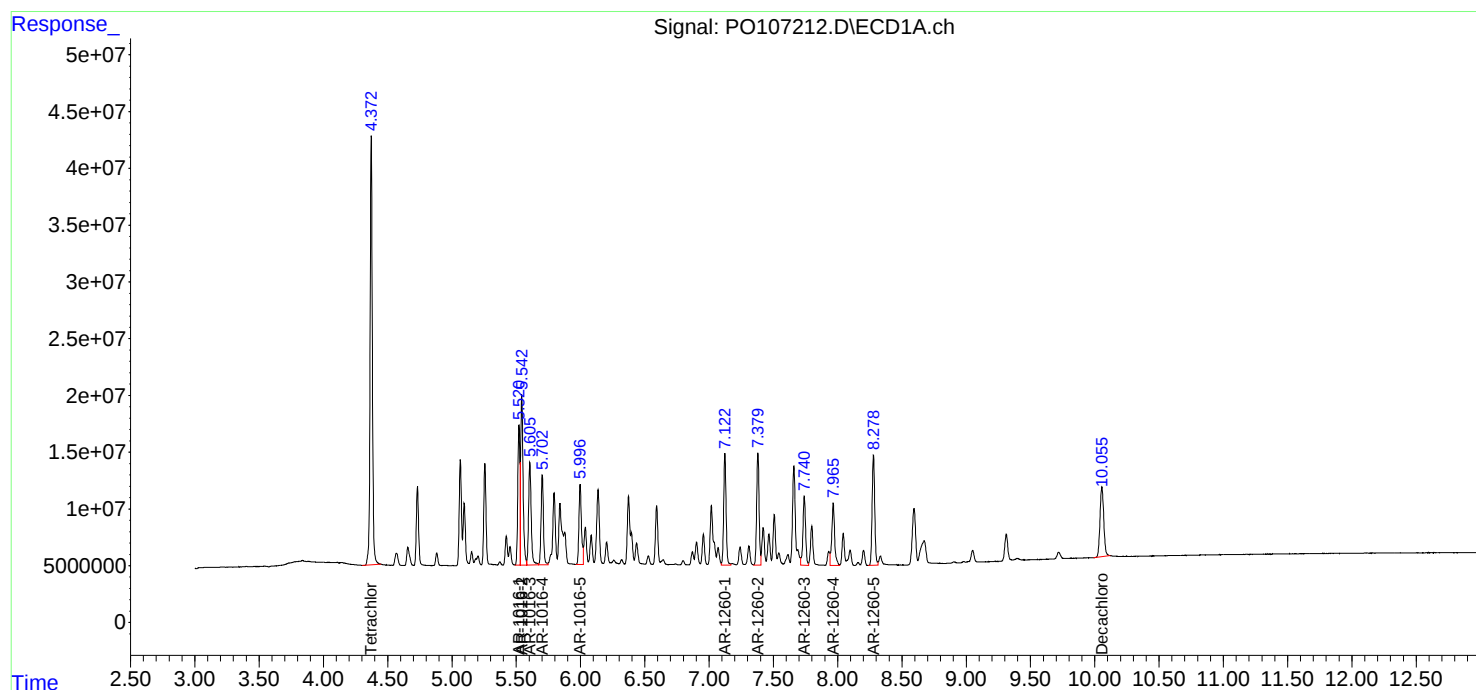

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 03:12
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:37:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:36:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	462.5E6	169.0E6	51.003	52.312
2) SA Decachlor...	10.058	8.637	124.4E6	137.6E6	50.838	50.298
Target Compounds						
16) L4 AR-1242-1	5.522	4.726	112.5E6	42391283	503.251	506.204
17) L4 AR-1242-2	5.544	4.745	161.7E6	59212746	499.677	512.049
18) L4 AR-1242-3	5.606	4.921	104.8E6	32647360	501.419	514.673
19) L4 AR-1242-4	5.703	5.004	80827975	32698937	505.157	510.527
20) L4 AR-1242-5	6.436	5.526	77500840	39282831	495.270	506.721



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 03:12
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:37:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:36:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

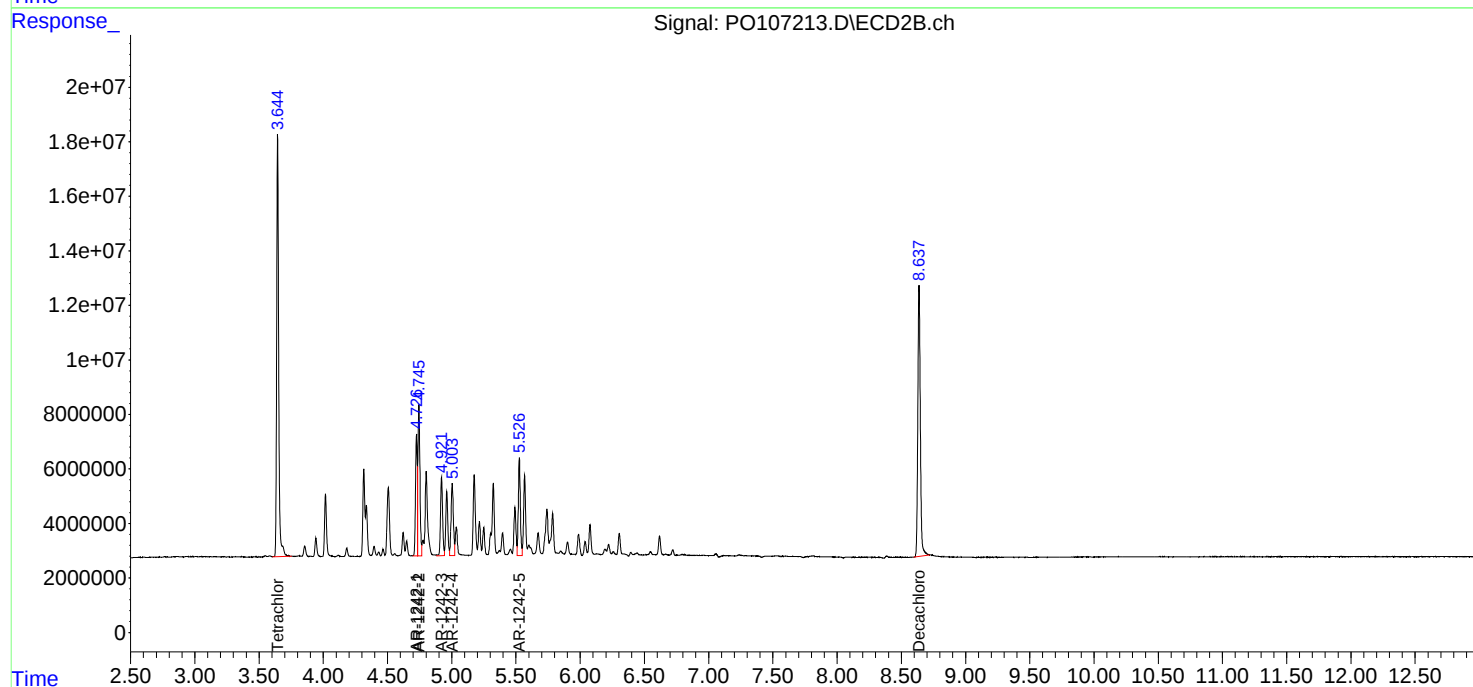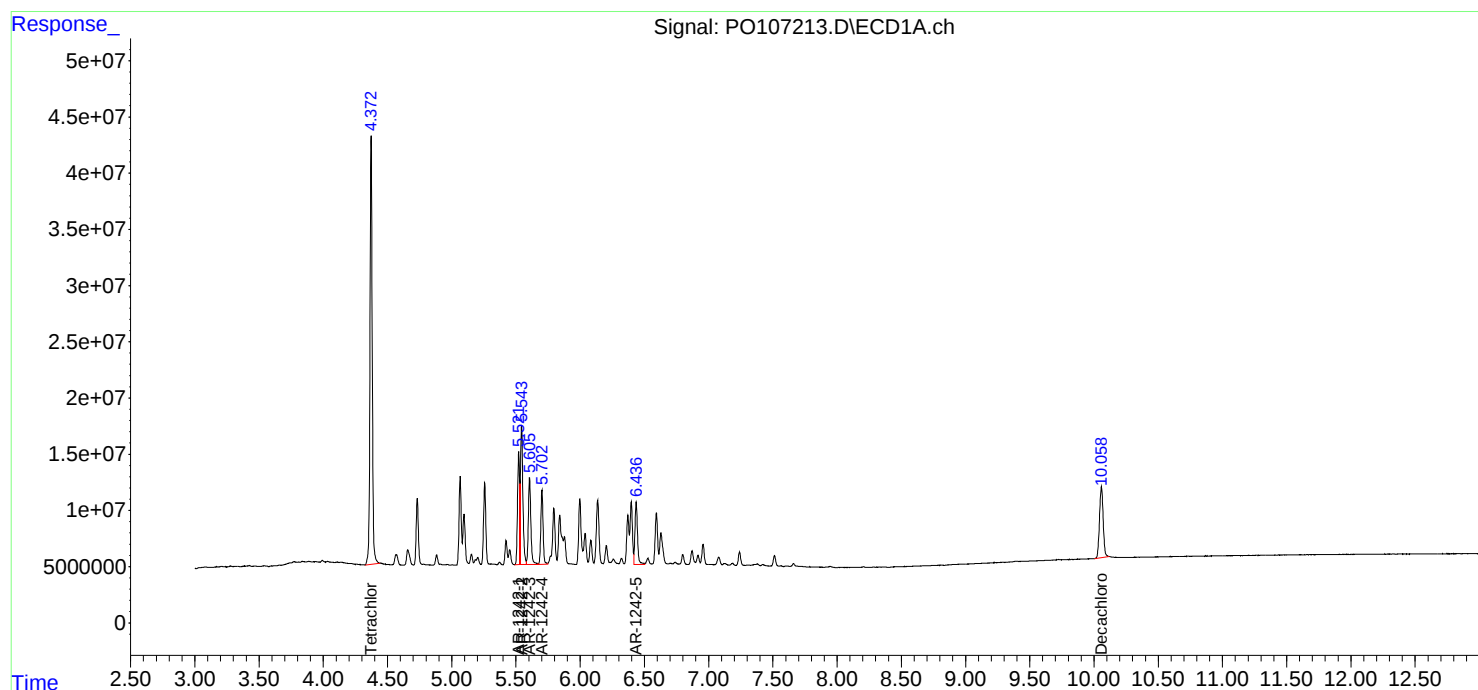

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 03:30
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:41:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:40:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	468.2E6	171.8E6	51.242	52.316
2) SA Decachlor...	10.056	8.637	126.4E6	139.3E6	51.882	50.991
Target Compounds						
21) L5 AR-1248-1	5.521	4.726	87306267	32470217	502.117	511.816
22) L5 AR-1248-2	5.794	4.962	126.0E6	46450269	498.018	507.736
23) L5 AR-1248-3	5.997	5.004	130.0E6	48736000	508.271	510.896
24) L5 AR-1248-4	6.397	5.175	129.0E6	57212370	500.494	510.195
25) L5 AR-1248-5	6.436	5.567	130.2E6	54714064	500.737	496.185



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 03:30
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:41:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:40:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

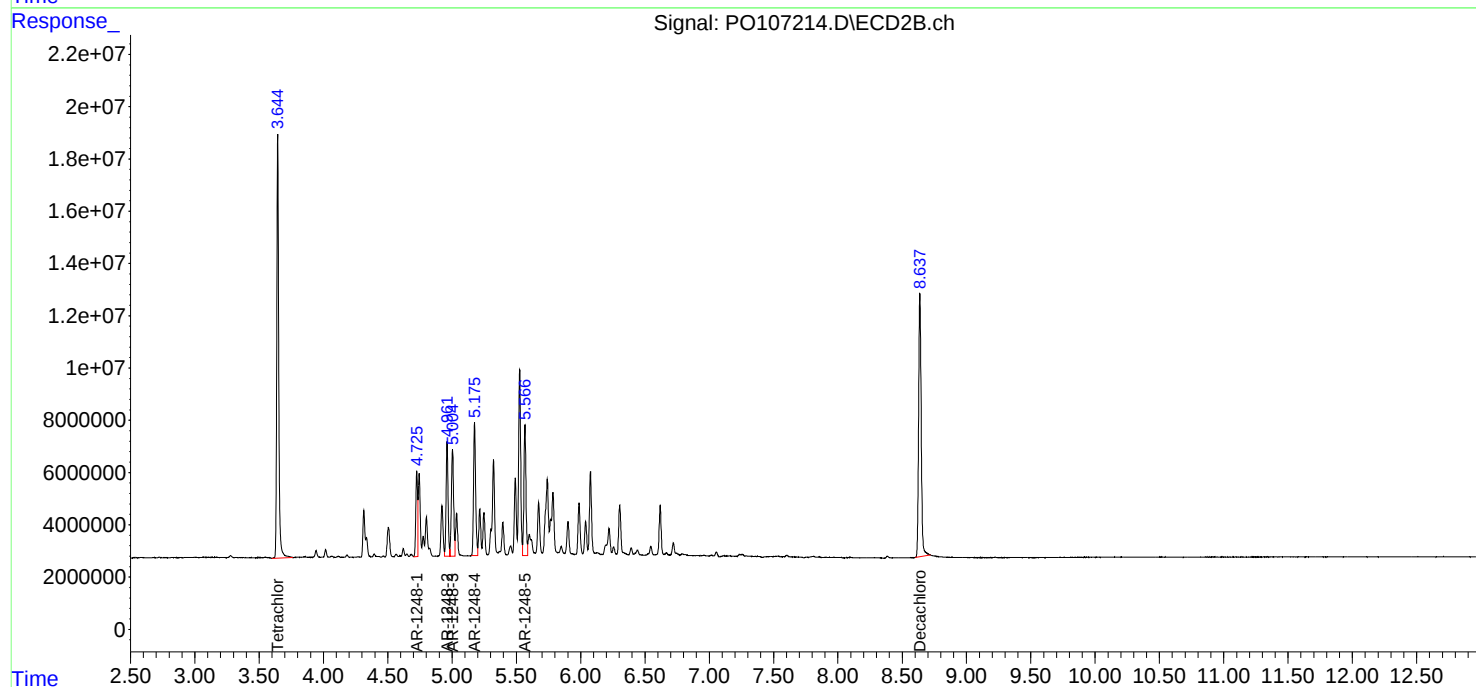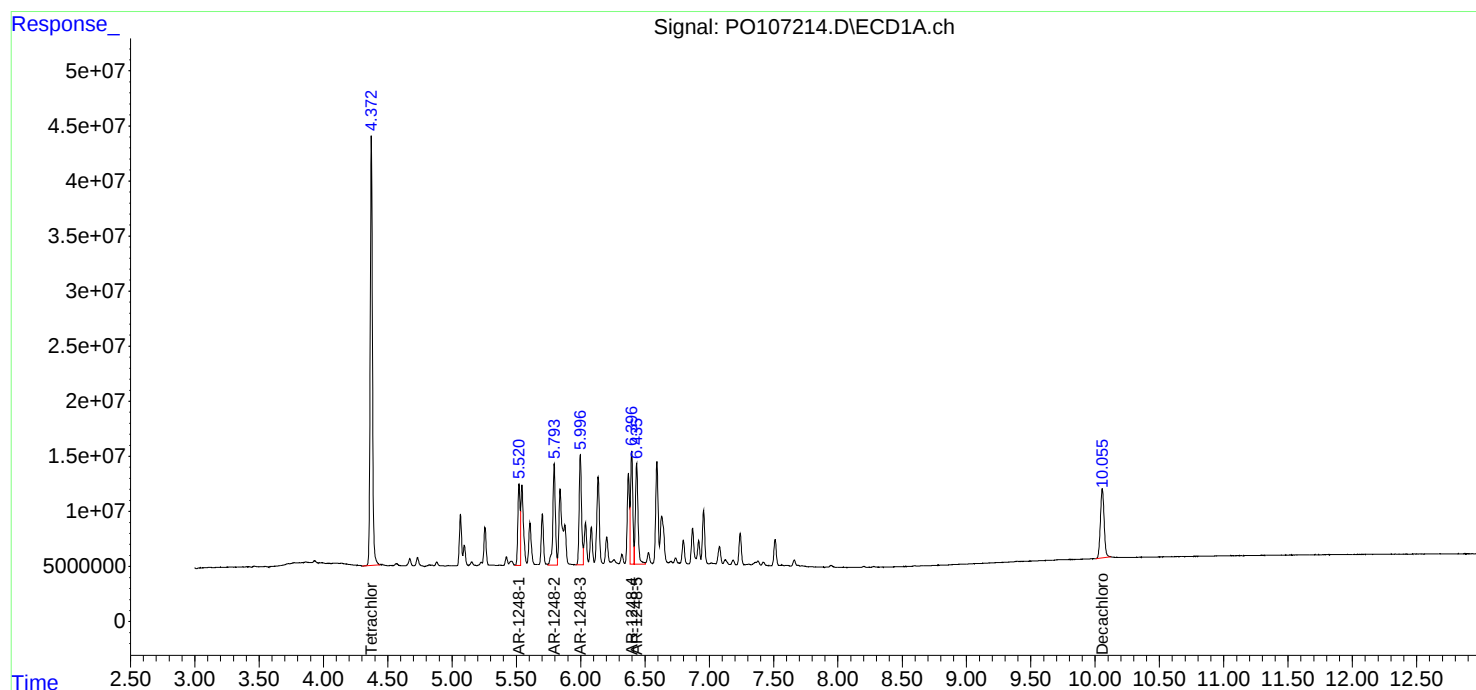

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 03:48
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:44:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:44:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	461.3E6	168.2E6	50.657	51.320
2) SA Decachlor...	10.057	8.638	125.1E6	138.4E6	51.131	50.597
Target Compounds						
26) L6 AR-1254-1	6.374	5.527	132.5E6	83096071	492.928	504.260
27) L6 AR-1254-2	6.592	5.673	186.6E6	72524753	494.424	500.299
28) L6 AR-1254-3	6.956	6.077	177.6E6	116.6E6	496.443	508.012
29) L6 AR-1254-4	7.242	6.304	112.6E6	65655140	490.851	507.289
30) L6 AR-1254-5	7.661	6.722	102.5E6	98535916	493.779	515.754



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 03:48
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:44:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:44:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

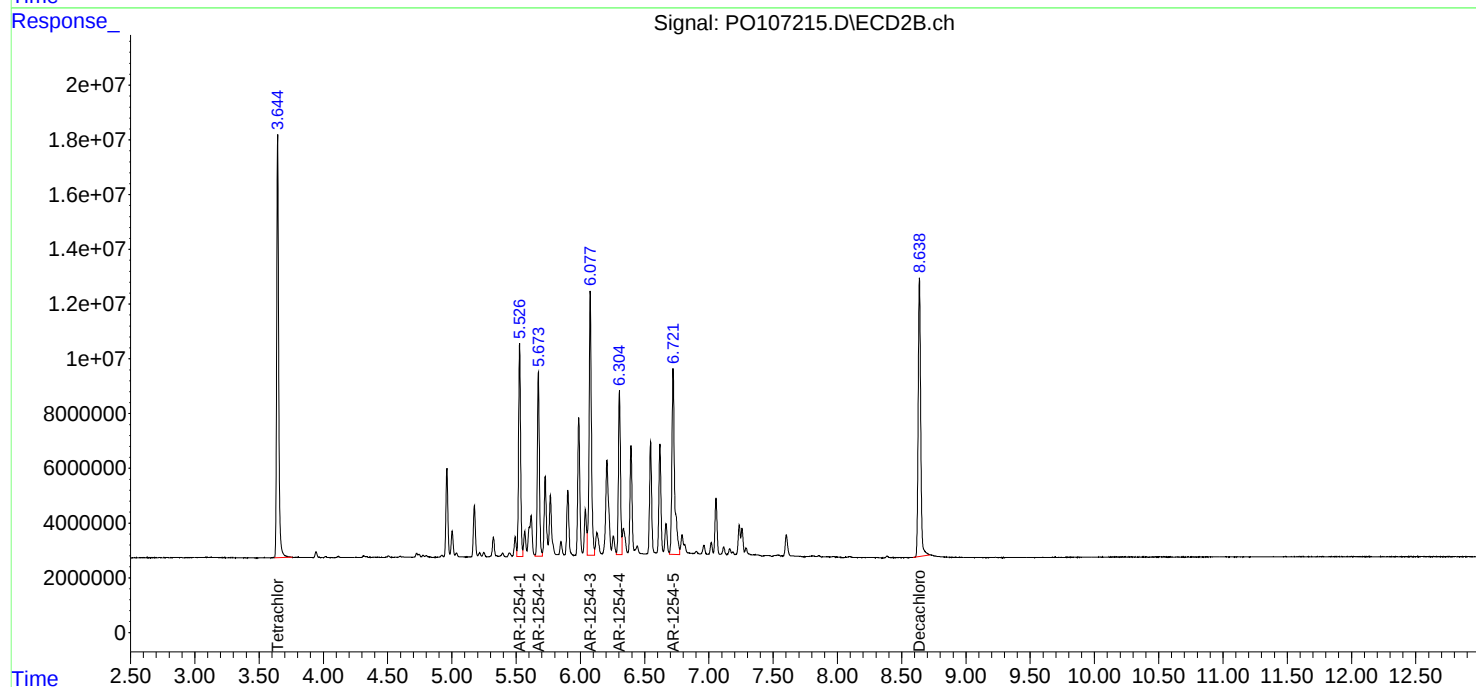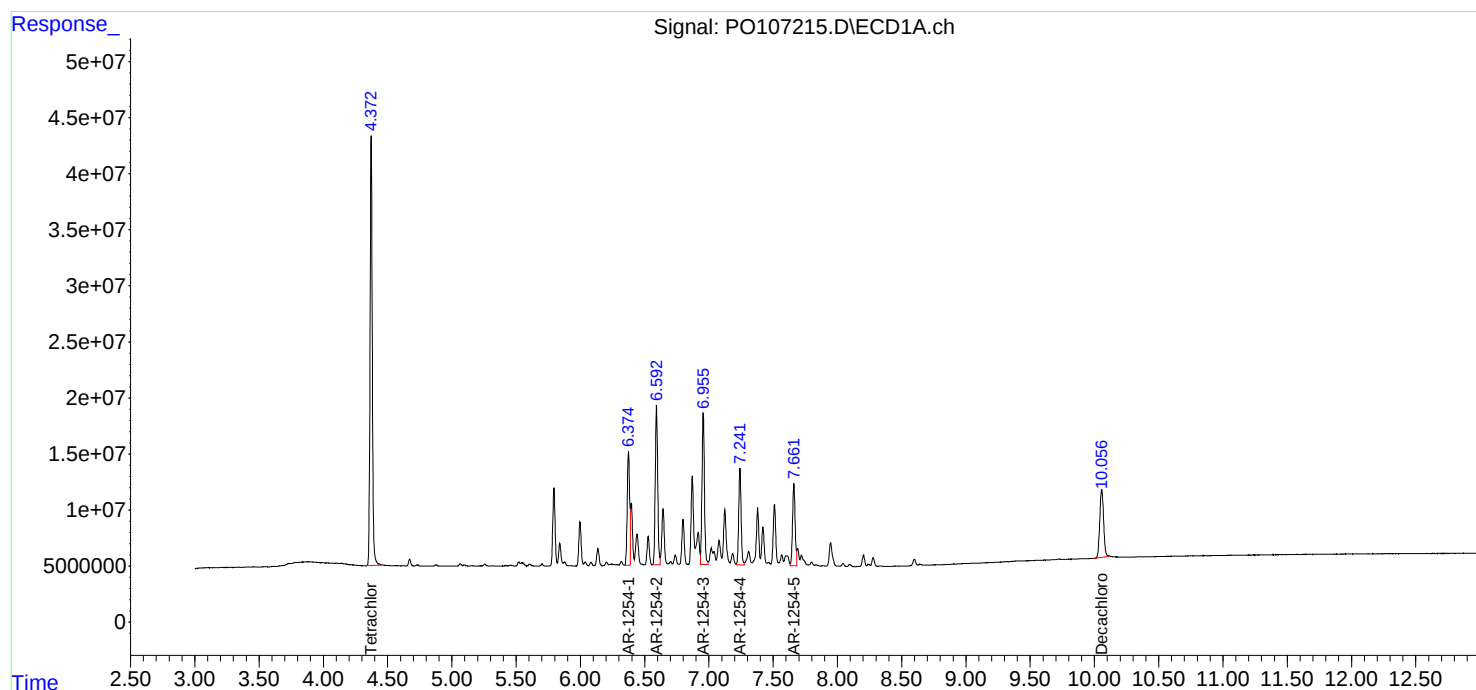

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101524\
 Data File : P0107216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 04:06
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO101524AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:22:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 02:38:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	461.5E6	169.8E6	49.559	49.696
2) SA Decachlor...	10.057	8.638	214.2E6	240.5E6	50.485	49.870
Target Compounds						
41) L9 AR-1268-1	8.588	7.541	182.7E6	207.4E6	501.152	501.118
42) L9 AR-1268-2	8.678	7.606	163.0E6	192.3E6	501.726	501.439
43) L9 AR-1268-3	8.907	7.812	141.7E6	170.9E6	501.280	503.353
44) L9 AR-1268-4	9.313	8.096	57558867	64279608	501.757	505.004
45) L9 AR-1268-5	9.721	8.385	423.5E6	510.6E6	499.926	501.994



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 04:06
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO101524AR1268

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:22:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 02:38:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

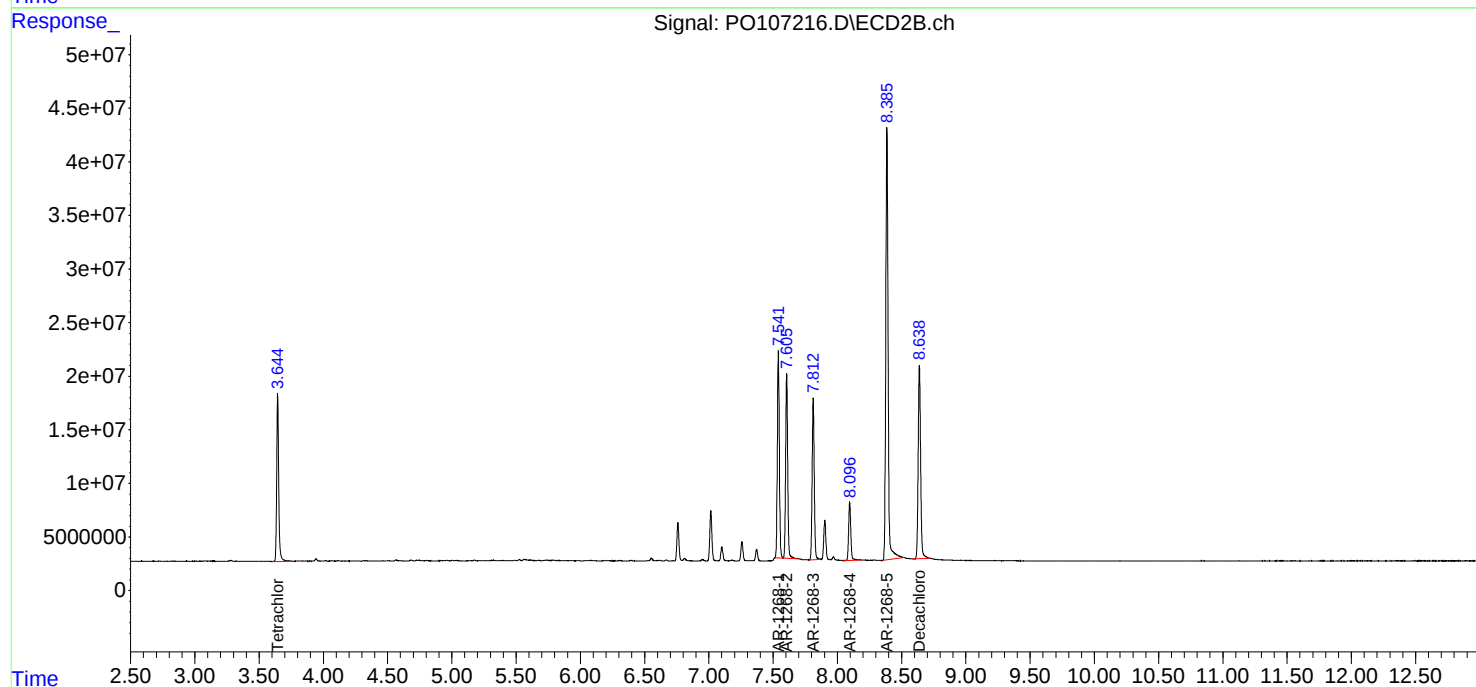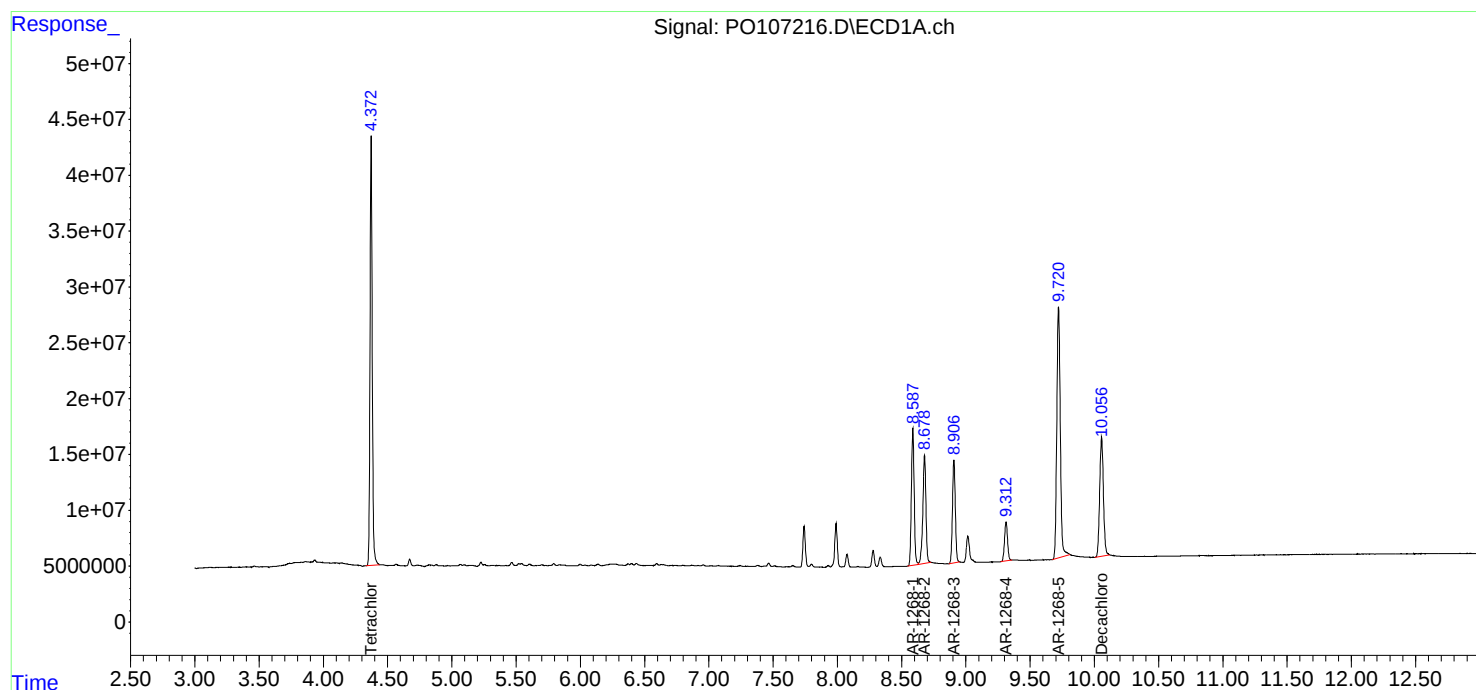



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Continuing Calib Date: 11/06/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 09:29 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.53	5.52	5.42	5.62	-0.01
Aroclor-1016-2	(2)	5.55	5.55	5.45	5.65	0.00
Aroclor-1016-3	(3)	5.61	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.71	5.70	5.60	5.80	-0.01
Aroclor-1016-5	(5)	6.00	6.00	5.90	6.10	0.00
Aroclor-1260-1	(1)	7.13	7.13	7.03	7.23	0.00
Aroclor-1260-2	(2)	7.39	7.38	7.28	7.48	-0.01
Aroclor-1260-3	(3)	7.75	7.74	7.64	7.84	-0.01
Aroclor-1260-4	(4)	7.98	7.97	7.87	8.07	-0.01
Aroclor-1260-5	(5)	8.29	8.28	8.18	8.38	-0.01
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.08	10.06	9.96	10.16	-0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Continuing Calib Date: 11/06/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 09:29 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.73	4.63	4.83	0.01
Aroclor-1016-2	(2)	4.74	4.75	4.65	4.85	0.01
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.17	5.18	5.08	5.28	0.01
Aroclor-1260-1	(1)	6.20	6.21	6.11	6.31	0.01
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.55	6.55	6.45	6.65	0.00
Aroclor-1260-4	(4)	7.02	7.02	6.92	7.12	0.00
Aroclor-1260-5	(5)	7.26	7.26	7.16	7.36	0.00
Tetrachloro-m-xylene		3.64	3.65	3.55	3.75	0.01
Decachlorobiphenyl		8.64	8.64	8.54	8.74	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL01 Date Analyzed: 11/06/2024

Lab Sample No.: AR1660CCC500 Data File : PO107726.D Time Analyzed: 09:29

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.525	5.423	5.623	511.290	500.000	2.3
Aroclor-1016-2	5.547	5.445	5.645	497.460	500.000	-0.5
Aroclor-1016-3	5.610	5.507	5.707	489.050	500.000	-2.2
Aroclor-1016-4	5.707	5.604	5.804	512.950	500.000	2.6
Aroclor-1016-5	6.002	5.899	6.099	511.100	500.000	2.2
Aroclor-1260-1	7.132	7.026	7.226	513.000	500.000	2.6
Aroclor-1260-2	7.389	7.282	7.482	542.700	500.000	8.5
Aroclor-1260-3	7.752	7.643	7.843	537.760	500.000	7.6
Aroclor-1260-4	7.977	7.868	8.068	552.670	500.000	10.5
Aroclor-1260-5	8.291	8.181	8.381	599.200	500.000	19.8
Decachlorobiphenyl	10.079	9.958	10.158	48.100	50.000	-3.8
Tetrachloro-m-xylene	4.373	4.274	4.474	51.680	50.000	3.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL01 Date Analyzed: 11/06/2024

Lab Sample No.: AR1660CCC500 Data File : PO107726.D Time Analyzed: 09:29

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.724	4.626	4.826	535.170	500.000	7.0
Aroclor-1016-2	4.743	4.645	4.845	548.800	500.000	9.8
Aroclor-1016-3	4.918	4.821	5.021	527.740	500.000	5.5
Aroclor-1016-4	4.960	4.862	5.062	488.290	500.000	-2.3
Aroclor-1016-5	5.174	5.076	5.276	523.130	500.000	4.6
Aroclor-1260-1	6.204	6.107	6.307	506.050	500.000	1.2
Aroclor-1260-2	6.392	6.294	6.494	533.470	500.000	6.7
Aroclor-1260-3	6.545	6.448	6.648	522.150	500.000	4.4
Aroclor-1260-4	7.017	6.918	7.118	519.510	500.000	3.9
Aroclor-1260-5	7.258	7.159	7.359	552.050	500.000	10.4
Decachlorobiphenyl	8.640	8.539	8.739	54.490	50.000	9.0
Tetrachloro-m-xylene	3.643	3.545	3.745	54.140	50.000	8.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 09:29
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 14:23:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.643	471.0E6	174.2E6	51.678	54.137
2) SA Decachlor...	10.079	8.640	118.0E6	149.4E6	48.104	54.493
Target Compounds						
3) L1 AR-1016-1	5.525	4.724	138.0E6	55264287	511.294	535.166
4) L1 AR-1016-2	5.547	4.743	197.4E6	77363781	497.458	548.805
5) L1 AR-1016-3	5.610	4.918	122.8E6	41557467	489.051	527.743
6) L1 AR-1016-4	5.707	4.960	98800866	32280302	512.953	488.294
7) L1 AR-1016-5	6.002	5.174	93353488	42966981	511.096	523.134
31) L7 AR-1260-1	7.132	6.204	132.7E6	78516248	512.996	506.052
32) L7 AR-1260-2	7.389	6.392	142.8E6	93952096	542.695	533.468
33) L7 AR-1260-3	7.752	6.545	96659887	87590361	537.761	522.154
34) L7 AR-1260-4	7.977	7.017	96994898	75163259	552.665	519.511
35) L7 AR-1260-5	8.291	7.258	170.4E6	181.9E6	599.198	552.051



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 09:29
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 14:23:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

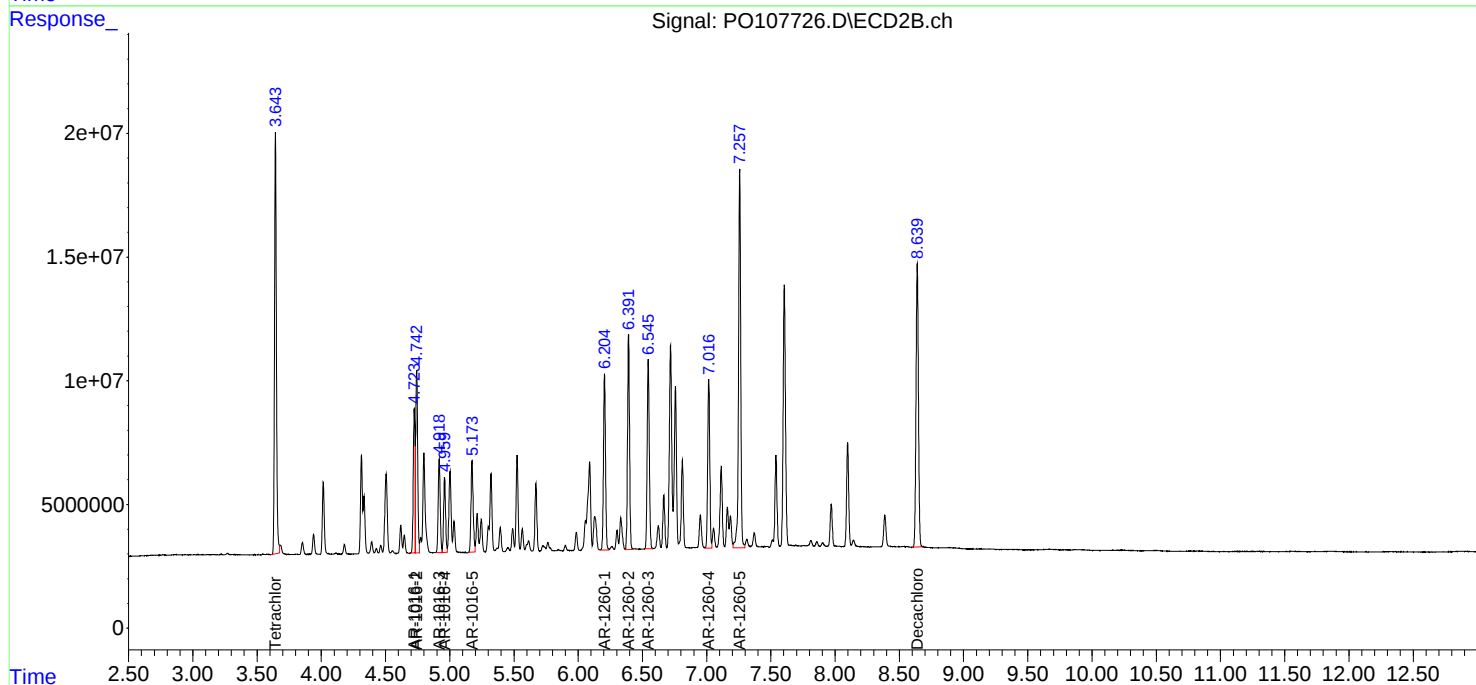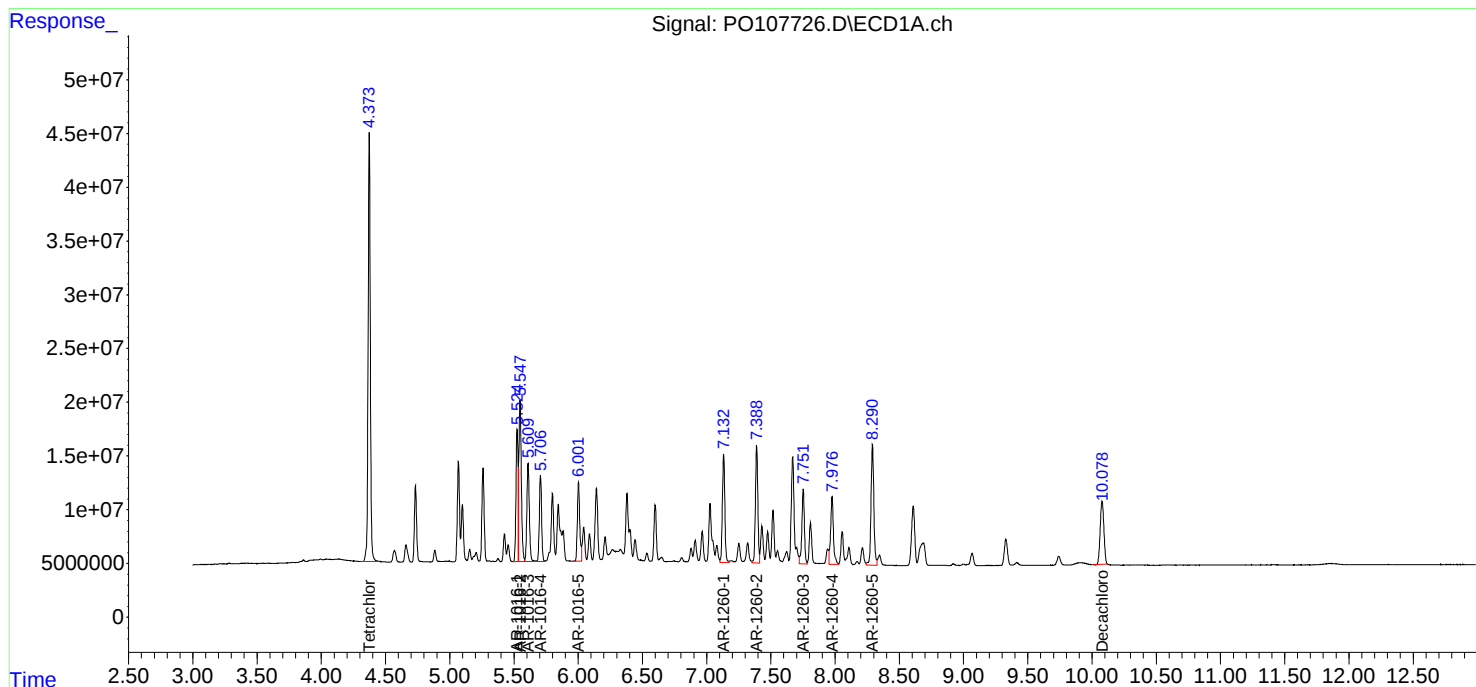



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Continuing Calib Date: 11/06/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 16:54 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.52	5.52	5.42	5.62	0.00
Aroclor-1016-2	(2)	5.55	5.55	5.45	5.65	0.00
Aroclor-1016-3	(3)	5.61	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.71	5.70	5.60	5.80	-0.01
Aroclor-1016-5	(5)	6.00	6.00	5.90	6.10	0.00
Aroclor-1260-1	(1)	7.13	7.13	7.03	7.23	0.00
Aroclor-1260-2	(2)	7.39	7.38	7.28	7.48	-0.01
Aroclor-1260-3	(3)	7.75	7.74	7.64	7.84	-0.01
Aroclor-1260-4	(4)	7.98	7.97	7.87	8.07	0.00
Aroclor-1260-5	(5)	8.29	8.28	8.18	8.38	-0.01
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.07	10.06	9.96	10.16	-0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Continuing Calib Date: 11/06/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 16:54 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.73	4.63	4.83	0.01
Aroclor-1016-2	(2)	4.74	4.75	4.65	4.85	0.01
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.17	5.18	5.08	5.28	0.01
Aroclor-1260-1	(1)	6.20	6.21	6.11	6.31	0.01
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.55	6.45	6.65	0.01
Aroclor-1260-4	(4)	7.02	7.02	6.92	7.12	0.00
Aroclor-1260-5	(5)	7.26	7.26	7.16	7.36	0.00
Tetrachloro-m-xylene		3.64	3.65	3.55	3.75	0.01
Decachlorobiphenyl		8.64	8.64	8.54	8.74	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL02 Date Analyzed: 11/06/2024

Lab Sample No.: AR1660CCC500 Data File : PO107741.D Time Analyzed: 16:54

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.524	5.423	5.623	463.130	500.000	-7.4
Aroclor-1016-2	5.546	5.445	5.645	444.160	500.000	-11.2
Aroclor-1016-3	5.608	5.507	5.707	441.970	500.000	-11.6
Aroclor-1016-4	5.706	5.604	5.804	462.710	500.000	-7.5
Aroclor-1016-5	6.001	5.899	6.099	463.090	500.000	-7.4
Aroclor-1260-1	7.130	7.026	7.226	456.620	500.000	-8.7
Aroclor-1260-2	7.387	7.282	7.482	464.280	500.000	-7.1
Aroclor-1260-3	7.750	7.643	7.843	448.010	500.000	-10.4
Aroclor-1260-4	7.975	7.868	8.068	465.650	500.000	-6.9
Aroclor-1260-5	8.289	8.181	8.381	482.090	500.000	-3.6
Decachlorobiphenyl	10.074	9.958	10.158	43.960	50.000	-12.1
Tetrachloro-m-xylene	4.372	4.274	4.474	52.670	50.000	5.3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL02 Date Analyzed: 11/06/2024

Lab Sample No.: AR1660CCC500 Data File : PO107741.D Time Analyzed: 16:54

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.723	4.626	4.826	534.360	500.000	6.9
Aroclor-1016-2	4.742	4.645	4.845	554.800	500.000	11.0
Aroclor-1016-3	4.918	4.821	5.021	533.240	500.000	6.6
Aroclor-1016-4	4.959	4.862	5.062	489.970	500.000	-2.0
Aroclor-1016-5	5.173	5.076	5.276	523.370	500.000	4.7
Aroclor-1260-1	6.204	6.107	6.307	496.980	500.000	-0.6
Aroclor-1260-2	6.391	6.294	6.494	518.510	500.000	3.7
Aroclor-1260-3	6.544	6.448	6.648	492.660	500.000	-1.5
Aroclor-1260-4	7.016	6.918	7.118	462.170	500.000	-7.6
Aroclor-1260-5	7.256	7.159	7.359	474.270	500.000	-5.1
Decachlorobiphenyl	8.637	8.539	8.739	41.590	50.000	-16.8
Tetrachloro-m-xylene	3.643	3.545	3.745	53.650	50.000	7.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 16:54
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:38:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.643	480.0E6	172.7E6	52.665	53.647
2) SA Decachlor...	10.074	8.637	107.8E6	114.0E6	43.957	41.586
Target Compounds						
3) L1 AR-1016-1	5.524	4.723	125.0E6	55181453	463.132	534.364
4) L1 AR-1016-2	5.546	4.742	176.3E6	78209203	444.165	554.802
5) L1 AR-1016-3	5.608	4.918	111.0E6	41989944	441.970	533.235
6) L1 AR-1016-4	5.706	4.959	89124288	32391058	462.714	489.969
7) L1 AR-1016-5	6.001	5.173	84585627	42986342	463.093	523.369
31) L7 AR-1260-1	7.130	6.204	118.1E6	77108982	456.618	496.982
32) L7 AR-1260-2	7.387	6.391	122.2E6	91318286	464.276	518.513
33) L7 AR-1260-3	7.750	6.544	80527891	82643460	448.012	492.664
34) L7 AR-1260-4	7.975	7.016	81723455	66867148	465.650	462.170
35) L7 AR-1260-5	8.289	7.256	137.1E6	156.2E6	482.089	474.267



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 16:54
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:38:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

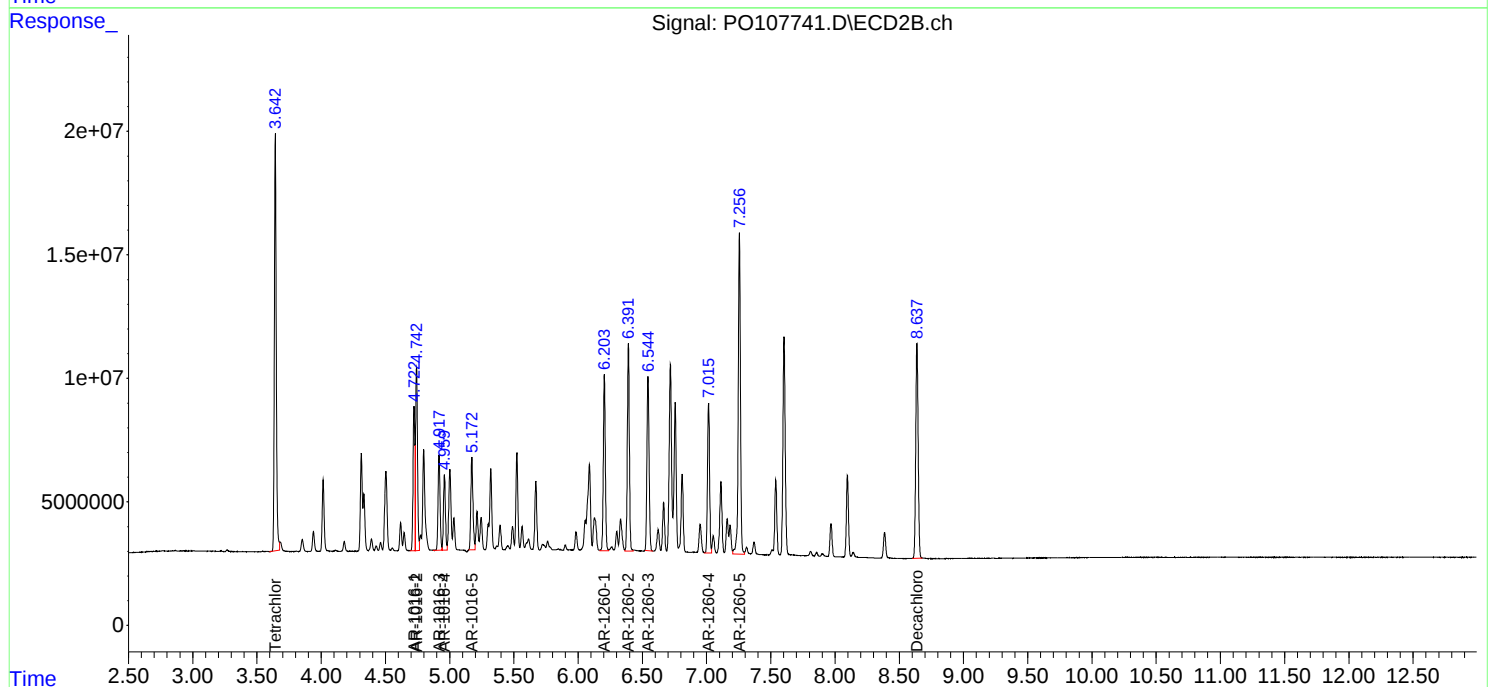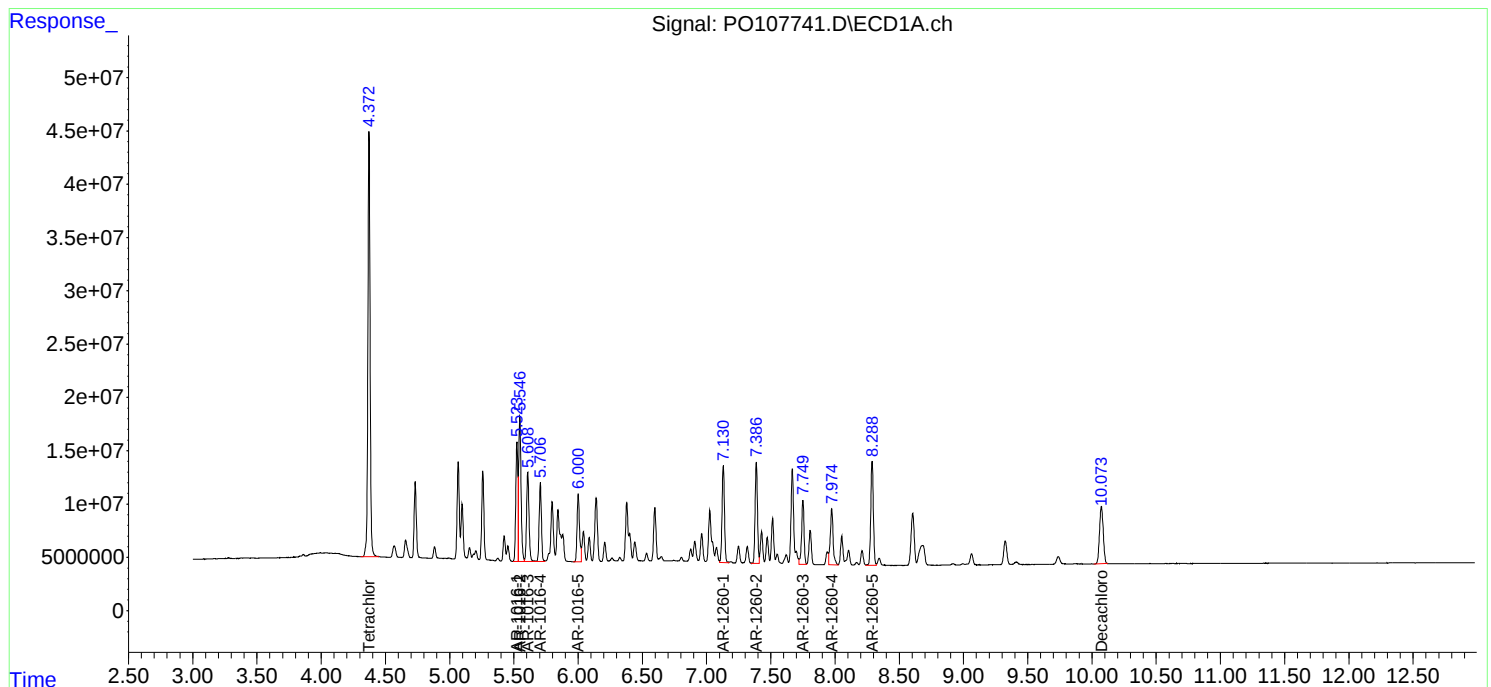



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Continuing Calib Date: 11/06/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 21:42 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Aroclor-1016-1	(1)	5.52	5.52	5.42	5.62	0.00
Aroclor-1016-2	(2)	5.55	5.55	5.45	5.65	0.00
Aroclor-1016-3	(3)	5.61	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.71	5.70	5.60	5.80	0.00
Aroclor-1016-5	(5)	6.00	6.00	5.90	6.10	0.00
Aroclor-1260-1	(1)	7.13	7.13	7.03	7.23	0.00
Aroclor-1260-2	(2)	7.39	7.38	7.28	7.48	-0.01
Aroclor-1260-3	(3)	7.75	7.74	7.64	7.84	-0.01
Aroclor-1260-4	(4)	7.98	7.97	7.87	8.07	-0.01
Aroclor-1260-5	(5)	8.29	8.28	8.18	8.38	-0.01
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.08	10.06	9.96	10.16	-0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Continuing Calib Date: 11/06/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 21:42 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.73	4.63	4.83	0.01
Aroclor-1016-2	(2)	4.74	4.75	4.65	4.85	0.01
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.17	5.18	5.08	5.28	0.01
Aroclor-1260-1	(1)	6.21	6.21	6.11	6.31	0.01
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.55	6.55	6.45	6.65	0.00
Aroclor-1260-4	(4)	7.02	7.02	6.92	7.12	0.00
Aroclor-1260-5	(5)	7.26	7.26	7.16	7.36	0.00
Tetrachloro-m-xylene		3.64	3.65	3.55	3.75	0.01
Decachlorobiphenyl		8.64	8.64	8.54	8.74	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL03 Date Analyzed: 11/06/2024

Lab Sample No.: AR1660CCC500 Data File : PO107756.D Time Analyzed: 21:42

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.523	5.423	5.623	521.970	500.000	4.4
Aroclor-1016-2	5.546	5.445	5.645	513.220	500.000	2.6
Aroclor-1016-3	5.608	5.507	5.707	503.460	500.000	0.7
Aroclor-1016-4	5.705	5.604	5.804	530.050	500.000	6.0
Aroclor-1016-5	6.001	5.899	6.099	533.120	500.000	6.6
Aroclor-1260-1	7.132	7.026	7.226	487.030	500.000	-2.6
Aroclor-1260-2	7.388	7.282	7.482	514.800	500.000	3.0
Aroclor-1260-3	7.751	7.643	7.843	532.710	500.000	6.5
Aroclor-1260-4	7.976	7.868	8.068	568.210	500.000	13.6
Aroclor-1260-5	8.290	8.181	8.381	561.040	500.000	12.2
Decachlorobiphenyl	10.077	9.958	10.158	47.560	50.000	-4.9
Tetrachloro-m-xylene	4.372	4.274	4.474	52.470	50.000	4.9



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL03 Date Analyzed: 11/06/2024

Lab Sample No.: AR1660CCC500 Data File : PO107756.D Time Analyzed: 21:42

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.724	4.626	4.826	531.640	500.000	6.3
Aroclor-1016-2	4.743	4.645	4.845	551.000	500.000	10.2
Aroclor-1016-3	4.919	4.821	5.021	530.220	500.000	6.0
Aroclor-1016-4	4.960	4.862	5.062	490.360	500.000	-1.9
Aroclor-1016-5	5.174	5.076	5.276	523.760	500.000	4.8
Aroclor-1260-1	6.205	6.107	6.307	511.170	500.000	2.2
Aroclor-1260-2	6.392	6.294	6.494	542.160	500.000	8.4
Aroclor-1260-3	6.546	6.448	6.648	529.960	500.000	6.0
Aroclor-1260-4	7.017	6.918	7.118	530.010	500.000	6.0
Aroclor-1260-5	7.258	7.159	7.359	565.090	500.000	13.0
Decachlorobiphenyl	8.639	8.539	8.739	54.600	50.000	9.2
Tetrachloro-m-xylene	3.643	3.545	3.745	53.910	50.000	7.8

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107756.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 21:42
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:48:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.643	478.2E6	173.5E6	52.472	53.915
2) SA Decachlor...	10.077	8.639	116.7E6	149.7E6	47.560	54.597
Target Compounds						
3) L1 AR-1016-1	5.523	4.724	140.8E6	54900264	521.975	531.641
4) L1 AR-1016-2	5.546	4.743	203.7E6	77673539	513.224	551.002
5) L1 AR-1016-3	5.608	4.919	126.5E6	41752668	503.458	530.222
6) L1 AR-1016-4	5.705	4.960	102.1E6	32417149	530.050	490.364
7) L1 AR-1016-5	6.001	5.174	97376331	43018414	533.120	523.760
31) L7 AR-1260-1	7.132	6.205	125.9E6	79310389	487.032	511.170
32) L7 AR-1260-2	7.388	6.392	135.5E6	95482454	514.805	542.158
33) L7 AR-1260-3	7.751	6.546	95751685	88900433	532.708	529.964
34) L7 AR-1260-4	7.976	7.017	99723075	76682351	568.210	530.011
35) L7 AR-1260-5	8.290	7.258	159.6E6	186.2E6	561.042	565.085



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107756.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 21:42
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:48:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

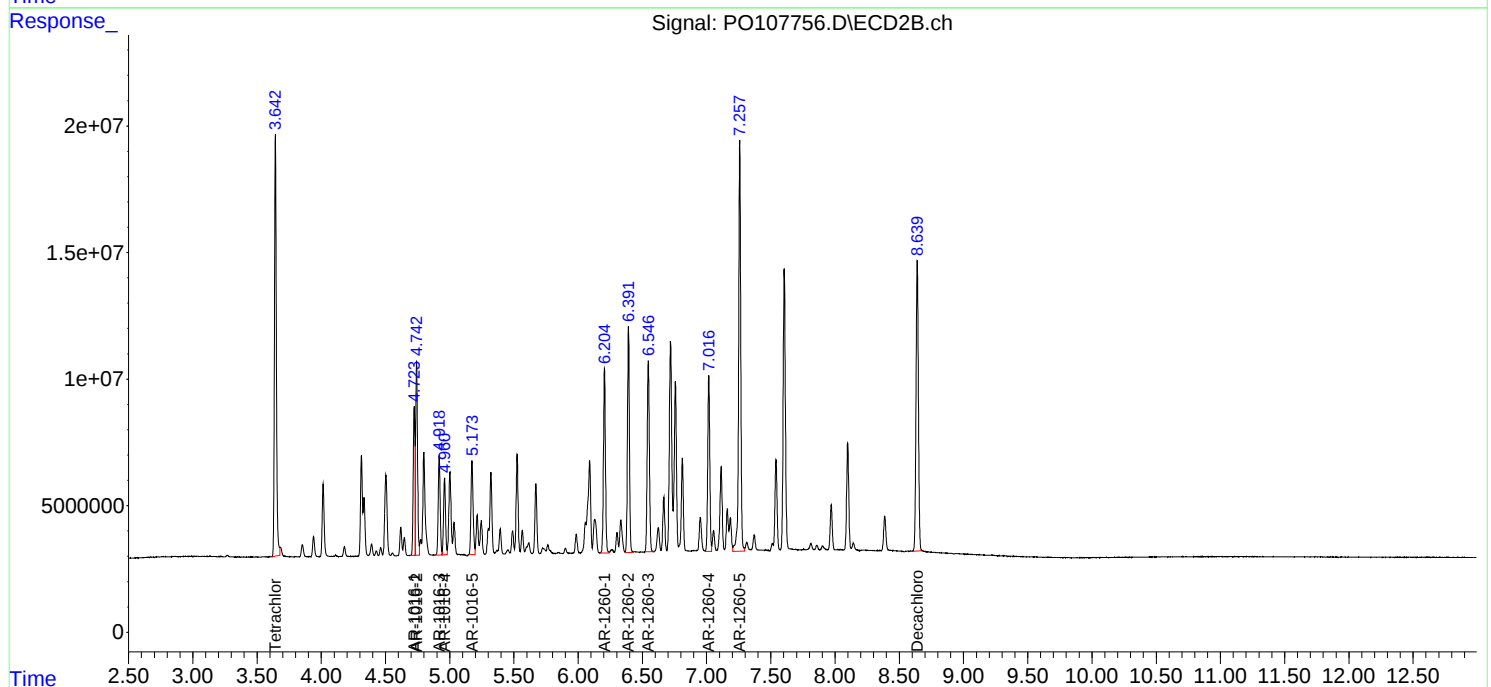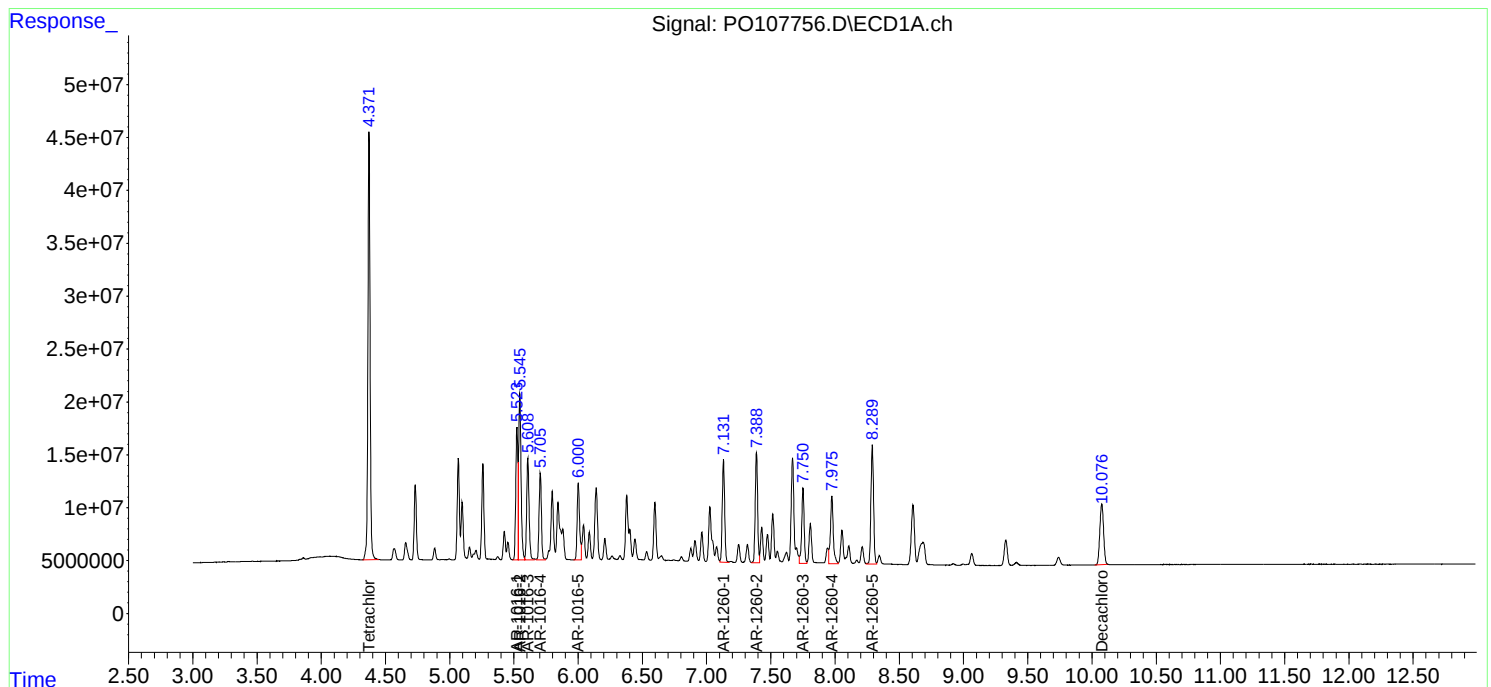



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Continuing Calib Date: 11/07/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 00:20 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.52	5.52	5.42	5.62	0.00
Aroclor-1016-2	(2)	5.55	5.55	5.45	5.65	0.00
Aroclor-1016-3	(3)	5.61	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.71	5.70	5.60	5.80	-0.01
Aroclor-1016-5	(5)	6.00	6.00	5.90	6.10	0.00
Aroclor-1260-1	(1)	7.13	7.13	7.03	7.23	0.00
Aroclor-1260-2	(2)	7.39	7.38	7.28	7.48	-0.01
Aroclor-1260-3	(3)	7.75	7.74	7.64	7.84	-0.01
Aroclor-1260-4	(4)	7.98	7.97	7.87	8.07	-0.01
Aroclor-1260-5	(5)	8.29	8.28	8.18	8.38	-0.01
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.08	10.06	9.96	10.16	-0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Continuing Calib Date: 11/07/2024 Initial Calibration Date(s): 10/15/2024 10/16/2024

Continuing Calib Time: 00:20 Initial Calibration Time(s): 18:27 02:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.73	4.63	4.83	0.01
Aroclor-1016-2	(2)	4.74	4.75	4.65	4.85	0.01
Aroclor-1016-3	(3)	4.92	4.92	4.82	5.02	0.00
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.17	5.18	5.08	5.28	0.01
Aroclor-1260-1	(1)	6.20	6.21	6.11	6.31	0.01
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.55	6.55	6.45	6.65	0.00
Aroclor-1260-4	(4)	7.02	7.02	6.92	7.12	0.00
Aroclor-1260-5	(5)	7.26	7.26	7.16	7.36	0.00
Tetrachloro-m-xylene		3.64	3.65	3.55	3.75	0.01
Decachlorobiphenyl		8.64	8.64	8.54	8.74	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL04 Date Analyzed: 11/07/2024

Lab Sample No.: AR1660CCC500 Data File : PO107763.D Time Analyzed: 00:20

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.523	5.423	5.623	547.580	500.000	9.5
Aroclor-1016-2	5.546	5.445	5.645	529.750	500.000	6.0
Aroclor-1016-3	5.608	5.507	5.707	527.770	500.000	5.6
Aroclor-1016-4	5.706	5.604	5.804	552.330	500.000	10.5
Aroclor-1016-5	6.001	5.899	6.099	549.630	500.000	9.9
Aroclor-1260-1	7.131	7.026	7.226	525.580	500.000	5.1
Aroclor-1260-2	7.388	7.282	7.482	540.410	500.000	8.1
Aroclor-1260-3	7.750	7.643	7.843	537.840	500.000	7.6
Aroclor-1260-4	7.976	7.868	8.068	568.050	500.000	13.6
Aroclor-1260-5	8.290	8.181	8.381	579.820	500.000	16.0
Decachlorobiphenyl	10.077	9.958	10.158	48.730	50.000	-2.5
Tetrachloro-m-xylene	4.372	4.274	4.474	53.790	50.000	7.6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 10/15/2024 10/15/2024

Client Sample No.: CCAL04 Date Analyzed: 11/07/2024

Lab Sample No.: AR1660CCC500 Data File : PO107763.D Time Analyzed: 00:20

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.723	4.626	4.826	549.090	500.000	9.8
Aroclor-1016-2	4.742	4.645	4.845	562.330	500.000	12.5
Aroclor-1016-3	4.918	4.821	5.021	540.540	500.000	8.1
Aroclor-1016-4	4.960	4.862	5.062	495.890	500.000	-0.8
Aroclor-1016-5	5.173	5.076	5.276	536.380	500.000	7.3
Aroclor-1260-1	6.204	6.107	6.307	525.020	500.000	5.0
Aroclor-1260-2	6.392	6.294	6.494	553.370	500.000	10.7
Aroclor-1260-3	6.545	6.448	6.648	536.080	500.000	7.2
Aroclor-1260-4	7.016	6.918	7.118	536.010	500.000	7.2
Aroclor-1260-5	7.257	7.159	7.359	565.900	500.000	13.2
Decachlorobiphenyl	8.639	8.539	8.739	55.530	50.000	11.1
Tetrachloro-m-xylene	3.642	3.545	3.745	55.140	50.000	10.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 00:20
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:52:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.642	490.2E6	177.5E6	53.790	55.140
2) SA Decachlor...	10.077	8.639	119.5E6	152.2E6	48.727	55.530
Target Compounds						
3) L1 AR-1016-1	5.523	4.723	147.7E6	56701828	547.582	549.087
4) L1 AR-1016-2	5.546	4.742	210.2E6	79270194	529.749	562.329
5) L1 AR-1016-3	5.608	4.918	132.6E6	42565204	527.775	540.540
6) L1 AR-1016-4	5.706	4.960	106.4E6	32782481	552.335	495.890
7) L1 AR-1016-5	6.001	5.173	100.4E6	44054819	549.631	536.378
31) L7 AR-1260-1	7.131	6.204	135.9E6	81459115	525.581	525.019
32) L7 AR-1260-2	7.388	6.392	142.2E6	97457195	540.407	553.371
33) L7 AR-1260-3	7.750	6.545	96673666	89926773	537.837	536.082
34) L7 AR-1260-4	7.976	7.016	99695059	77549788	568.050	536.006
35) L7 AR-1260-5	8.290	7.257	164.9E6	186.4E6	579.820	565.902



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 00:20
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:52:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

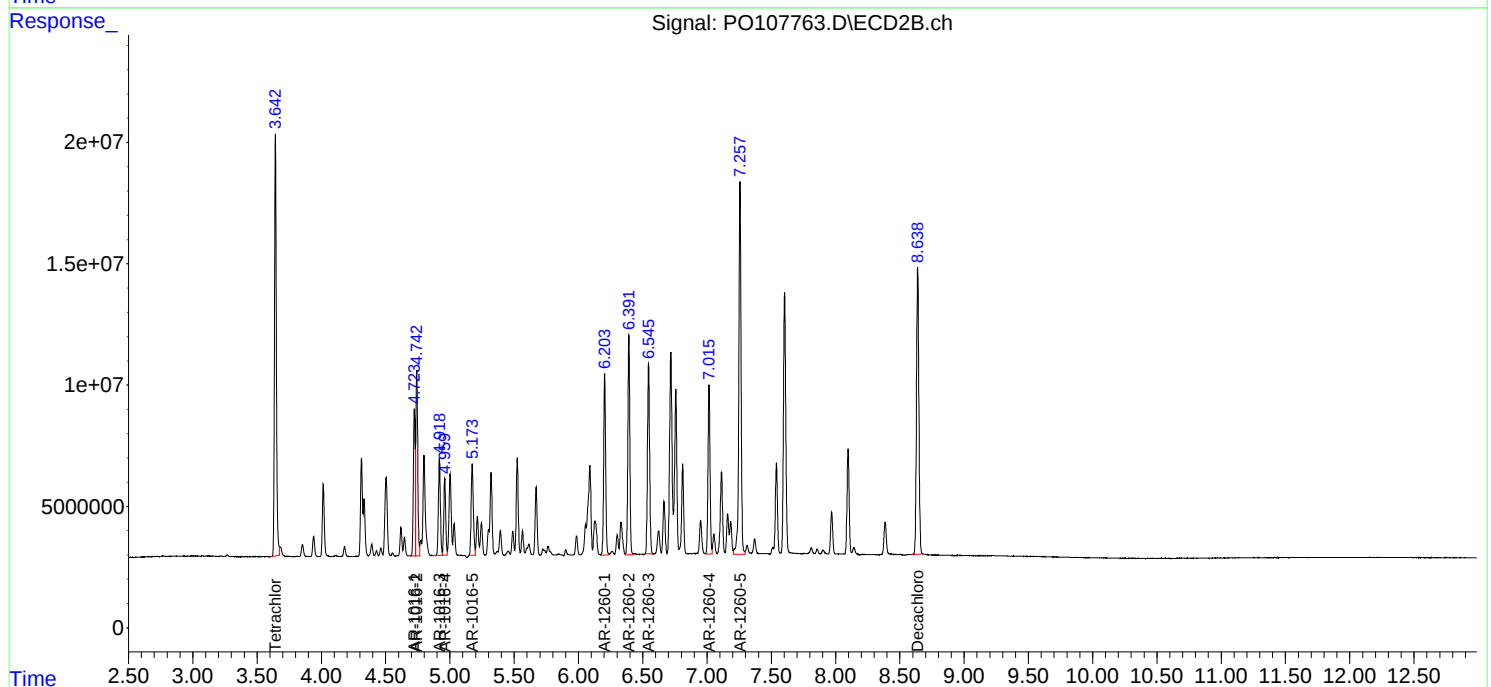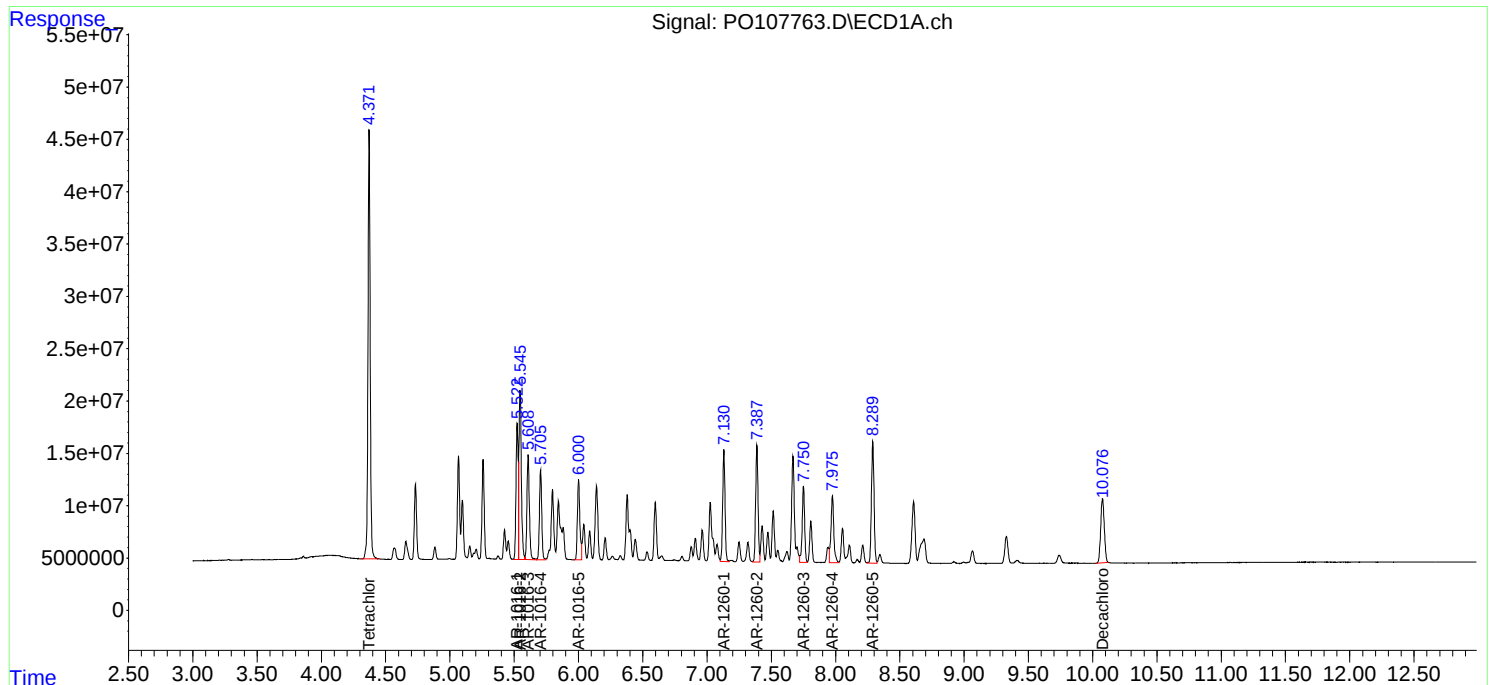

Analytical Sequence

Client: Portal Partners Tri-Venture	SDG No.: P4718
Project: Amtrak Sawtooth Bridges 2024	Instrument ID: ECD_O
GC Column: ZB-MR1	ID: 0.32 (mm) Inst. Calib. Date(s): 10/15/2024 10/15/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	10/15/2024	18:08	PO107183.D	10.06	4.37
AR1660ICC1000	AR1660ICC1000	10/15/2024	18:27	PO107184.D	10.06	4.37
AR1660ICC750	AR1660ICC750	10/15/2024	18:45	PO107185.D	10.06	4.37
AR1660ICC500	AR1660ICC500	10/15/2024	19:03	PO107186.D	10.06	4.37
AR1660ICC250	AR1660ICC250	10/15/2024	19:21	PO107187.D	10.06	4.37
AR1660ICC050	AR1660ICC050	10/15/2024	19:39	PO107188.D	10.06	4.37
AR1221ICC500	AR1221ICC500	10/15/2024	19:57	PO107189.D	10.06	4.37
AR1232ICC500	AR1232ICC500	10/15/2024	20:15	PO107190.D	10.06	4.37
AR1242ICC1000	AR1242ICC1000	10/15/2024	20:34	PO107191.D	10.06	4.37
AR1242ICC750	AR1242ICC750	10/15/2024	20:52	PO107192.D	10.06	4.37
AR1242ICC500	AR1242ICC500	10/15/2024	21:10	PO107193.D	10.06	4.37
AR1242ICC250	AR1242ICC250	10/15/2024	21:28	PO107194.D	10.06	4.37
AR1242ICC050	AR1242ICC050	10/15/2024	21:46	PO107195.D	10.06	4.37
AR1248ICC1000	AR1248ICC1000	10/15/2024	22:04	PO107196.D	10.06	4.37
AR1248ICC750	AR1248ICC750	10/15/2024	22:22	PO107197.D	10.06	4.37
AR1248ICC500	AR1248ICC500	10/15/2024	22:41	PO107198.D	10.06	4.37
AR1248ICC250	AR1248ICC250	10/15/2024	22:59	PO107199.D	10.06	4.37
AR1248ICC050	AR1248ICC050	10/15/2024	23:17	PO107200.D	10.06	4.37
AR1254ICC1000	AR1254ICC1000	10/15/2024	23:35	PO107201.D	10.06	4.37
AR1254ICC750	AR1254ICC750	10/15/2024	23:53	PO107202.D	10.06	4.37
AR1254ICC500	AR1254ICC500	10/16/2024	00:11	PO107203.D	10.06	4.37
AR1254ICC250	AR1254ICC250	10/16/2024	00:29	PO107204.D	10.06	4.37
AR1254ICC050	AR1254ICC050	10/16/2024	00:47	PO107205.D	10.06	4.37
AR1262ICC500	AR1262ICC500	10/16/2024	01:05	PO107206.D	10.06	4.37
AR1268ICC1000	AR1268ICC1000	10/16/2024	01:23	PO107207.D	10.06	4.37
AR1268ICC750	AR1268ICC750	10/16/2024	01:41	PO107208.D	10.06	4.37
AR1268ICC500	AR1268ICC500	10/16/2024	01:59	PO107209.D	10.06	4.37
AR1268ICC250	AR1268ICC250	10/16/2024	02:18	PO107210.D	10.06	4.37
AR1268ICC050	AR1268ICC050	10/16/2024	02:36	PO107211.D	10.06	4.37
AR1660CCC500	AR1660CCC500	11/06/2024	09:29	PO107726.D	10.08	4.37
IBLK	IBLK	11/06/2024	10:33	PO107730.D	10.07	4.37
PB164700BL	PB164700BL	11/06/2024	13:10	PO107731.D	10.08	4.37
PB164700BS	PB164700BS	11/06/2024	13:26	PO107732.D	10.08	4.37
TR-04-110424MS	P4706-01MS	11/06/2024	14:30	PO107736.D	10.08	4.37
TR-04-110424MSD	P4706-01MSD	11/06/2024	14:46	PO107737.D	10.08	4.37
WB-307-SB01	P4718-01	11/06/2024	15:35	PO107740.D	10.08	4.37
AR1660CCC500	AR1660CCC500	11/06/2024	16:54	PO107741.D	10.07	4.37
IBLK	IBLK	11/06/2024	17:59	PO107745.D	10.07	4.37
PB164704BL	PB164704BL	11/06/2024	18:15	PO107746.D	10.07	4.37
PB164704BS	PB164704BS	11/06/2024	18:31	PO107747.D	10.07	4.37
PB164704BSD	PB164704BSD	11/06/2024	18:47	PO107748.D	10.08	4.37
WB-307-SW	P4718-04	11/06/2024	20:41	PO107755.D	10.08	4.37

Analytical Sequence

AR1660CCC500	AR1660CCC500	11/06/2024	21:42	PO107756.D	10.08	4.37
I.BLK	I.BLK	11/06/2024	22:46	PO107760.D	10.08	4.37
WB-307-SB02	P4718-02	11/06/2024	23:02	PO107761.D	10.08	4.37
AR1660CCC500	AR1660CCC500	11/07/2024	00:20	PO107763.D	10.08	4.37
I.BLK	I.BLK	11/07/2024	01:25	PO107767.D	10.08	4.37

Analytical Sequence

Client: Portal Partners Tri-Venture

SDG No.: P4718

Project: Amtrak Sawtooth Bridges 2024

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 10/15/2024

10/15/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	10/15/2024	18:08	PO107183.D	8.64	3.64
AR1660ICC1000	AR1660ICC1000	10/15/2024	18:27	PO107184.D	8.64	3.64
AR1660ICC750	AR1660ICC750	10/15/2024	18:45	PO107185.D	8.64	3.64
AR1660ICC500	AR1660ICC500	10/15/2024	19:03	PO107186.D	8.64	3.65
AR1660ICC250	AR1660ICC250	10/15/2024	19:21	PO107187.D	8.64	3.64
AR1660ICC050	AR1660ICC050	10/15/2024	19:39	PO107188.D	8.64	3.64
AR1221ICC500	AR1221ICC500	10/15/2024	19:57	PO107189.D	8.64	3.64
AR1232ICC500	AR1232ICC500	10/15/2024	20:15	PO107190.D	8.64	3.64
AR1242ICC1000	AR1242ICC1000	10/15/2024	20:34	PO107191.D	8.64	3.64
AR1242ICC750	AR1242ICC750	10/15/2024	20:52	PO107192.D	8.64	3.64
AR1242ICC500	AR1242ICC500	10/15/2024	21:10	PO107193.D	8.64	3.64
AR1242ICC250	AR1242ICC250	10/15/2024	21:28	PO107194.D	8.64	3.65
AR1242ICC050	AR1242ICC050	10/15/2024	21:46	PO107195.D	8.64	3.64
AR1248ICC1000	AR1248ICC1000	10/15/2024	22:04	PO107196.D	8.64	3.64
AR1248ICC750	AR1248ICC750	10/15/2024	22:22	PO107197.D	8.64	3.64
AR1248ICC500	AR1248ICC500	10/15/2024	22:41	PO107198.D	8.64	3.64
AR1248ICC250	AR1248ICC250	10/15/2024	22:59	PO107199.D	8.64	3.64
AR1248ICC050	AR1248ICC050	10/15/2024	23:17	PO107200.D	8.64	3.64
AR1254ICC1000	AR1254ICC1000	10/15/2024	23:35	PO107201.D	8.64	3.65
AR1254ICC750	AR1254ICC750	10/15/2024	23:53	PO107202.D	8.64	3.64
AR1254ICC500	AR1254ICC500	10/16/2024	00:11	PO107203.D	8.64	3.64
AR1254ICC250	AR1254ICC250	10/16/2024	00:29	PO107204.D	8.64	3.64
AR1254ICC050	AR1254ICC050	10/16/2024	00:47	PO107205.D	8.64	3.65
AR1262ICC500	AR1262ICC500	10/16/2024	01:05	PO107206.D	8.64	3.64
AR1268ICC1000	AR1268ICC1000	10/16/2024	01:23	PO107207.D	8.64	3.65
AR1268ICC750	AR1268ICC750	10/16/2024	01:41	PO107208.D	8.64	3.64
AR1268ICC500	AR1268ICC500	10/16/2024	01:59	PO107209.D	8.64	3.65
AR1268ICC250	AR1268ICC250	10/16/2024	02:18	PO107210.D	8.64	3.64
AR1268ICC050	AR1268ICC050	10/16/2024	02:36	PO107211.D	8.64	3.65
AR1660CCC500	AR1660CCC500	11/06/2024	09:29	PO107726.D	8.64	3.64
IBLK	IBLK	11/06/2024	10:33	PO107730.D	8.64	3.64
PB164700BL	PB164700BL	11/06/2024	13:10	PO107731.D	8.64	3.64
PB164700BS	PB164700BS	11/06/2024	13:26	PO107732.D	8.64	3.64
TR-04-110424MS	P4706-01MS	11/06/2024	14:30	PO107736.D	8.64	3.64
TR-04-110424MSD	P4706-01MSD	11/06/2024	14:46	PO107737.D	8.64	3.64
WB-307-SB01	P4718-01	11/06/2024	15:35	PO107740.D	8.64	3.64
AR1660CCC500	AR1660CCC500	11/06/2024	16:54	PO107741.D	8.64	3.64
IBLK	IBLK	11/06/2024	17:59	PO107745.D	8.64	3.64
PB164704BL	PB164704BL	11/06/2024	18:15	PO107746.D	8.64	3.64
PB164704BS	PB164704BS	11/06/2024	18:31	PO107747.D	8.64	3.64
PB164704BSD	PB164704BSD	11/06/2024	18:47	PO107748.D	8.64	3.64
WB-307-SW	P4718-04	11/06/2024	20:41	PO107755.D	8.64	3.64

Analytical Sequence

AR1660CCC500	AR1660CCC500	11/06/2024	21:42	PO107756.D	8.64	3.64
I.BLK	I.BLK	11/06/2024	22:46	PO107760.D	8.64	3.64
WB-307-SB02	P4718-02	11/06/2024	23:02	PO107761.D	8.64	3.64
AR1660CCC500	AR1660CCC500	11/07/2024	00:20	PO107763.D	8.64	3.64
I.BLK	I.BLK	11/07/2024	01:25	PO107767.D	8.64	3.64

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB164700BS

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Lab Sample ID: PB164700BS Date(s) Analyzed: 11/06/2024 11/06/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO107732.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.524	5.474	5.574	166	163	3.12
COLUMN 1	2	5.546	5.496	5.596	160		
	3	5.609	5.559	5.659	159		
	4	5.706	5.656	5.756	167		
	5	6.001	5.951	6.051	163		
	1	4.724	4.674	4.774	162		
COLUMN 2	2	4.743	4.693	4.793	168	158	
	3	4.919	4.869	4.969	161		
	4	4.96	4.91	5.01	146		
	5	5.174	5.124	5.224	155		
Aroclor-1260	1	7.131	7.081	7.181	171	168	5.5
COLUMN 1	2	7.388	7.338	7.438	178		
	3	7.75	7.7	7.8	157		
	4	7.975	7.925	8.025	174		
	5	8.29	8.24	8.34	160		
	1	6.205	6.155	6.255	162	159	
COLUMN 2	2	6.393	6.343	6.443	170		
	3	6.545	6.495	6.595	166		
	4	7.016	6.966	7.066	144		
	5	7.258	7.208	7.308	154		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

TR-04-110424MS

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Lab Sample ID: P4706-01MS Date(s) Analyzed: 11/06/2024 11/06/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO107736.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.523	5.473	5.573	145	139	2.84
COLUMN 1	2	5.546	5.496	5.596	133		
	3	5.608	5.558	5.658	136		
	4	5.705	5.655	5.755	148		
	5	5.999	5.949	6.049	131		
COLUMN 2	1	4.723	4.673	4.773	150	143	
	2	4.742	4.692	4.792	152		
	3	4.918	4.868	4.968	144		
	4	4.96	4.91	5.01	132		
	5	5.172	5.122	5.222	134		
Aroclor-1260	1	7.13	7.08	7.18	139	142	15.15
COLUMN 1	2	7.387	7.337	7.437	155		
	3	7.749	7.699	7.799	123		
	4	7.973	7.923	8.023	150		
	5	8.288	8.238	8.338	144		
COLUMN 2	1	6.204	6.154	6.254	128	122	
	2	6.391	6.341	6.441	136		
	3	6.544	6.494	6.594	128		
	4	7.016	6.966	7.066	106		
	5	7.257	7.207	7.307	113		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

TR-04-110424MSD

Contract: PORT06

Lab Code: CHEM Case No.: P4718 SAS No.: P4718 SDG NO.: P4718

Lab Sample ID: P4706-01MSD Date(s) Analyzed: 11/06/2024 11/06/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO107737.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.523	5.473	5.573	136	131	5.93
COLUMN 1	2	5.545	5.495	5.595	126		
	3	5.608	5.558	5.658	128		
	4	5.705	5.655	5.755	139		
	5	6	5.95	6.05	127		
	1	4.724	4.674	4.774	146		
COLUMN 2	2	4.743	4.693	4.793	149	139	
	3	4.919	4.869	4.969	141		
	4	4.96	4.91	5.01	129		
	5	5.173	5.123	5.223	131		
Aroclor-1260	1	7.13	7.08	7.18	131	135	14.29
COLUMN 1	2	7.387	7.337	7.437	146		
	3	7.749	7.699	7.799	120		
	4	7.974	7.924	8.024	140		
	5	8.289	8.239	8.339	139		
	1	6.204	6.154	6.254	123	117	
COLUMN 2	2	6.391	6.341	6.441	130		
	3	6.545	6.495	6.595	123		
	4	7.016	6.966	7.066	101		
	5	7.257	7.207	7.307	108		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB164704BS

Contract: PORT06

Lab Code: CHEM

Case No.: P4718

SAS No.: P4718

SDG NO.: P4718

Lab Sample ID: PB164704BS

Date(s) Analyzed: 11/06/2024

11/06/2024

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO107747.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.523	5.473	5.573	4.34	4.20	0
	2	5.545	5.495	5.595	4.25		
	3	5.608	5.558	5.658	4.18		
	4	5.705	5.655	5.755	4.34		
	5	6	5.95	6.05	4.00		
COLUMN 1	1	4.723	4.673	4.773	4.43	4.20	
	2	4.742	4.692	4.792	4.53		
	3	4.918	4.868	4.968	4.26		
	4	4.959	4.909	5.009	3.86		
	5	5.173	5.123	5.223	4.08		
COLUMN 2	1	7.129	7.079	7.179	4.04	4.20	2.35
	2	7.386	7.336	7.436	4.48		
	3	7.748	7.698	7.798	3.76		
	4	7.974	7.924	8.024	4.65		
	5	8.289	8.239	8.339	3.93		
Aroclor-1260	1	6.204	6.154	6.254	4.39	4.30	
	2	6.391	6.341	6.441	4.63		
	3	6.545	6.495	6.595	4.51		
	4	7.015	6.965	7.065	3.90		
	5	7.256	7.206	7.306	4.15		
COLUMN 1	1						
	2						
	3						
	4						
	5						
COLUMN 2	1						
	2						
	3						
	4						
	5						

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB164704BSD

Contract: PORT06

Lab Code: CHEM

Case No.: P4718

SAS No.: P4718

SDG NO.: P4718

Lab Sample ID: PB164704BSD

Date(s) Analyzed: 11/06/2024

11/06/2024

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO107748.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.522	5.472	5.572	4.50	4.40	2.25
COLUMN 1	2	5.545	5.495	5.595	4.39		
	3	5.607	5.557	5.657	4.39		
	4	5.705	5.655	5.755	4.53		
	5	6	5.95	6.05	4.32		
	1	4.723	4.673	4.773	4.61		
COLUMN 2	2	4.742	4.692	4.792	4.70	4.50	
	3	4.918	4.868	4.968	4.52		
	4	4.96	4.91	5.01	4.10		
	5	5.173	5.123	5.223	4.33		
Aroclor-1260	1	7.129	7.079	7.179	4.10	4.20	6.9
COLUMN 1	2	7.386	7.336	7.436	4.66		
	3	7.749	7.699	7.799	3.99		
	4	7.974	7.924	8.024	4.34		
	5	8.289	8.239	8.339	4.11		
	1	6.204	6.154	6.254	4.53		
COLUMN 2	2	6.391	6.341	6.441	4.80	4.50	
	3	6.544	6.494	6.594	4.68		
	4	7.015	6.965	7.065	4.06		
	5	7.257	7.207	7.307	4.32		



QC SAMPLE DATA

Report of Analysis

Client:	Portal Partners Tri-Venture		Date Collected:		
Project:	Amtrak Sawtooth Bridges 2024		Date Received:		
Client Sample ID:	PB164700BL		SDG No.:	P4718	
Lab Sample ID:	PB164700BL		Matrix:	SOIL	
Analytical Method:	SW8082A		% Solid:	100	Decanted:
Sample Wt/Vol:	30.01	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107731.D	1	11/06/24 09:10	11/06/24 13:10	PB164700

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	3.40	U	3.40	17.0	ug/kg
11104-28-2	Aroclor-1221	6.40	U	6.40	17.0	ug/kg
11141-16-5	Aroclor-1232	3.40	U	3.40	17.0	ug/kg
53469-21-9	Aroclor-1242	3.40	U	3.40	17.0	ug/kg
12672-29-6	Aroclor-1248	7.90	U	7.90	17.0	ug/kg
11097-69-1	Aroclor-1254	2.70	U	2.70	17.0	ug/kg
37324-23-5	Aroclor-1262	4.60	U	4.60	17.0	ug/kg
11100-14-4	Aroclor-1268	3.40	U	3.40	17.0	ug/kg
11096-82-5	Aroclor-1260	2.90	U	2.90	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.5		30 (32) - 150 (144)	108%	SPK: 20
2051-24-3	Decachlorobiphenyl	24.1		30 (32) - 150 (175)	121%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 13:10
 Operator : YP/AJ
 Sample : PB164700BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB164700BL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/06/2024
 Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 14:27:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.644	196.1E6	69316988	21.520	21.537
2) SA Decachlor...	10.081	8.641	56085345	66156116	22.860m	24.131

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 13:10
Operator : YP/AJ
Sample : PB164700BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB164700BL



Manual Integrations**APPROVED**


Reviewed By :Yogesh Patel 11/06/2024

Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 14:27:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

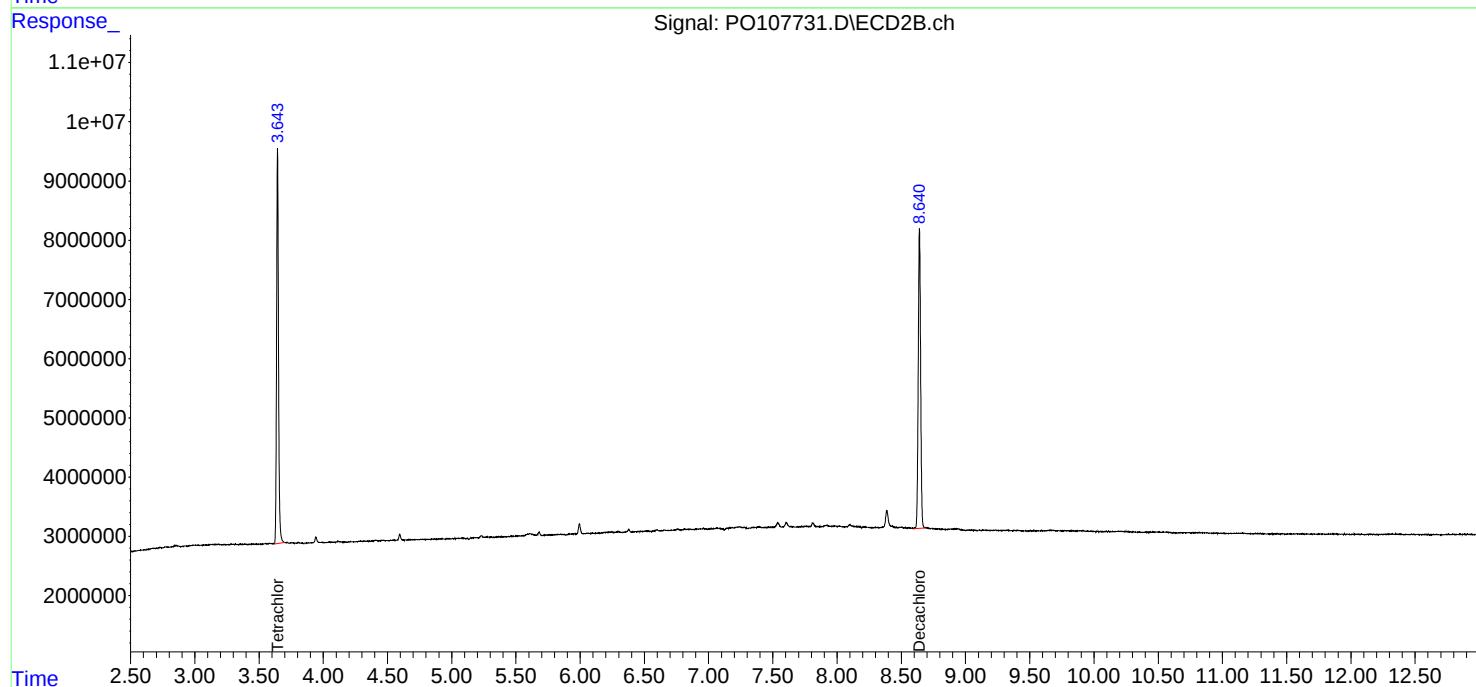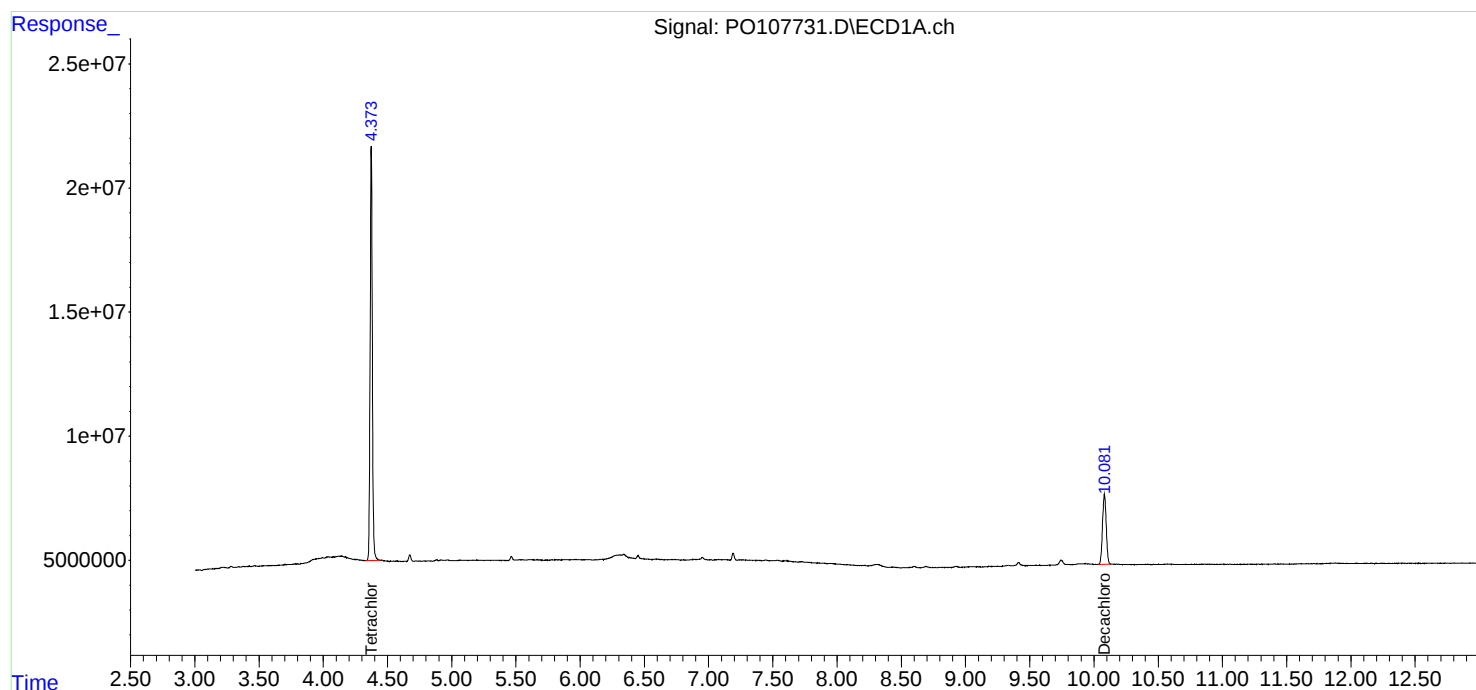

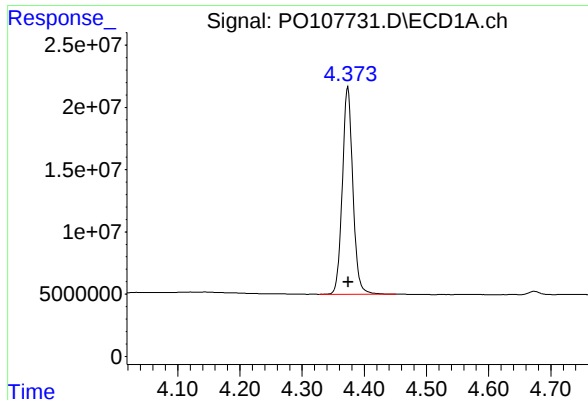


#1 Tetrachloro-m-xylene

R.T.: 4.374 min
Delta R.T.: 0.000 min
Response: 196130859
Conc: 21.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB164700BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/06/2024
Supervised By :Ankita Jodhani 11/07/2024

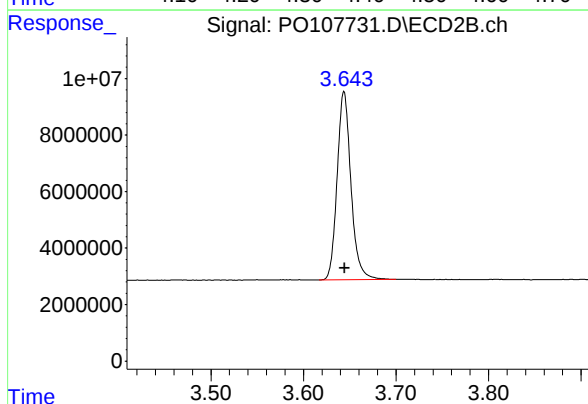


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.000 min
Response: 69316988
Conc: 21.54 ng/ml

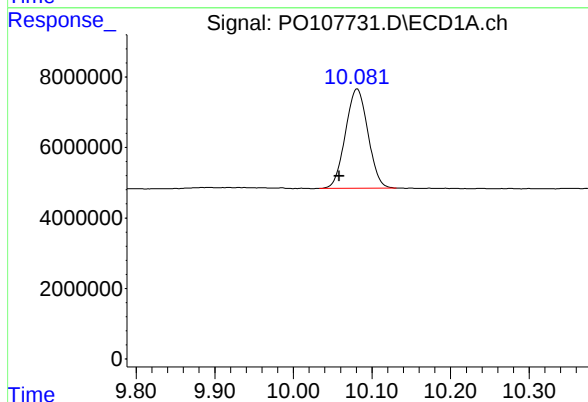

#2 Decachlorobiphenyl

R.T.: 10.081 min
Delta R.T.: 0.022 min
Response: 56085345
Conc: 22.86 ng/ml m

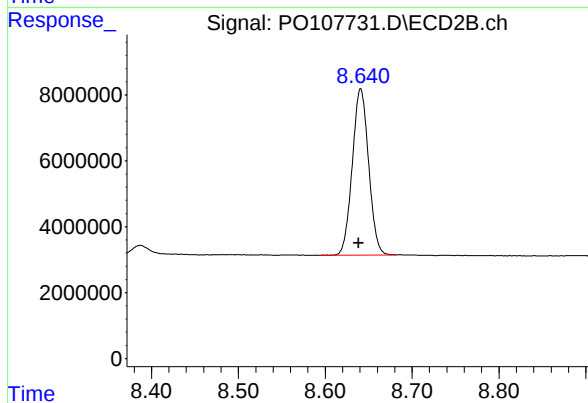

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.002 min
Response: 66156116
Conc: 24.13 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	
Client Sample ID:	PB164704BL	SDG No.:	P4718
Lab Sample ID:	PB164704BL	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107746.D	1	11/06/24 08:25	11/06/24 18:15	PB164704

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.8		30 (10) - 150 (157)	99%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.0		30 (10) - 150 (173)	95%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 18:15
 Operator : YP/AJ
 Sample : PB164704BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB164704BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:41:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	173.1E6	63762629	18.998	19.811
2) SA Decachlor...	10.074	8.638	46582557	50525503	18.987	18.429

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 18:15
Operator : YP/AJ
Sample : PB164704BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB164704BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:41:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

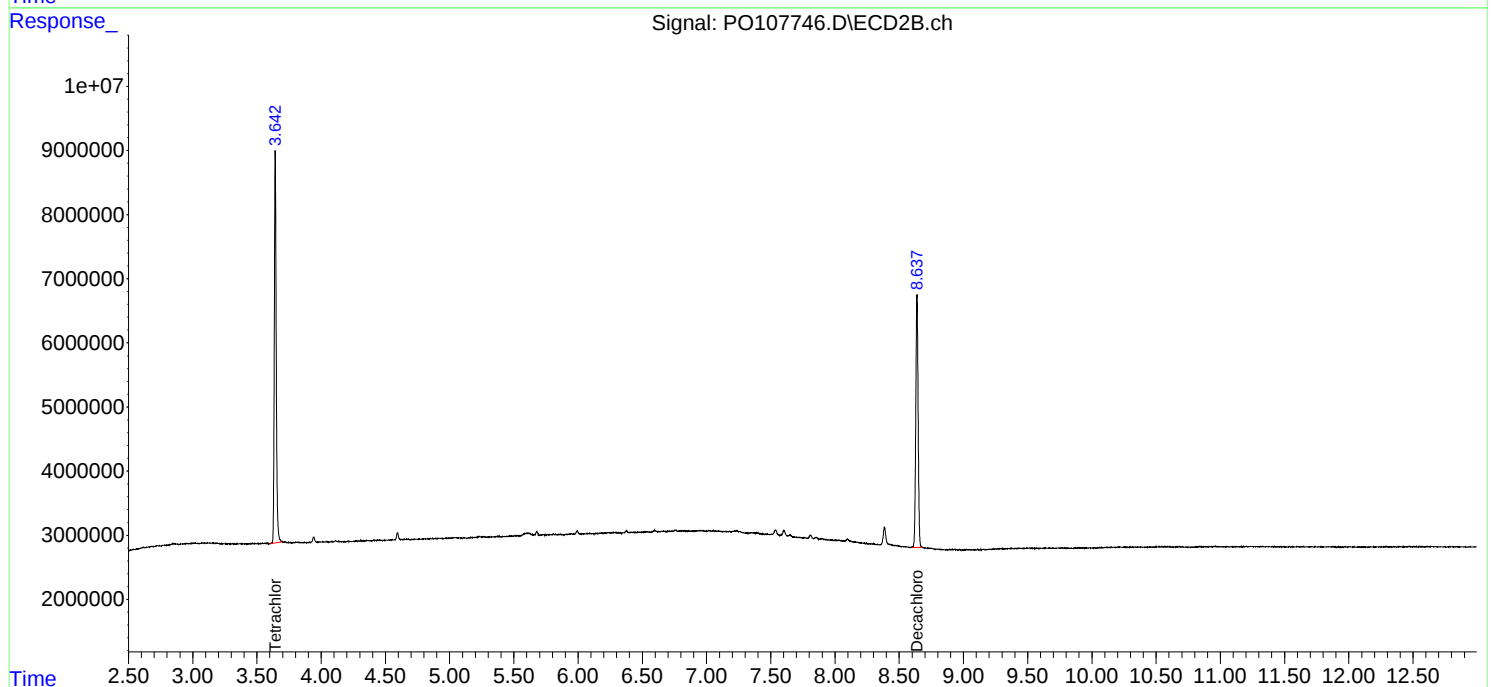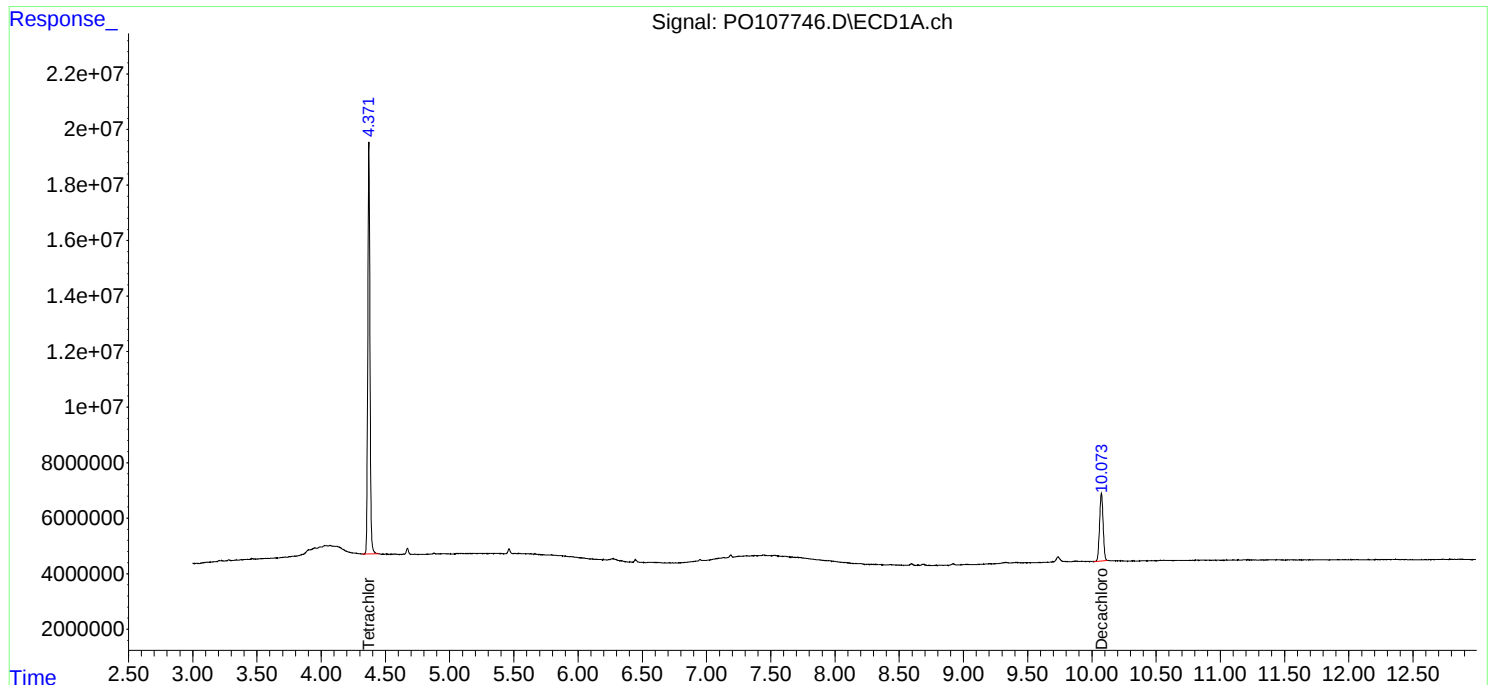


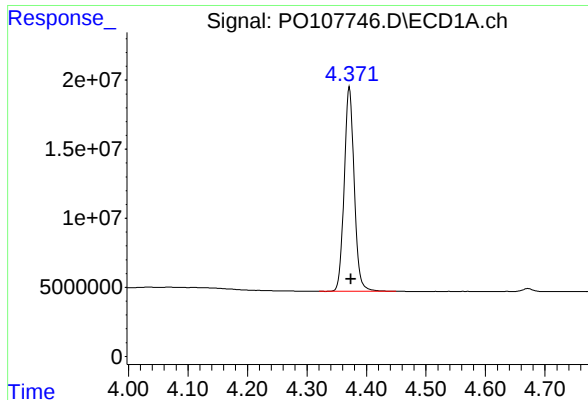

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 173141855
Conc: 19.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB164704BL

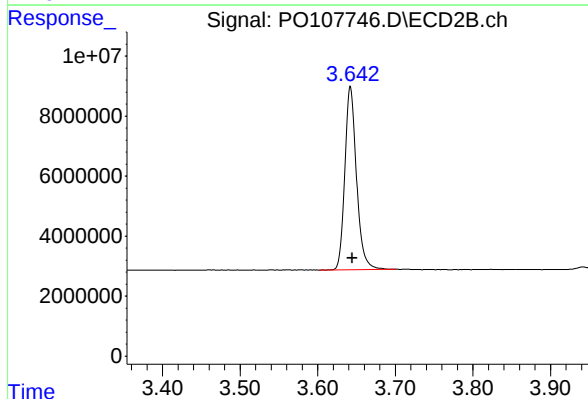


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.002 min
Response: 63762629
Conc: 19.81 ng/ml

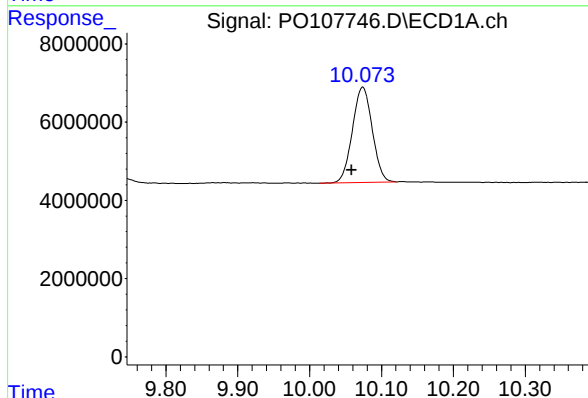

#2 Decachlorobiphenyl

R.T.: 10.074 min
Delta R.T.: 0.016 min
Response: 46582557
Conc: 18.99 ng/ml

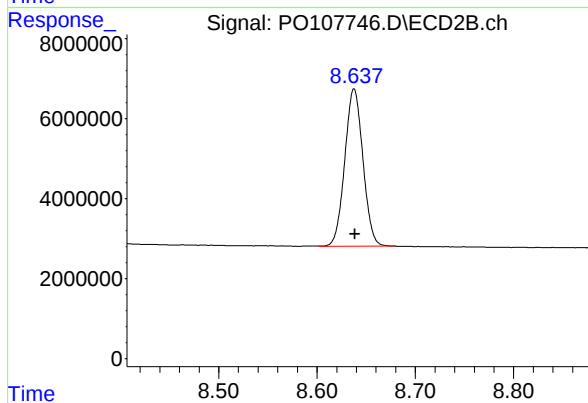

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 50525503
Conc: 18.43 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	10/15/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	10/15/24
Client Sample ID:	PIBLK-PO107183.D	SDG No.:	P4718
Lab Sample ID:	I.BLK-PO107183.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107183.D	1		10/15/24	po101524

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.1		70 (60) - 130 (140)	110%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.8		70 (60) - 130 (140)	114%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
 Data File : PO107183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 18:08
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 04:56:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:53:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	204.9E6	71065652	22.480	22.080
2) SA Decachlor...	10.057	8.638	57445703	62504934	23.415	22.799

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101524\
Data File : PO107183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 18:08
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 04:56:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:53:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

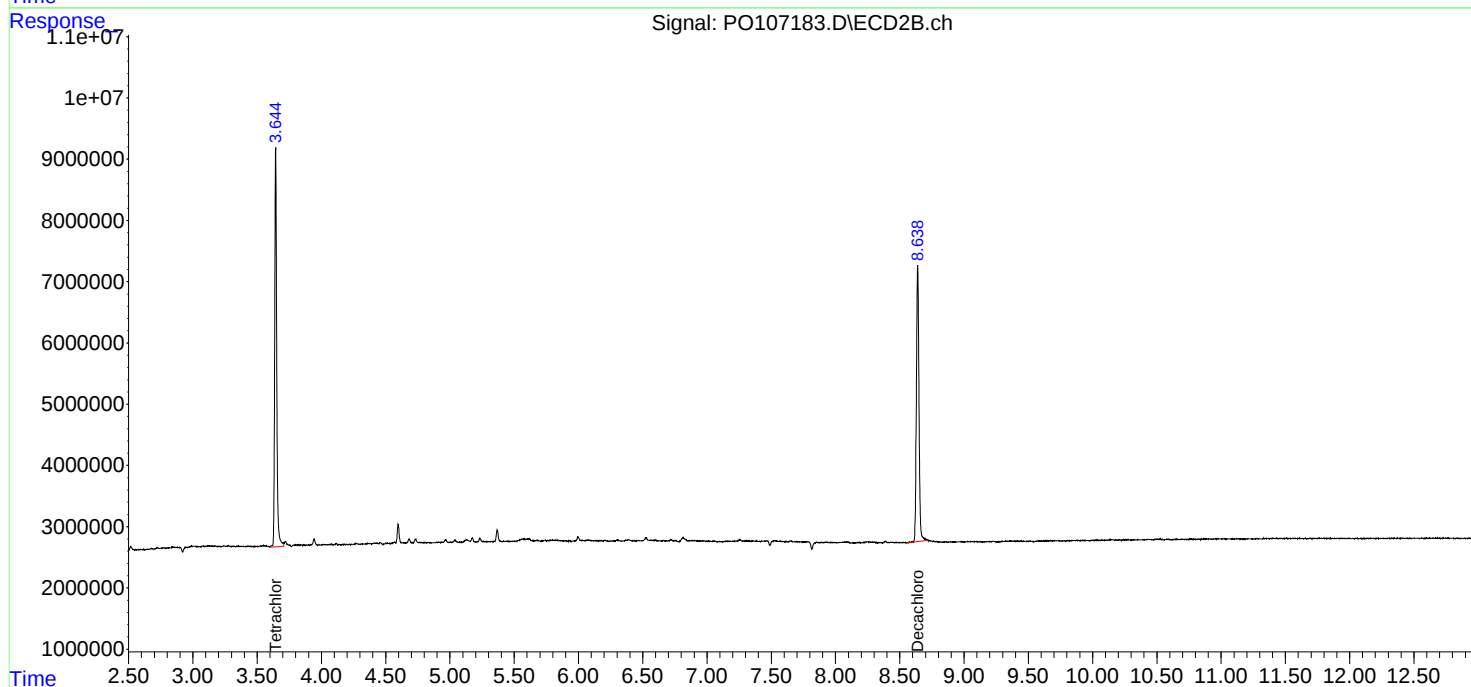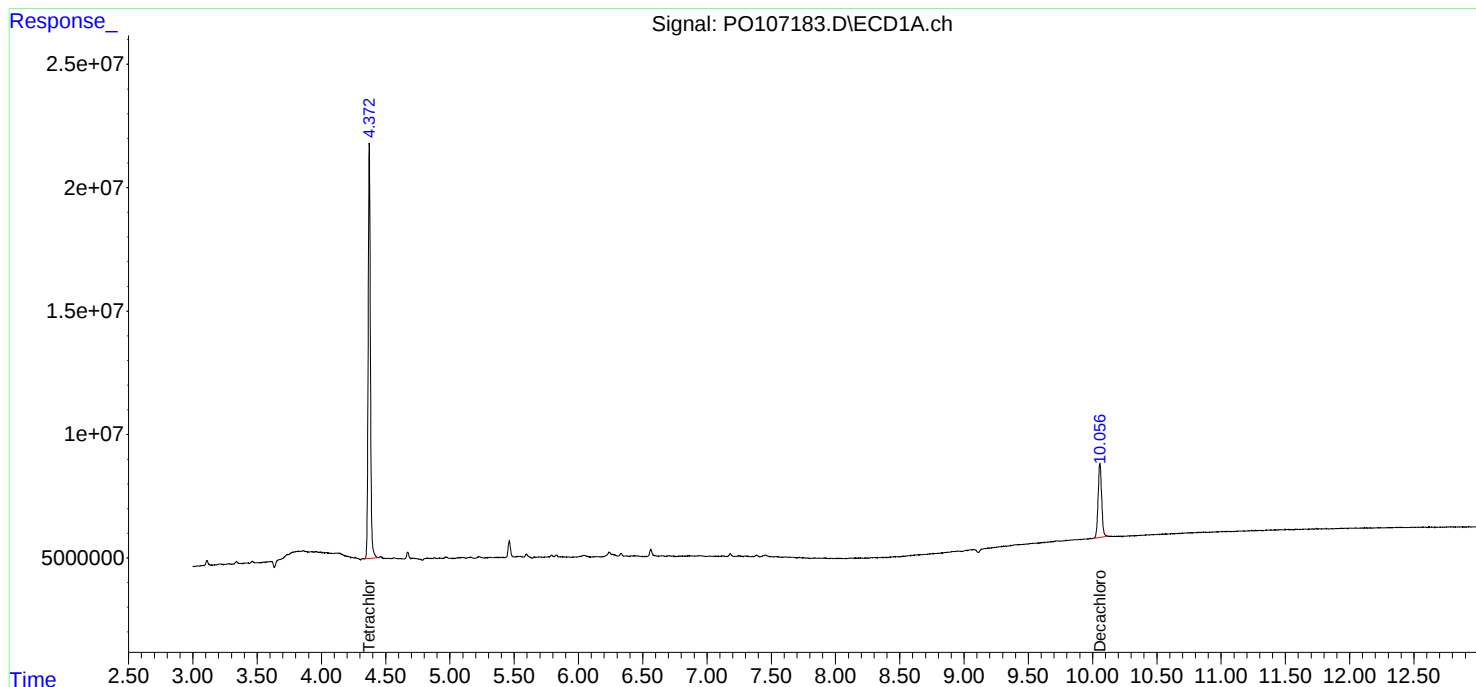


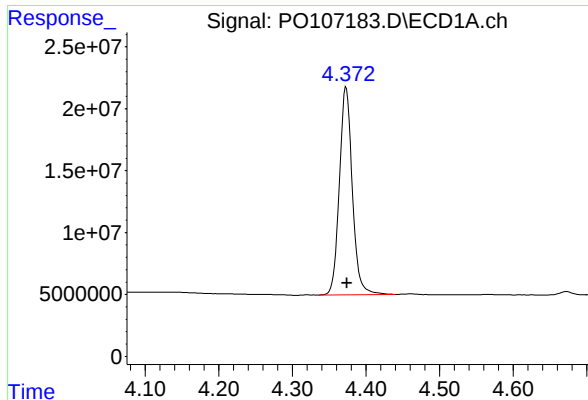

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: -0.001 min
Response: 204884980
Conc: 22.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

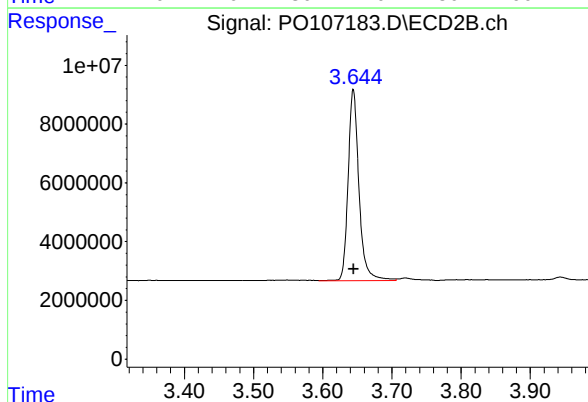


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.000 min
Response: 71065652
Conc: 22.08 ng/ml

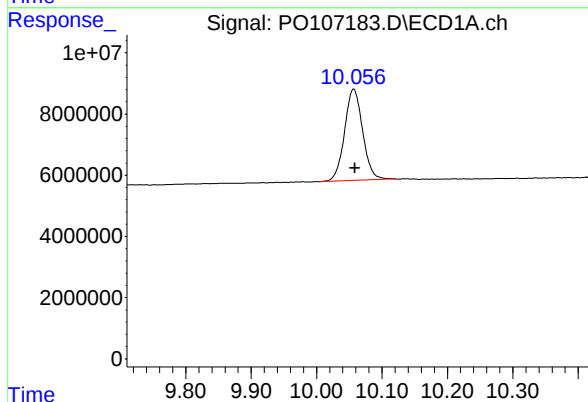

#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: -0.002 min
Response: 57445703
Conc: 23.41 ng/ml

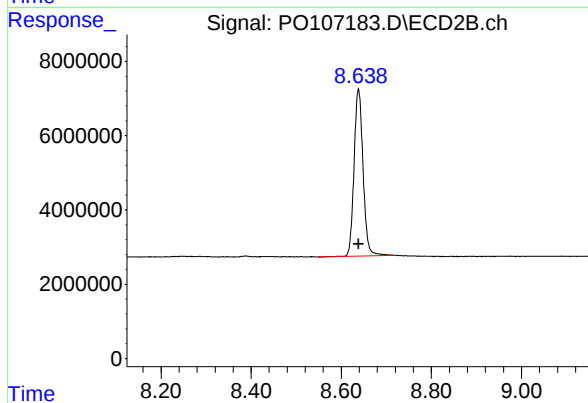

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 62504934
Conc: 22.80 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/06/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/06/24
Client Sample ID:	PIBLK-PO107730.D	SDG No.:	P4718
Lab Sample ID:	I.BLK-PO107730.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107730.D	1		11/06/24	PO110624

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.9		70 (60) - 130 (140)	100%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.1		70 (60) - 130 (140)	105%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 10:33
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 14:26:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.643	181.8E6	64909332	19.950	20.168
2) SA Decachlor...	10.072	8.638	51715567	60895233	21.079	22.212

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 10:33
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 14:26:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

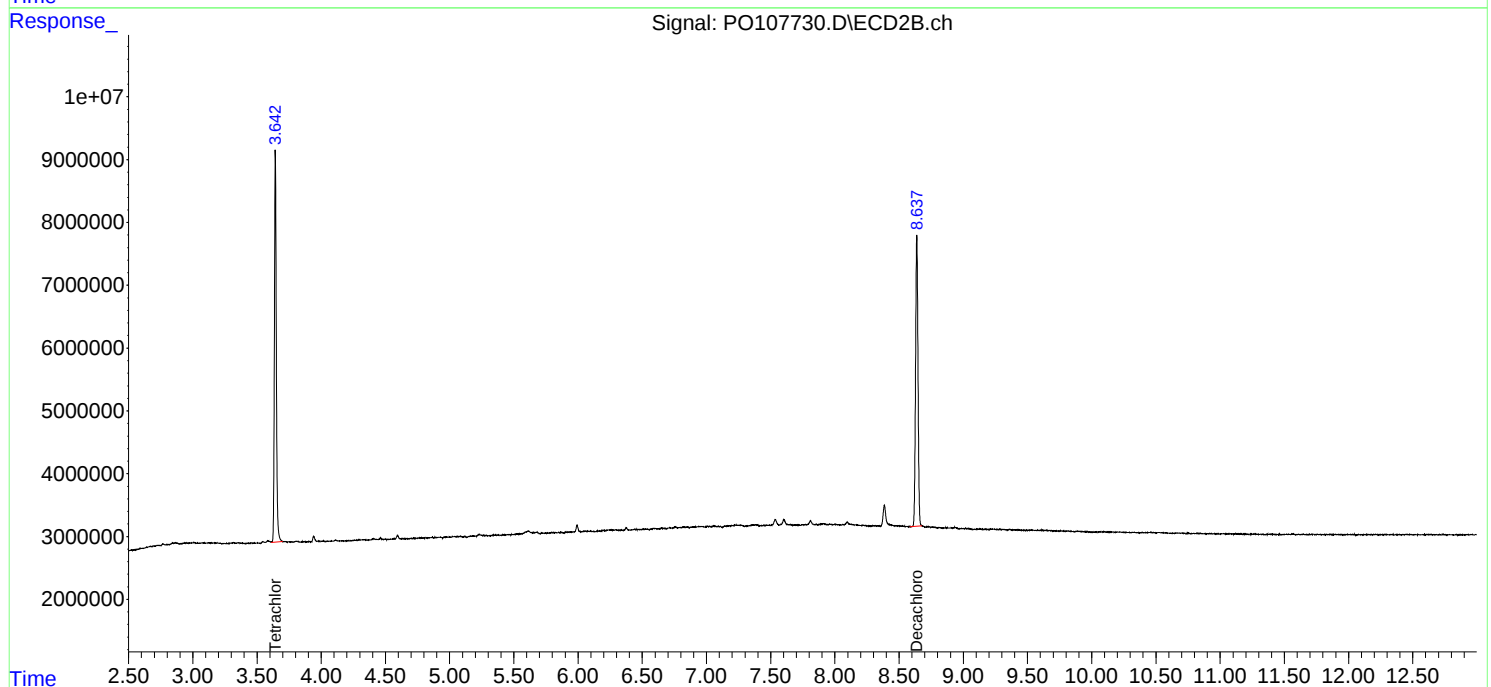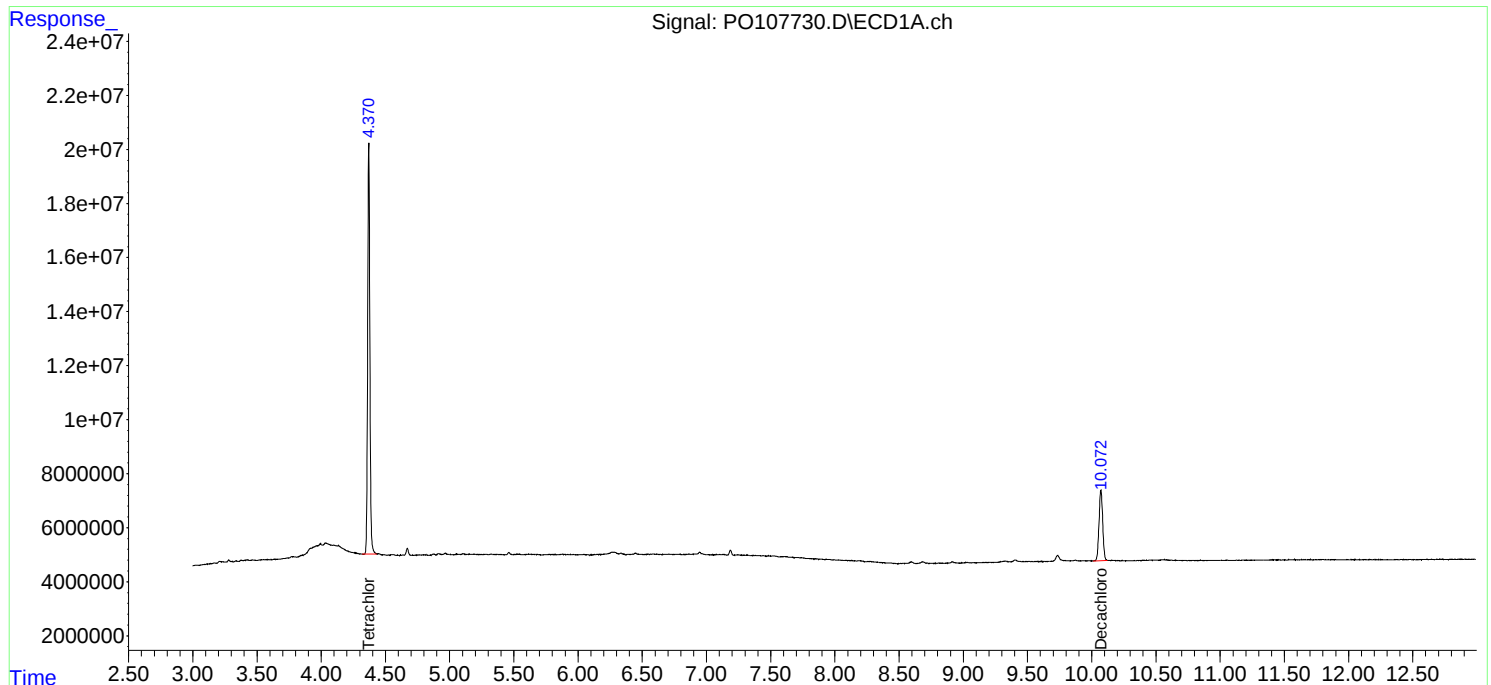


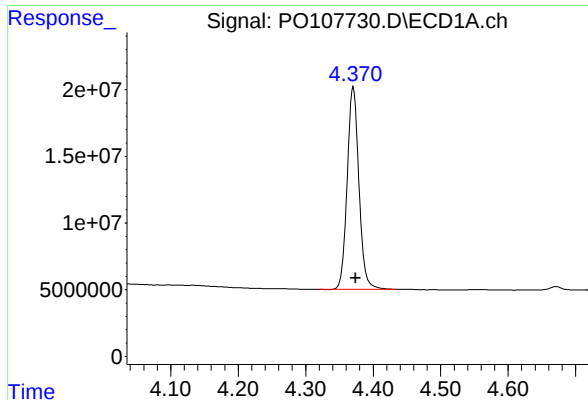

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 181826550
Conc: 19.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

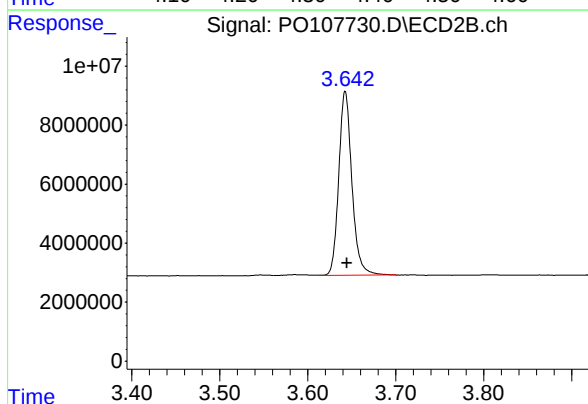


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.002 min
Response: 64909332
Conc: 20.17 ng/ml

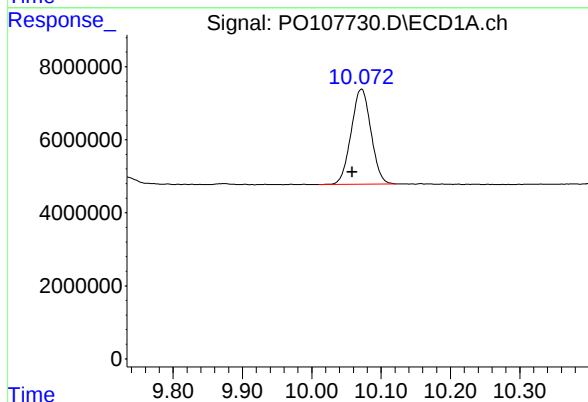

#2 Decachlorobiphenyl

R.T.: 10.072 min
Delta R.T.: 0.014 min
Response: 51715567
Conc: 21.08 ng/ml

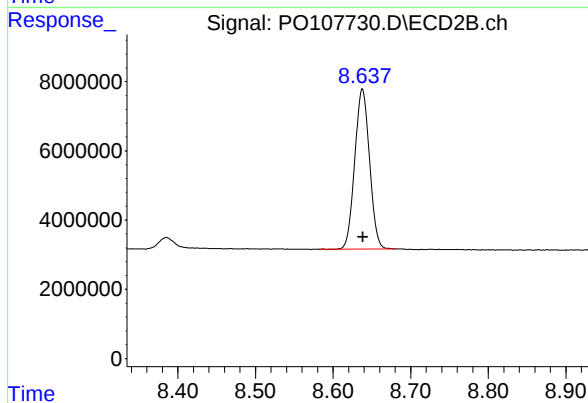

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 60895233
Conc: 22.21 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/06/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/06/24
Client Sample ID:	PIBLK-PO107745.D	SDG No.:	P4718
Lab Sample ID:	I.BLK-PO107745.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107745.D	1		11/06/24	PO110624

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.2		70 (60) - 130 (140)	96%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.1		70 (60) - 130 (140)	91%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 17:59
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:41:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.643	174.6E6	64463660	19.163	20.029
2) SA Decachlor...	10.074	8.638	46158721	49625061	18.814	18.101

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 17:59
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:41:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

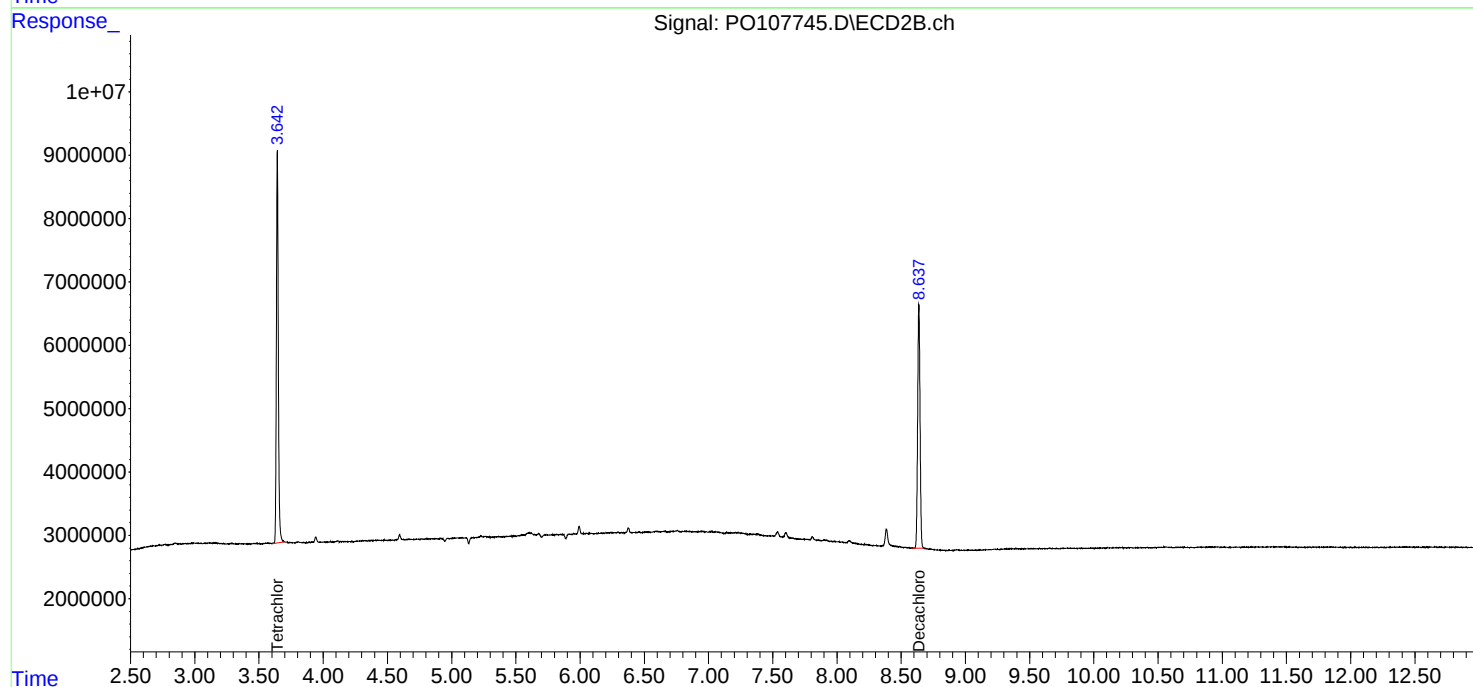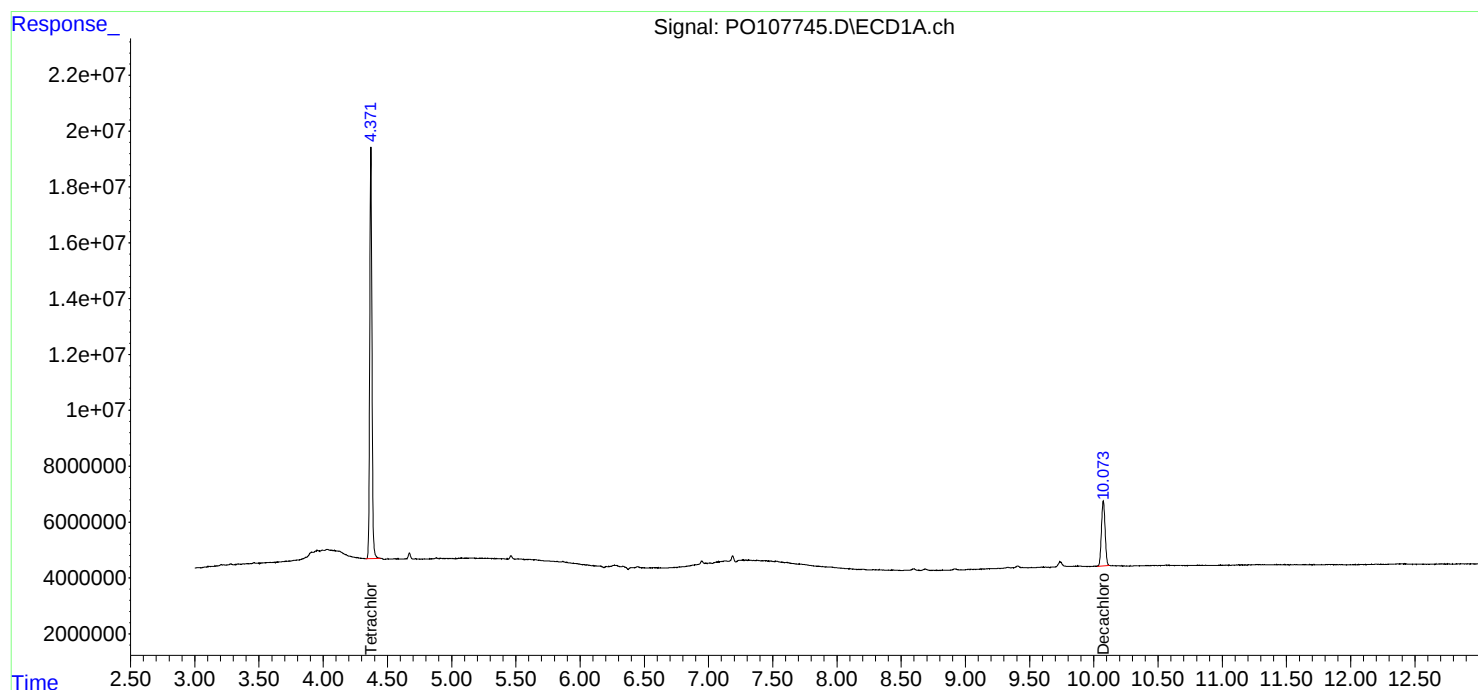


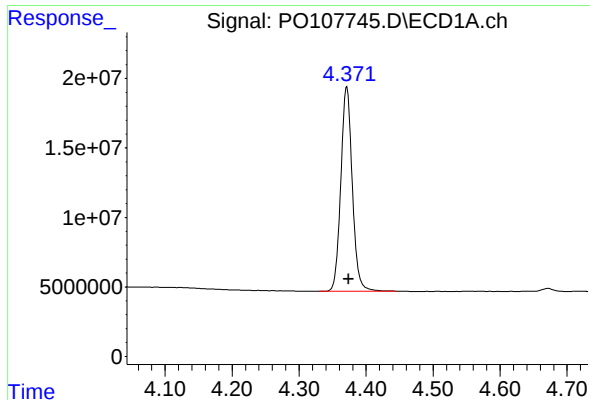

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 174647606
Conc: 19.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

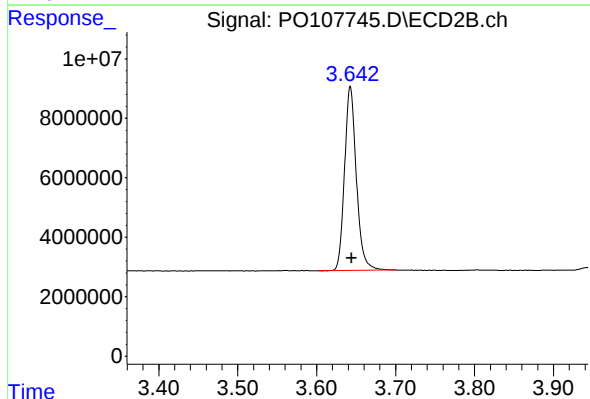


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.002 min
Response: 64463660
Conc: 20.03 ng/ml

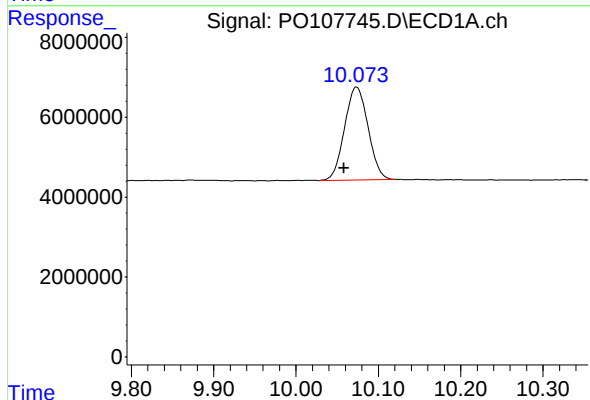

#2 Decachlorobiphenyl

R.T.: 10.074 min
Delta R.T.: 0.015 min
Response: 46158721
Conc: 18.81 ng/ml

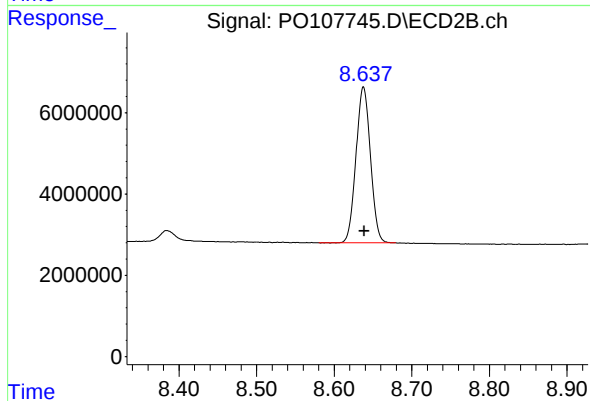

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 49625061
Conc: 18.10 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/06/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/06/24
Client Sample ID:	PIBLK-PO107760.D	SDG No.:	P4718
Lab Sample ID:	I.BLK-PO107760.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0	PH :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107760.D	1		11/06/24	PO110624

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.1		70 (60) - 130 (140)	101%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.2		70 (60) - 130 (140)	101%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 22:46
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:50:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	183.2E6	66419635	20.098	20.637
2) SA Decachlor...	10.077	8.638	49527790	62047881	20.188	22.632

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 22:46
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:50:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

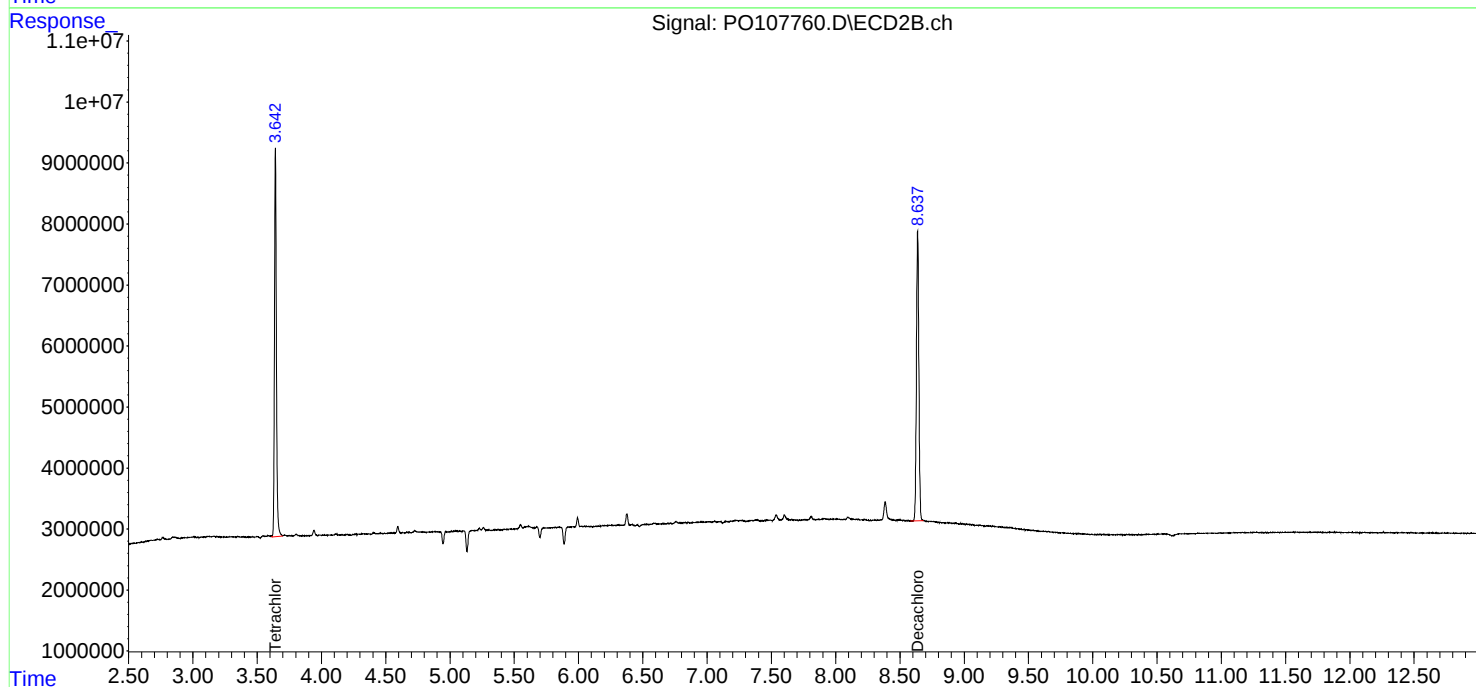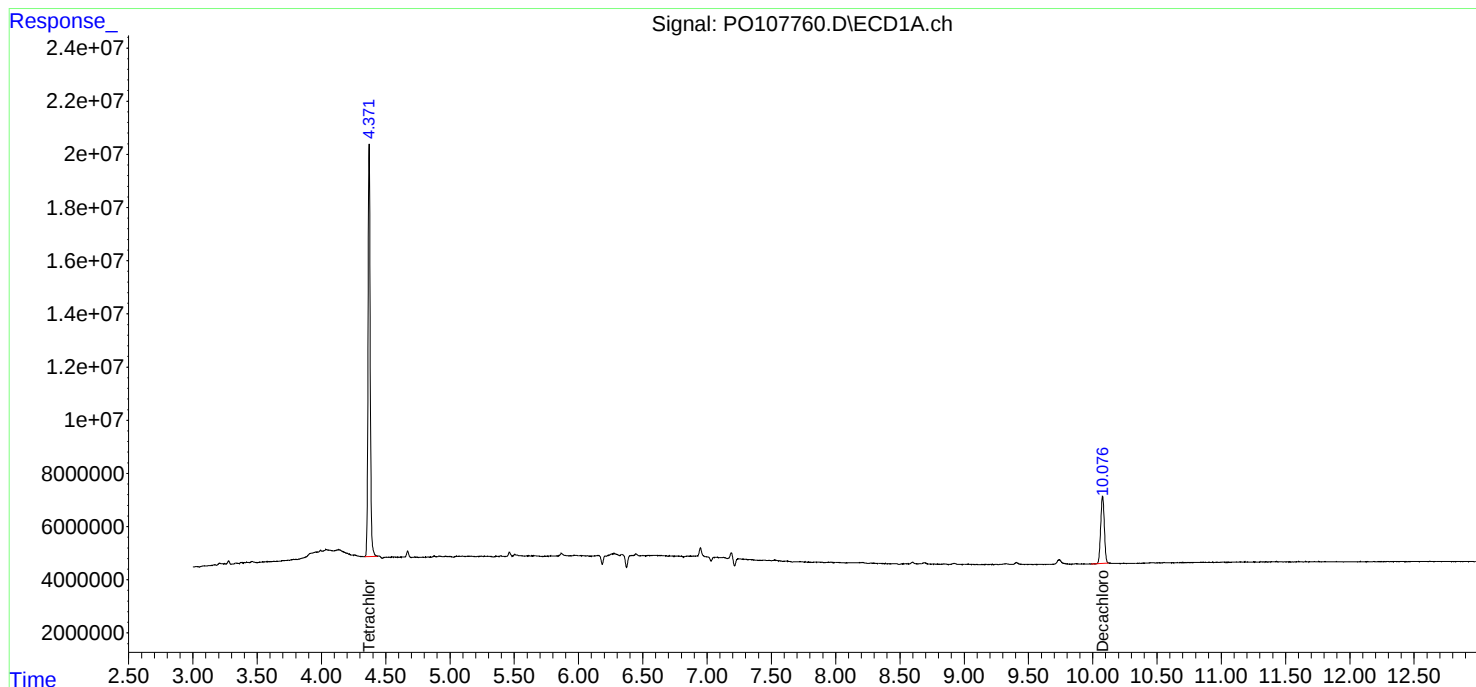


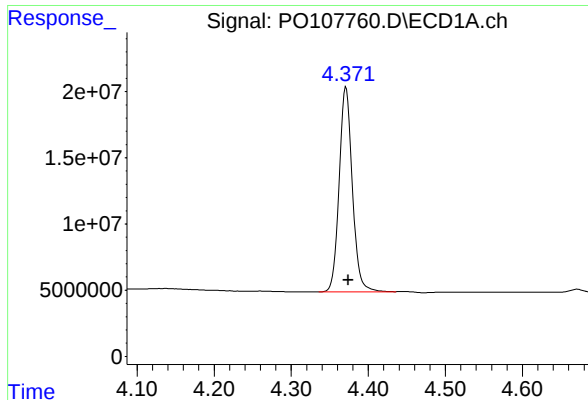

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 183174154
Conc: 20.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

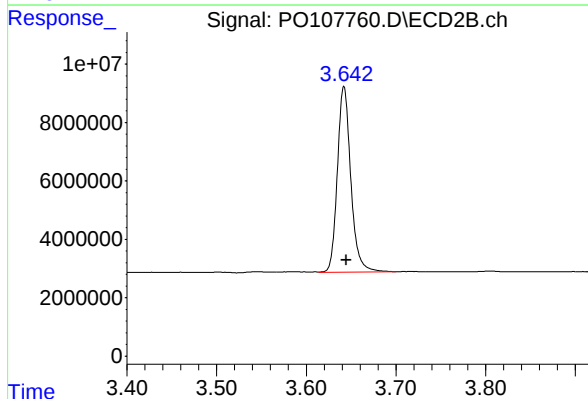


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.003 min
Response: 66419635
Conc: 20.64 ng/ml

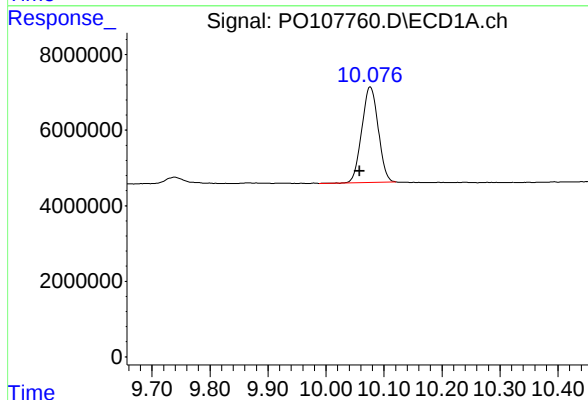

#2 Decachlorobiphenyl

R.T.: 10.077 min
Delta R.T.: 0.018 min
Response: 49527790
Conc: 20.19 ng/ml

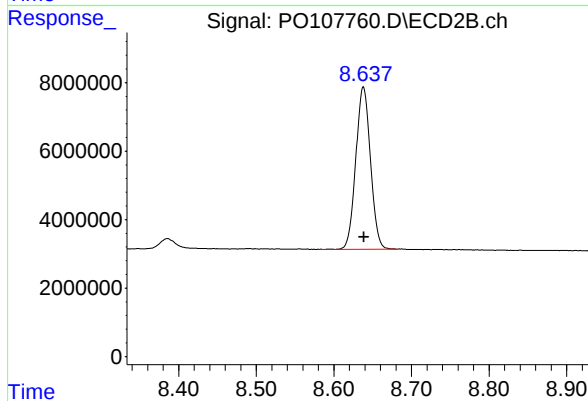

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 62047881
Conc: 22.63 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/07/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/07/24
Client Sample ID:	PIBLK-PO107767.D	SDG No.:	P4718
Lab Sample ID:	I.BLK-PO107767.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107767.D	1		11/07/24	PO110624

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.6		70 (60) - 130 (140)	103%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.1		70 (60) - 130 (140)	106%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 01:25
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 01:37:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	188.1E6	66740978	20.639	20.737
2) SA Decachlor...	10.076	8.637	51848598	61863131	21.134	22.565

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 01:25
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 01:37:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

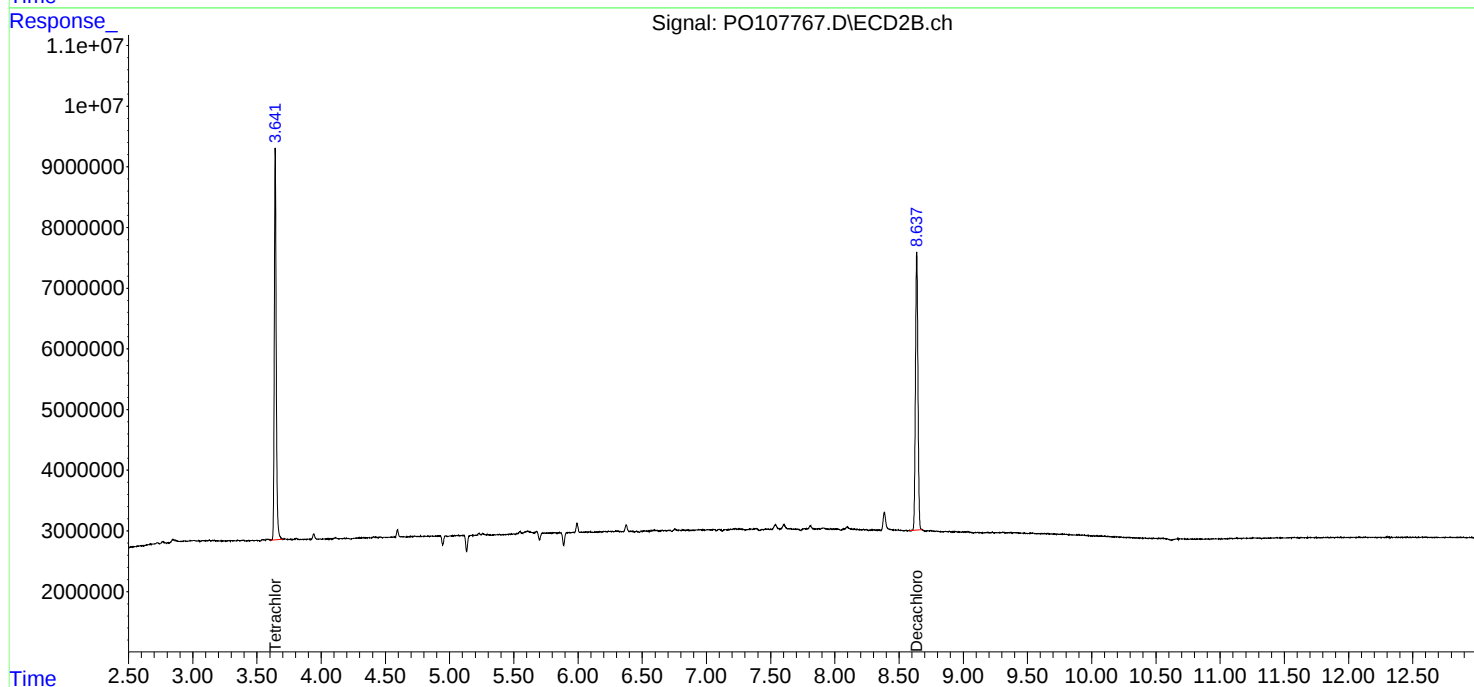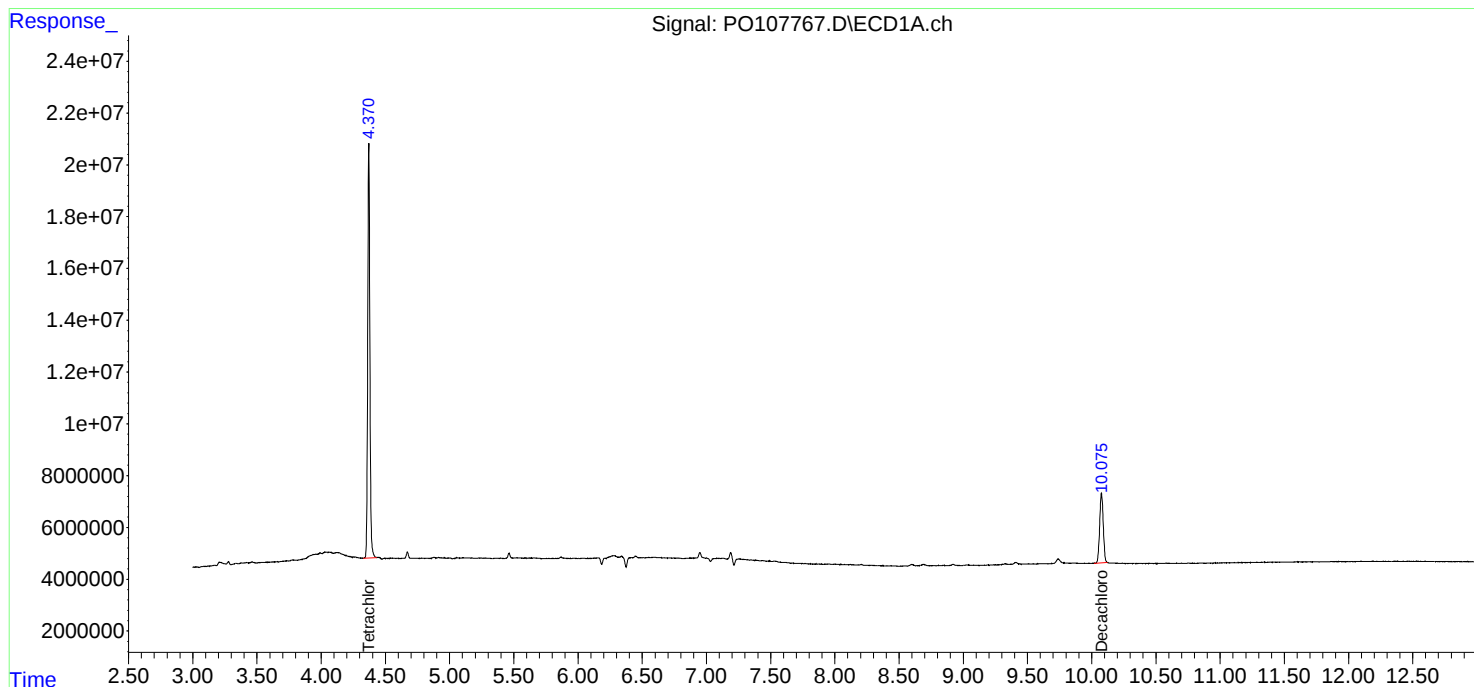


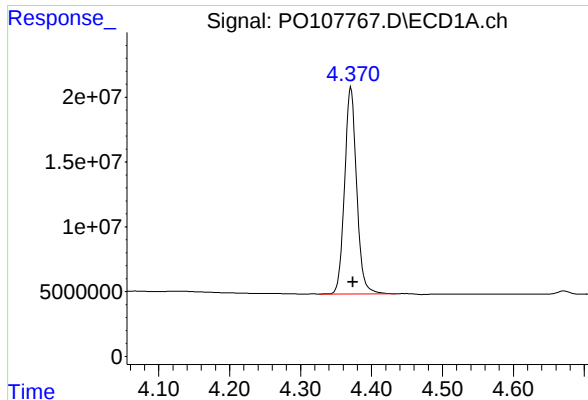

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 188103228
Conc: 20.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

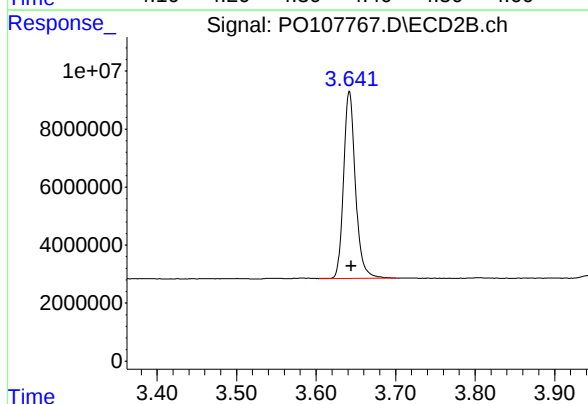


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.003 min
Response: 66740978
Conc: 20.74 ng/ml

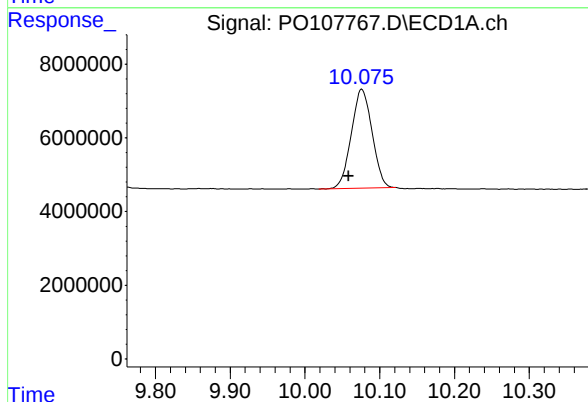

#2 Decachlorobiphenyl

R.T.: 10.076 min
Delta R.T.: 0.018 min
Response: 51848598
Conc: 21.13 ng/ml

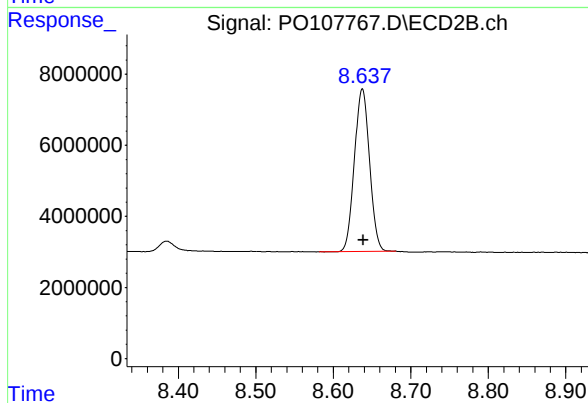

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.001 min
Response: 61863131
Conc: 22.56 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	
Client Sample ID:	PB164700BS	SDG No.:	P4718
Lab Sample ID:	PB164700BS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	100 Decanted:
Sample Wt/Vol:	30.03 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107732.D	1	11/06/24 09:10	11/06/24 13:26	PB164700

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	163		3.40	17.0	ug/kg
11104-28-2	Aroclor-1221	6.40	U	6.40	17.0	ug/kg
11141-16-5	Aroclor-1232	3.40	U	3.40	17.0	ug/kg
53469-21-9	Aroclor-1242	3.40	U	3.40	17.0	ug/kg
12672-29-6	Aroclor-1248	7.90	U	7.90	17.0	ug/kg
11097-69-1	Aroclor-1254	2.70	U	2.70	17.0	ug/kg
37324-23-5	Aroclor-1262	4.60	U	4.60	17.0	ug/kg
11100-14-4	Aroclor-1268	3.40	U	3.40	17.0	ug/kg
11096-82-5	Aroclor-1260	168		2.90	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.6		30 (32) - 150 (144)	108%	SPK: 20
2051-24-3	Decachlorobiphenyl	23.5		30 (32) - 150 (175)	117%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 13:26
 Operator : YP/AJ
 Sample : PB164700BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB164700BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 14:28:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.644	196.5E6	65305545	21.561	20.291
2) SA Decachlor...	10.078	8.640	55115919	64406717	22.465	23.492
Target Compounds						
3) L1 AR-1016-1	5.524	4.724	134.2E6	50310036	497.297	487.190
4) L1 AR-1016-2	5.546	4.743	190.2E6	71097228	479.230	504.351
5) L1 AR-1016-3	5.609	4.919	120.1E6	38063818	478.231	483.377
6) L1 AR-1016-4	5.706	4.960	96535995	29004573	501.194	438.743
7) L1 AR-1016-5	6.001	5.174	89678218	38109669	490.974	463.995
31) L7 AR-1260-1	7.131	6.205	132.8E6	75350909	513.712	485.650
32) L7 AR-1260-2	7.388	6.393	140.6E6	90134523	534.137	511.792
33) L7 AR-1260-3	7.750	6.545	84929464	83746756	472.499	499.241
34) L7 AR-1260-4	7.975	7.016	91447040	62486944	521.054	431.895
35) L7 AR-1260-5	8.290	7.258	136.7E6	152.4E6	480.655	462.561



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 13:26
Operator : YP/AJ
Sample : PB164700BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB164700BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 14:28:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

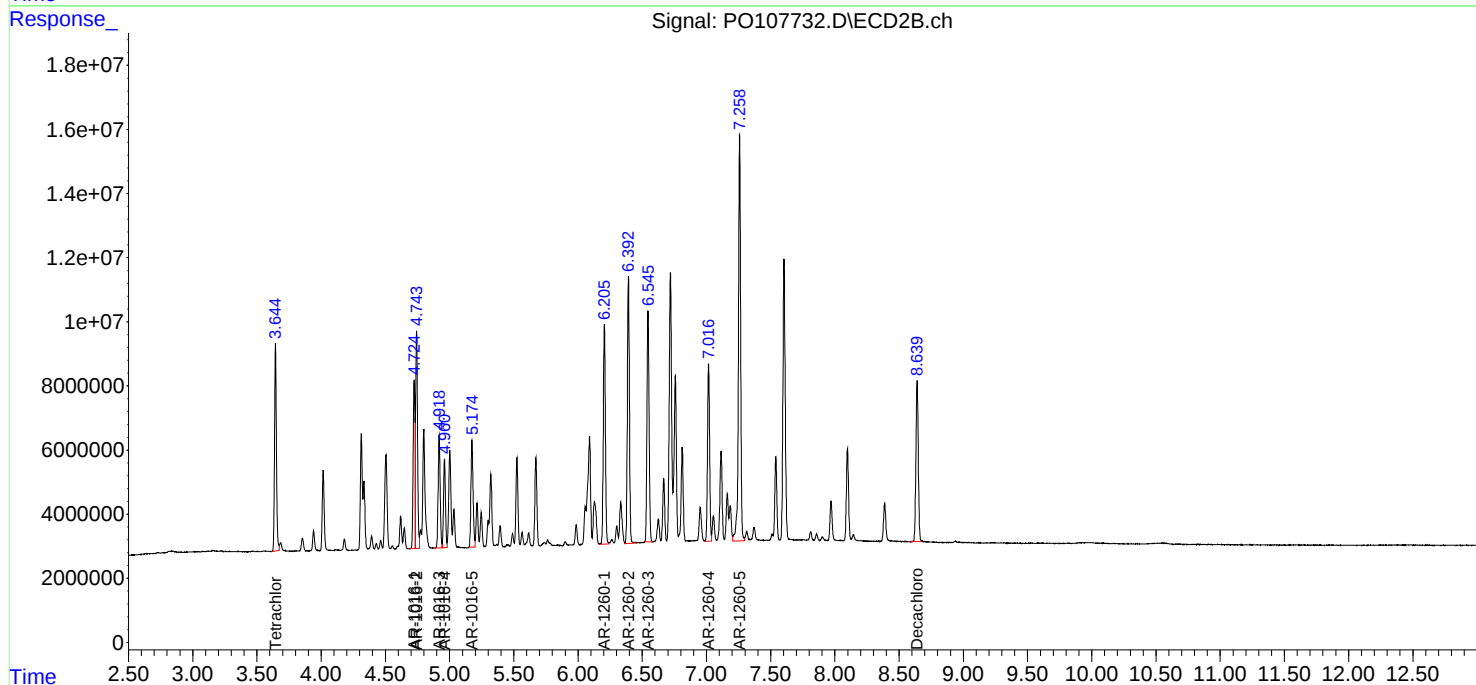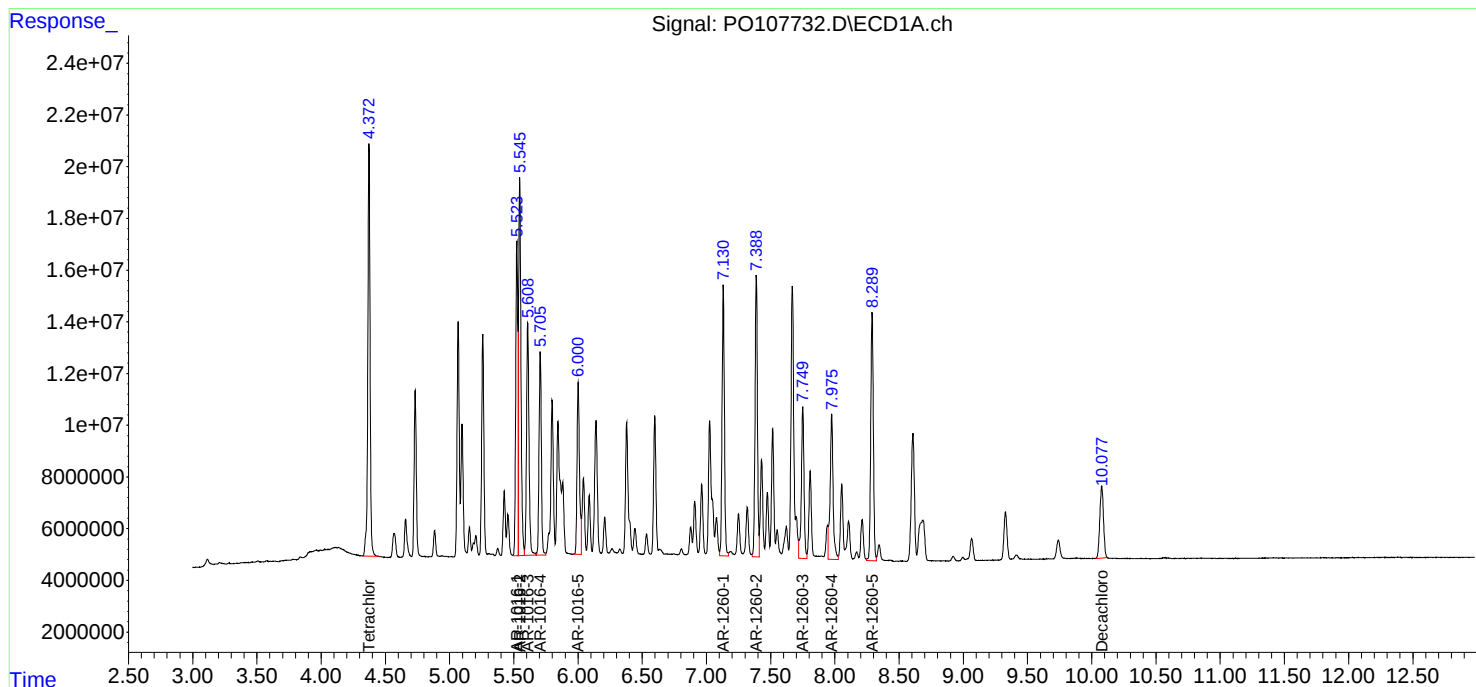

Report of Analysis

Client:	Portal Partners Tri-Venture		Date Collected:		
Project:	Amtrak Sawtooth Bridges 2024		Date Received:		
Client Sample ID:	PB164704BS		SDG No.:	P4718	
Lab Sample ID:	PB164704BS		Matrix:	WATER	
Analytical Method:	SW8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107747.D	1	11/06/24 08:25	11/06/24 18:31	PB164704

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	4.20		0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
11096-82-5	Aroclor-1260	4.30		0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.7		30 (10) - 150 (157)	93%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.8		30 (10) - 150 (173)	94%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 18:31
 Operator : YP/AJ
 Sample : PB164704BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB164704BS

Manual Integrations**APPROVED**

Reviewed By :Yogesh Patel 11/07/2024

Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:42:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.643	170.1E6	60074781	18.660	18.665
2) SA Decachlor...	10.074	8.638	46118064	50619964	18.798	18.464
Target Compounds						
3) L1 AR-1016-1	5.523	4.723	117.1E6	45751939	433.858	443.051
4) L1 AR-1016-2	5.545	4.742	168.5E6	63898497	424.550	453.284
5) L1 AR-1016-3	5.608	4.918	105.1E6	33507344	418.312	425.514
6) L1 AR-1016-4	5.705	4.959	83633165	25486426	434.206	385.525
7) L1 AR-1016-5	6.000	5.173	73111448	33503207	400.274	407.910
31) L7 AR-1260-1	7.129	6.204	104.4E6	68121902	403.836m	439.058
32) L7 AR-1260-2	7.386	6.391	117.9E6	81564327	447.861m	463.129
33) L7 AR-1260-3	7.748	6.545	67578108	75682256	375.966m	451.166
34) L7 AR-1260-4	7.974	7.015	81592652	56379969	464.905m	389.685
35) L7 AR-1260-5	8.289	7.256	111.9E6	136.7E6	393.419	415.085

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 18:31
Operator : YP/AJ
Sample : PB164704BS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB164704BS



Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:42:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

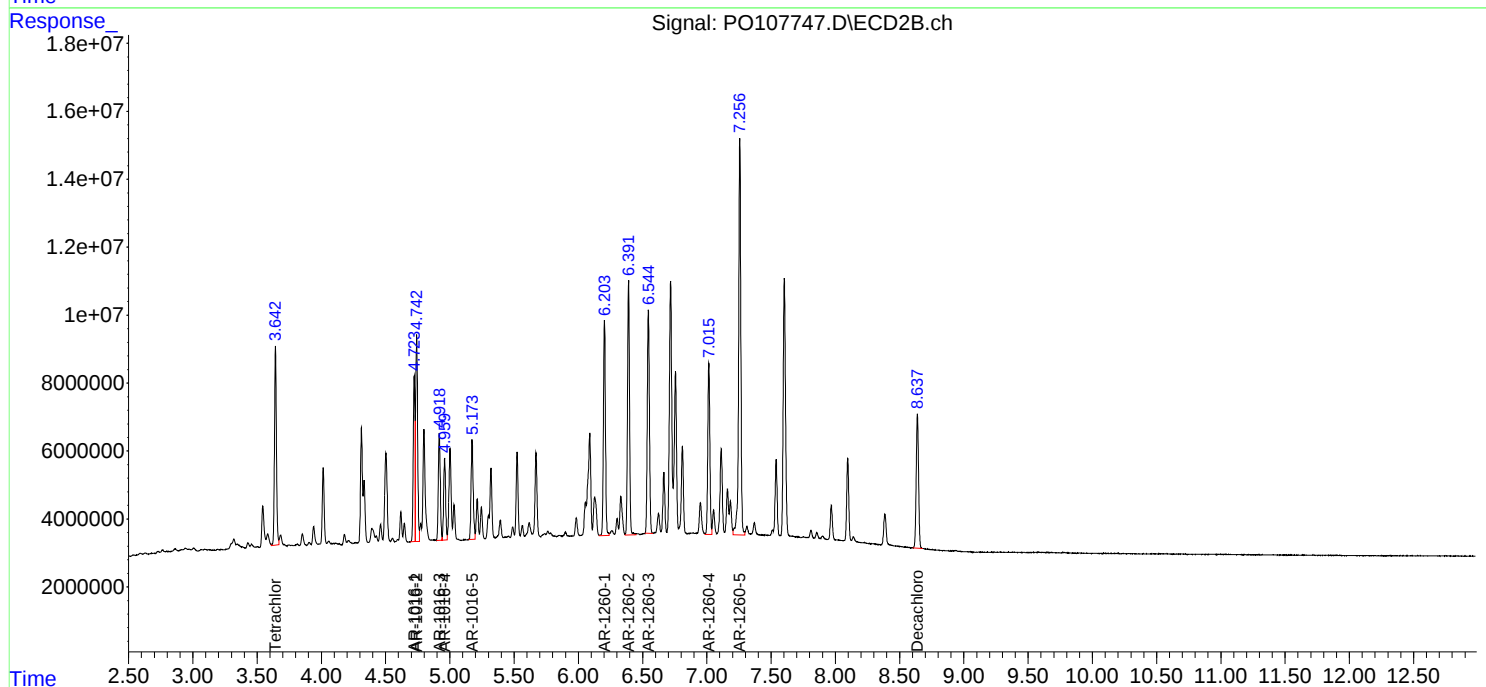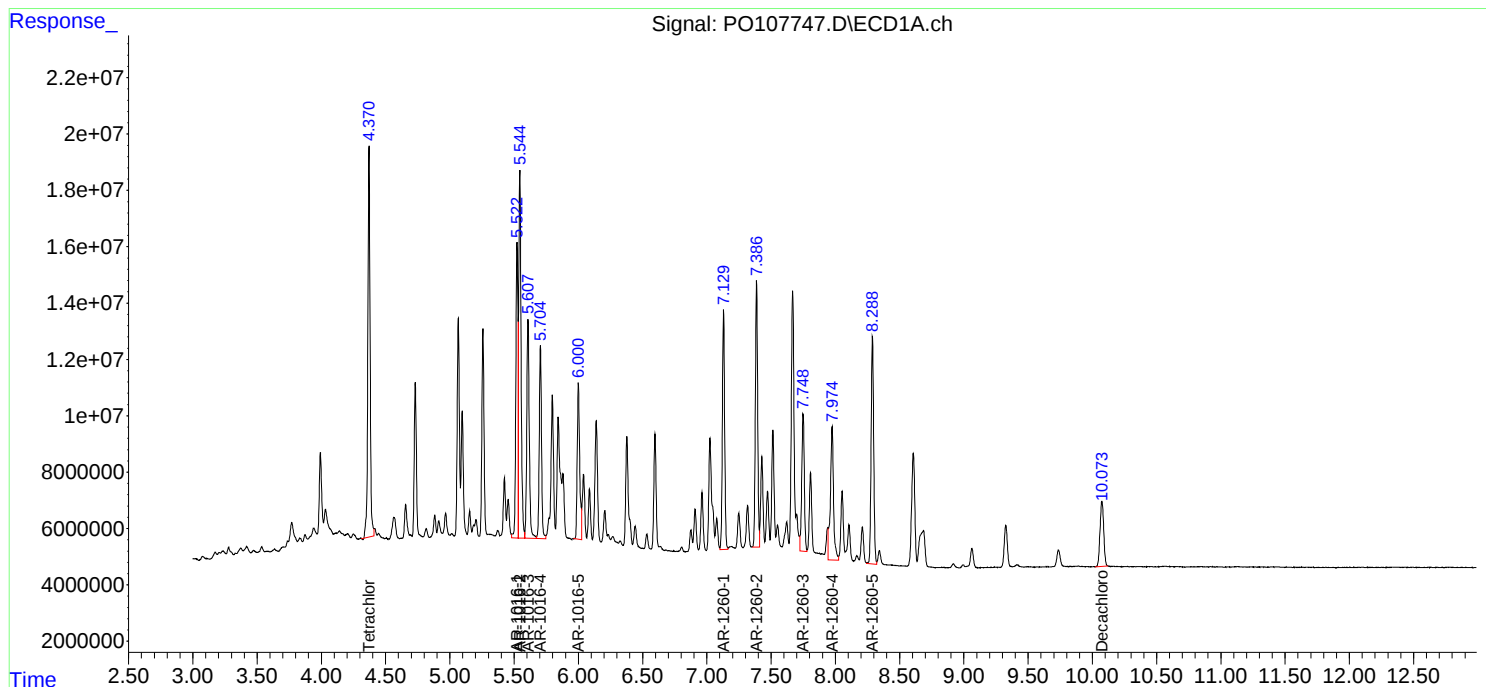

Report of Analysis

Client:	Portal Partners Tri-Venture		Date Collected:		
Project:	Amtrak Sawtooth Bridges 2024		Date Received:		
Client Sample ID:	PB164704BSD		SDG No.:	P4718	
Lab Sample ID:	PB164704BSD		Matrix:	WATER	
Analytical Method:	SW8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107748.D	1	11/06/24 08:25	11/06/24 18:47	PB164704

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	4.50		0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
11096-82-5	Aroclor-1260	4.50		0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.6		30 (10) - 150 (157)	98%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.5		30 (10) - 150 (173)	98%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107748.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 18:47
 Operator : YP/AJ
 Sample : PB164704BSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB164704BSD

Manual Integrations**APPROVED**

Reviewed By :Yogesh Patel 11/07/2024

Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:43:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.643	179.1E6	62155249	19.655	19.312
2) SA Decachlor...	10.076	8.638	47831458	52987232	19.496	19.327
Target Compounds						
3) L1 AR-1016-1	5.522	4.723	121.4E6	47636084	449.929	461.296
4) L1 AR-1016-2	5.545	4.742	174.1E6	66300185	438.696	470.322
5) L1 AR-1016-3	5.607	4.918	110.4E6	35609026	439.374	452.203
6) L1 AR-1016-4	5.705	4.960	87239370	27111910	452.928	410.113
7) L1 AR-1016-5	6.000	5.173	78851351	35566527	431.699	433.031
31) L7 AR-1260-1	7.129	6.204	106.0E6	70303008	409.806m	453.116
32) L7 AR-1260-2	7.386	6.391	122.6E6	84508840	465.917m	479.849
33) L7 AR-1260-3	7.749	6.544	71743188	78482348	399.138m	467.858
34) L7 AR-1260-4	7.974	7.015	76227838	58763052	434.337m	406.157
35) L7 AR-1260-5	8.289	7.257	116.9E6	142.4E6	411.157	432.180

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107748.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 18:47
Operator : YP/AJ
Sample : PB164704BSD
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB164704BSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:43:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

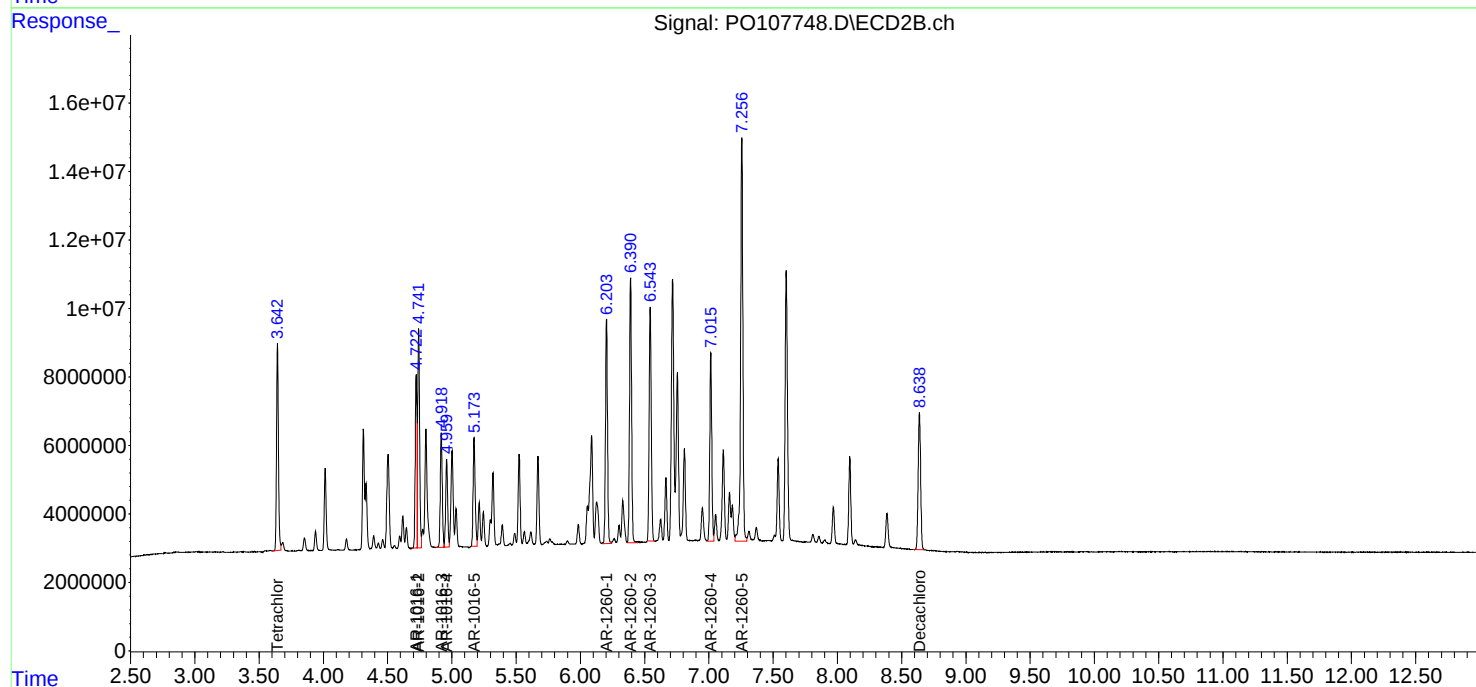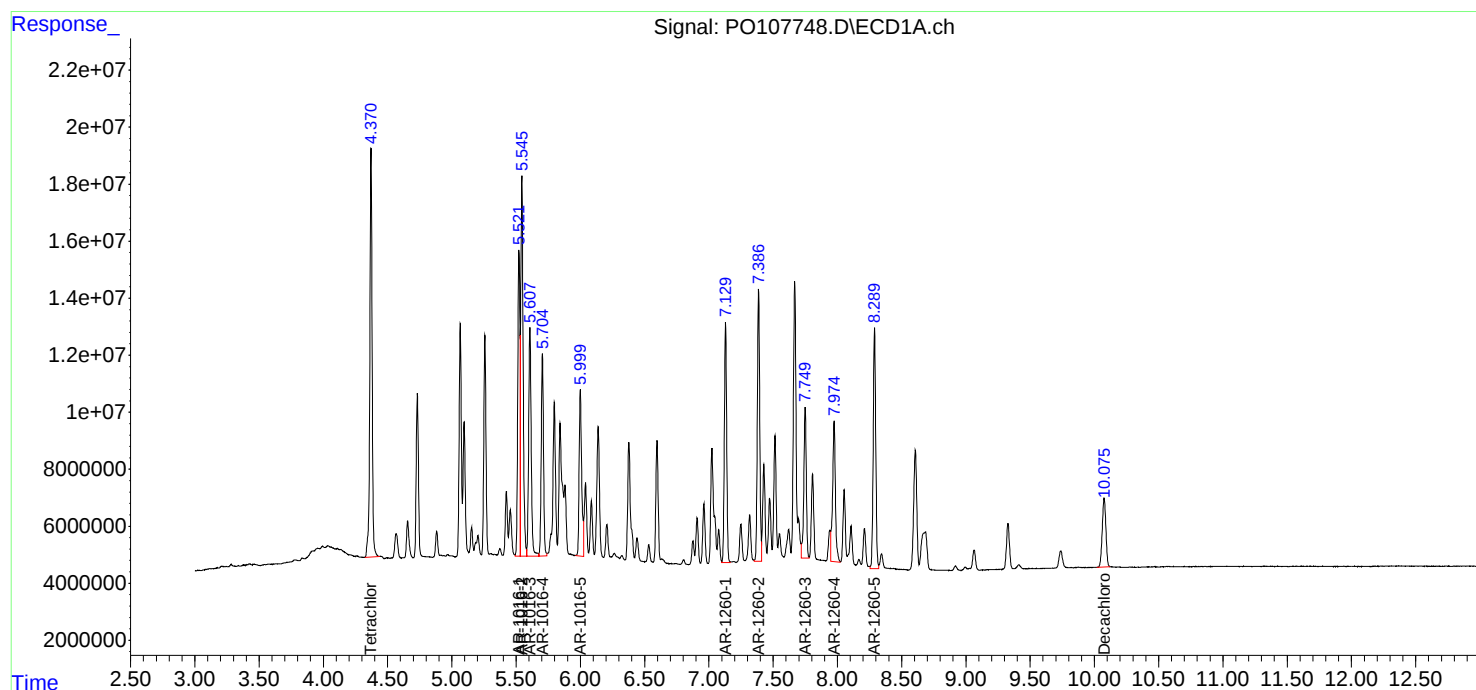

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/04/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/04/24
Client Sample ID:	TR-04-110424MS	SDG No.:	P4718
Lab Sample ID:	P4706-01MS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	93.5
Sample Wt/Vol:	30.03 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107736.D	1	11/06/24 09:10	11/06/24 14:30	PB164700

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	143		3.60	18.2	ug/kg
11104-28-2	Aroclor-1221	6.80	U	6.80	18.2	ug/kg
11141-16-5	Aroclor-1232	3.60	U	3.60	18.2	ug/kg
53469-21-9	Aroclor-1242	3.60	U	3.60	18.2	ug/kg
12672-29-6	Aroclor-1248	8.40	U	8.40	18.2	ug/kg
11097-69-1	Aroclor-1254	2.90	U	2.90	18.2	ug/kg
37324-23-5	Aroclor-1262	4.90	U	4.90	18.2	ug/kg
11100-14-4	Aroclor-1268	3.70	U	3.70	18.2	ug/kg
11096-82-5	Aroclor-1260	142		3.10	18.2	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	16.6		30 (32) - 150 (144)	83%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.9		30 (32) - 150 (175)	89%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 14:30
 Operator : YP/AJ
 Sample : P4706-01MS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-110424MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/07/2024
 Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:34:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.643	147.1E6	53355016	16.142m	16.578
2) SA Decachlor...	10.076	8.639	43865714	40338913	17.880	14.714
Target Compounds						
3) L1 AR-1016-1	5.523	4.723	110.0E6	43462795	407.788	420.883
4) L1 AR-1016-2	5.546	4.742	147.9E6	60169490	372.701	426.832
5) L1 AR-1016-3	5.608	4.918	95926694	31857064	381.920	404.557
6) L1 AR-1016-4	5.705	4.960	80053309	24592553	415.620	372.004
7) L1 AR-1016-5	5.999	5.172	67336051	30918011	368.654m	376.434
31) L7 AR-1260-1	7.130	6.204	100.6E6	55815921	389.170	359.744
32) L7 AR-1260-2	7.387	6.391	114.3E6	67433200	434.201	382.892
33) L7 AR-1260-3	7.749	6.544	61922678	60504417	344.503	360.686
34) L7 AR-1260-4	7.973	7.016	73926864	42919423	421.226m	296.649 #
35) L7 AR-1260-5	8.288	7.257	114.9E6	104.6E6	404.057	317.603

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 14:30
Operator : YP/AJ
Sample : P4706-01MS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

TR-04-110424MS

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 11/07/2024

Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:34:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

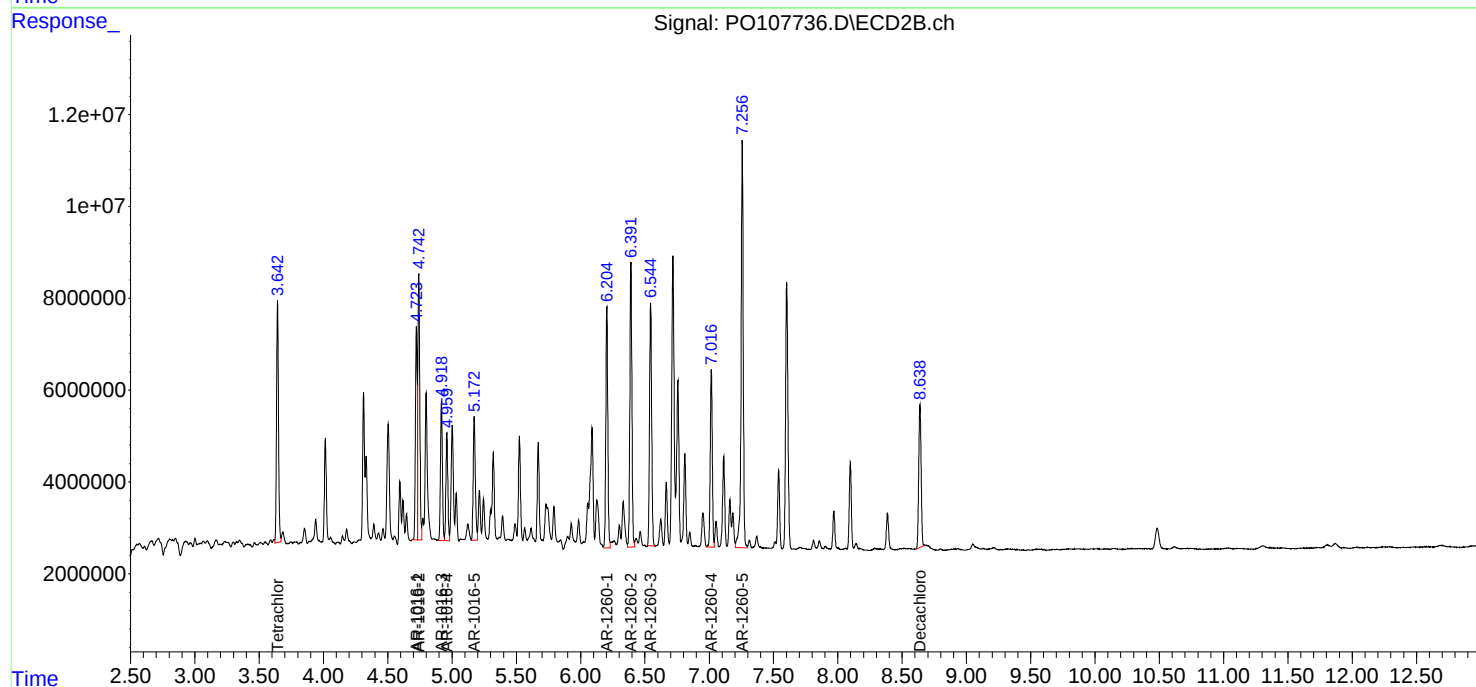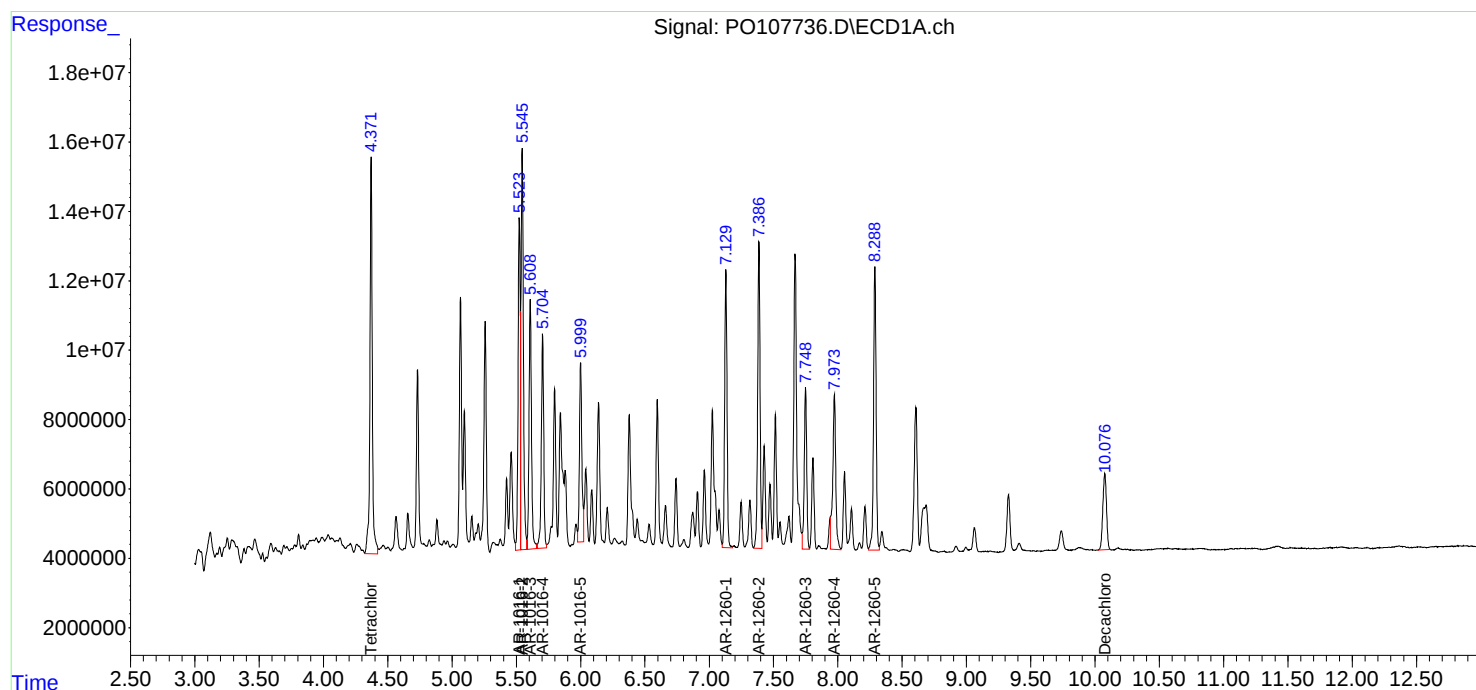

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	11/04/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	11/04/24
Client Sample ID:	TR-04-110424MSD	SDG No.:	P4718
Lab Sample ID:	P4706-01MSD	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	93.5
Sample Wt/Vol:	30.05 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO107737.D	1	11/06/24 09:10	11/06/24 14:46	PB164700

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	139		3.60	18.2	ug/kg
11104-28-2	Aroclor-1221	6.80	U	6.80	18.2	ug/kg
11141-16-5	Aroclor-1232	3.60	U	3.60	18.2	ug/kg
53469-21-9	Aroclor-1242	3.60	U	3.60	18.2	ug/kg
12672-29-6	Aroclor-1248	8.40	U	8.40	18.2	ug/kg
11097-69-1	Aroclor-1254	2.90	U	2.90	18.2	ug/kg
37324-23-5	Aroclor-1262	4.90	U	4.90	18.2	ug/kg
11100-14-4	Aroclor-1268	3.70	U	3.70	18.2	ug/kg
11096-82-5	Aroclor-1260	135		3.10	18.2	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	16.4		30 (32) - 150 (144)	82%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.2		30 (32) - 150 (175)	86%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
 Data File : PO107737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 14:46
 Operator : YP/AJ
 Sample : P4706-01MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

TR-04-110424MSD

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/07/2024

Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:35:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.643	140.5E6	52758307	15.411m	16.392
2) SA Decachlor...	10.076	8.639	42103541	37929995	17.161	13.835
Target Compounds						
3) L1 AR-1016-1	5.523	4.724	103.1E6	42420485	382.230	410.790
4) L1 AR-1016-2	5.545	4.743	140.4E6	58840351	353.867	417.403
5) L1 AR-1016-3	5.608	4.919	90547433	31220967	360.503	396.479
6) L1 AR-1016-4	5.705	4.960	75146983	24000225	390.147	363.044
7) L1 AR-1016-5	6.000	5.173	64995622	30315402	355.841m	369.098
31) L7 AR-1260-1	7.130	6.204	95080857	53484580	367.692	344.718
32) L7 AR-1260-2	7.387	6.391	107.9E6	64487662	409.936	366.167
33) L7 AR-1260-3	7.749	6.545	60416250	58073864	336.122	346.197
34) L7 AR-1260-4	7.974	7.016	69106702	41118906	393.762	284.204 #
35) L7 AR-1260-5	8.289	7.257	111.3E6	99587138	391.284	302.292

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 14:46
Operator : YP/AJ
Sample : P4706-01MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-110424MSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2024
Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:35:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

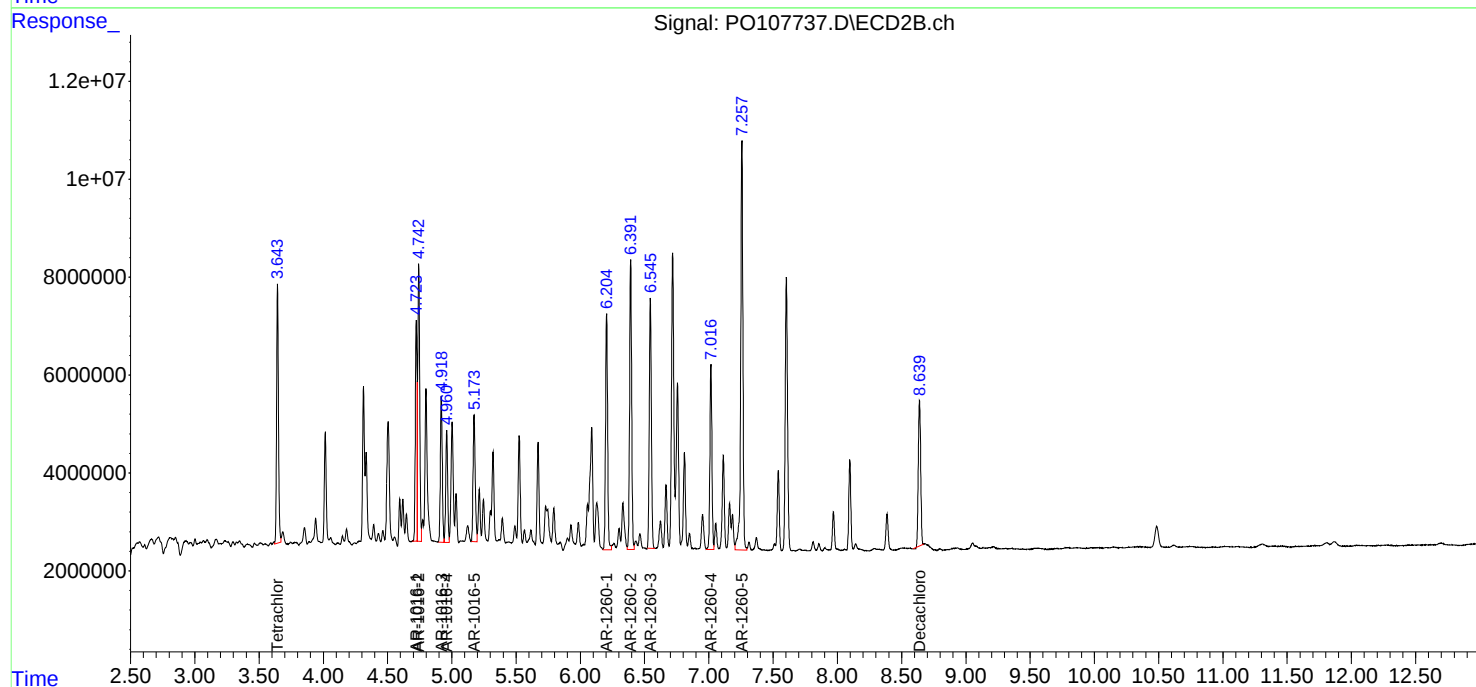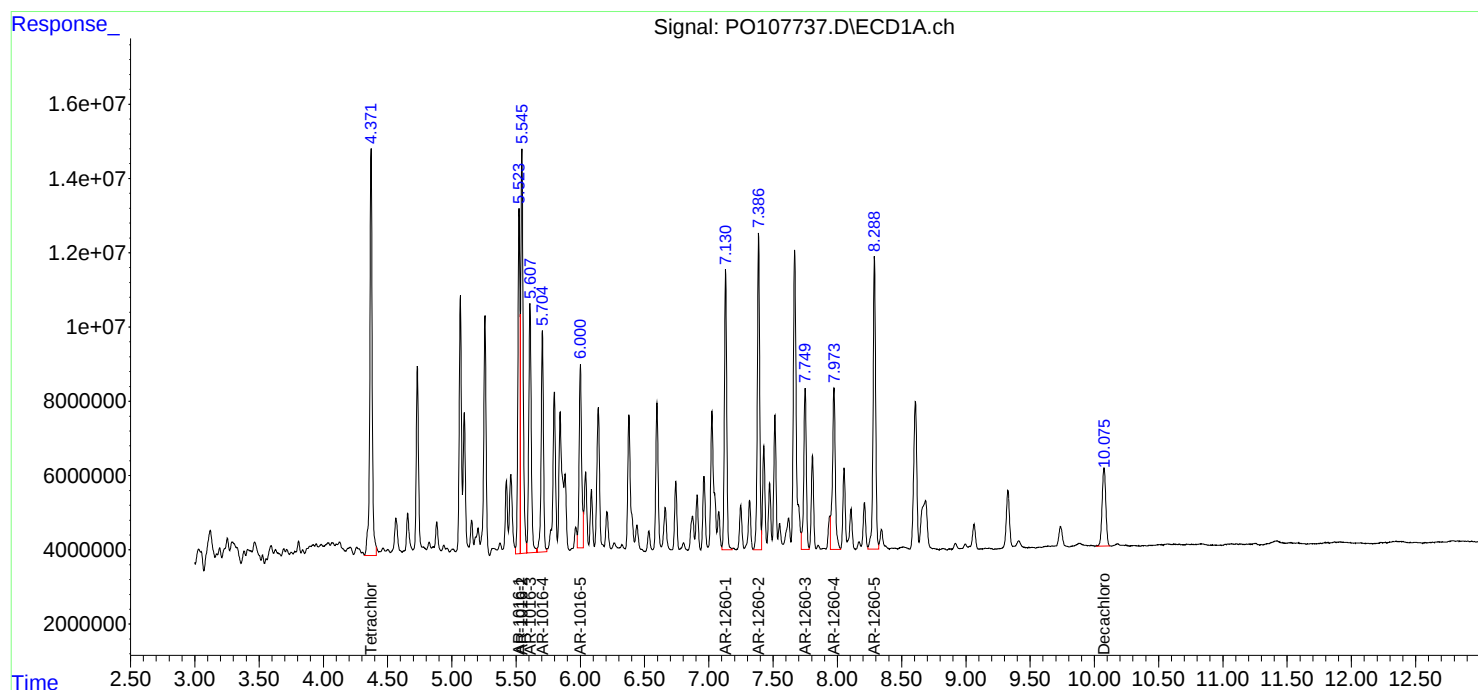

Manual Integration Report

Sequence:

po101524

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC050	PO107188.D	AR-1260-1 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-2 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-3	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-3 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-4 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-5	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	AR-1260-5 #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1660ICC050	PO107188.D	Decachlorobiphenyl #2	yogesh	10/16/2024 8:48:58 AM	Ankita	10/16/2024 9:57:34	Peak Integrated by Software
AR1268ICC050	PO107211.D	AR-1268-1	yogesh	10/16/2024 8:49:03 AM	Ankita	10/16/2024 9:57:36	Peak Integrated by Software

Manual Integration Report

Sequence:	PO110624	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254CCC500	PO107729.D	AR-1254-2 #2	yogesh	11/6/2024 4:45:16 PM	Ankita	11/7/2024 10:11:05	Peak Integrated by Software
PB164700BL	PO107731.D	Decachlorobiphenyl	yogesh	11/6/2024 4:45:16 PM	Ankita	11/7/2024 10:11:06	Peak Integrated by Software
P4706-01MS	PO107736.D	AR-1016-5	yogesh	11/7/2024 8:50:03 AM	Ankita	11/7/2024 10:11:10	Peak Integrated by Software
P4706-01MS	PO107736.D	AR-1260-4	yogesh	11/7/2024 8:50:03 AM	Ankita	11/7/2024 10:11:10	Peak Integrated by Software
P4706-01MS	PO107736.D	Tetrachloro-m-xylene	yogesh	11/7/2024 8:50:03 AM	Ankita	11/7/2024 10:11:10	Peak Integrated by Software
P4706-01MSD	PO107737.D	AR-1016-5	yogesh	11/7/2024 8:50:05 AM	Ankita	11/7/2024 10:11:12	Peak Integrated by Software
P4706-01MSD	PO107737.D	Tetrachloro-m-xylene	yogesh	11/7/2024 8:50:05 AM	Ankita	11/7/2024 10:11:12	Peak Integrated by Software
AR1254CCC500	PO107744.D	AR-1254-2 #2	yogesh	11/7/2024 8:50:08 AM	Ankita	11/7/2024 10:11:15	Peak Integrated by Software
PB164704BS	PO107747.D	AR-1260-1	yogesh	11/7/2024 8:50:09 AM	Ankita	11/7/2024 10:11:17	Peak Integrated by Software
PB164704BS	PO107747.D	AR-1260-2	yogesh	11/7/2024 8:50:09 AM	Ankita	11/7/2024 10:11:17	Peak Integrated by Software
PB164704BS	PO107747.D	AR-1260-3	yogesh	11/7/2024 8:50:09 AM	Ankita	11/7/2024 10:11:17	Peak Integrated by Software
PB164704BS	PO107747.D	AR-1260-4	yogesh	11/7/2024 8:50:09 AM	Ankita	11/7/2024 10:11:17	Peak Integrated by Software
PB164704BSD	PO107748.D	AR-1260-1	yogesh	11/7/2024 8:50:11 AM	Ankita	11/7/2024 10:11:19	Peak Integrated by Software

Manual Integration Report

Sequence:

PO110624

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
PB164704BSD	PO107748.D	AR-1260-2	yogesh	11/7/2024 8:50:11 AM	Ankita	11/7/2024 10:11:19	Peak Integrated by Software
PB164704BSD	PO107748.D	AR-1260-3	yogesh	11/7/2024 8:50:11 AM	Ankita	11/7/2024 10:11:19	Peak Integrated by Software
PB164704BSD	PO107748.D	AR-1260-4	yogesh	11/7/2024 8:50:11 AM	Ankita	11/7/2024 10:11:19	Peak Integrated by Software
AR1248CCC500	PO107758.D	AR-1248-5 #2	yogesh	11/7/2024 8:50:18 AM	Ankita	11/7/2024 10:11:29	Peak Integrated by Software
AR1254CCC500	PO107759.D	AR-1254-2 #2	yogesh	11/7/2024 8:50:19 AM	Ankita	11/7/2024 10:11:30	Peak Integrated by Software
AR1248CCC500	PO107765.D	Decachlorobiphenyl	yogesh	11/7/2024 8:50:23 AM	Ankita	11/7/2024 10:12:28	Peak Integrated by Software
AR1254CCC500	PO107766.D	AR-1254-2 #2	yogesh	11/7/2024 8:50:24 AM	Ankita	11/7/2024 10:12:29	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO107180.D	15 Oct 2024 13:05	YP/AJ	Ok
2	AR1660CCC500	PO107181.D	15 Oct 2024 13:23	YP/AJ	Not Ok
3	HEXANE	PO107182.D	15 Oct 2024 17:50	YP/AJ	Ok
4	I.BLK	PO107183.D	15 Oct 2024 18:08	YP/AJ	Ok
5	AR1660ICC1000	PO107184.D	15 Oct 2024 18:27	YP/AJ	Ok
6	AR1660ICC750	PO107185.D	15 Oct 2024 18:45	YP/AJ	Ok
7	AR1660ICC500	PO107186.D	15 Oct 2024 19:03	YP/AJ	Ok
8	AR1660ICC250	PO107187.D	15 Oct 2024 19:21	YP/AJ	Ok
9	AR1660ICC050	PO107188.D	15 Oct 2024 19:39	YP/AJ	Ok,M
10	AR1221ICC500	PO107189.D	15 Oct 2024 19:57	YP/AJ	Ok
11	AR1232ICC500	PO107190.D	15 Oct 2024 20:15	YP/AJ	Ok
12	AR1242ICC1000	PO107191.D	15 Oct 2024 20:34	YP/AJ	Ok
13	AR1242ICC750	PO107192.D	15 Oct 2024 20:52	YP/AJ	Ok
14	AR1242ICC500	PO107193.D	15 Oct 2024 21:10	YP/AJ	Ok
15	AR1242ICC250	PO107194.D	15 Oct 2024 21:28	YP/AJ	Ok
16	AR1242ICC050	PO107195.D	15 Oct 2024 21:46	YP/AJ	Ok
17	AR1248ICC1000	PO107196.D	15 Oct 2024 22:04	YP/AJ	Ok
18	AR1248ICC750	PO107197.D	15 Oct 2024 22:22	YP/AJ	Ok
19	AR1248ICC500	PO107198.D	15 Oct 2024 22:41	YP/AJ	Ok
20	AR1248ICC250	PO107199.D	15 Oct 2024 22:59	YP/AJ	Ok
21	AR1248ICC050	PO107200.D	15 Oct 2024 23:17	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC1000	PO107201.D	15 Oct 2024 23:35	YP/AJ	Ok
23	AR1254ICC750	PO107202.D	15 Oct 2024 23:53	YP/AJ	Ok
24	AR1254ICC500	PO107203.D	16 Oct 2024 00:11	YP/AJ	Ok
25	AR1254ICC250	PO107204.D	16 Oct 2024 00:29	YP/AJ	Ok
26	AR1254ICC050	PO107205.D	16 Oct 2024 00:47	YP/AJ	Ok
27	AR1262ICC500	PO107206.D	16 Oct 2024 01:05	YP/AJ	Ok
28	AR1268ICC1000	PO107207.D	16 Oct 2024 01:23	YP/AJ	Ok
29	AR1268ICC750	PO107208.D	16 Oct 2024 01:41	YP/AJ	Ok
30	AR1268ICC500	PO107209.D	16 Oct 2024 01:59	YP/AJ	Ok
31	AR1268ICC250	PO107210.D	16 Oct 2024 02:18	YP/AJ	Ok
32	AR1268ICC050	PO107211.D	16 Oct 2024 02:36	YP/AJ	Ok,M
33	PO101524ICV500	PO107212.D	16 Oct 2024 02:54	YP/AJ	Ok
34	AR1242ICV500	PO107213.D	16 Oct 2024 03:12	YP/AJ	Ok
35	AR1248ICV500	PO107214.D	16 Oct 2024 03:30	YP/AJ	Ok
36	AR1254ICV500	PO107215.D	16 Oct 2024 03:48	YP/AJ	Ok
37	AR1268ICV500	PO107216.D	16 Oct 2024 04:06	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110624

Review By	yogesh	Review On	11/7/2024 8:50:43 AM
Supervise By	Ankita	Supervise On	11/7/2024 10:12:36 AM
SubDirectory	PO110624	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO107725.D	06 Nov 2024 09:13	YP/AJ	Ok
2	AR1660CCC500	PO107726.D	06 Nov 2024 09:29	YP/AJ	Ok
3	AR1242CCC500	PO107727.D	06 Nov 2024 09:45	YP/AJ	Ok
4	AR1248CCC500	PO107728.D	06 Nov 2024 10:01	YP/AJ	Ok
5	AR1254CCC500	PO107729.D	06 Nov 2024 10:17	YP/AJ	Ok,M
6	I.BLK	PO107730.D	06 Nov 2024 10:33	YP/AJ	Ok
7	PB164700BL	PO107731.D	06 Nov 2024 13:10	YP/AJ	Ok,M
8	PB164700BS	PO107732.D	06 Nov 2024 13:26	YP/AJ	Ok
9	P4709-01	PO107733.D	06 Nov 2024 13:42	YP/AJ	Ok
10	P4709-03	PO107734.D	06 Nov 2024 13:58	YP/AJ	Ok
11	P4706-01	PO107735.D	06 Nov 2024 14:14	YP/AJ	Ok,M
12	P4706-01MS	PO107736.D	06 Nov 2024 14:30	YP/AJ	Ok,M
13	P4706-01MSD	PO107737.D	06 Nov 2024 14:46	YP/AJ	Ok,M
14	P4707-01	PO107738.D	06 Nov 2024 15:03	YP/AJ	Ok
15	P4708-01	PO107739.D	06 Nov 2024 15:19	YP/AJ	Ok,M
16	P4718-01	PO107740.D	06 Nov 2024 15:35	YP/AJ	Ok
17	AR1660CCC500	PO107741.D	06 Nov 2024 16:54	YP/AJ	Ok
18	AR1242CCC500	PO107742.D	06 Nov 2024 17:10	YP/AJ	Ok
19	AR1248CCC500	PO107743.D	06 Nov 2024 17:26	YP/AJ	Ok
20	AR1254CCC500	PO107744.D	06 Nov 2024 17:43	YP/AJ	Ok,M
21	I.BLK	PO107745.D	06 Nov 2024 17:59	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110624

Review By	yogesh	Review On	11/7/2024 8:50:43 AM
Supervise By	Ankita	Supervise On	11/7/2024 10:12:36 AM
SubDirectory	PO110624	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	PB164704BL	PO107746.D	06 Nov 2024 18:15	YP/AJ	Ok
23	PB164704BS	PO107747.D	06 Nov 2024 18:31	YP/AJ	Ok,M
24	PB164704BSD	PO107748.D	06 Nov 2024 18:47	YP/AJ	Ok,M
25	P4661-03	PO107749.D	06 Nov 2024 19:03	YP/AJ	Ok,M
26	P4684-03	PO107750.D	06 Nov 2024 19:20	YP/AJ	Ok
27	P4702-01	PO107751.D	06 Nov 2024 19:36	YP/AJ	Ok
28	P4704-01	PO107752.D	06 Nov 2024 19:52	YP/AJ	Dilution
29	P4704-02	PO107753.D	06 Nov 2024 20:08	YP/AJ	Ok,M
30	P4704-03	PO107754.D	06 Nov 2024 20:24	YP/AJ	Ok
31	P4718-04	PO107755.D	06 Nov 2024 20:41	YP/AJ	Ok
32	AR1660CCC500	PO107756.D	06 Nov 2024 21:42	YP/AJ	Ok
33	AR1242CCC500	PO107757.D	06 Nov 2024 21:58	YP/AJ	Ok
34	AR1248CCC500	PO107758.D	06 Nov 2024 22:14	YP/AJ	Ok,M
35	AR1254CCC500	PO107759.D	06 Nov 2024 22:30	YP/AJ	Ok,M
36	I.BLK	PO107760.D	06 Nov 2024 22:46	YP/AJ	Ok
37	P4718-02	PO107761.D	06 Nov 2024 23:02	YP/AJ	Ok
38	P4719-01	PO107762.D	06 Nov 2024 23:19	YP/AJ	Ok,M
39	AR1660CCC500	PO107763.D	07 Nov 2024 00:20	YP/AJ	Ok
40	AR1242CCC500	PO107764.D	07 Nov 2024 00:36	YP/AJ	Ok
41	AR1248CCC500	PO107765.D	07 Nov 2024 00:53	YP/AJ	Ok,M
42	AR1254CCC500	PO107766.D	07 Nov 2024 01:09	YP/AJ	Ok,M
43	I.BLK	PO107767.D	07 Nov 2024 01:25	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO107180.D	15 Oct 2024 13:05		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO107181.D	15 Oct 2024 13:23	need ICAL	YP/AJ	Not Ok
3	HEXANE	HEXANE	PO107182.D	15 Oct 2024 17:50		YP/AJ	Ok
4	I.BLK	I.BLK	PO107183.D	15 Oct 2024 18:08		YP/AJ	Ok
5	AR1660ICC1000	AR1660ICC1000	PO107184.D	15 Oct 2024 18:27		YP/AJ	Ok
6	AR1660ICC750	AR1660ICC750	PO107185.D	15 Oct 2024 18:45		YP/AJ	Ok
7	AR1660ICC500	AR1660ICC500	PO107186.D	15 Oct 2024 19:03		YP/AJ	Ok
8	AR1660ICC250	AR1660ICC250	PO107187.D	15 Oct 2024 19:21		YP/AJ	Ok
9	AR1660ICC050	AR1660ICC050	PO107188.D	15 Oct 2024 19:39		YP/AJ	Ok,M
10	AR1221ICC500	AR1221ICC500	PO107189.D	15 Oct 2024 19:57		YP/AJ	Ok
11	AR1232ICC500	AR1232ICC500	PO107190.D	15 Oct 2024 20:15		YP/AJ	Ok
12	AR1242ICC1000	AR1242ICC1000	PO107191.D	15 Oct 2024 20:34		YP/AJ	Ok
13	AR1242ICC750	AR1242ICC750	PO107192.D	15 Oct 2024 20:52		YP/AJ	Ok
14	AR1242ICC500	AR1242ICC500	PO107193.D	15 Oct 2024 21:10		YP/AJ	Ok
15	AR1242ICC250	AR1242ICC250	PO107194.D	15 Oct 2024 21:28		YP/AJ	Ok
16	AR1242ICC050	AR1242ICC050	PO107195.D	15 Oct 2024 21:46		YP/AJ	Ok
17	AR1248ICC1000	AR1248ICC1000	PO107196.D	15 Oct 2024 22:04		YP/AJ	Ok
18	AR1248ICC750	AR1248ICC750	PO107197.D	15 Oct 2024 22:22		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248ICC500	AR1248ICC500	PO107198.D	15 Oct 2024 22:41		YP/AJ	Ok
20	AR1248ICC250	AR1248ICC250	PO107199.D	15 Oct 2024 22:59		YP/AJ	Ok
21	AR1248ICC050	AR1248ICC050	PO107200.D	15 Oct 2024 23:17		YP/AJ	Ok
22	AR1254ICC1000	AR1254ICC1000	PO107201.D	15 Oct 2024 23:35		YP/AJ	Ok
23	AR1254ICC750	AR1254ICC750	PO107202.D	15 Oct 2024 23:53		YP/AJ	Ok
24	AR1254ICC500	AR1254ICC500	PO107203.D	16 Oct 2024 00:11		YP/AJ	Ok
25	AR1254ICC250	AR1254ICC250	PO107204.D	16 Oct 2024 00:29		YP/AJ	Ok
26	AR1254ICC050	AR1254ICC050	PO107205.D	16 Oct 2024 00:47		YP/AJ	Ok
27	AR1262ICC500	AR1262ICC500	PO107206.D	16 Oct 2024 01:05		YP/AJ	Ok
28	AR1268ICC1000	AR1268ICC1000	PO107207.D	16 Oct 2024 01:23		YP/AJ	Ok
29	AR1268ICC750	AR1268ICC750	PO107208.D	16 Oct 2024 01:41		YP/AJ	Ok
30	AR1268ICC500	AR1268ICC500	PO107209.D	16 Oct 2024 01:59		YP/AJ	Ok
31	AR1268ICC250	AR1268ICC250	PO107210.D	16 Oct 2024 02:18		YP/AJ	Ok
32	AR1268ICC050	AR1268ICC050	PO107211.D	16 Oct 2024 02:36		YP/AJ	Ok,M
33	PO101524ICV500	ICVPO101524	PO107212.D	16 Oct 2024 02:54		YP/AJ	Ok
34	AR1242ICV500	ICVPO101524AR1242	PO107213.D	16 Oct 2024 03:12		YP/AJ	Ok
35	AR1248ICV500	ICVPO101524AR1248	PO107214.D	16 Oct 2024 03:30		YP/AJ	Ok
36	AR1254ICV500	ICVPO101524AR1254	PO107215.D	16 Oct 2024 03:48		YP/AJ	Ok
37	AR1268ICV500	ICVPO101524AR1268	PO107216.D	16 Oct 2024 04:06		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO101524

Review By	yogesh	Review On	10/16/2024 8:49:12 AM
Supervise By	Ankita	Supervise On	10/16/2024 9:57:42 AM
SubDirectory	PO101524	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23792		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110624

Review By	yogesh	Review On	11/7/2024 8:50:43 AM
Supervise By	Ankita	Supervise On	11/7/2024 10:12:36 AM
SubDirectory	PO110624	HP Acquire Method	HP Processing Method PO101524

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO107725.D	06 Nov 2024 09:13		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO107726.D	06 Nov 2024 09:29		YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO107727.D	06 Nov 2024 09:45		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO107728.D	06 Nov 2024 10:01		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO107729.D	06 Nov 2024 10:17		YP/AJ	Ok,M
6	I.BLK	I.BLK	PO107730.D	06 Nov 2024 10:33		YP/AJ	Ok
7	PB164700BL	PB164700BL	PO107731.D	06 Nov 2024 13:10		YP/AJ	Ok,M
8	PB164700BS	PB164700BS	PO107732.D	06 Nov 2024 13:26		YP/AJ	Ok
9	P4709-01	HR-02-110424	PO107733.D	06 Nov 2024 13:42		YP/AJ	Ok
10	P4709-03	HR-03-110424	PO107734.D	06 Nov 2024 13:58		YP/AJ	Ok
11	P4706-01	TR-04-110424	PO107735.D	06 Nov 2024 14:14		YP/AJ	Ok,M
12	P4706-01MS	TR-04-110424MS	PO107736.D	06 Nov 2024 14:30		YP/AJ	Ok,M
13	P4706-01MSD	TR-04-110424MSD	PO107737.D	06 Nov 2024 14:46		YP/AJ	Ok,M
14	P4707-01	HD-02-110424	PO107738.D	06 Nov 2024 15:03		YP/AJ	Ok
15	P4708-01	OR-02-110424	PO107739.D	06 Nov 2024 15:19		YP/AJ	Ok,M
16	P4718-01	WB-307-SB01	PO107740.D	06 Nov 2024 15:35		YP/AJ	Ok
17	AR1660CCC500	AR1660CCC500	PO107741.D	06 Nov 2024 16:54		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110624

Review By	yogesh	Review On	11/7/2024 8:50:43 AM
Supervise By	Ankita	Supervise On	11/7/2024 10:12:36 AM
SubDirectory	PO110624	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

18	AR1242CCC500	AR1242CCC500	PO107742.D	06 Nov 2024 17:10	AR1242 3 peak low in 1st column	YP/AJ	Ok
19	AR1248CCC500	AR1248CCC500	PO107743.D	06 Nov 2024 17:26		YP/AJ	Ok
20	AR1254CCC500	AR1254CCC500	PO107744.D	06 Nov 2024 17:43		YP/AJ	Ok,M
21	I.BLK	I.BLK	PO107745.D	06 Nov 2024 17:59		YP/AJ	Ok
22	PB164704BL	PB164704BL	PO107746.D	06 Nov 2024 18:15		YP/AJ	Ok
23	PB164704BS	PB164704BS	PO107747.D	06 Nov 2024 18:31		YP/AJ	Ok,M
24	PB164704BSD	PB164704BSD	PO107748.D	06 Nov 2024 18:47		YP/AJ	Ok,M
25	P4661-03	102324-A	PO107749.D	06 Nov 2024 19:03		YP/AJ	Ok,M
26	P4684-03	MECHANIC-ST-OIL-W	PO107750.D	06 Nov 2024 19:20		YP/AJ	Ok
27	P4702-01	TOTE-1	PO107751.D	06 Nov 2024 19:36		YP/AJ	Ok
28	P4704-01	NWB-2111	PO107752.D	06 Nov 2024 19:52	AR1242 Hit, Need 10x Dilution	YP/AJ	Dilution
29	P4704-02	NWB-2056	PO107753.D	06 Nov 2024 20:08		YP/AJ	Ok,M
30	P4704-03	NWB-2108	PO107754.D	06 Nov 2024 20:24		YP/AJ	Ok
31	P4718-04	WB-307-SW	PO107755.D	06 Nov 2024 20:41		YP/AJ	Ok
32	AR1660CCC500	AR1660CCC500	PO107756.D	06 Nov 2024 21:42		YP/AJ	Ok
33	AR1242CCC500	AR1242CCC500	PO107757.D	06 Nov 2024 21:58		YP/AJ	Ok
34	AR1248CCC500	AR1248CCC500	PO107758.D	06 Nov 2024 22:14		YP/AJ	Ok,M
35	AR1254CCC500	AR1254CCC500	PO107759.D	06 Nov 2024 22:30		YP/AJ	Ok,M
36	I.BLK	I.BLK	PO107760.D	06 Nov 2024 22:46		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO110624

Review By	yogesh	Review On	11/7/2024 8:50:43 AM
Supervise By	Ankita	Supervise On	11/7/2024 10:12:36 AM
SubDirectory	PO110624	HP Acquire Method	HP Processing Method PO101524
STD. NAME	STD REF.#		
Tune/Reschk	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775 PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773 PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

37	P4718-02	WB-307-SB02	PO107761.D	06 Nov 2024 23:02		YP/AJ	Ok
38	P4719-01	BAYAVE-STOCKPILE	PO107762.D	06 Nov 2024 23:19	AR1254 Hit	YP/AJ	Ok,M
39	AR1660CCC500	AR1660CCC500	PO107763.D	07 Nov 2024 00:20		YP/AJ	Ok
40	AR1242CCC500	AR1242CCC500	PO107764.D	07 Nov 2024 00:36		YP/AJ	Ok
41	AR1248CCC500	AR1248CCC500	PO107765.D	07 Nov 2024 00:53		YP/AJ	Ok,M
42	AR1254CCC500	AR1254CCC500	PO107766.D	07 Nov 2024 01:09		YP/AJ	Ok,M
43	I.BLK	I.BLK	PO107767.D	07 Nov 2024 01:25		YP/AJ	Ok

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 11/6/2024

OVENTEMP IN Celsius(°C): 107
Time IN: 17:00
In Date: 11/05/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 103
Time OUT: 08:00
Out Date: 11/06/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB133300

Lab ID	Client SampleID	Dish #	Dish Wt (g) (A)	Sample Wt (g)	Dish + Sample Wt (g) (B)	Dish+Dry Sample Wt (g) (C)	% Solid	Comments
P4452-04	ETGI-285	1	1.00	1.00	2.00	2.00	100.0	CONCRETE sample
P4706-01	TR-04-110424	2	1.16	8.71	9.87	9.3	93.5	
P4706-02	TR-04-110424-E2	3	1.17	8.55	9.72	8.81	89.4	
P4707-01	HD-02-110424	4	1.18	8.57	9.75	9.21	93.7	
P4707-02	HD-02-110424-E2	5	1.14	8.40	9.54	9.07	94.4	
P4708-01	OR-02-110424	6	1.15	8.66	9.81	9.26	93.6	
P4708-02	OR-02-110424-E2	7	1.19	8.76	9.95	9.39	93.6	
P4709-01	HR-02-110424	8	1.16	8.71	9.87	8.79	87.6	
P4709-02	HR-02-110424-E2	9	1.14	8.82	9.96	8.76	86.4	
P4709-03	HR-03-110424	10	1.15	8.83	9.98	9.32	92.5	
P4709-04	HR-03-110424-E2	11	1.19	8.48	9.67	8.9	90.9	
P4718-01	WB-307-SB01	12	1.17	8.40	9.57	7.72	78.0	
P4718-02	WB-307-SB02	13	1.15	8.83	9.98	8.00	77.6	
P4719-01	BAYAVE-STOCKPILE	14	1.16	8.48	9.64	9.42	97.4	
P4719-02	BAYAVE-STOCKPILE-E2	15	1.17	8.67	9.84	9.3	93.8	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

133300

WorkList Name : %1-110524

WorkList ID : 185126

Department : Wet-Chemistry

Date : 11-05-2024 08:12:46

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P4452-04	ETGI-285	Solid	Percent Solids	Cool 4 deg C	PSEG03	K51	10/18/2024	Chemtech -SO
P4706-01	TR-04-110424	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4706-02	TR-04-110424-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4707-01	HD-02-110424	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4707-02	HD-02-110424-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4708-01	OR-02-110424	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4708-02	OR-02-110424-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4709-01	HR-02-110424	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4709-02	HR-02-110424-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4709-03	HR-03-110424	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4709-04	HR-03-110424-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4718-01	WB-307-SB01	Solid	Percent Solids	Cool 4 deg C	PSEG05	L23	11/04/2024	Chemtech -SO
P4718-02	WB-307-SB02	Solid	Percent Solids	Cool 4 deg C	PORT06	L21	11/04/2024	Chemtech -SO
P4719-01	BAYAVE-STOCKPILE	Solid	Percent Solids	Cool 4 deg C	PORT06	L21	11/04/2024	Chemtech -SO
P4719-02	BAYAVE-STOCKPILE-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	K21	11/05/2024	Chemtech -SO
					PSEG03	K21	11/05/2024	Chemtech -SO

Date/Time 11/05/24 15:40

Raw Sample Received by: ad woc

Raw Sample Relinquished by: ad woc

Date/Time 11/05/24

Raw Sample Received by: ad woc

Raw Sample Relinquished by: ad woc

SOP ID: M3541-ASE Extraction-14

Clean Up SOP #: Acid Cleanup

Matrix: Solid

Weigh By: RJ

Balance check: RJ

Balance ID: EX-SC-2

pH Strip Lot#: N/A

Extraction By: RJ

Filter By: RJ

pH Meter ID: N/A

Hood ID: 3,7

Extraction Start Date: 11/06/2024

Extraction Start Time: 09:10

Extraction End Date: 11/06/2024

Extraction End Time: 12:10

Concentration By: RS

Supervisor By: rajesh

Extraction Method: ☐ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☒ Soxhlet

Standardized Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP23640
Surrogate	1.0ML	200 PPB	PP23858
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2539
Baked Na2SO4	N/A	EP2556
Hexane	N/A	E3825
Sand	N/A	E2865
H2SO4 1:1	N/A	EP2548
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40BTS721.

KD Bath ID: N/A

KD Bath Temperature: N/A

Envap ID: NEVAP-02

Envap Temperature: 40 °C


Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
11/6/24	RP (EPT-105)	AJ/EST PCB Lab
12:15	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-14

Concentration Date: 11/06/2024

Sample ID	Client Sample ID	Test	g / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB164700BL	ABLK700	PCB	30.01	N/A	ritesh	RUPESH	10			U5-1
PB164700BS	ALCS700	PCB	30.03	N/A	ritesh	RUPESH	10			2
P4706-01	TR-04-110424	PCB	30.09	N/A	ritesh	RUPESH	10	D		3
P4706-01MS	TR-04-110424MS	PCB	30.03	N/A	ritesh	RUPESH	10	D		4
P4706-01MS D	TR-04-110424MSD	PCB	30.05	N/A	ritesh	RUPESH	10	D		5
P4707-01	HD-02-110424	PCB	30.02	N/A	ritesh	RUPESH	10	D		6
P4708-01	OR-02-110424	PCB	30.01	N/A	ritesh	RUPESH	10	D		U6-1
P4709-01	HR-02-110424	PCB	30.10	N/A	ritesh	RUPESH	10	D		2
P4709-03	HR-03-110424	PCB	30.08	N/A	ritesh	RUPESH	10	D		3
P4718-01	WB-307-SB01	PCB	30.06	N/A	ritesh	RUPESH	10	E		4
P4718-02	WB-307-SB02	PCB	30.03	N/A	ritesh	RUPESH	10	E		5
P4719-01	BAYAVE-STOCKPILE	PCB	30.05	N/A	ritesh	RUPESH	10	E		6

* Extracts relinquished on the same date as received.



164703
09/11/24

WORKLIST(Hardcopy Internal Chain)

WorkList Name : P4706 WorkList ID : 185154 Department : Extraction Date : 11-06-2024 08:17:18

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P4706-01	TR-04-110424	Solid	PCB	Cool 4 deg C	PSEG05	L23	11/04/2024	8082A
P4707-01	HD-02-110424	Solid	PCB	Cool 4 deg C	PSEG05	L23	11/04/2024	8082A
P4708-01	OR-02-110424	Solid	PCB	Cool 4 deg C	PSEG05	L23	11/04/2024	8082A
P4709-01	HR-02-110424	Solid	PCB	Cool 4 deg C	PSEG05	L23	11/04/2024	8082A
P4709-03	HR-03-110424	Solid	PCB	Cool 4 deg C	PSEG05	L23	11/04/2024	8082A
P4718-01	WB-307-SB01	Solid	PCB	Cool 4 deg C	PORT06	L21	11/04/2024	8082A
P4718-02	WB-307-SB02	Solid	PCB	Cool 4 deg C	PORT06	L21	11/04/2024	8082A
P4719-01	BAYAVE-STOCKPILE	Solid	PCB	Cool 4 deg C	PSEG03	K21	11/05/2024	8082A

Date/Time 11/6/24 9:05
Raw Sample Received by: RT (Sig last)
Raw Sample Relinquished by: CP (Sig last)

Date/Time 11/6/24 9:30
Raw Sample Received by: CP (Sig last)
Raw Sample Relinquished by: RT (Sig last)

SOP ID: M3510C,3580A-Extraction PCB-14

Clean Up SOP #: Acid Cleanup

Extraction Start Date : 11/06/2024

Matrix : Water

Extraction Start Time : 08:25

Weigh By: N/A

Extraction By: RJ

Extraction End Date : 11/06/2024

Balance check: N/A

Filter By: RJ

Extraction End Time : 13:25

Balance ID: N/A

pH Meter ID: N/A

Concentration By: RS

pH Strip Lot#: E3574

Hood ID: 4,6,7

Supervisor By : rajesh

Extraction Method: ☒ Separatory Funnel

☐ Continous Liquid/Liquid

☐ Sonication

☐ Waste Dilution

☐ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Surrogate	1.0ML	200 PPB	PP23858
Spike Sol 1	1.0ML	5000 PPB	PP23640
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3823
Baked Na2SO4	N/A	EP2556
Hexane	N/A	E3823
H2SO4 1:1	N/A	EP2524
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40 BTS721. P4718-04 Limited volume recd.

KD Bath ID: WATER BATH-1,2

Envap ID: NEVAP-02

KD Bath Temperature: 60 °C

Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
11/6/24	RP (Est 246)	AJ EST PCA Leeb
13:30	Preparation Group	Analysis Group

Analytical Method: M3510C,3580A-Extraction PCB-14

Concentration Date: 11/06/2024

Sample ID	Client Sample ID	Test	g / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB164704BL	ABLK704	PCB	1000	6	RUPESH	rajesh	10			SEP-01
PB164704BS	ALCS704	PCB	1000	6	RUPESH	rajesh	10			2
PB164704BSD	ALCSD704	PCB	1000	6	RUPESH	rajesh	10			3
P4661-03	102324-A	PCB	970	6	RUPESH	rajesh	10	C		4
P4684-03	MECHANIC-ST-OIL-WATER	PCB	990	6	RUPESH	rajesh	10	D		5
P4702-01	TOTE-1	PCB	980	6	RUPESH	rajesh	10	E		6
P4704-01	NWB-2111	PCB	1000	6	RUPESH	rajesh	10	D		7
P4704-02	NWB-2056	PCB	1000	6	RUPESH	rajesh	10	D		8
P4704-03	NWB-2108	PCB	1000	6	RUPESH	rajesh	10	D		9
P4718-04	WB-307-SW	PCB	450	6	RUPESH	rajesh	5	F		10

* Extracts relinquished on the same date as received.



10/27/24 8:23

WORKLIST(Hardcopy Internal Chain)

WorkList Name : P4661P WorkList ID : 185157 Department : Extraction Date : 11-06-2024 08:21:08

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P4661-03	102324-A	Water	PCB	Cool 4 deg C	PSEG03	K51	10/31/2024	8082A
P4684-03	MECHANIC-ST-OIL-WATER	Water	PCB	Cool 4 deg C	PSEG03	L13	11/01/2024	8082A
P4702-01	TOTE-1	Water	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4704-01	NWB-2111	Water	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4704-02	NWB-2056	Water	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4704-03	NWB-2108	Water	PCB	Cool 4 deg C	PSEG03	L23	11/04/2024	8082A
P4718-04	WB-307-SW	Water	PCB	Cool 4 deg C	PORT06	L21	11/04/2024	8082A

Date/Time 11/6/24 8:23
Raw Sample Received by: RJ (Est Lab)
Raw Sample Relinquished by: JD (CSM)

Date/Time 11/6/24 9:00
Raw Sample Received by: JD (CSM)
Raw Sample Relinquished by: RJ (Est Lab)

Prep Standard - Chemical Standard Summary

Order ID : P4718

Test : PCB

Prepbatch ID : PB164700,PB164704,

Sequence ID/Qc Batch ID: PO110624,

Standard ID :

EP2524,EP2539,EP2548,EP2556,PP23640,PP23733,PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775,PP23776,PP23777,PP23778,PP23779,PP23780,PP23781,PP23782,PP23783,PP23784,PP23785,PP23786,PP23787,PP23788,PP23789,PP23790,PP23858,

Chemical ID :

E2865,E3551,E3788,E3792,E3793,E3804,E3805,E3815,E3823,E3825,M5037,M5178,P10483,P10500,P11507,P11512,P11581,P11587,P11590,P11597,P12698,P12929,P12934,P12946,P12947,P12957,P13033,P13350,P13351,P13372,W3112,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2524	08/14/2024	12/15/2024	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 08/14/2024

FROM 1000.00000ml of M5037 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2539	09/17/2024	03/11/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 09/17/2024

FROM 4000.00000ml of E3792 + 4000.00000ml of E3793 = Final Quantity: 8000.000 ml

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2548	10/16/2024	04/16/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 10/16/2024

FROM 1000.00000ml of W3112 + 4000.00000ml of M5178 = Final Quantity: 2000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2556	11/03/2024	01/03/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 11/03/2024

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP23640	09/09/2024	01/12/2025	Ankita Jodhani	None	None	Yogesh Patel
								09/10/2024

FROM 0.50000ml of P12946 + 99.50000ml of E3788 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP23733	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13350 + 9.00000ml of E3805 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP23735	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10483 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP23736	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP23737	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23735 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP23738	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP23739	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23737 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP23740	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11581 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP23741	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP23742	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23740 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP23743	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP23744	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23742 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP23745	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11587 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP23747	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP23748	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23745 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP23749	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP23750	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23748 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP23751	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12929 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP23752	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP23753	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23751 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP23754	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP23755	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23753 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP23756	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12934 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP23757	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP23758	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23756 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP23759	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP23760	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23758 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP23761	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11590 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP23762	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP23763	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23761 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP23764	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP23765	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23763 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP23766	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10500 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP23767	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP23768	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23766 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP23769	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP23770	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23768 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP23771	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11597 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP23772	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP23773	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23771 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP23774	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP23775	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23773 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP23776	10/03/2024	04/01/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 1.00000ml of P12947 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP23777	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 98.50000ml of E3805 + 0.50000ml of PP23733 + 1.00000ml of PP23776 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP23778	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23777 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP23779	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13372 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3790	AR1221 500 PPB ICV(AGILENT)	PP23780	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23779 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP23781	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12698 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP23782	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P11507 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP23783	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23781 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP23784	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23782 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP23785	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11512 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP23786	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23785 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP23787	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12957 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP23788	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23787 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP23789	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P13033 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP23790	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23789 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP23858	10/14/2024	04/04/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/14/2024

FROM 1.00000ml of P13351 + 999.00000ml of E3815 = Final Quantity: 1000.000 ml

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	01/03/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	23H1462005	04/23/2025	08/13/2024 / Rajesh	08/13/2024 / Rajesh	E3788

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/11/2025	09/12/2024 / Rajesh	09/11/2024 / Rajesh	E3792

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	03/11/2025	09/12/2024 / Rajesh	09/11/2024 / Rajesh	E3793

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/30/2025	09/30/2024 / Rajesh	09/25/2024 / Rajesh	E3805

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	04/04/2025	10/04/2024 / Rajesh	10/04/2024 / Rajesh	E3815

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24I2662006	05/03/2025	11/03/2024 / Rajesh	10/24/2024 / Rajesh	E3823

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	11/06/2025	11/06/2024 / Rajesh	11/01/2024 / Rajesh	E3825

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000250349	12/15/2024	01/06/2022 / mohan	09/18/2021 / mohan	M5037

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	03/29/2026	05/25/2022 / william	04/05/2022 / william	M5178

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0163157	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Abdul	P10483

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0167722	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Ankita	P10500

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11507

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006626997	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11512

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0175456	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11581

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0173309	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11587

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0175403	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11590

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0181782	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11597

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	04/03/2025	10/03/2024 / Ankita	08/07/2023 / Ankita	P12698

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12929

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12934

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	01/12/2025	07/12/2024 / Abdul	12/20/2023 / Yogesh	P12946

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12947

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	90165 / Aroclor 1262	112322	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P13033

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/03/2025	10/03/2024 / Ankita	04/22/2024 / Abdul	P13350

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/14/2025	10/14/2024 / Abdul	04/22/2024 / Abdul	P13351

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	04/03/2025	10/03/2024 / Ankita	05/02/2024 / Ankita	P13372

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1


Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865

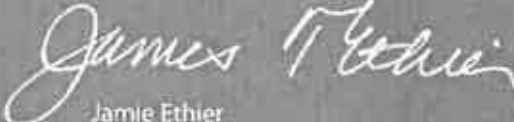
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03
Batch No.: 23H1462005
Manufactured Date: 2023-07-26
Expiration Date: 2026-07-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 8/13/24

E 3788

Ken Koehnlein
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 09/11/24

E 3192

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
CMOS

avantor™



Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

>>> Continued on page 2 >>>

Recd. by RP on 9/11/24

E3793

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use
Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC

Michelle Bales
Sr. Manager, Quality Assurance

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 9/25/24

E 3805

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 24H1462005
Manufactured Date: 2024-05-24
Expiration Date: 2027-05-24
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3815

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)

 **avantorsTM**



Material No.: 9266-A4

Batch No.: 24I2662006

Manufactured Date: 2024-08-29

Expiration Date: 2025-11-28

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	3
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	99.9%
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3823



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

£3825

Jamie Croak
Director Quality Operations, Bioscience Production

Sulfuric Acid

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

Low Selenium

avantorsm



Material No.: 9673-33

Batch No.: 0000250349

Manufactured Date: 2019/12/17

Retest Date: 2024/12/15

Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS - Assay (H ₂ SO ₄)	95.0 - 98.0 %	96.5
Appearance	Passes Test	PT
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	1
ACS - Substances Reducing Permanganate (as SO ₂)	<= 2 ppm	< 2
Ammonium (NH ₄)	<= 1 ppm	< 1
Chloride (Cl)	<= 0.1 ppm	< 0.1
Nitrate (NO ₃)	<= 0.2 ppm	< 0.1
Phosphate (PO ₄)	<= 0.5 ppm	< 0.1
Trace Impurities - Aluminum (Al)	<= 30.0 ppb	0.2
Arsenic and Antimony (as As)	<= 4 ppb	< 2
Trace Impurities - Barium (Ba)	<= 10.0 ppb	< 1.0
Trace Impurities - Beryllium (Be)	<= 10.0 ppb	< 1.0
Trace Impurities - Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities - Boron (B)	<= 10.0 ppb	< 5.0
Trace Impurities - Cadmium (Cd)	<= 2.0 ppb	< 0.3
Trace Impurities - Calcium (Ca)	<= 50.0 ppb	2.9
Trace Impurities - Chromium (Cr)	<= 6.0 ppb	< 0.4
Trace Impurities - Cobalt (Co)	<= 0.5 ppb	< 0.3
Trace Impurities - Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities - Gallium (Ga)	<= 10.0 ppb	< 1.0
Trace Impurities - Germanium (Ge)	<= 10.0 ppb	< 10.0
Trace Impurities - Gold (Au)	<= 10.0 ppb	< 0.2
Heavy Metals (as Pb)	<= 500 ppb	< 100

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC


100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Material No.: 9673-33
Batch No.: 0000250349

Test	Specification	Result
Trace Impurities - Iron (Fe)	<= 50.0 ppb	4.1
Trace Impurities - Lead (Pb)	<= 0.5 ppb	< 0.5
Trace Impurities - Lithium (Li)	<= 10.0 ppb	< 1.0
Trace Impurities - Magnesium (Mg)	<= 7.0 ppb	0.4
Trace Impurities - Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities - Mercury (Hg)	<= 0.5 ppb	< 0.1
Trace Impurities - Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities - Nickel (Ni)	<= 2.0 ppb	< 0.3
Trace Impurities - Niobium (Nb)	<= 10.0 ppb	< 1.0
Trace Impurities - Potassium (K)	<= 500.0 ppb	< 2.0
Trace Impurities - Selenium (Se)	<= 50.0 ppb	22.9
Trace Impurities - Silicon (Si)	<= 100.0 ppb	< 10.0
Trace Impurities - Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities - Sodium (Na)	<= 500.0 ppb	2.7
Trace Impurities - Strontium (Sr)	<= 5.0 ppb	< 0.2
Trace Impurities - Tantalum (Ta)	<= 10.0 ppb	< 5.0
Trace Impurities - Thallium (Tl)	<= 20.0 ppb	< 5.0
Trace Impurities - Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities - Titanium (Ti)	<= 10.0 ppb	< 1.0
Trace Impurities - Vanadium (V)	<= 10.0 ppb	< 1.0
Trace Impurities - Zinc (Zn)	<= 5.0 ppb	0.3
Trace Impurities - Zirconium (Zr)	<= 10.0 ppb	< 1.0

For Laboratory, Research or Manufacturing Use

Country of Origin: US
Packaging Site: Phillipsburg Mfg Ctr & DC

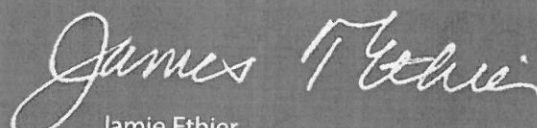
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Hydrochloric Acid, 36.5–38.0%
 BAKER INSTRA-ANALYZED® Reagent
 For Trace Metal Analysis



Material No.: 9530-33
 Batch No.: 0000281827
 Manufactured Date: 2021/03/30
 Retest Date: 2026/03/29
 Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
 Avantor Performance Materials, LLC
 100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 **Lot No.:** A0163157

Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2026 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1016 CAS # 12674-11-2 (Lot 04) Purity ----%	1,007.0 µg/mL	+/- 5.8683 µg/mL Gravimetric +/- 31.9082 µg/mL Unstressed +/- 41.6868 µg/mL Stressed
2	Aroclor 1260 CAS # 11096-82-5 (Lot 07) Purity ----%	1,008.0 µg/mL	+/- 5.8741 µg/mL Gravimetric +/- 31.9399 µg/mL Unstressed +/- 41.7282 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 10476

P 10480

AR
02/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

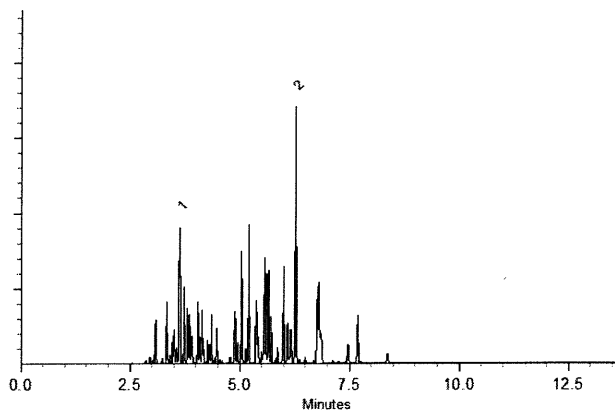

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 03-Aug-2020

Balance: B442140311

Justine Albertson - Operations Tech-ARM QC

Date Passed: 05-Aug-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32409 Lot No.: A0167722
Description : Aroclor® 1262 Standard
Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : April 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1262	1,004.0 µg/mL	+/- 5.9635 µg/mL Gravimetric
	CAS # 37324-23-5 (Lot 10849100)		+/- 31.8340 µg/mL Unstressed
	Purity ----%		+/- 41.5787 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P10496
↓
P10500

AJ
09/19/21

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

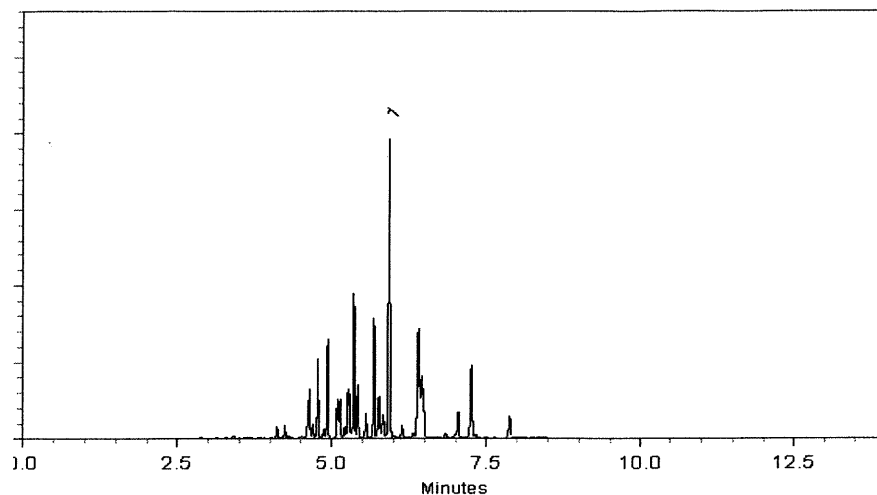

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 03-Jan-2021


Balance: B707717271

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 05-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
Aroclor 1242	100.4	± 0.5 µg/mL		053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11503
↓
P11507

AJ
02/21/22

Page: 1 of 2

CSD-QA-015.1

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2


www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1248 Standard

Lot Number: 0006626997

Product Number: PP-342-1

Lot Issue Date: 17-Aug-2021

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 30-Sep-2025

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1248	100.3	± 0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11508


↓

P11512

AJ

2/21/22

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 Lot No.: A0175456
Description : Aroclor® 1221 Standard
Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1221	1,002.0 µg/mL	+/- 5.9516 µg/mL Gravimetric
	CAS # 11104-28-2 (Lot 10210500)		+/- 31.7706 µg/mL Unstressed
	Purity ----%		+/- 41.4958 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11578
↓
P 11582 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

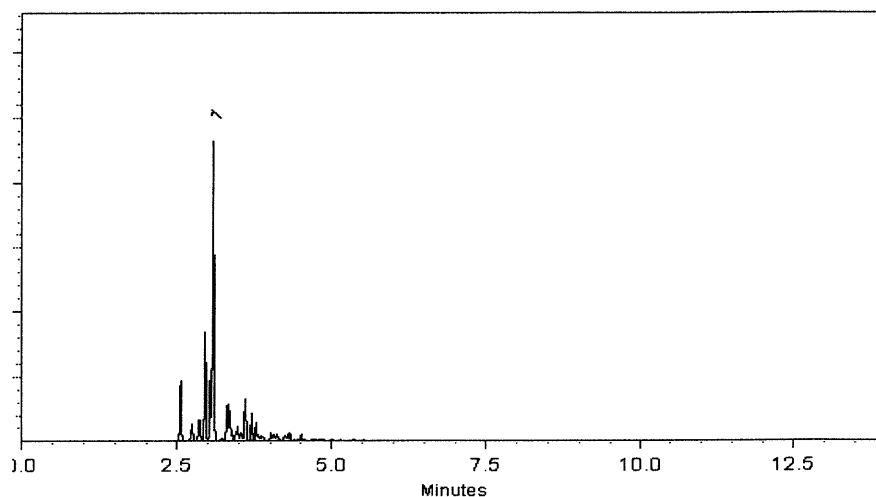

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 16-Aug-2021 Balance: B442140311

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 18-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11578
↓
P11582 / (S)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008 Lot No.: A0173309
Description : Aroclor® 1232 Standard
Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : September 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1232	1,001.0 µg/mL	+/- 5.9456 µg/mL Gravimetric
	CAS # 11141-16-5 (Lot 15665-01)		+/- 31.7389 µg/mL Unstressed
	Purity ----%		+/- 41.4544 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11583
↓
P11587 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

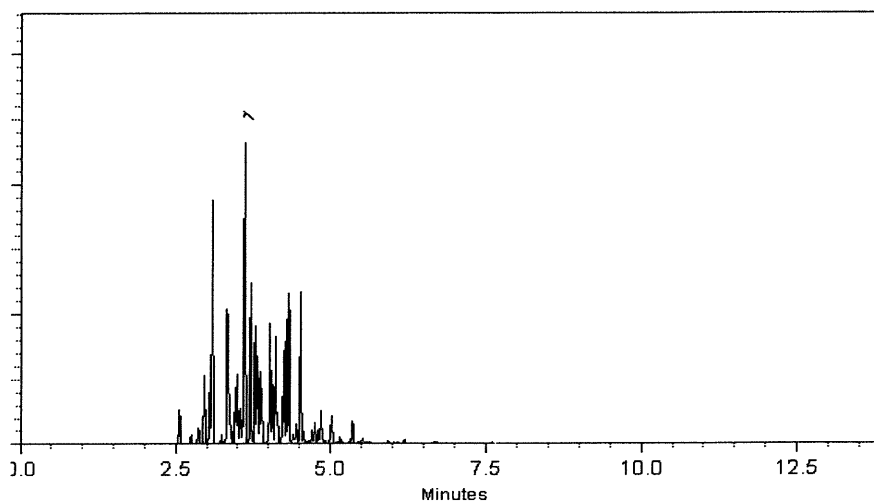

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 13-Jun-2021 **Balance:** B442140311

Alexis Shelow
Alexis Shelow - Operations Tech I

Date Passed: 16-Jun-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11583
↓
P11587 (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 Lot No.: A0175403
Description : Aroclor® 1254 Standard
Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1254 CAS # 11097-69-1 (Lot 124-191-B) Purity ----%	1,000.7 µg/mL	+/- 5.9437 µg/mL Gravimetric +/- 31.7284 µg/mL Unstressed +/- 41.4406 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11588
↓
P11592 / (S)

AR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

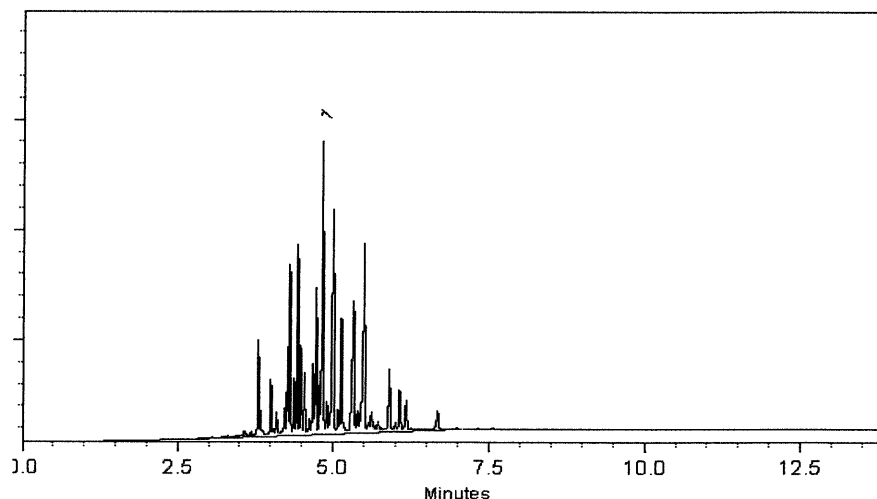

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cathleen Soltis

Cathleen Soltis - Mix Technician

Date Mixed: 15-Aug-2021

Balance: 1128360905

Alexis Shelow

Alexis Shelow - Operations Tech I

Date Passed: 17-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11588
↓
P11592 / (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410 Lot No.: A0181782
Description : Aroclor® 1268 Standard
Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : May 31, 2028 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1268 CAS # 11100-14-4 Purity ----%	1,001.4 µg/mL (Lot 10947000)	+/- 5.9480 µg/mL Gravimetric +/- 31.7516 µg/mL Unstressed +/- 41.4710 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11593
↓
P 11597
⑤

UAR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

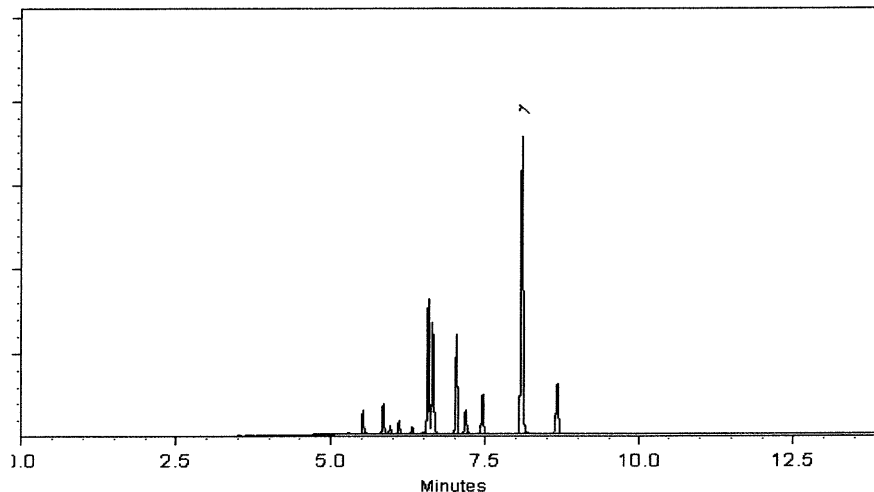

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope S. Riglin
Penelope Riglin - Operations Tech I

Date Mixed: 14-Feb-2022

Balance: 1128360905

Clara Windle
Clara Windle - Operations Technician I

Date Passed: 17-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 11593 / (5)
↓
P 11597
[Signature]
04/30/2022



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration ($\mu\text{g/mL}$): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3

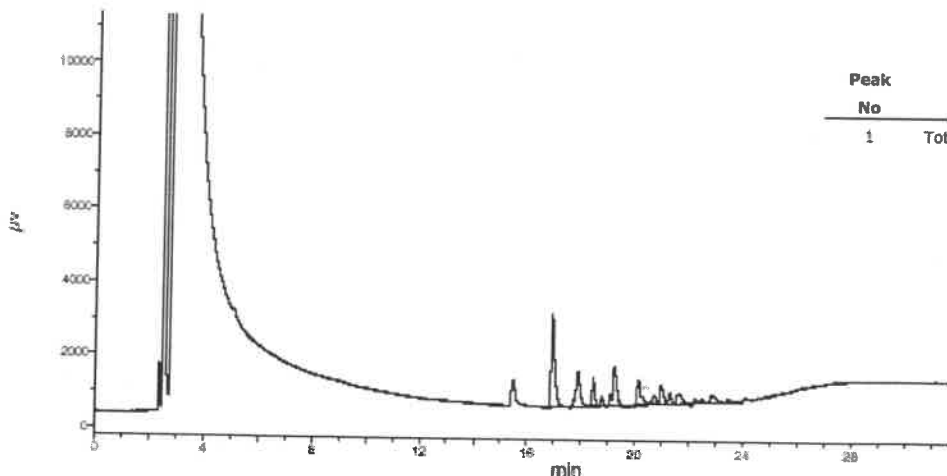




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32009 **Lot No.:** A0203672

Description: Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

p12928

→

p12932

AJ

12/27/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

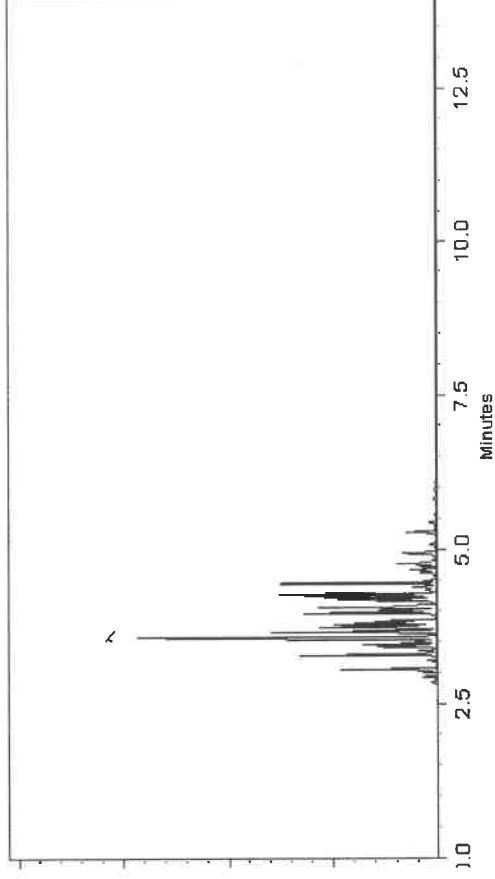

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boothamer

Russ Boothamer - Operations Technician I

Date Mixed: 26-Oct-2023

Balance Serial #

B442140311

Jennifer Polino

Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010 **Lot No.:** A0202803

Description: Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P1210967
P1210977
P1210973

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 µg/mL	+/- 55.5850

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

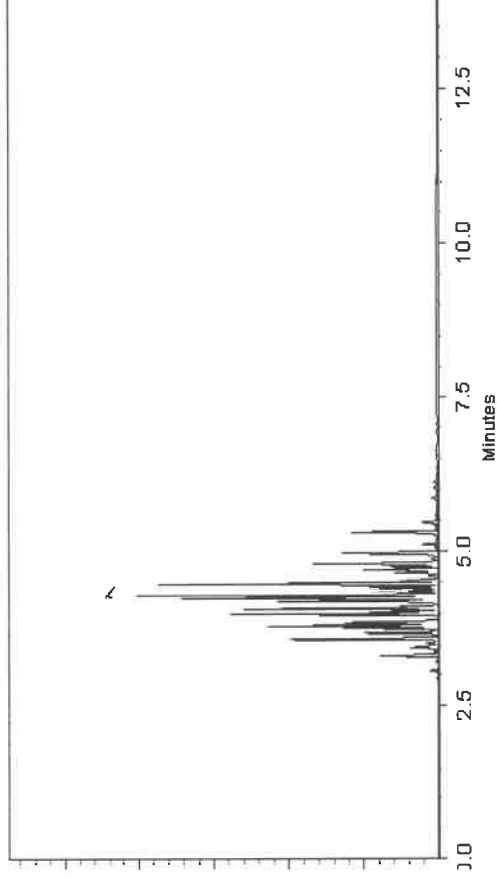

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 03-Oct-2023

Balance Serial # 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty


Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

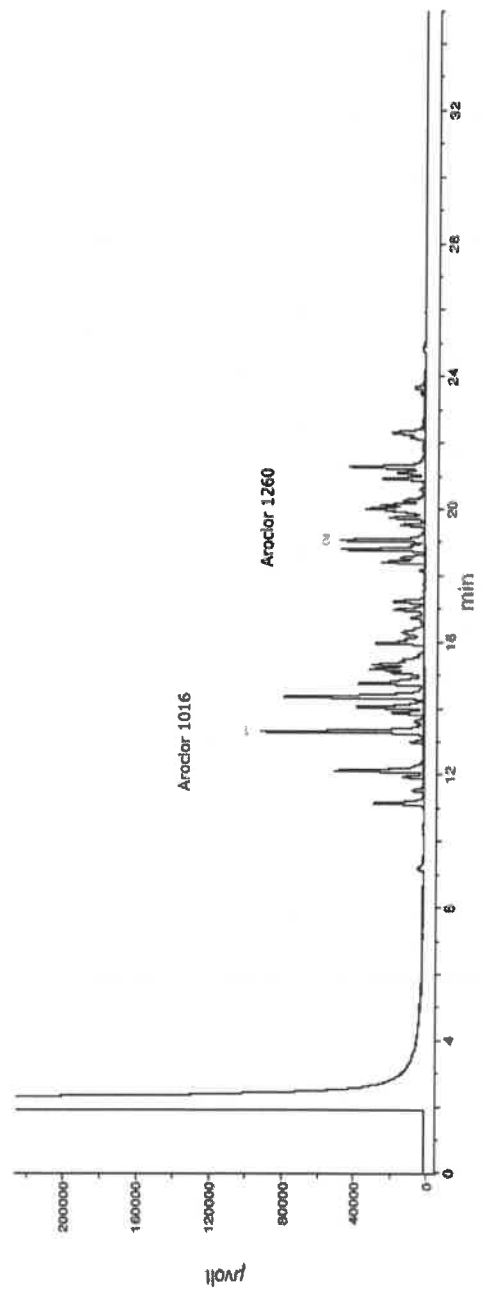



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

Weight(s) shown below were combined and diluted to (mL.):
200.0

Balance Uncertainty
0.010

Flask Uncertainty
0.010

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

Weight(s) shown below were combined and diluted to (mL.):
200.0


Balance Uncertainty
0.010

Flask Uncertainty
0.010

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty (%)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11096-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

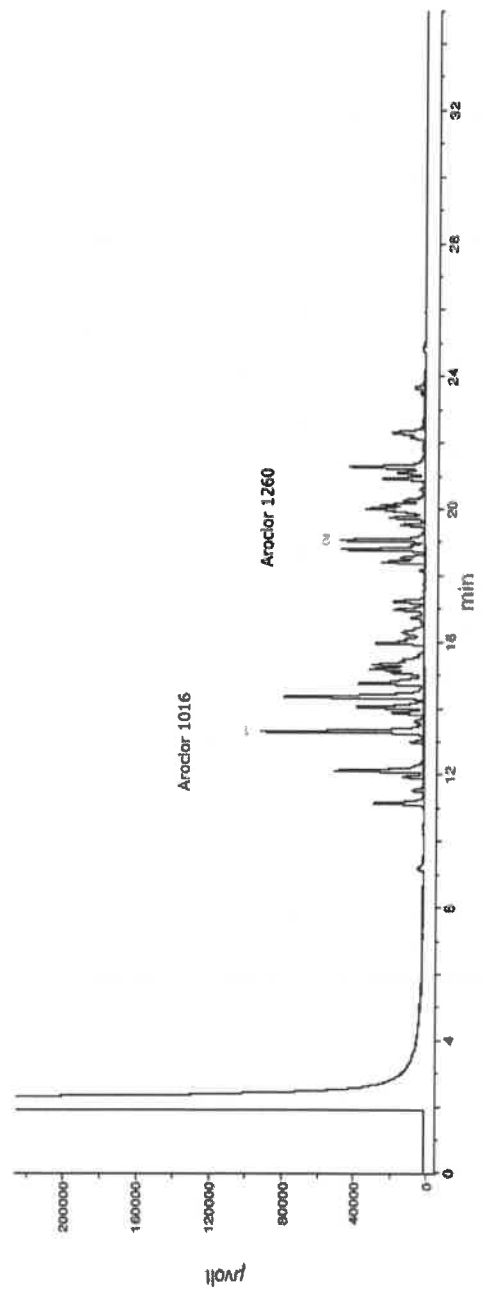



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

Solvent(s): Iso-octane
Lot#: 82227

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE

P12956 / Y.P.
L
P12957 / 12/18/23


Note: Aroclor 1254 is a mix of isomers.

Compound		Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Initial Uncertainty	Pipette (mL)	Conc.(µg/mL)	Initial Conc.(µg/mL)	Final Conc.(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1254		79100	121823	0.10	2.00	0.017	0.017	1003.3	100.1	11097-69-1	1.8	0.5mg/m3 (skin)	or-rat 1295mg/kg	

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 250 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

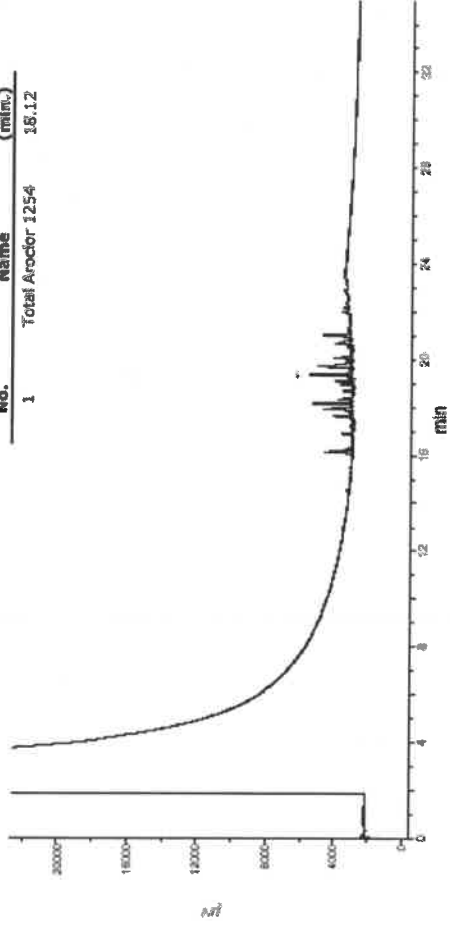



CERTIFIED WEIGHT REPORT

Part Number: 90165
Lot Number: 112322
Description: Atrocior 1262
Expiration Date: 112332
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6LUTB
Weight(s) shown were combined and diluted to (mL): 50.0

Solvent(s): Lot#
Hexane 273615

SE-05 Balance Uncertainty
0.005 Flask Uncertainty


Formulated By:	Prashant Chauhan	112322	DATE
Reviewed By:	Pedro L. Rentes	112322	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	--------------------	-------------------	-------------------	---------------------	----------------------------------	------	----------------	------

1. Atrocior 1262 444 W-130-05 1000 100 0.2 0.05003 0.05016 1002.7 4.5 37324-23-5 N/A or-tal 11300mg/kg

Method GC/MSD-7.M: Column:(30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (0min.), Temp 2 = 290°C (12.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C.

TIC: [BSB1]P70444-2.D

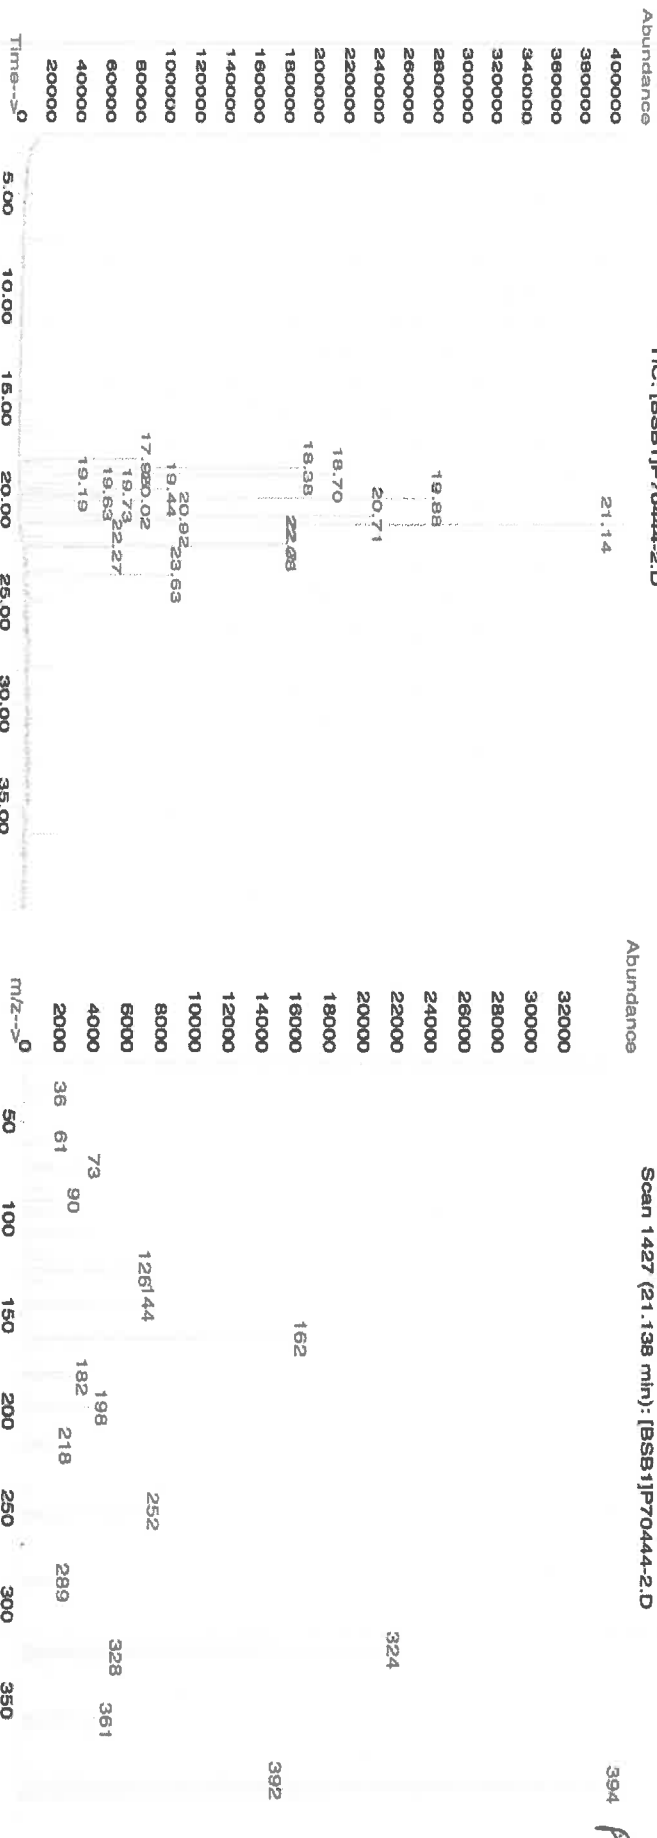




Run 20, "P90165 L112322 [1000µg/mL in hexane]"

Run Length: 35.00 min, 21000 points at 10 points/second.
Created: Thu, Dec 8, 2022 at 2:31:02 AM.
Sampled: Sequence "120722-GC3M1", Method "GC3-M1".
Analyzed using Method "GC3-M1".

Comments

GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3

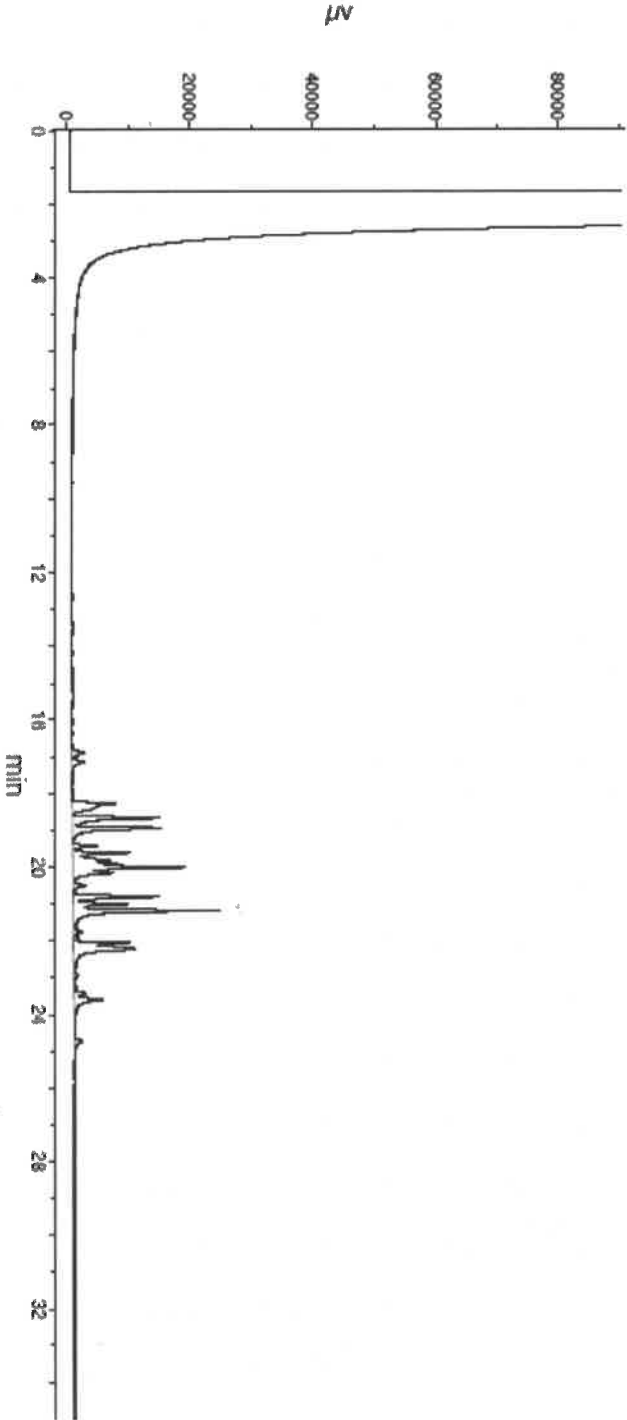



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

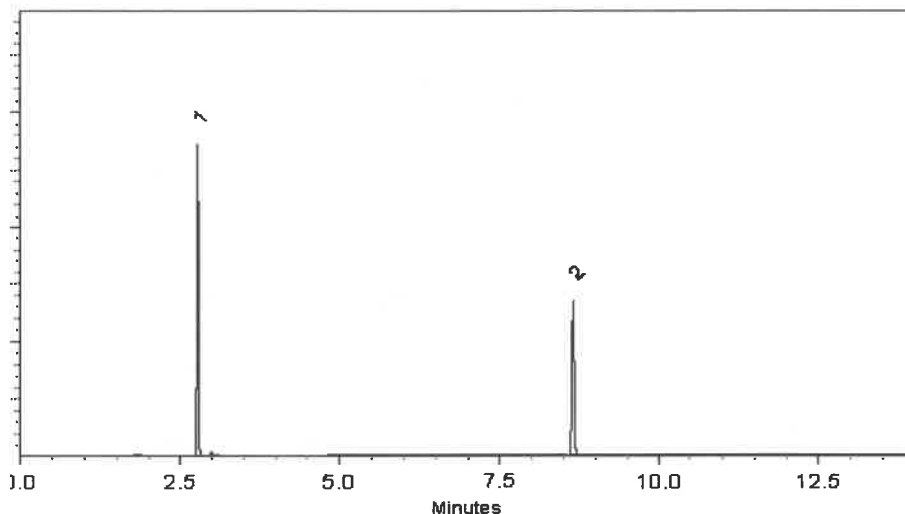


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

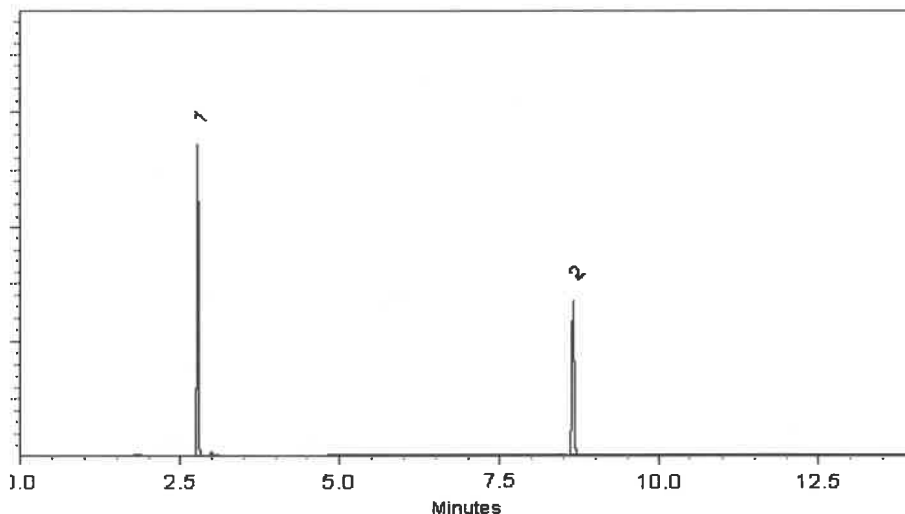


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name: Aroclor 1221 Standard
Product Number: PP-292-1
Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006783205
Lot Issue Date: 20-Feb-2024
Expiration Date: 31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ±	0.5 µg/mL	011104-28-2	NT01017

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342
AJ
05106124
P13343

Page: 1 of 2

CSD-QA-015.2

ISO 17025
Cert No. AT-1937


250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



SHIPPING DOCUMENTS

CHEMTECH

CHAIN OF CUSTODY RECORD

284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 • Fax (908) 789-8922
www.chemtech.net

CHEMTECH PROJECT NO. **P4718**
QUOTE NO.
COC Number **2042034**

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: Glannett Fleming
ADDRESS: 1010 Adams Avenue
CITY: Audobon STATE: PA ZIP: 19403
ATTENTION: Joe Krupansky
PHONE: 610-801-8362 FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Amtrak's sep. of SB
PROJECT NO.: 9500000218 LOCATION: Keating NJ
PROJECT MANAGER: Joe Krupansky
e-mail: QAQC@bamays.com
PHONE: 610-801-8362 FAX:

CLIENT BILLING INFORMATION

BILL TO: Chemtech PO#:
ADDRESS: 984 Sheffield St.
CITY: Mountainside STATE: NJ ZIP: 07092
ATTENTION: Samuel PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) _____ DAYS*
HARDCOPY (DATA PACKAGE): 10 DAYS*
EDD: 10 DAYS*
*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☒ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other _____
☐ EDD FORMAT BEN EDD.

1. TA VOC+10
2. TA PAH
3. TAH NPAHs
4. PCB's
5. CAHs, G/L/V
6. EPH
7. TOX
8. EDDA TCA P
9. RCRA Parameters

PRESERVATIVES

COMMENTS

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS	
			COMP	GRAB	DATE	TIME		A		B		F						
1.	<u>WB-307-SW</u>	<u>GW</u>		<u>X</u>	<u>11/04</u>	<u>8:20</u>	<u>7</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>					
2.	<u>WB-307-SB01</u>	<u>S</u>	<u>X</u>		<u>11/04</u>	<u>9:45</u>	<u>10</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>					
3.	<u>WB-307-SB02</u>	<u>S</u>	<u>X</u>		<u>11/04</u>	<u>10:45</u>	<u>10</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>	<u>X</u>		
4.	<u>TB-11042024</u>																	
5.																		
6.																		
7.																		
8.																		
9.																		
10.																		

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	Conditions of bottles or coolers at receipt:	☐ COMPLIANT ☐ NON COMPLIANT ☒ COOLER TEMP	<u>4.0</u> °C
1. <u>Yanda</u>	<u>11/6/24 11:19</u>	1. <u>[Signature]</u>	Comments:	<u>No Ice.</u>	
RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:			
2. <u>[Signature]</u>		2. <u>[Signature]</u>			
RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:			
3. <u>[Signature]</u>	<u>11-3-2024</u>	3. <u>[Signature]</u>			

Page ____ of ____

CLIENT: ☐ Hand Delivered ☐ Other _____
CHEMTECH: ☐ Picked Up ☐ Field Sampling

Shipment Complete
☐ YES ☐ NO



284 Sheffield Street, Mountainside NJ 07092 (908)-789-8900 Fax : 908 789 8922

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

LOGIN REPORT/SAMPLE TRANSFER

Order ID : P4718	PORT06	Order Date : 11/5/2024 1:31:00 PM	Project Mgr :
Client Name : Portal Partners Tri-Venture		Project Name : Amtrak Sawtooth Bridges 2	Report Type : NJ Reduced
Client Contact : Joseph Krupansky		Receive DateTime : 11/5/2024 12:15:00 PM	EDD Type : EXCEL NJCLEANUP
Invoice Name : Portal Partners Tri-Venture		Purchase Order :	Hard Copy Date :
Invoice Contact : Joseph Krupansky			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
P4718-01	WB-307-SB01	Solid	11/04/2024	09:45					
					VOC-TCLVOA-10		8260D	10 Bus. Days	
P4718-02	WB-307-SB02	Solid	11/04/2024	09:45					
					VOC-TCLVOA-10		8260D	10 Bus. Days	
P4718-04	WB-307-SW	Water	11/04/2024	08:20					
					VOC-TCLVOA-10		8260-Low	10 Bus. Days	
P4718-05	TB-11042024	Water	11/04/2024	00:00					
					VOC-TCLVOA-10		8260-Low	10 Bus. Days	

Relinquished By :

Date / Time :

LCJ
11.5.2024 14:27

Received By :

Date / Time :

[Signature]
11.5.2024 14:27

Storage Area : VOA Refridgerator Room