


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111324\  
Data File : BF140331.D  
Acq On : 13 Nov 2024 08:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF111324.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Nov 13 14:40:06 2024

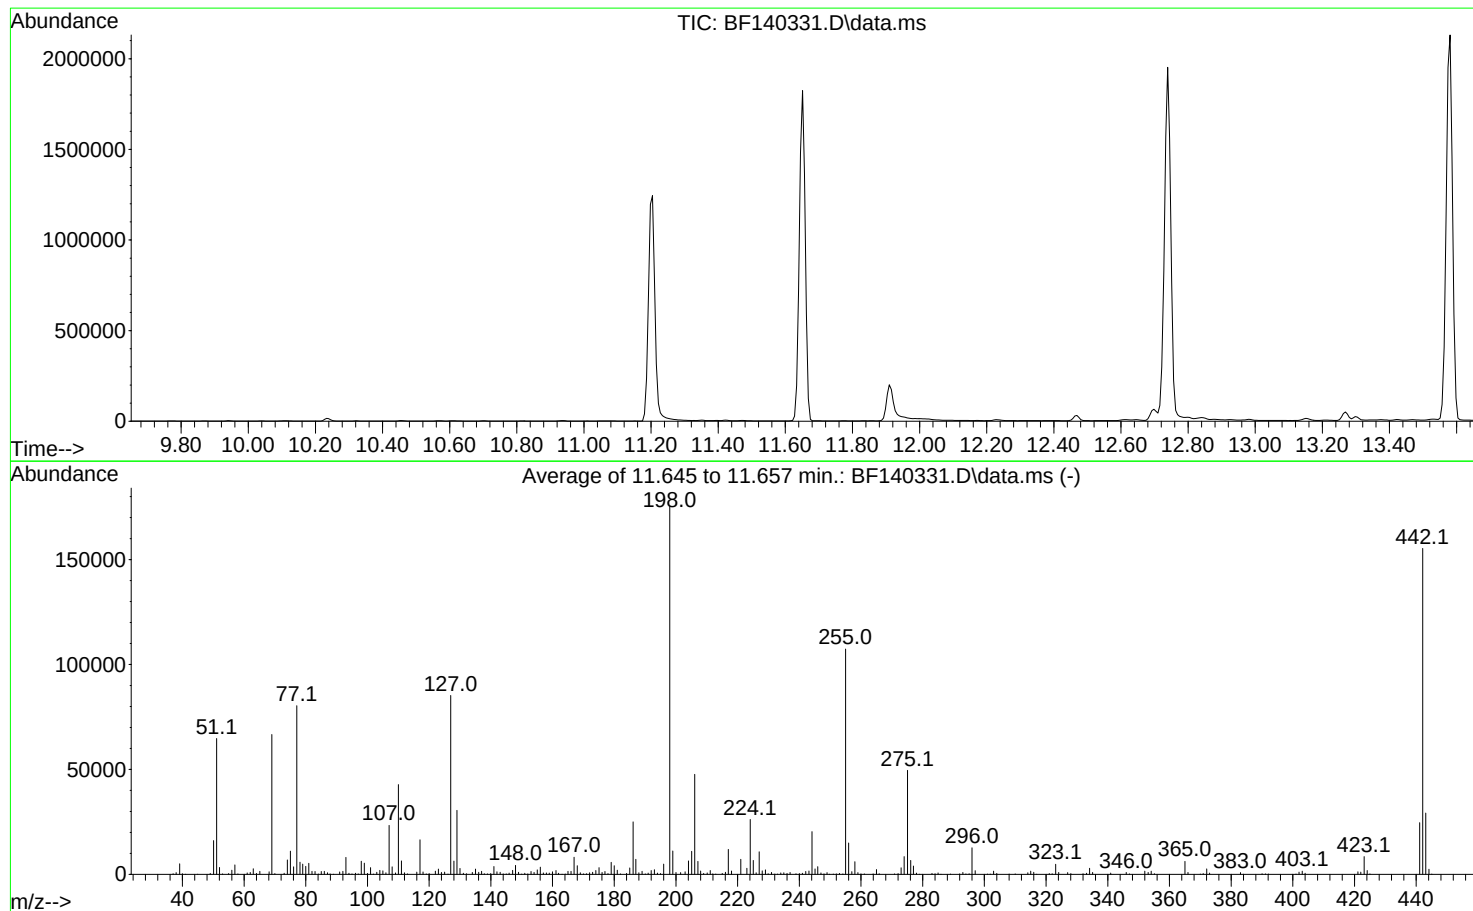




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.9         | 64757      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1226       | PASS                |
| 69             | 198             | 0.00            | 100             | 38.0         | 66677      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 372        | PASS                |
| 127            | 198             | 10              | 80              | 48.6         | 85245      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 175296     | PASS                |
| 199            | 198             | 5               | 9               | 6.4          | 11148      | PASS                |
| 275            | 198             | 10              | 60              | 28.3         | 49536      | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 6203       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.0         | 24595      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 155288     | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 29203      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111324\  
Data File : BF140331.D  
Acq On : 13 Nov 2024 08:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 13 14:44:41 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF111324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 13 14:40:06 2024  
Response via : Initial Calibration

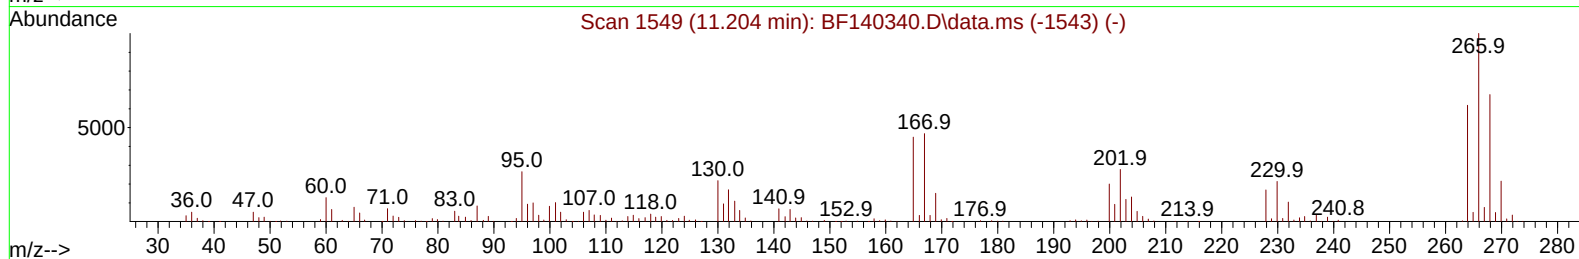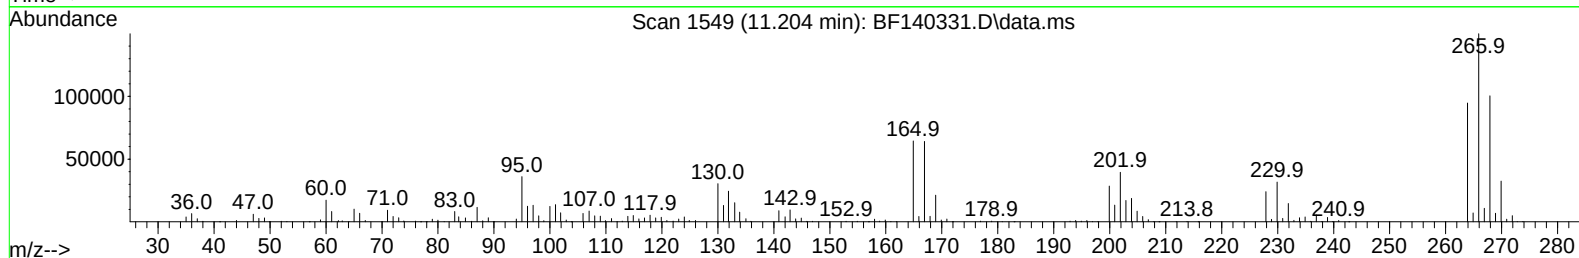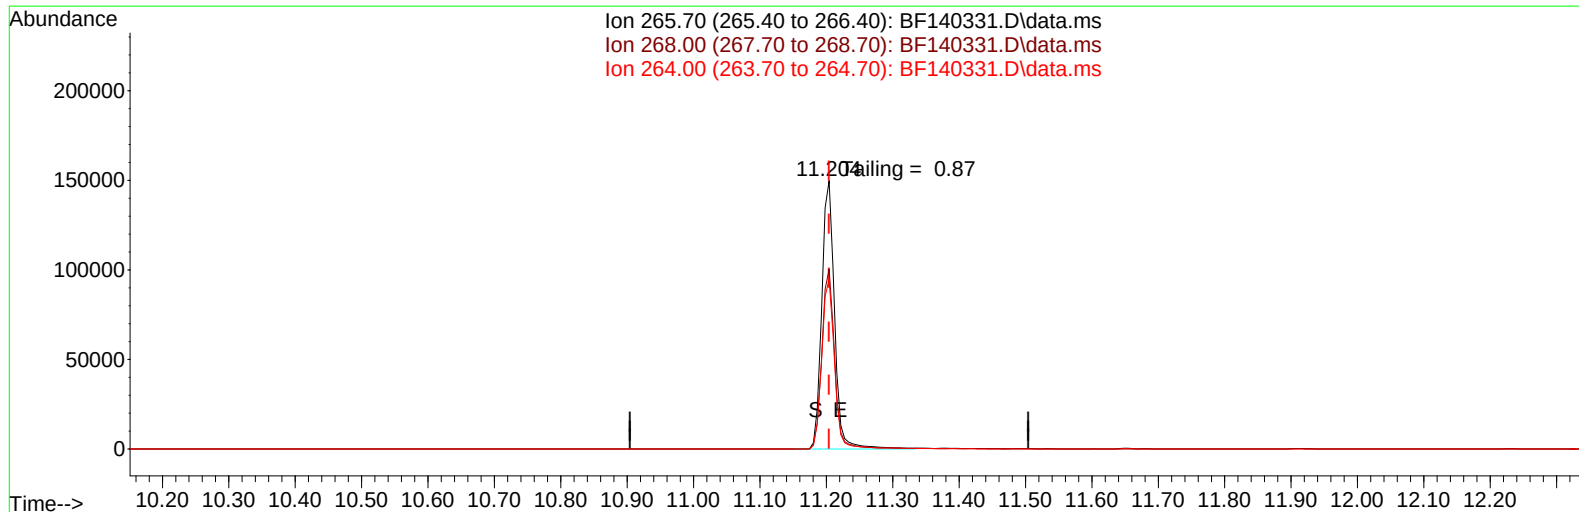

TIC: BF140331.D\data.ms

**(70) Pentachlorophenol (C)**

11.204min ( 0.000) 23118.21 ng




response 201406

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.10  | 67.05  |
| 264.00 | 62.90  | 63.20  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111324\  
Data File : BF140331.D  
Acq On : 13 Nov 2024 08:35  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 13 14:44:41 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF111324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 13 14:40:06 2024  
Response via : Initial Calibration

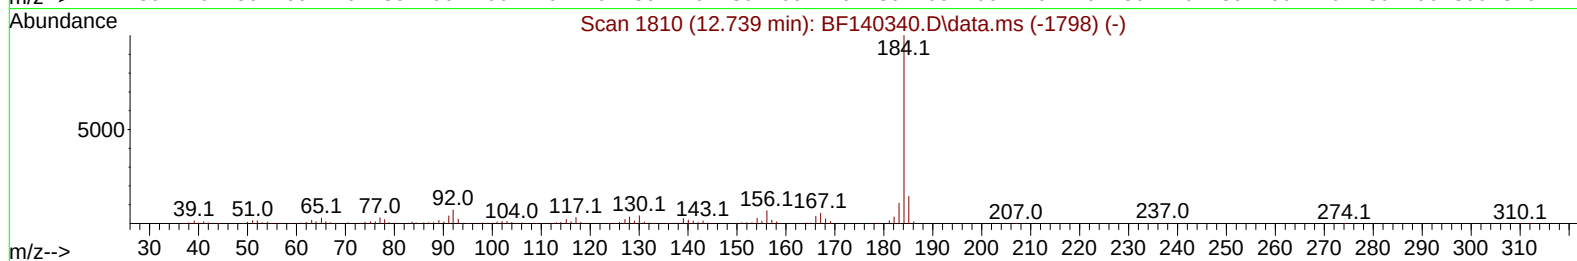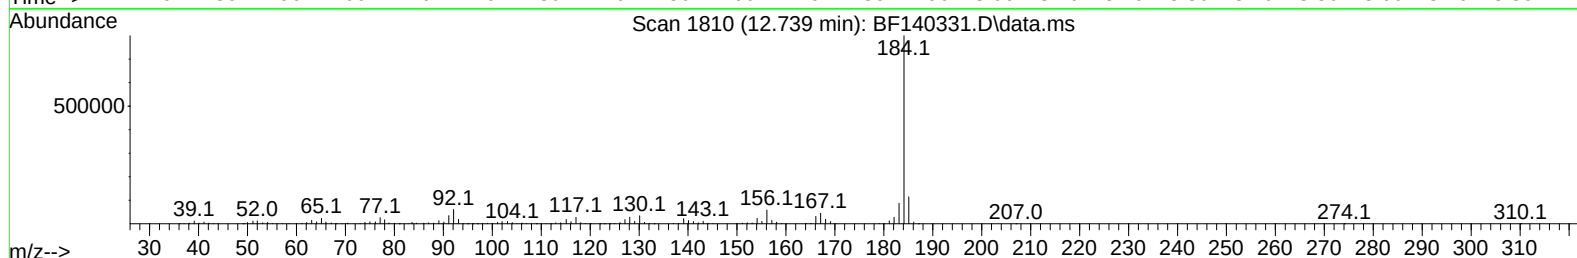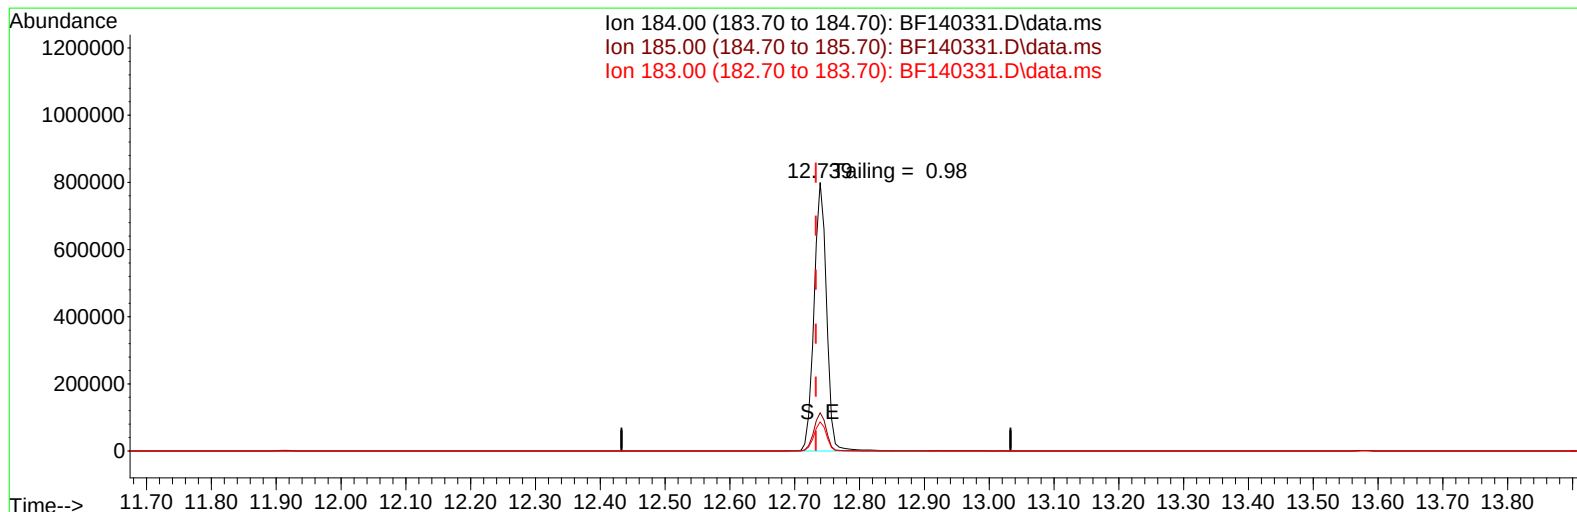

TIC: BF140331.D\data.ms

**(77) Benzidine**

**12.739min (+ 0.006) 47514.94 ng**

**response 1075955**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 14.29  |
| 183.00 | 10.80  | 10.88  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/13/2024    | BNA_F            | <u>BF140331.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 544964           | 13.58              |
| DDD           | 17817            | 13.269             |
| DDE           | 776              | 12.927             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 18593         | 563557           | 3.30               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP