


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140350.D
Acq On : 14 Nov 2024 08:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

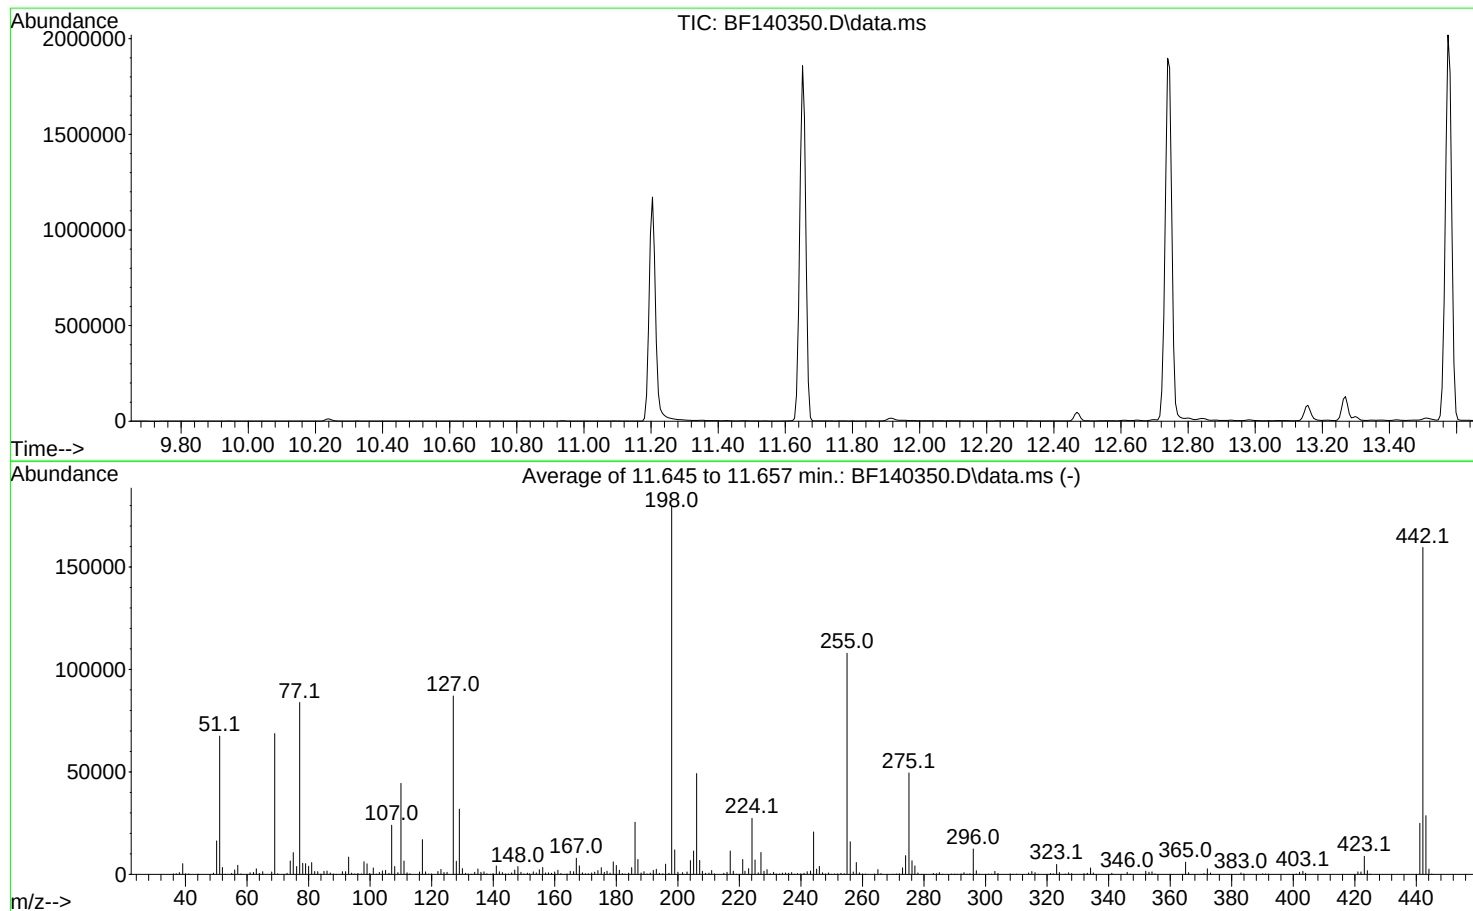




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	67499	PASS
68	69	0.00	2	1.7	1197	PASS
69	198	0.00	100	38.3	68728	PASS
70	69	0.00	2	0.4	296	PASS
127	198	10	80	48.5	87083	PASS
197	198	0.00	2	0.3	544	PASS
198	198	100	100	100.0	179520	PASS
199	198	5	9	6.6	11931	PASS
275	198	10	60	27.6	49539	PASS
365	198	1	100	3.3	5926	PASS
441	198	0.01	100	13.9	24939	PASS
442	442	50	100	100.0	159507	PASS
443	442	15	24	18.0	28645	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140350.D
Acq On : 14 Nov 2024 08:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 14 10:48:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

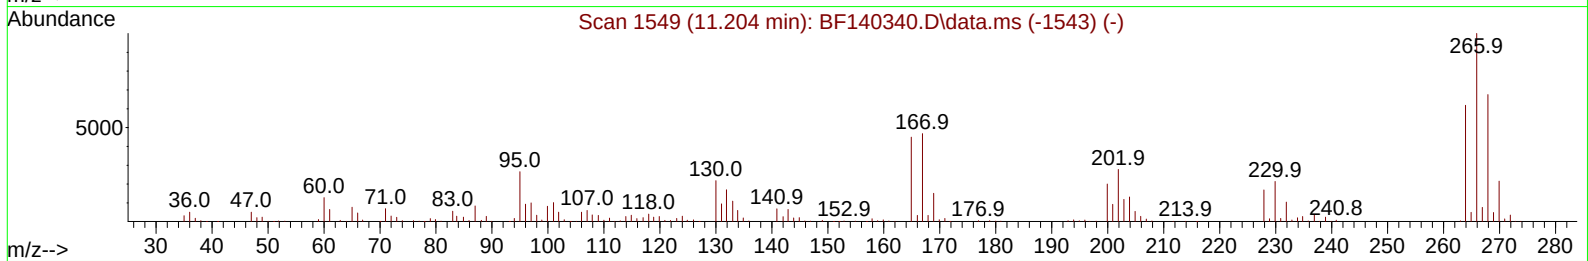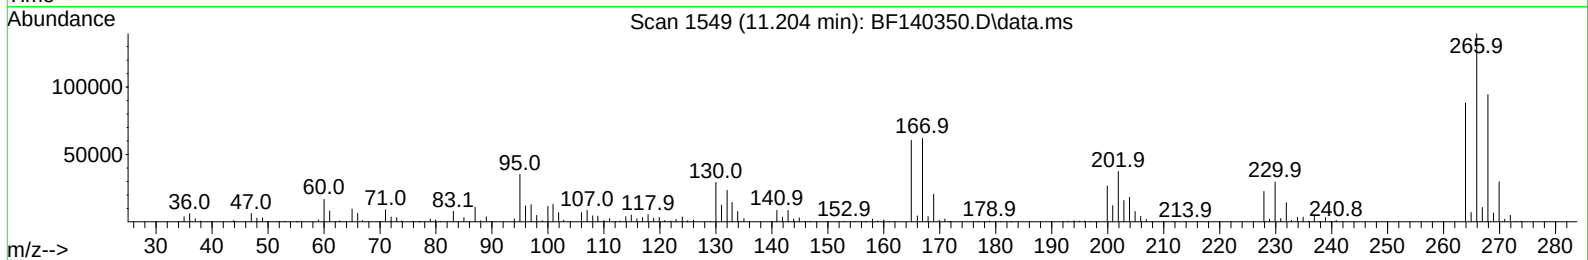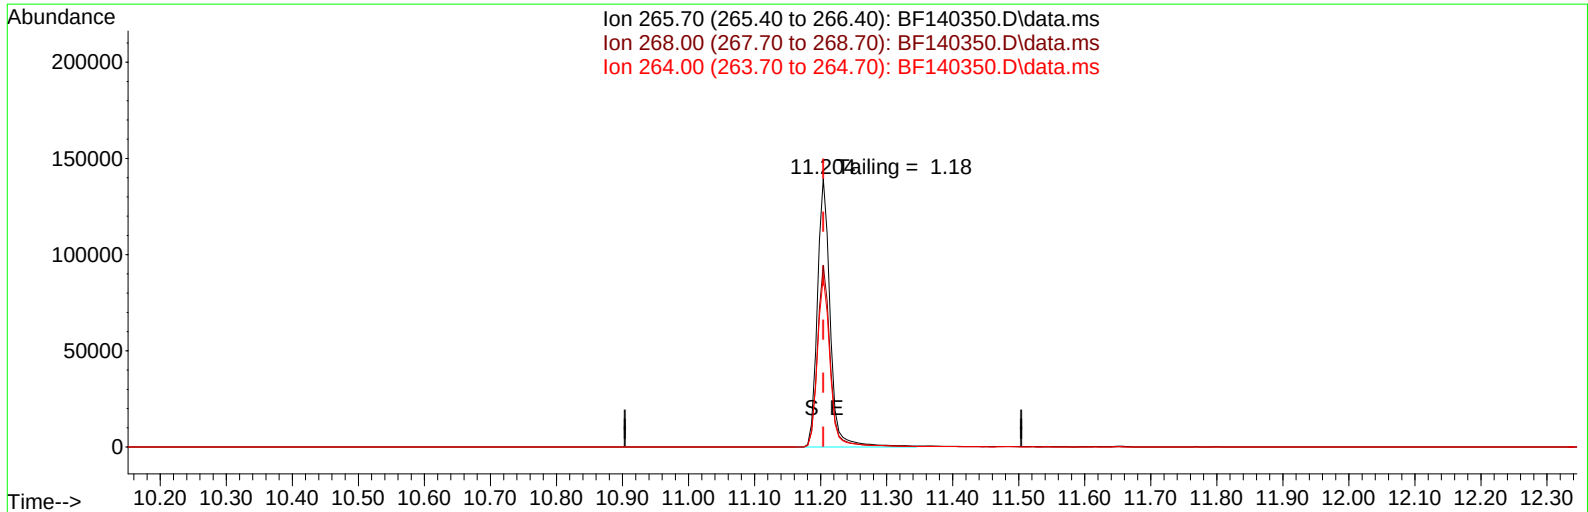

TIC: BF140350.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.000) 30509.82 ng




response 188723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.69
264.00	62.90	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140350.D
Acq On : 14 Nov 2024 08:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 14 10:48:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

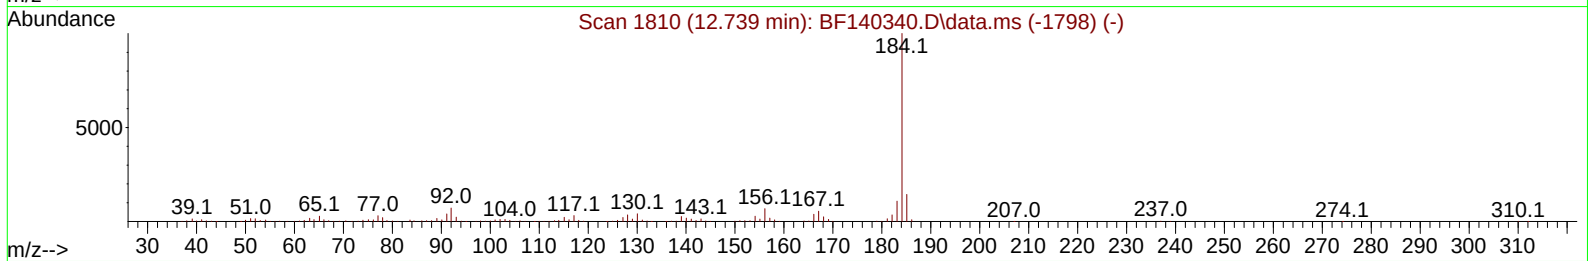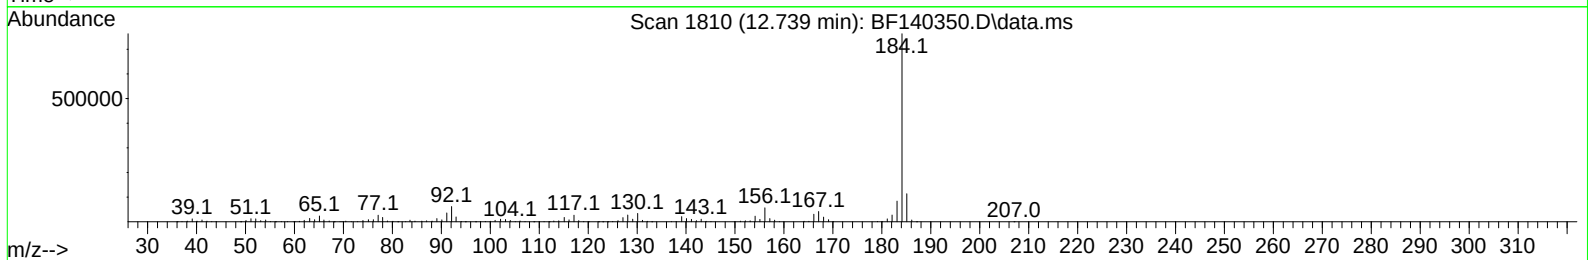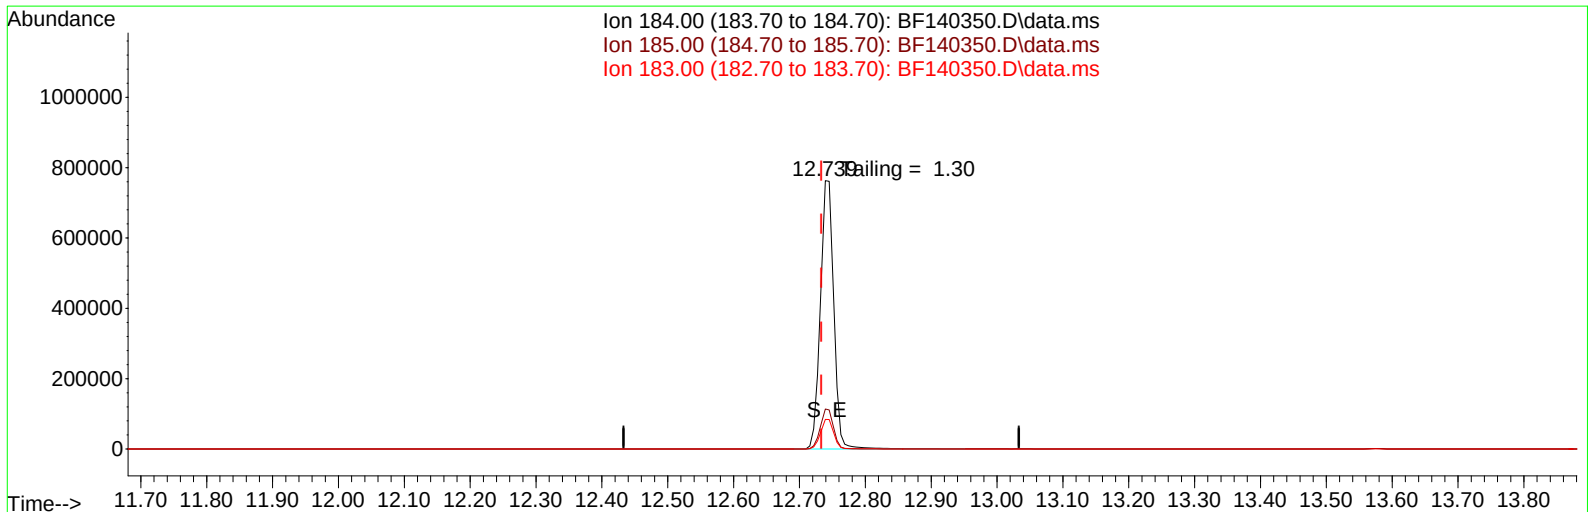

TIC: BF140350.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 49755.95 ng

response 1078960

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.90
183.00	10.80	11.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/14/2024	BNA_F	<u>BF140350.D</u>
Compound Name	Response	Retention Time
DDT	519001	13.574
DDD	38421	13.269
DDE	863	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39284	558285	7.04

Instrument :
BNA_F
ClientSampleId :
DFTPP