

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
Data File : FG014676.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2024 15:56
Operator : YP\AJ
Sample : P4721-06 10X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
EX-11-TPH-3

Integration File: autoint1.e
Quant Time: Nov 08 05:26:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
Quant Title :
QLast Update : Mon Oct 21 17:03:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.050	139952	1.170 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
Data File : FG014676.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2024 15:56
Operator : YP\AJ
Sample : P4721-06 10X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
EX-11-TPH-3

Integration File: autoint1.e
Quant Time: Nov 08 05:26:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
Quant Title :
QLast Update : Mon Oct 21 17:03:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

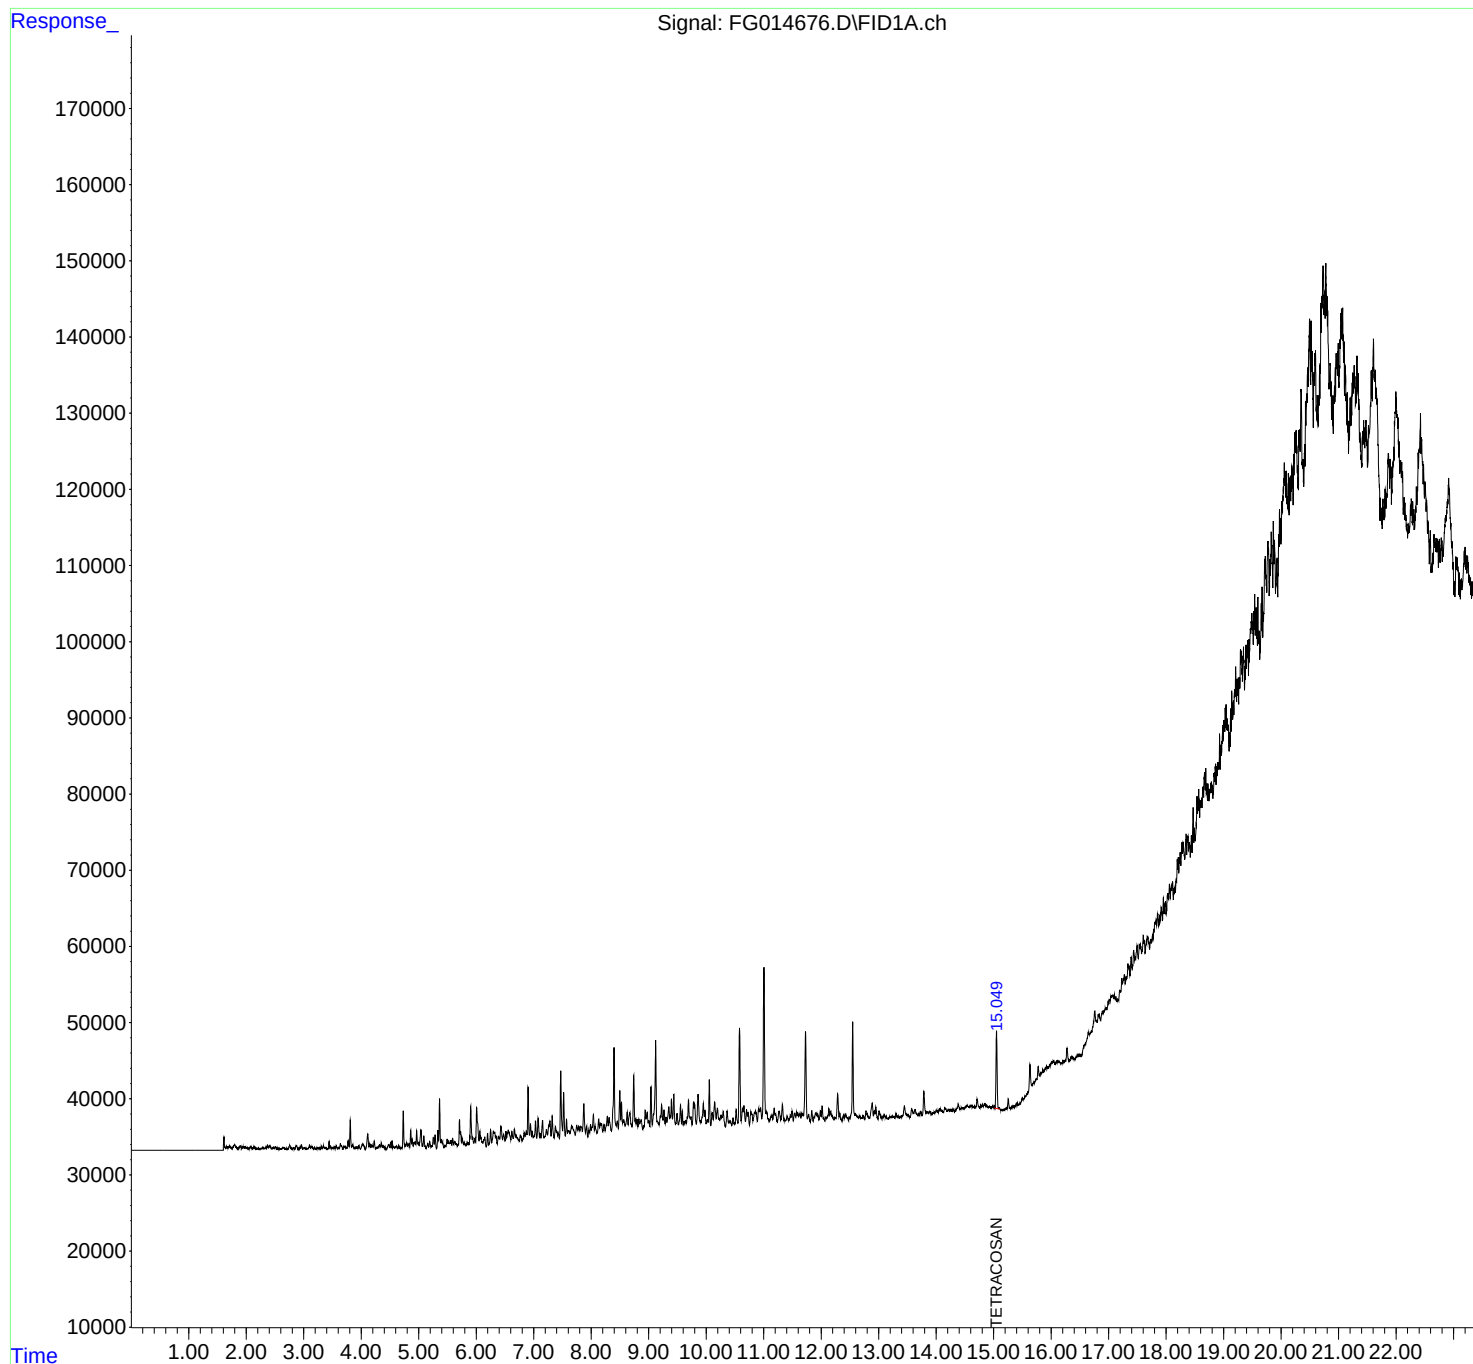

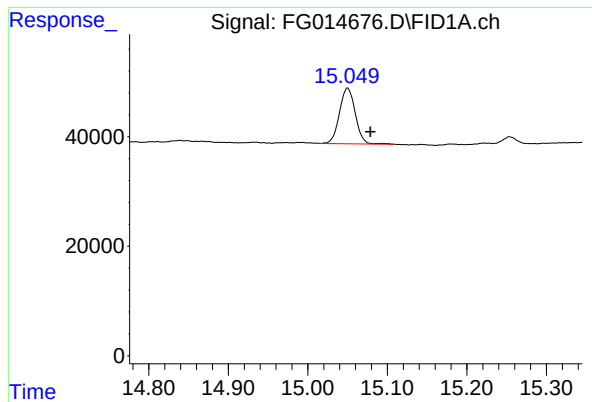

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.050 min
Delta R.T.: -0.029 min
Response: 139952
Conc: 1.17 ug/ml

Instrument :
FID_G
ClientSampleId :
EX-11-TPH-3