

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
Data File : FG014704.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2024 09:27
Operator : YP\AJ
Sample : P4721-13
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
EX-9-TPH-6

Integration File: autoint1.e
Quant Time: Nov 09 00:04:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
Quant Title :
QLast Update : Mon Oct 21 17:03:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.047	1360926	11.378 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
Data File : FG014704.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2024 09:27
Operator : YP\AJ
Sample : P4721-13
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
EX-9-TPH-6

Integration File: autoint1.e
Quant Time: Nov 09 00:04:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
Quant Title :
QLast Update : Mon Oct 21 17:03:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

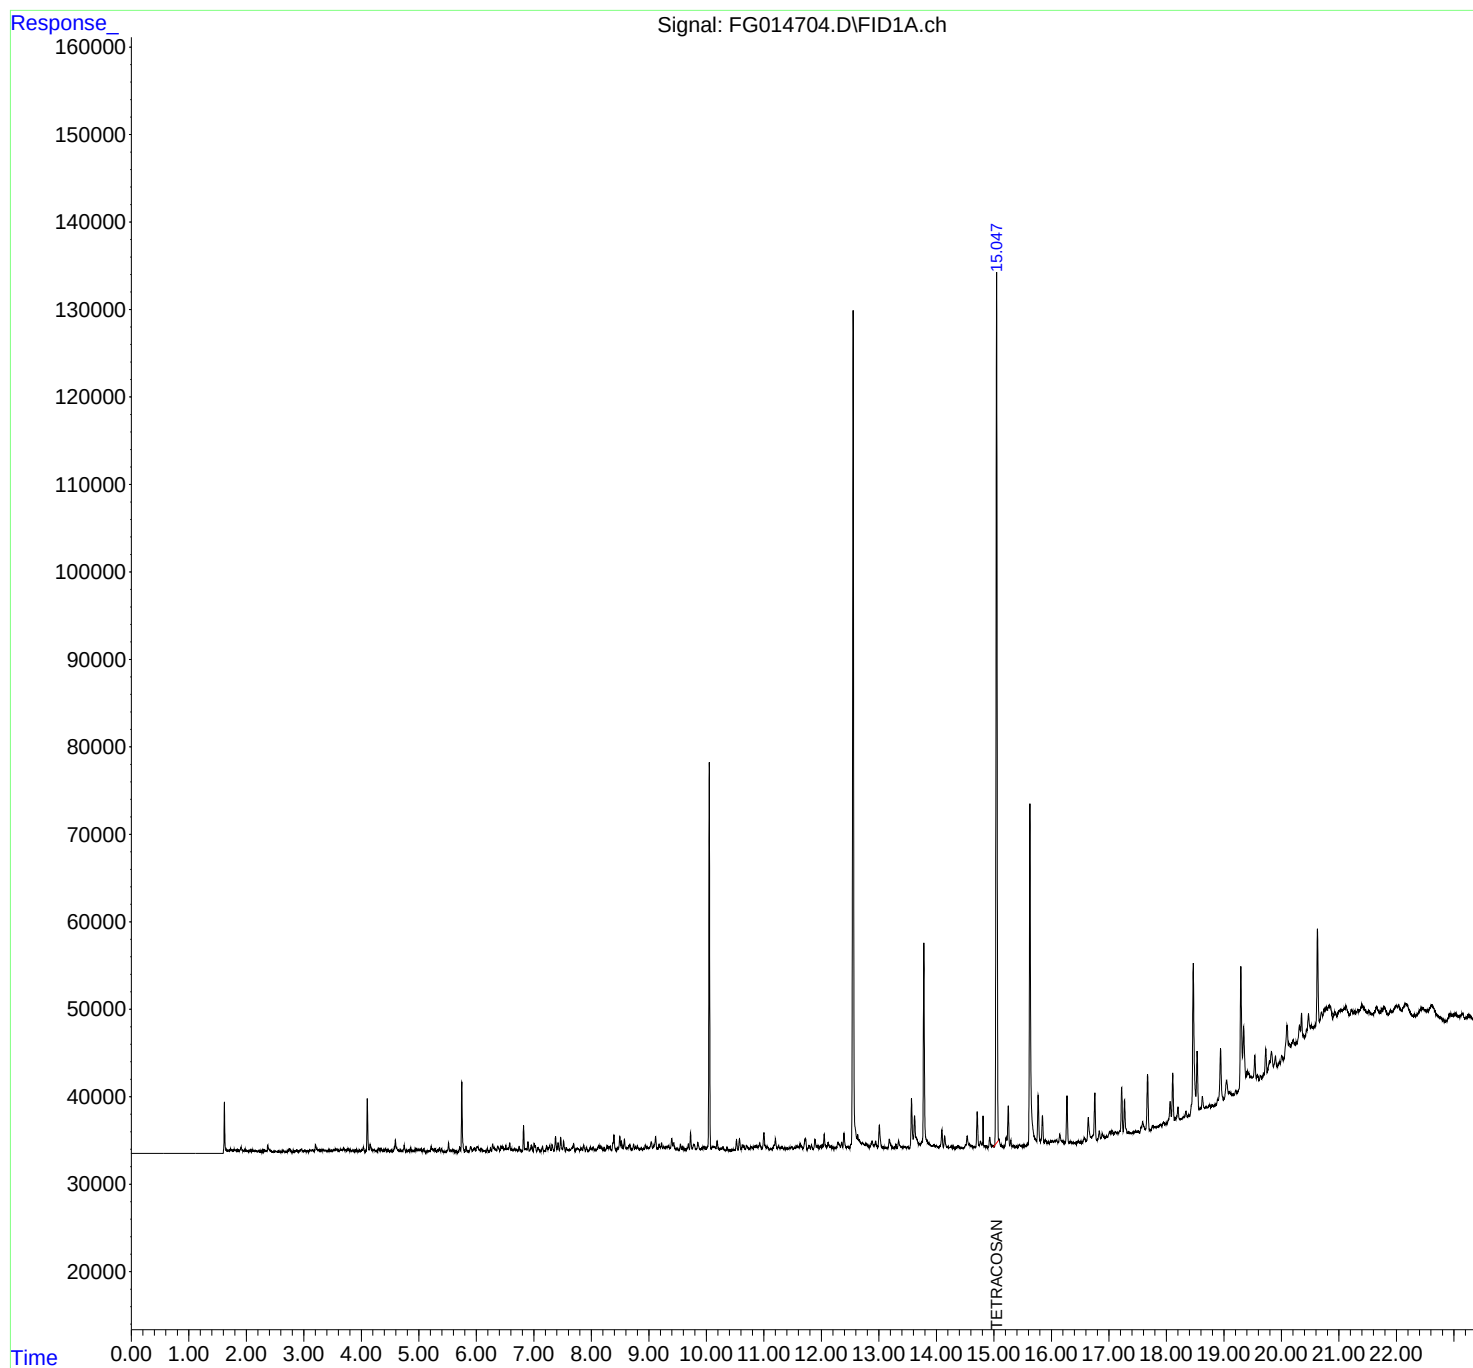

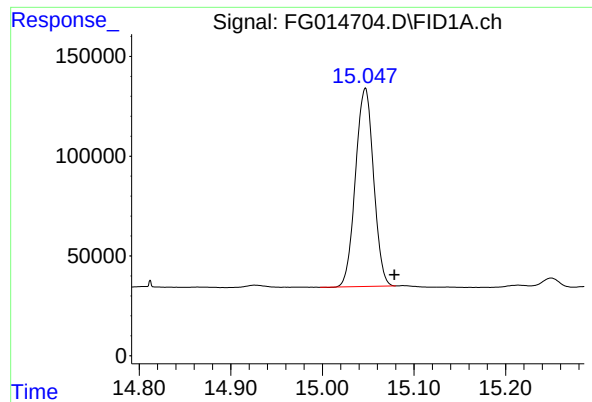

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.047 min
Delta R.T.: -0.032 min
Response: 1360926
Conc: 11.38 ug/ml

Instrument :
FID_G
ClientSampleId :
EX-9-TPH-6