


LB133334

7471B

INSTRUMENT ID: CV1

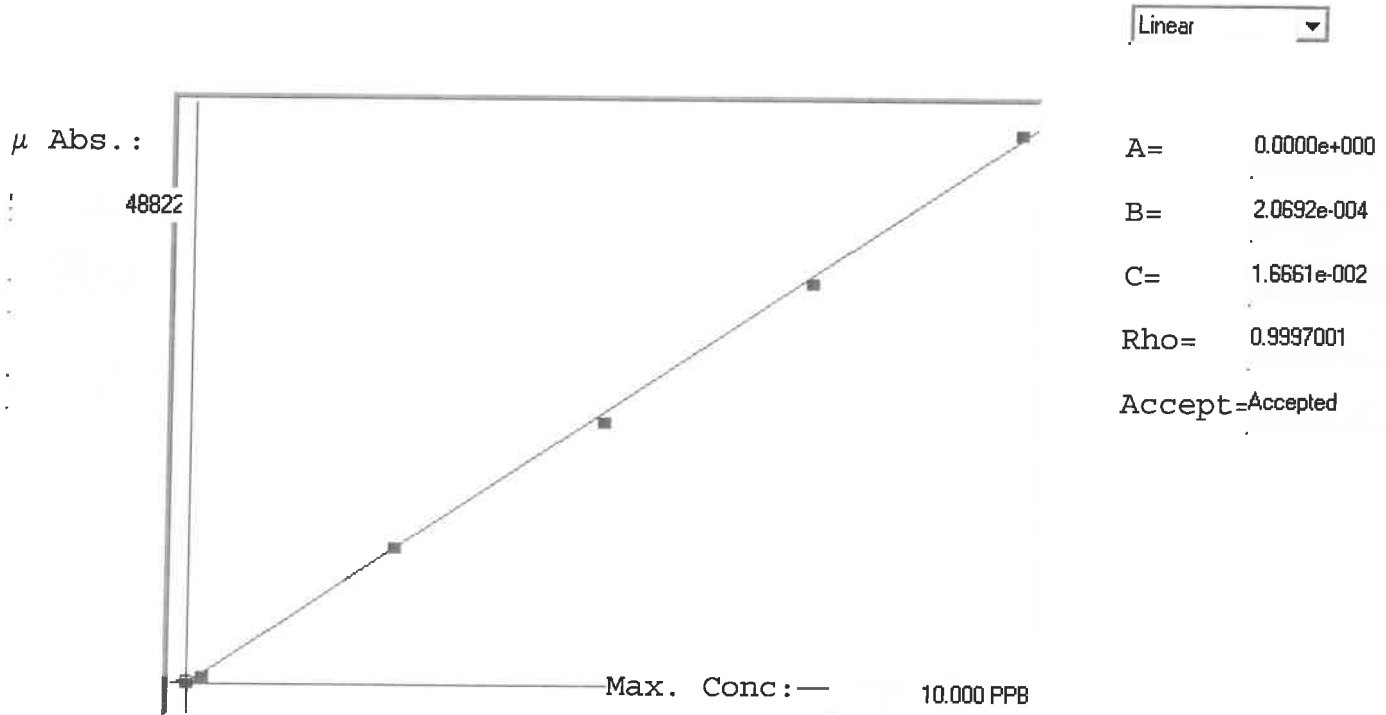

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	9/10
0.0	0.000	0.084	0.084	324	0.000	324					-
0.2	0.200	0.176	-0.024	770	0.0 %	770					12
2.5	2.500	2.544	0.044	12213	0.0 %	12213					2
5.0	5.000	4.870	-0.130	23455	0.0 %	23455					-3
7.5	7.500	7.408	-0.092	35721	0.0 %	35721					-1
10.0	10.000	10.119	0.119	48822	0.0 %	48822					1

LB133334 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 07 Nov 2024 14:17:01

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	324	-	0.0000	7471B	PPB	07 Nov 2024 14:17:09	S	Std
0.2 - 1	50.2	770	-	0.2000	7471B	PPB	07 Nov 2024 14:19:25	S	Std
2.5 - 1	52.5	12213	-	2.5000	7471B	PPB	07 Nov 2024 14:21:42	S	Std
5.0 - 1	55	23455	-	5.0000	7471B	PPB	07 Nov 2024 14:26:50	S	Std
7.5 - 1	59.5	35721	-	7.5000	7471B	PPB	07 Nov 2024 14:29:06	S	Std
10.0 - 1	510	48822	-	10.0000	7471B	PPB	07 Nov 2024 14:38:20	S	Std
ICV74 - 1	ICV74	18921	3.9317	-7471B	PPB	07 Nov 2024 14:41:20	U	SMPL	
ICB74 - 1	ICB74	-154	-0.0152	-7471B	PPB	07 Nov 2024 14:43:35	U	SMPL	
CCV47 - 1	CCV47	23145	4.8057	-7471B	PPB	07 Nov 2024 14:45:53	U	SMPL	
CCB47 - 1	CCB47	-188	-0.0222	-7471B	PPB	07 Nov 2024 14:48:08	U	SMPL	
CRA - 1	CRA	725	0.1667	-7471B	PPB	07 Nov 2024 14:50:25	U	SMPL	
HighStd - 1	HighStd	49480	10.2549	-7471B	PPB	07 Nov 2024 14:52:40	U	SMPL	
ChkStd - 1	ChkStd	32968	6.8383	-7471B	PPB	07 Nov 2024 14:54:55	U	SMPL	
PB164762BL - 1	PBS	-313	-0.0481	-7471B	PPB	07 Nov 2024 14:57:19	U	SMPL	
PB164762BS - 1	LCSS	21305	4.4250	-7471B	PPB	07 Nov 2024 14:59:40	U	SMPL	
P4662-06 - 1	102524-D	328	0.0845	-7471B	PPB	07 Nov 2024 15:01:56	U	SMPL	
P4706-01 - 1	TR-04-110424	4097	0.8644	-7471B	PPB	07 Nov 2024 15:04:15	U	SMPL	
P4706-01MS - 1	TR-04-110424MS	23144	4.8055	-7471B	PPB	07 Nov 2024 15:08:51	U	SMPL	
P4706-01MSD - 1	TR-04-110424MSD	22260	4.6226	-7471B	PPB	07 Nov 2024 15:11:08	U	SMPL	
CCV48 - 1	CCV48	23580	4.8958	-7471B	PPB	07 Nov 2024 15:13:27	U	SMPL	
CCB48 - 1	CCB48	-76	0.0009	-7471B	PPB	07 Nov 2024 15:15:45	U	SMPL	
P4707-01 - 1	HD-02-110424	2165	0.4646	-7471B	PPB	07 Nov 2024 15:18:03	U	SMPL	
P4708-01 - 1	OR-02-110424	3112	0.6606	-7471B	PPB	07 Nov 2024 15:20:18	U	SMPL	
P4718-01 - 1	WB-307-SB01	417	0.1029	-7471B	PPB	07 Nov 2024 15:22:34	U	SMPL	
P4718-02 - 1	WB-307-SB02	994	0.2223	-7471B	PPB	07 Nov 2024 15:24:51	U	SMPL	
P4719-01 - 1	BAYAVE-STOCKPILE	1251	0.2755	-7471B	PPB	07 Nov 2024 15:27:08	U	SMPL	
P4720-01 - 1	JC-701-COMP-01	27291	5.6636	-7471B	PPB	07 Nov 2024 15:29:24	U	SMPL	
P4722-03 - 1	WC-1(0-6)	12843	2.6741	-7471B	PPB	07 Nov 2024 15:31:40	U	SMPL	
P4722-08 - 1	WC-2(0-6)	2528	0.5397	-7471B	PPB	07 Nov 2024 15:34:00	U	SMPL	
P4722-13 - 1	WC-3(0-6)	28819	5.9798	-7471B	PPB	07 Nov 2024 15:36:19	U	SMPL	
P4732-01 - 1	PPE-COMP	33	0.0235	-7471B	PPB	07 Nov 2024 15:38:34	U	SMPL	
CCV49 - 1	CCV49	23712	4.9231	-7471B	PPB	07 Nov 2024 15:40:53	U	SMPL	
CCB49 - 1	CCB49	-40	0.0084	-7471B	PPB	07 Nov 2024 15:43:08	U	SMPL	
P4734-01 - 1	EO-03-11062024	3433	0.7270	-7471B	PPB	07 Nov 2024 15:45:26	U	SMPL	
P4737-01 - 1	TP2	1337	0.2933	-7471B	PPB	07 Nov 2024 15:47:41	U	SMPL	
P4738-01 - 1	72-12018	121	0.0417	-7471B	PPB	07 Nov 2024 15:49:58	U	SMPL	
P4739-01 - 1	TP-14	2305	0.4936	-7471B	PPB	07 Nov 2024 15:52:13	U	SMPL	
P4739-05 - 1	BP-G2	11995	2.4986	-7471B	PPB	07 Nov 2024 15:54:29	U	SMPL	
P4739-09 - 1	BP-B2	3346	0.7090	-7471B	PPB	07 Nov 2024 15:56:47	U	SMPL	
P4739-13 - 1	TP-11	4588	0.9660	-7471B	PPB	07 Nov 2024 15:59:05	U	SMPL	
P4706-01DUP - 1	TR-04-110124DUP	4628	0.9743	-7471B	PPB	07 Nov 2024 16:01:22	U	SMPL	
P4706-01LX5 - 1		286	0.0758	-7471B	PPB	07 Nov 2024 16:03:41	U	SMPL	
P4706-01A - 1		22703	4.7143	-7471B	PPB	07 Nov 2024 16:05:56	U	SMPL	
CCV50 - 1	CCV50	23681	4.9167	-7471B	PPB	07 Nov 2024 16:08:13	U	SMPL	
CCB50 - 1	CCB50	-54	0.0055	-7471B	PPB	07 Nov 2024 16:10:31	U	SMPL	