


LB133407

7470A

INSTRUMENT 1A: CV1

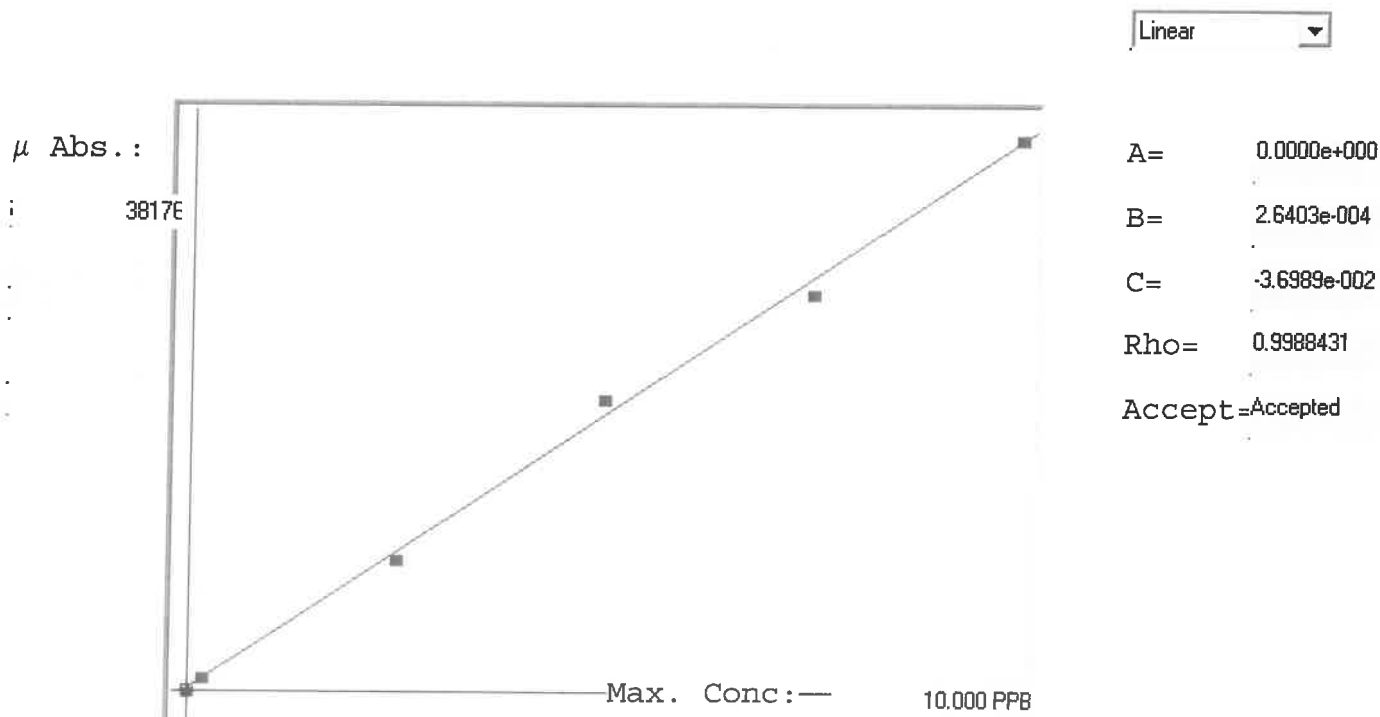

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/p
0.0	0.000	-0.016	-0.016	78	0.000	78	0				7
0.2	0.200	0.215	0.015	954	0.0 %	954					7
2.5	2.500	2.399	-0.101	9227	0.0 %	9227					4
5.0	5.000	5.325	0.325	20310	0.0 %	20310					7
7.5	7.500	7.234	-0.266	27540	0.0 %	27540					7
10.0	10.000	10.043	0.043	38176	0.0 %	38176					0

LB133407 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Nov 2024 14:00:55

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	78	-	0.0000	7470A	PPB	12 Nov 2024 14:03:41	S	Std
0.2 - 1	50.2	954	-	0.2000	7470A	PPB	12 Nov 2024 14:05:57	S	Std
2.5 - 1	52.4	9227	-	2.5000	7470A	PPB	12 Nov 2024 14:08:14	S	Std
5.0 - 1	55	20310	-	5.0000	7470A	PPB	12 Nov 2024 14:10:31	S	Std
7.5 - 1	59.5	27540	-	7.5000	7470A	PPB	12 Nov 2024 14:12:47	S	Std
10.0 - 1	310	38176	-	10.0000	7470A	PPB	12 Nov 2024 14:15:08	S	Std
ICV83 - 1	ICV83	14018	4.0035	-7470A	PPB	12 Nov 2024 14:17:48	U	SMPL	
ICB83 - 1	ICB83	512	0.0310	-7470A	PPB	12 Nov 2024 14:22:35	U	SMPL	
CCV75 - 1	CCV75	16948	4.8653	-7470A	PPB	12 Nov 2024 14:27:35	U	SMPL	
CCB75 - 1	CCB75	184	-0.0655	-7470A	PPB	12 Nov 2024 14:29:49	U	SMPL	
CRA - 1	CRA	1218	0.2386	-7470A	PPB	12 Nov 2024 14:39:58	U	SMPL	
HighStd - 1	HighStd	35792	10.4080	-7470A	PPB	12 Nov 2024 14:42:13	U	SMPL	
ChkStd - 1	ChkStd	23864	6.8996	-7470A	PPB	12 Nov 2024 14:44:28	U	SMPL	
PB164892BL - 1	PBW	276	-0.0385	-7470A	PPB	12 Nov 2024 14:49:28	U	SMPL	
PB164892BS - 1	LCSW	14715	4.2085	-7470A	PPB	12 Nov 2024 14:51:43	U	SMPL	
P4722-05 - 1	WC-1(0-6)	-159	-0.1664	-7470A	PPB	12 Nov 2024 14:53:59	U	SMPL	
P4722-10 - 1	WC-2(0-6)	-33	-0.1293	-7470A	PPB	12 Nov 2024 14:56:17	U	SMPL	
P4722-15 - 1	WC-3(0-6)	35	-0.1093	-7470A	PPB	12 Nov 2024 14:58:34	U	SMPL	
P4722-15DUP - 1	WC-3(0-6)DUP	124	-0.0832	-7470A	PPB	12 Nov 2024 15:00:50	U	SMPL	
P4722-15MS - 1	WC-3(0-6)MS	14091	4.0250	-7470A	PPB	12 Nov 2024 15:03:05	U	SMPL	
CCV76 - 1	CCV76	17759	5.1039	-7470A	PPB	12 Nov 2024 15:05:21	U	SMPL	
CCB76 - 1	CCB76	329	-0.0229	-7470A	PPB	12 Nov 2024 15:07:38	U	SMPL	
P4722-15MSD - 1	WC-3(0-6)MSD	15390	4.4071	-7470A	PPB	12 Nov 2024 15:09:56	U	SMPL	
PB164893BS - 1	LCSW	15025	4.2997	-7470A	PPB	12 Nov 2024 15:14:28	U	SMPL	
P4756-04 - 1	BP-B4	-270	-0.1991	-7470A	PPB	12 Nov 2024 15:16:43	U	SMPL	
P4771-06 - 1	P-1	-21	-0.1258	-7470A	PPB	12 Nov 2024 15:19:01	U	SMPL	
P4771-08 - 1	P-2	11	-0.1164	-7470A	PPB	12 Nov 2024 15:21:17	U	SMPL	
P4788-04 - 1	BP-G3	54	-0.1038	-7470A	PPB	12 Nov 2024 15:23:33	U	SMPL	
P4789-04 - 1	BP-F21	53	-0.1041	-7470A	PPB	12 Nov 2024 15:25:50	U	SMPL	
P4792-01 - 1	DIESE-DRUM	840	0.1274	-7470A	PPB	12 Nov 2024 15:28:08	U	SMPL	
P4792-06 - 1	OILY-STONE-DRUM	-50	-0.1343	-7470A	PPB	12 Nov 2024 15:30:23	U	SMPL	
CCV77 - 1	CCV77	18451	5.3074	-7470A	PPB	12 Nov 2024 15:32:38	U	SMPL	
CCB77 - 1	CCB77	454	0.0139	-7470A	PPB	12 Nov 2024 15:37:32	U	SMPL	
P4793-02 - 1	M00-24-00345	40	-0.1079	-7470A	PPB	12 Nov 2024 15:39:48	U	SMPL	
P4795-02 - 1	LAW-23-00189	157	-0.0735	-7470A	PPB	12 Nov 2024 15:42:03	U	SMPL	
P4798-04 - 1	MH-6	622	0.0633	-7470A	PPB	12 Nov 2024 15:44:18	U	SMPL	
P4798-04DUP - 1	MH-6DUP	-46	-0.1332	-7470A	PPB	12 Nov 2024 15:49:25	U	SMPL	
P4798-04MS - 1	MH-6MS	12787	3.6414	-7470A	PPB	12 Nov 2024 15:51:40	U	SMPL	
P4798-04MSD - 1	MH-6MSD	13736	3.9206	-7470A	PPB	12 Nov 2024 15:56:48	U	SMPL	
CCV78 - 1	CCV78	15815	4.5321	-7470A	PPB	12 Nov 2024 15:59:04	U	SMPL	
CCB78 - 1	CCB78	135	-0.0799	-7470A	PPB	12 Nov 2024 16:01:23	U	SMPL	
PB164792TB - 1		544	0.0404	-7470A	PPB	12 Nov 2024 16:06:20	U	SMPL	
PB164793TB - 1		369	-0.0111	-7470A	PPB	12 Nov 2024 16:08:35	U	SMPL	
P4722-15LX5 - 1		56	-0.1032	-7470A	PPB	12 Nov 2024 16:10:50	U	SMPL	
P4722-15A - 1		13146	3.7470	-7470A	PPB	12 Nov 2024 16:13:06	U	SMPL	
P4798-04LX5 - 1		-128	-0.1573	-7470A	PPB	12 Nov 2024 16:15:21	U	SMPL	
P4798-04A - 1		13086	3.7294	-7470A	PPB	12 Nov 2024 16:17:37	U	SMPL	
PB164893BL - 1	PBW	289	-0.0346	-7470A	PPB	12 Nov 2024 16:19:52	U	SMPL	
CCV79 - 1	CCV79	16429	4.7127	-7470A	PPB	12 Nov 2024 16:25:37	U	SMPL	
CCB79 - 1	CCB79	139	-0.0788	-7470A	PPB	12 Nov 2024 16:27:53	U	SMPL	