

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110924\
 Data File : PS028362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2024 17:46
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 21:39:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.249	7.755	1339.3E6	785.3E6	485.104	492.829
Target Compounds							
1) T	Dalapon	2.628	0.000	5659194	0	1.586	N.D. #
2) T	3,5-DICHL...	6.403	6.698	1499460	2664429	<MDL	1.125 #
3) T	4-Nitroph...	7.036	7.252f	24693955	1935692	13.318	1.828 #
5) T	DICAMBA	0.000	7.951	0	3898048	N.D.	<MDL
6) T	MCPD	7.675f	8.050	46977495	2854053	5.744	<MDL #
7) T	MCPA	7.796	8.277f	970738	9800297	<MDL	1.224 #
8) T	DICHLORPROP	8.175f	0.000	1753576	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.935	0	9837817	N.D.	<MDL
12) T	2,4,5-T	9.508f	10.330	22862454	4735081	1.180	<MDL #
14) T	DINOSEB	11.340	0.000	5404080	0	<MDL	N.D. #
15) T	Picloram	11.148	12.378	65643032	18592175	2.090	1.292 #
16) T	DCPA	11.622	0.000	8599562	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110924\
Data File : PS028362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2024 17:46
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 21:39:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

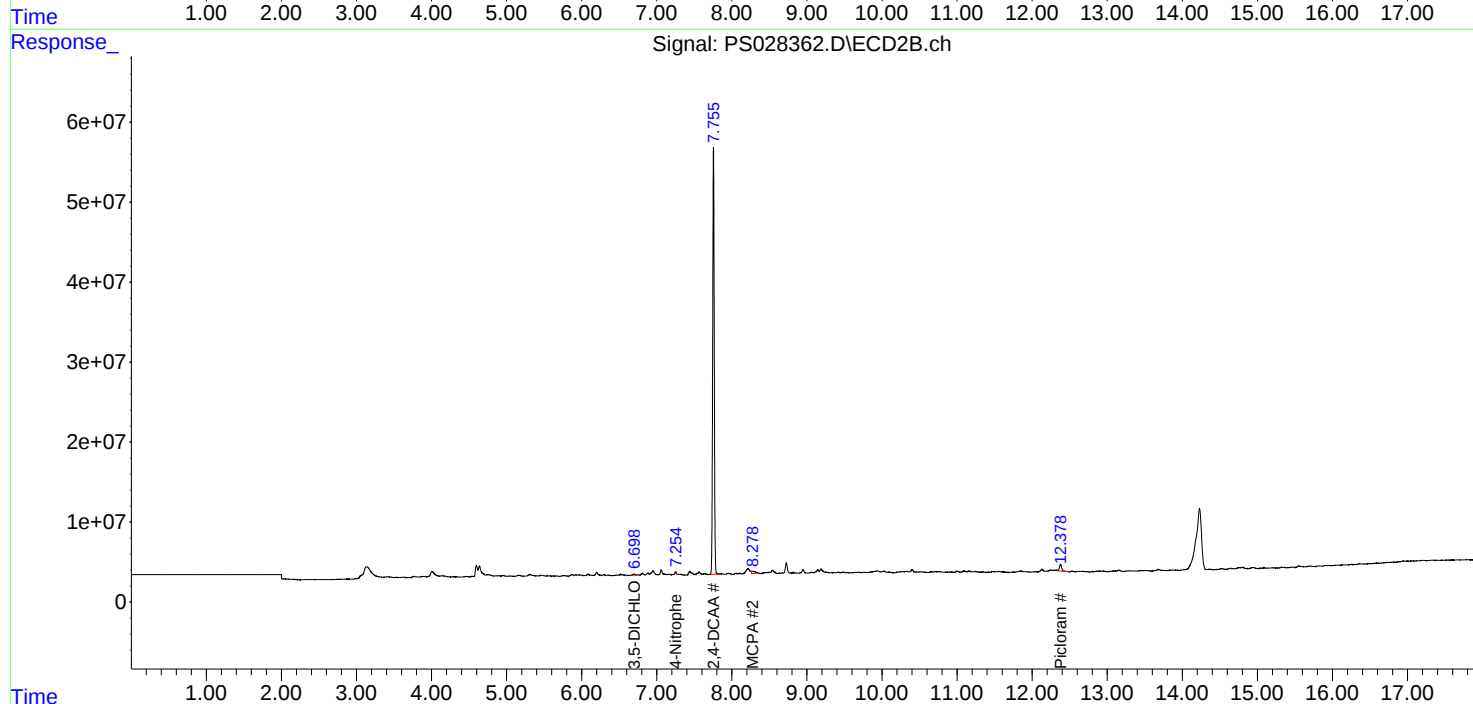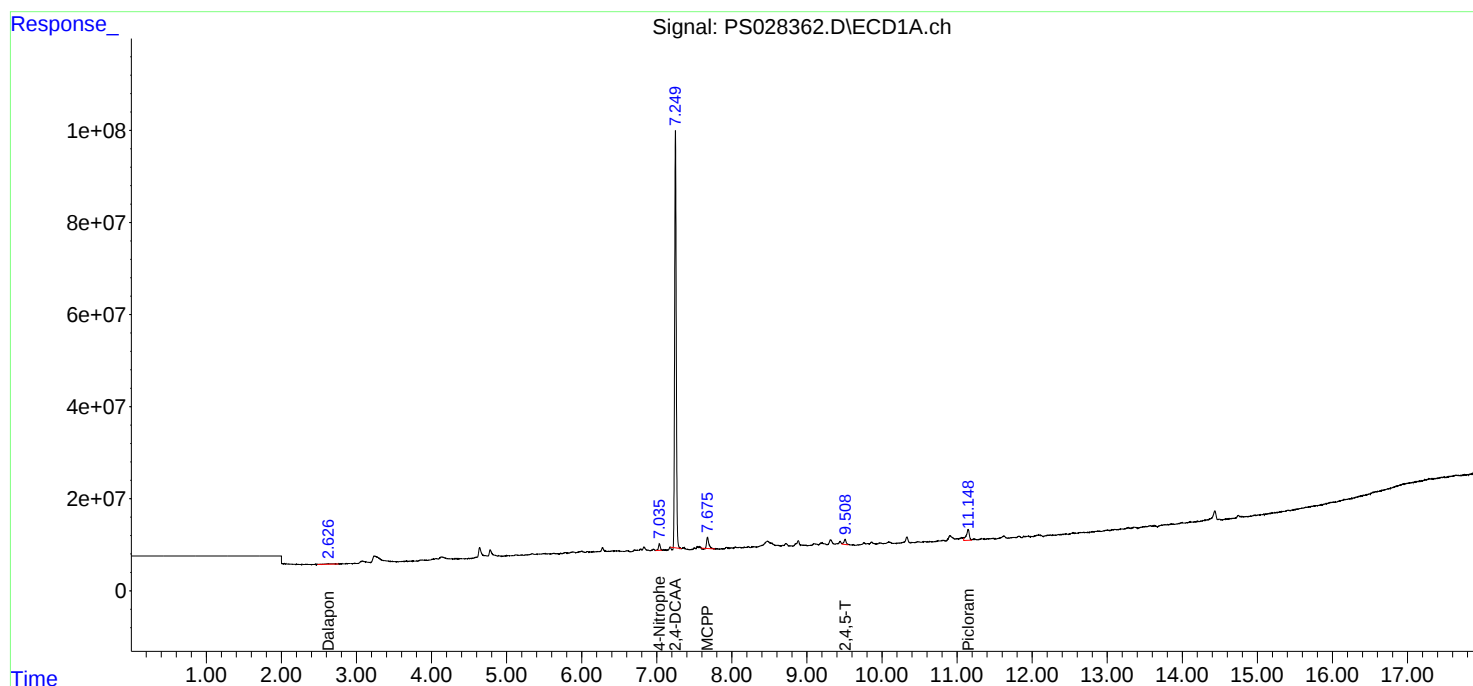


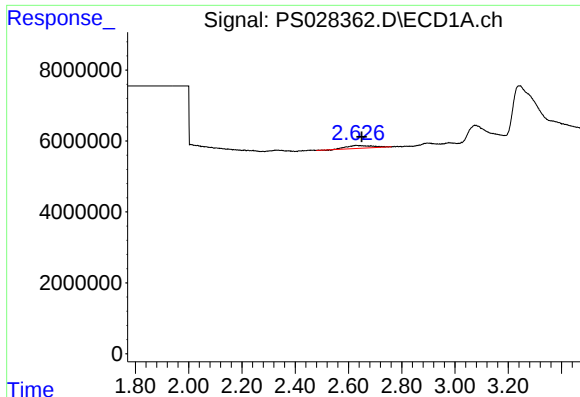

#1 Dalapon


R.T.: 2.628 min
Delta R.T.: -0.022 min
Response: 5659194
Conc: 1.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

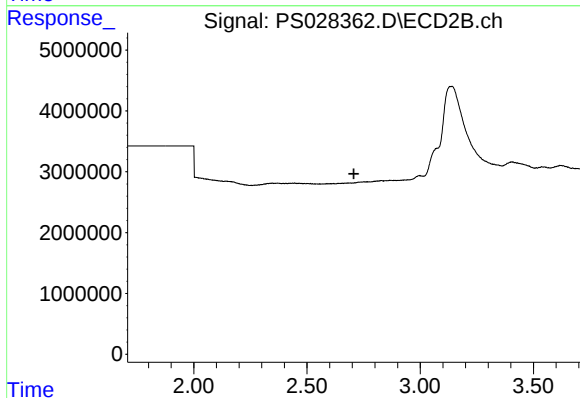


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.707 min
Response: 0
Conc: N.D.

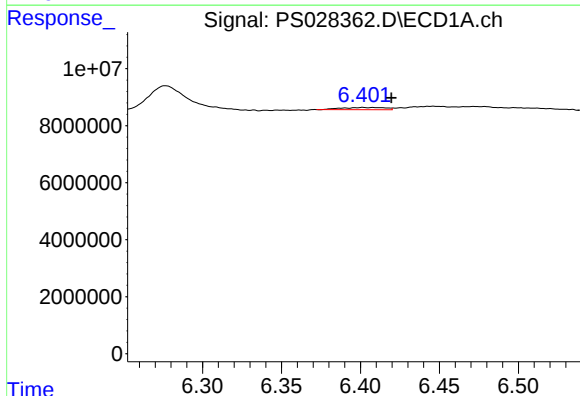


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.403 min
Delta R.T.: -0.016 min
Response: 1499460
Conc: N.D.

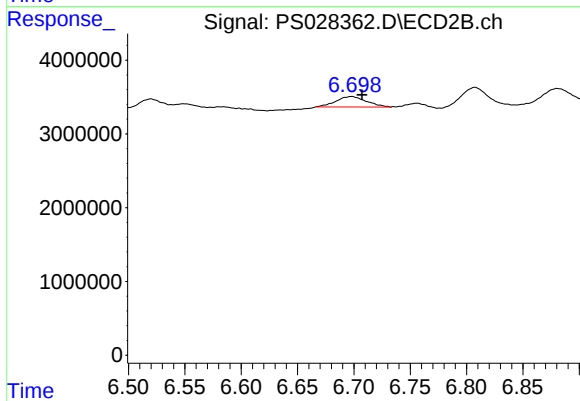

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.698 min
Delta R.T.: -0.009 min
Response: 2664429
Conc: 1.12 ng/ml

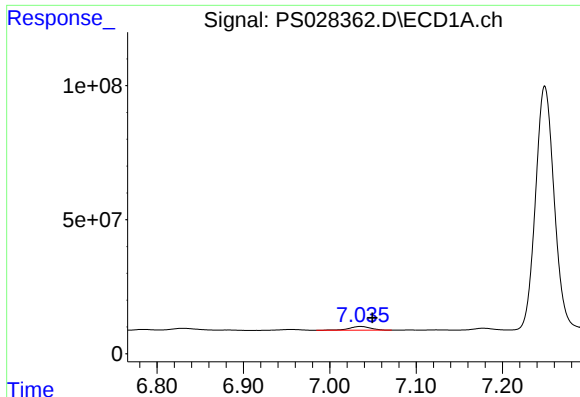

#3 4-Nitrophenol


R.T.: 7.036 min
Delta R.T.: -0.014 min
Response: 24693955
Conc: 13.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

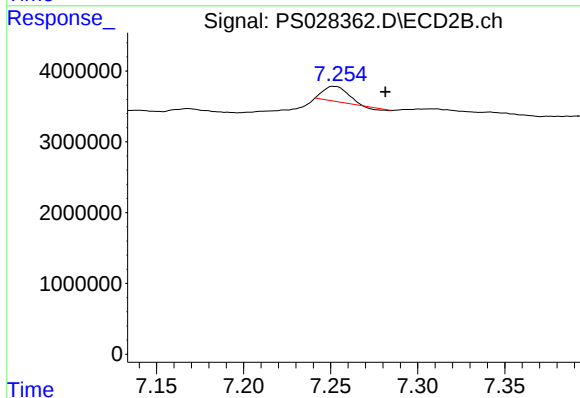


#3 4-Nitrophenol

R.T.: 7.252 min
Delta R.T.: -0.029 min
Response: 1935692
Conc: 1.83 ng/ml

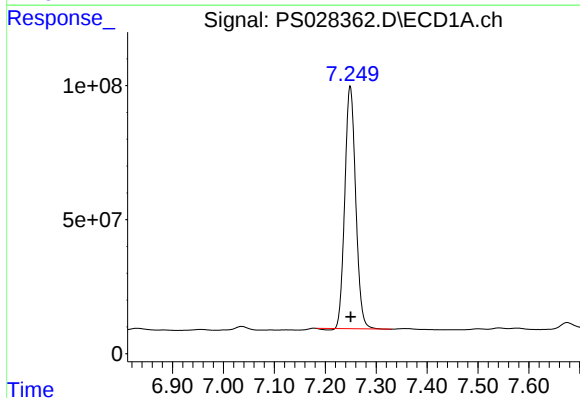


#4 2,4-DCAA

R.T.: 7.249 min
Delta R.T.: -0.001 min
Response: 1339253870
Conc: 485.10 ng/ml

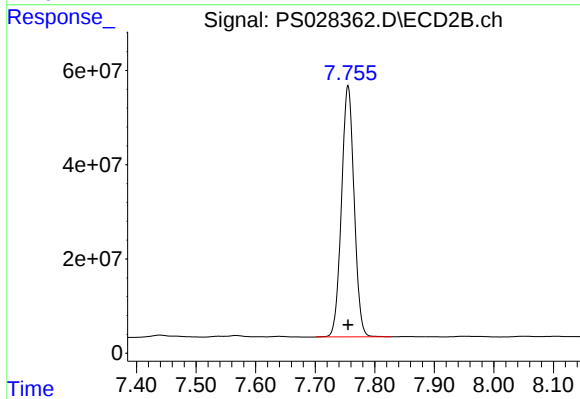

#4 2,4-DCAA


R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 785284113
Conc: 492.83 ng/ml

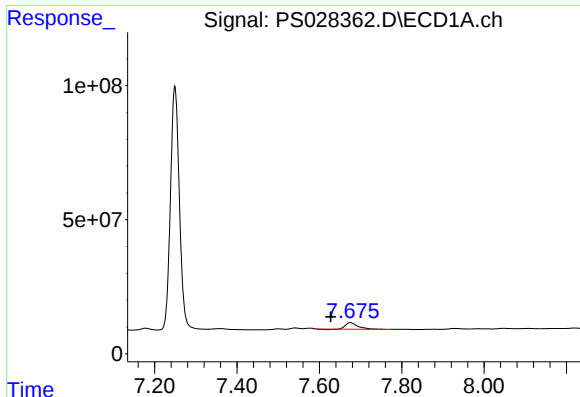

#6 MCPP


R.T.: 7.675 min
Delta R.T.: 0.048 min
Response: 46977495
Conc: 5.74 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

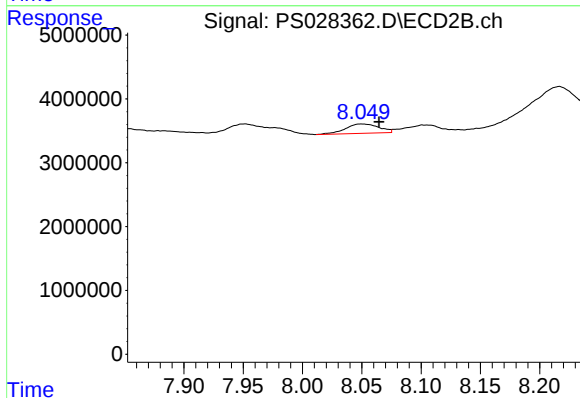


#6 MCPP

R.T.: 8.050 min
Delta R.T.: -0.015 min
Response: 2854053
Conc: N.D.

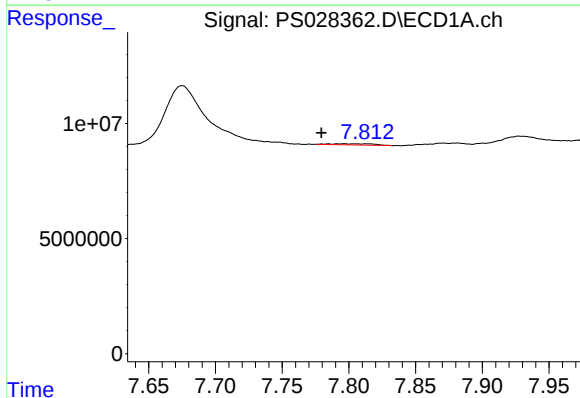


#7 MCPA

R.T.: 7.796 min
Delta R.T.: 0.016 min
Response: 970738
Conc: N.D.

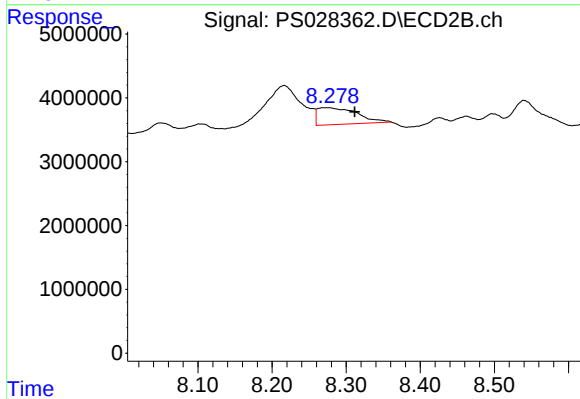

#7 MCPA


R.T.: 8.277 min
Delta R.T.: -0.035 min
Response: 9800297
Conc: 1.22 ug/ml

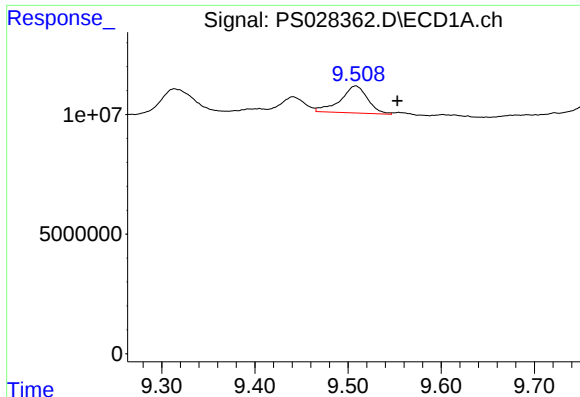

#12 2,4,5-T


R.T.: 9.508 min
Delta R.T.: -0.045 min
Response: 22862454
Conc: 1.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

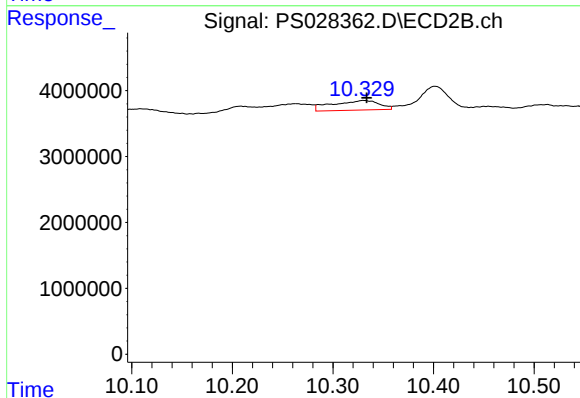


#12 2,4,5-T

R.T.: 10.330 min
Delta R.T.: -0.003 min
Response: 4735081
Conc: N.D.

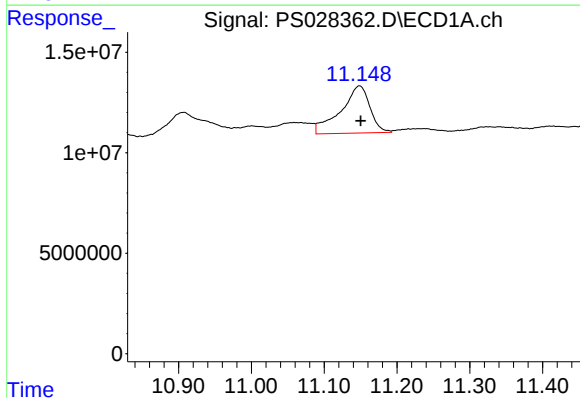

#15 Picloram

R.T.: 11.148 min
Delta R.T.: -0.002 min
Response: 65643032
Conc: 2.09 ng/ml

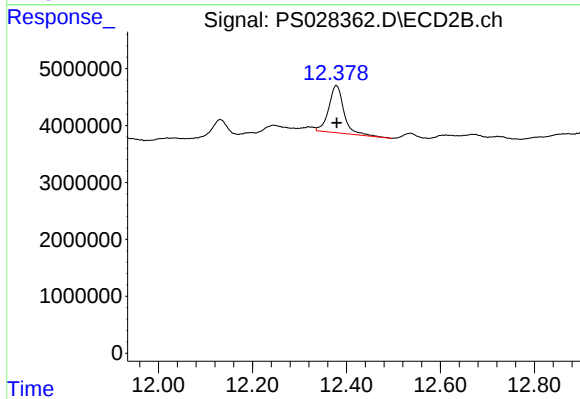

#15 Picloram

R.T.: 12.378 min
Delta R.T.: 0.000 min
Response: 18592175
Conc: 1.29 ng/ml