
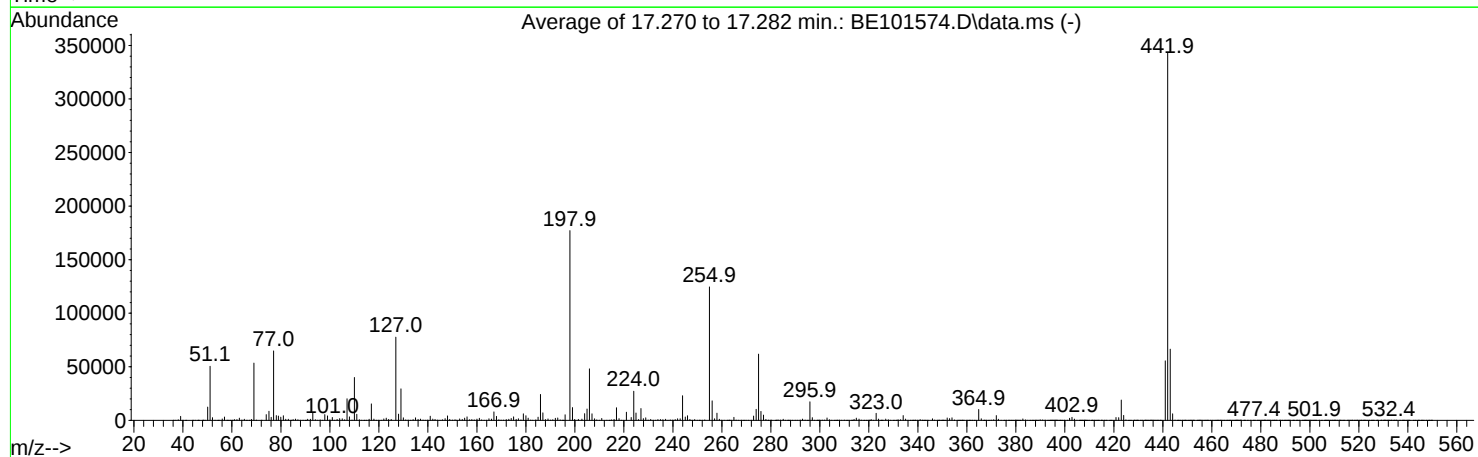


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101574.D
Acq On : 12 Nov 2024 9:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 00:01:20 2024

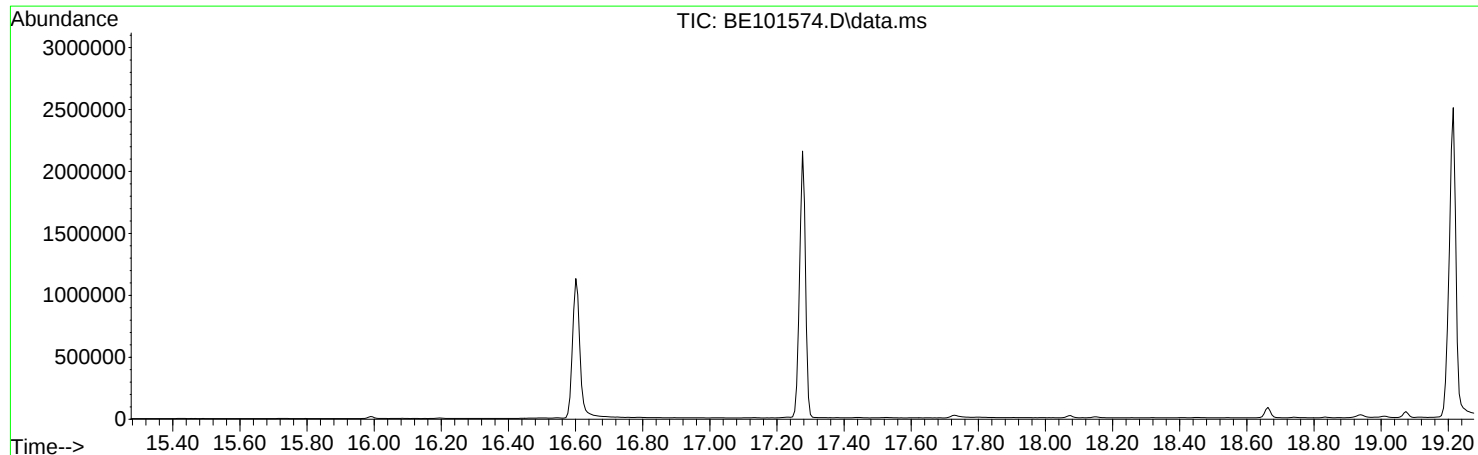




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2491

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	28.5	50565	PASS
68	69	0.00	2	1.7	904	PASS
69	198	0.00	100	30.2	53455	PASS
70	69	0.00	2	0.5	244	PASS
127	198	10	80	43.9	77729	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	177164	PASS
199	198	5	9	6.8	11982	PASS
275	198	10	60	34.9	61835	PASS
365	198	1	100	5.7	10154	PASS
441	198	0.01	100	31.4	55627	PASS
442	442	50	100	100.0	343375	PASS
443	442	15	24	19.4	66533	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101574.D
Acq On : 12 Nov 2024 9:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 12 11:49:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

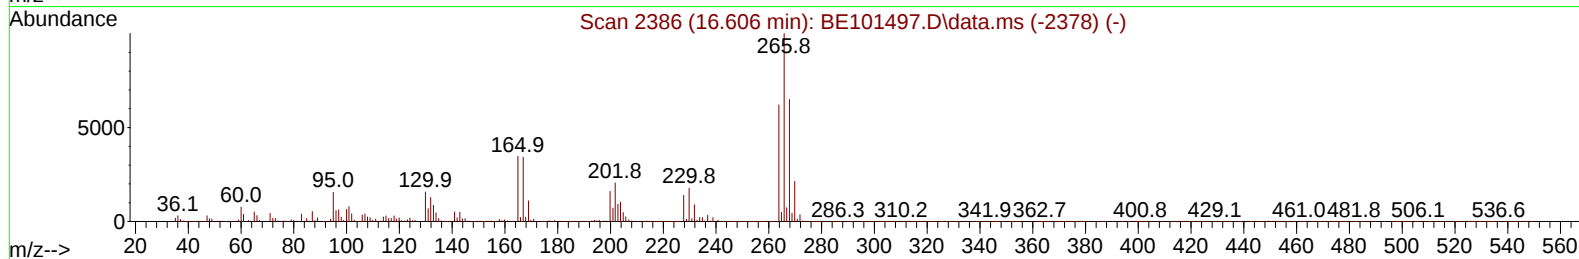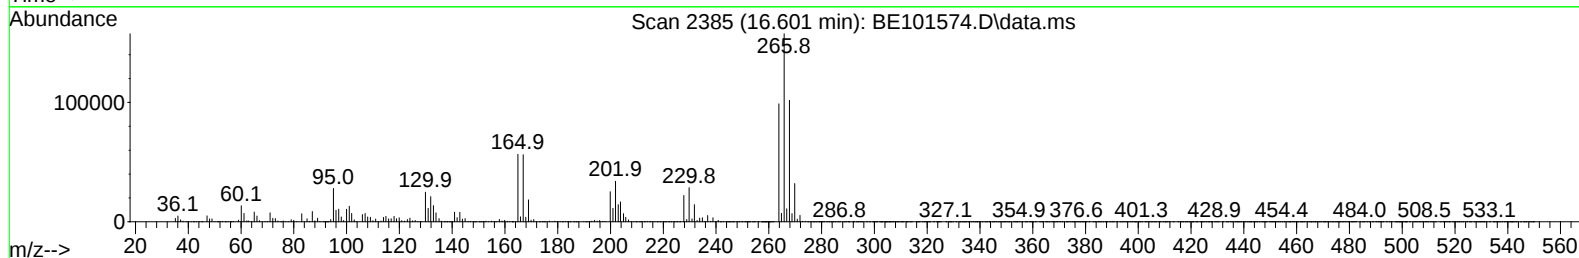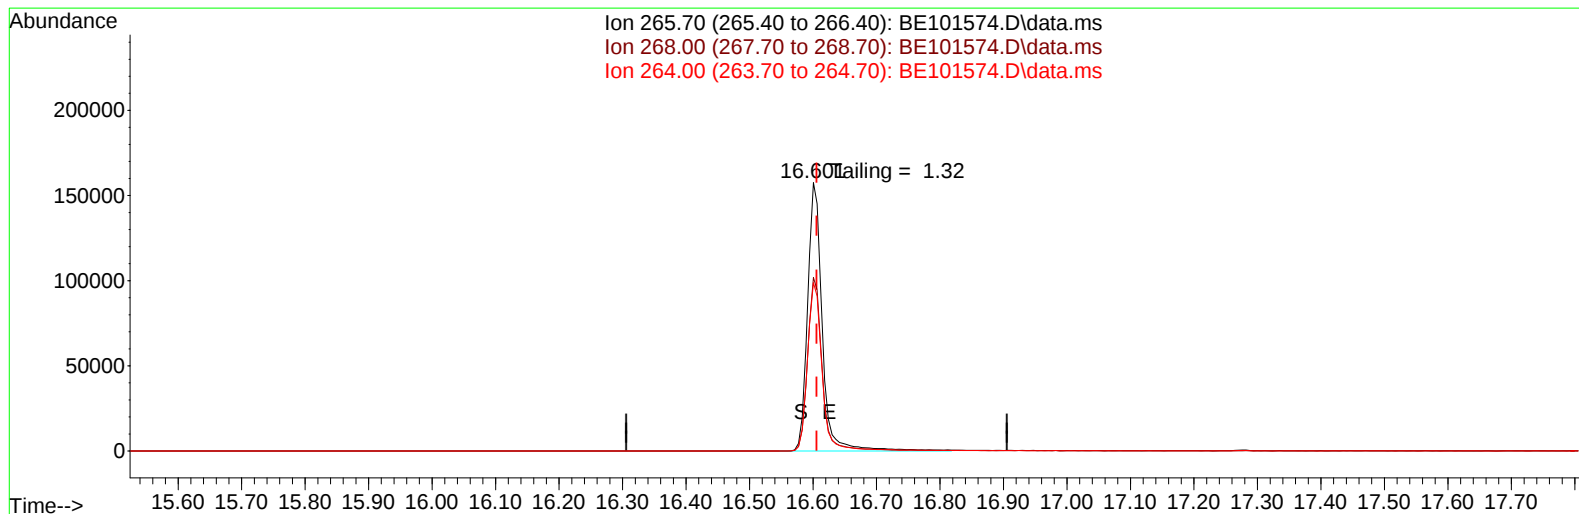

TIC: BE101574.D\data.ms

(70) Pentachlorophenol (C)

16.601min (-0.005) 60825.00 ng




response 252938

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	64.63
264.00	62.00	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101574.D
Acq On : 12 Nov 2024 9:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 12 11:49:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

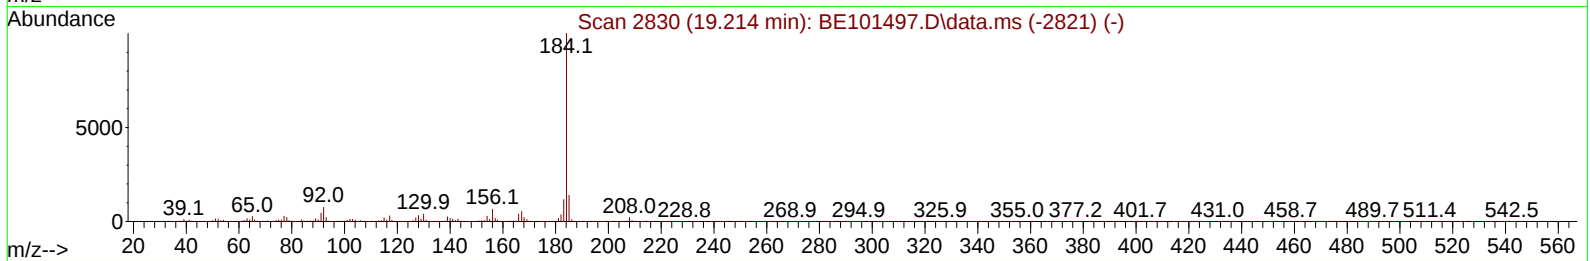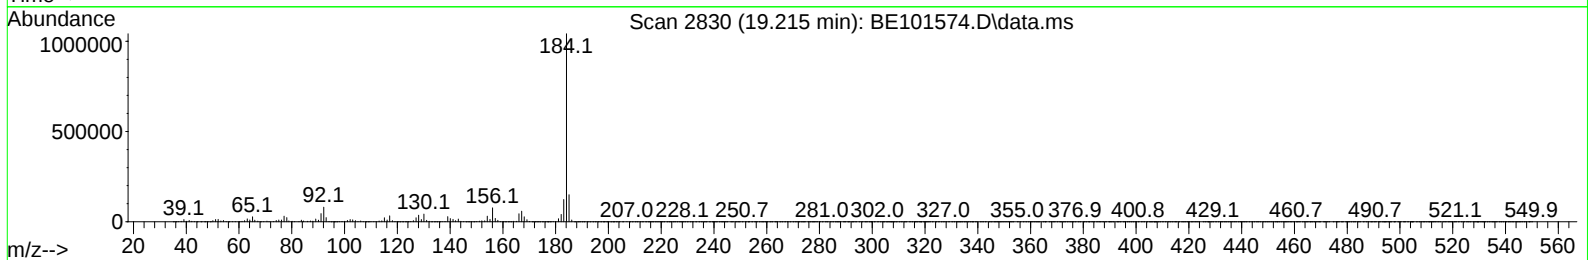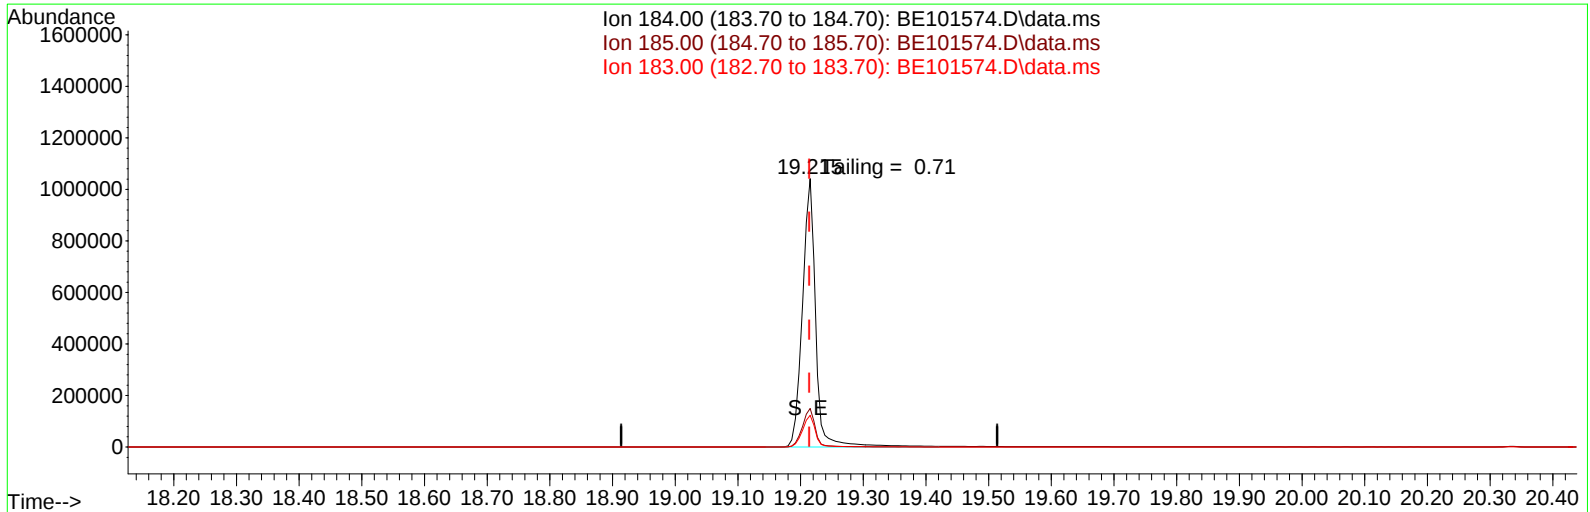

TIC: BE101574.D\data.ms

(77) Benzidine

19.215min (+ 0.001) 5484.13 ng

response 1525802

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.36
183.00	11.70	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/12/2024	BNA_E	<u>BE101574.D</u>
Compound Name	Response	Retention Time
DDT	806084	20.337
DDD	20095	19.903
DDE	818	19.386
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20913	826997	2.53

Instrument :
BNA_E
ClientSampleId :
DFTPP