
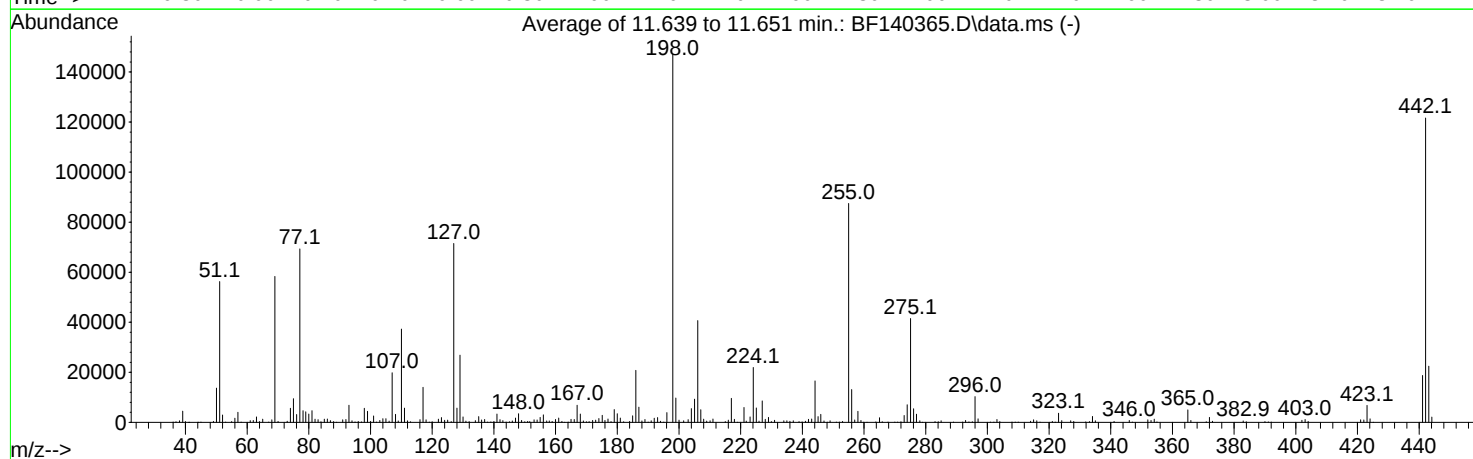


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140365.D
Acq On : 14 Nov 2024 16:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

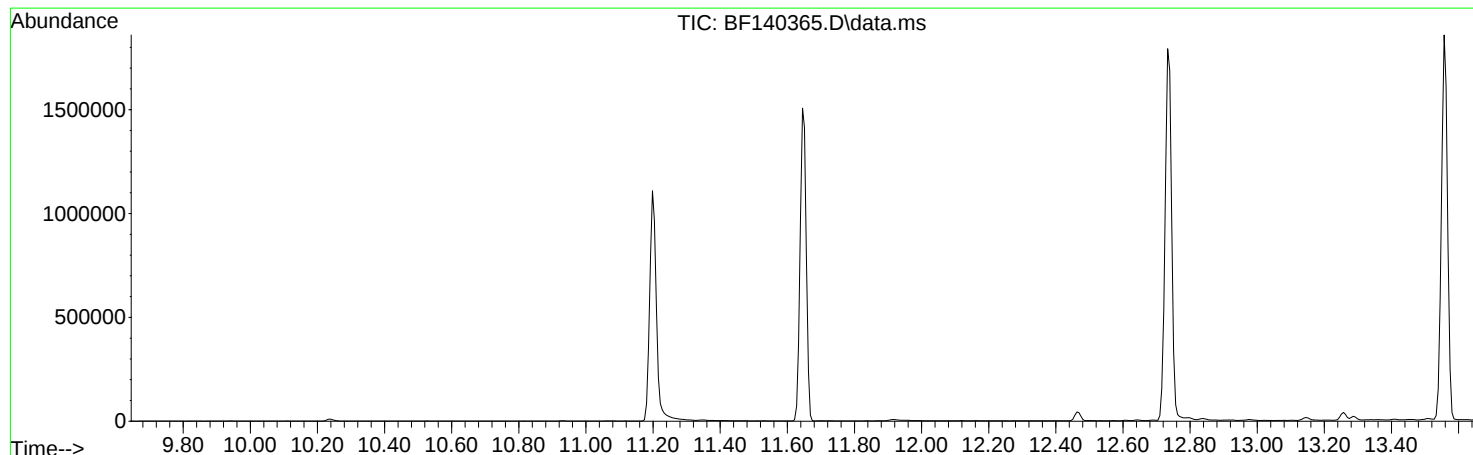




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	56256	PASS
68	69	0.00	2	1.8	1048	PASS
69	198	0.00	100	39.7	58288	PASS
70	69	0.00	2	0.6	372	PASS
127	198	10	80	48.6	71504	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146981	PASS
199	198	5	9	6.6	9705	PASS
275	198	10	60	28.2	41477	PASS
365	198	1	100	3.4	5013	PASS
441	198	0.01	100	12.8	18763	PASS
442	442	50	100	100.0	121611	PASS
443	442	15	24	18.4	22419	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140365.D
Acq On : 14 Nov 2024 16:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 15 03:47:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

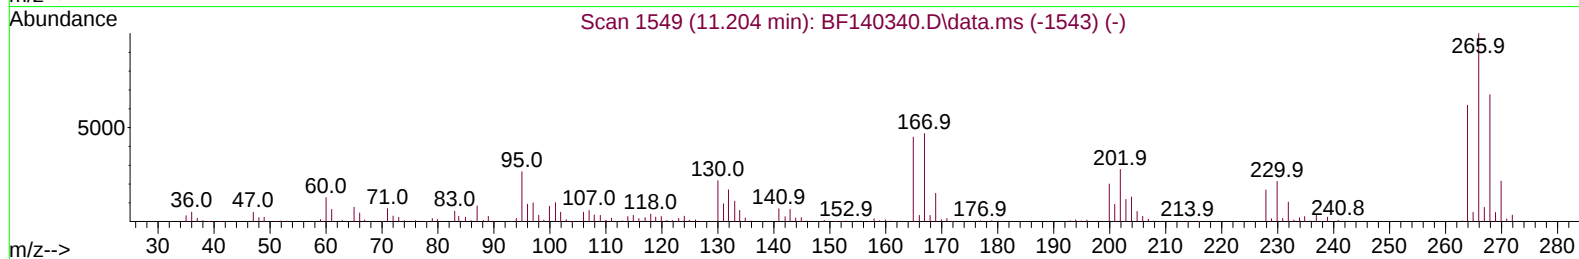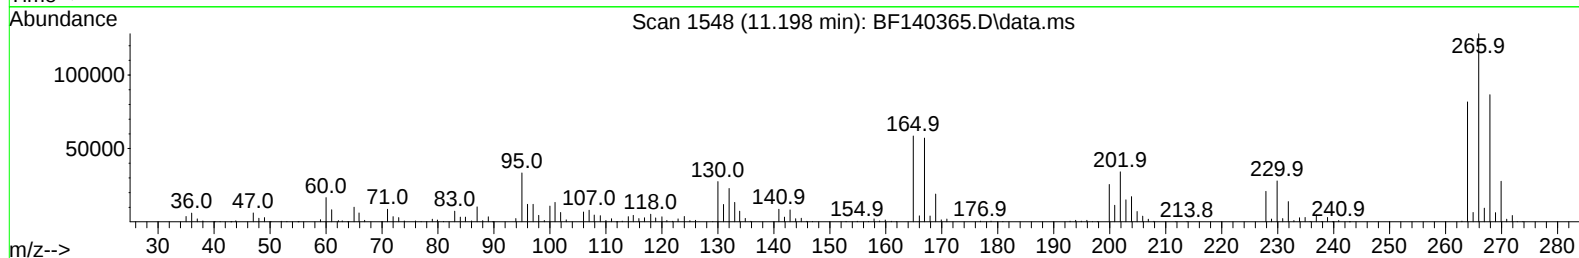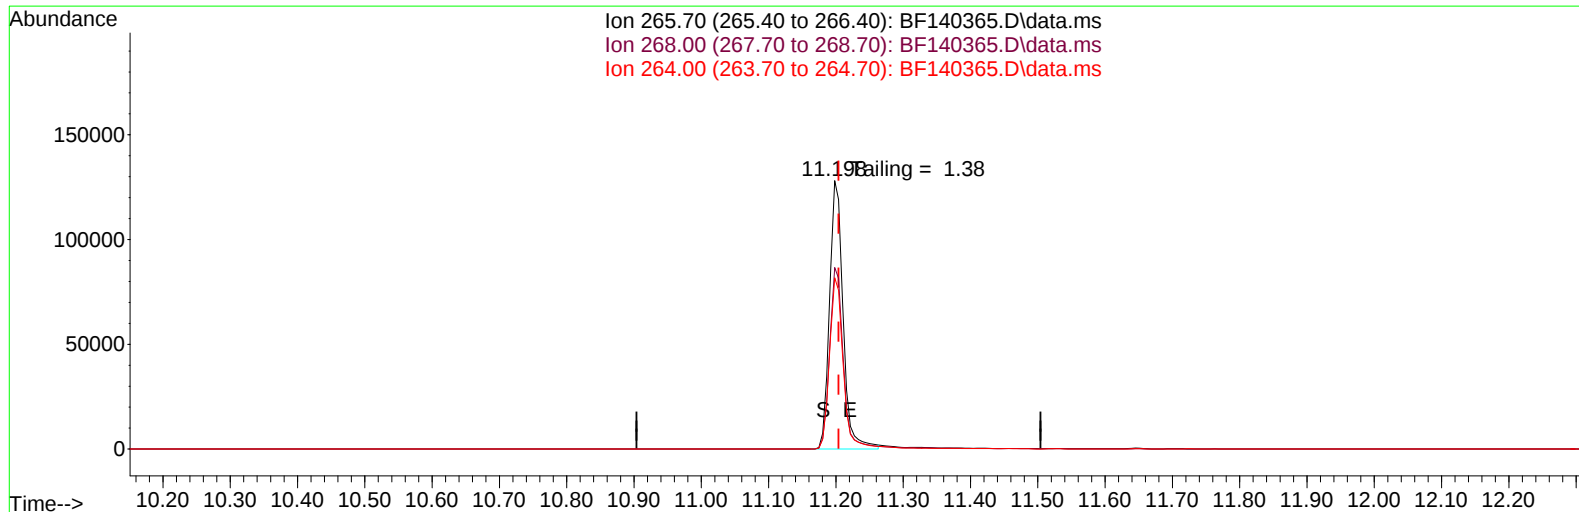

TIC: BF140365.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 63998.59 ng




response 182621

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.63
264.00	62.90	63.80
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\  
Data File : BF140365.D  
Acq On    : 14 Nov 2024  16:35  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 15 03:47:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

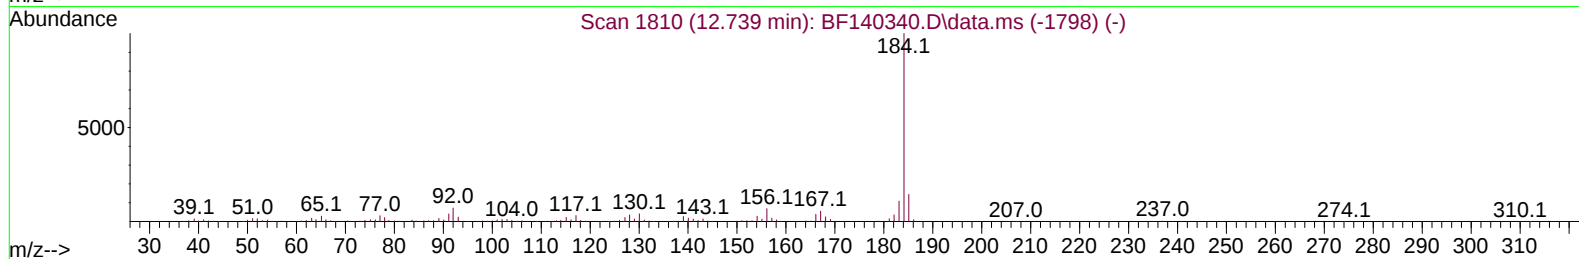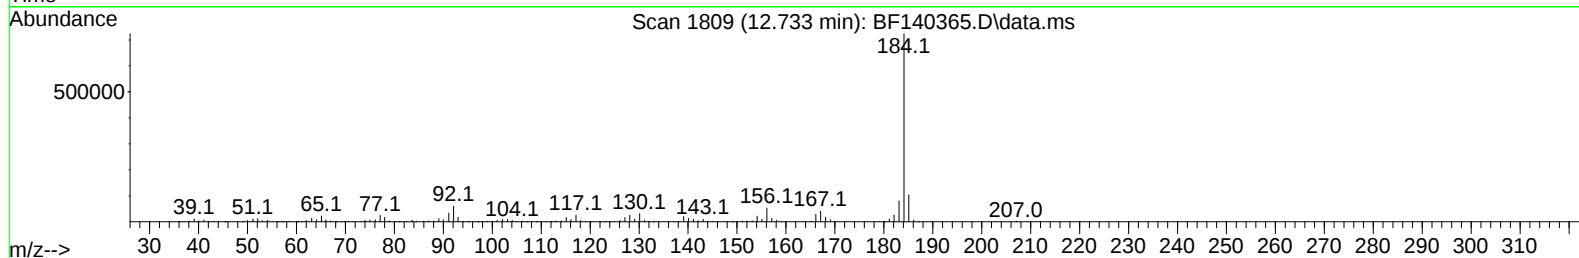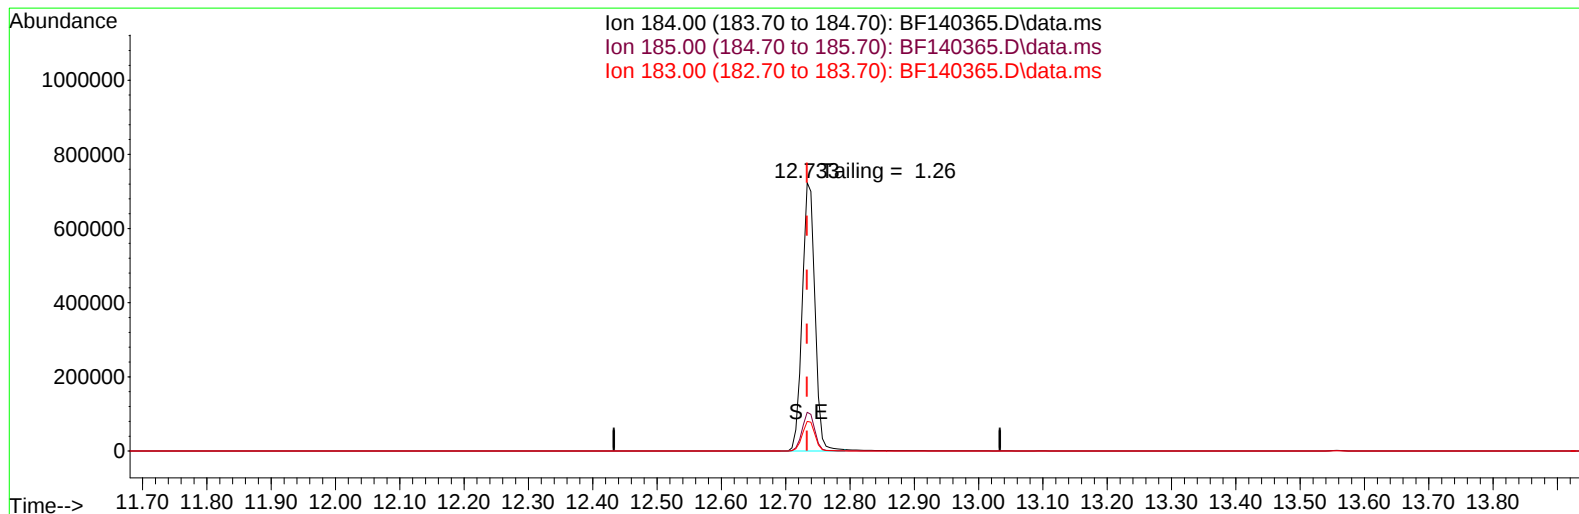

TIC: BF140365.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 36692.71 ng

response **1009743**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.42
183.00	10.80	11.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/14/2024	BNA_F	<u>BF140365.D</u>
Compound Name	Response	Retention Time
DDT	468813	13.557
DDD	15679	13.257
DDE	402	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16081	484894	3.32

Instrument :
BNA_F
ClientSampleId :
DFTPP