


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101491.D
Acq On : 6 Nov 2024 11:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 00:01:20 2024

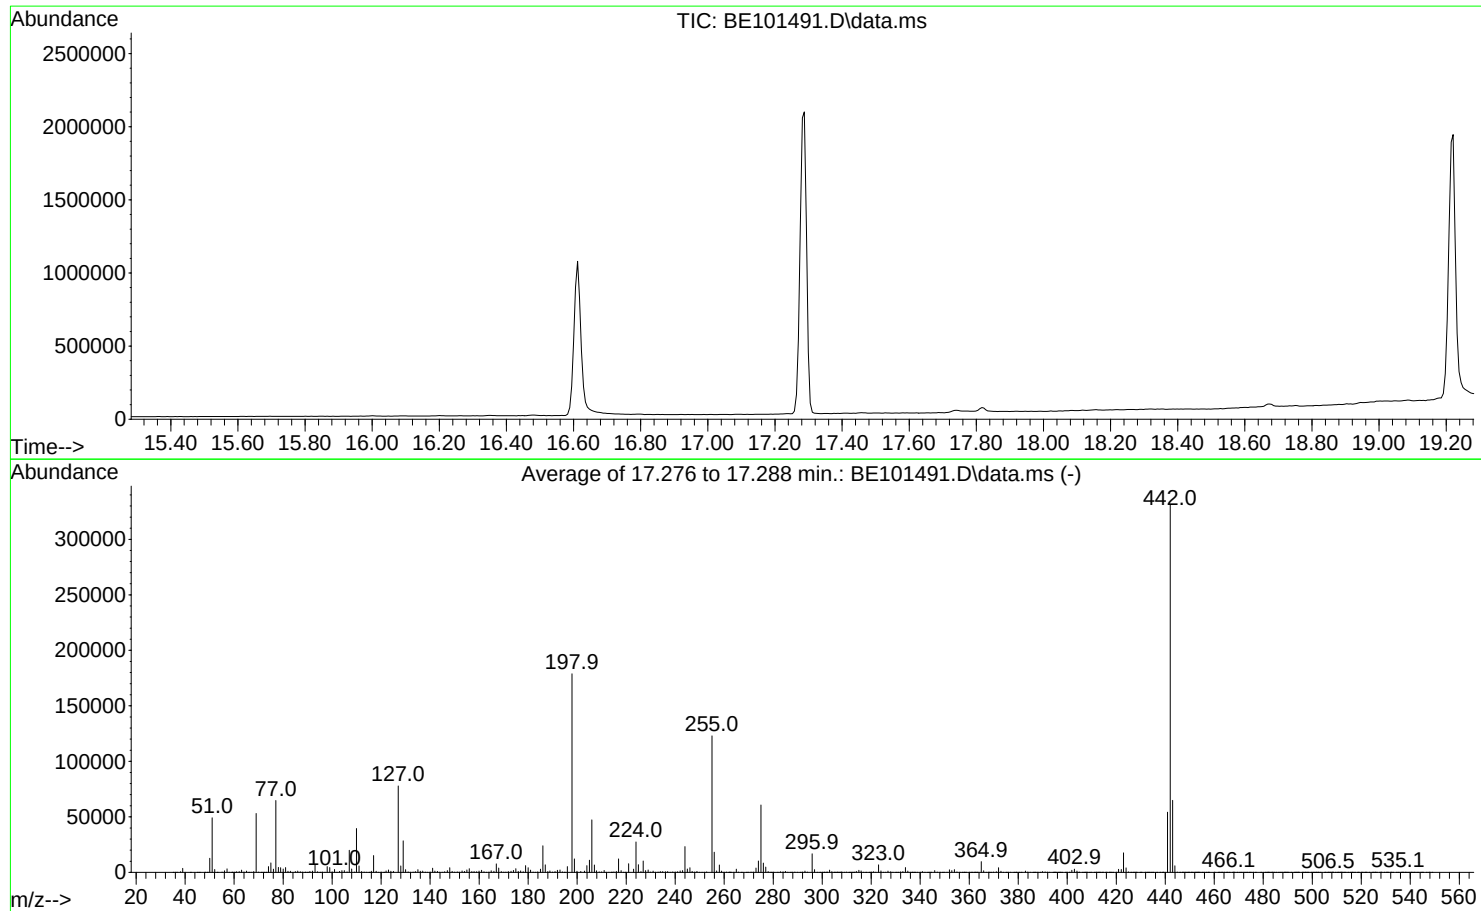




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	49133	PASS
68	69	0.00	2	1.3	713	PASS
69	198	0.00	100	29.7	53047	PASS
70	69	0.00	2	0.4	228	PASS
127	198	10	80	43.5	77857	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	178817	PASS
199	198	5	9	6.7	12064	PASS
275	198	10	60	34.0	60764	PASS
365	198	1	100	5.4	9623	PASS
441	198	0.01	100	30.3	54192	PASS
442	442	50	100	100.0	331371	PASS
443	442	15	24	19.6	64909	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101491.D
Acq On : 6 Nov 2024 11:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 06 14:00:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

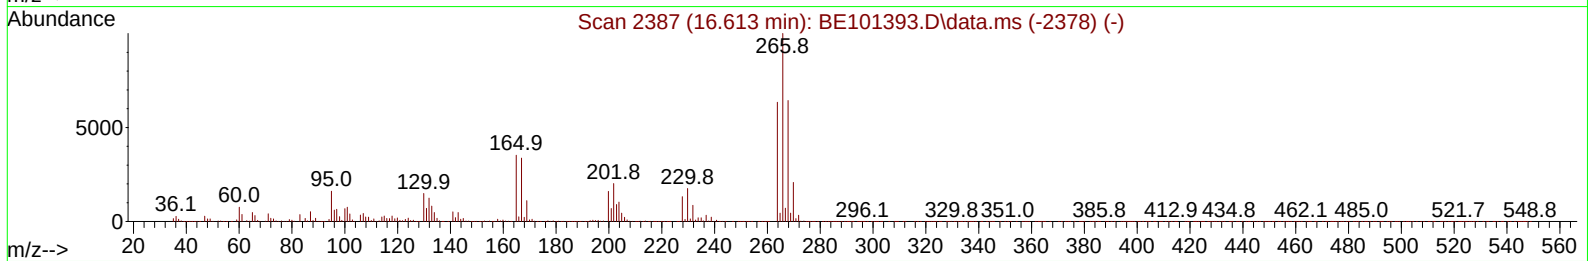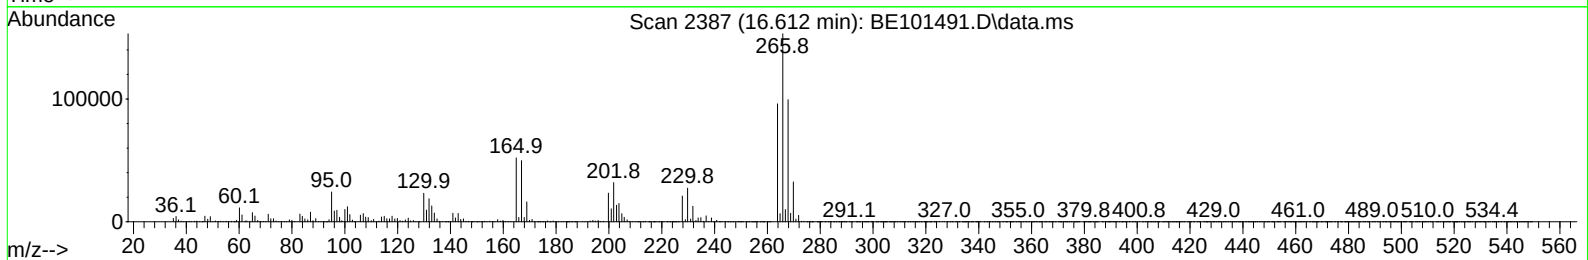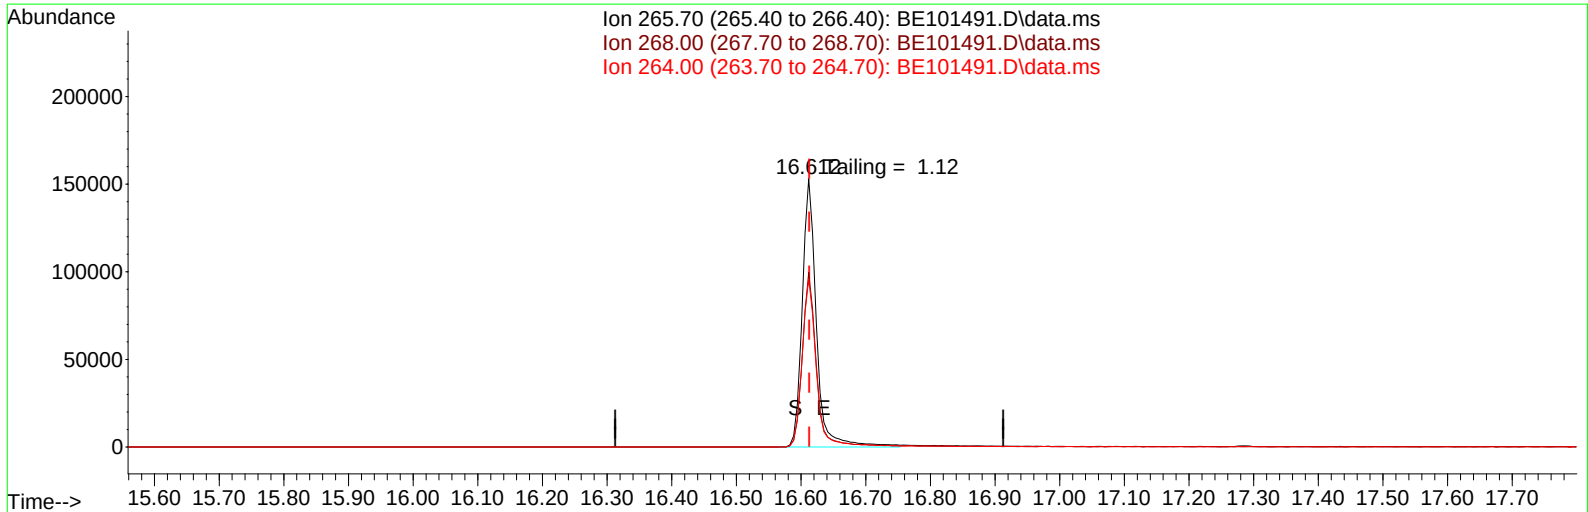

TIC: BE101491.D\data.ms

(70) Pentachlorophenol (C)

16.612min (-0.001) 879438.33 ng




response 237313

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.98
264.00	63.40	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101491.D
Acq On : 6 Nov 2024 11:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 06 14:00:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

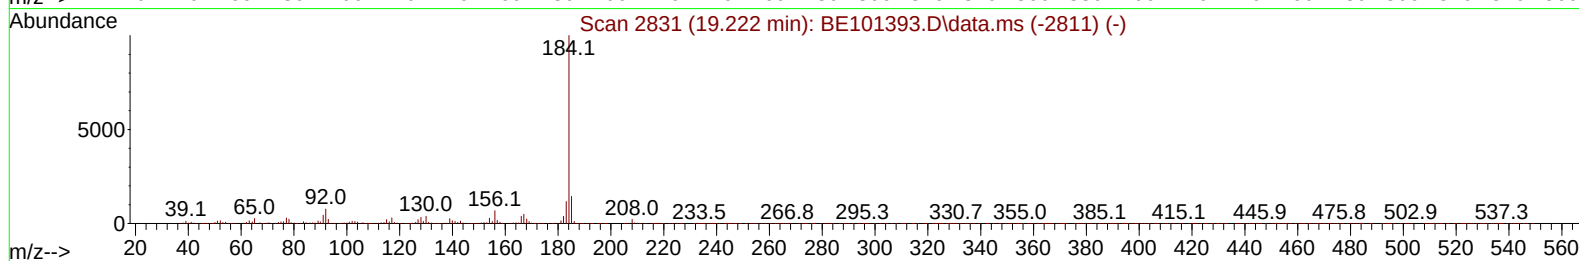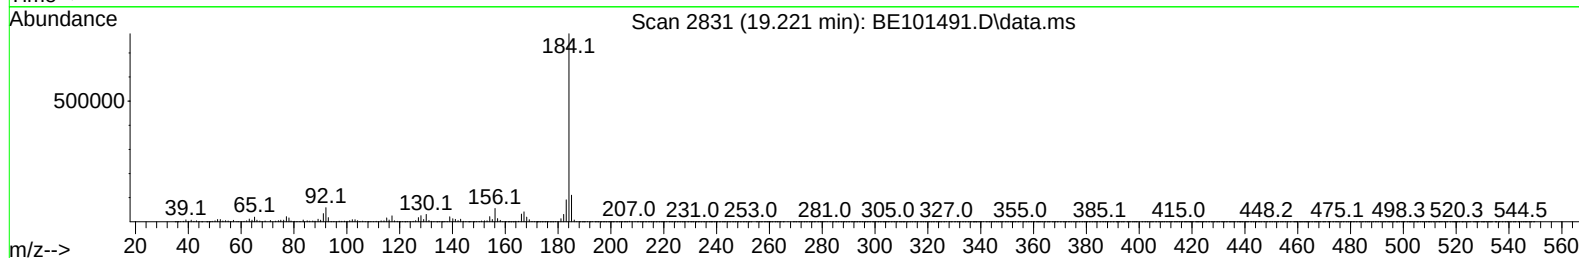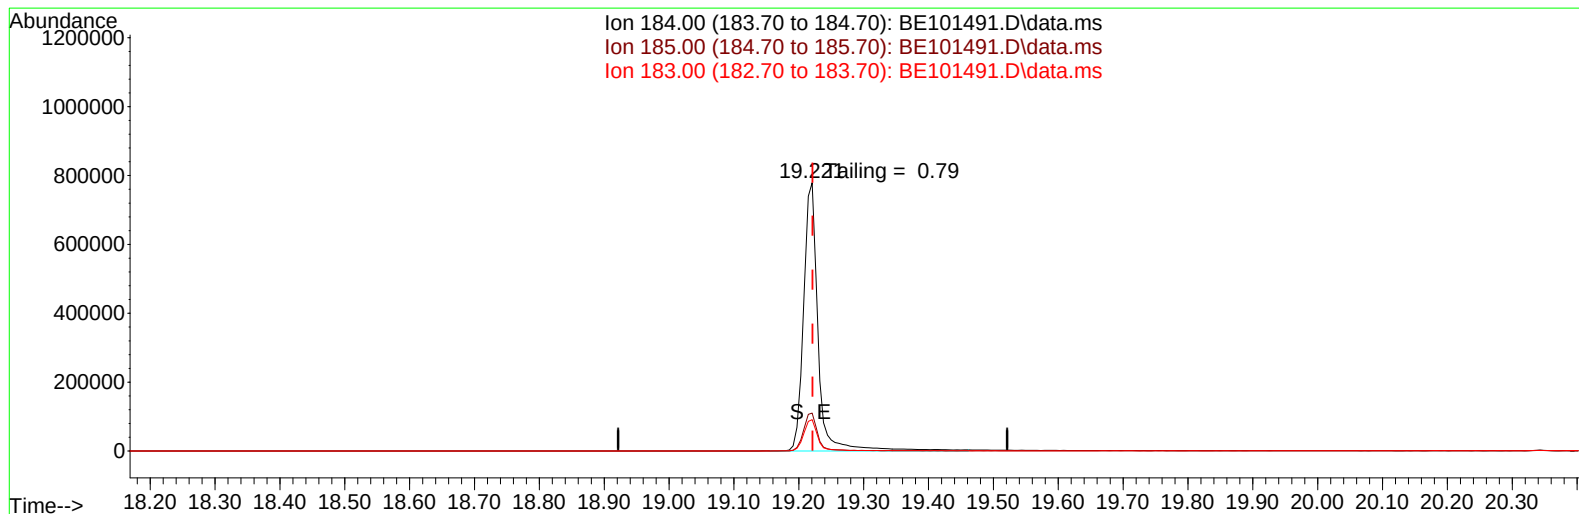

TIC: BE101491.D\data.ms

(77) Benzidine

19.221min (-0.001) 515869.86 ng

response 1191601

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	11.60	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/6/2024	BNA_E	<u>BE101491.D</u>
Compound Name	Response	Retention Time
DDT	583091	20.343
DDD	92284	19.914
DDE	1528	19.397
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
93812	676903	13.86

Instrument :
BNA_E
ClientSampleId :
DFTPP