
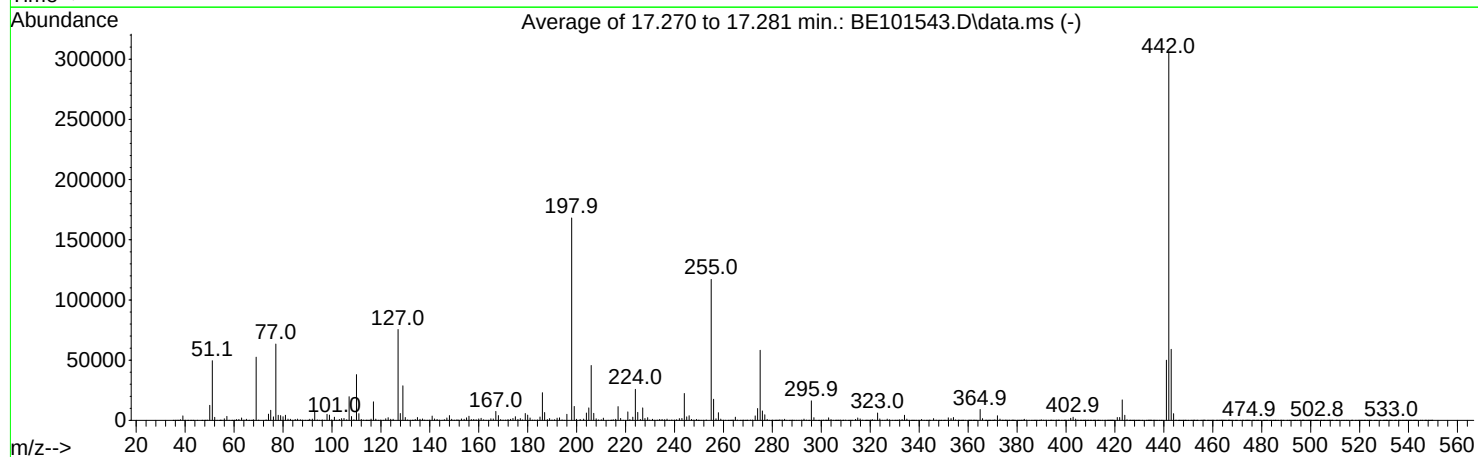


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101543.D
Acq On : 8 Nov 2024 9:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 00:01:20 2024

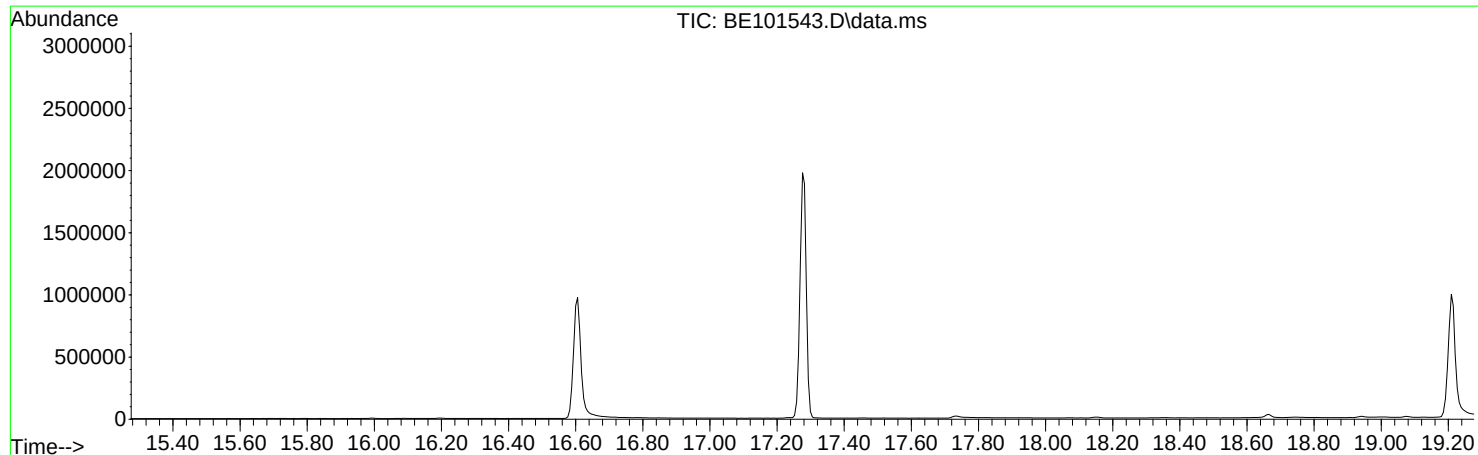

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	49550	PASS
68	69	0.00	2	1.0	549	PASS
69	198	0.00	100	31.3	52541	PASS
70	69	0.00	2	0.5	244	PASS
127	198	10	80	44.9	75486	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	168071	PASS
199	198	5	9	6.9	11633	PASS
275	198	10	60	34.7	58267	PASS
365	198	1	100	5.4	9101	PASS
441	198	0.01	100	29.7	49976	PASS
442	442	50	100	100.0	305553	PASS
443	442	15	24	19.3	58991	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/8/2024	BNA_E	<u>BE101543.D</u>
Compound Name	Response	Retention Time
DDT	773969	20.337
DDD	15959	19.955
DDE	485	19.391
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16444	790413	2.08

Instrument :
BNA_E
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101543.D
Acq On : 8 Nov 2024 9:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 08 10:13:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

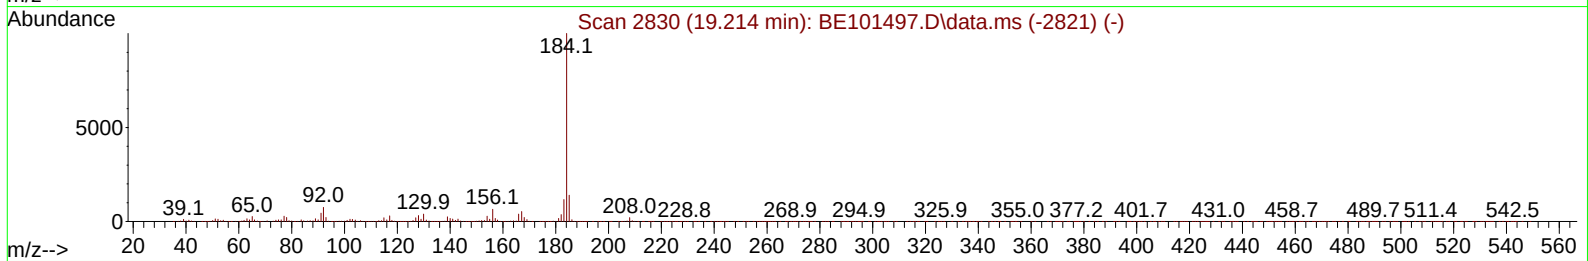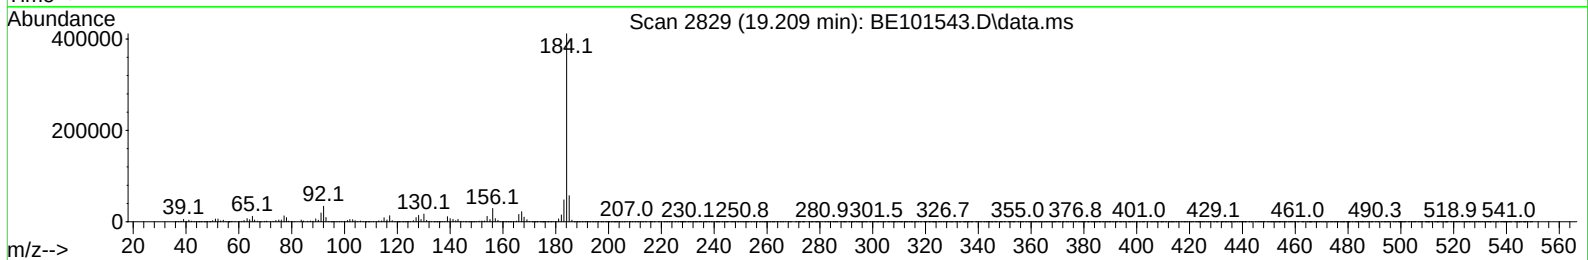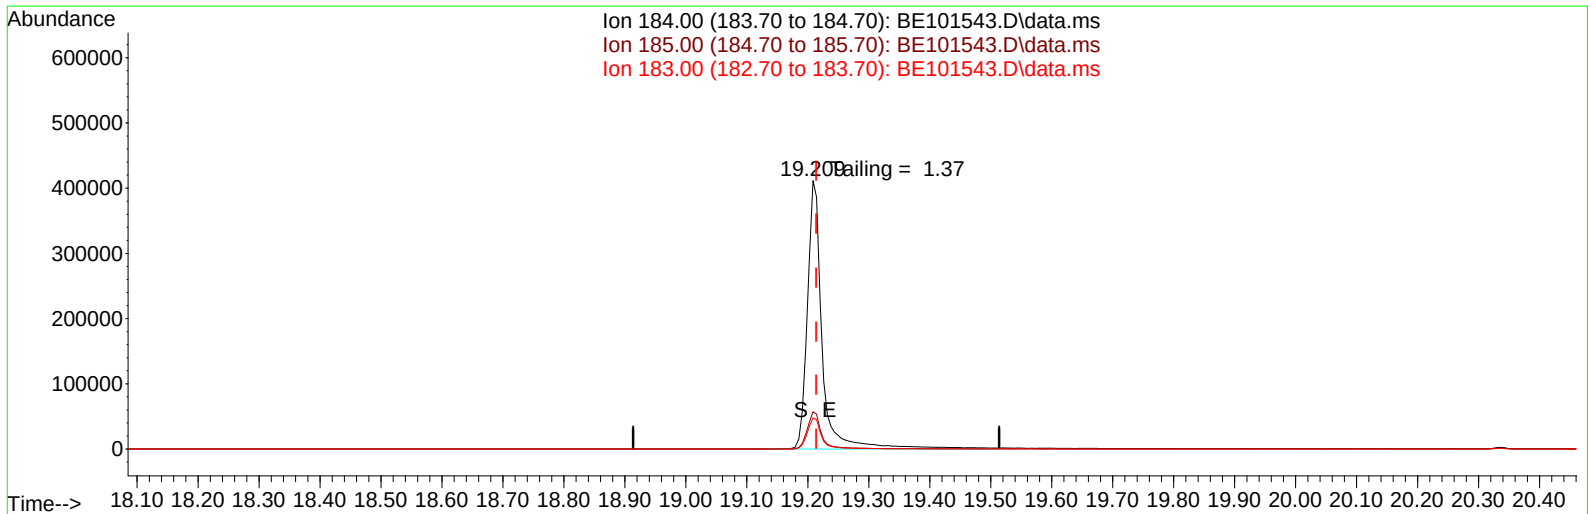

TIC: BE101543.D\data.ms

(77) Benzidine

19.209min (-0.005) 40480.74 ng

response 698261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.90
183.00	11.70	11.67
0.00	0.00	0.00