
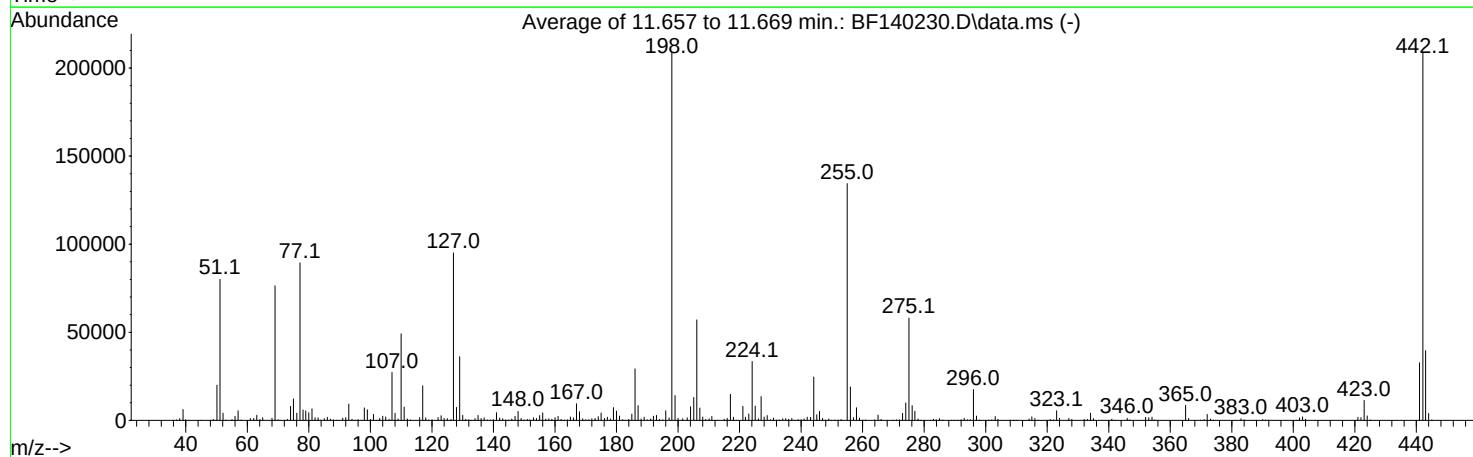


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110524\
Data File : BF140230.D
Acq On : 05 Nov 2024 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 05 16:47:56 2024

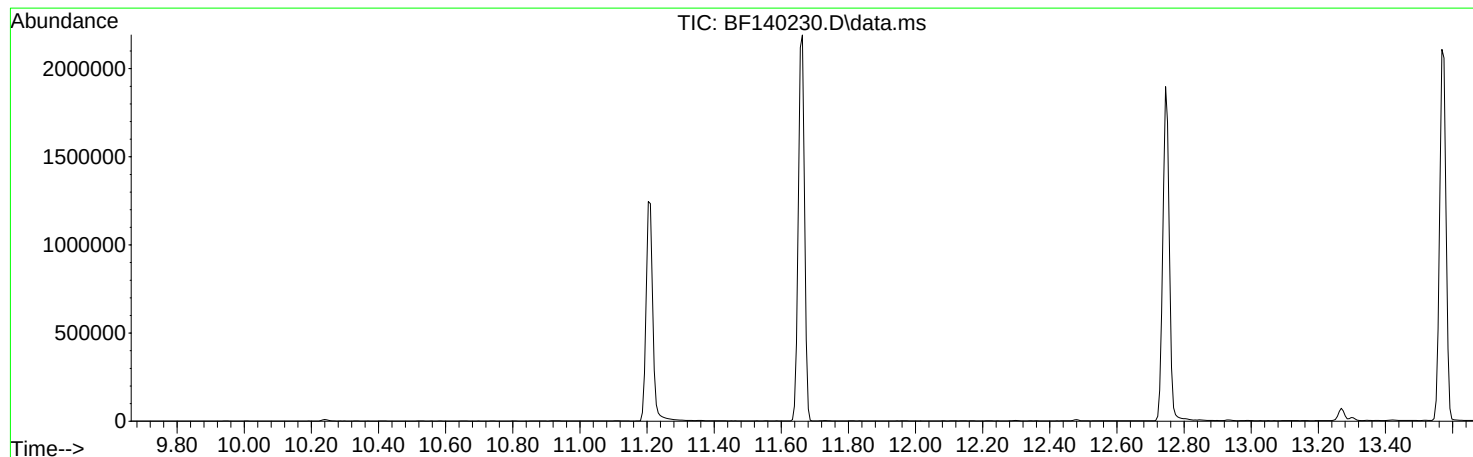




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	80133	PASS
68	69	0.00	2	1.6	1231	PASS
69	198	0.00	100	36.6	76347	PASS
70	69	0.00	2	0.5	377	PASS
127	198	10	80	45.6	95101	PASS
197	198	0.00	2	0.7	1410	PASS
198	198	100	100	100.0	208661	PASS
199	198	5	9	6.8	14126	PASS
275	198	10	60	27.8	58061	PASS
365	198	1	100	4.1	8531	PASS
441	198	0.01	100	15.7	32669	PASS
442	442	50	100	100.0	208811	PASS
443	442	15	24	19.0	39576	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110524\
Data File : BF140230.D
Acq On : 05 Nov 2024 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 05 12:57:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 17:12:57 2024
Response via : Initial Calibration

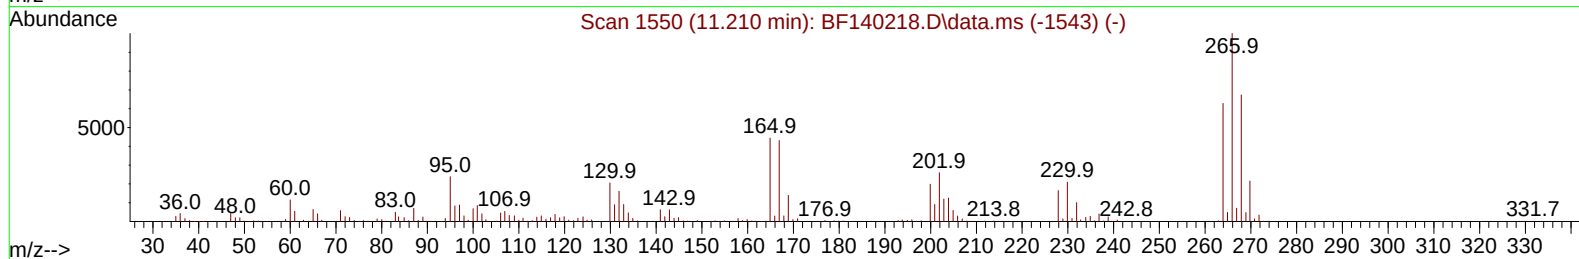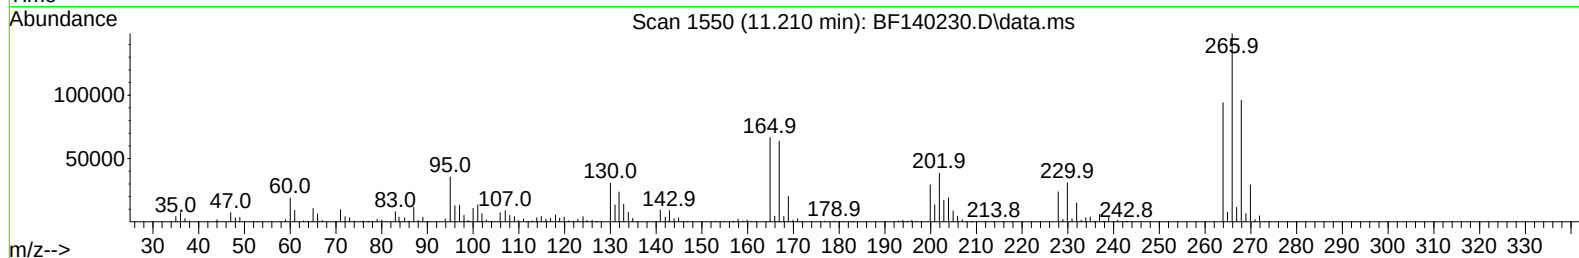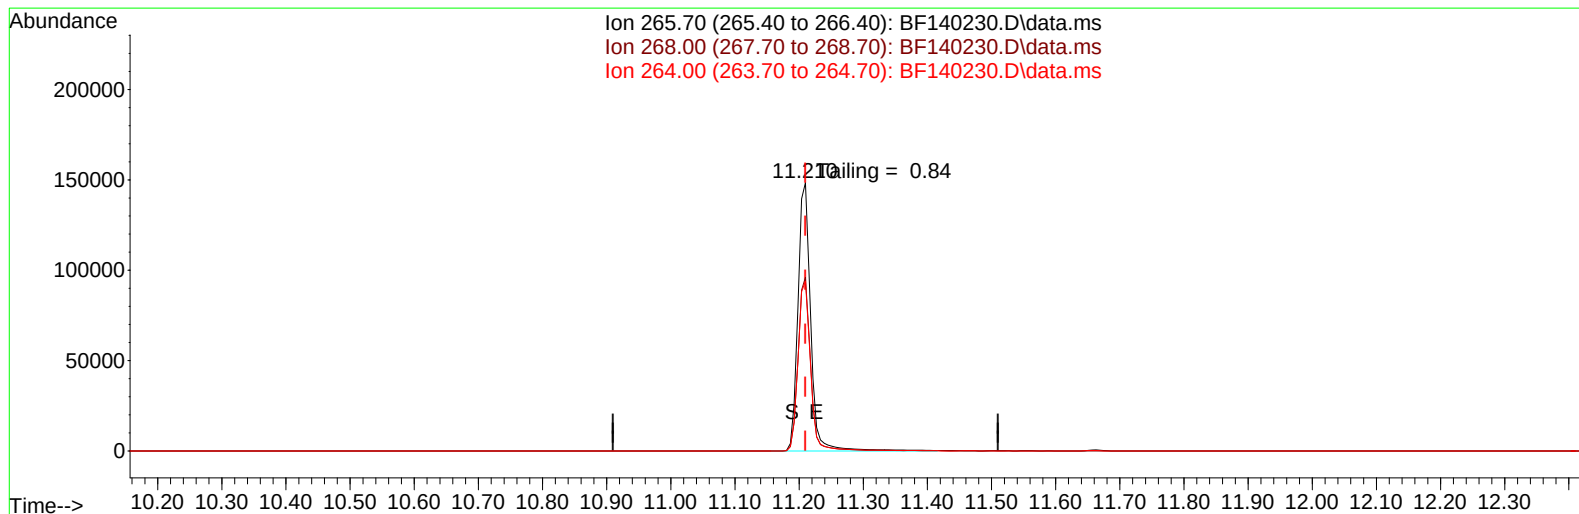

TIC: BF140230.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.000) 149686.01 ng




response 206677

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	64.67
264.00	62.90	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110524\
Data File : BF140230.D
Acq On : 05 Nov 2024 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 05 12:57:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 17:12:57 2024
Response via : Initial Calibration

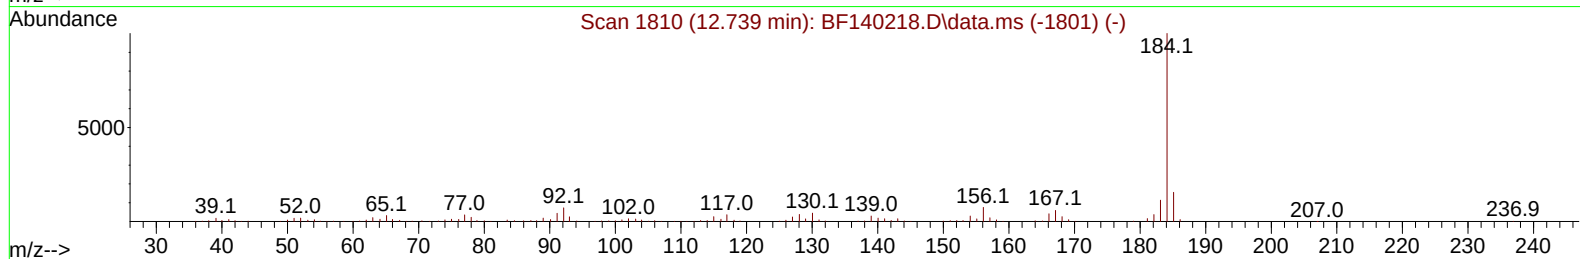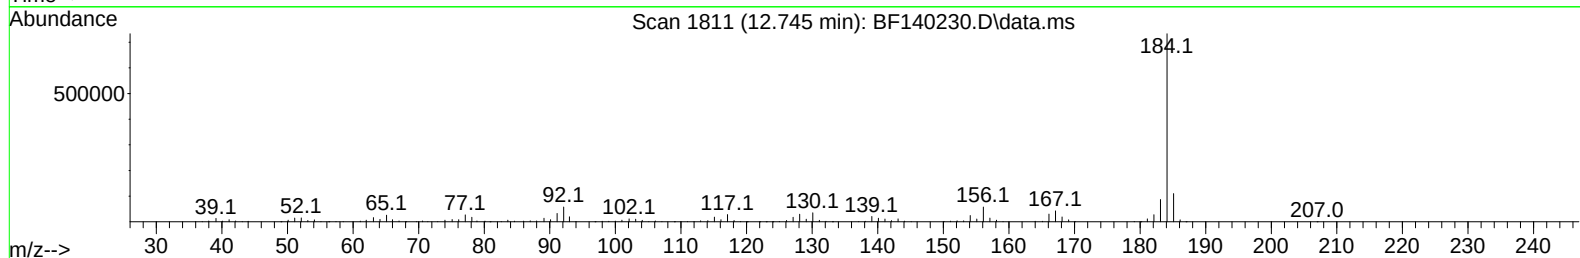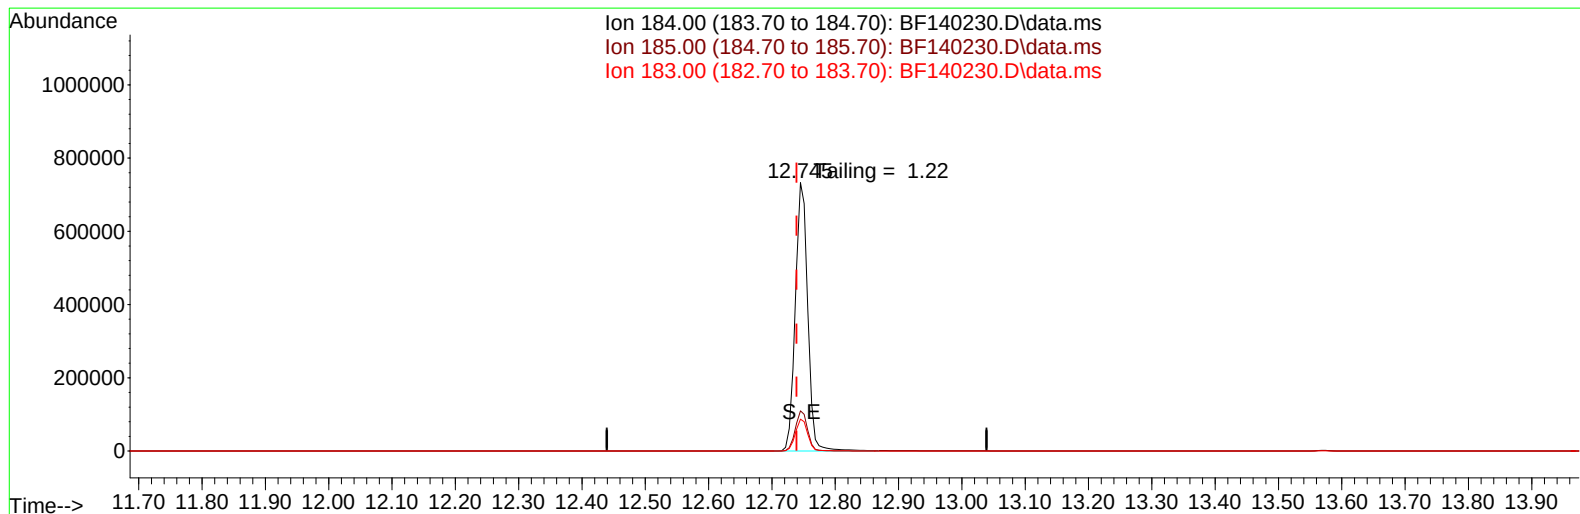

TIC: BF140230.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 305940.83 ng

response 1003011

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.97
183.00	11.30	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/5/2024	BNA_F	<u>BF140230.D</u>
Compound Name	Response	Retention Time
DDT	522863	13.574
DDD	21565	13.268
DDE	1336	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22901	545764	4.20

Instrument :
BNA_F
ClientSampleId :
DFTPP