
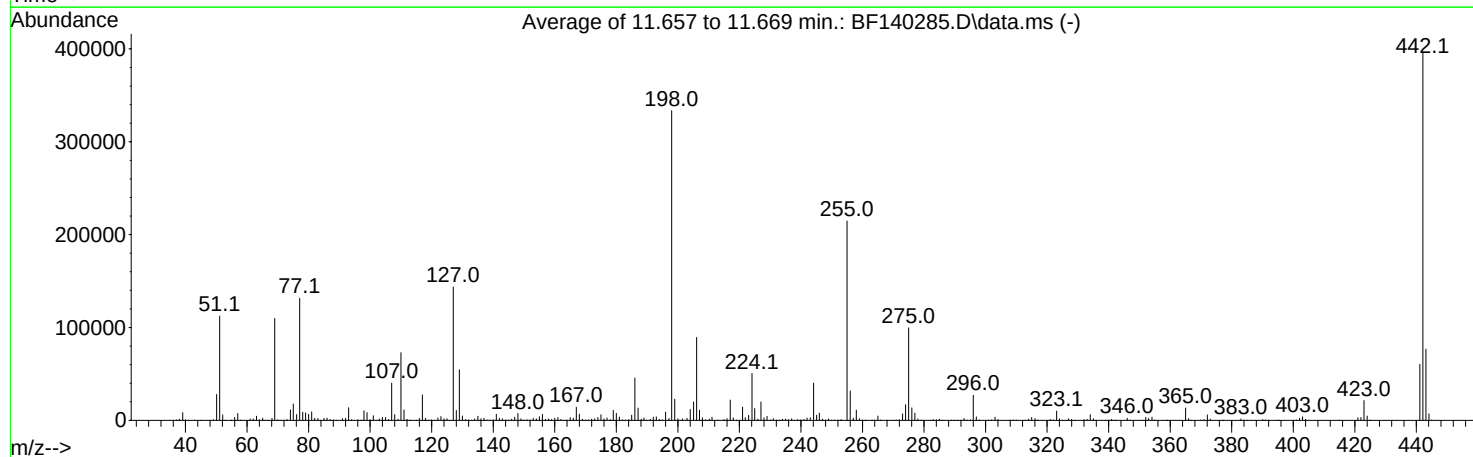


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110824\
Data File : BF140285.D
Acq On : 08 Nov 2024 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 05 16:47:56 2024

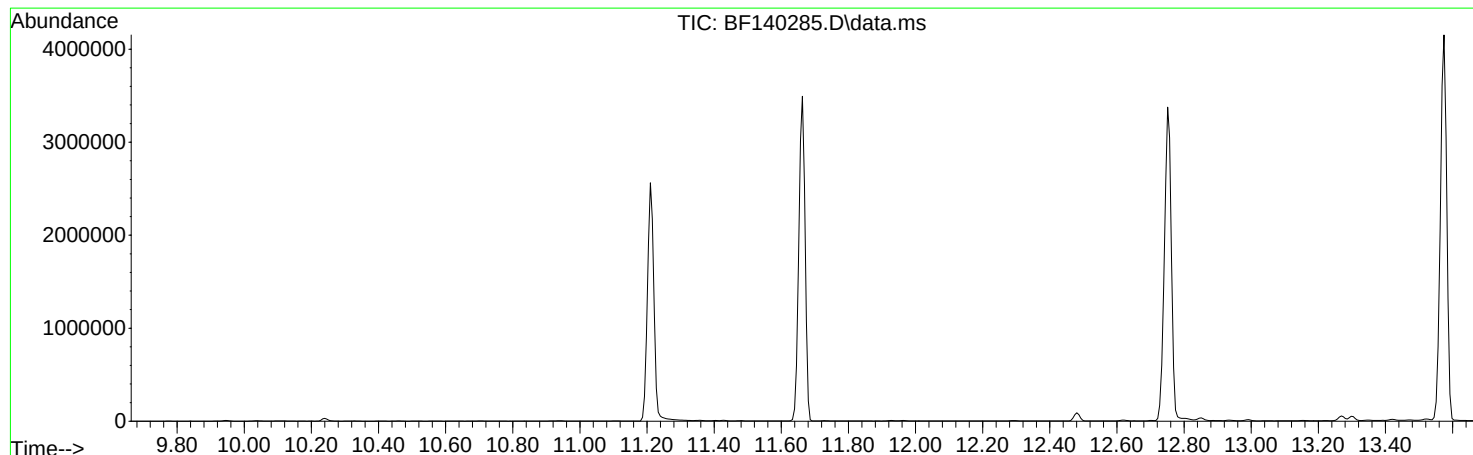

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	112429	PASS
68	69	0.00	2	2.0	2148	PASS
69	198	0.00	100	32.9	109765	PASS
70	69	0.00	2	0.6	648	PASS
127	198	10	80	43.1	143768	PASS
197	198	0.00	2	0.6	2149	PASS
198	198	100	100	100.0	333589	PASS
199	198	5	9	6.8	22803	PASS
275	198	10	60	29.9	99640	PASS
365	198	1	100	4.0	13268	PASS
441	198	0.01	100	18.1	60392	PASS
442	442	50	100	100.0	396117	PASS
443	442	15	24	19.4	76731	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/8/2024	BNA_F	<u>BF140285.D</u>
Compound Name	Response	Retention Time
DDT	1118785	13.575
DDD	23060	13.269
DDE	1849	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24909	1143694	2.18

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110824\
Data File : BF140285.D
Acq On : 08 Nov 2024 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 08 10:16:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 16:47:56 2024
Response via : Initial Calibration

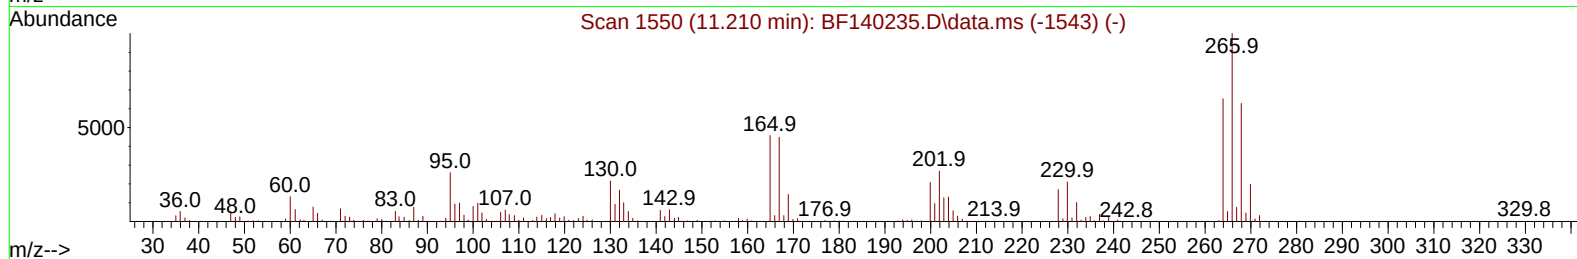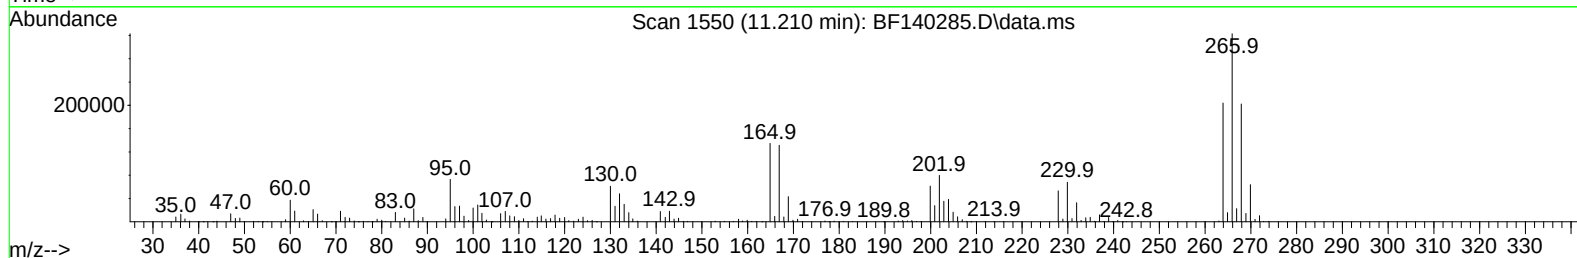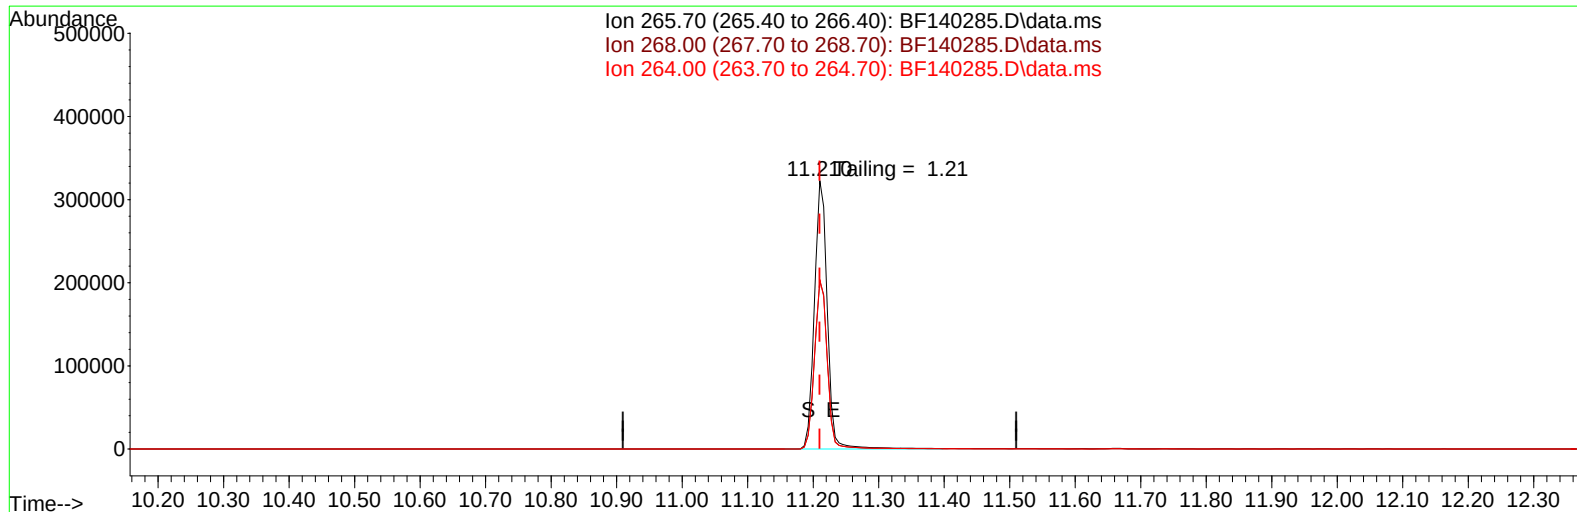

TIC: BF140285.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.000) 32243.25 ng




response 440973

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.68
264.00	65.30	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110824\
Data File : BF140285.D
Acq On : 08 Nov 2024 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 08 10:16:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 16:47:56 2024
Response via : Initial Calibration

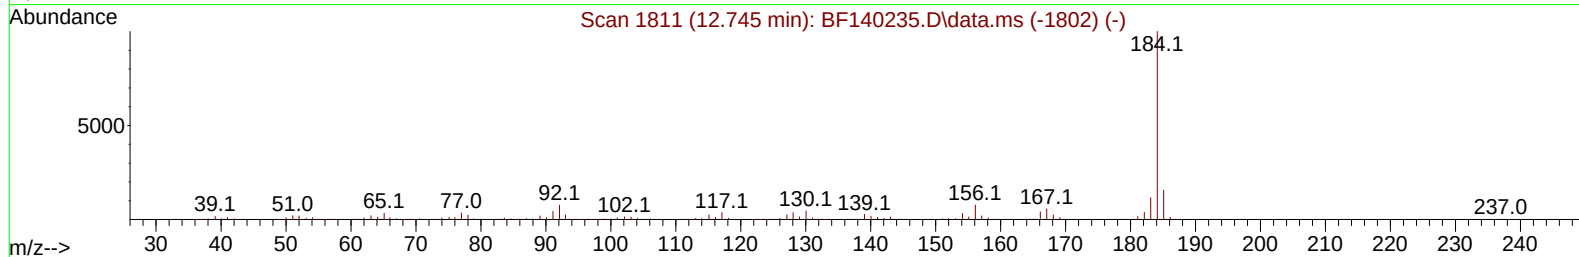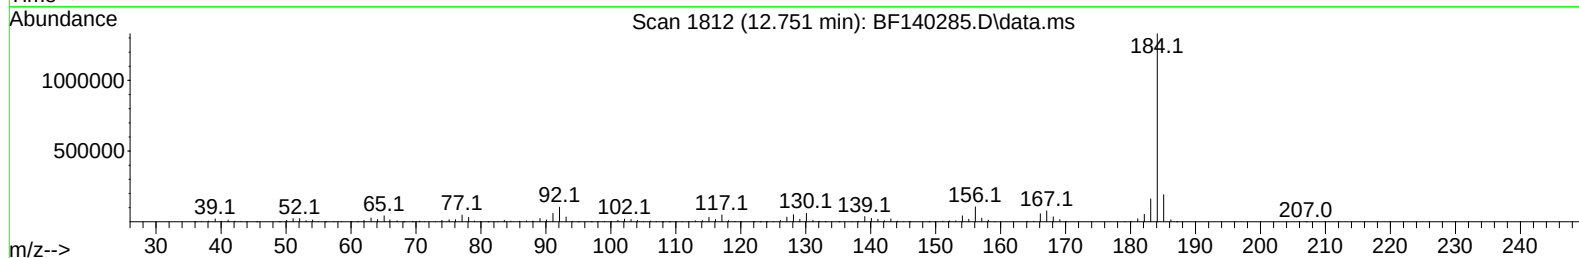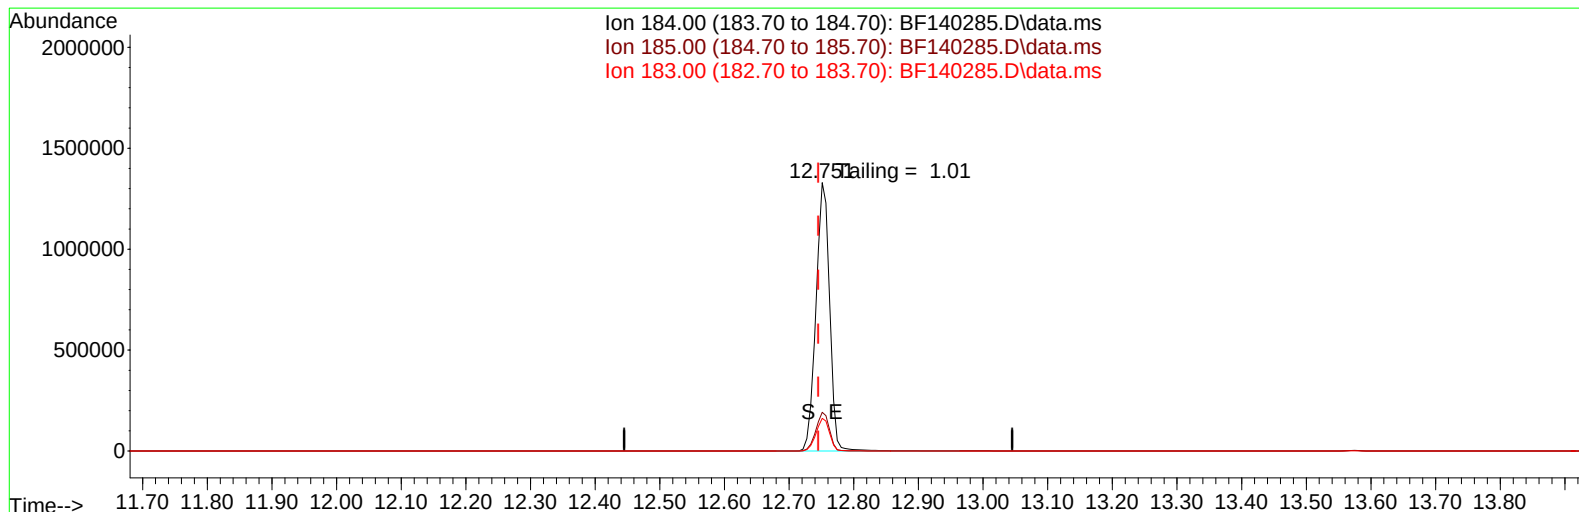

TIC: BF140285.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 52057.10 ng

response 1958264

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.44
183.00	11.60	12.17
0.00	0.00	0.00