
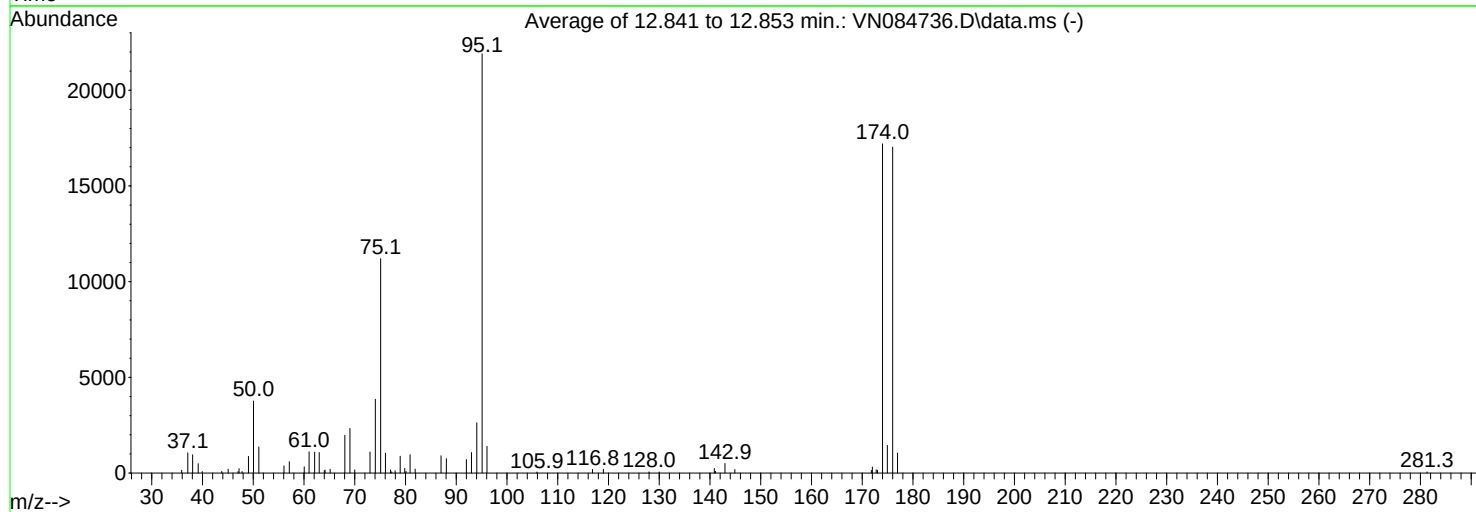


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN110824\
Data File : VN084736.D
Acq On : 08 Nov 2024 08:18
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

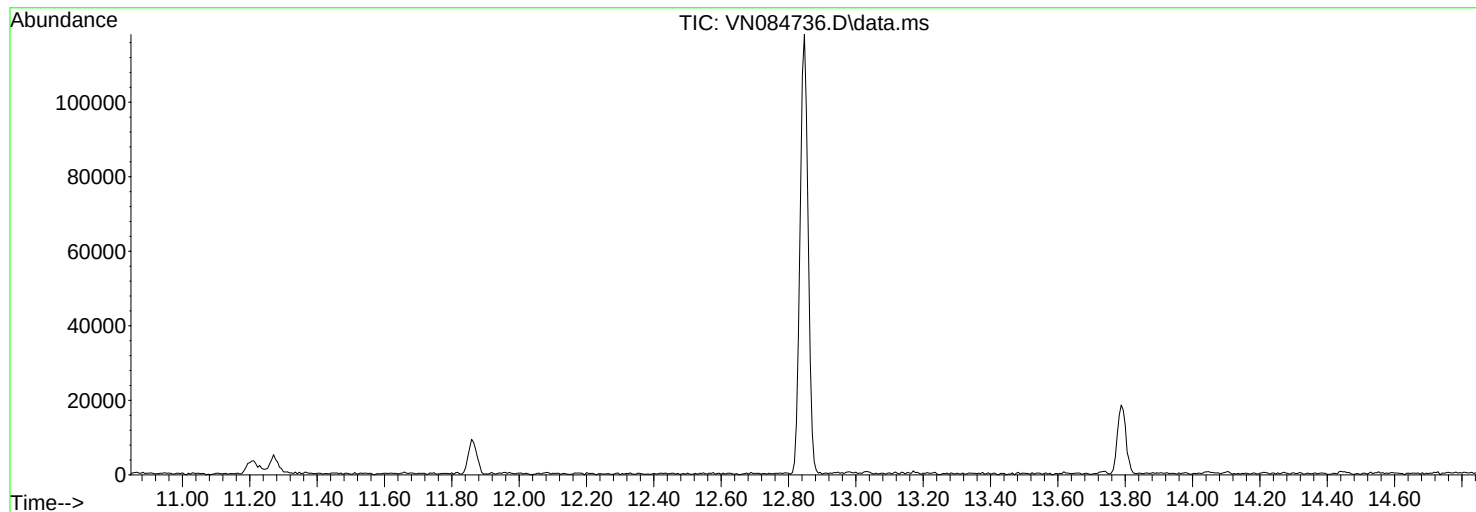

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	3766	PASS
75	95	30	60	51.1	11200	PASS
95	95	100	100	100.0	21907	PASS
96	95	5	9	6.4	1400	PASS
173	174	0.00	2	1.0	167	PASS
174	95	50	100	78.5	17202	PASS
175	174	5	9	8.4	1446	PASS
176	174	95	101	99.0	17029	PASS
177	176	5	9	6.2	1049	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	152	50.05	3766	68.05	1978	79.85	245
37.10	1056	51.10	1363	69.05	2331	80.10	89
38.05	955	56.05	374	70.00	167	80.90	960
39.15	491	57.10	594	73.00	1101	81.90	207
39.95	77	60.05	328	74.05	3860	87.00	906
43.80	85	61.00	1111	75.10	11200	88.05	752
45.05	203	62.10	1093	76.05	1043	92.00	705
47.00	80	63.00	1076	77.05	166	93.00	1070
47.20	234	64.00	129	77.30	62	94.05	2629
47.80	83	64.15	159	77.95	125	95.10	21907
49.05	872	65.15	200	78.95	880	96.05	1400

Average of 12.841 to 12.853 min.: VN084736.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.90	54	172.75	167				
116.85	190	173.00	149				
119.00	190	174.00	17202				
128.00	64	174.95	1446				
130.00	60	176.00	17029				
140.85	244	176.95	1049				
141.10	90	281.30	62				
142.95	505						
144.90	188						
171.80	144						
172.00	318						

Instrument :

MSVOA_N

ClientSampleId :

BFB