
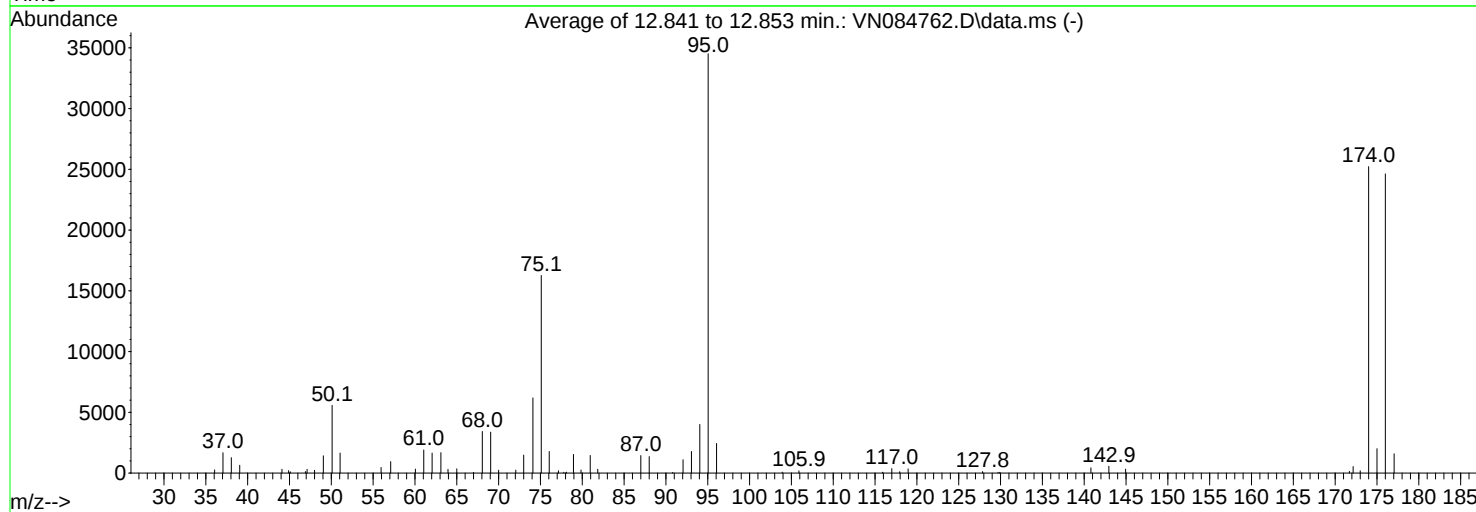


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111124\
Data File : VN084762.D
Acq On : 11 Nov 2024 10:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

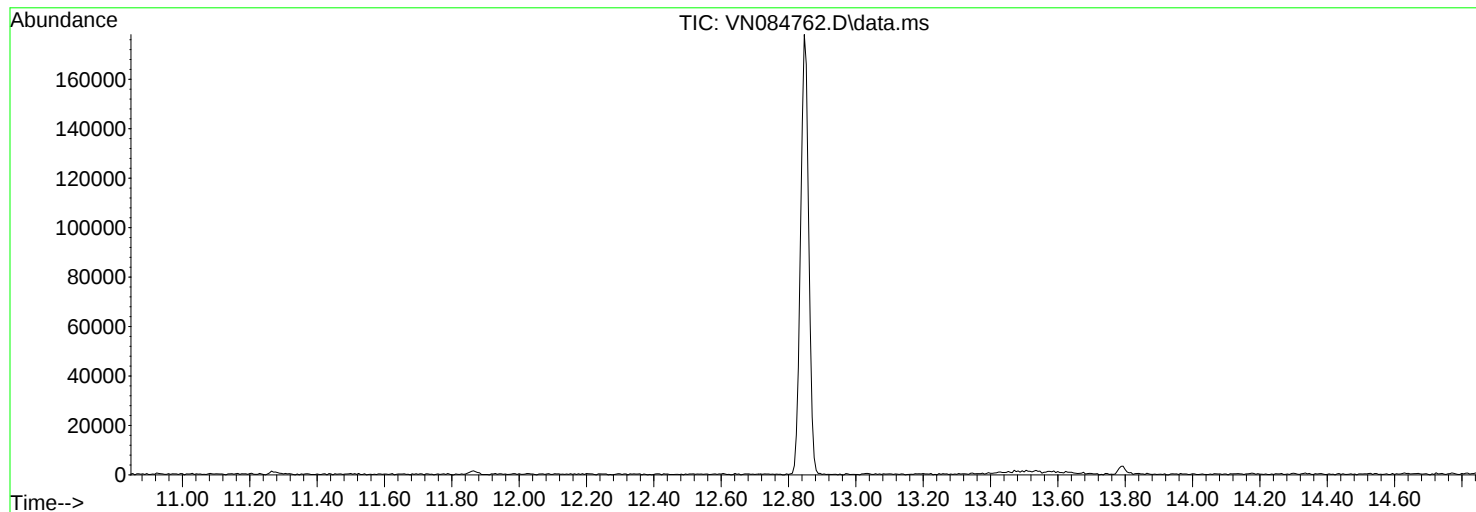

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	5574	PASS
75	95	30	60	47.1	16266	PASS
95	95	100	100	100.0	34517	PASS
96	95	5	9	7.1	2436	PASS
173	174	0.00	2	0.8	191	PASS
174	95	50	100	73.1	25224	PASS
175	174	5	9	8.0	2010	PASS
176	174	95	101	97.6	24629	PASS
177	176	5	9	6.5	1591	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	262	50.10	5574	68.05	3426	78.95	1533
37.05	1676	51.05	1650	69.05	3373	79.85	253
38.05	1270	55.95	465	70.00	243	80.95	1453
39.05	643	57.10	946	72.05	244	81.85	318
44.10	312	60.05	328	73.00	1483	87.00	1445
44.90	200	61.05	1903	74.10	6188	88.00	1360
45.10	102	62.05	1647	75.10	16266	90.80	52
46.90	129	63.10	1682	76.05	1778	92.05	1105
47.10	313	63.95	309	77.15	189	93.05	1781
48.00	231	65.00	350	77.80	69	94.05	4004
49.05	1425	67.00	61	78.10	79	95.05	34517

Average of 12.841 to 12.853 min.: VN084762.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	2436	142.95	566				
103.90	79	144.95	325				
105.90	184	171.70	144				
115.90	77	172.15	536				
117.00	372	173.00	191				
117.95	114	174.00	25224				
118.95	342	175.00	2010				
127.85	127	176.00	24629				
129.70	59	177.05	1591				
129.90	59						
140.80	431						

Instrument :

MSVOA_N

ClientSampleId :

BFB