

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
 Data File : BE101493.D
 Acq On : 6 Nov 2024 13:51
 Operator : RC/JU
 Sample : SSTDICC2.5
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC2.5

Quant Time: Nov 06 23:14:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 06 23:10:33 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.566	152	55140	20.000	ng	0.00	
21) Naphthalene-d8	10.333	136	244662	20.000	ng	0.00	
39) Acenaphthene-d10	14.176	164	174059	20.000	ng	0.00	
64) Phenanthrene-d10	16.908	188	418467	20.000	ng	0.00	
76) Chrysene-d12	21.074	240	553680	20.000	ng	0.00	
86) Perylene-d12	23.359	264	716356	20.000	ng	0.00	
System Monitoring Compounds							
5) 2-Fluorophenol	0.000	112	0d	0.000	ng		
7) Phenol-d6	0.000	99	0d	0.000	ng		
23) Nitrobenzene-d5	0.000	82	0d	0.000	ng		
42) 2,4,6-Tribromophenol	0.000	330	0d	0.000	ng		
45) 2-Fluorobiphenyl	0.000	172	0d	0.000	ng		
79) Terphenyl-d14	0.000	244	0d	0.000	ng		
Target Compounds							
19) n-Nitroso-di-n-propyla...	8.371	70	6602	2.281	ng		Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
 Data File : BE101493.D
 Acq On : 6 Nov 2024 13:51
 Operator : RC/JU
 Sample : SSTDICC2.5
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC2.5

Quant Time: Nov 06 23:14:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 06 23:10:33 2024
 Response via : Initial Calibration

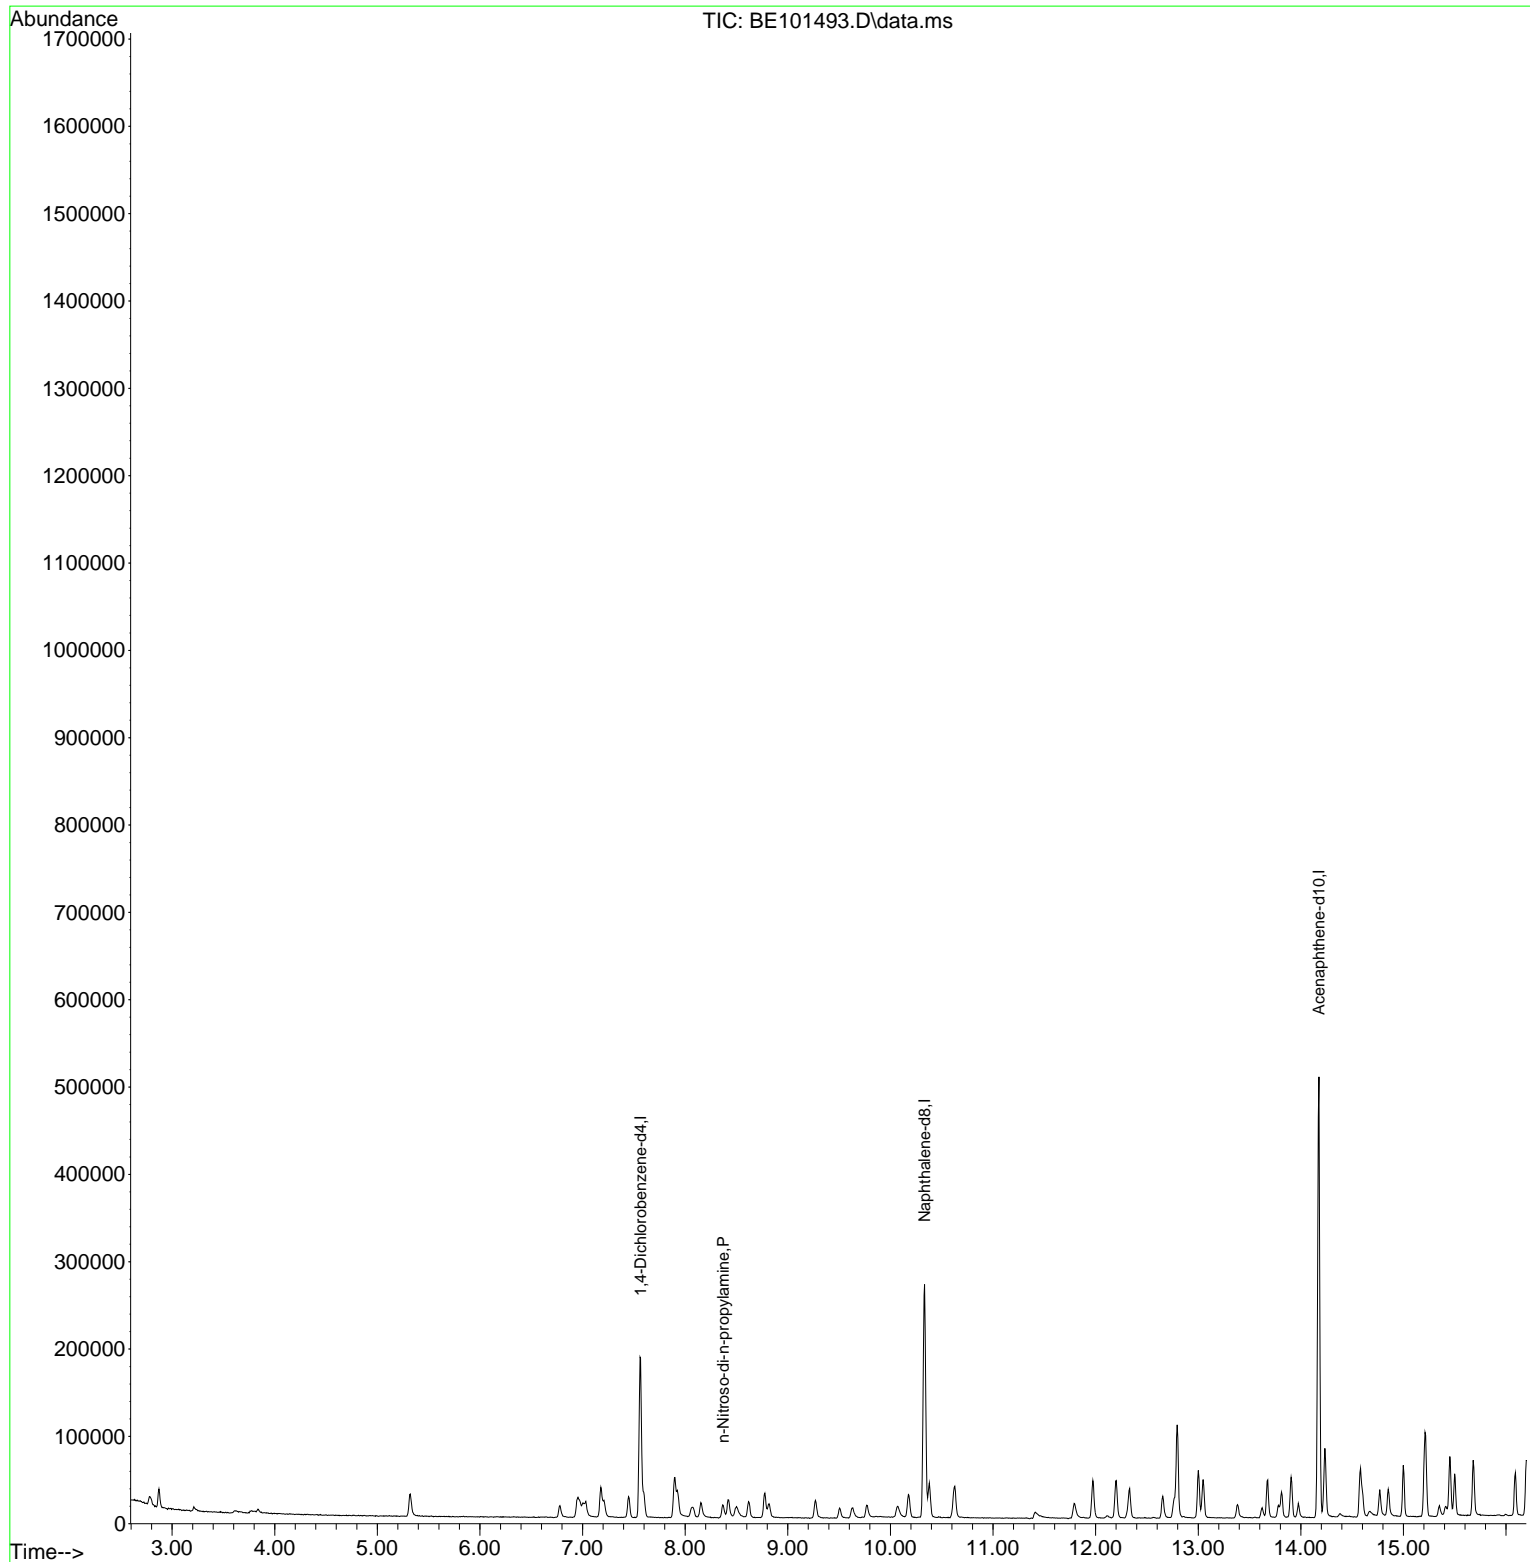

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
 Data File : BE101493.D
 Acq On : 6 Nov 2024 13:51
 Operator : RC/JU
 Sample : SSTDICC2.5
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC2.5

Quant Time: Nov 06 23:14:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 06 23:10:33 2024
 Response via : Initial Calibration

