


LB133402

7471B

INSTRUMENT ID: CV1

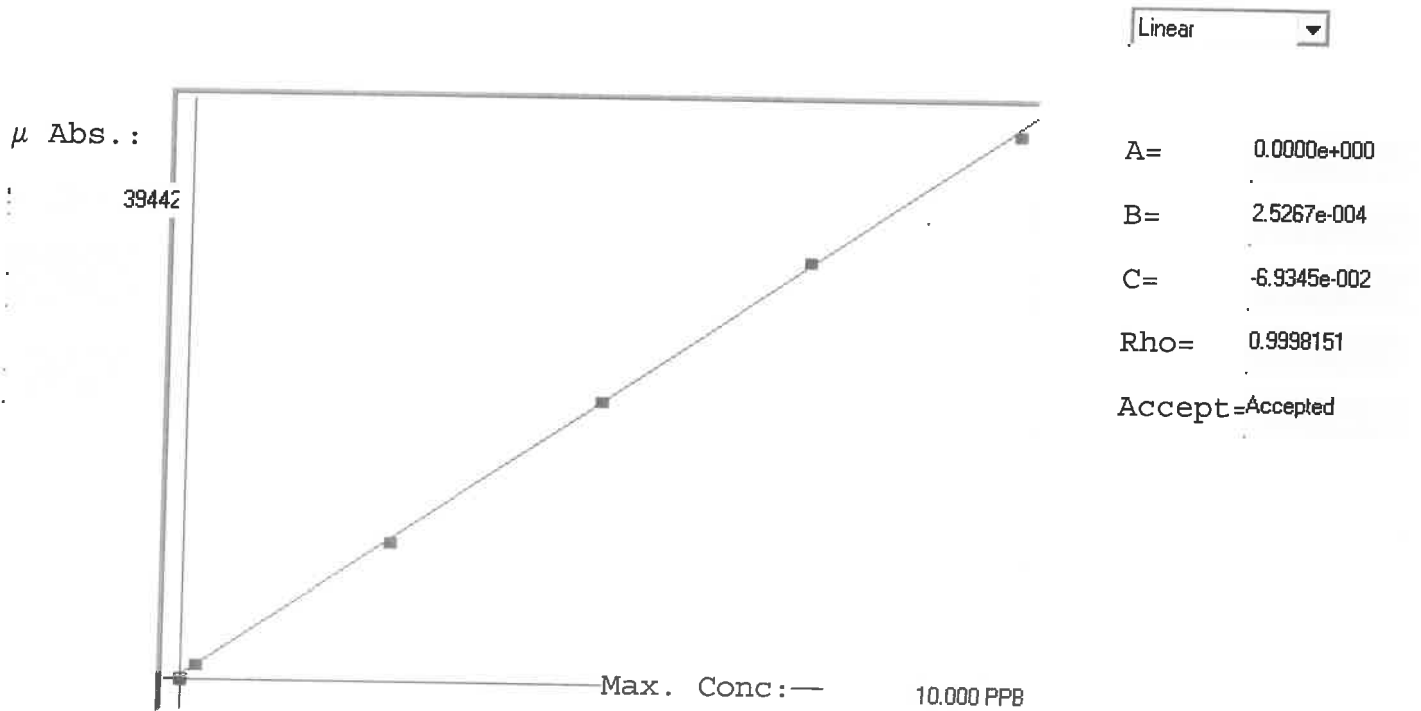

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.061	-0.061	32	0.000	32					
0.2	0.200	0.231	0.031	1190	0.0 %	1190					16
2.5	2.500	2.479	-0.021	10085	0.0 %	10085					1
5.0	5.000	5.043	0.043	20234	0.0 %	20234					1
7.5	7.500	7.612	0.112	30399	0.0 %	30399					1
10.0	10.000	9.896	-0.104	39442	0.0 %	39442					1

LB133402 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 12 Nov 2024 10:26:25

Sample ID	Extended ID	µ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	SD	32	-	0.0000	7471B	PPB	12 Nov 2024 10:39:43	S	Std
0.2 - 1	SD	1190	-	0.2000	7471B	PPB	12 Nov 2024 10:42:00	S	Std
2.5 - 1	SD	10085	-	2.5000	7471B	PPB	12 Nov 2024 10:44:16	S	Std
5.0 - 1	SD	20234	-	5.0000	7471B	PPB	12 Nov 2024 10:50:07	S	Std
7.5 - 1	SD	30399	-	7.5000	7471B	PPB	12 Nov 2024 10:52:23	S	Std
10.0 - 1	SD	39442	-	10.0000	7471B	PPB	12 Nov 2024 10:57:27	S	Std
ICV82 - 1	ICV82	15394	3.8202	-	7471B	PPB	12 Nov 2024 11:00:36	U	SMPL
ICB82 - 1	ICB82	-16	-0.0734	-	7471B	PPB	12 Nov 2024 11:06:58	U	SMPL
CCV71 - 1	CCV71	19670	4.9007	-	7471B	PPB	12 Nov 2024 11:09:15	U	SMPL
CCB71 - 1	CCB71	167	-0.0271	-	7471B	PPB	12 Nov 2024 11:11:30	U	SMPL
CRA - 1	CRA	1103	0.2093	-	7471B	PPB	12 Nov 2024 11:13:47	U	SMPL
HighStd - 1	HighStd	38731	9.7168	-	7471B	PPB	12 Nov 2024 11:16:02	U	SMPL
ChkStd - 1	ChkStd	26357	6.5902	-	7471B	PPB	12 Nov 2024 11:18:17	U	SMPL
PB164891BS - 1	PB164891BS	18344	4.5656	-	7471B	PPB	12 Nov 2024 11:22:58	U	SMPL
P4756-01 - 1	BP-B4	15422	3.8273	-	7471B	PPB	12 Nov 2024 11:25:15	U	SMPL
P4768-01 - 1	B-3-1	1423	0.2902	-	7471B	PPB	12 Nov 2024 11:27:33	U	SMPL
P4768-02 - 1	B-3-2	8931	2.1872	-	7471B	PPB	12 Nov 2024 11:29:53	U	SMPL
P4768-03 - 1	B-3-3	1278	0.2536	-	7471B	PPB	12 Nov 2024 11:32:11	U	SMPL
P4768-04 - 1	B-4	17900	4.4534	-	7471B	PPB	12 Nov 2024 11:34:28	U	SMPL
PB164891BL - 1	PB164891BL	102	-0.0436	-	7471B	PPB	12 Nov 2024 11:36:58	U	SMPL
PB164891BS - 1	PB164891BS	0	-0.0693	-	7471B	PPB	12 Nov 2024 11:39:16	U	SMPL
CCV72 - 1	CCV72	20226	5.0411	-	7471B	PPB	12 Nov 2024 11:39:41	U	SMPL
CCB72 - 1	CCB72	20	-0.0643	-	7471B	PPB	12 Nov 2024 11:41:55	U	SMPL
P4768-05 - 1	B-5	547	0.0689	-	7471B	PPB	12 Nov 2024 11:44:13	U	SMPL
P4768-06 - 1	B-6-2	33978	8.5158	-	7471B	PPB	12 Nov 2024 11:46:28	U	SMPL
P4768-07 - 1	B-6-3	209	-0.0165	-	7471B	PPB	12 Nov 2024 11:48:44	U	SMPL
P4768-07DUP - 1	B-6-3DUP	465	0.0481	-	7471B	PPB	12 Nov 2024 11:51:03	U	SMPL
P4768-07MS - 1	B-6-3MS	16509	4.1020	-	7471B	PPB	12 Nov 2024 11:55:56	U	SMPL
P4768-07MSD - 1	B-6-3MSD	16295	4.0479	-	7471B	PPB	12 Nov 2024 11:58:12	U	SMPL
P4771-05 - 1	P-1	481	0.0522	-	7471B	PPB	12 Nov 2024 12:00:32	U	SMPL
P4771-07 - 1	P-2	486	0.0535	-	7471B	PPB	12 Nov 2024 12:02:50	U	SMPL
P4788-01 - 1	BP-G3	420	0.0368	-	7471B	PPB	12 Nov 2024 12:05:07	U	SMPL
P4789-01 - 1	BP-F21	711	0.1103	-	7471B	PPB	12 Nov 2024 12:07:23	U	SMPL
CCV73 - 1	CCV73	20405	5.0864	-	7471B	PPB	12 Nov 2024 12:09:38	U	SMPL
CCB73 - 1	CCB73	167	-0.0271	-	7471B	PPB	12 Nov 2024 12:11:53	U	SMPL
P4792-03 - 1	OILY-STONE-DRUM	778	0.1267	-	7471B	PPB	12 Nov 2024 12:14:12	U	SMPL
P4793-01 - 1	M00-24-00345	2395	0.5358	-	7471B	PPB	12 Nov 2024 12:16:27	U	SMPL
P4795-01 - 1	LAW-23-00189	4521	1.0730	-	7471B	PPB	12 Nov 2024 12:18:42	U	SMPL
P4796-01 - 1	TP-1	1185	0.2301	-	7471B	PPB	12 Nov 2024 12:20:58	U	SMPL
P4796-03 - 1	TP-2	629	0.0896	-	7471B	PPB	12 Nov 2024 12:23:15	U	SMPL
P4796-05 - 1	TP-3	1183	0.2296	-	7471B	PPB	12 Nov 2024 12:25:31	U	SMPL
P4796-07 - 1	TP-4	879	0.1528	-	7471B	PPB	12 Nov 2024 12:27:47	U	SMPL
P4798-01 - 1	MH-6	25839	6.4594	-	7471B	PPB	12 Nov 2024 12:30:04	U	SMPL
P4768-07LX5 - 1		-157	-0.1090	-	7471B	PPB	12 Nov 2024 12:32:20	U	SMPL
P4768-07A - 1		20105	5.0106	-	7471B	PPB	12 Nov 2024 12:34:38	U	SMPL
CCV74 - 1	CCV74	20945	5.2228	-	7471B	PPB	12 Nov 2024 12:36:54	U	SMPL
CCB74 - 1	CCB74	151	-0.0312	-	7471B	PPB	12 Nov 2024 12:39:11	U	SMPL