

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110824\
 Data File : PO107818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2024 17:10
 Operator : YP/AJ
 Sample : P4768-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-6-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :Ankita Jodhani 11/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 01:39:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.641	233.8E6	78694372	25.657m	24.451m
2) SA Decachlor...	10.081	8.638	55016906	55450924	22.425	20.226

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110824\
Data File : PO107818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2024 17:10
Operator : YP/AJ
Sample : P4768-06
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B-6-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :Ankita Jodhani 11/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 01:39:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

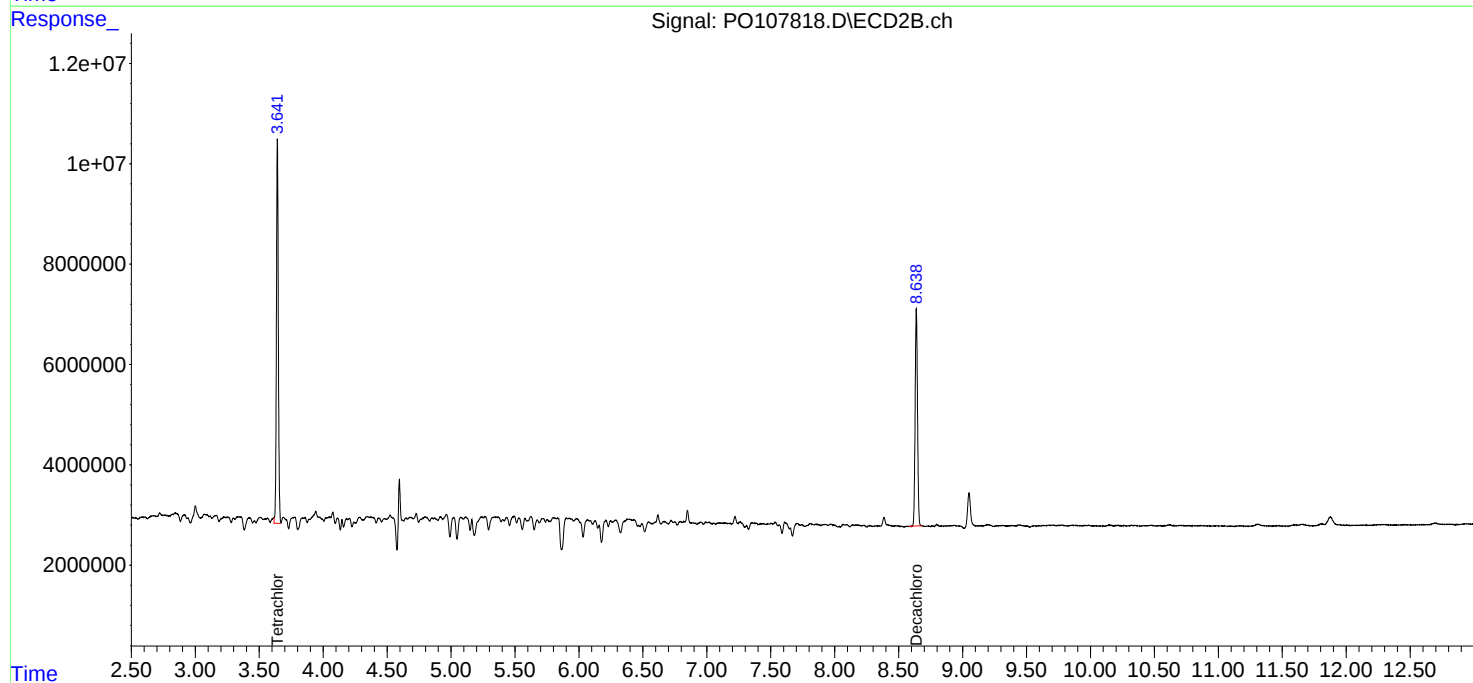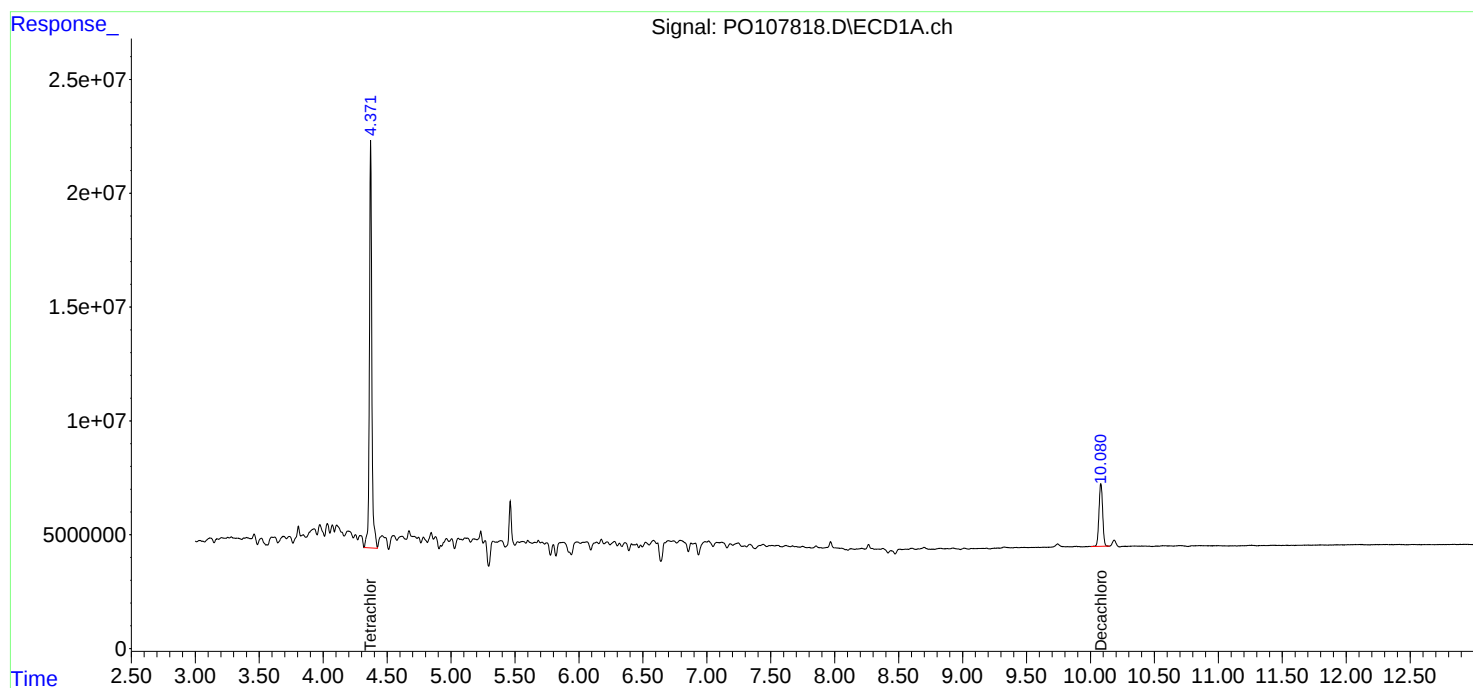

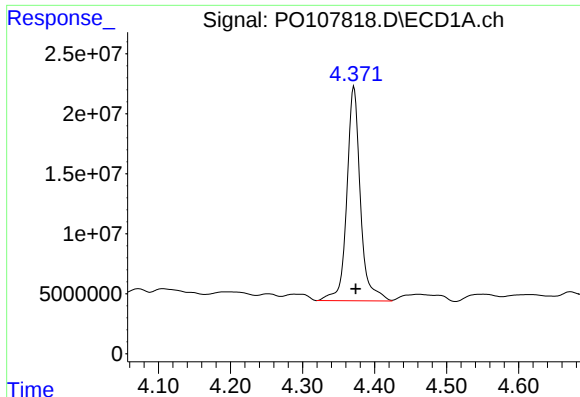

#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 233834870
Conc: 25.66 ng/ml

Instrument :

ECD_O


ClientSampleId :

B-6-2

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :Ankita Jodhani 11/11/2024

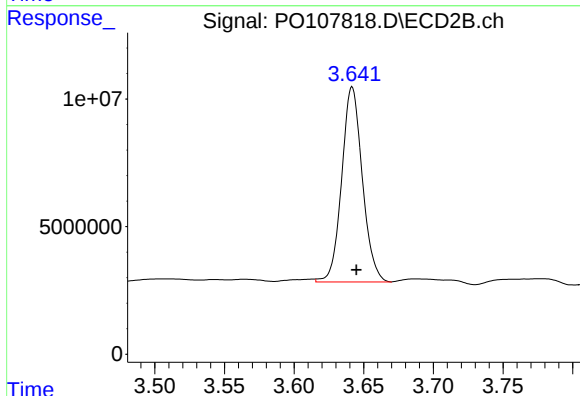


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: -0.003 min
Response: 78694372
Conc: 24.45 ng/ml m

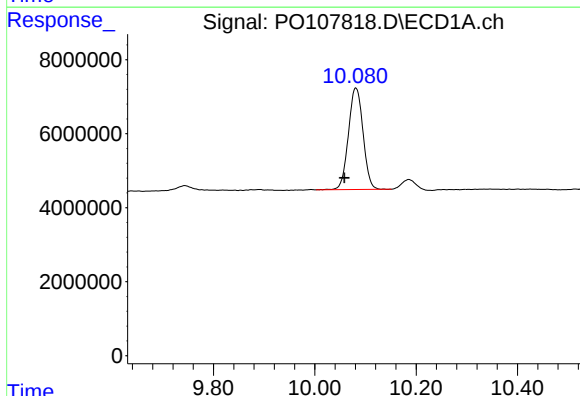

#2 Decachlorobiphenyl

R.T.: 10.081 min
Delta R.T.: 0.023 min
Response: 55016906
Conc: 22.42 ng/ml

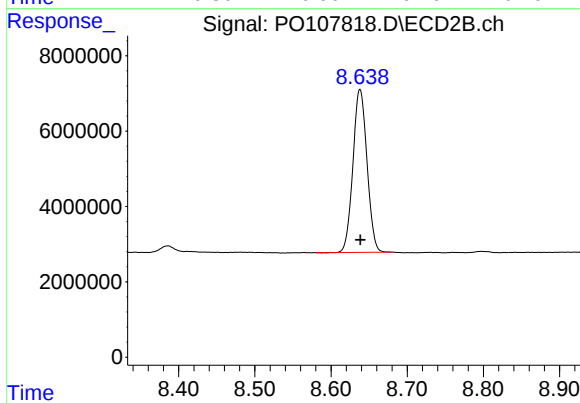

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 55450924
Conc: 20.23 ng/ml