
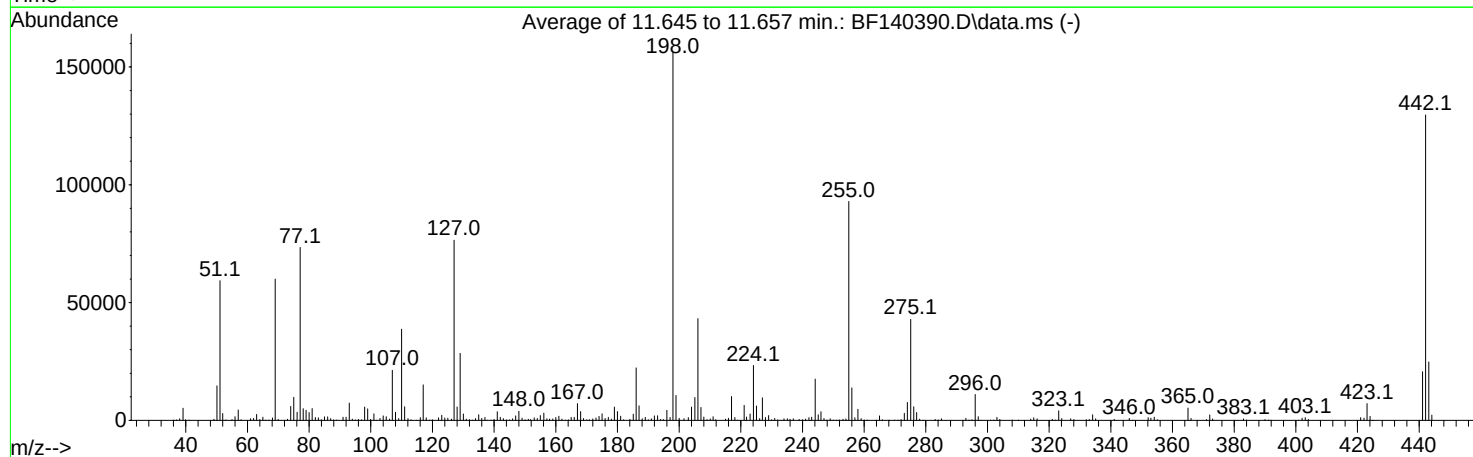


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111524\
Data File : BF140390.D
Acq On : 15 Nov 2024 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

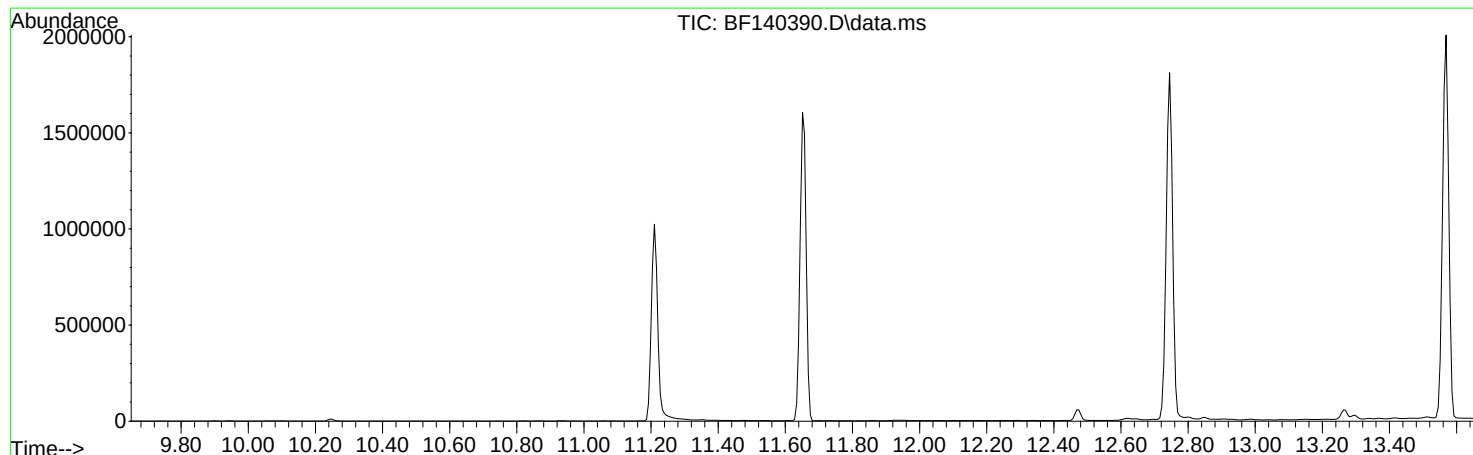

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	59293	PASS
68	69	0.00	2	1.7	1041	PASS
69	198	0.00	100	38.4	59949	PASS
70	69	0.00	2	0.6	377	PASS
127	198	10	80	49.0	76480	PASS
197	198	0.00	2	0.8	1225	PASS
198	198	100	100	100.0	156141	PASS
199	198	5	9	6.8	10617	PASS
275	198	10	60	27.5	42883	PASS
365	198	1	100	3.3	5208	PASS
441	198	0.01	100	13.2	20622	PASS
442	442	50	100	100.0	129669	PASS
443	442	15	24	19.1	24766	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/15/2024	BNA_F	<u>BF140390.D</u>
Compound Name	Response	Retention Time
DDT	501404	13.569
DDD	18593	13.263
DDE	712	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19305	520709	3.71

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111524\
Data File : BF140390.D
Acq On : 15 Nov 2024 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 15 10:40:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

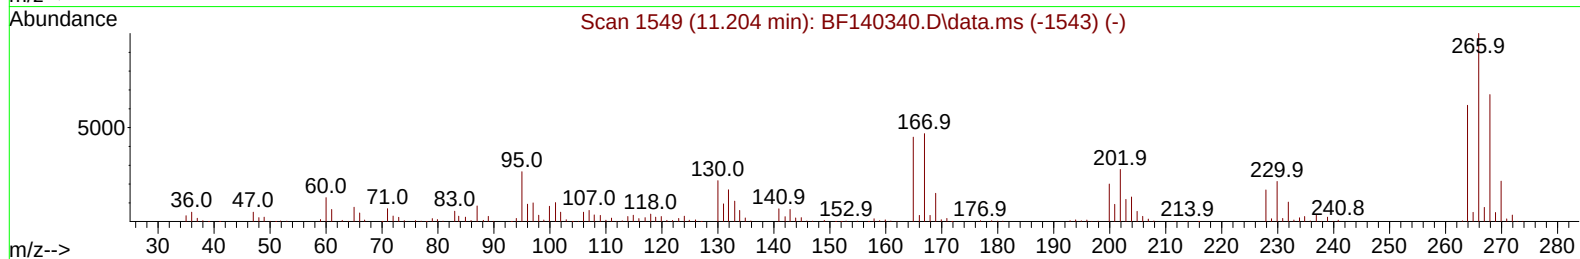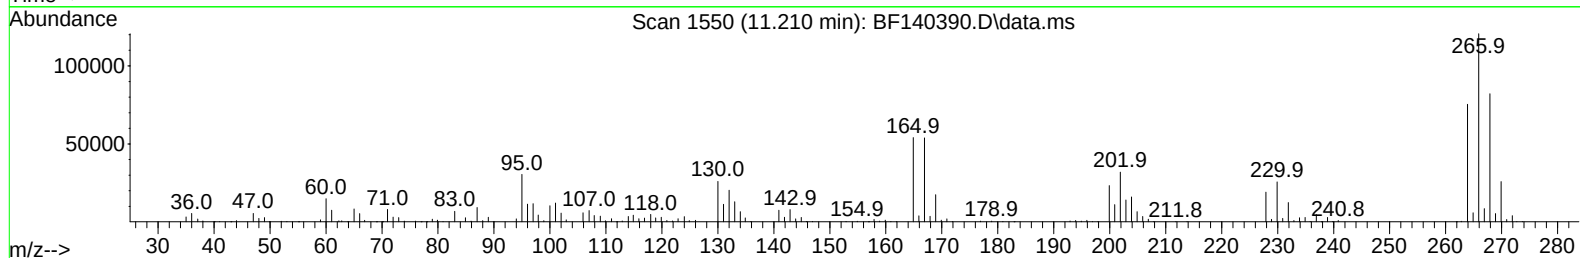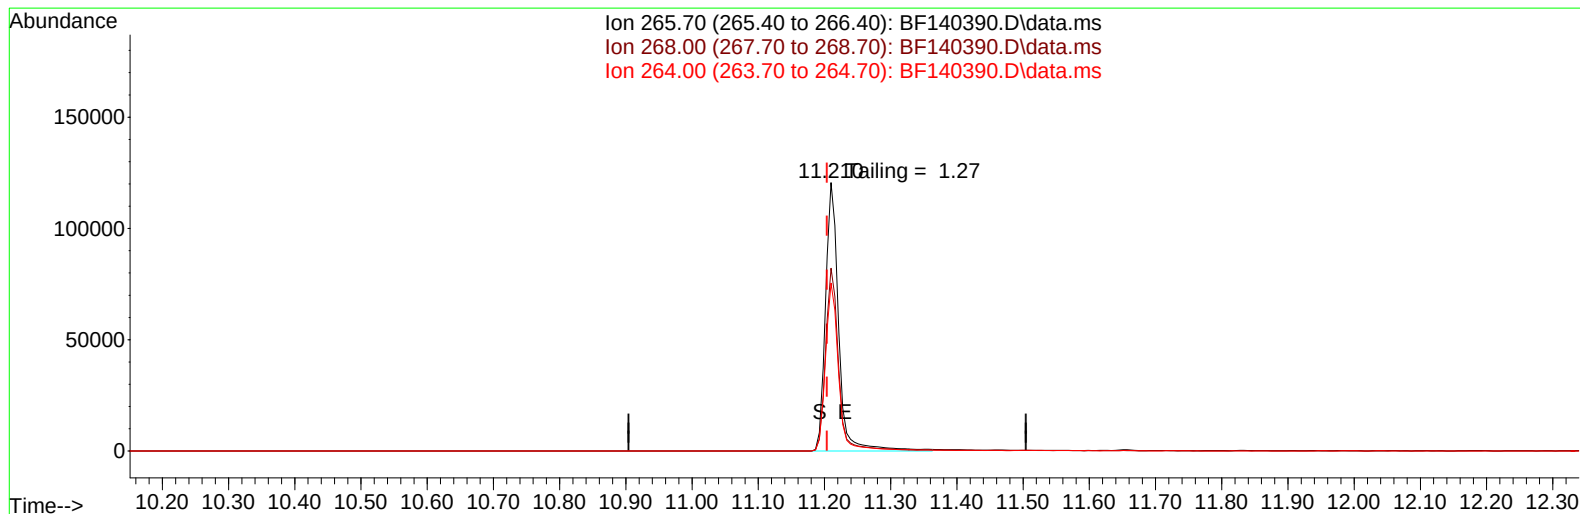

TIC: BF140390.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.006) 50509.13 ng




response 166467

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	68.10
264.00	62.90	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111524\
Data File : BF140390.D
Acq On : 15 Nov 2024 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 15 10:40:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

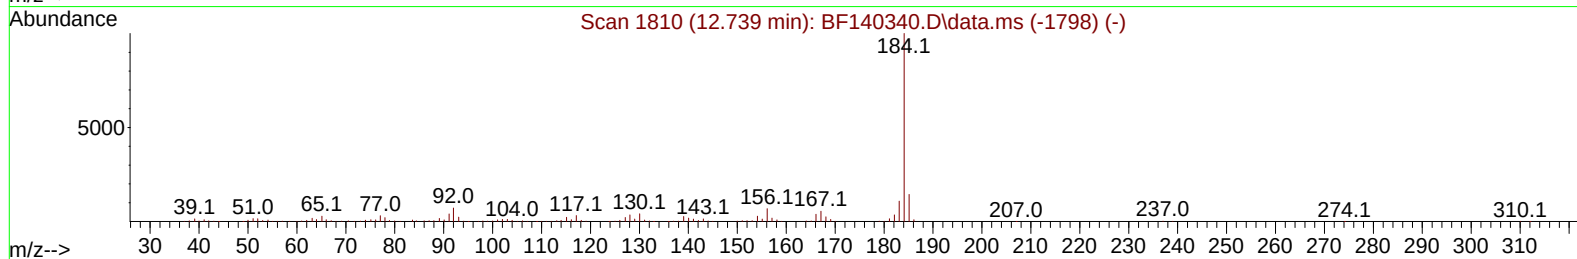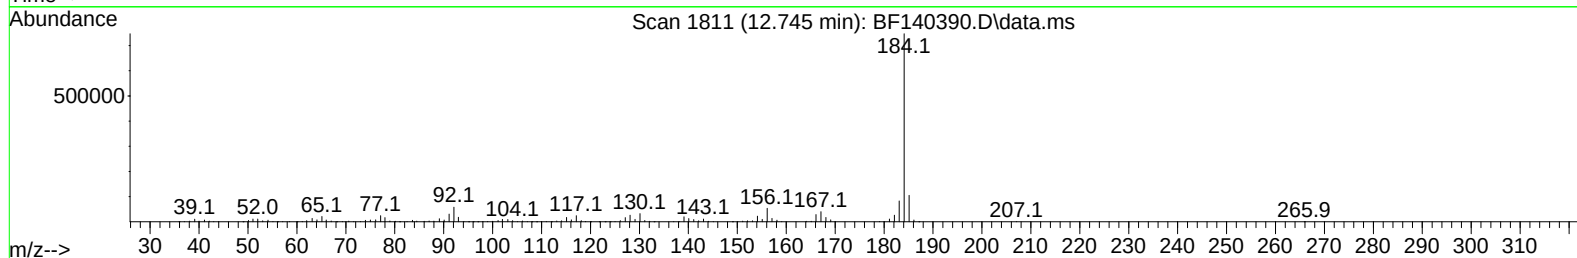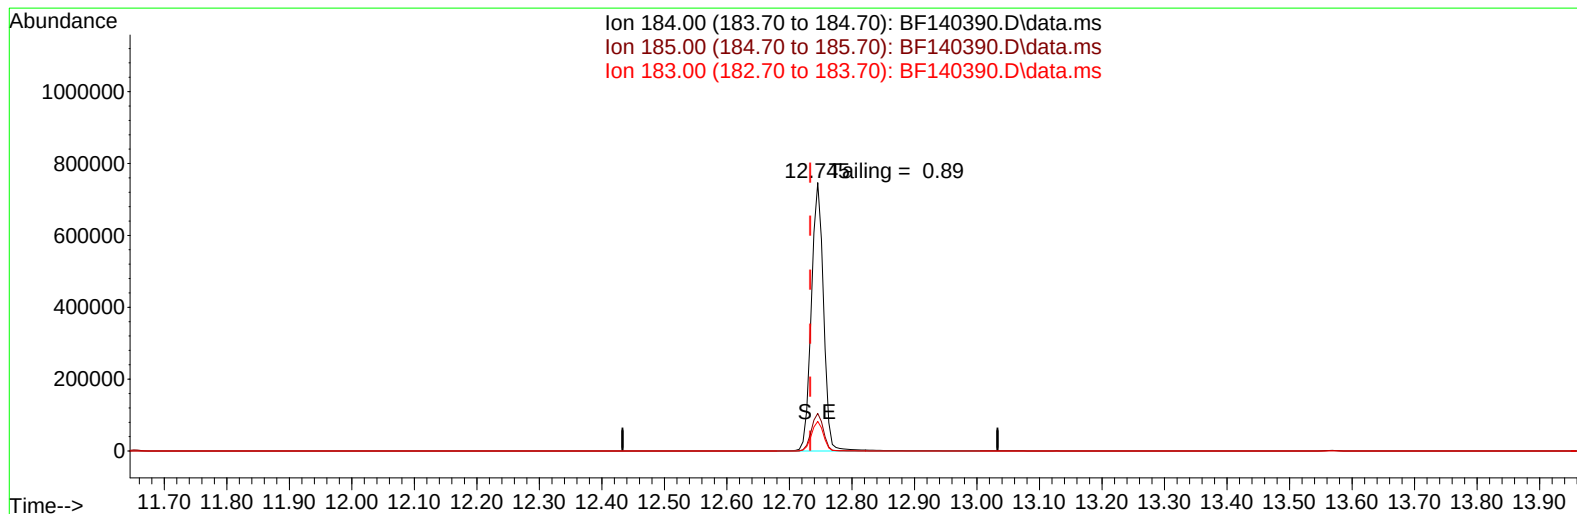

TIC: BF140390.D\data.ms

(77) Benzidine

12.745min (+ 0.012) 31749.52 ng

response 1013847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.05
183.00	10.80	11.05
0.00	0.00	0.00