


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140500.D
Acq On : 20 Nov 2024 15:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

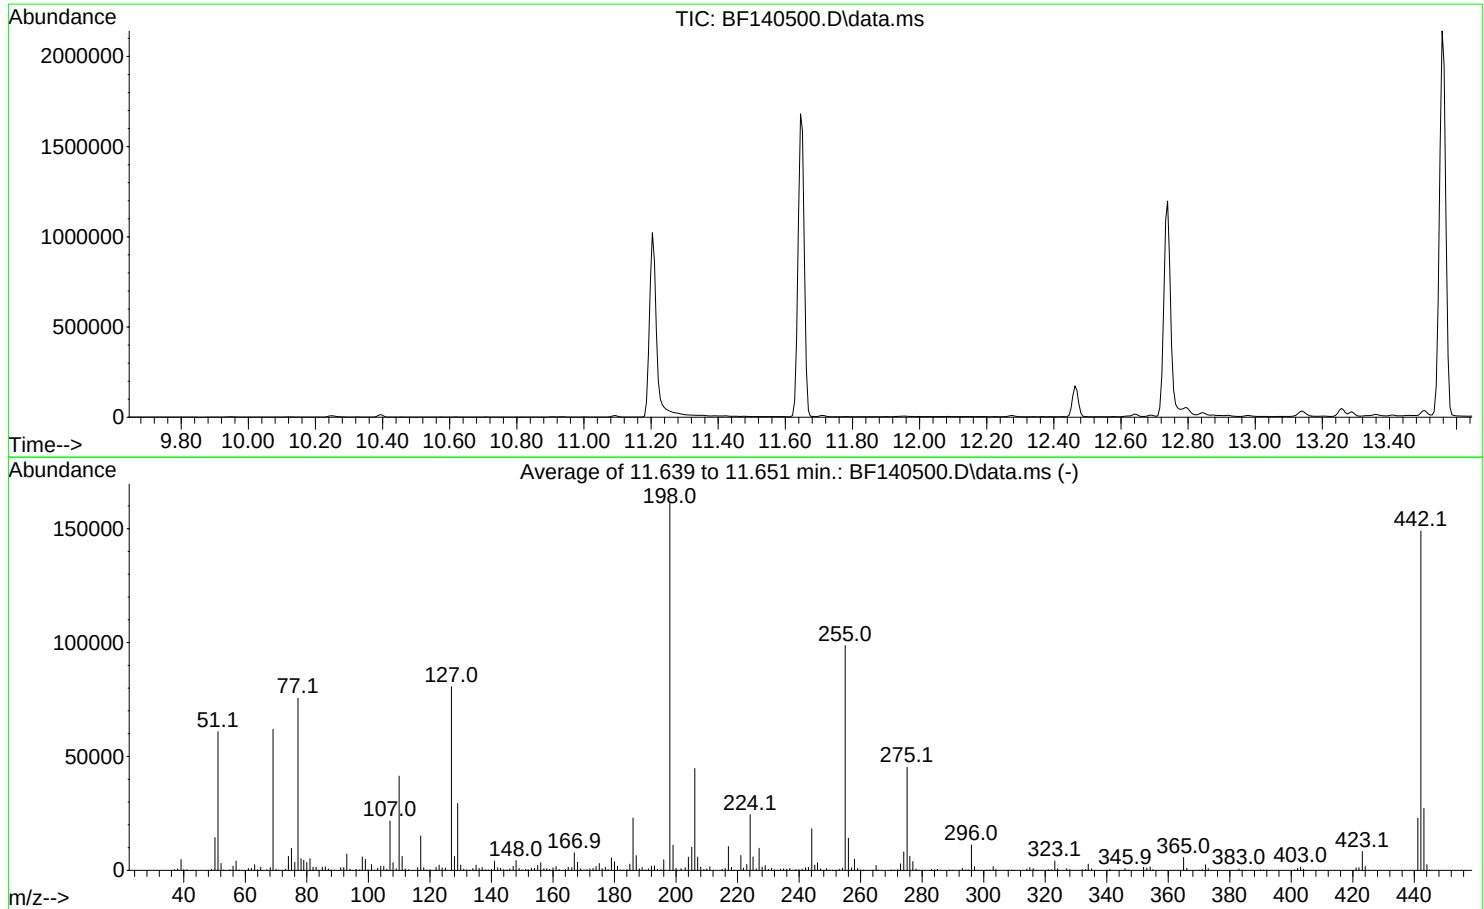

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	60928	PASS
68	69	0.00	2	1.9	1186	PASS
69	198	0.00	100	38.4	61936	PASS
70	69	0.00	2	0.7	421	PASS
127	198	10	80	50.0	80672	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	161499	PASS
199	198	5	9	6.8	11020	PASS
275	198	10	60	28.1	45307	PASS
365	198	1	100	3.5	5617	PASS
441	198	0.01	100	14.2	22910	PASS
442	442	50	100	100.0	148963	PASS
443	442	15	24	18.3	27253	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/20/2024	BNA_F	<u>BF140500.D</u>
Compound Name	Response	Retention Time
DDT	548560	13.557
DDD	17777	13.257
DDE	1079	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18856	567416	3.32

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140500.D
Acq On : 20 Nov 2024 15:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 20 17:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

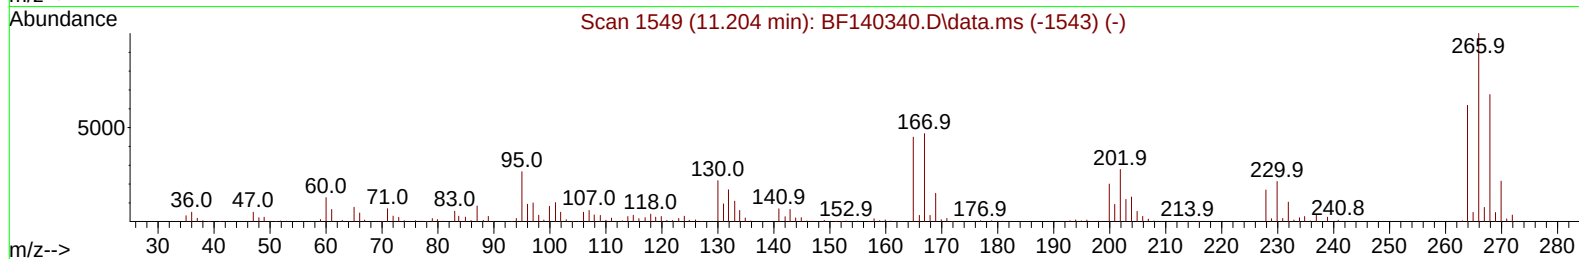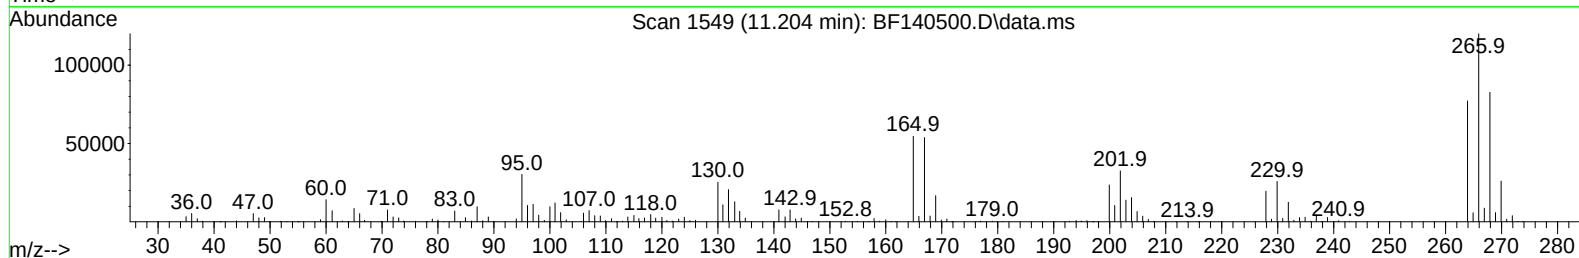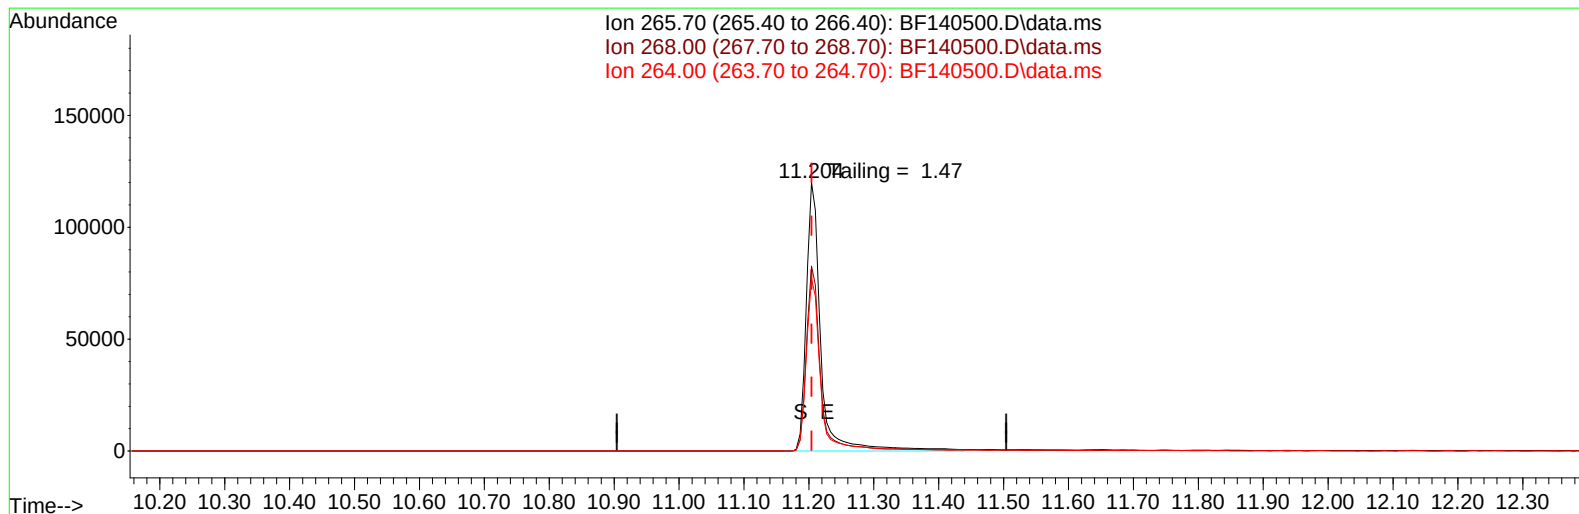

TIC: BF140500.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.000) 29007.72 ng




response 185231

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	68.93
264.00	62.90	64.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140500.D
Acq On : 20 Nov 2024 15:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 20 17:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

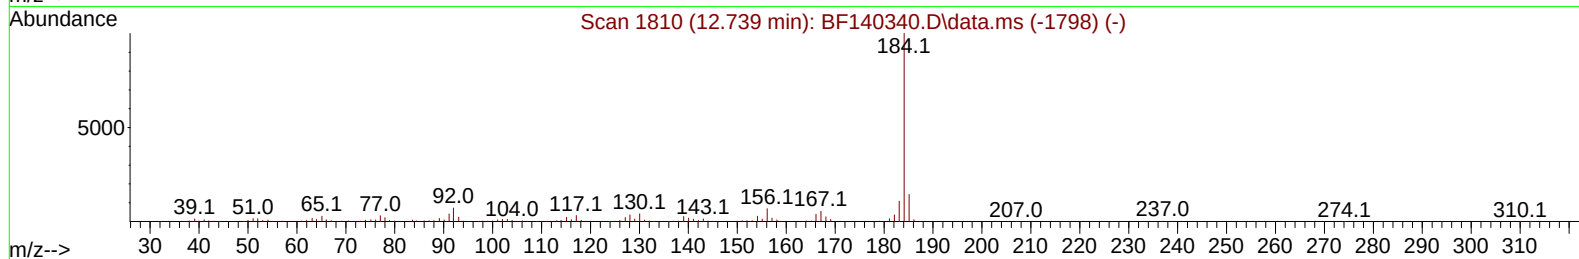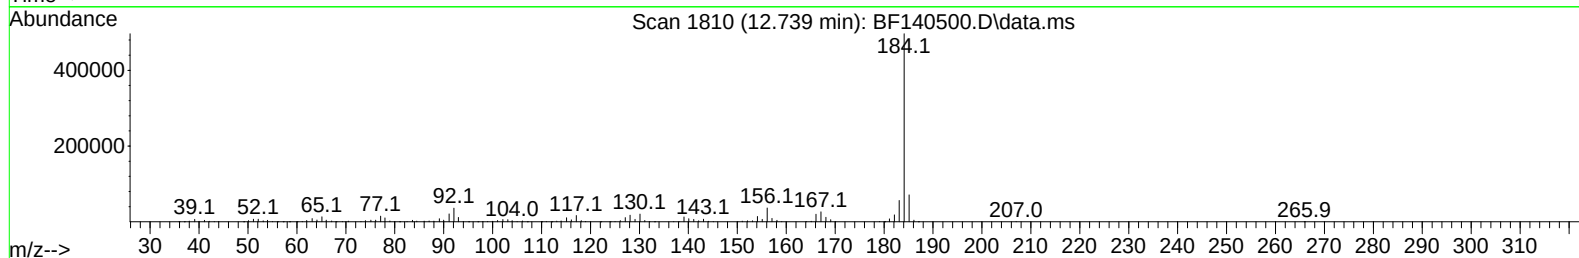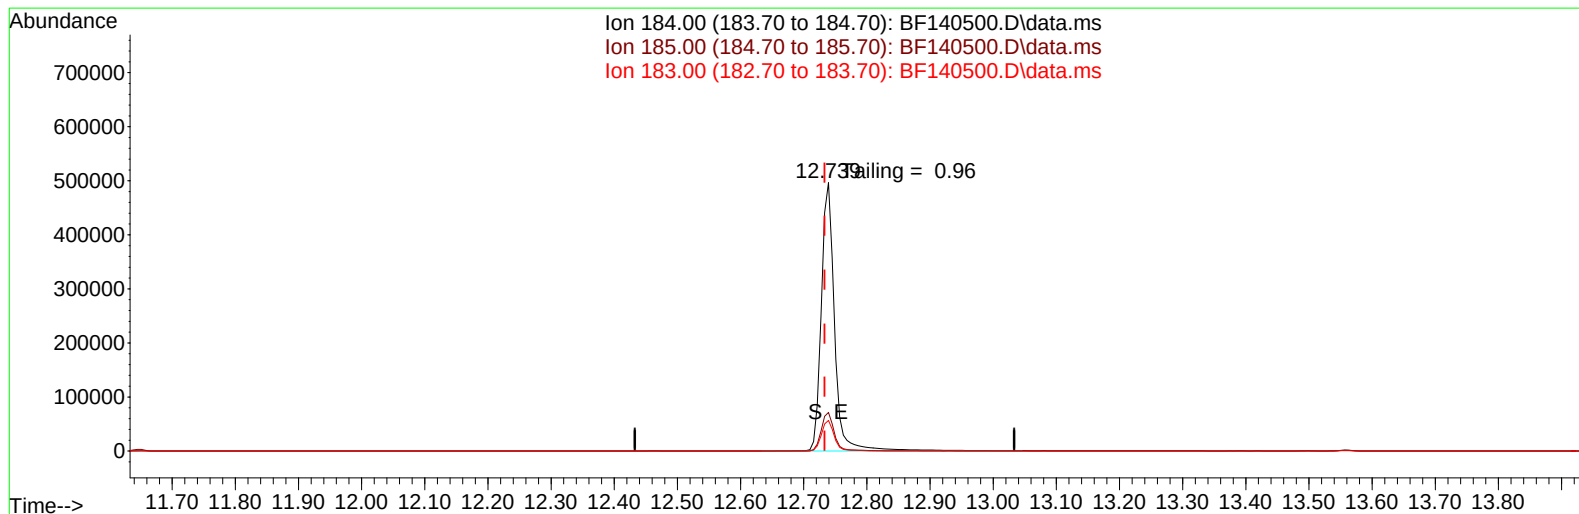

TIC: BF140500.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 19345.82 ng

response 723942

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.37
183.00	10.80	11.38
0.00	0.00	0.00