
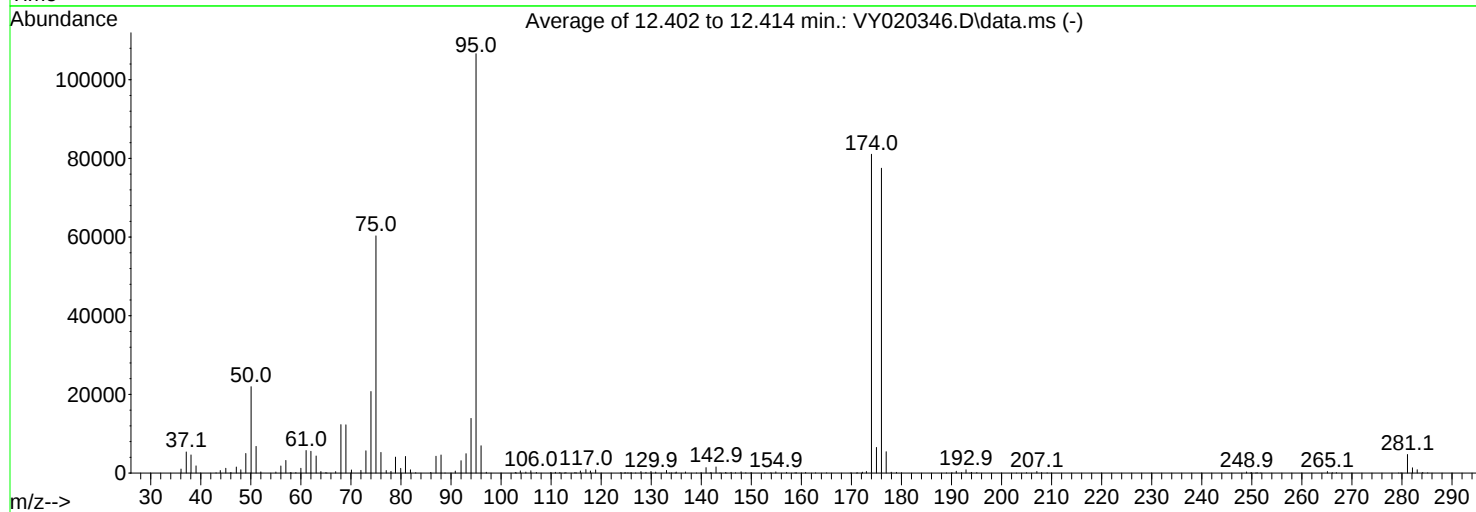


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112024\
Data File : VY020346.D
Acq On : 20 Nov 2024 08:23
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
Title : SW846 8260
Last Update : Wed Nov 20 04:38:24 2024

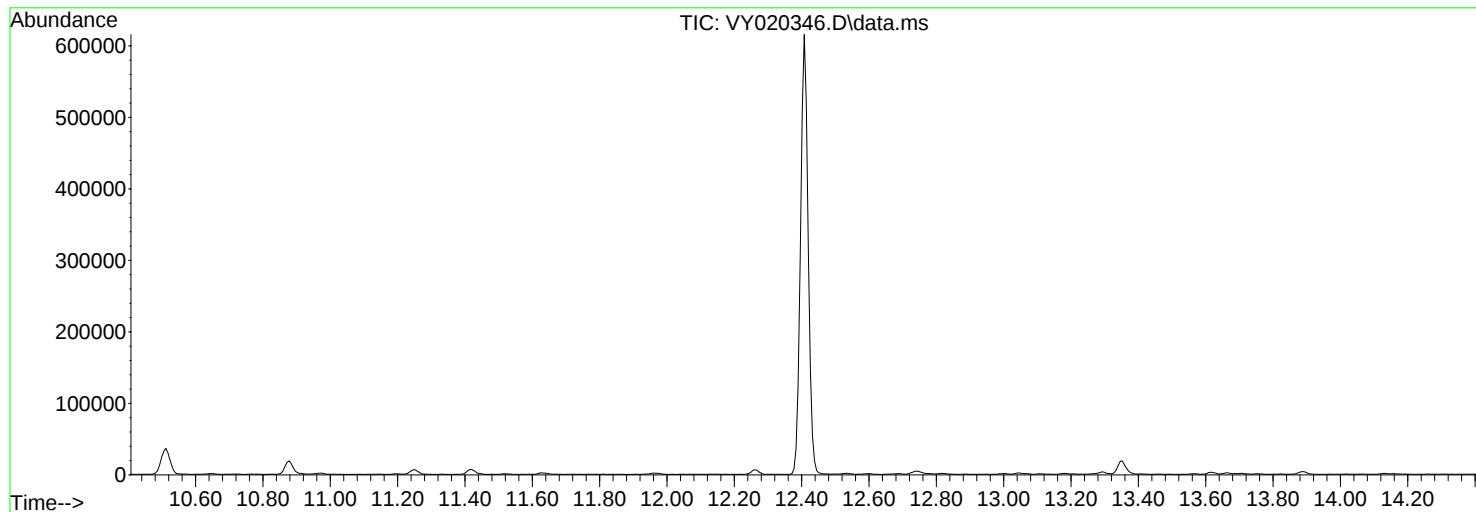

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	21968	PASS
75	95	30	60	56.6	60315	PASS
95	95	100	100	100.0	106611	PASS
96	95	5	9	6.5	6941	PASS
173	174	0.00	2	0.5	403	PASS
174	95	50	100	76.0	81061	PASS
175	174	5	9	8.0	6522	PASS
176	174	95	101	95.6	77504	PASS
177	176	5	9	7.0	5439	PASS