
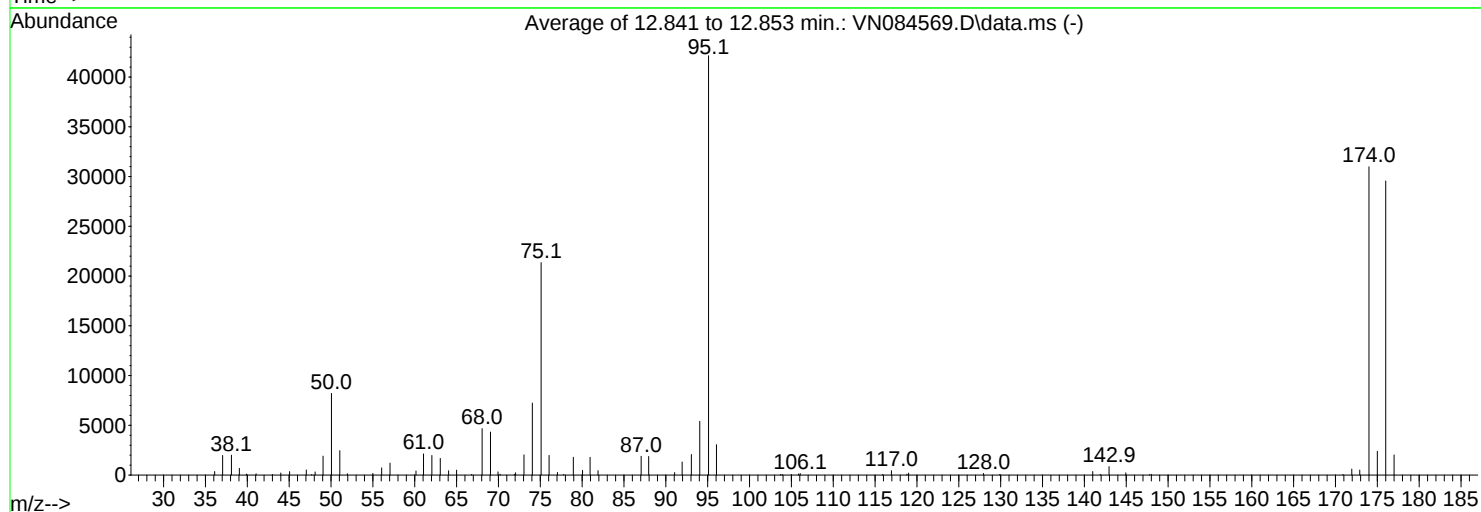


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103024\
Data File : VN084569.D
Acq On : 30 Oct 2024 10:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

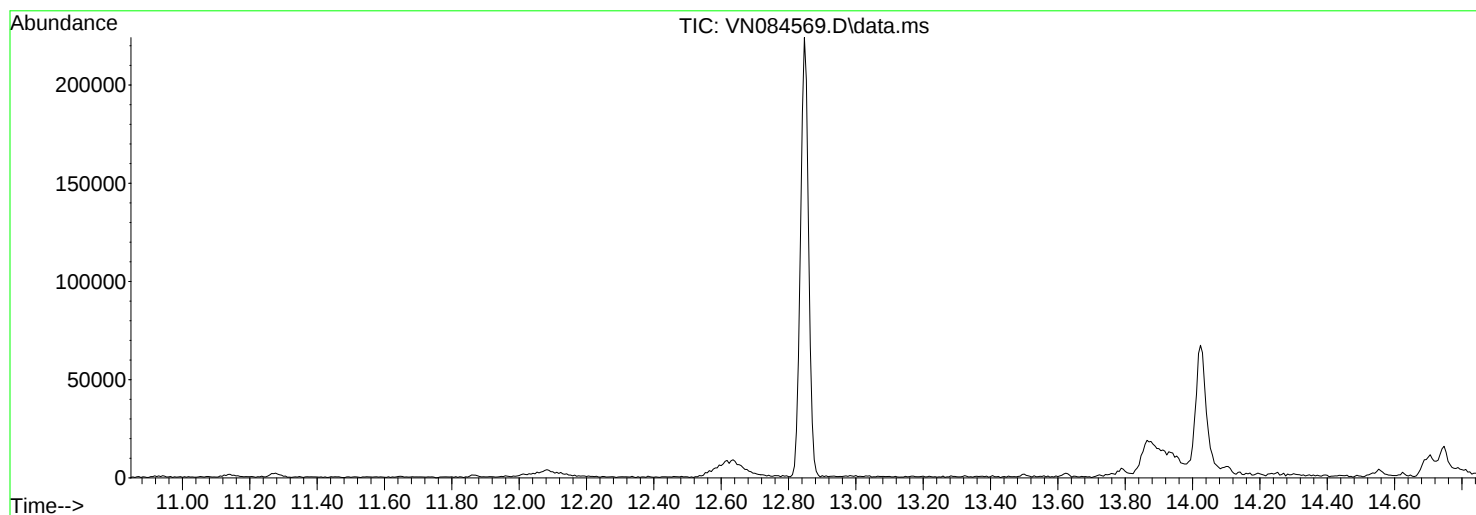

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	8210	PASS
75	95	30	60	50.7	21357	PASS
95	95	100	100	100.0	42141	PASS
96	95	5	9	7.2	3053	PASS
173	174	0.00	2	1.6	502	PASS
174	95	50	100	73.5	30984	PASS
175	174	5	9	7.7	2392	PASS
176	174	95	101	95.4	29560	PASS
177	176	5	9	6.9	2026	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	359	48.10	321	63.05	1677	74.05	7235
37.05	1972	49.05	1905	64.05	441	75.10	21357
38.10	2004	50.05	8210	65.00	496	76.05	1981
39.05	674	51.05	2454	66.80	70	77.05	260
39.90	98	51.95	137	68.05	4674	77.80	63
41.05	129	55.00	174	69.05	4327	78.95	1789
43.00	58	56.05	724	69.95	329	80.05	481
44.00	211	57.05	1205	70.20	94	80.95	1784
45.05	351	60.15	415	71.90	82	81.90	450
47.05	515	61.05	2127	72.05	237	87.05	1893
47.70	66	62.05	1973	73.05	2035	87.95	1870

Average of 12.841 to 12.853 min.: VN084569.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.05	256	115.90	54	148.00	75		
91.95	1316	116.95	438	170.90	52		
93.05	2070	118.80	90	171.95	607		
94.05	5401	119.00	202	172.90	502		
95.10	42141	127.95	162	174.00	30984		
96.05	3053	129.90	69	175.00	2392		
103.70	65	141.00	358	176.00	29560		
103.90	65	141.90	66	177.00	2026		
105.00	53	142.95	857				
105.85	107	144.95	228				
106.05	162	147.80	53				

Instrument :

MSVOA_N

ClientSampleId :

BFB