

Prep Standard - Chemical Standard Summary

Order ID : P4810

Test : TPH GC

Prepbatch ID : PB164989,

Sequence ID/Qc Batch ID: FG111524,

Standard ID :

EP2538,EP2551,PP23454,PP23935,PP23961,PP23962,PP23963,PP23964,PP23965,PP23966,PP23967,

Chemical ID :

E2865,E3551,E3759,E3793,E3794,E3822,E3823,E3828,P 11950,P11958,P11959,P11960,P13213,P13218,P13219,P13492,P13493,P13494,P13495,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3868	METHELENE CHLORIDE+ACETONE	EP2538	09/17/2024	03/11/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 09/17/2024

FROM 8000.00000ml of E3793 + 8000.00000ml of E3794 = Final Quantity: 1600.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2551	10/18/2024	01/03/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 10/18/2024

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3609	20 PPM DRO SPIKE SOLUTION (RESTEK)	PP23454	06/10/2024	12/08/2024	Yogesh Patel	None	None	Ankita Jodhani
								06/12/2024

FROM 1.00000ml of P11950 + 1.00000ml of P11960 + 48.00000ml of E3759 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
147	20 PPM DRO Surrogate Spike Solution	PP23935	11/01/2024	04/23/2025	Yogesh Patel	None	None	Ankita Jodhani
								11/04/2024

FROM 1.00000ml of P13492 + 1.00000ml of P13493 + 1.00000ml of P13494 + 1.00000ml of P13495 + 196.00000ml of E3822 = Final Quantity: 200.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
433	100/100 PPM DRO (Restek)	PP23961	11/13/2024	05/09/2025	Yogesh Patel	None	None	Ankita Jodhani
								11/13/2024

FROM 1.00000ml of P11958 + 1.00000ml of P11959 + 1.00000ml of P13213 + 7.00000ml of E3828 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3796	100/100 PPM DRO STD (CPI)	PP23962	11/13/2024	02/14/2025	Yogesh Patel	None	None	Ankita Jodhani
								11/13/2024

FROM 1.00000ml of P13213 + 1.00000ml of P13218 + 1.00000ml of P13219 + 7.00000ml of E3828 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
435	50 PPM ICC DRO STD (Restek)	PP23963	11/13/2024	05/09/2025	Yogesh Patel	None	None	Ankita Jodhani
								11/13/2024

FROM 0.50000ml of E3828 + 0.50000ml of PP23961 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
437	20 PPM ICC DRO STD (Restek)	PP23964	11/13/2024	05/09/2025	Yogesh Patel	None	None	Ankita Jodhani
								11/13/2024

FROM 0.80000ml of E3828 + 0.20000ml of PP23961 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
438	10 PPM ICC DRO STD (Restek)	PP23965	11/13/2024	05/09/2025	Yogesh Patel	None	None	Ankita Jodhani
								11/13/2024

FROM 0.90000ml of E3828 + 0.10000ml of PP23961 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
439	5 PPM ICC DRO STD (Restek)	PP23966	11/13/2024	05/09/2025	Yogesh Patel	None	None	Ankita Jodhani
								11/13/2024

FROM 0.90000ml of E3828 + 0.10000ml of PP23963 = Final Quantity: 1.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3797	50 PPM DRO ICV STD (CPI)	PP23967	11/13/2024	02/14/2025	Yogesh Patel	None	None	Ankita Jodhani 11/13/2024
<u>FROM</u>	0.80000ml of E3828 + 0.50000ml of PP23962 = Final Quantity: 1.000 ml							

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	01/03/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24D1962005	12/08/2024	06/08/2024 / Rajesh	05/31/2024 / Rajesh	E3759

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	03/11/2025	09/12/2024 / Rajesh	09/11/2024 / Rajesh	E3793

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24G2362009	03/17/2025	09/17/2024 / Rajesh	09/03/2024 / Rajesh	E3794

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24I2662006	04/23/2025	10/24/2024 / Rajesh	10/24/2024 / Rajesh	E3822

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24I2662006	05/03/2025	11/03/2024 / Rajesh	10/24/2024 / Rajesh	E3823

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24G0862003	05/09/2025	11/09/2024 / Rajesh	11/04/2024 / Rajesh	E3828

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0186840	12/10/2024	06/10/2024 / yogesh	07/11/2022 / Yogesh	P11950

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0186840	05/13/2025	11/13/2024 / yogesh	07/11/2022 / Yogesh	P11958

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0186840	05/13/2025	11/13/2024 / yogesh	07/11/2022 / Yogesh	P11959

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0186840	12/10/2024	06/10/2024 / yogesh	07/11/2022 / Yogesh	P11960

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	05/13/2025	11/13/2024 / yogesh	01/17/2024 / Ankita	P13213

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	514983	02/14/2025	08/14/2024 / yogesh	01/31/2024 / Ankita	P13218

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	514983	05/13/2025	11/13/2024 / yogesh	01/31/2024 / Ankita	P13219

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	05/01/2025	11/01/2024 / yogesh	07/24/2024 / yogesh	P13492

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	05/01/2025	11/01/2024 / yogesh	07/24/2024 / yogesh	P13493

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	05/01/2025	11/01/2024 / yogesh	07/24/2024 / yogesh	P13494

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	05/01/2025	11/01/2024 / yogesh	07/24/2024 / yogesh	P13495

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1

Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 24D1962005
Manufactured Date: 2024-03-16
Expiration Date: 2025-06-15
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	8
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	99.9 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.1 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC
Manufacturer source batch: MG24C16563

E 3759

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
CMOS

avantor™



Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

>>> Continued on page 2 >>>

Recd. by RP on 9/11/24

E3793

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use
Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC

Michelle Bales
Sr. Manager, Quality Assurance

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4

Batch No.: 24I2662006

Manufactured Date: 2024-08-29

Expiration Date: 2025-11-28

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	3
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	99.9%
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3822

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)

 **avantors**TM



Material No.: 9266-A4

Batch No.: 24I2662006

Manufactured Date: 2024-08-29

Expiration Date: 2025-11-28

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	3
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	99.9%
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3823



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)

 **avantors**TM



Material No.: 9266-A4

Batch No.: 24J0862003

Manufactured Date: 2024-09-12

Expiration Date: 2025-12-12

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	1
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3828



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



CERTIFIED REFERENCE MATERIAL

110 Benner Circle


Belleville, PA 16823-8812

Tel: (800)356-1688

Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266

Lot No.: A0186840

Description :

Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size :

2 mL

Pkg Amt: > 1 mL

Expiration Date :

July 31, 2029

Storage: 25°C nominal

Handling:

Sonicate prior to use.

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	505.0 µg/mL	+/- 2.9995 µg/mL +/- 12.5465 µg/mL +/- 15.0390 µg/mL	Gravimetric Unstressed Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	503.0 µg/mL	+/- 2.9877 µg/mL +/- 12.4968 µg/mL +/- 14.9795 µg/mL	Gravimetric Unstressed Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	503.5 µg/mL	+/- 2.9906 µg/mL +/- 12.5092 µg/mL +/- 14.9944 µg/mL	Gravimetric Unstressed Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	505.0 µg/mL	+/- 2.9995 µg/mL +/- 12.5465 µg/mL +/- 15.0390 µg/mL	Gravimetric Unstressed Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	504.7 µg/mL	+/- 2.9978 µg/mL +/- 12.5390 µg/mL +/- 15.0301 µg/mL	Gravimetric Unstressed Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	504.4 µg/mL	+/- 2.9960 µg/mL +/- 12.5316 µg/mL +/- 15.0212 µg/mL	Gravimetric Unstressed Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	503.5 µg/mL	+/- 2.9906 µg/mL +/- 12.5092 µg/mL +/- 14.9944 µg/mL	Gravimetric Unstressed Stressed

P11948
P11962 } 7.8
07/11/16

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 99%	(Lot MKCN9321)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	504.4 µg/mL	+/- 2.9960 +/- 12.5316 +/- 15.0212	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

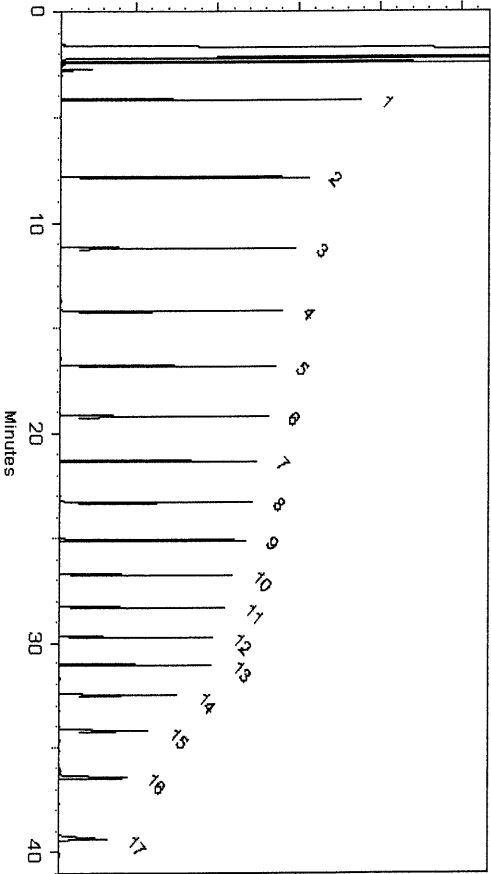

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brittany Federinko

Brittany Federinko - Operations Tech I

Date Mixed: 29-Jun-2022

Balance: 1128360905

Christie Mills

Christie Mills - Operations Tech II - ARM QC

Date Passed: 01-Jul-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-US for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-US.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle


Belleville, PA 16823-8812

Tel: (800)356-1688

Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266

Lot No.: A0186840

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2029

Storage: 25°C nominal

Handling: Sonicate prior to use.

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL Gravimetric Unstressed Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL Gravimetric Unstressed Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL Gravimetric Unstressed Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL Gravimetric Unstressed Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL Gravimetric Unstressed Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	504.4 µg/mL	+/- 2.9960 +/- 12.5316 +/- 15.0212	µg/mL Gravimetric Unstressed Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL Gravimetric Unstressed Stressed

P11948 } 7.8
P11962 } 07/11/16

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 99%	(Lot MKCN9321)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	504.4 µg/mL	+/- 2.9960 +/- 12.5316 +/- 15.0212	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

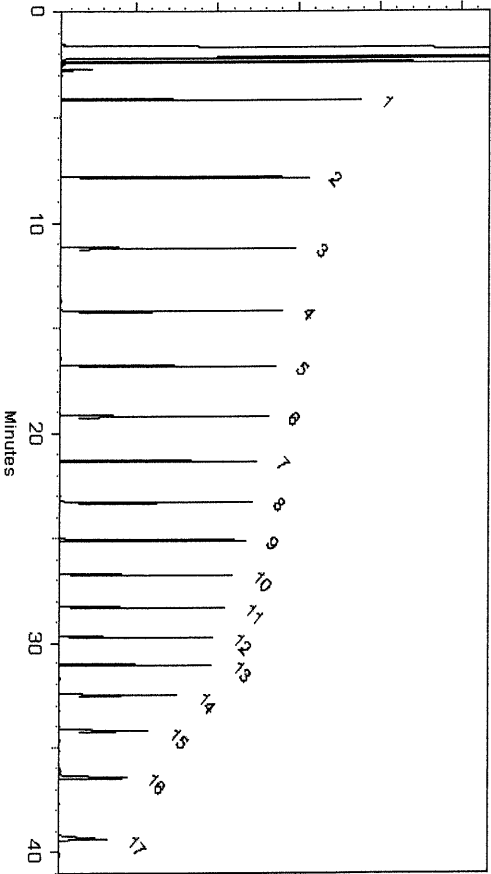

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brittany Federinko

Brittany Federinko - Operations Tech I

Date Mixed: 29-Jun-2022

Balance: 1128360905

Christie Mills

Christie Mills - Operations Tech II - ARM QC

Date Passed: 01-Jul-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-US for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-US.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle


Belleville, PA 16823-8812

Tel: (800)356-1688

Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266

Lot No.: A0186840

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2029

Storage: 25°C nominal

Handling: Sonicate prior to use.

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	505.0 µg/mL	+/- 2.9995 µg/mL +/- 12.5465 µg/mL +/- 15.0390 µg/mL	Gravimetric Unstressed Unstressed Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	503.0 µg/mL	+/- 2.9877 µg/mL +/- 12.4968 µg/mL +/- 14.9795 µg/mL	Gravimetric Unstressed Unstressed Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	503.5 µg/mL	+/- 2.9906 µg/mL +/- 12.5092 µg/mL +/- 14.9944 µg/mL	Gravimetric Unstressed Unstressed Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	505.0 µg/mL	+/- 2.9995 µg/mL +/- 12.5465 µg/mL +/- 15.0390 µg/mL	Gravimetric Unstressed Unstressed Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	504.7 µg/mL	+/- 2.9978 µg/mL +/- 12.5390 µg/mL +/- 15.0301 µg/mL	Gravimetric Unstressed Unstressed Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	504.4 µg/mL	+/- 2.9960 µg/mL +/- 12.5316 µg/mL +/- 15.0212 µg/mL	Gravimetric Unstressed Unstressed Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	503.5 µg/mL	+/- 2.9906 µg/mL +/- 12.5092 µg/mL +/- 14.9944 µg/mL	Gravimetric Unstressed Unstressed Stressed

P11948 } 7.8
P11962 } 07/11/16

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 99%	(Lot MKCN9321)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	504.4 µg/mL	+/- 2.9960 +/- 12.5316 +/- 15.0212	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

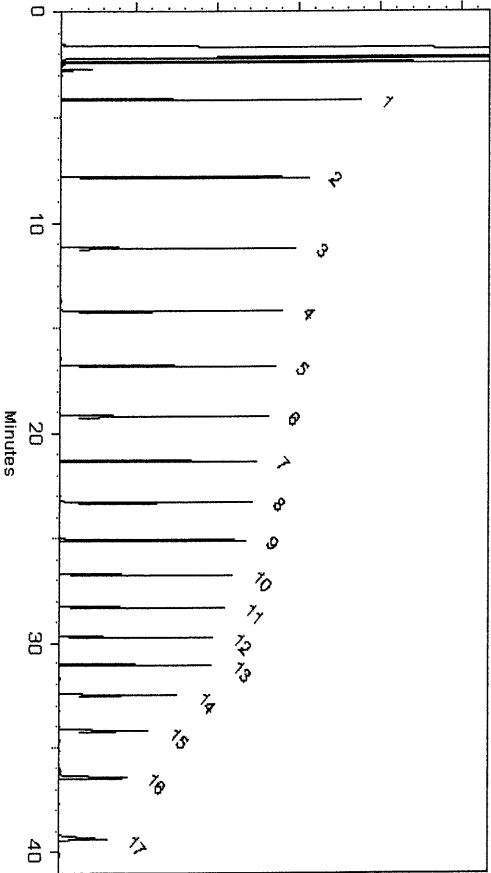

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brittany Federinko

Brittany Federinko - Operations Tech I

Date Mixed: 29-Jun-2022

Balance: 1128360905

Christie Mills

Christie Mills - Operations Tech II - ARM QC

Date Passed: 01-Jul-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-US for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-US.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle


Belleville, PA 16823-8812

Tel: (800)356-1688

Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266

Lot No.: A0186840

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2029

Storage: 25°C nominal

Handling: Sonicate prior to use.

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL Gravimetric Unstressed Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL Gravimetric Unstressed Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL Gravimetric Unstressed Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL Gravimetric Unstressed Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL Gravimetric Unstressed Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	504.4 µg/mL	+/- 2.9960 +/- 12.5316 +/- 15.0212	µg/mL Gravimetric Unstressed Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL Gravimetric Unstressed Stressed

P11948 } 7.8
P11962 } 07/11/16

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 99%	(Lot MKCN9321)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	504.4 µg/mL	+/- 2.9960 +/- 12.5316 +/- 15.0212	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

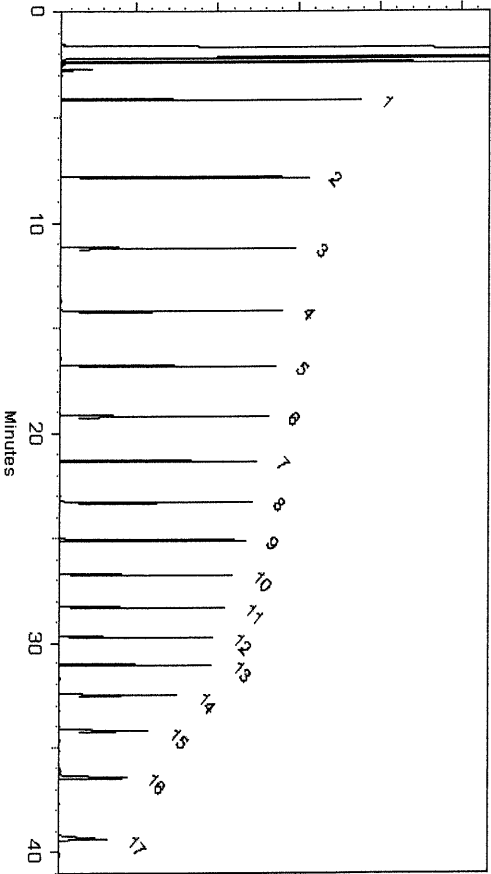

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brittany Federinko

Brittany Federinko - Operations Tech I

Date Mixed: 29-Jun-2022

Balance: 1128360905

Christie Mills

Christie Mills - Operations Tech II - ARM QC

Date Passed: 01-Jul-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-US for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-US.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

72072
101122
n-Tetracosane-d50

Solvent(s):
Methylene chloride

Lot#
105345

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

101132
Ambient (20 °C)
1000
6UTB

5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0

Formulated By:	Prashant Chauhan	101122	DATE
Reviewed By:	Pedro L. Renteria	101122	DATE

SDS Information

Expanded
Uncertainty
(+/-) (µg/mL)

Actual
Conc (µg/mL)

Actual
Weight(g)

Target
Weight(g)

Assay
(%D)

Purity
(%)

Nominal
Conc (µg/mL)

Lot
Number

RM#

Compound

2072

PR-26606

1000

98.7

0.2

99.0

(Solvent Safety Info. On Attached pg.)

CAS#

OSHA PEL (TWA)

LD50

0.20482

0.20471

1000.6

4.1

16416-32-3

N/A

N/A

N/A

N/A

N/A

N/A

N/A

N/A

N/A

1. n-Tetracosane-d50

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

Abundance

23.16

15.00

10.00

5.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00

0.00


0.00

P13205

P13214

AJ

61/17/24

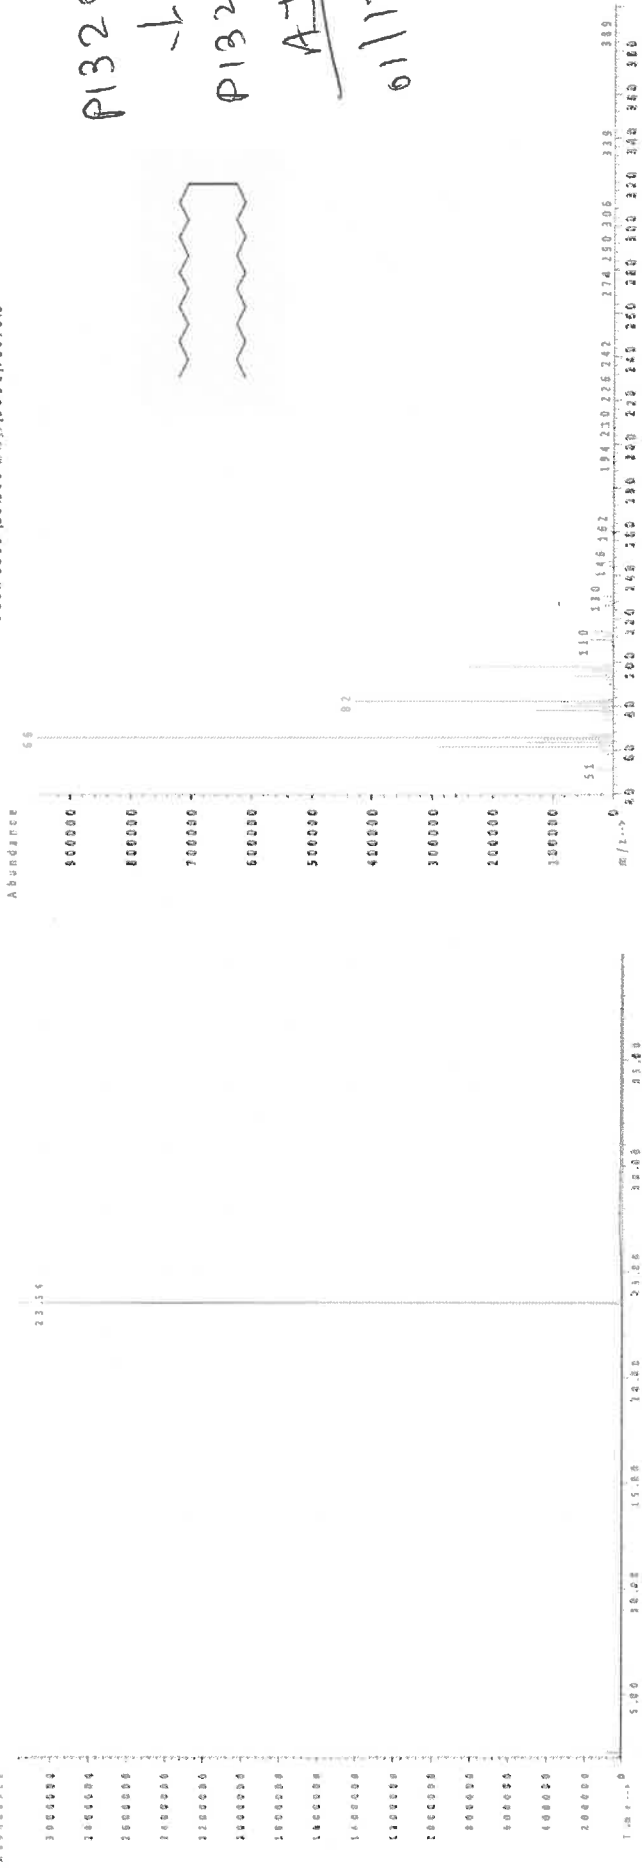

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



5580 Skylane Blvd
Santa Rosa, CA 95403
(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400-05 514983 ≤-10 Degrees C

Solvent:

Hexane

Exp. Date:

11/20/2028

Description:

TRPH Standard (C8-C40), 500 mg/L, 1 ml

-01

Compound

CAS No.

Purity (%)

Compound Lot No.

Concentration, mg/L

decane (C10)

124-18-5

99.7

415.7.2P

498.5 ± 6.92

docosane (C22)

629-97-0

98.8

420.9.1P

499.4 ± 6.93

dodecane (C12)

112-40-3

99.7

416.9.3P

502 ± 6.97

dotriacontane (C32)

544-85-4

97

425.9.2.2P

499.6 ± 8.53

eicosane (C20)

112-95-8

99.8

419.7.1P

501 ± 6.95

hexacosane (C26)

630-01-3

99.3

422.7.2.1P

501 ± 6.95

hexatriacontane (C36)

630-06-8

98

427.29.1.1P

499.3 ± 8.53

n-hexadecane (C16)

544-76-3

99.45

368.27.1.1P

498.7 ± 6.91

octacosane (C28)

630-02-4

99.1

423.24.1P

500.5 ± 6.95

n-octadecane (C18)

593-45-3

99.5

418.29.1P

499.5 ± 6.92

octane (C8)

111-65-9

99.4

385.7.2.1P

498.5 ± 6.92

octatriacontane (C38)

7194-85-6

95

428.1.2P

500.2 ± 6.94

tetracontane (C40)

4181-95-7

97

429.7.2P

499.6 ± 6.93

n-tetracosane (C24)

646-31-1

99.5

421.7.1P

499.5 ± 6.93

n-tetradecane (C14)

629-59-4

99.3

417.9.1P

500 ± 6.94

tetatriacontane (C34)

14167-59-0

96.1

426.7.2.2P

499.7 ± 8.53

triacontane (C30)

638-68-6

99.5

424.7.1.1P

500 ± 6.94

Let the standard warm to room temperature and sonicate before opening.

P13215

↓

P13224

AJ
01131124

*Not a certified value

Andrea Schaible

Certified By: _____
Andrea Schaible
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.



5580 Skylane Blvd
Santa Rosa, CA 95403
(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400-05 514983 ≤-10 Degrees C

Solvent:

Hexane

Exp. Date:

11/20/2028

Description:

TRPH Standard (C8-C40), 500 mg/L, 1 ml

-01

Compound

CAS No.

Purity (%)

Compound Lot No.

Concentration, mg/L

decane (C10)

124-18-5

99.7

415.7.2P

498.5 ± 6.92

docosane (C22)

629-97-0

98.8

420.9.1P

499.4 ± 6.93

dodecane (C12)

112-40-3

99.7

416.9.3P

502 ± 6.97

dotriacontane (C32)

544-85-4

97

425.9.2.2P

499.6 ± 8.53

eicosane (C20)

112-95-8

99.8

419.7.1P

501 ± 6.95

hexacosane (C26)

630-01-3

99.3

422.7.2.1P

501 ± 6.95

hexatriacontane (C36)

630-06-8

98

427.29.1.1P

499.3 ± 8.53

n-hexadecane (C16)

544-76-3

99.45

368.27.1.1P

498.7 ± 6.91

octacosane (C28)

630-02-4

99.1

423.24.1P

500.5 ± 6.95

n-octadecane (C18)

593-45-3

99.5

418.29.1P

499.5 ± 6.92

octane (C8)

111-65-9

99.4

385.7.2.1P

498.5 ± 6.92

octatriacontane (C38)

7194-85-6

95

428.1.2P

500.2 ± 6.94

tetracontane (C40)

4181-95-7

97

429.7.2P

499.6 ± 6.93

n-tetracosane (C24)

646-31-1

99.5

421.7.1P

499.5 ± 6.93

n-tetradecane (C14)

629-59-4

99.3

417.9.1P

500 ± 6.94

tetatriacontane (C34)

14167-59-0

96.1

426.7.2.2P

499.7 ± 8.53

triacontane (C30)

638-68-6

99.5

424.7.1.1P

500 ± 6.94

Let the standard warm to room temperature and sonicate before opening.

P13215

↓

P13224

AJ
01/31/24

*Not a certified value

Andrea Schaible

Andrea Schaible
Chemist

Certified By: _____

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.

ABSOLUTE STANDARDS, INC.

ISO - 17034



Certificate of Analysis



Certified Reference Material (CRM)

Conformance: The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

Health & Safety: See the attached SDS & Certified Weight Report before use.

Intended Use: This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

Characterization Values: In production, gravimetric/volumetric readings are certified to be within $\pm 0.5\%$ of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

Homogeneity: Uncertainties that are due to the analytical procedure(s) are within $\pm 5\%$ unless specifically stated on the Certified Wt. Report.

Verification: Uncertainties that are due to the analytical procedure(s) are within $\pm 5\%$ unless specifically stated on the Certified Wt. Report.

Stability: Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

Uncertainty: UCRM is the expanded uncertainty which utilizes a $K = 2$ (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

Purity & Identity: Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neats are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

Storage: Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

Usage: Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

Minimum Sample Size: 0.5 uL for analytical applications.

Legal Notice: Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

Certifying Officer: Stephen J. Arpie, M.S., Director General

Page 1 of 2



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514
Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com
Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019



ABSOLUTE STANDARDS, INC.

ISO - 17034

Understanding the Certified Weight Report

Each Certified Reference Material (CRM) is supported by a Certified Weight Report. Assigned values for concentrations and associated uncertainties are based upon NIST traceable masses & volumes used in production.

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com

Certified Reference Material CRM

ISO 17034 Accredited
Scope: http://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT

Part # 10009R
Lot # 070716
Description: CLP Priority Pollutant Internal Standards
GC/MS Calibration - 6 components
Expiration Date: 070721
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 4000
NIST Test ID#: 822-275872-11
Weight(s) shown below were combined and diluted to (mL): 500.0

Solvent(s): Methylene chloride
Lot# 78782

Formulated By: Paul Barron
Reviewed By: Pedro L. Rentes

DATE: 070716
DATE: 070716

MSDS Information
(Solvent Safety Info. On Attached pg.)

Compound	SMW	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty (%)	Target Weight (µg)	Actual Weight (µg)	Actual Conc (µg/mL)	Expanded Uncertainty (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. 1,4-Dichlorobenzene-d4	118	PR-1845M07287CB1	4000	98	0.2	2.04093	2.04335	4004.7	15.4	2055-02-1	N/A	or-rat 500mg/kg
2. Naphthalene-d8	223	PR-2339M031612HP1	4000	99	0.2	2.02032	2.02084	4001.0	15.2	1168-85-2	10 ppm (50mg/m3)(H)	or-rat 400mg/kg
3. Acenaphthene-d10	2	PR-25444	4000	99	0.2	2.02032	2.02245	4004.2	15.2	15067-28-2	N/A	or-rat 500mg/kg
4. Phenanthrene-d10	248	PR-2305M081711PM1	4000	98	0.2	2.04093	2.04135	4000.8	15.4	1517-25-2	N/A	N/A
5. Chrysene-d12	92	I-19290	4000	98	0.2	2.04093	2.04150	4001.3	15.4	1719-03-5	N/A	N/A
6. Perylene-d12	247	PR-24113	4000	98	0.2	2.04093	2.04155	4001.2	15.4	1503-58-3	N/A	N/A

Run 35, "P10009R L070716 [4000µg/mL in MeCl2]"
Run Length: 40.00 min, 23900 points at 10 points/second.
Created: Sat, Jul 9, 2016 at 1:54:53 PM.
Sampled: Sequence "070716-GC/MS2", Method "GC-MS2".
Analyzed using Method "GC-MS2".

Comments:
GC-MS2 Analysis by Melissa Siciric
Column ID SPB-5 30 meter x 0.53mm x 1.5um Film Thickness.
Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 0.5 mL, Helium (make-up) = 25 mL.
Hydrogen (detector) = 30 mL, Air (detector) = 300 mL, Oven Temp 1 = 50°C (1 min).
Rise = 10°C/min, Oven Temp 2 = 300°C (14 min). Total Run Time = 40 Minutes. Injector Temp = 250°C.
FID Temp = 300°C, FID Signal = sData Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 4

Peak Data:

Peak No.	Name	Retention Time (min)
1	1,4-Dichlorobenzene-d4	6.34
2	Naphthalene-d8	8.98
3	Acenaphthene-d10	12.97
4	Phenanthrene-d10	16.37
5	Chrysene-d12	22.62
6	Perylene-d12	25.75

Qualitative Quantitative

3rd Party Comparison

Analyte	Sup/Abs Dev (%)
1,4-Dichlorobenzene-d4	2.55
Naphthalene-d8	2.43
Acenaphthene-d10	2.74
Phenanthrene-d10	0.65
Chrysene-d12	1.93
Perylene-d12	-1.72
Total	-0.55

Part # 10009R Lot # 041219 1 of 2 Printed: 5/8/2019, 12:55:50 PM

For More Information, Contact:

StephenArpie@AbsoluteStandards.com

Page 2 of 2



CERTIFIED WEIGHT REPORT

Part Number: **72072**
Lot Number: **101122**
Description: **n-Tetracosane-d50**

Solvent(s):
Methylene chloride

Lot#
105345


Expiration Date: **101132**
Recommended Storage: **Ambient (20 °C)**
Nominal Concentration (µg/mL): **1000**
NIST Test ID#: **6UB3**
Weight(s) shown below were combined and diluted to (mL): **200.0**
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

P13437
13496
07/24/24
X.F.

Formulated By:	<i>Prashant Chauhan</i>	101122
Reviewed By:	<i>Pedro L. Rentas</i>	101122
	Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20482	1000.6	4.1	16416-32-3	N/A

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B = 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

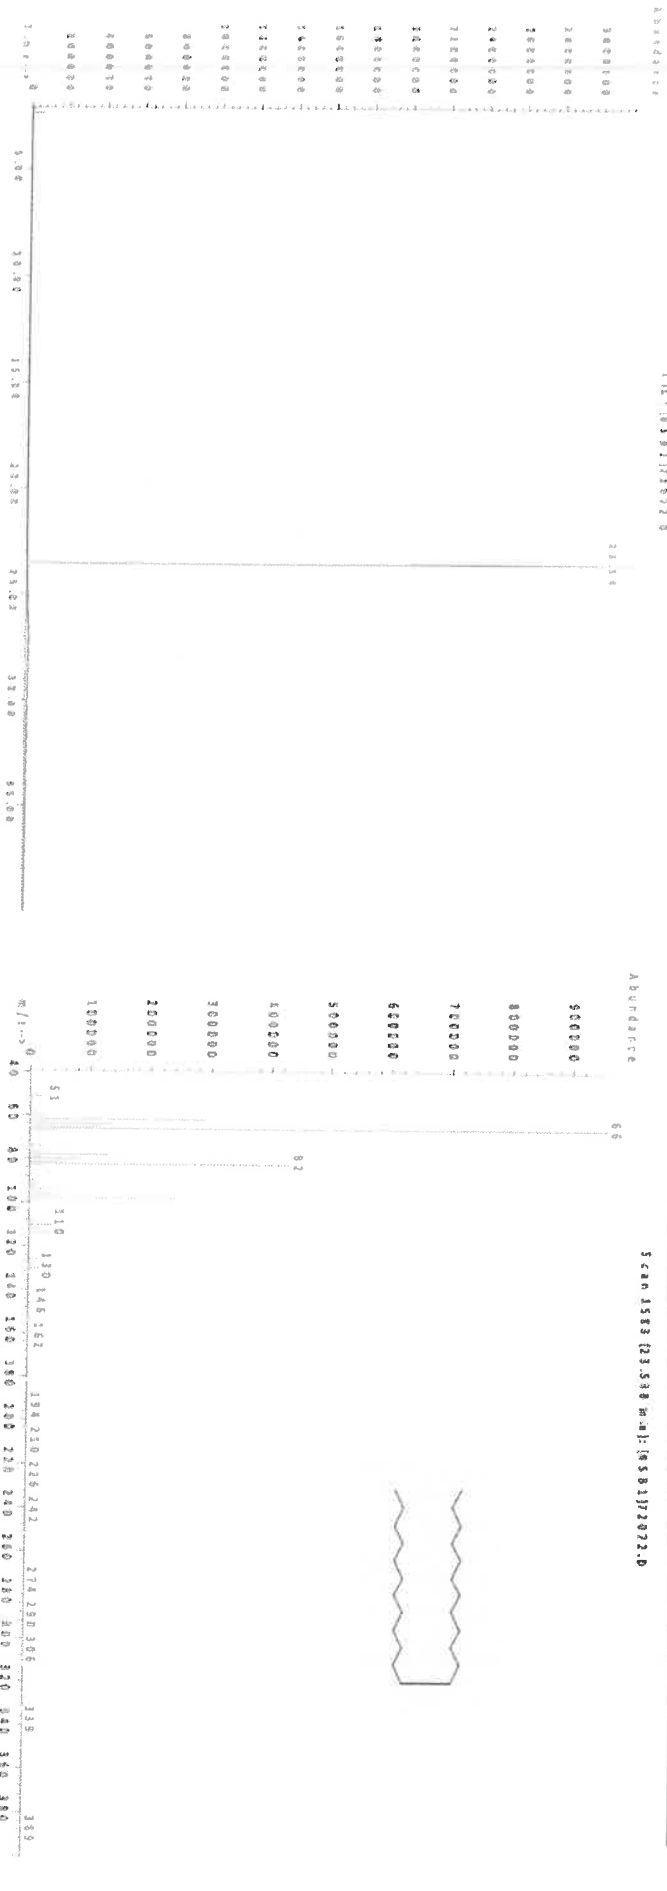

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty References: Taylor, B.N., and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

ABSOLUTE STANDARDS, INC.

ISO - 17034



Certificate of Analysis



Certified Reference Material (CRM)

Conformance: The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

Health & Safety: See the attached SDS & Certified Weight Report before use.

Intended Use: This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

Characterization Values: In production, gravimetric/volumetric readings are certified to be within $\pm 0.5\%$ of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

Homogeneity: Uncertainties that are due to the analytical procedure(s) are within $\pm 5\%$ unless specifically stated on the Certified Wt. Report.

Verification: Uncertainties that are due to the analytical procedure(s) are within $\pm 5\%$ unless specifically stated on the Certified Wt. Report.

Stability: Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

Uncertainty: UCRM is the expanded uncertainty which utilizes a $K = 2$ (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

Purity & Identity: Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neats are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

Storage: Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

Usage: Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

Minimum Sample Size: 0.5 uL for analytical applications.

Legal Notice: Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

Certifying Officer: Stephen J. Arpie, M.S., Director General

Page 1 of 2



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514
Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com
Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019



ABSOLUTE STANDARDS, INC.

ISO - 17034

Understanding the Certified Weight Report

Each Certified Reference Material (CRM) is supported by a Certified Weight Report. Assigned values for concentrations and associated uncertainties are based upon NIST traceable masses & volumes used in production.

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com

Certified Reference Material CRM

ISO 17034 Accredited
Scope: http://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT

Part # 10009R
Lot # 070716
Shelf Life 070716

Part Number: 10009R
Lot Number: 070716
Description: CLP Priority Pollutant Internal Standards
GC/MS Calibration - 6 components
Expiration Date: 070721
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 4000
NIST Test ID#: 822-275872-11
Weight(s) shown below were combined and diluted to (mL): 500.0

Solvent(s): Methylene chloride
Lot# 78782

5E-05 Balance Uncertainty
0.058 Peak Uncertainty

Formulated By: Paul Barron
Reviewed By: Pedro L. Rentes

070716
070716

MSDS Information
(Solvent Safety Info. On Attached pg.)

Compound	SMW	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty (%)	Target Weight (µg)	Actual Weight (µg)	Actual Conc (µg/mL)	Expanded Uncertainty (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. 1,4-Dichlorobenzene-d4	118	PR-1845M07287CB1	4000	98	0.2	2.04093	2.04335	4004.7	15.4	2055-02-1	N/A	or-nr 500mg/kg
2. Naphthalene-d8	223	PR-2339M031612HP1	4000	99	0.2	2.02032	2.02084	4001.0	15.2	1146-85-2	10 ppm (50mg/m3/8h)	or-nr 400mg/kg
3. Acenaphthene-d10	2	PR-25444	4000	99	0.2	2.02032	2.02245	4004.2	15.2	15067-28-2	N/A	or-nr 500mg/kg
4. Phenanthrene-d10	248	PR-2305M081711PM1	4000	98	0.2	2.04093	2.04135	4000.8	15.4	1517-25-2	N/A	N/A
5. Chrysene-d12	92	I-19290	4000	98	0.2	2.04093	2.04159	4001.3	15.4	1719-03-5	N/A	N/A
6. Perylene-d12	247	PR-24113	4000	98	0.2	2.04093	2.04155	4001.2	15.4	1503-58-3	N/A	N/A

Run 35, "P10009R L070716 [4000µg/mL in MeCl2]"
Run Length: 40.00 min, 23900 points at 10 points/second.
Created: Sat, Jul 9, 2016 at 1:54:53 PM.
Sampled: Sequence "070716-GC/MS", Method "GC-MS".
Analyzed using Method "GC-MS".

Comments
GC-MS Analysis by Melissa Siciric
Column ID SPB-5 30 meter x 0.53mm x 1.5um Film Thickness.
Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 0.5 mL, Helium (make-up) = 25 mL.
Hydrogen (detector) = 30 mL, Air (detector) = 300 mL, Oven Temp 1 = 50°C (1 min).
Rise = 10°C/min, Oven Temp 2 = 300°C (14 min). Total Run Time = 40 Minutes. Injector Temp = 250°C.
FID Temp = 300°C, FID Signal = aDaq Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 4

Peak Data

Peak No.	Name	FID RT (min)
1	1,4-Dichlorobenzene-d4	6.34
2	Naphthalene-d8	8.98
3	Acenaphthene-d10	12.97
4	Phenanthrene-d10	16.37
5	Chrysene-d12	22.62
6	Perylene-d12	25.75

Qualitative Quantitative

3rd Party Comparison

Analyte	Sup/Abs Dev (%)
1,4-Dichlorobenzene-d4	2.55
Naphthalene-d8	2.43
Acenaphthene-d10	2.74
Phenanthrene-d10	0.65
Chrysene-d12	1.93
Perylene-d12	-1.72
Total	-0.55

Printed: 5/8/2019, 12:55:50 PM

For More Information, Contact:

StephenArpie@AbsoluteStandards.com

Page 2 of 2



CERTIFIED WEIGHT REPORT

Part Number: **72072**
Lot Number: **101122**
Description: **n-Tetracosane-d50**

Solvent(s):
Methylene chloride
Lot#
105345


Expiration Date: **101132**
Recommended Storage: **Ambient (20 °C)**
Nominal Concentration (µg/mL): **1000**
NIST Test ID#: **6UB3**
Weight(s) shown below were combined and diluted to (mL): **200.0**
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

P13437
13436
07/24/24
X.F.

Formulated By:	<i>Prashant Chauhan</i>	101122
Reviewed By:	<i>Pedro L. Rentas</i>	101122
DATE		

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20482	1000.6	4.1	16416-32-3	N/A

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B = 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

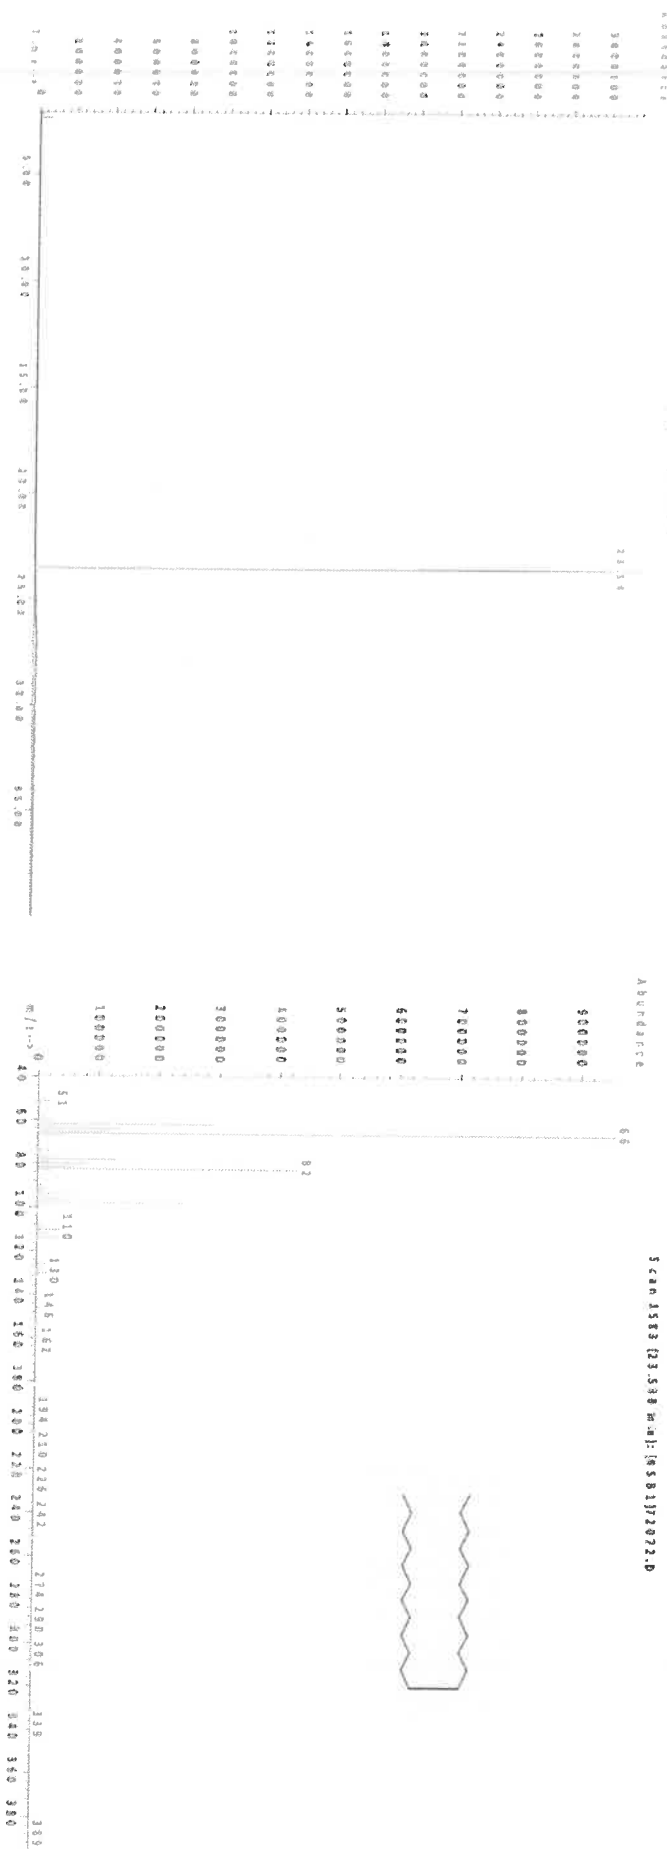

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N., and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

ABSOLUTE STANDARDS, INC.

ISO - 17034



Certificate of Analysis



Certified Reference Material (CRM)

Conformance: The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

Health & Safety: See the attached SDS & Certified Weight Report before use.

Intended Use: This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

Characterization Values: In production, gravimetric/volumetric readings are certified to be within $\pm 0.5\%$ of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

Homogeneity: Uncertainties that are due to the analytical procedure(s) are within $\pm 5\%$ unless specifically stated on the Certified Wt. Report.

Verification: Uncertainties that are due to the analytical procedure(s) are within $\pm 5\%$ unless specifically stated on the Certified Wt. Report.

Stability: Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

Uncertainty: UCRM is the expanded uncertainty which utilizes a $K = 2$ (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

Purity & Identity: Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neats are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

Storage: Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

Usage: Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

Minimum Sample Size: 0.5 uL for analytical applications.

Legal Notice: Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

Certifying Officer: Stephen J. Arpie, M.S., Director General

Page 1 of 2



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514
Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com
Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019



ABSOLUTE STANDARDS, INC.

ISO - 17034

Understanding the Certified Weight Report

Each Certified Reference Material (CRM) is supported by a Certified Weight Report. Assigned values for concentrations and associated uncertainties are based upon NIST traceable masses & volumes used in production.

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com

Certified Reference Material CRM

ISO 17034 Accredited
Scope: http://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT

Part # 10009R
Lot # 070716
Shelf Life Description: CLP Priority Pollutant Internal Standards
GC/MS Calibration - 6 components
070721
Expiration Date: Ambient (20 °C)
Recommended Storage: 4000
Nominal Concentration (µg/mL): 822-275872-11
NIST Test ID#: 5E-05 Balance Uncertainty
0.058 Mass Uncertainty

Solvent(s): Methylene chloride
Lot# 78782

Formulated By: Paul Barron
Reviewed By: Pedro L. Rentes

070716
070716

Weight(s) shown below were combined and diluted to (mL): 500.0

Compound	SMW	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (µg)	Actual Weight (µg)	Actual Conc (µg/mL)	Expanded Uncertainty (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. 1,4-Dichlorobenzene-d4	118	PR-1845M07287CB1	4000	98	0.2	2.04093	2.04335	4004.7	15.4	2055-02-1	N/A	or-rat 500mg/kg
2. Naphthalene-d8	223	PR-2339M031612HP1	4000	99	0.2	2.02032	2.02084	4001.0	15.2	1146-85-2	10 ppm (50mg/m3/8h)	or-rat 400mg/kg
3. Acenaphthene-d10	2	PR-25444	4000	99	0.2	2.02032	2.02245	4004.2	15.2	15067-28-2	N/A	or-rat 500mg/kg
4. Phenanthrene-d10	248	PR-2305M081711PM1	4000	98	0.2	2.04093	2.04135	4000.8	15.4	1517-25-2	N/A	N/A
5. Chrysene-d12	92	I-19290	4000	98	0.2	2.04093	2.04150	4001.3	15.4	1719-03-5	N/A	N/A
6. Perylene-d12	247	PR-24113	4000	98	0.2	2.04093	2.04155	4001.2	15.4	1503-58-3	N/A	N/A

Run 35, "P10009R L070716 [4000µg/mL in MeCl2]"
Run Length: 40.00 min, 23900 points at 10 points/second.
Created: Sat, Jul 9, 2016 at 1:54:53 PM.
Sampled: Sequence "070716-GC/MS", Method "GC-MS".
Analyzed using Method "GC-MS".

Comments:
GC-MS Analysis by Melissa Siciric
Column ID SPB-5 30 meter x 0.53mm x 1.5um Film Thickness.
Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 0.5 mL, Helium (make-up) = 25 mL.
Hydrogen (detector) = 30 mL, Air (detector) = 300 mL, Oven Temp 1 = 50°C (1 min).
Rise = 10°C/min, Oven Temp 2 = 300°C (14 min), Total Run Time = 40 Minutes, Injector Temp = 250°C.
FID Temp = 300°C, FID Signal = sData Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 4

Peak No. Name FID RT (min)

1	1,4-Dichlorobenzene-d4	8.34
2	Naphthalene-d8	8.98
3	Acenaphthene-d10	12.97
4	Phenanthrene-d10	16.37
5	Chrysene-d12	22.62
6	Perylene-d12	25.75

Supra, Inc. PP10009R L070716
Supra, Inc. PP10009R L070716

Analyte	Sup/Abs Dev (%)
1,4-Dichlorobenzene-d4	2.55
Naphthalene-d8	2.43
Acenaphthene-d10	2.74
Phenanthrene-d10	0.65
Chrysene-d12	1.93
Perylene-d12	-1.72
Total	-0.55

Printed: 5/8/2019, 12:55:50 PM

Formulator
Reviewer

Actual
Concentration
Uncertainty
Values

Health &
Safety

3rd Party
Comparison

For More Information, Contact:

StephenArpie@AbsoluteStandards.com

Page 2 of 2



CERTIFIED WEIGHT REPORT

Part Number: **72072**
Lot Number: **101122**
Description: **n-Tetracosane-d50**

Solvent(s):
Methylene chloride
Lot#
105345



Expiration Date: **101132**
Recommended Storage: **Ambient (20 °C)**
Nominal Concentration (µg/mL): **1000**
NIST Test ID#: **6UB3**
Weight(s) shown below were combined and diluted to (mL): **200.0**
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

P13437
13496
07/24/24
X.F.

Formulated By:	<i>Prashant Chauhan</i>	101122
Reviewed By:	<i>Pedro L. Rentas</i>	101122
DATE		DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20482	1000.6	4.1	16416-32-3	N/A

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B = 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

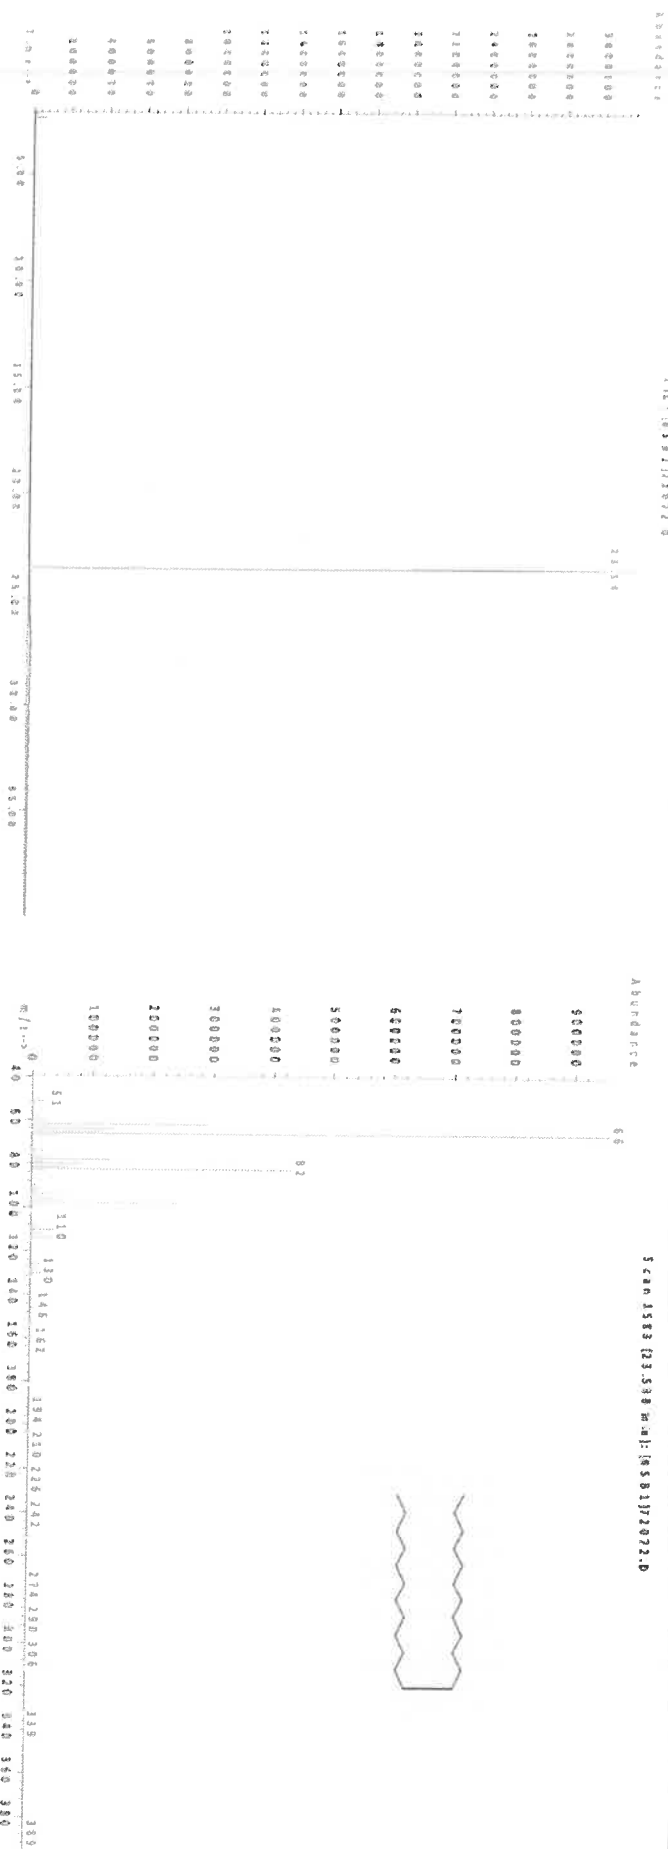

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N., and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

ABSOLUTE STANDARDS, INC.

ISO - 17034



Certificate of Analysis



Certified Reference Material (CRM)

Conformance: The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

Health & Safety: See the attached SDS & Certified Weight Report before use.

Intended Use: This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

Characterization Values: In production, gravimetric/volumetric readings are certified to be within $\pm 0.5\%$ of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

Homogeneity: Uncertainties that are due to the analytical procedure(s) are within $\pm 5\%$ unless specifically stated on the Certified Wt. Report.

Verification: Uncertainties that are due to the analytical procedure(s) are within $\pm 5\%$ unless specifically stated on the Certified Wt. Report.

Stability: Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

Uncertainty: UCRM is the expanded uncertainty which utilizes a $K = 2$ (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

Purity & Identity: Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neats are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

Storage: Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

Usage: Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

Minimum Sample Size: 0.5 uL for analytical applications.

Legal Notice: Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

Certifying Officer: Stephen J. Arpie, M.S., Director General

Page 1 of 2



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514
Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com
Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019



ABSOLUTE STANDARDS, INC.

ISO - 17034

Understanding the Certified Weight Report

Each Certified Reference Material (CRM) is supported by a Certified Weight Report. Assigned values for concentrations and associated uncertainties are based upon NIST traceable masses & volumes used in production.

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com

Certified Reference Material CRM

ISO 17034 Accredited
Scope: http://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT

Part # 10009R
Lot # 070716
Shelf Life Description: CLP Priority Pollutant Internal Standards
GC/MS Calibration - 6 components
070721
Expiration Date: Ambient (20 °C)
Recommended Storage: 4000
Nominal Concentration (µg/mL): 822-275872-11
NIST Test ID#: 5E-05 Balance Uncertainty
0.058 Mass Uncertainty

Solvent(s): Methylene chloride
Lot# 78782

Formulated By: Paul Barron
Reviewed By: Pedro L. Rentes

070716
070716

Weight(s) shown below were combined and diluted to (mL): 500.0

Compound	SMW	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (µg)	Actual Weight (µg)	Actual Conc (µg/mL)	Expanded Uncertainty (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. 1,4-Dichlorobenzene-d4	118	PR-1845M07287CB1	4000	98	0.2	2.04093	2.04335	4004.7	15.4	2055-02-1	N/A	or-rat 500mg/kg
2. Naphthalene-d8	223	PR-2339M031612HP1	4000	99	0.2	2.02032	2.02084	4001.0	15.2	1146-85-2	10 ppm (50mg/m3/8h)	or-rat 400mg/kg
3. Acenaphthene-d10	2	PR-25444	4000	99	0.2	2.02032	2.02245	4004.2	15.2	15067-28-2	N/A	or-rat 500mg/kg
4. Phenanthrene-d10	248	PR-2305M081711PM1	4000	98	0.2	2.04093	2.04135	4000.8	15.4	1517-25-2	N/A	N/A
5. Chrysene-d12	92	I-19290	4000	98	0.2	2.04093	2.04150	4001.3	15.4	1719-03-5	N/A	N/A
6. Perylene-d12	247	PR-24113	4000	98	0.2	2.04093	2.04155	4001.2	15.4	1503-58-3	N/A	N/A

Run 35, "P10009R L070716 [4000µg/mL in MeCl2]"
Run Length: 40.00 min, 23900 points at 10 points/second.
Created: Sat, Jul 9, 2016 at 1:54:53 PM.
Sampled: Sequence "070716-GC/MS", Method "GC-MS".
Analyzed using Method "GC-MS".

Comments:
GC-MS Analysis by Melissa Siciric
Column ID SPB-5 30 meter x 0.53mm x 1.5um Film Thickness.
Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 0.5 mL, Helium (make-up) = 25 mL.
Hydrogen (detector) = 30 mL, Air (detector) = 300 mL, Oven Temp 1 = 50°C (1 min).
Rise = 10°C/min, Oven Temp 2 = 300°C (14 min). Total Run Time = 40 Minutes. Injector Temp = 250°C.
FID Temp = 300°C, FID Signal = sData Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 4

Peak No. Name FID RT (min)

1	1,4-Dichlorobenzene-d4	8.34
2	Naphthalene-d8	8.98
3	Acenaphthene-d10	12.97
4	Phenanthrene-d10	16.37
5	Chrysene-d12	22.62
6	Perylene-d12	25.75

Supra, Inc. PP10009R L070716
Supra, Inc. PP10009R L070716

Analyte	Sup/Abs Dev (%)
1,4-Dichlorobenzene-d4	2.55
Naphthalene-d8	2.43
Acenaphthene-d10	2.74
Phenanthrene-d10	0.65
Chrysene-d12	1.93
Perylene-d12	-1.72
Total	-0.55

Printed: 5/8/2019, 12:55:50 PM

Formulator
Reviewer

Actual
Concentration
Uncertainty
Values

Health &
Safety

3rd Party
Comparison

For More Information, Contact:

StephenArpie@AbsoluteStandards.com

Page 2 of 2



CERTIFIED WEIGHT REPORT

Part Number: **72072**
Lot Number: **101122**
Description: **n-Tetracosane-d50**

Solvent(s):
Methylene chloride

Lot#
105345


Expiration Date: **101132**
Recommended Storage: **Ambient (20 °C)**
Nominal Concentration (µg/mL): **1000**
NIST Test ID#: **6UB3**
Weight(s) shown below were combined and diluted to (mL): **200.0**
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

P13437
13496
07/24/24

Formulated By:	<i>Prashant Chauhan</i>	101122
Reviewed By:	<i>Pedro L. Rentas</i>	101122
DATE		DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)	LD50
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	------------------------------------	--	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20482 1000.6 4.1 16416-32-3 N/A
Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B = 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

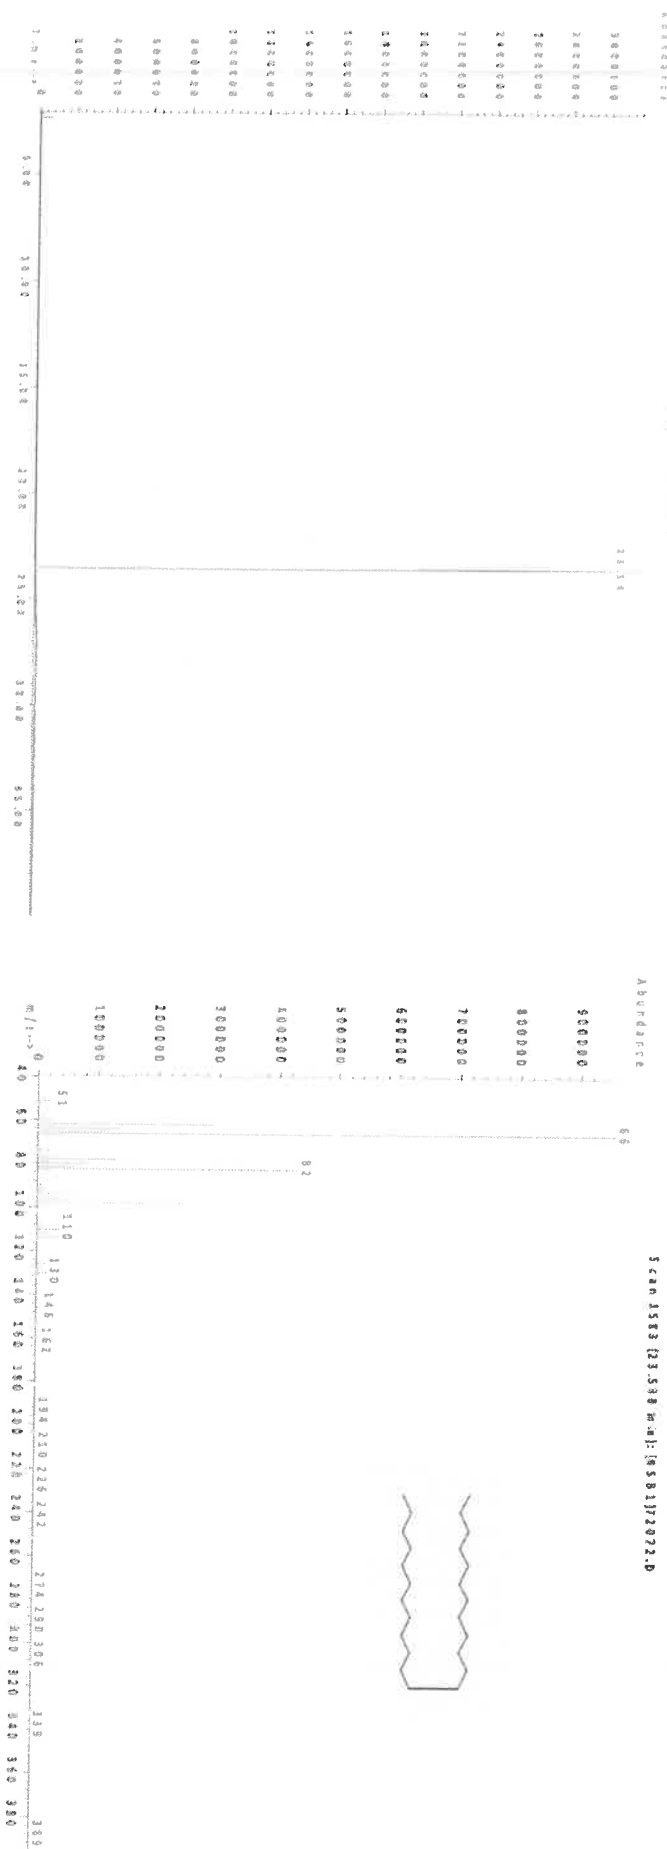

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N., and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

