
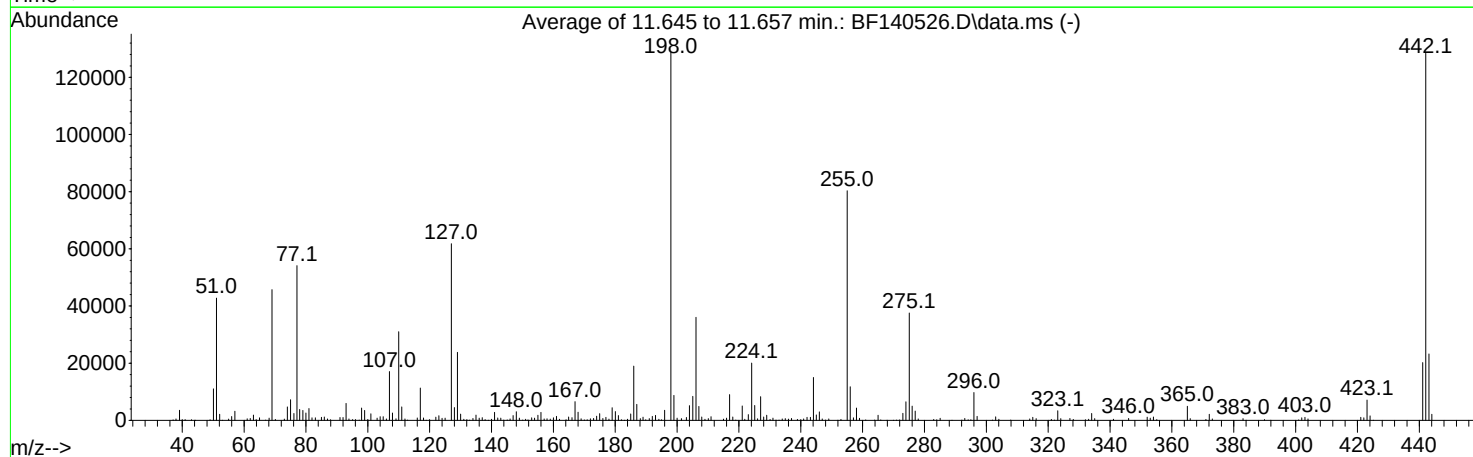


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140526.D
Acq On : 21 Nov 2024 10:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

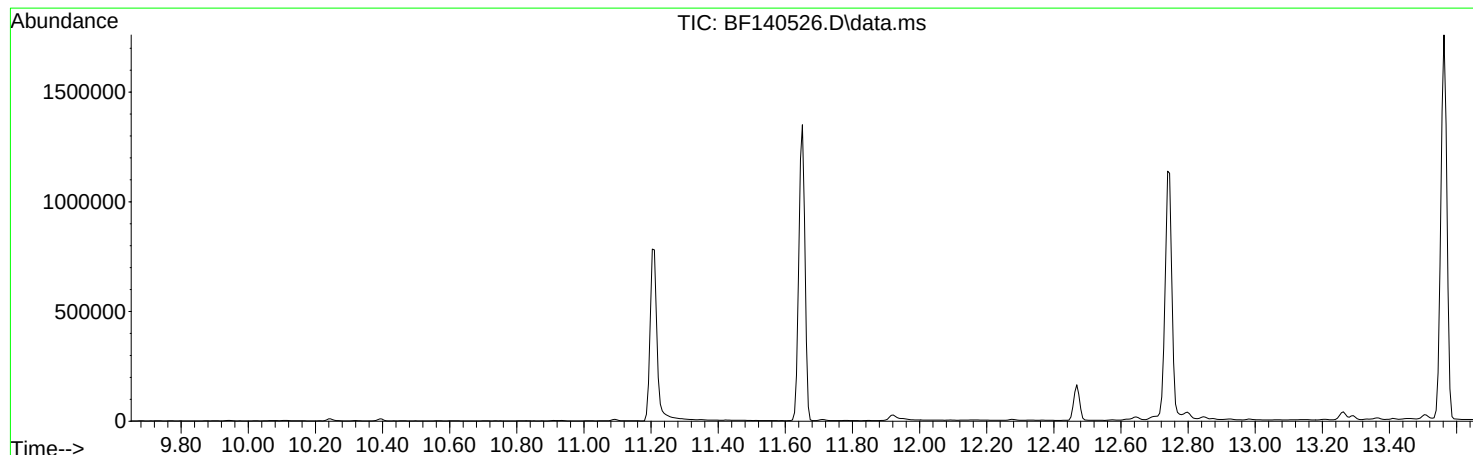

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	42792	PASS
68	69	0.00	2	1.8	810	PASS
69	198	0.00	100	35.5	45731	PASS
70	69	0.00	2	0.7	327	PASS
127	198	10	80	48.0	61811	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128688	PASS
199	198	5	9	6.8	8723	PASS
275	198	10	60	29.2	37552	PASS
365	198	1	100	3.8	4944	PASS
441	198	0.01	100	15.7	20189	PASS
442	442	50	100	100.0	128421	PASS
443	442	15	24	18.1	23261	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/21/2024	BNA_F	<u>BF140526.D</u>
Compound Name	Response	Retention Time
DDT	424151	13.562
DDD	14557	13.262
DDE	1132	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15689	439840	3.57

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
 Data File : BF140526.D
 Acq On : 21 Nov 2024 10:17
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP




Quant Time: Nov 21 15:24:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 15:23:48 2024
 Response via : Initial Calibration



Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140526.D
Acq On : 21 Nov 2024 10:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 21 15:24:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

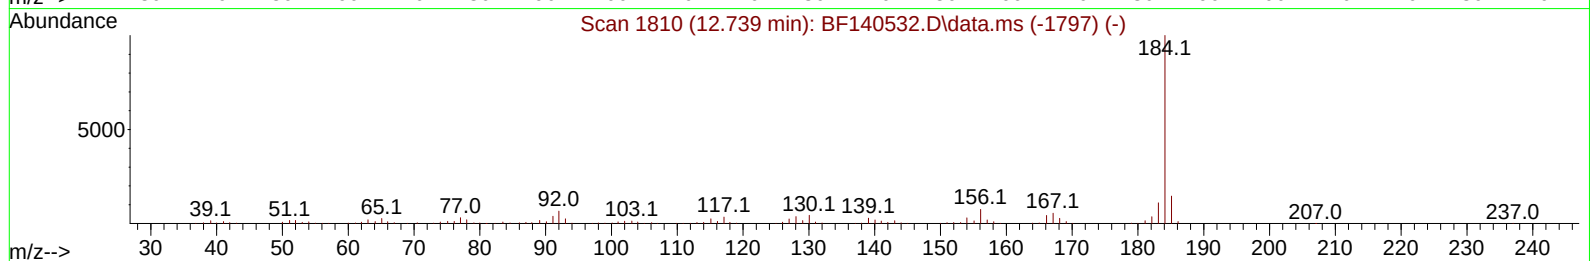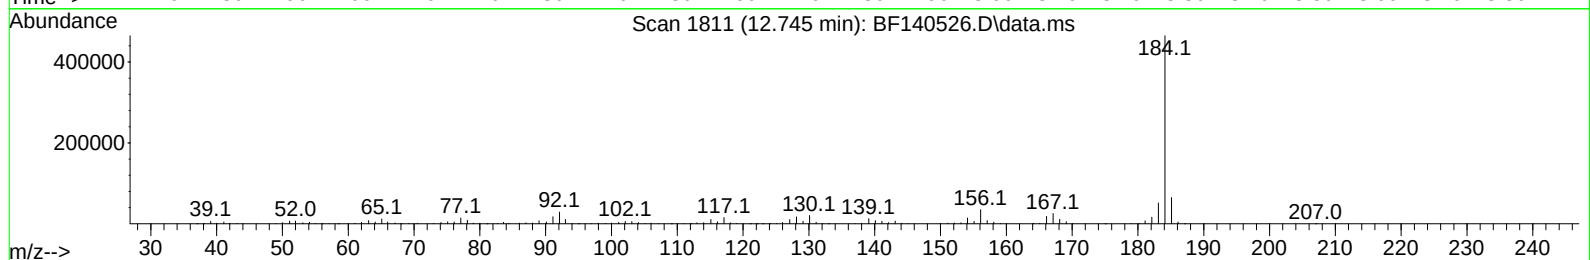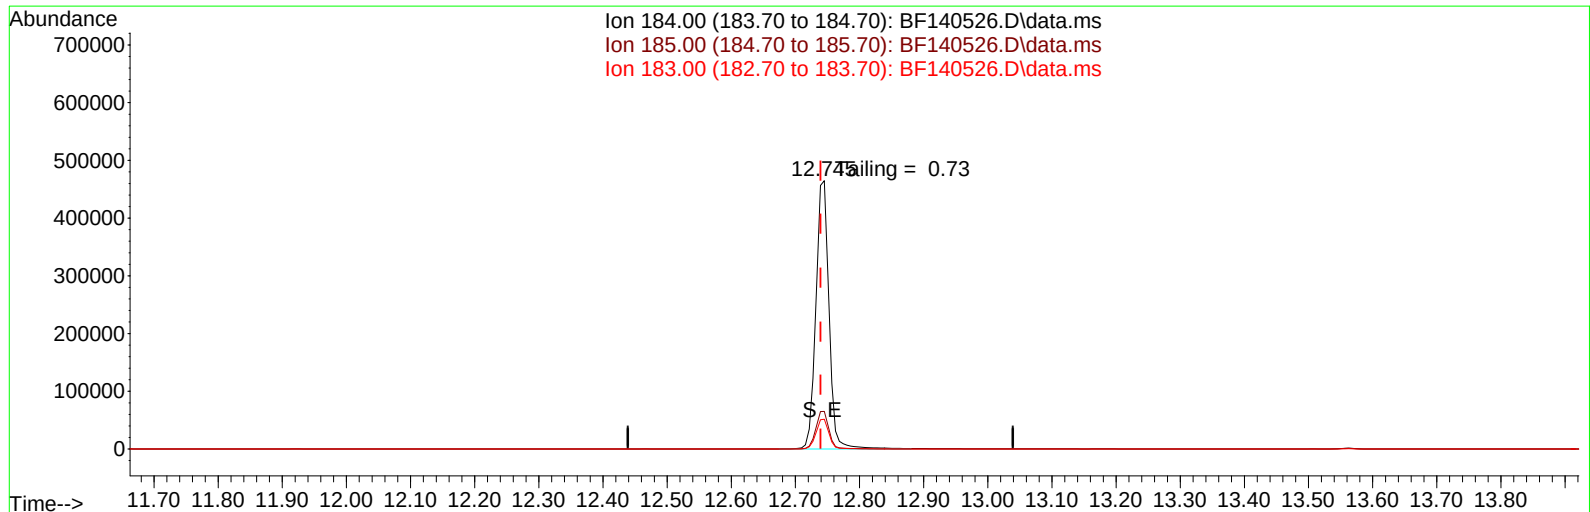

TIC: BF140526.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 32779.12 ng

response 668077

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.02
183.00	11.00	11.11
0.00	0.00	0.00