

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111824\
Data File : FF015080.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2024 12:00
Operator : YP\AJ
Sample : P4839-21
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EX-4-TPH-5

Integration File: autoint1.e
Quant Time: Nov 19 00:21:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111324.M
Quant Title :
QLast Update : Wed Nov 13 12:50:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.021	1802060	16.349 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111824\
Data File : FF015080.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2024 12:00
Operator : YP\AJ
Sample : P4839-21
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EX-4-TPH-5

Integration File: autoint1.e
Quant Time: Nov 19 00:21:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111324.M
Quant Title :
QLast Update : Wed Nov 13 12:50:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

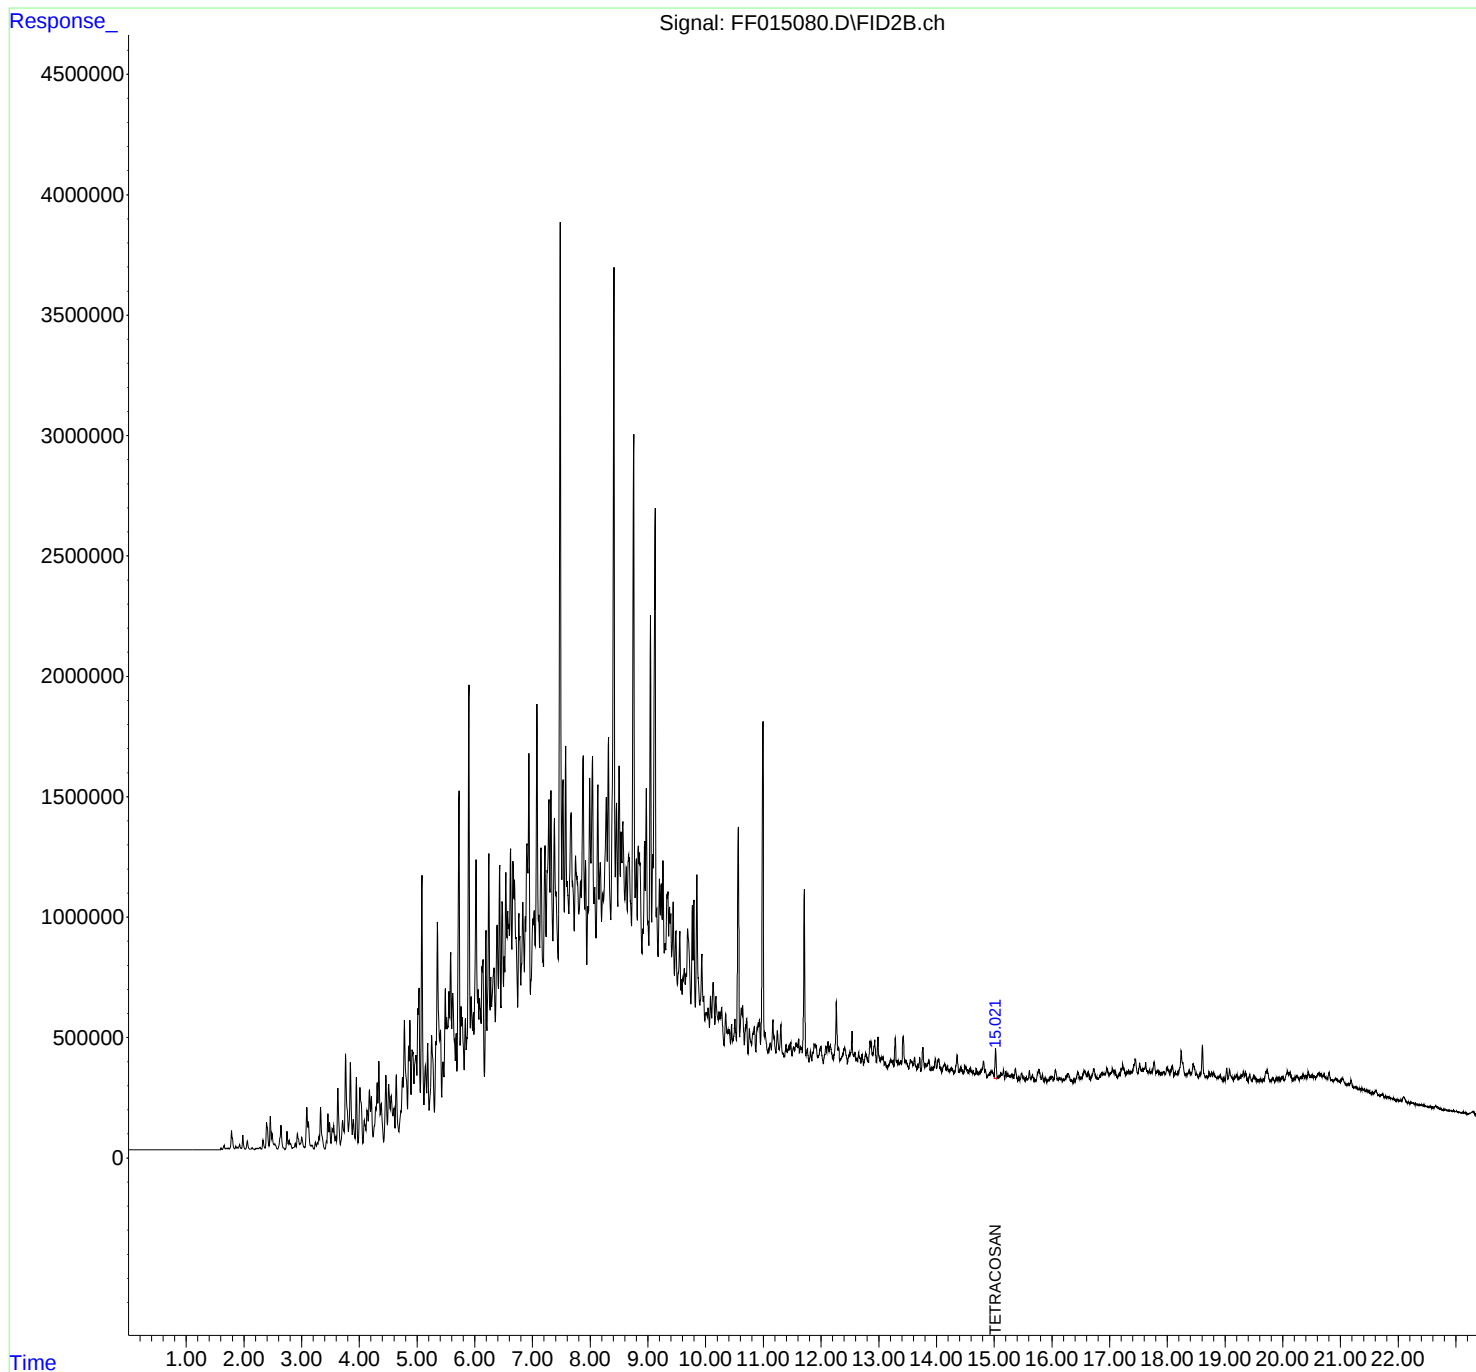

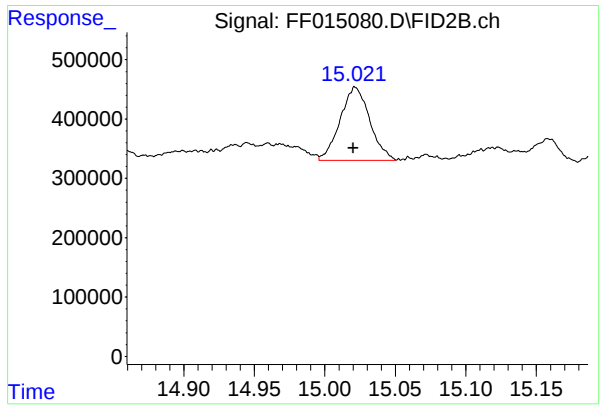

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.021 min
Delta R.T.: 0.000 min
Response: 1802060
Conc: 16.35 ug/ml

Instrument :
FID_F
ClientSampleId :
EX-4-TPH-5