

Ident	Instrument IC-1			Analyst: NF		Method: 300.0 / 9056A		Initial w Analyst		
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	
STD1	0	0	0	0	0	0	0	IC1-101624	10/16/2024 10:55	10 NF/IZ
STD2	0.424	0.632	0.639	2.106	0.535	1.072	3.276	IC1-101624	10/16/2024 11:17	10 NF/IZ
STD3	0.796	1.206	1.205	4.013	1	2	6.052	IC1-101624	10/16/2024 11:38	10 NF/IZ
STD4	1.032	1.537	1.531	5.116	1.277	2.557	7.662	IC1-101624	10/16/2024 11:59	10 NF/IZ
STD5	1.966	2.927	2.921	9.77	2.439	4.871	14.51	IC1-101624	10/16/2024 12:21	10 NF/IZ
STD6	3.88	5.901	5.91	19.683	4.912	9.831	29.286	IC1-101624	10/16/2024 12:42	10 NF/IZ
STD7	5.102	7.598	7.593	25.312	6.337	12.67	37.714	IC1-101624	10/16/2024 13:04	10 NF/IZ
ICV	1.966	2.997	3	9.969	2.497	4.753	14.85	IC1-101624	10/16/2024 13:37	10 NF/IZ
ICB	0	0	0	0	0	0	0	IC1-101624	10/16/2024 13:59	10 NF/IZ
CCV	2.104	3.126	3.09	10.436	2.625	5.261	15.528	IC1-101624	11/14/2024 10:35	10 NF/IZ
CCB	0	0	0	0	0	0	0	IC1-101624	11/14/2024 10:56	10 NF/IZ
LB133442BLW	0	0	0	0	0	0	0	IC1-101624	11/14/2024 11:18	10 NF/IZ
LB133442BSW	2.061	3.073	3.082	10.274	2.581	5.133	15.168	IC1-101624	11/14/2024 11:39	10 NF/IZ
P4843-01	0.53	24.432	0.179	0.823	0.802	0	540.327	IC1-101624	11/14/2024 12:01	10 NF/IZ
P4843-01MS	2.479	26.82	3.199	11.391	3.598	0.795	532.358	IC1-101624	11/14/2024 12:22	10 NF/IZ
P4843-01MSD	2.48	26.786	3.203	11.323	3.589	1.167	531.158	IC1-101624	11/14/2024 12:44	10 NF/IZ
P4843-01DLX10	0.081	2.34	0	0	0	0	42.586	IC1-101624	11/14/2024 13:06	10 NF/IZ
CCV	1.963	2.926	2.959	9.651	2.435	4.943	14.593	IC1-101624	11/14/2024 13:27	10 NF/IZ
CCB	0	0	0	0	0	0	0	IC1-101624	11/14/2024 13:49	10 NF/IZ

Clear table


Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A

ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentratio n HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-101624	10/16/2024 10:55	10	NF/IZ
STD2	0.424	0.632	0.639	2.106	0.535	1.072	3.276	IC1-101624	10/16/2024 11:17	10	NF/IZ
STD3	0.796	1.206	1.205	4.013	1.000	2.000	6.052	IC1-101624	10/16/2024 11:38	10	NF/IZ
STD4	1.032	1.537	1.531	5.116	1.277	2.557	7.662	IC1-101624	10/16/2024 11:59	10	NF/IZ
STD5	1.966	2.927	2.921	9.77	2.439	4.871	14.51	IC1-101624	10/16/2024 12:21	10	NF/IZ
STD6	3.88	5.901	5.91	19.683	4.912	9.831	29.286	IC1-101624	10/16/2024 12:42	10	NF/IZ
STD7	5.102	7.598	7.593	25.312	6.337	12.67	37.714	IC1-101624	10/16/2024 13:04	10	NF/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	6.0000	5.3333	6.5000	5.3000	7.0000	7.2000	9.2000
STD3	-0.5000	0.5000	0.4167	0.3250	0.0000	0.0000	0.8667
STD4	3.2000	2.4667	2.0667	2.3200	2.1600	2.2800	2.1600
STD5	-1.7000	-2.4333	-2.6333	-2.3000	-2.4400	-2.5800	-3.2667
STD6	-3.0000	-1.6500	-1.5000	-1.5850	-1.7600	-1.6900	-2.3800
STD7	2.0400	1.3067	1.2400	1.2480	1.3920	1.3600	1.9297

Fluoride (Anions)

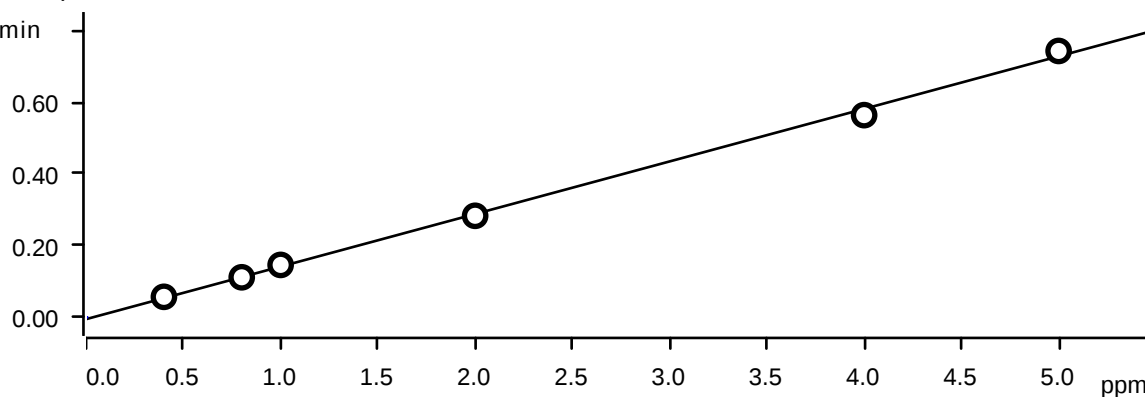
 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -5.06114E-3 + 0.0146570 \times Q$

Relative standard deviation 3.824450 %

Correlation coefficient 0.999229

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.112	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.146	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.283	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.564	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.743	STD7	2024-10-16 13:04:15 UTC-4	used


Chloride (Anions)

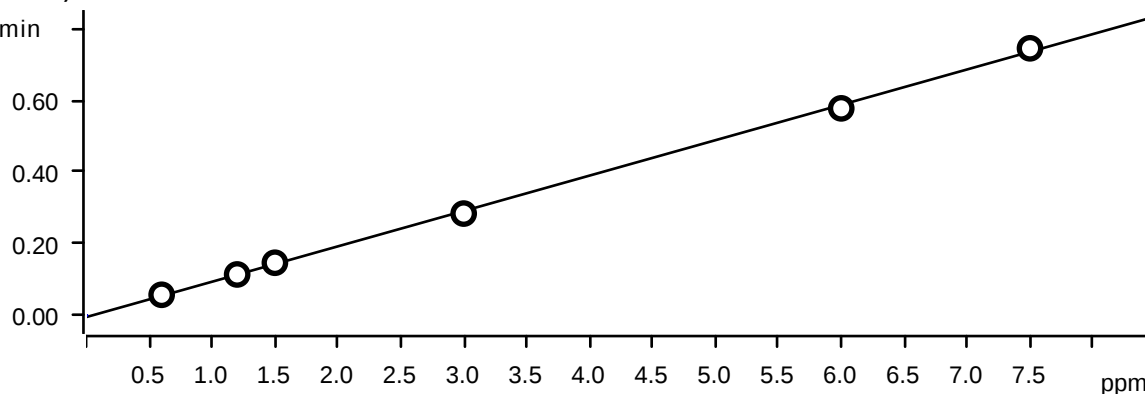 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -4.66155E-3 + 9.86442E-3 \times Q$

Relative standard deviation 2.532075 %

Correlation coefficient 0.999661

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.058	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.114	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.147	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.284	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.577	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.745	STD7	2024-10-16 13:04:15 UTC-4	used

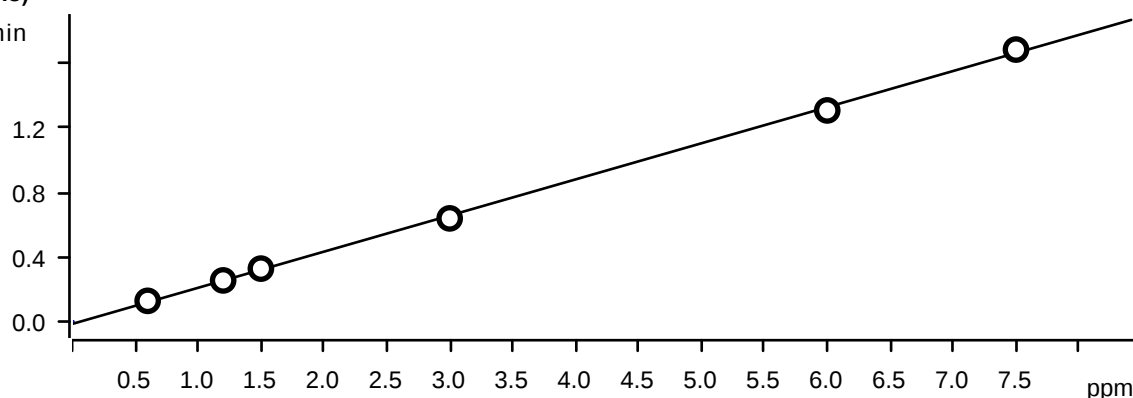Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0158639 + 0.0223869 \times Q$


Relative standard deviation 2.476730 %

Correlation coefficient 0.999680

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.127	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.254	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.638	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.307	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.684	STD7	2024-10-16 13:04:15 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

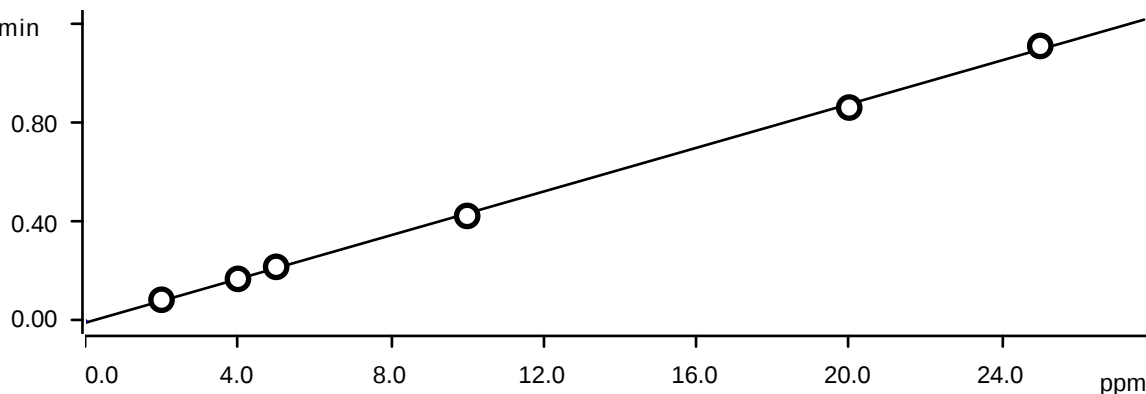

Function: $A = -7.83486E-3 + 4.40426E-3 \times Q$


Relative standard deviation 2.425045 %

Correlation coefficient 0.999690

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.085	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.217	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.422	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.859	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.107	STD7	2024-10-16 13:04:15 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

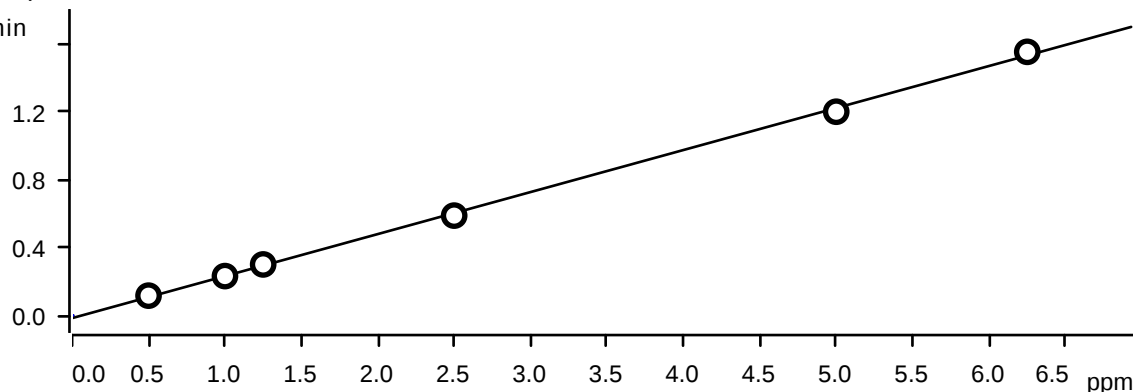


Function: $A = -0.0159932 + 0.0247327 \times Q$

Relative standard deviation 2.693966 %

Correlation coefficient 0.999623

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.116	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.231	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.300	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.587	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.199	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.551	STD7	2024-10-16 13:04:15 UTC-4	used

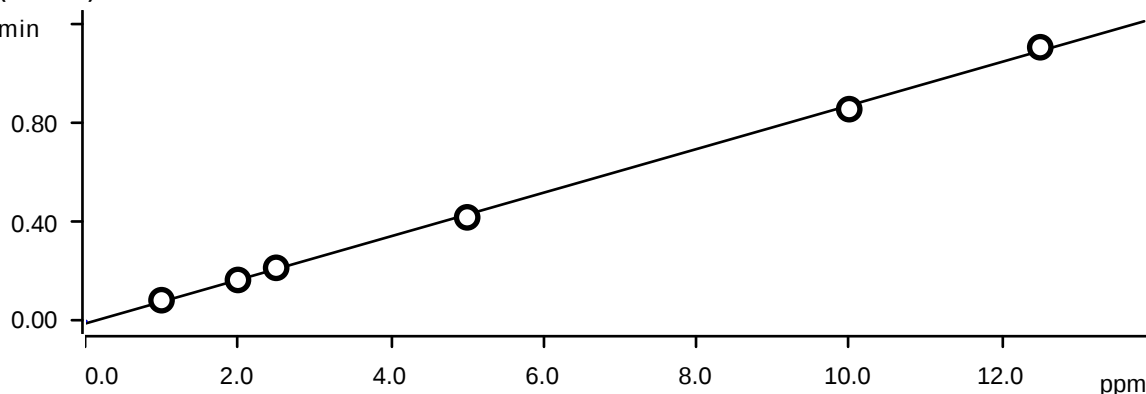
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -9.96170E-3 + 8.78405E-3 \times Q$

Relative standard deviation 2.667639 %

Correlation coefficient 0.999628

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.084	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.166	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.215	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.418	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.854	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.103	STD7	2024-10-16 13:04:15 UTC-4	used

Sulfate (Anions)

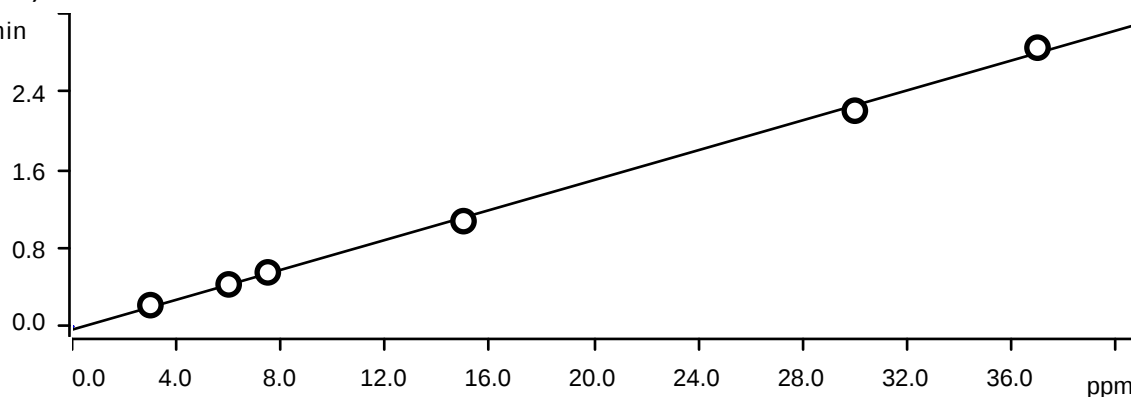 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0322401 + 7.64234E-3 \times Q$

Relative standard deviation 3.651427 %

Correlation coefficient 0.999303


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.430	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.553	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.077	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.206	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.850	STD7	2024-10-16 13:04:15 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2024-10-16 10:55:46 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

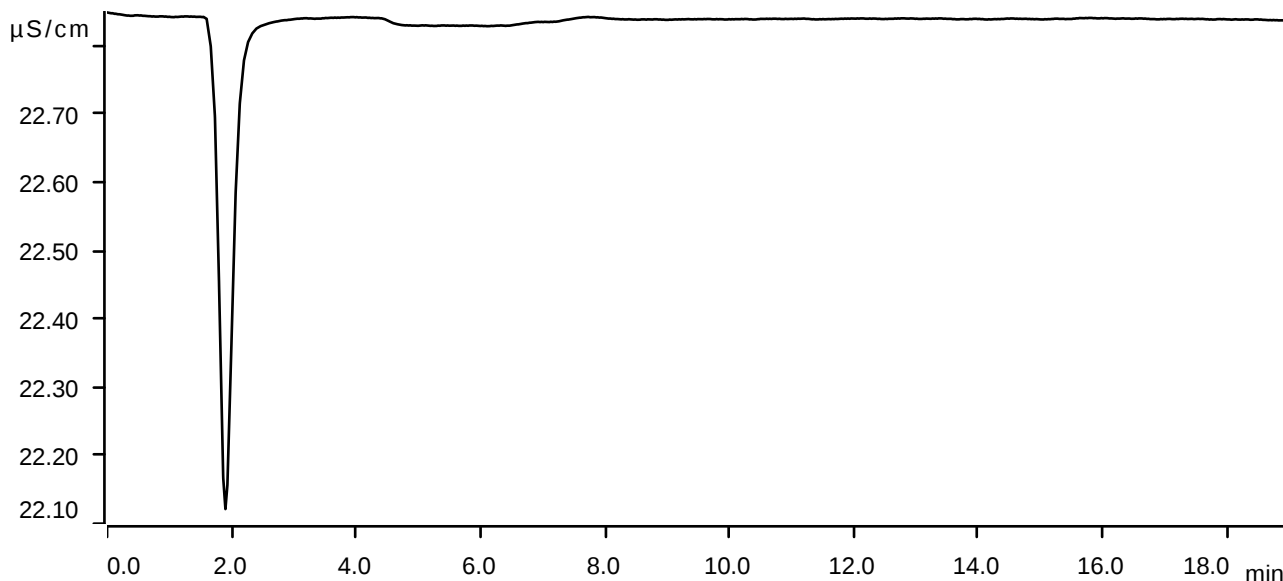Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2024-10-16 11:17:08 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

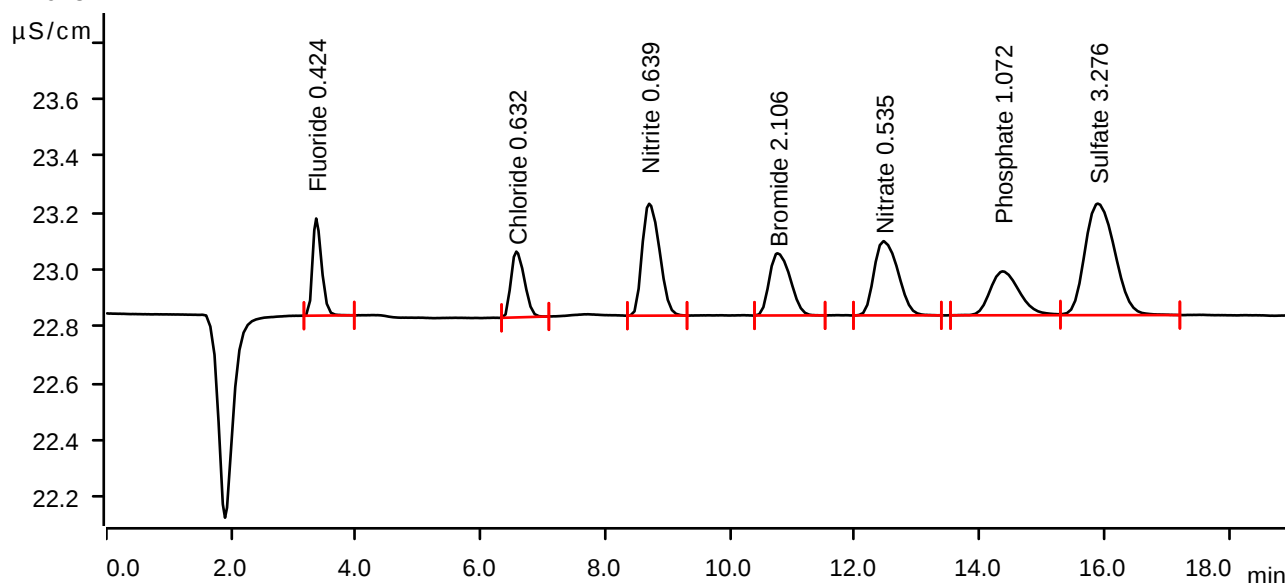

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.365	0.0571	0.341	0.424	Fluoride
2	6.573	0.0576	0.231	0.632	Chloride
3	8.703	0.1273	0.393	0.639	Nitrite
4	10.758	0.0849	0.219	2.106	Bromide
5	12.458	0.1163	0.261	0.535	Nitrate
6	14.368	0.0842	0.154	1.072	Phosphate
7	15.893	0.2181	0.392	3.276	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2024-10-16 11:38:32 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

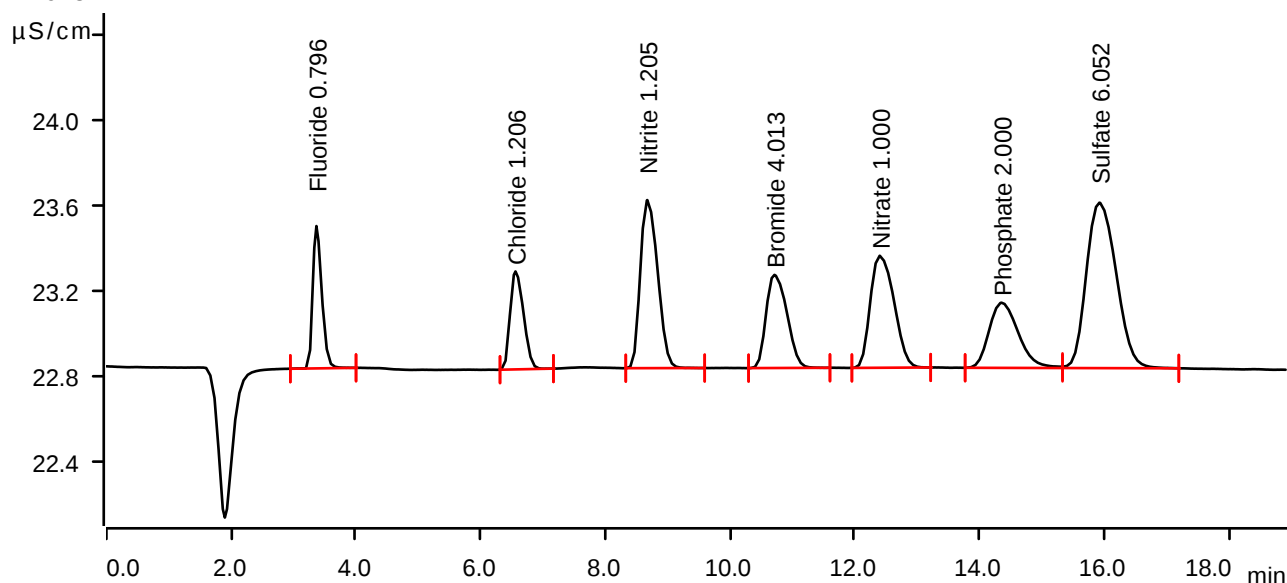

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.368	0.1116	0.667	0.796	Fluoride
2	6.560	0.1143	0.459	1.206	Chloride
3	8.673	0.2538	0.788	1.205	Nitrite
4	10.712	0.1689	0.436	4.013	Bromide
5	12.398	0.2314	0.525	1.000	Nitrate
6	14.353	0.1657	0.305	2.000	Phosphate
7	15.922	0.4302	0.775	6.052	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2024-10-16 11:59:57 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

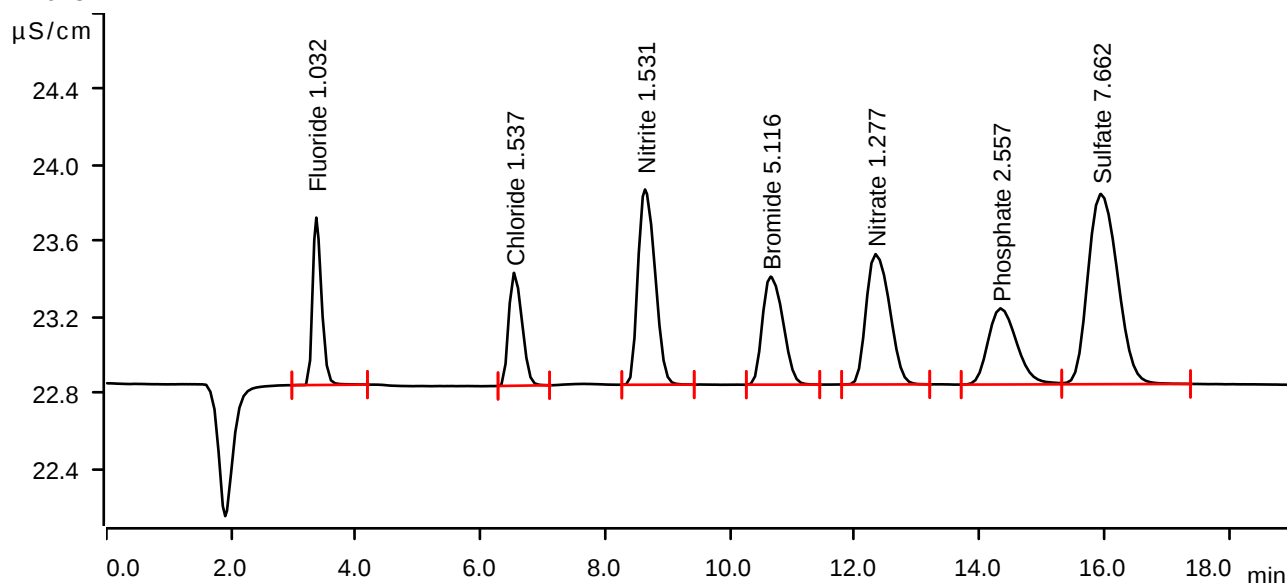

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.367	0.1462	0.882	1.032	Fluoride
2	6.537	0.1469	0.595	1.537	Chloride
3	8.637	0.3270	1.029	1.531	Nitrite
4	10.650	0.2175	0.569	5.116	Bromide
5	12.332	0.2999	0.687	1.277	Nitrate
6	14.337	0.2147	0.401	2.557	Phosphate
7	15.945	0.5533	1.003	7.662	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2024-10-16 12:21:22 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

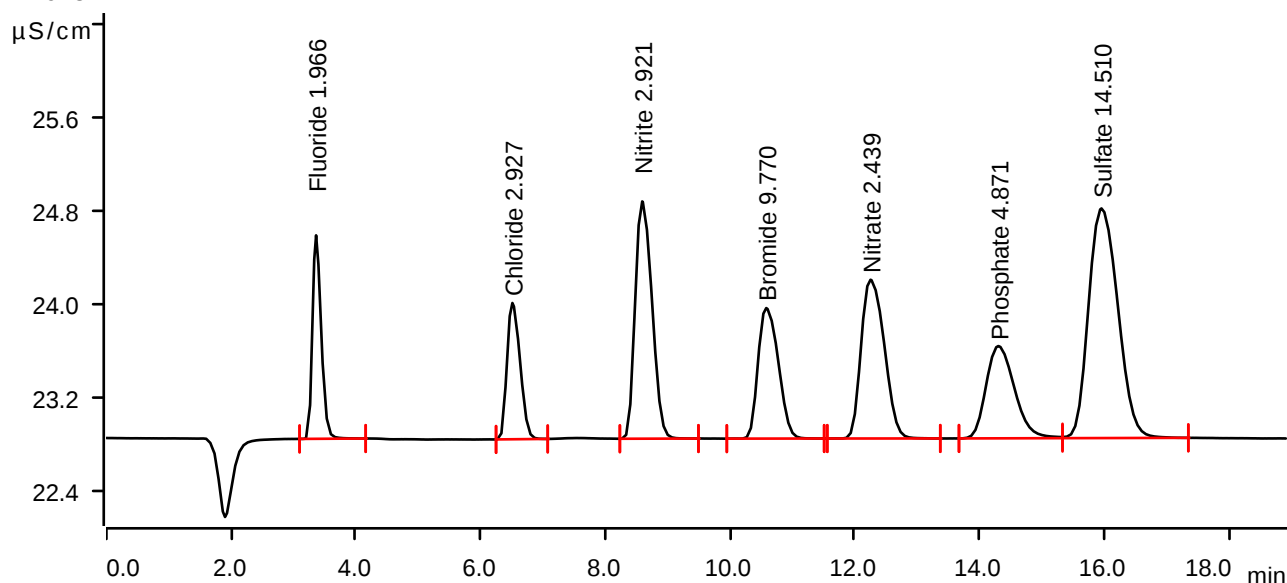

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.2831	1.748	1.966	Fluoride
2	6.510	0.2841	1.170	2.927	Chloride
3	8.592	0.6381	2.038	2.921	Nitrite
4	10.580	0.4225	1.121	9.770	Bromide
5	12.252	0.5873	1.364	2.439	Nitrate
6	14.302	0.4179	0.793	4.871	Phosphate
7	15.955	1.0767	1.972	14.510	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2024-10-16 12:42:48 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

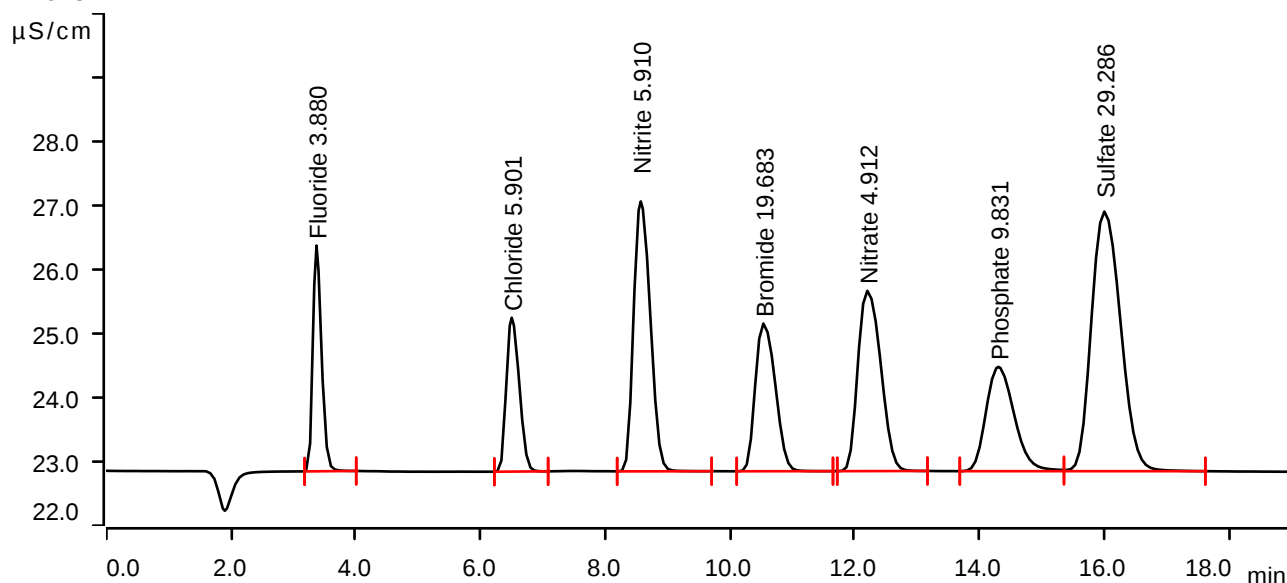

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.370	0.5637	3.525	3.880	Fluoride
2	6.500	0.5774	2.404	5.901	Chloride
3	8.568	1.3072	4.215	5.910	Nitrite
4	10.535	0.8590	2.306	19.683	Bromide
5	12.202	1.1988	2.815	4.912	Nitrate
6	14.302	0.8536	1.629	9.831	Phosphate
7	16.002	2.2059	4.054	29.286	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2024-10-16 13:04:15 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

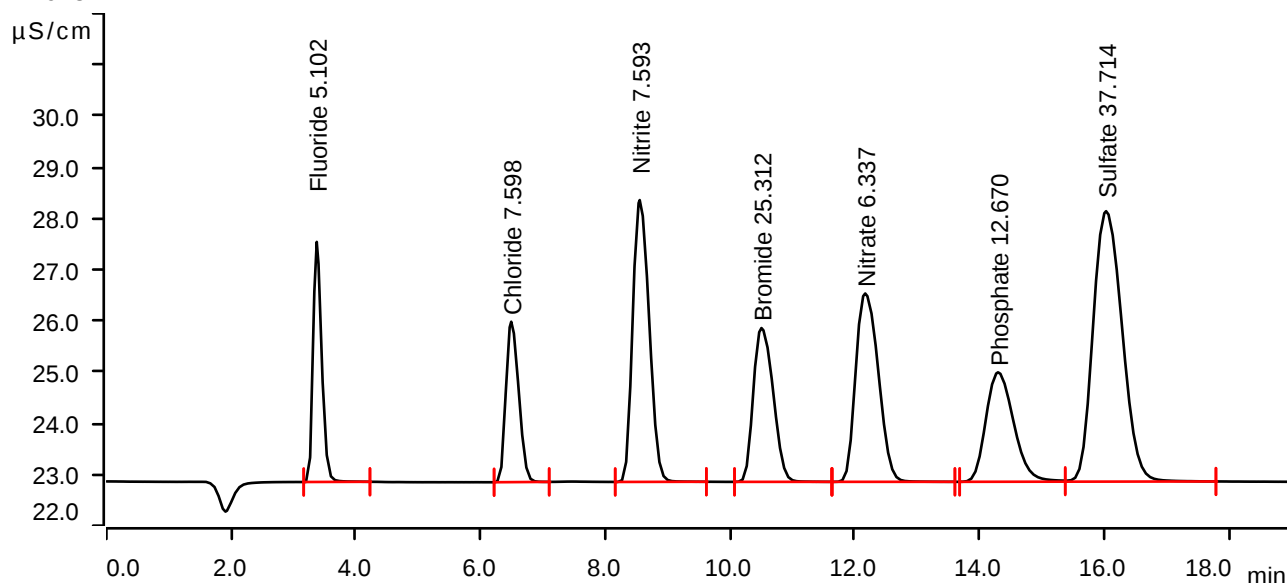

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.7427	4.687	5.102	Fluoride
2	6.492	0.7448	3.132	7.598	Chloride
3	8.552	1.6841	5.502	7.593	Nitrite
4	10.503	1.1070	3.003	25.312	Bromide
5	12.167	1.5512	3.678	6.337	Nitrate
6	14.297	1.1030	2.137	12.670	Phosphate
7	16.028	2.8500	5.280	37.714	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-10-16 13:37:49 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

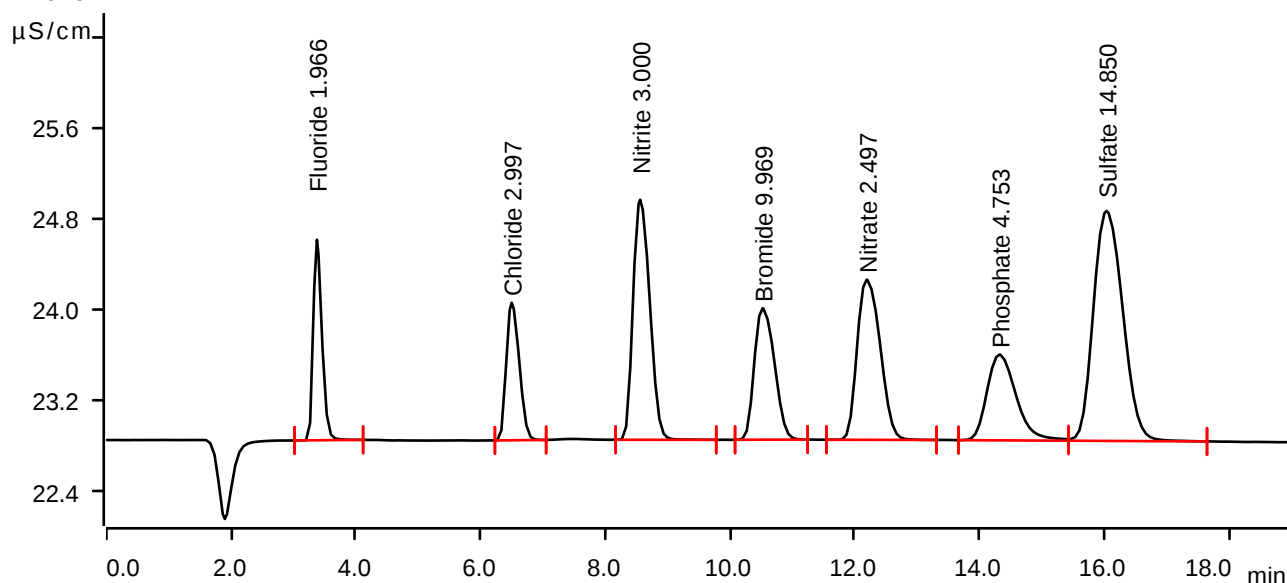


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.377	0.2830	1.762	1.966	Fluoride
2	6.498	0.2910	1.209	2.997	Chloride
3	8.558	0.6557	2.109	3.000	Nitrite
4	10.522	0.4312	1.155	9.969	Bromide
5	12.190	0.6017	1.407	2.497	Nitrate
6	14.320	0.4076	0.753	4.753	Phosphate
7	16.035	1.1027	2.020	14.850	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2024-10-16 13:59:18 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

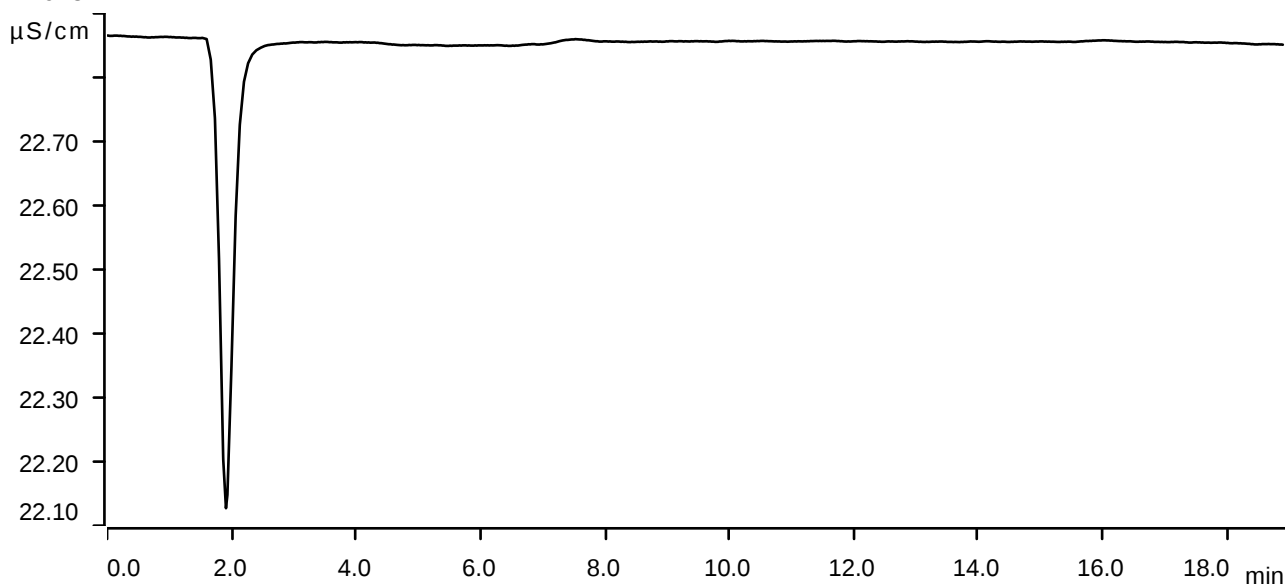Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-11-14 10:35:16 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

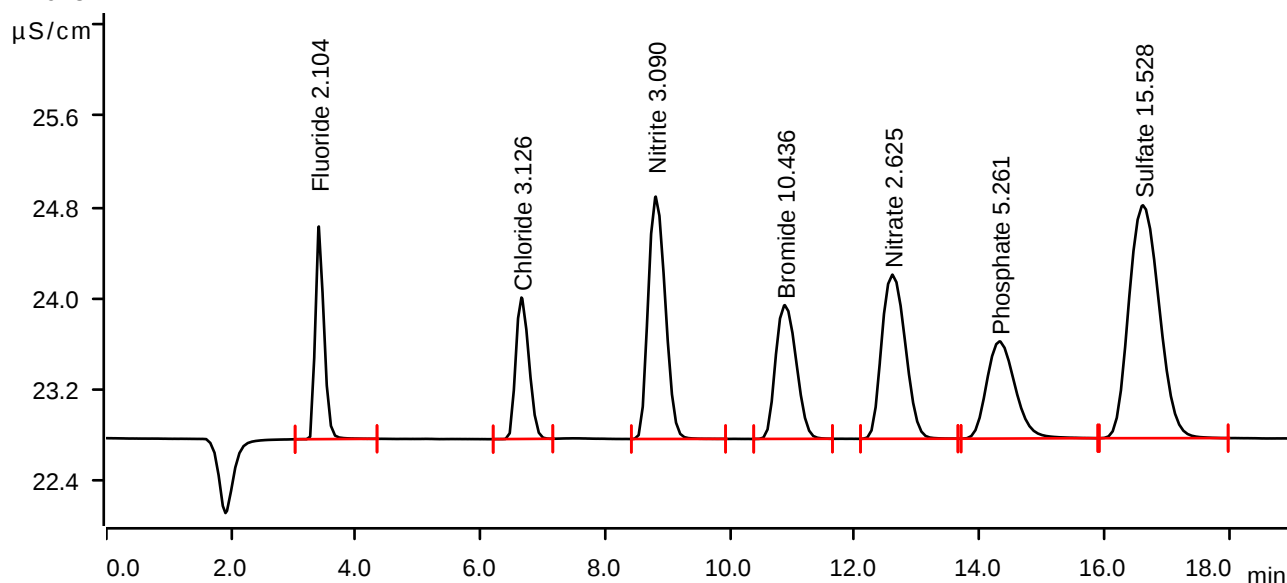


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.407	0.3033	1.868	2.104	Fluoride
2	6.655	0.3037	1.242	3.126	Chloride
3	8.808	0.6760	2.129	3.090	Nitrite
4	10.878	0.4518	1.175	10.436	Bromide
5	12.605	0.6333	1.441	2.625	Nitrate
6	14.320	0.4522	0.854	5.261	Phosphate
7	16.620	1.1544	2.046	15.528	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-11-14 10:56:46 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

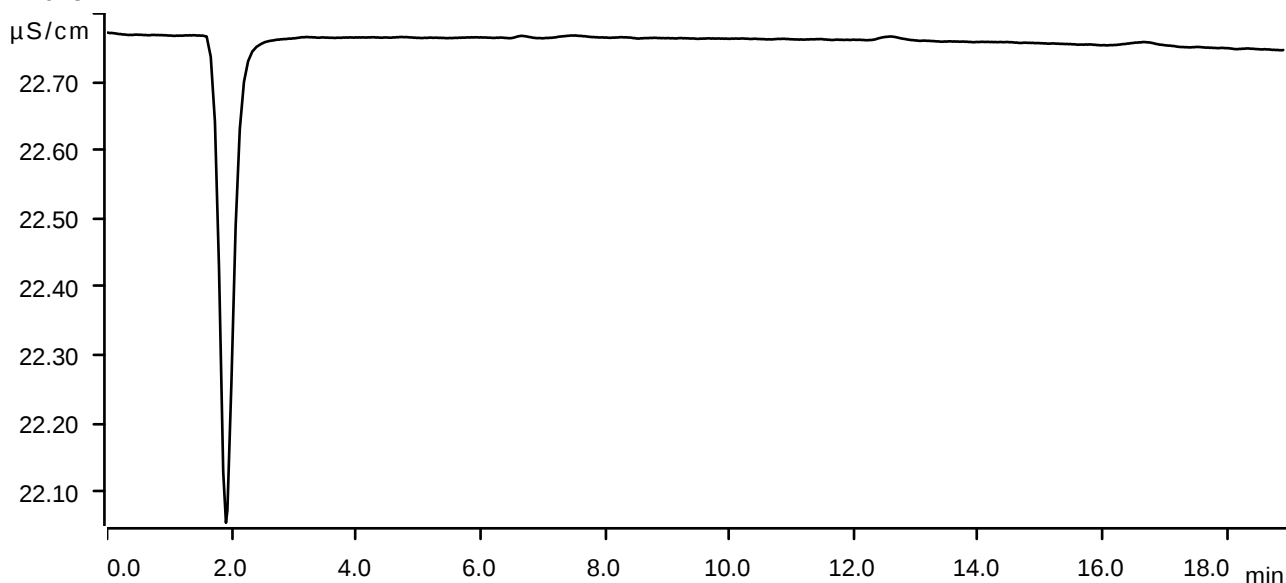Anions


Sample data

Ident LB133442BLW
Sample type Sample
Determination start 2024-11-14 11:18:16 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

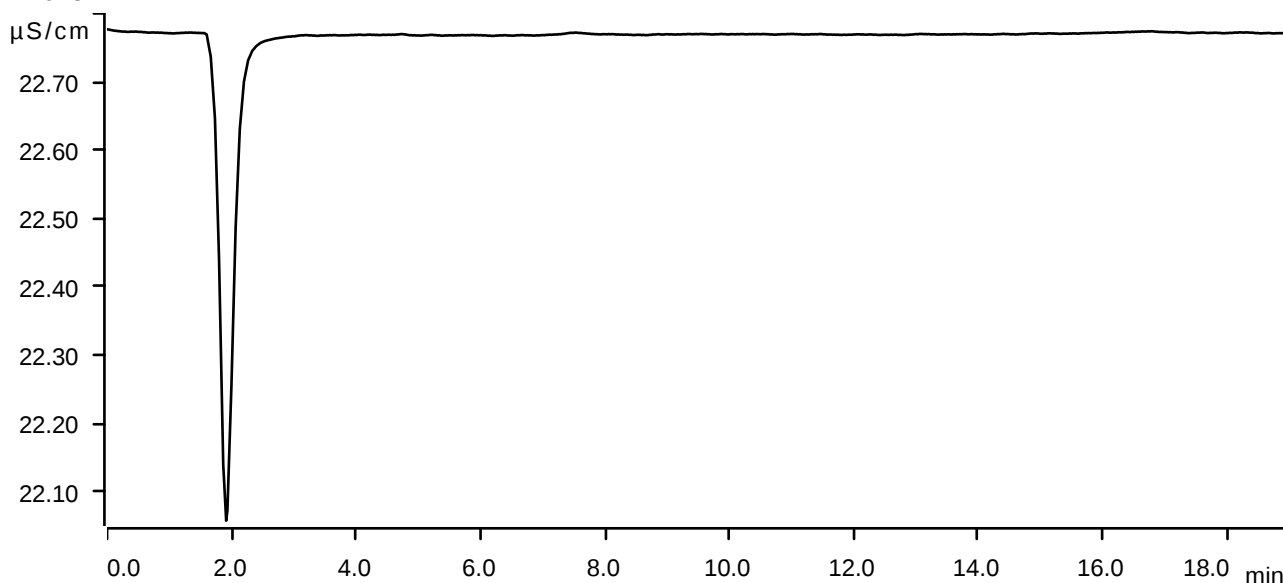


Sample data

Ident LB133442BSW
Sample type Check standard 1
Determination start 2024-11-14 11:39:47 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

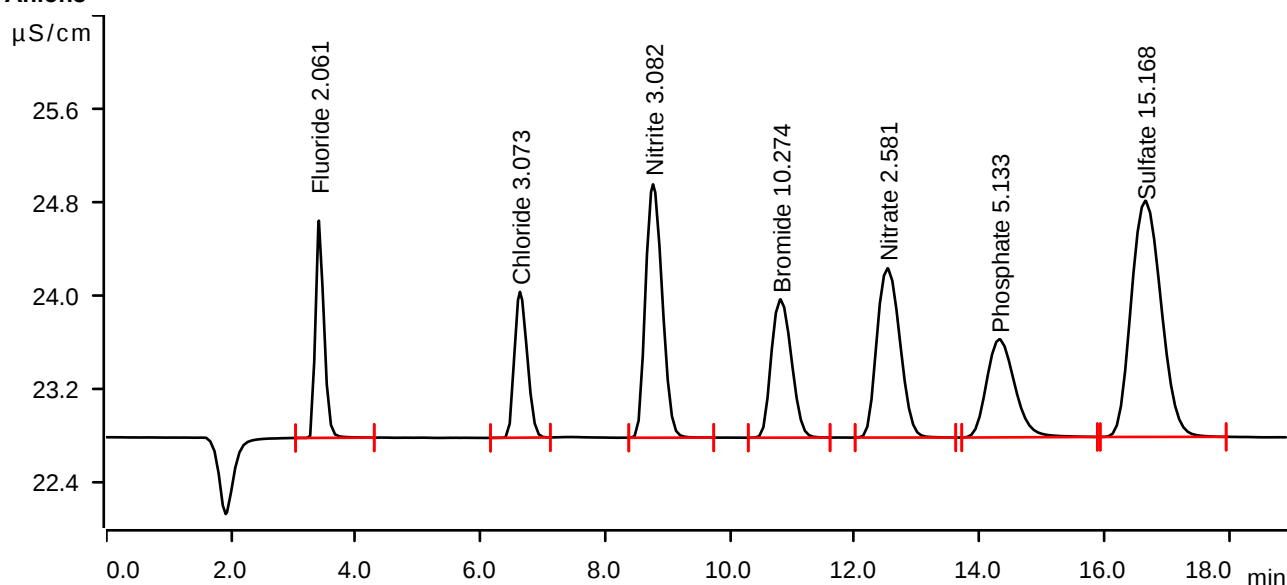

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.408	0.2969	1.866	2.061	Fluoride
2	6.632	0.2985	1.252	3.073	Chloride
3	8.765	0.6740	2.177	3.082	Nitrite
4	10.810	0.4446	1.188	10.274	Bromide
5	12.525	0.6224	1.454	2.581	Nitrate
6	14.317	0.4409	0.843	5.133	Phosphate
7	16.657	1.1270	2.029	15.168	Sulfate


Sample data

Ident P4843-01
Sample type Sample
Determination start 2024-11-14 12:01:19 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

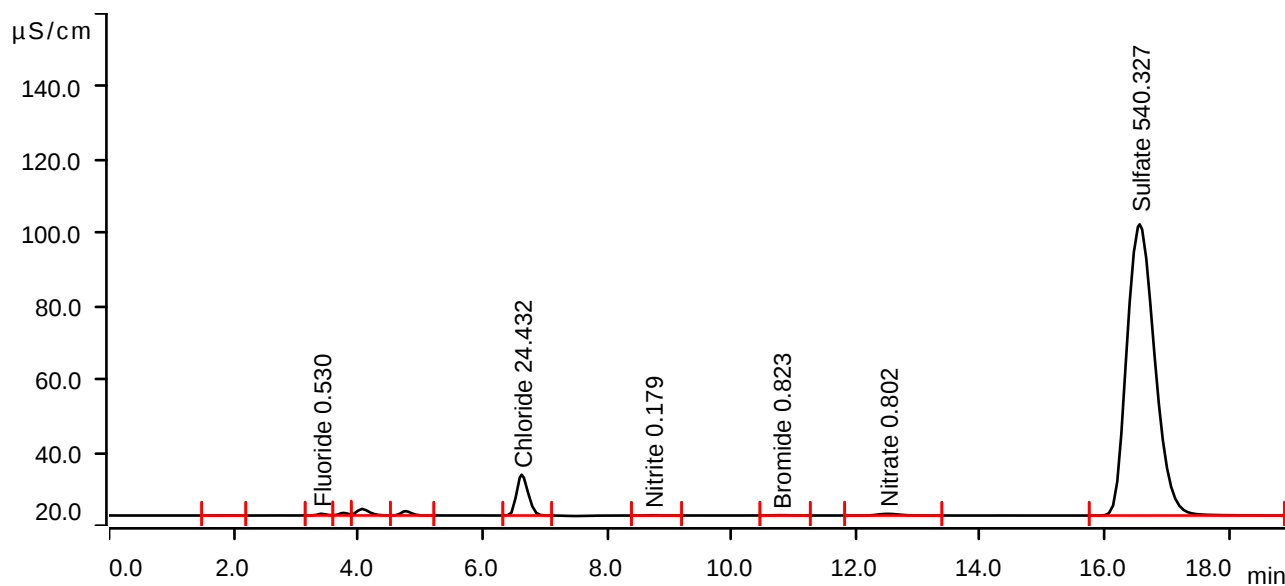

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.933	0.0086	0.037	invalid	
2	3.410	0.0727	0.451	0.530	Fluoride
3	3.768	0.1189	0.678	invalid	
4	4.067	0.4220	1.781	invalid	
5	4.765	0.2284	1.171	invalid	
6	6.632	2.4054	11.151	24.432	Chloride
7	8.740	0.0242	0.082	0.179	Nitrite
8	10.790	0.0284	0.084	0.823	Bromide
9	12.515	0.1823	0.454	0.802	Nitrate
10	16.562	41.2614	79.587	540.327	Sulfate


Sample data

Ident P4843-01MS
Sample type Sample
Determination start 2024-11-14 12:22:52 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

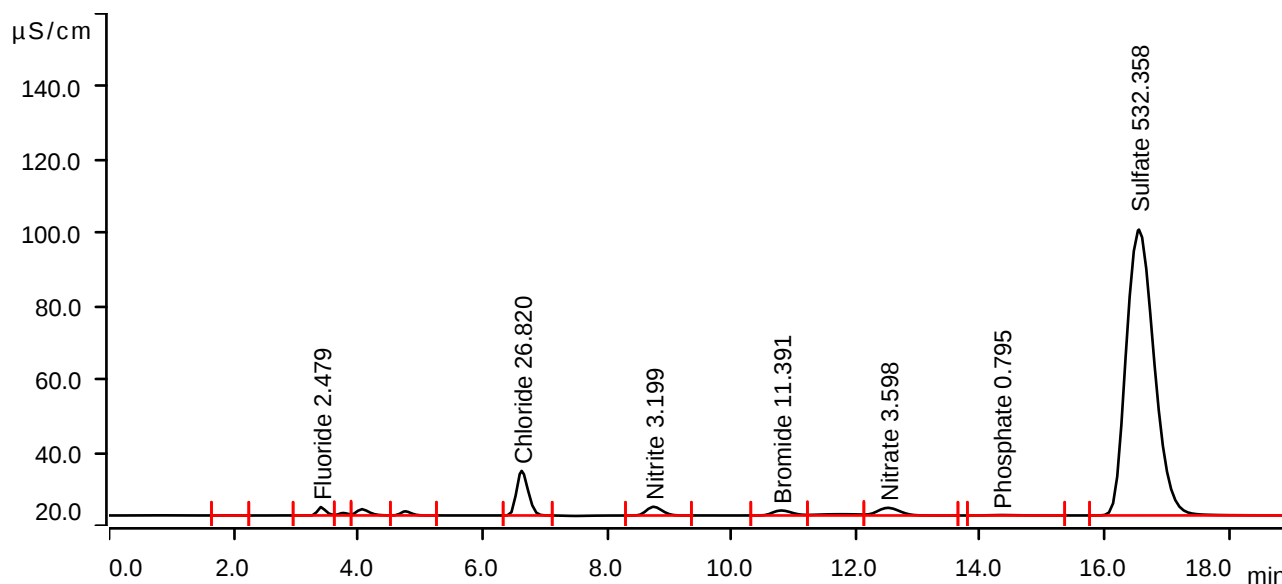

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	1.937	0.0086	0.037	invalid	
2	3.407	0.3582	2.276	2.479	Fluoride
3	3.763	0.1182	0.667	invalid	
4	4.065	0.4082	1.710	invalid	
5	4.762	0.2208	1.122	invalid	
6	6.632	2.6410	12.190	26.820	Chloride
7	8.752	0.7004	2.378	3.199	Nitrite
8	10.803	0.4939	1.362	11.391	Bromide
9	11.765	0.2529	0.341	invalid	
10	12.518	0.8738	2.079	3.598	Nitrate
11	14.358	0.0599	0.117	0.795	Phosphate
12	16.550	40.6524	78.120	532.358	Sulfate


Sample data

Ident P4843-01MSD
Sample type Sample
Determination start 2024-11-14 12:44:27 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

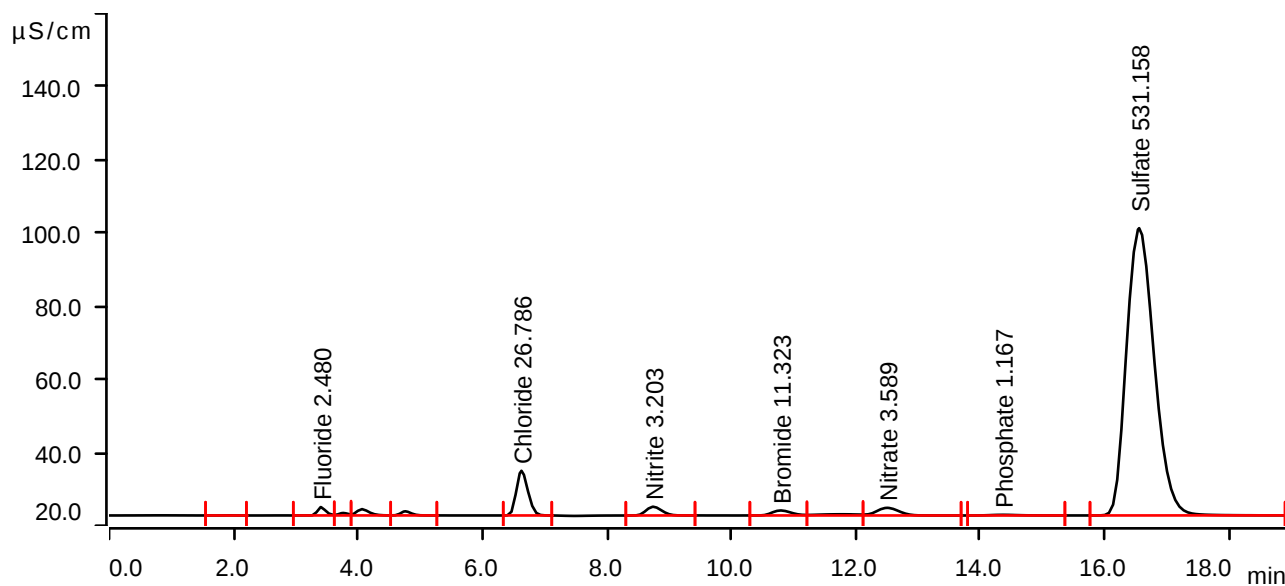

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	1.932	0.0085	0.037	invalid	
2	3.407	0.3585	2.281	2.480	Fluoride
3	3.763	0.1185	0.671	invalid	
4	4.065	0.4074	1.716	invalid	
5	4.762	0.2210	1.128	invalid	
6	6.628	2.6377	12.216	26.786	Chloride
7	8.745	0.7013	2.390	3.203	Nitrite
8	10.793	0.4909	1.365	11.323	Bromide
9	11.755	0.2389	0.325	invalid	
10	12.505	0.8717	2.087	3.589	Nitrate
11	14.367	0.0926	0.183	1.167	Phosphate
12	16.553	40.5606	78.520	531.158	Sulfate


Sample data

Ident P4843-01DLX10
Sample type Sample
Determination start 2024-11-14 13:06:00 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

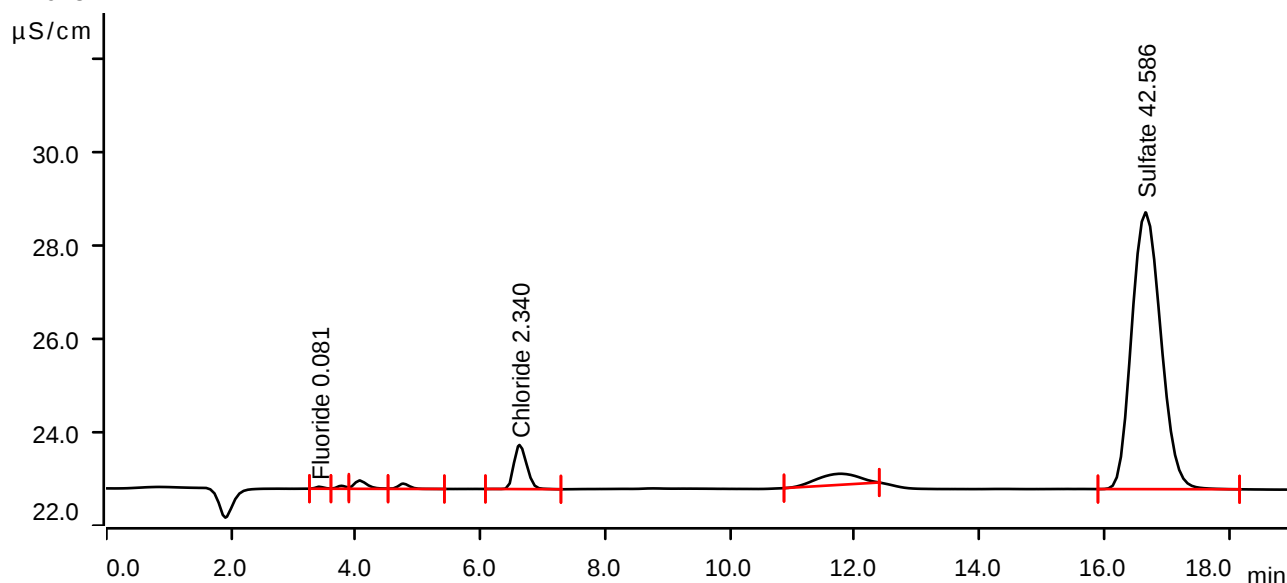

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.412	0.0068	0.043	0.081	Fluoride
2	3.770	0.0108	0.064	invalid	
3	4.058	0.0438	0.179	invalid	
4	4.758	0.0239	0.113	invalid	
5	6.625	0.2261	0.947	2.340	Chloride
6	11.783	0.1858	0.236	invalid	
7	16.660	3.2224	5.943	42.586	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-11-14 13:27:34 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

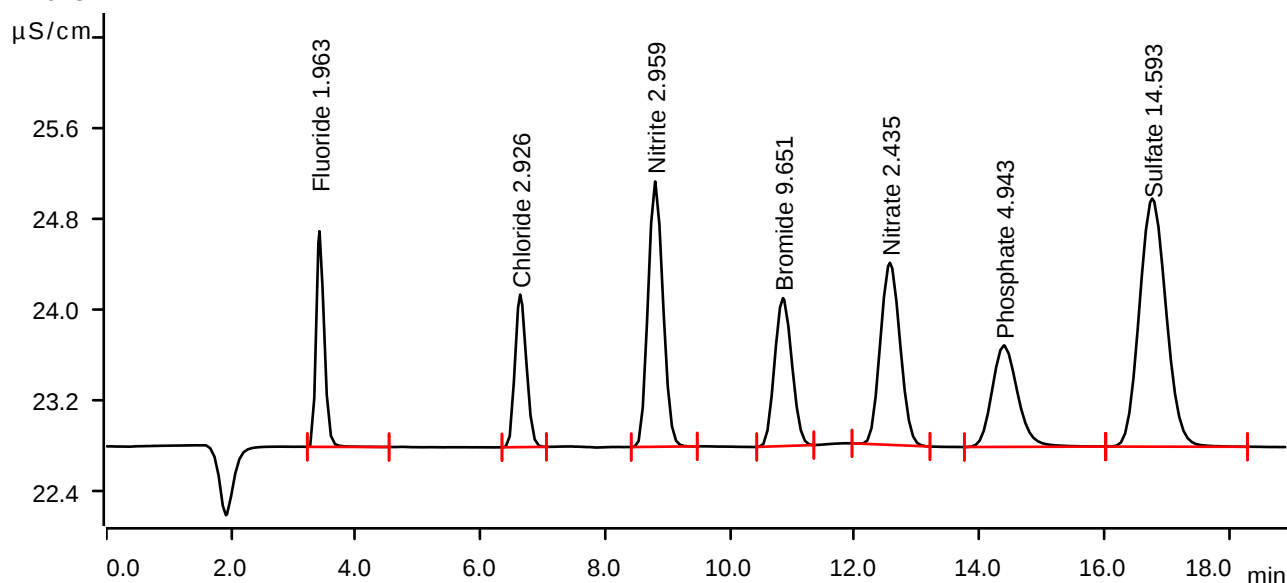

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.418	0.2827	1.894	1.963	Fluoride
2	6.635	0.2840	1.340	2.926	Chloride
3	8.798	0.6465	2.331	2.959	Nitrite
4	10.848	0.4172	1.300	9.651	Bromide
5	12.563	0.5863	1.600	2.435	Nitrate
6	14.390	0.4243	0.892	4.943	Phosphate
7	16.768	1.0830	2.180	14.593	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-11-14 13:49:04 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

