
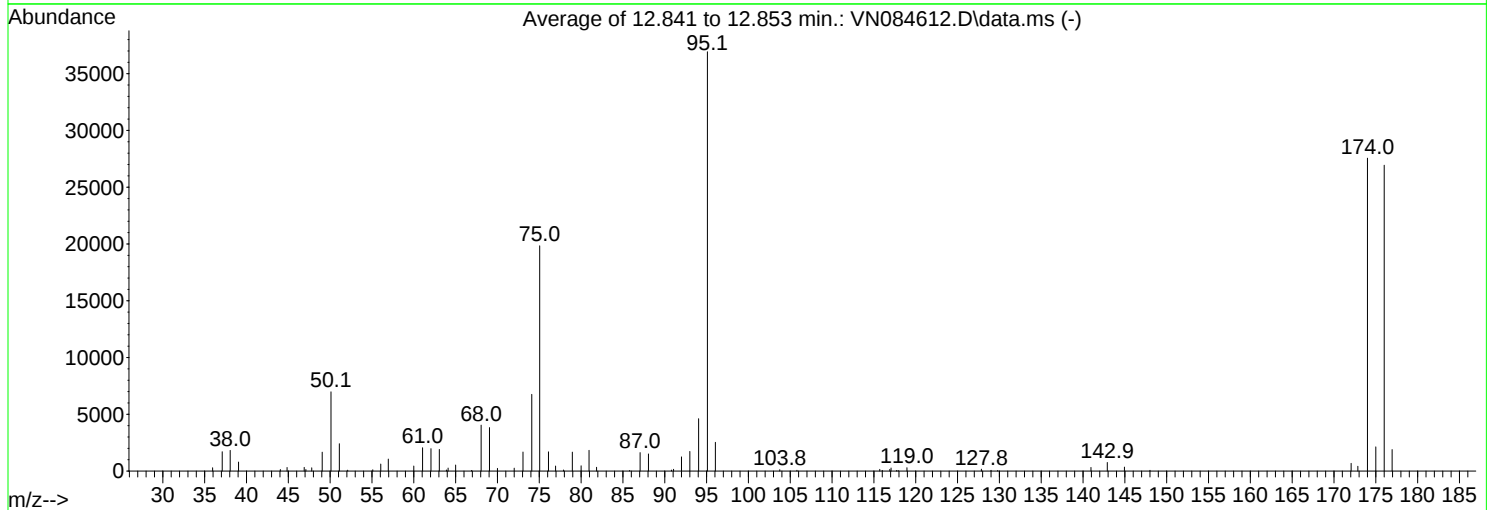


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN103124\
Data File : VN084612.D
Acq On : 31 Oct 2024 10:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N103124W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Nov 01 02:38:04 2024

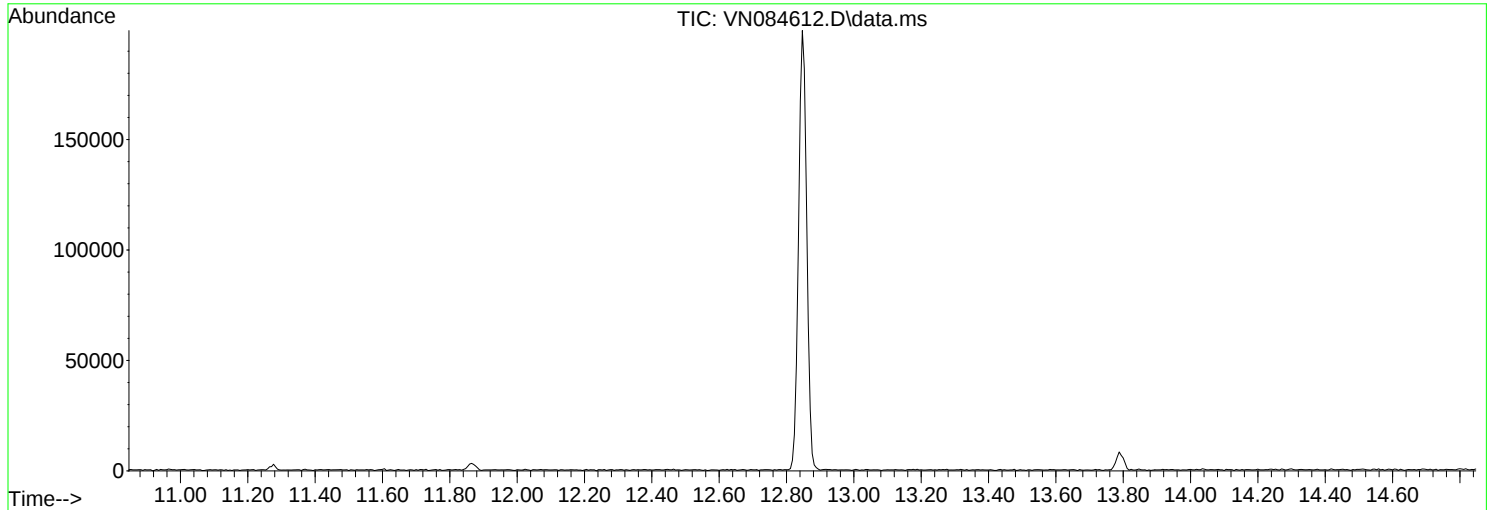

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	6981	PASS
75	95	30	60	53.7	19840	PASS
95	95	100	100	100.0	36931	PASS
96	95	5	9	6.9	2535	PASS
173	174	0.00	2	1.5	422	PASS
174	95	50	100	74.6	27560	PASS
175	174	5	9	7.7	2131	PASS
176	174	95	101	97.7	26936	PASS
177	176	5	9	7.0	1894	PASS