
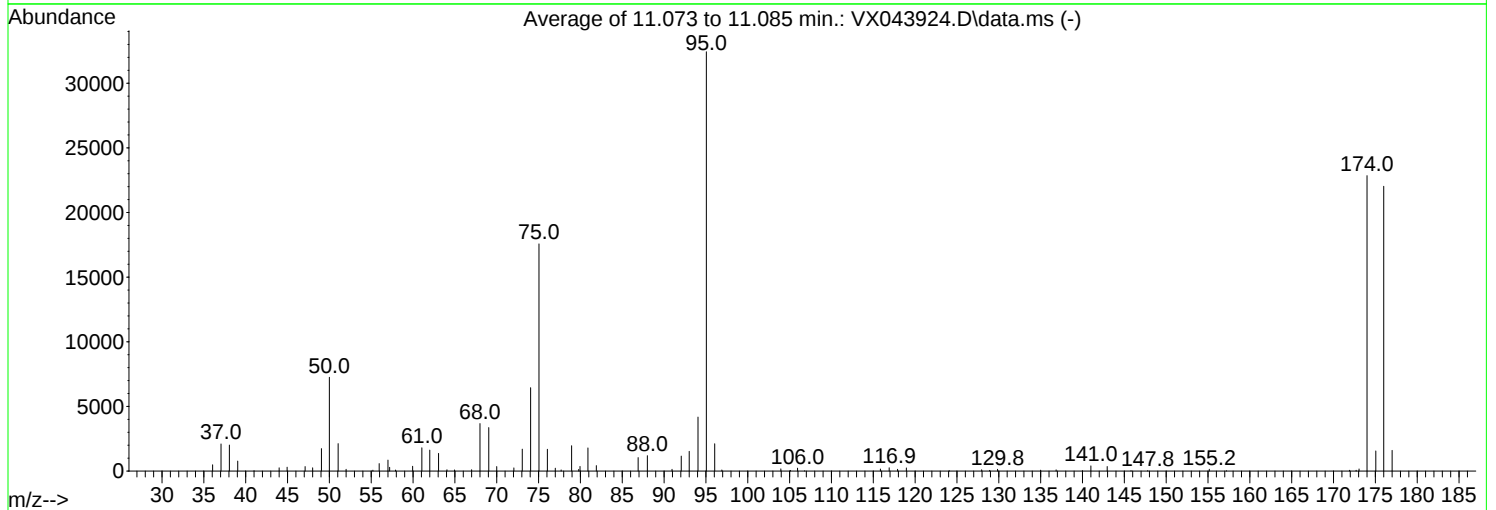


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112124\
Data File : VX043924.D
Acq On : 21 Nov 2024 08:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112024W.M
Title : SW846 8260
Last Update : Fri Nov 22 00:18:05 2024

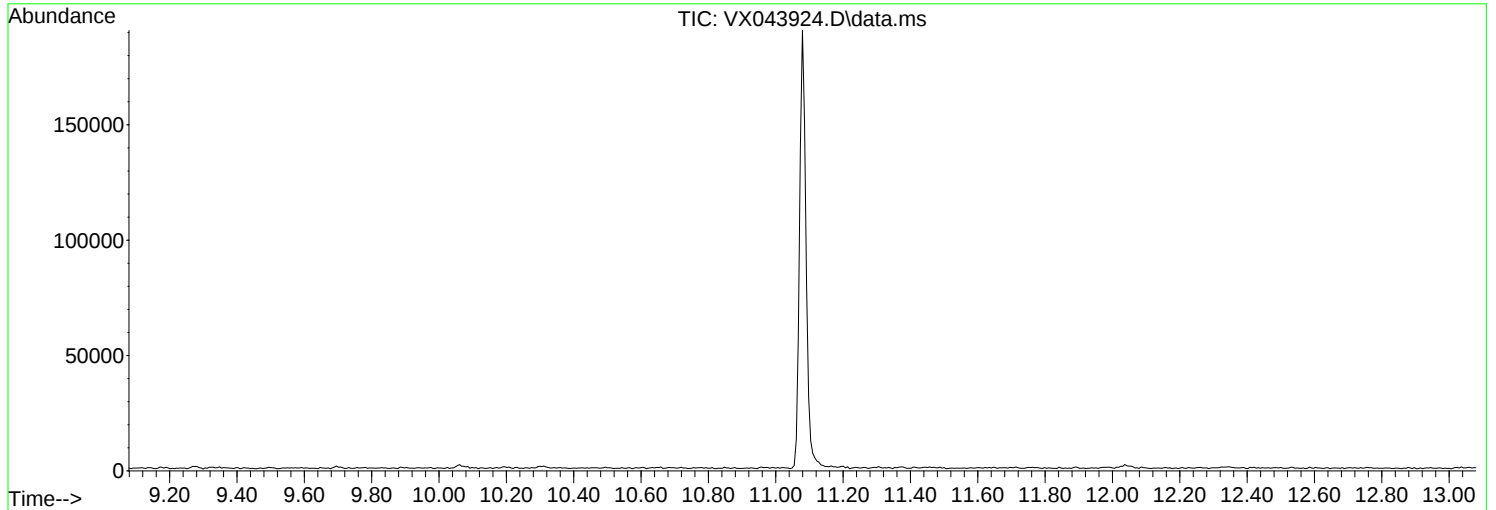

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	7254	PASS
75	95	30	60	54.2	17573	PASS
95	95	100	100	100.0	32437	PASS
96	95	5	9	6.5	2112	PASS
173	174	0.00	2	0.7	162	PASS
174	95	50	100	70.5	22853	PASS
175	174	5	9	6.8	1557	PASS
176	174	95	101	96.4	22030	PASS
177	176	5	9	7.3	1600	PASS