

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111524\
 Data File : PP068519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2024 22:51
 Operator : YP\AJ
 Sample : P4861-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-11-A-202411

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :Ankita Jodhani 11/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 01:44:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.760	4.052	18680623	19346580	19.246m	19.980
2) SA Decachlor...	10.680	9.210	20567309	18317576	16.434	16.193

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111524\
Data File : PP068519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2024 22:51
Operator : YP\AJ
Sample : P4861-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-11-A-202411


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 01:44:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

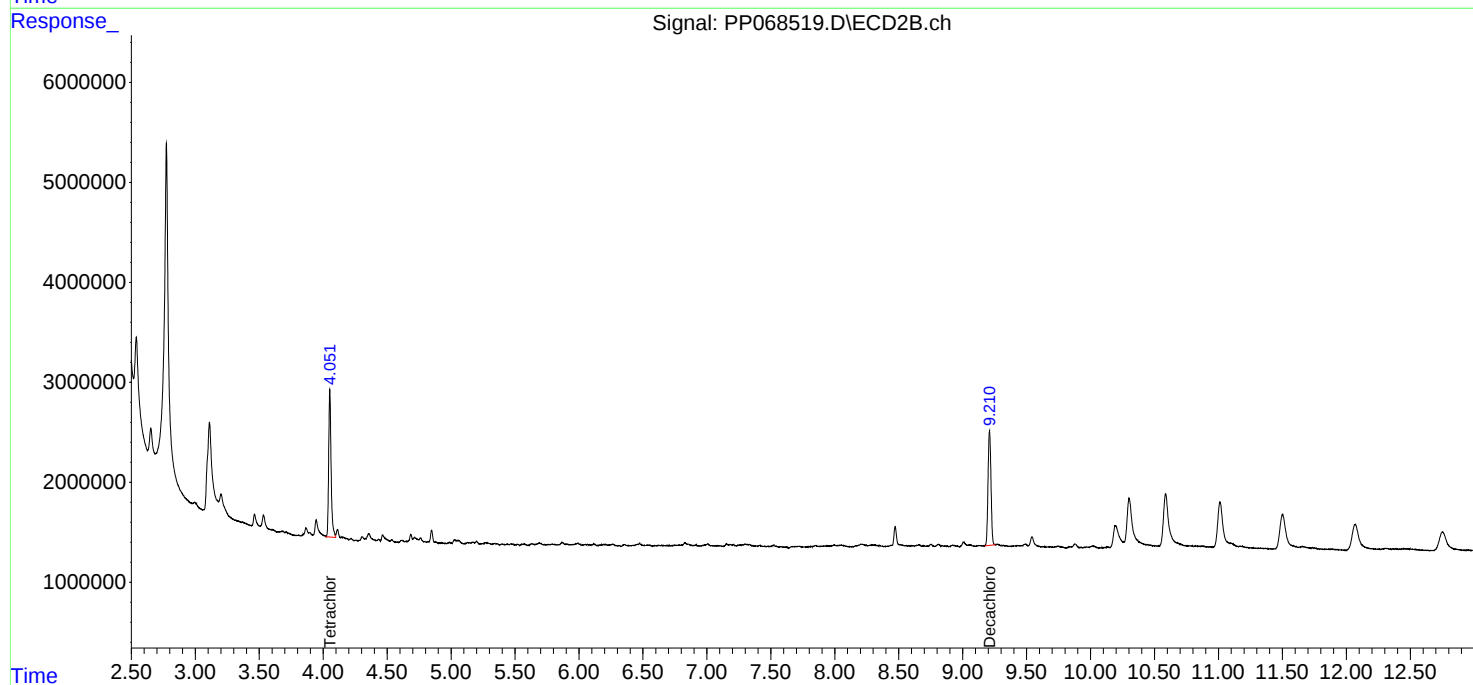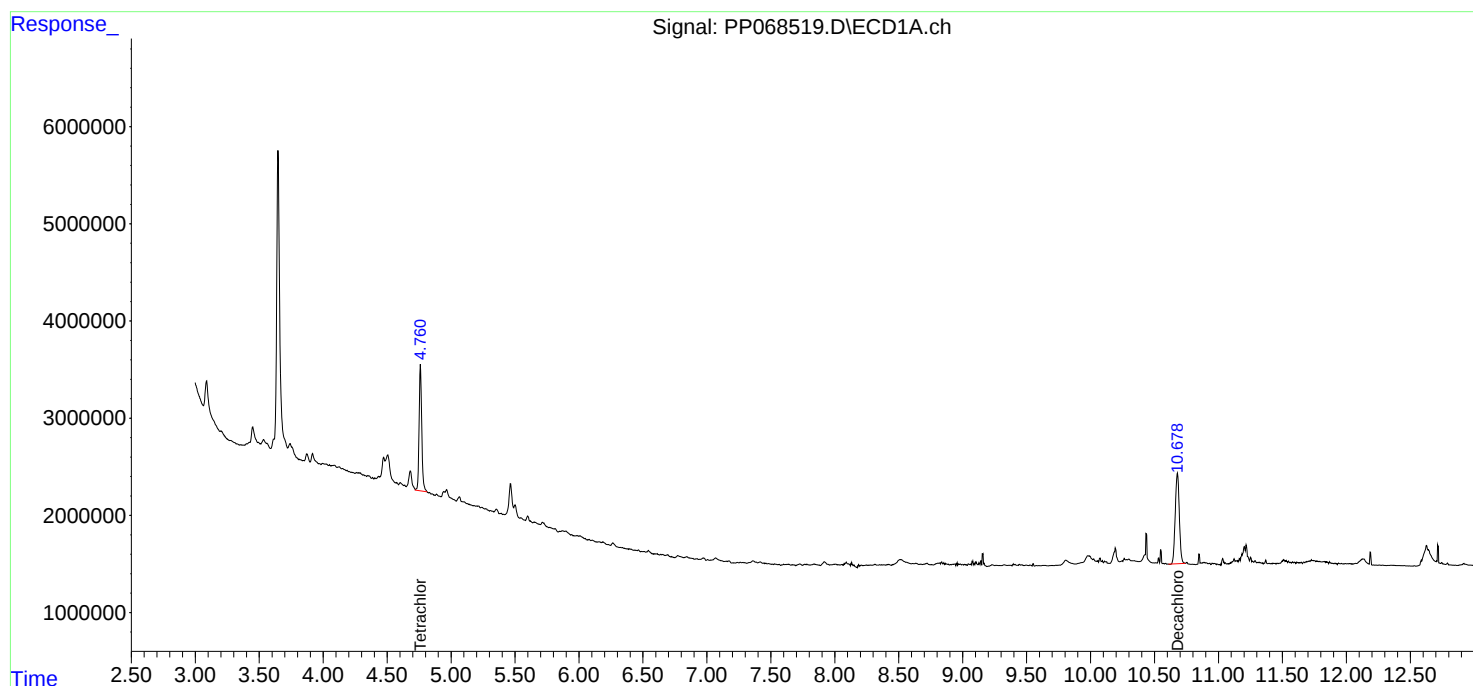

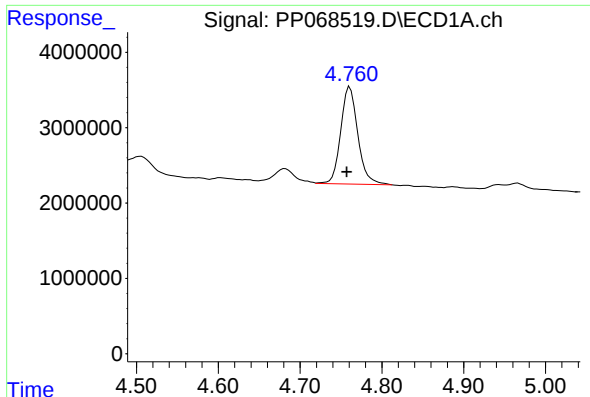


#1 Tetrachloro-m-xylene

R.T.: 4.760 min
Delta R.T.: 0.003 min
Response: 18680623
Conc: 19.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-11-A-202411


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

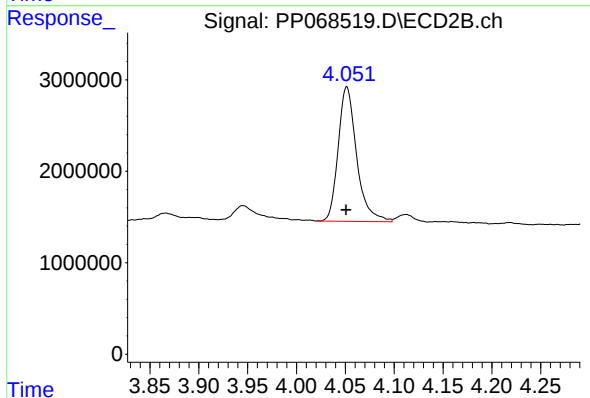


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 19346580
Conc: 19.98 ng/ml

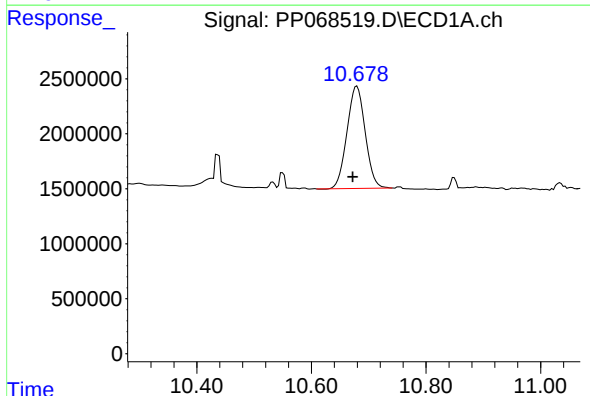

#2 Decachlorobiphenyl

R.T.: 10.680 min
Delta R.T.: 0.007 min
Response: 20567309
Conc: 16.43 ng/ml

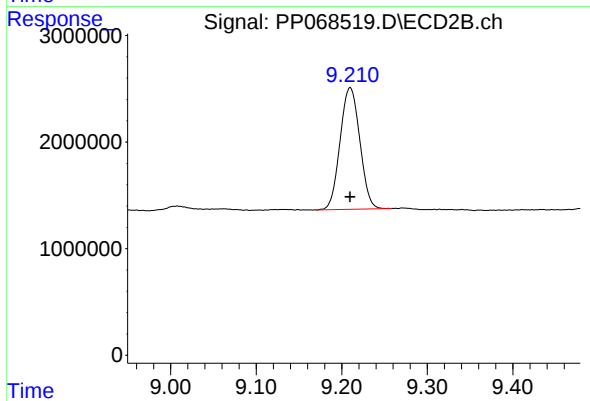

#2 Decachlorobiphenyl

R.T.: 9.210 min
Delta R.T.: 0.000 min
Response: 18317576
Conc: 16.19 ng/ml