
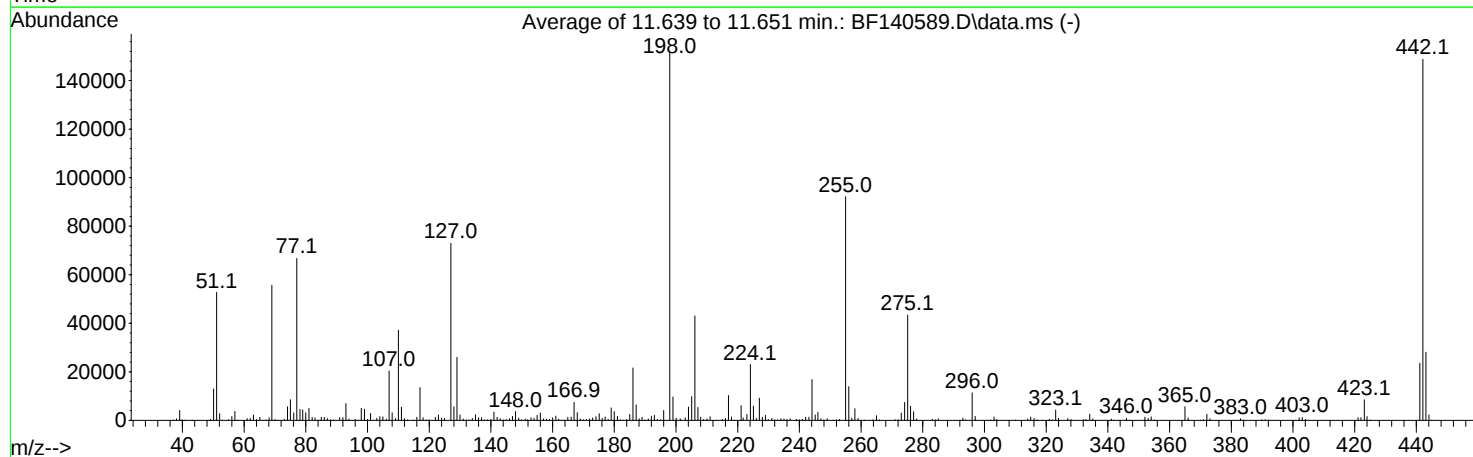


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140589.D
Acq On : 25 Nov 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

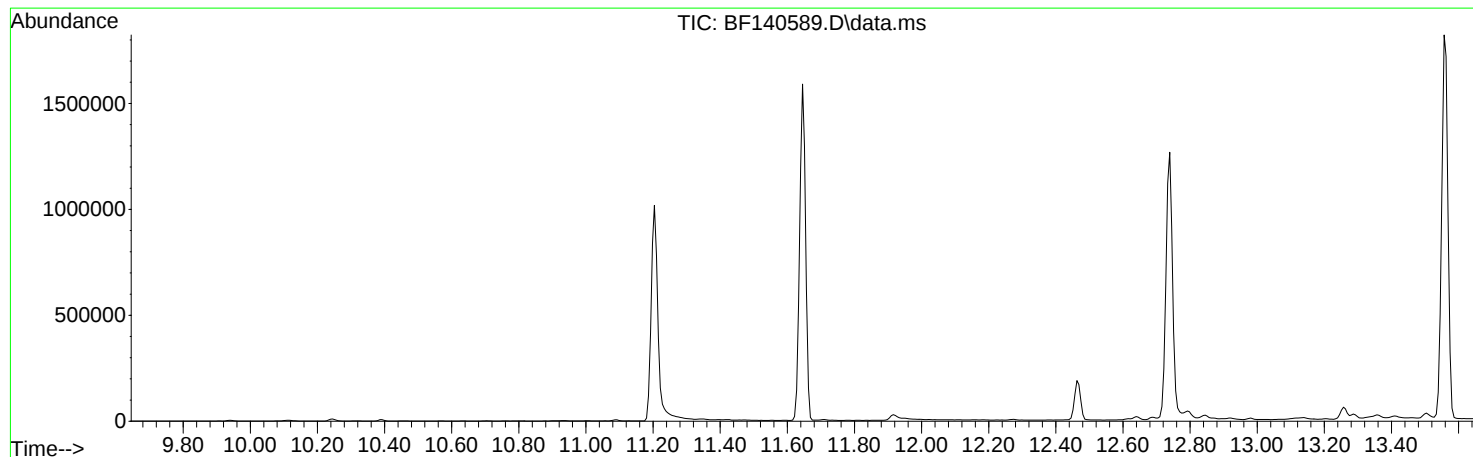

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	52725	PASS
68	69	0.00	2	1.9	1053	PASS
69	198	0.00	100	36.7	55652	PASS
70	69	0.00	2	0.6	343	PASS
127	198	10	80	48.2	73005	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	151552	PASS
199	198	5	9	6.4	9710	PASS
275	198	10	60	28.6	43365	PASS
365	198	1	100	3.7	5678	PASS
441	198	0.01	100	15.5	23530	PASS
442	442	50	100	100.0	148813	PASS
443	442	15	24	18.9	28083	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/25/2024	BNA_F	<u>BF140589.D</u>
Compound Name	Response	Retention Time
DDT	468664	13.557
DDD	19968	13.257
DDE	1731	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21699	490363	4.43

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140589.D
Acq On : 25 Nov 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 10:32:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

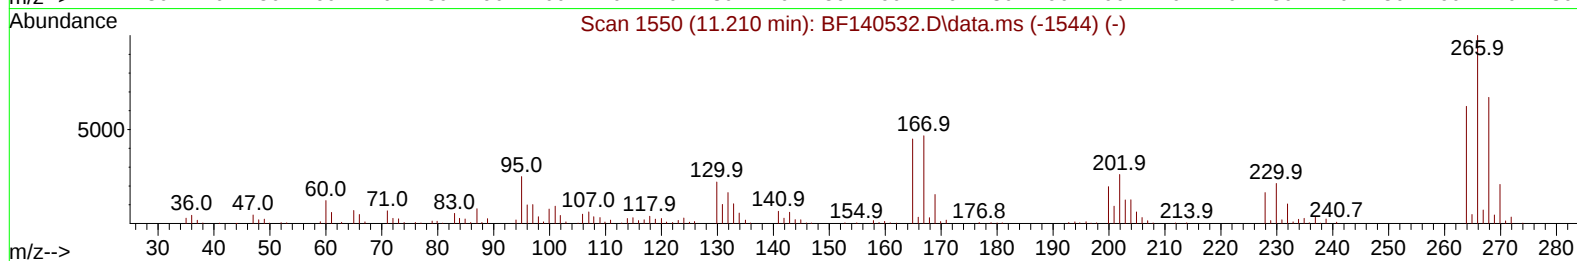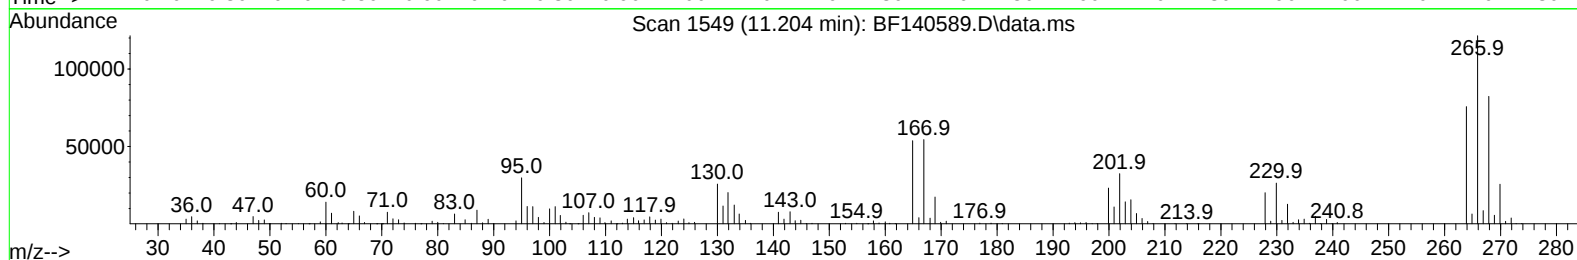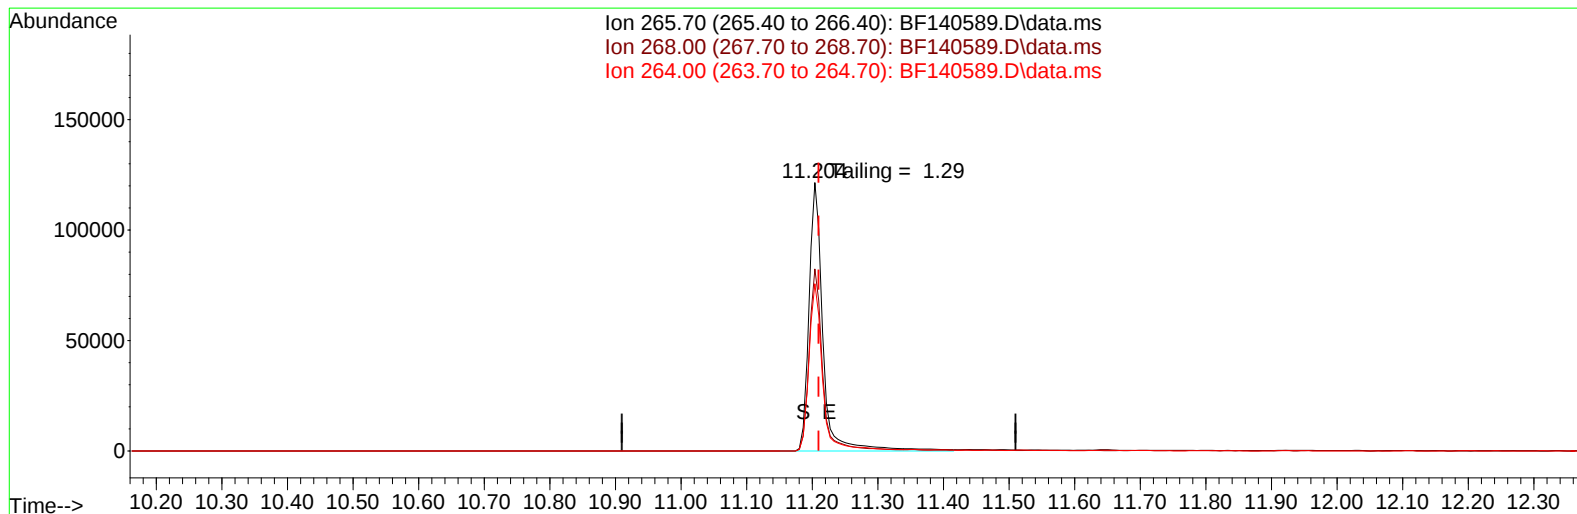

TIC: BF140589.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 31422.92 ng




response 179265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	67.82
264.00	62.30	62.34
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\  
Data File : BF140589.D  
Acq On    : 25 Nov 2024  09:07  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 10:32:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

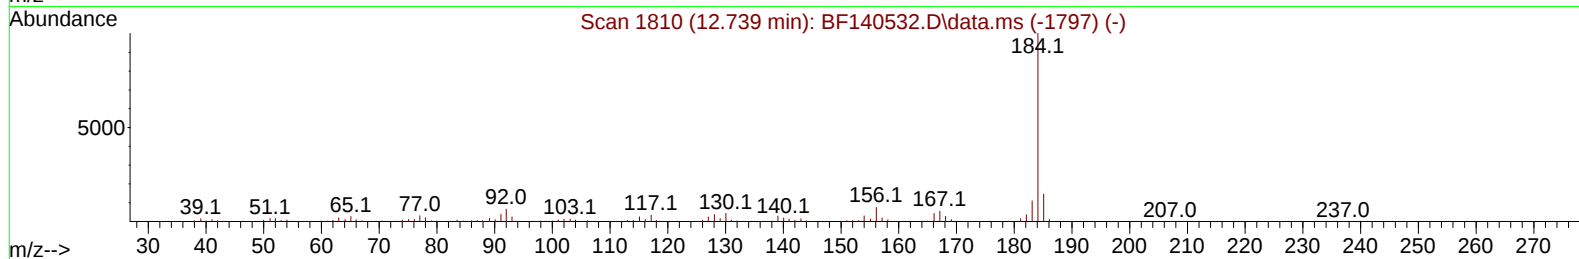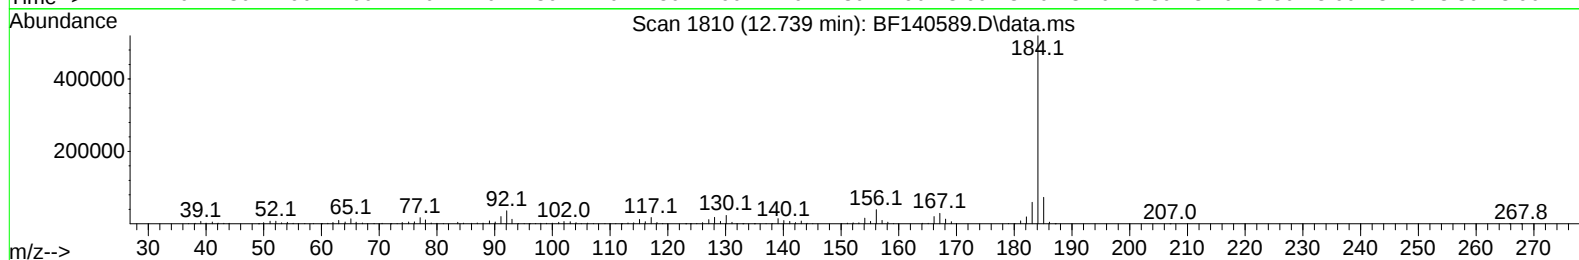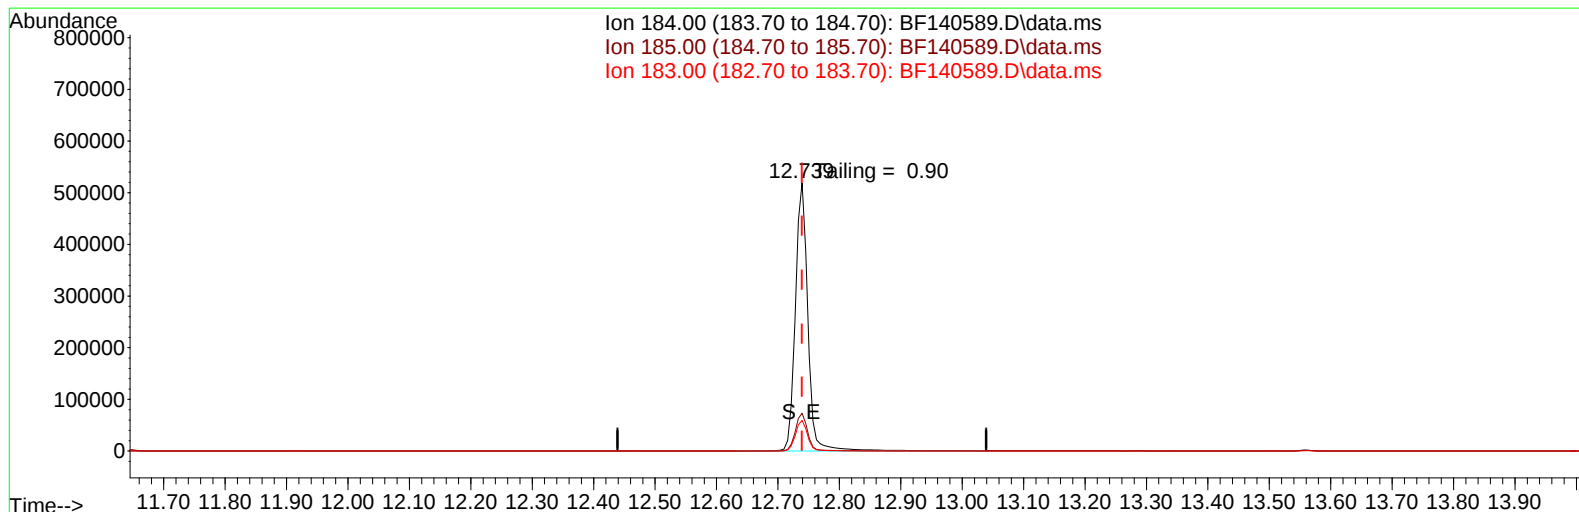

TIC: BF140589.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 27658.53 ng

response 736607

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.07
183.00	11.00	11.40
0.00	0.00	0.00