
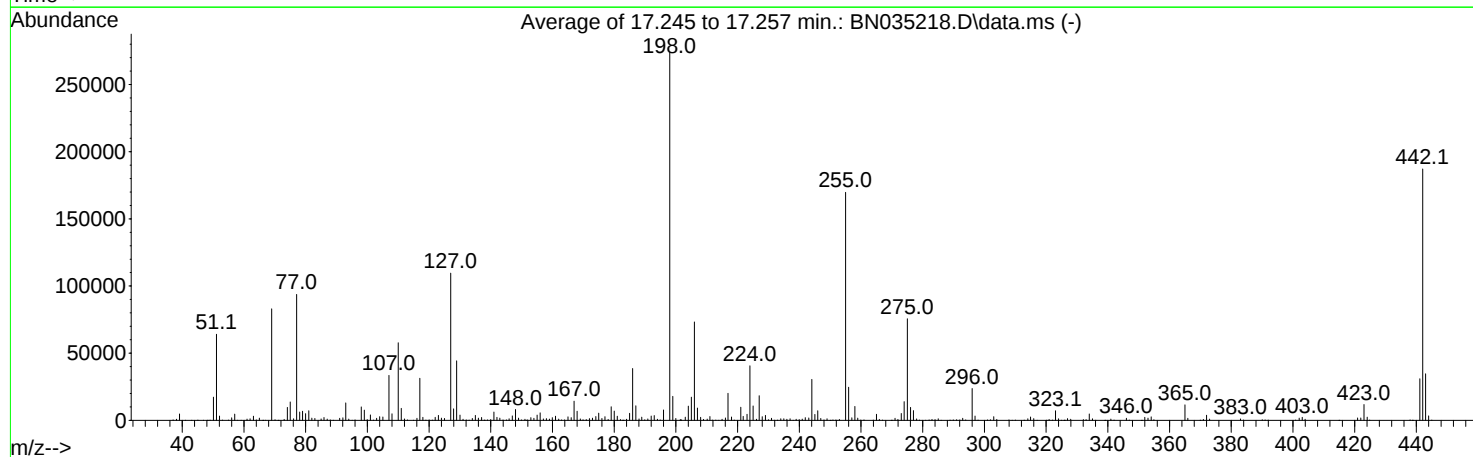


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112124\
Data File : BN035218.D
Acq On : 21 Nov 2024 12:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 14:00:03 2024

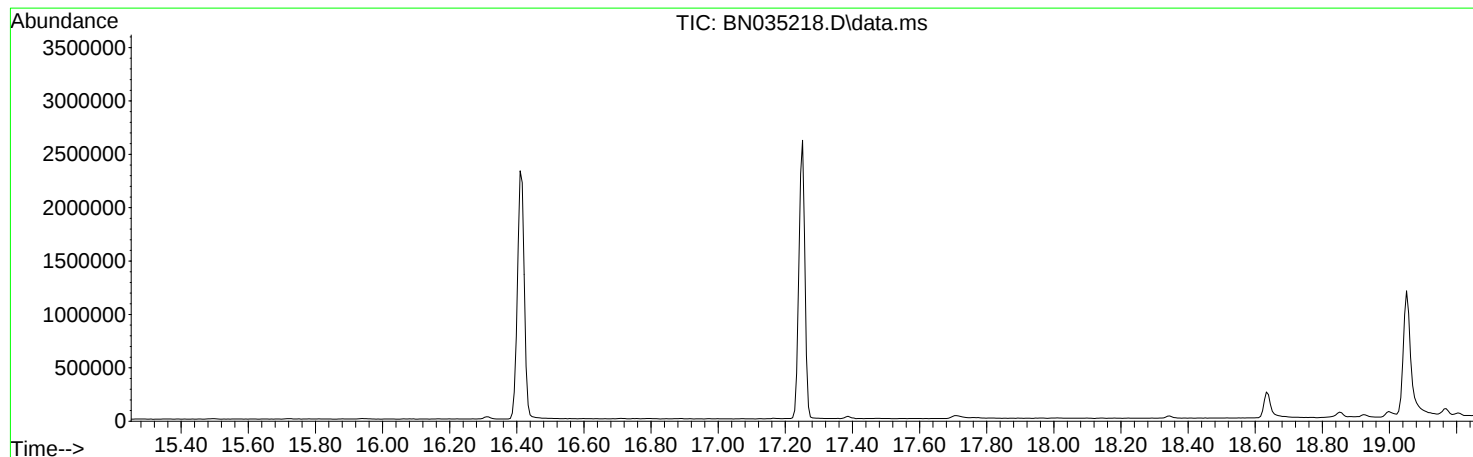

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	64069	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.3	82985	PASS
70	69	0.00	2	0.5	452	PASS
127	198	10	80	40.0	109557	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	273835	PASS
199	198	5	9	6.5	17904	PASS
275	198	10	60	27.6	75661	PASS
365	198	1	100	4.2	11505	PASS
441	198	0.01	100	11.3	30941	PASS
442	442	50	100	100.0	187179	PASS
443	442	15	24	18.5	34664	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/21/2024	BNA_N	<u>BN035218.D</u>
Compound Name	Response	Retention Time
DDT	699093	20.31
DDD	18584	19.863
DDE	951	19.351
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19535	718628	2.72

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112124\
Data File : BN035218.D
Acq On : 21 Nov 2024 12:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 21 15:34:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 03:21:56 2024
Response via : Initial Calibration

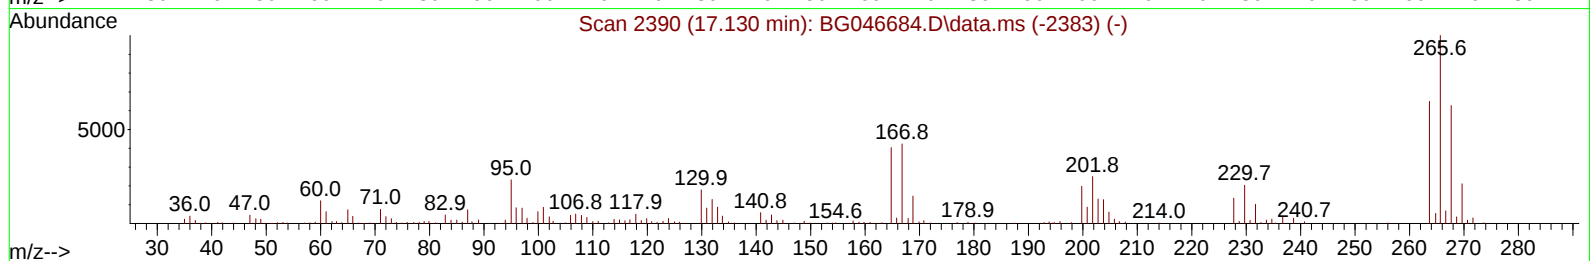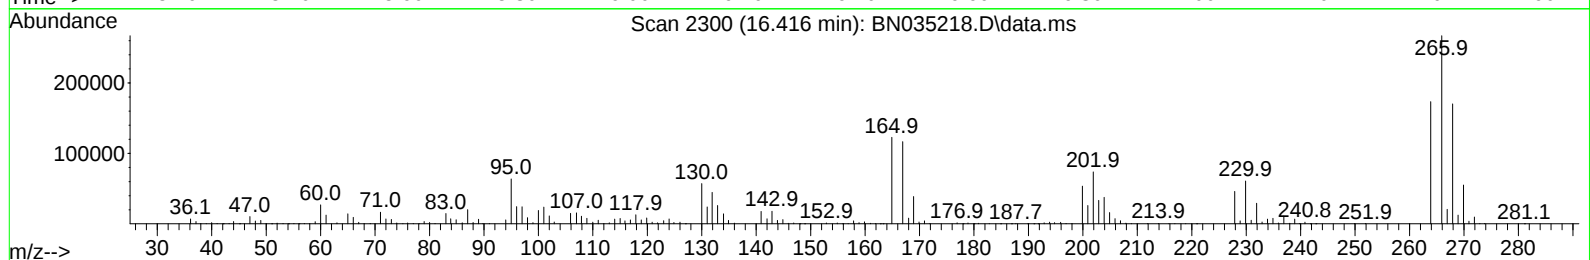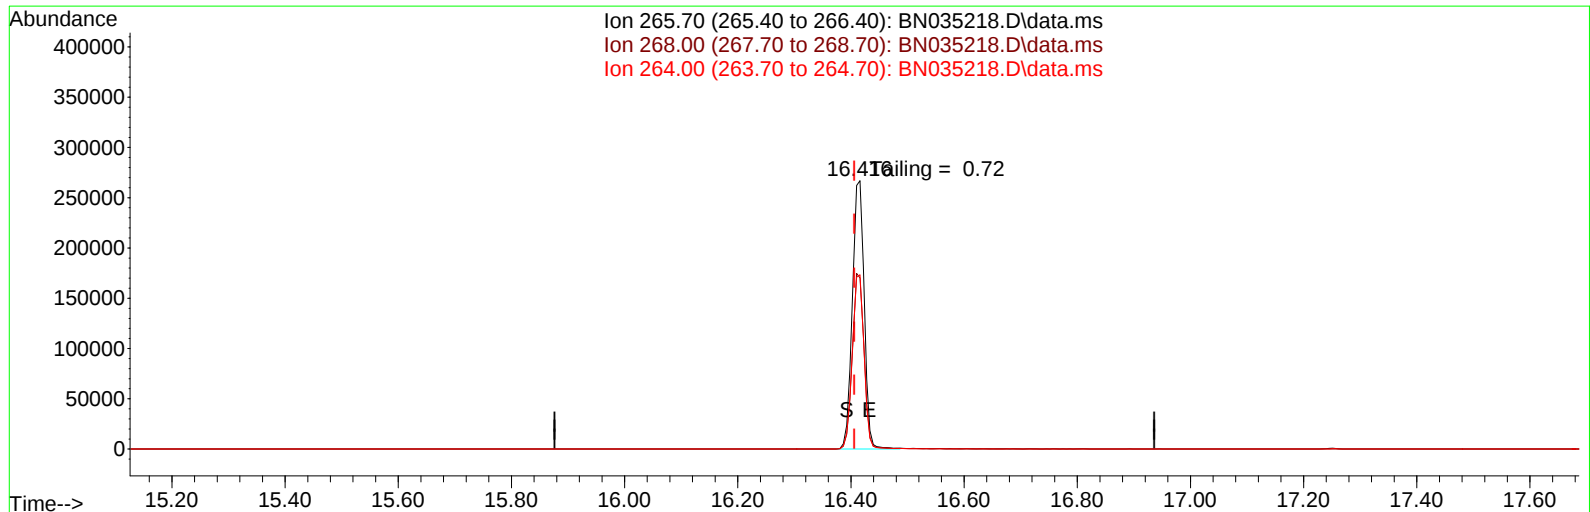

TIC: BN035218.D\data.ms

(70) Pentachlorophenol (C)

16.416min (+ 0.010) 32791.32 ng m




response 386007

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.76
264.00	61.60	64.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112124\
Data File : BN035218.D
Acq On : 21 Nov 2024 12:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 21 15:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 03:21:56 2024
Response via : Initial Calibration

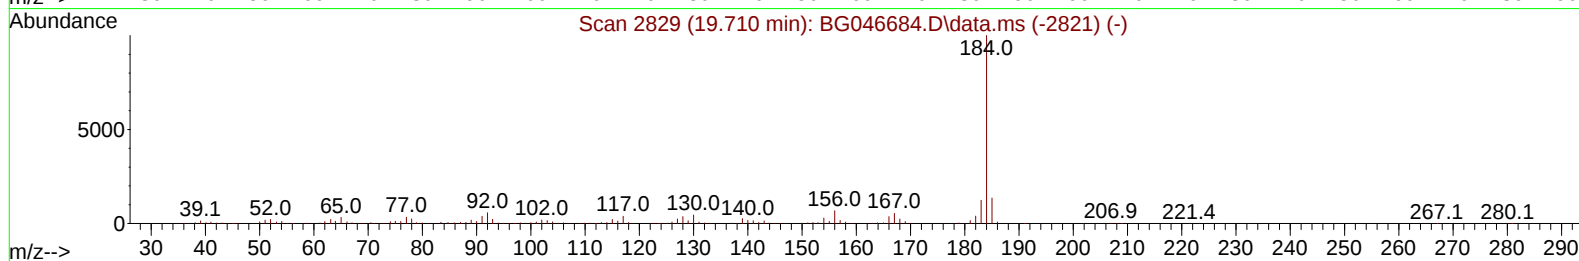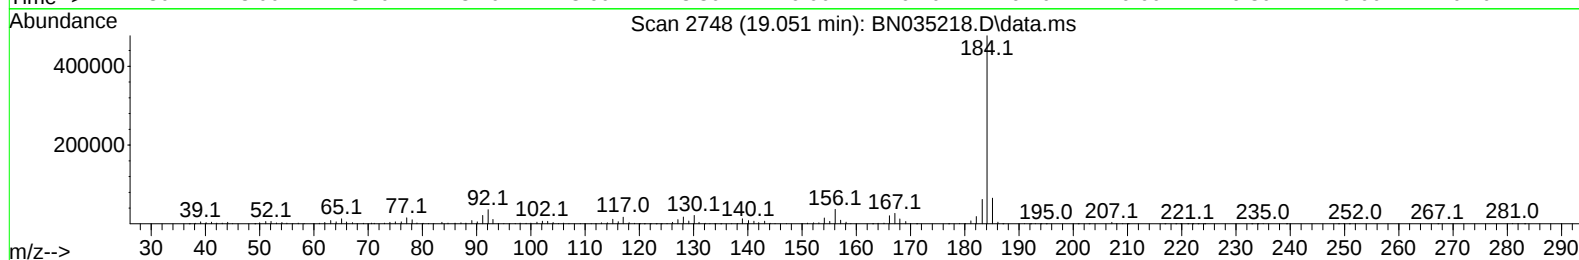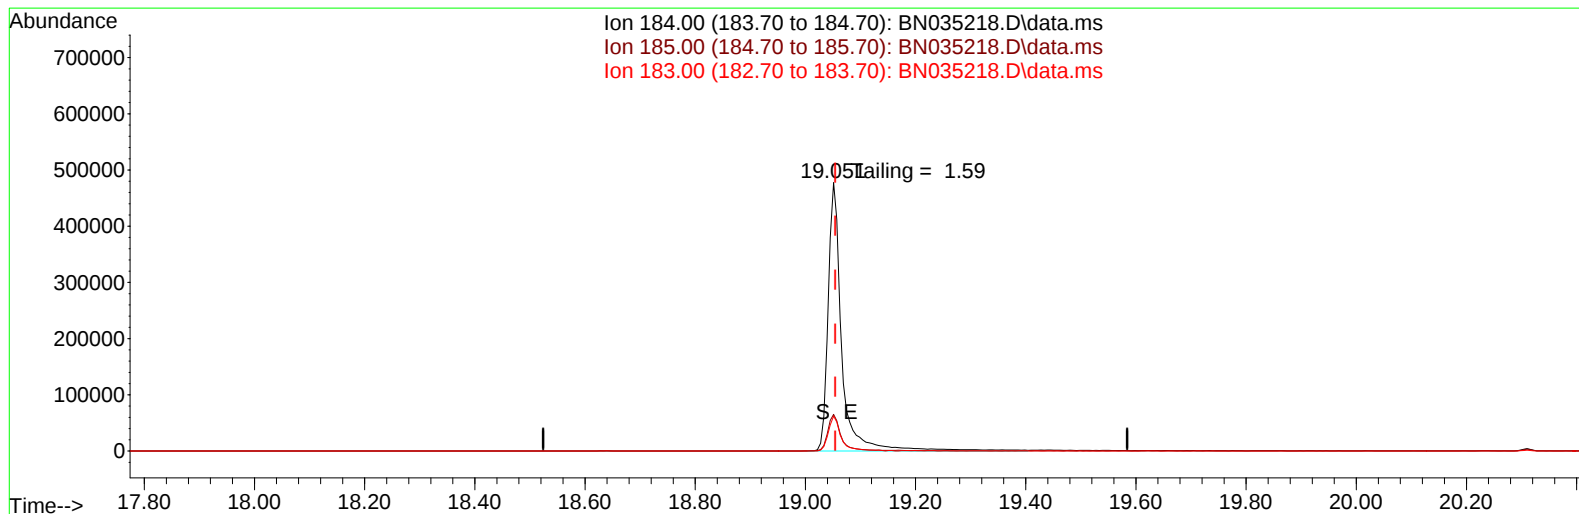

TIC: BN035218.D\data.ms

(77) Benzidine

19.051min (-0.003) 13099.41 ng m

response 829797

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.69
183.00	13.20	13.01
0.00	0.00	0.00