

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112524\
 Data File : VX043985.D
 Acq On : 25 Nov 2024 14:40
 Operator : JC/MD
 Sample : P4886-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Storage-Blank-WATER-REF-5

Quant Time: Nov 26 00:48:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	119026	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	226356	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	196892	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	84391	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	100685	49.319	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.640%
35) Dibromofluoromethane	5.379	113	75345	46.583	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.160%
50) Toluene-d8	8.647	98	277795	49.825	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.640%
62) 4-Bromofluorobenzene	11.079	95	90384	47.634	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	95.260%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112524\
Data File : VX043985.D
Acq On : 25 Nov 2024 14:40
Operator : JC/MD
Sample : P4886-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Quant Time: Nov 26 00:48:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration

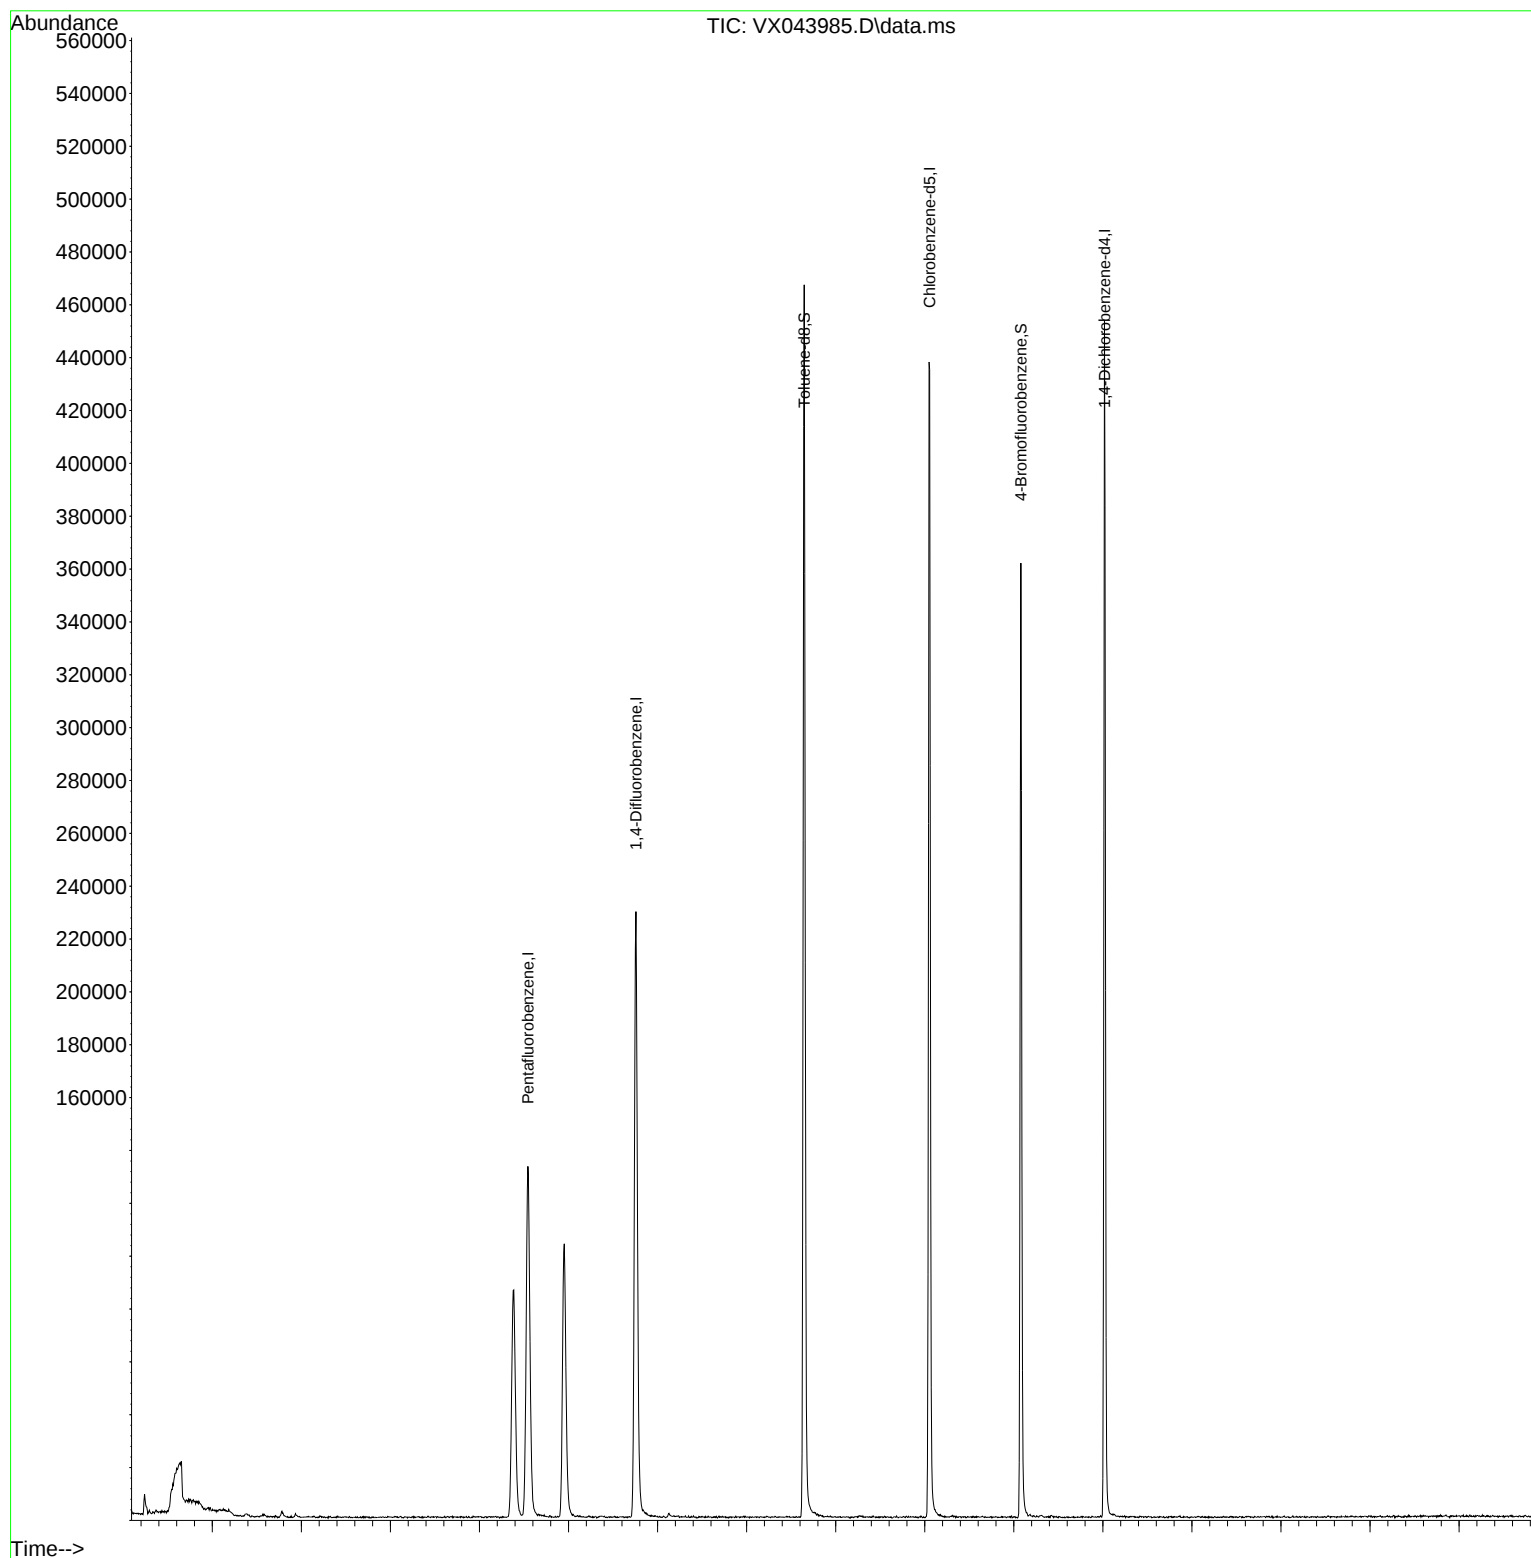






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. 0.006 min
Lab File: VX043985.D
Acq: 25 Nov 2024 14:40

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5



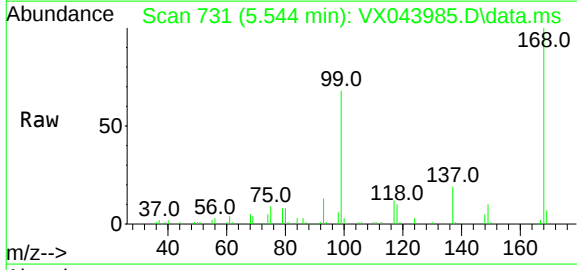



Tgt Ion:168 Resp: 119026
Ion Ratio Lower Upper
168 100
99 67.6 51.8 77.8

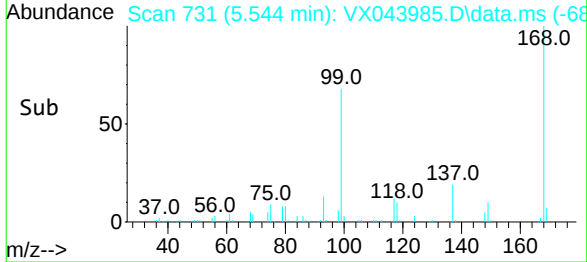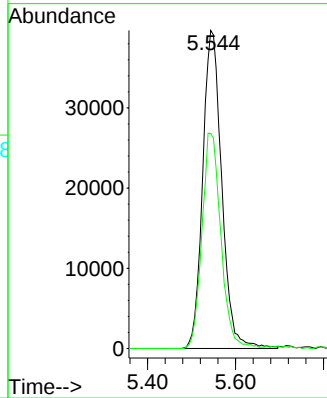

#33
1,2-Dichloroethane-d4
Concen: 49.319 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX043985.D
Acq: 25 Nov 2024 14:40

Tgt Ion: 65 Resp: 100685
Ion Ratio Lower Upper
65 100
67 51.2 0.0 100.8


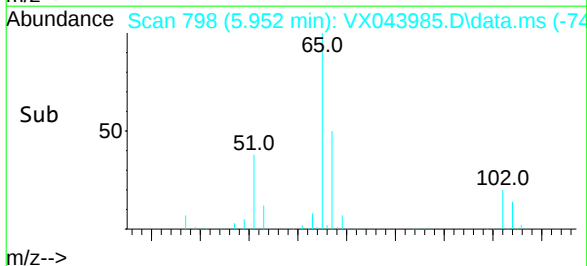
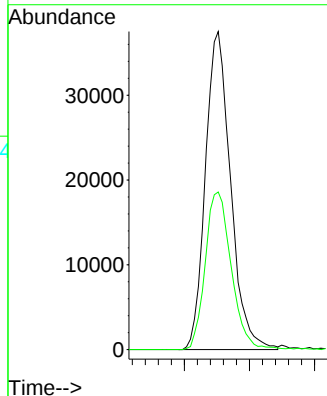
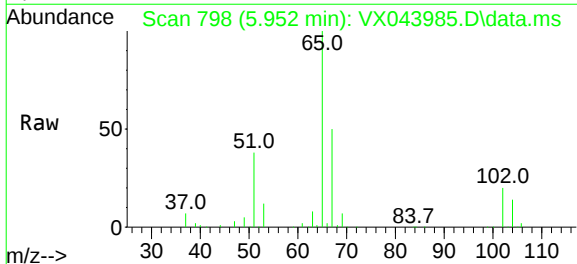




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.000 min
Lab File: VX043985.D
Acq: 25 Nov 2024 14:40




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion:	114	Resp:	226356
Ion	Ratio	Lower	Upper
114	100		
63	20.4	0.0	44.0
88	14.6	0.0	32.4

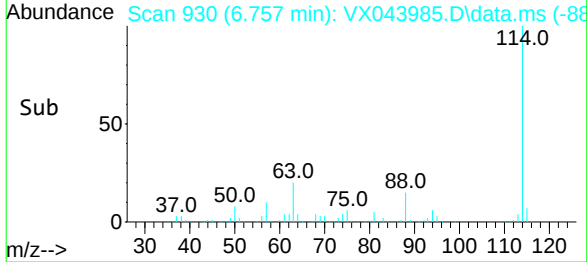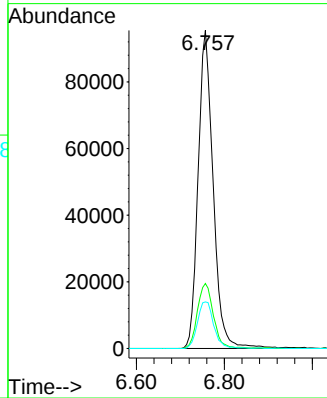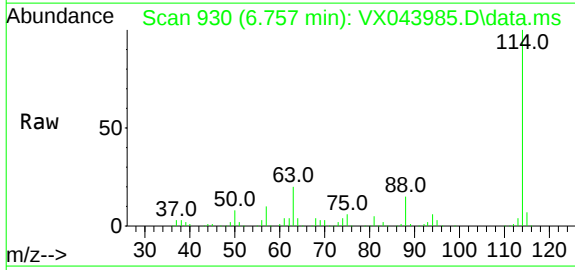

#35
Dibromofluoromethane
Concen: 46.583 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX043985.D
Acq: 25 Nov 2024 14:40

Tgt Ion:	113	Resp:	75345
Ion	Ratio	Lower	Upper
113	100		
111	102.6	81.0	121.4
192	17.7	13.0	19.6


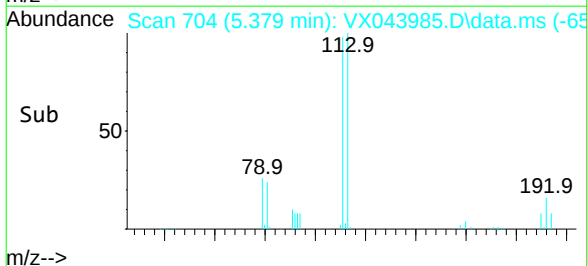
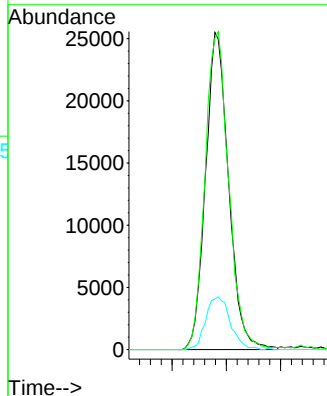
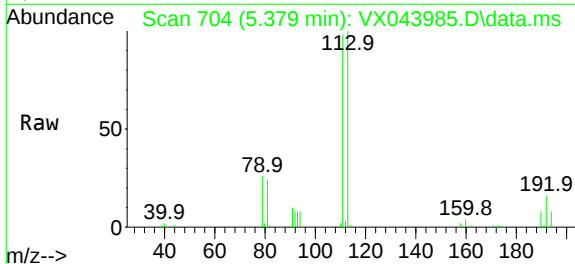




#50
Toluene-d8
Concen: 49.825 ug/l
RT: 8.647 min Scan# 1239
Delta R.T. 0.006 min
Lab File: VX043985.D
Acq: 25 Nov 2024 14:40




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion: 98 Resp: 277795
Ion Ratio Lower Upper
98 100
100 63.9 52.6 79.0

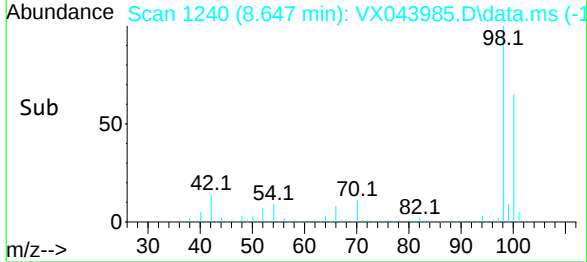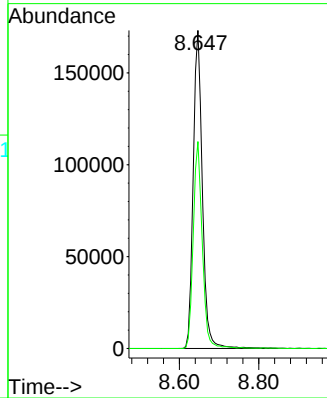

#62
4-Bromofluorobenzene
Concen: 47.634 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX043985.D
Acq: 25 Nov 2024 14:40

Tgt Ion: 95 Resp: 90384
Ion Ratio Lower Upper
95 100
174 74.6 0.0 150.4
176 73.3 0.0 146.0

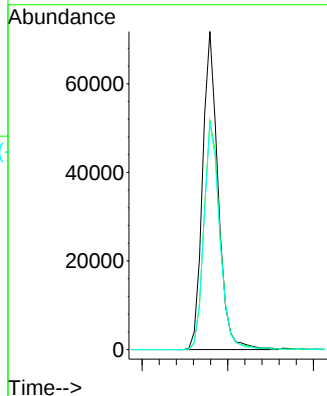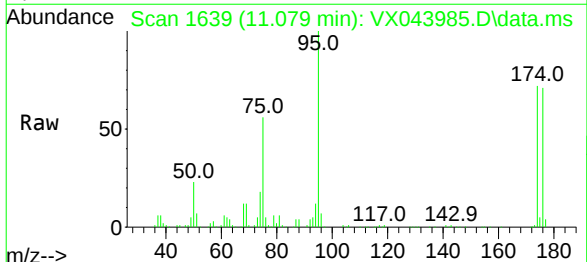



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.006 min

Lab File: VX043985.D

Acq: 25 Nov 2024 14:40

Instrument :

MSVOA_X

ClientSampleId :

Storage-Blank-WATER-REF-5





Tgt Ion:117 Resp: 196892

Ion Ratio Lower Upper

117 100

82 57.7 46.4 69.6

119 33.9 24.6 37.0

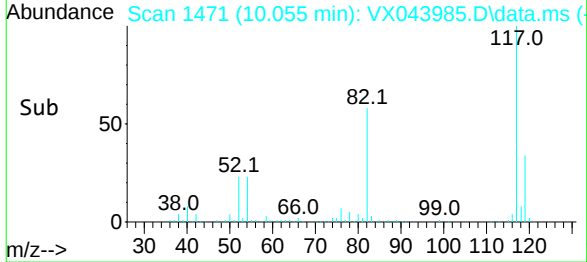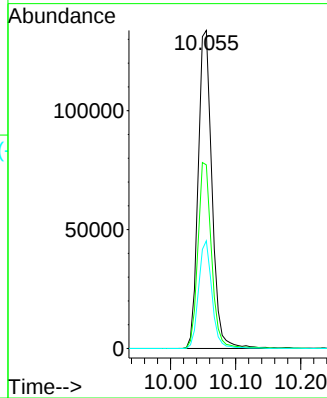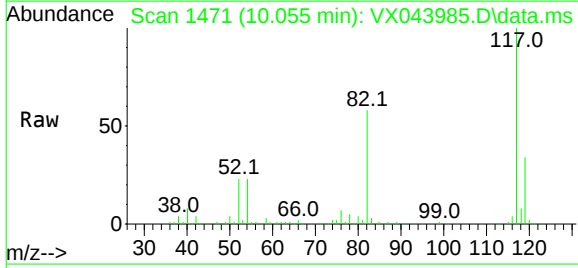

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX043985.D

Acq: 25 Nov 2024 14:40

Tgt Ion:152 Resp: 84391

Ion Ratio Lower Upper

152 100

115 62.2 45.4 136.2

150 156.1 0.0 353.0

