

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112024\
 Data File : P0108163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 00:12
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:16:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.371	3.638	203.8E6	78678373	23.410	23.206
2) SA Decachlor...	10.094	8.635	80103065	79365693	26.227	23.331

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112024\
Data File : PO108163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 00:12
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:16:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

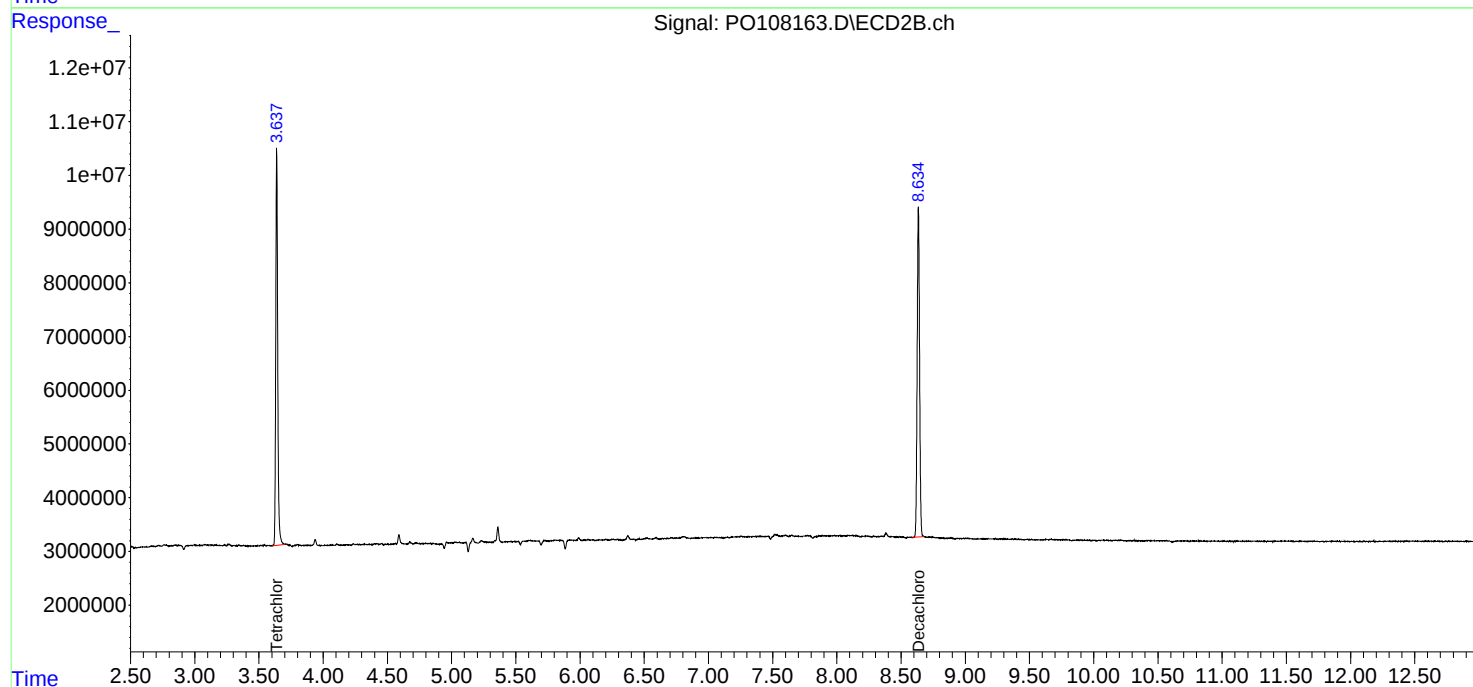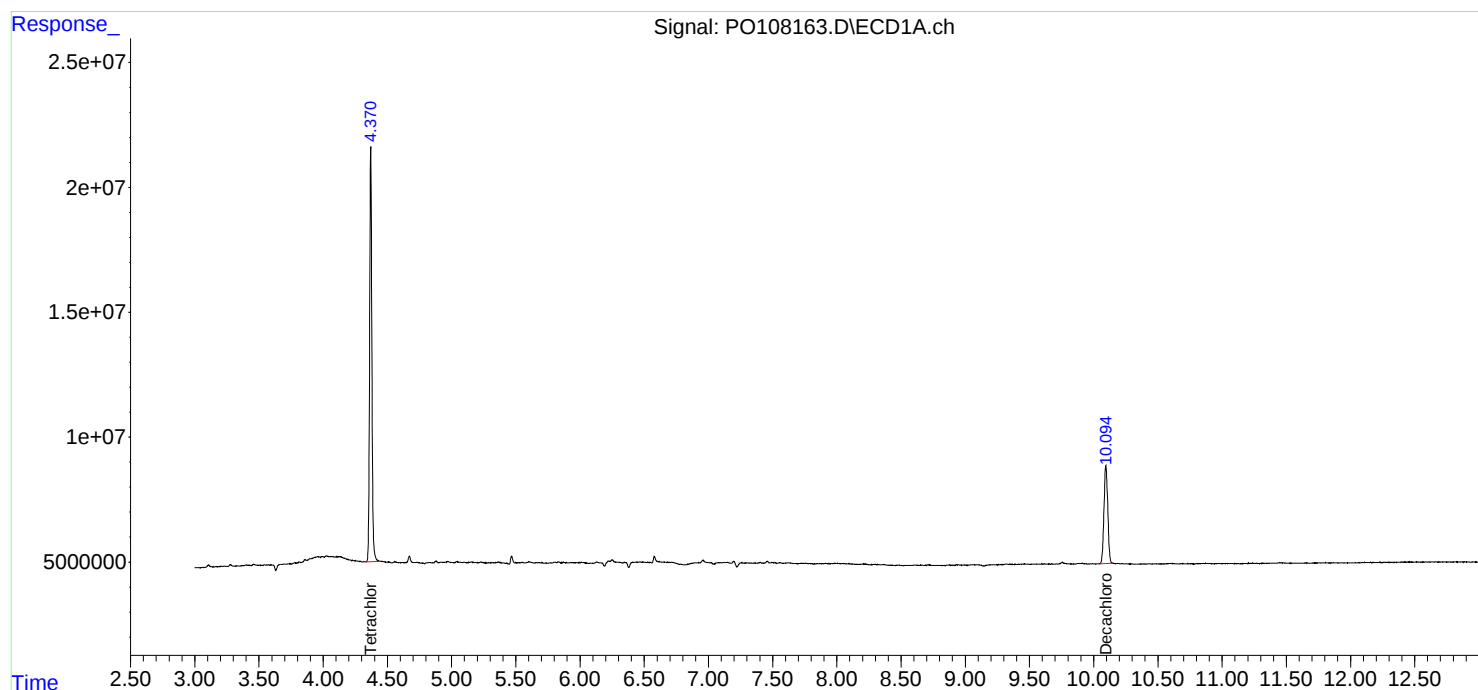


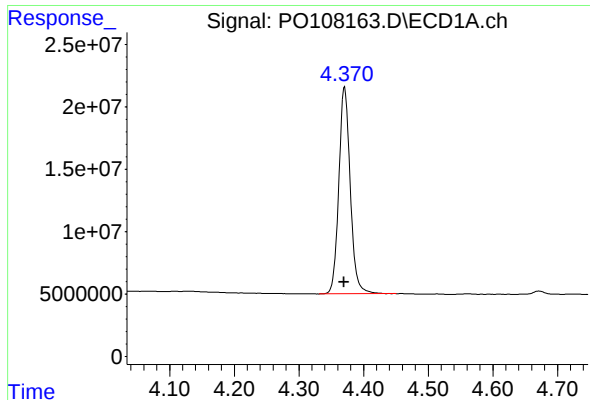

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 203805657
Conc: 23.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

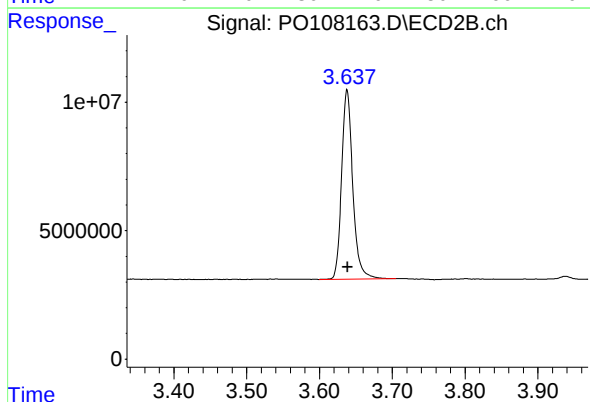


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.000 min
Response: 78678373
Conc: 23.21 ng/ml

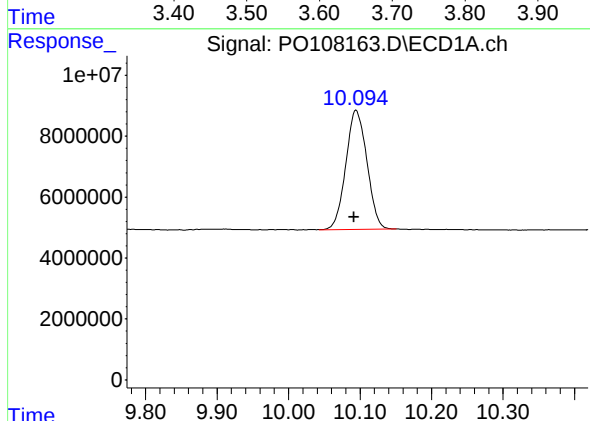

#2 Decachlorobiphenyl

R.T.: 10.094 min
Delta R.T.: 0.003 min
Response: 80103065
Conc: 26.23 ng/ml

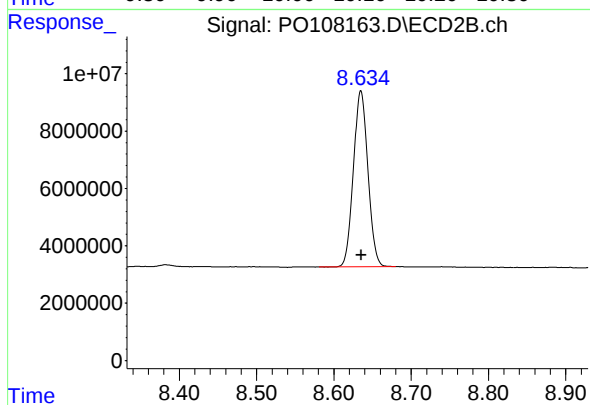

#2 Decachlorobiphenyl

R.T.: 8.635 min
Delta R.T.: 0.000 min
Response: 79365693
Conc: 23.33 ng/ml