

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112224\
Data File : PS028600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2024 12:25
Operator : AR\AJ
Sample : P4892-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WB-310-BOT

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2024
Supervised By :Ankita Jodhani 11/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 21:01:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.231	7.730	1398.0E6	605.3E6	546.962m	468.400m
------	----------	-------	-------	----------	---------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112224\
Data File : PS028600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2024 12:25
Operator : AR\AJ
Sample : P4892-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
WB-310-BOT


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/25/2024
Supervised By :Ankita Jodhani 11/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 21:01:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

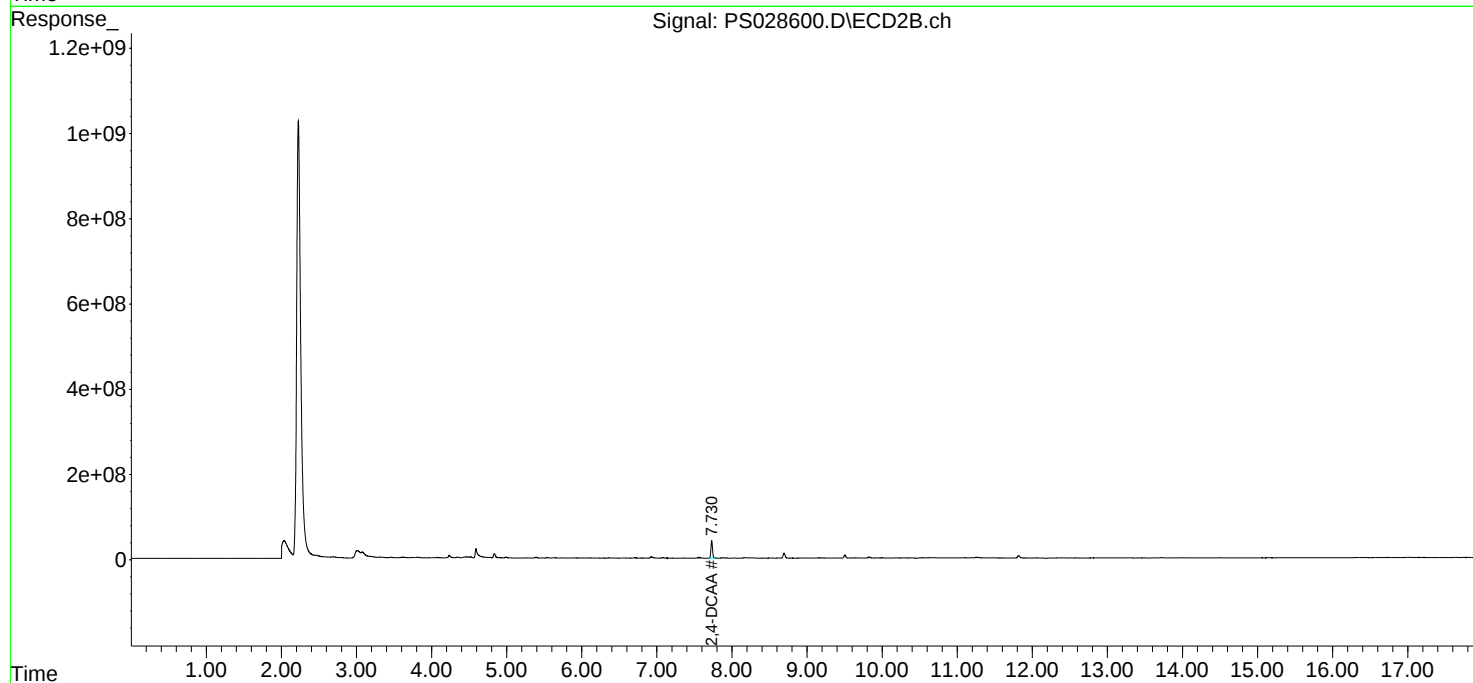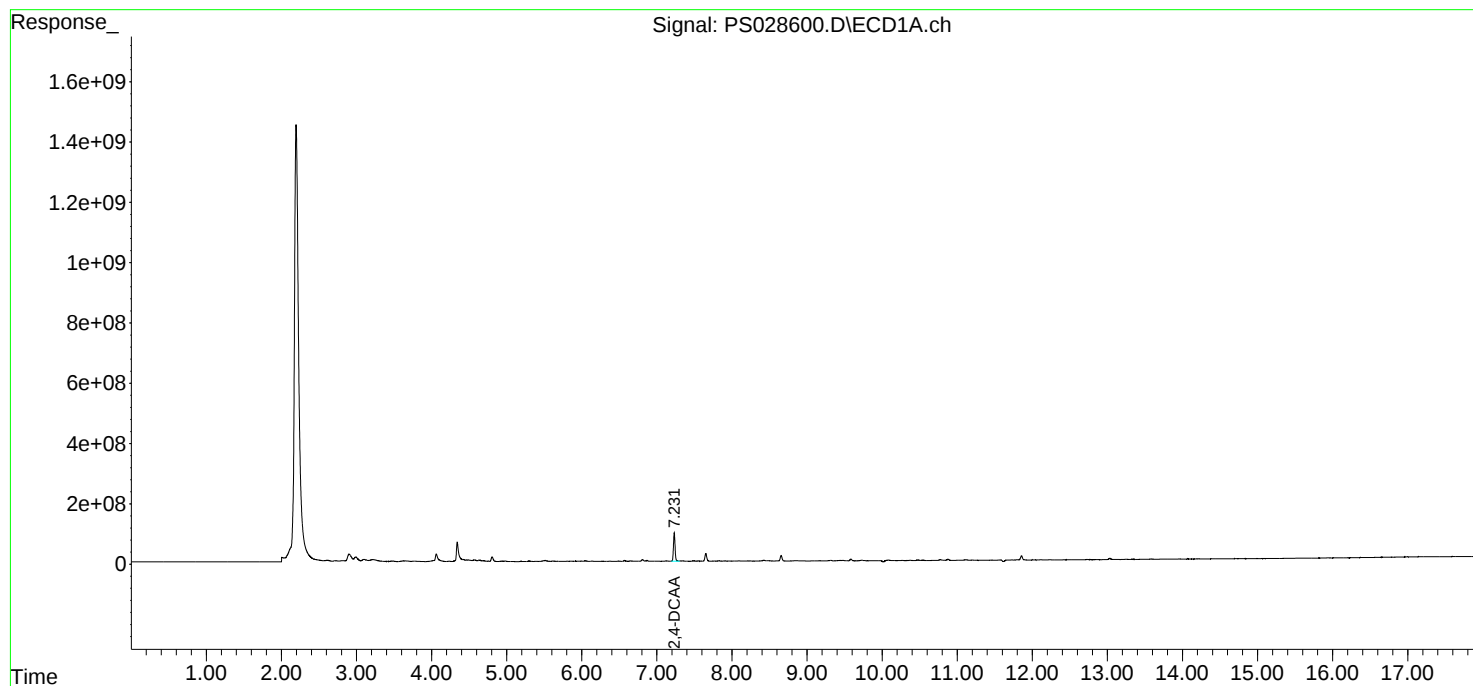

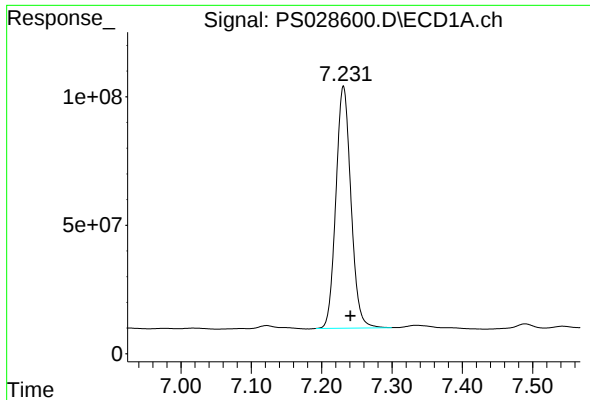

#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.010 min
Response: 1397969975
Conc: 546.96 ng/ml

Instrument :

ECD_S


ClientSampleId :

WB-310-BOT

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/25/2024
Supervised By :Ankita Jodhani 11/25/2024

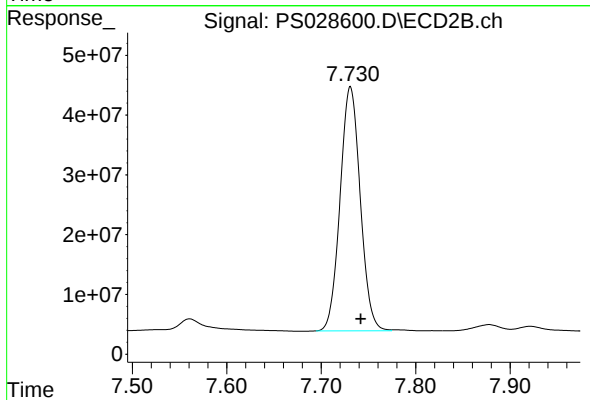

#4 2,4-DCAA

R.T.: 7.730 min
Delta R.T.: -0.011 min
Response: 605316166
Conc: 468.40 ng/ml m