
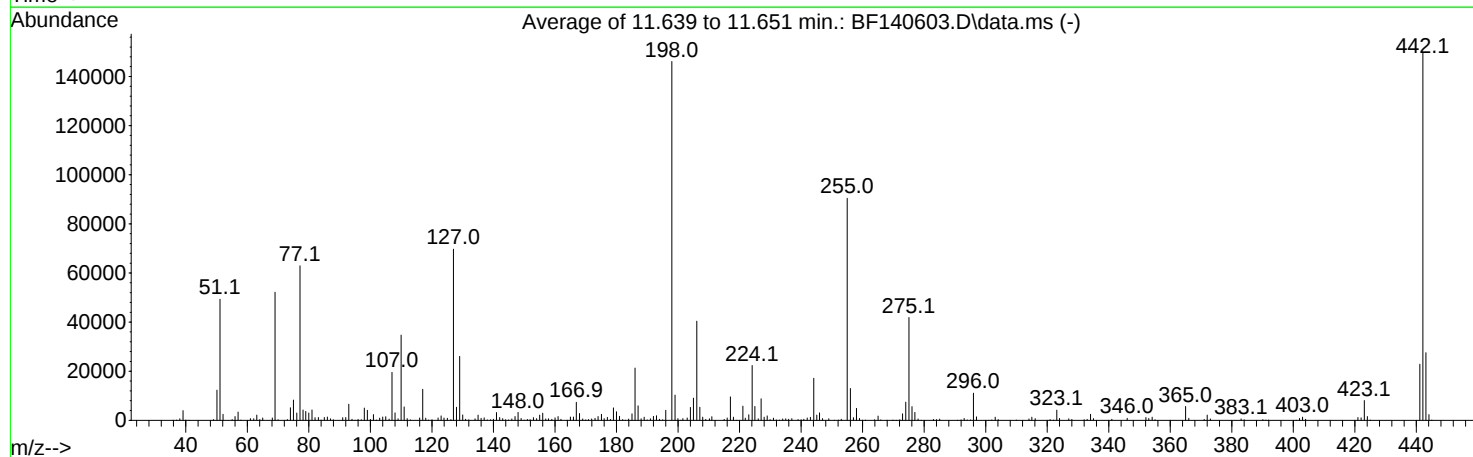


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140603.D
Acq On : 25 Nov 2024 15:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

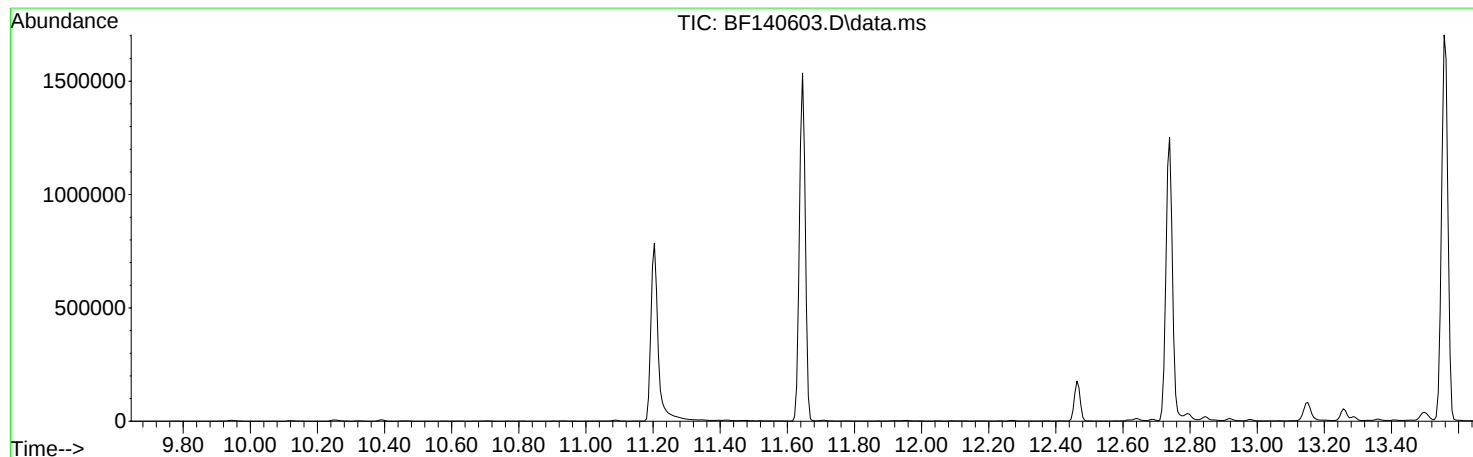

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	49309	PASS
68	69	0.00	2	1.8	961	PASS
69	198	0.00	100	35.7	52187	PASS
70	69	0.00	2	0.5	279	PASS
127	198	10	80	47.7	69688	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146083	PASS
199	198	5	9	7.0	10280	PASS
275	198	10	60	28.7	41893	PASS
365	198	1	100	3.9	5656	PASS
441	198	0.01	100	15.6	22843	PASS
442	442	50	100	100.0	149765	PASS
443	442	15	24	18.4	27568	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/25/2024	BNA_F	<u>BF140603.D</u>
Compound Name	Response	Retention Time
DDT	443715	13.557
DDD	19336	13.257
DDE	2495	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21831	465546	4.69

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140603.D
Acq On : 25 Nov 2024 15:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 15:47:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

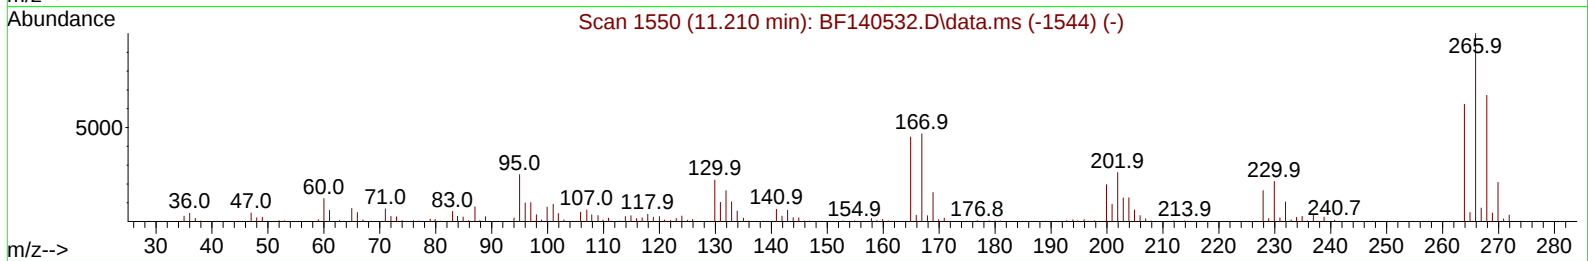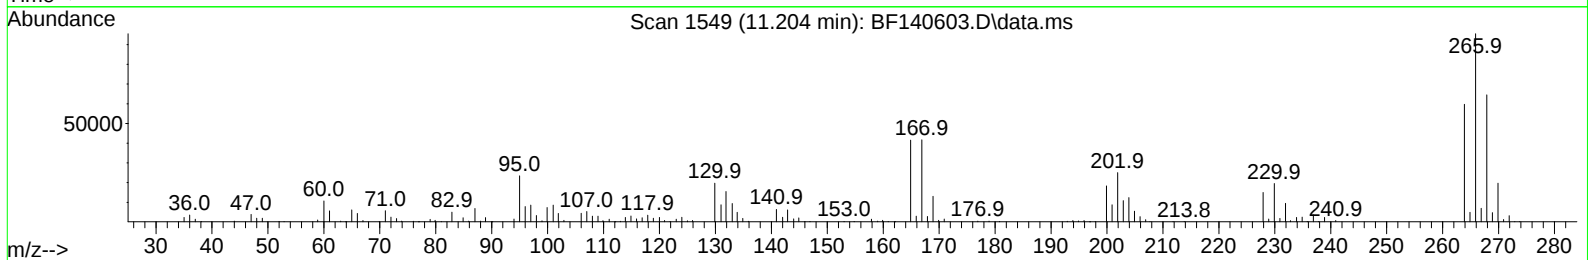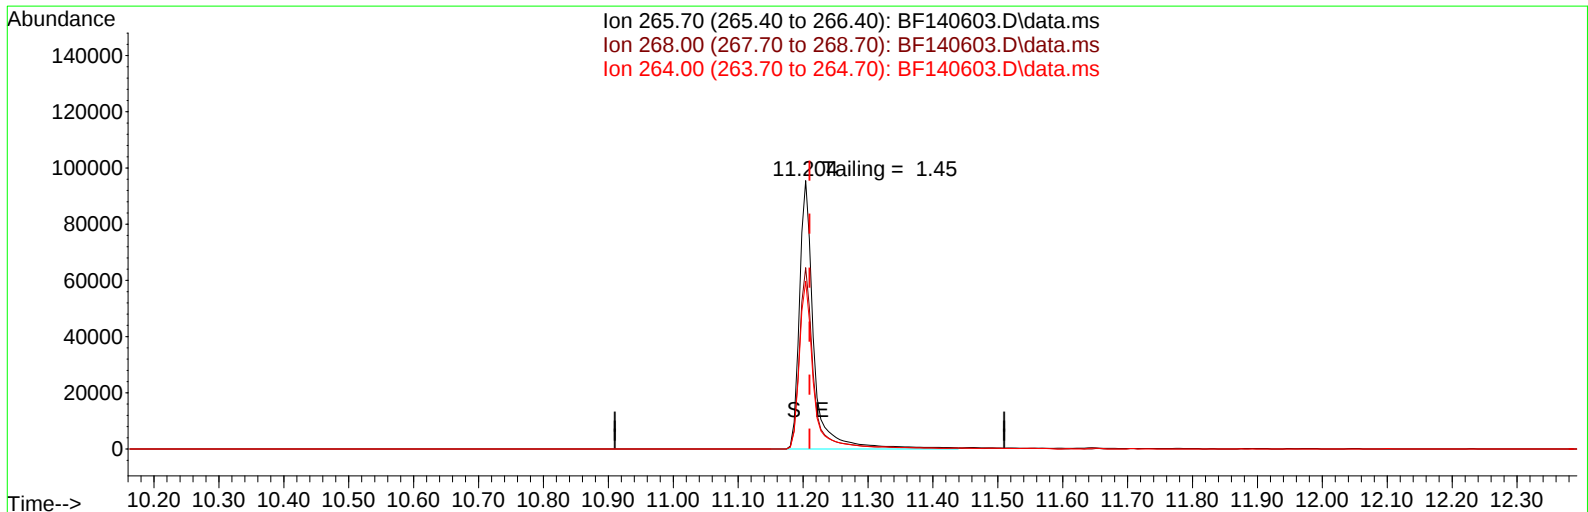

TIC: BF140603.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 19738.30 ng




response 147516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	67.54
264.00	62.30	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140603.D
Acq On : 25 Nov 2024 15:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 15:47:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

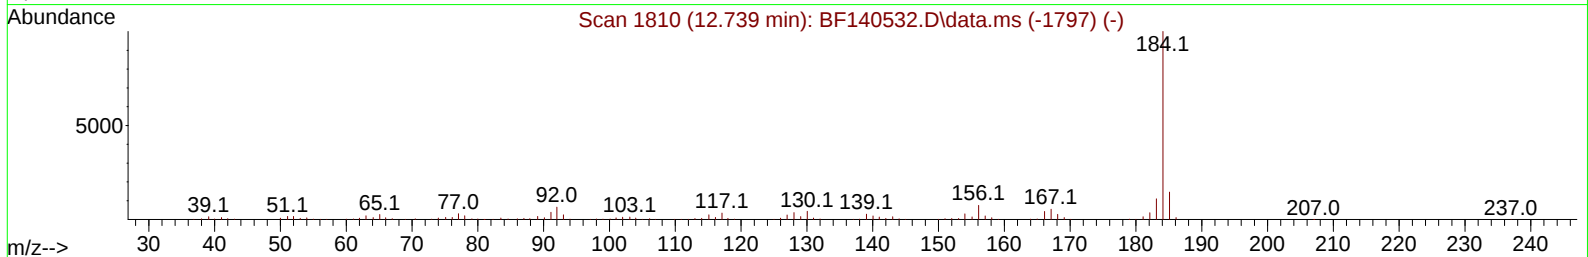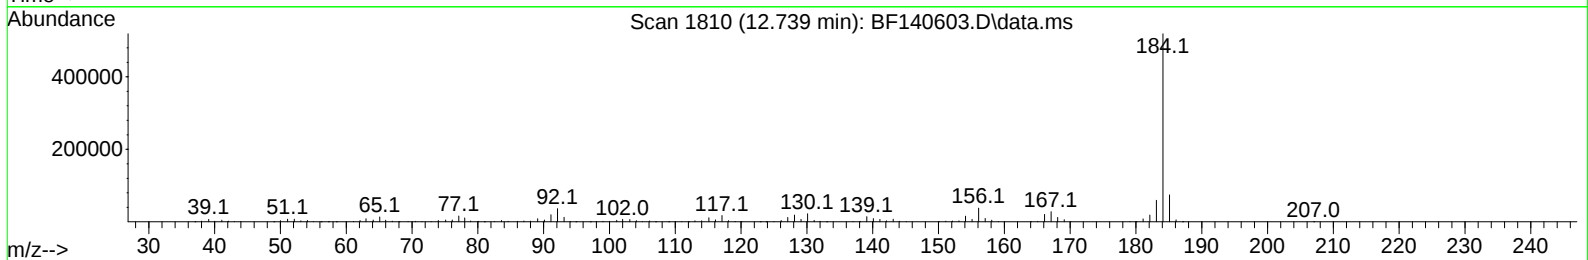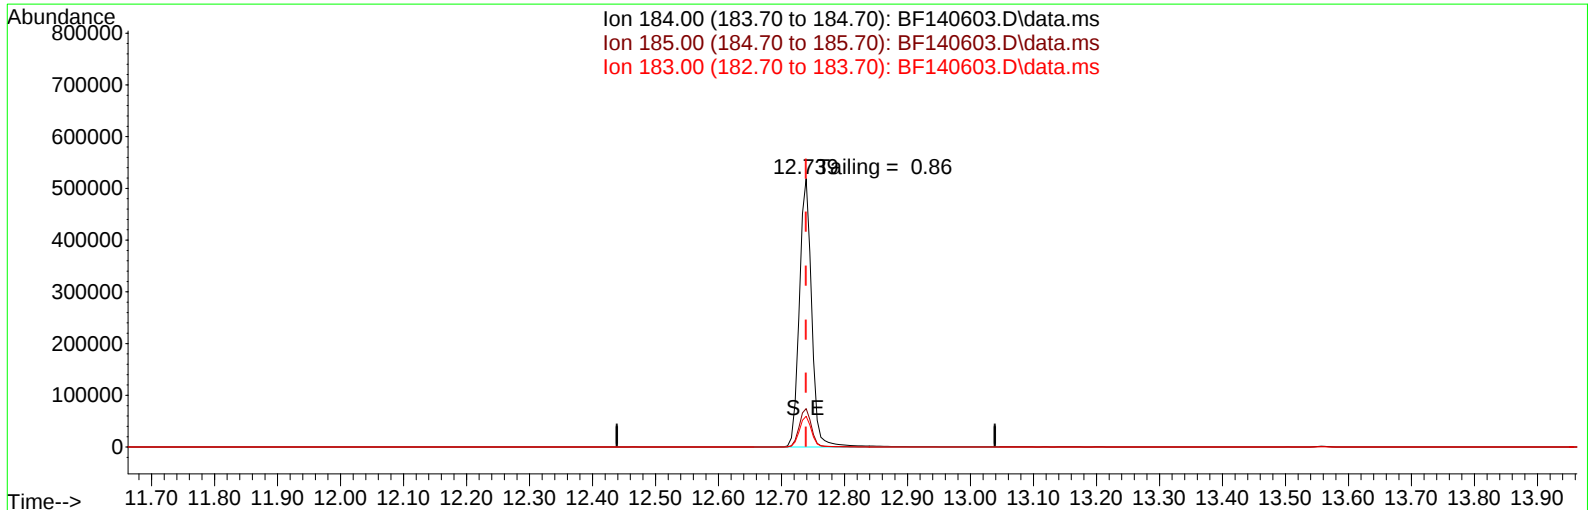

TIC: BF140603.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 26793.97 ng

response 714361

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	11.00	11.43
0.00	0.00	0.00