

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140502.D
Acq On : 20 Nov 2024 16:25
Operator : RC/JU
Sample : PB165086BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165086BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	13	24	33	rVB	36727	68976	1.59%	0.265%
2	5.510	575	581	601	rBV	2436895	3313261	76.37%	12.715%
3	6.510	745	751	772	rBV	2373825	3422684	78.89%	13.135%
4	6.869	807	812	818	rBV	588850	747517	17.23%	2.869%
5	7.434	901	908	913	rBV	1631004	2262765	52.16%	8.684%
6	8.151	1024	1030	1042	rBV	739729	978201	22.55%	3.754%
7	9.228	1206	1213	1239	rBV	3140239	4255047	98.08%	16.329%
8	9.904	1319	1328	1351	rVB	835802	1151952	26.55%	4.421%
9	10.698	1457	1463	1489	rBV	1853447	2633458	60.70%	10.106%
10	11.398	1576	1582	1598	rBV	954304	1240417	28.59%	4.760%
11	12.986	1846	1852	1857	rBV	3254922	4338530	100.00%	16.649%
12	14.045	2026	2032	2048	rVB	683287	933706	21.52%	3.583%
13	15.539	2279	2286	2299	rBV	405830	711575	16.40%	2.731%




Sum of corrected areas: 26058089

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140502.D
Acq On : 20 Nov 2024 16:25
Operator : RC/JU
Sample : PB165086BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

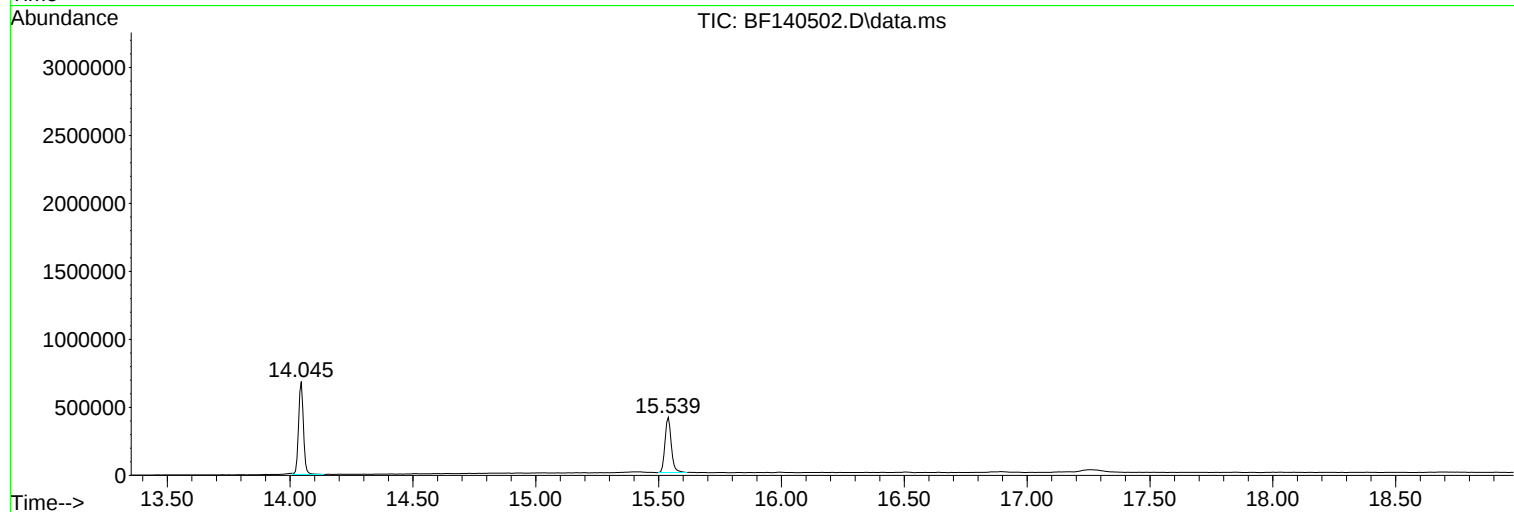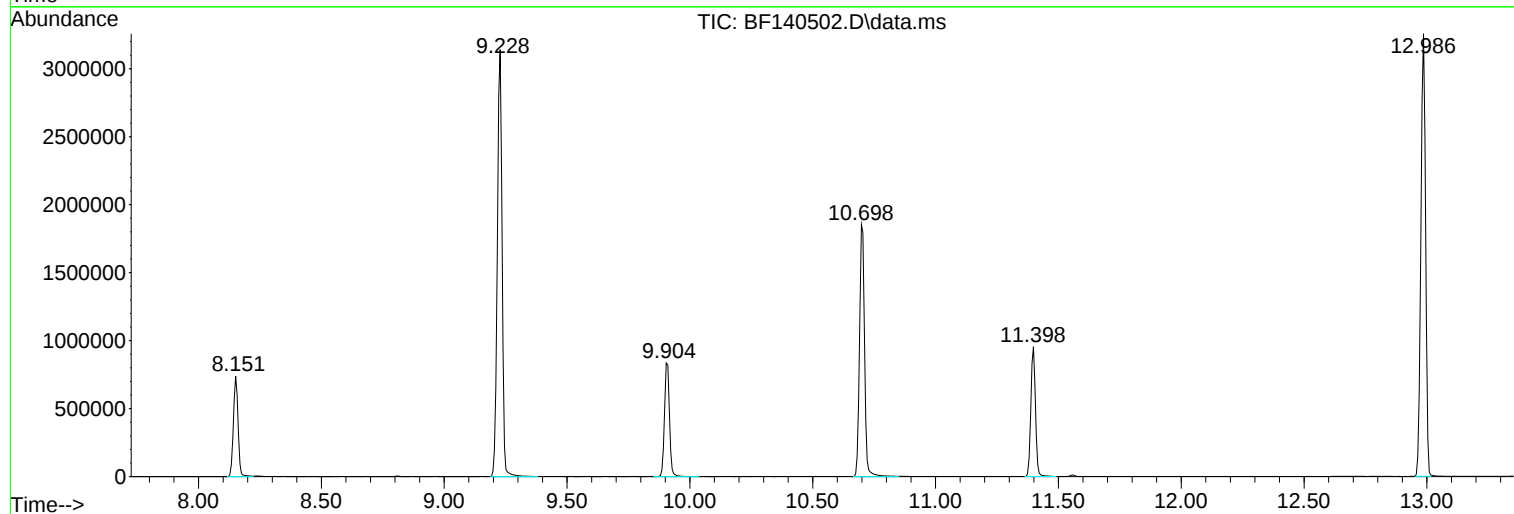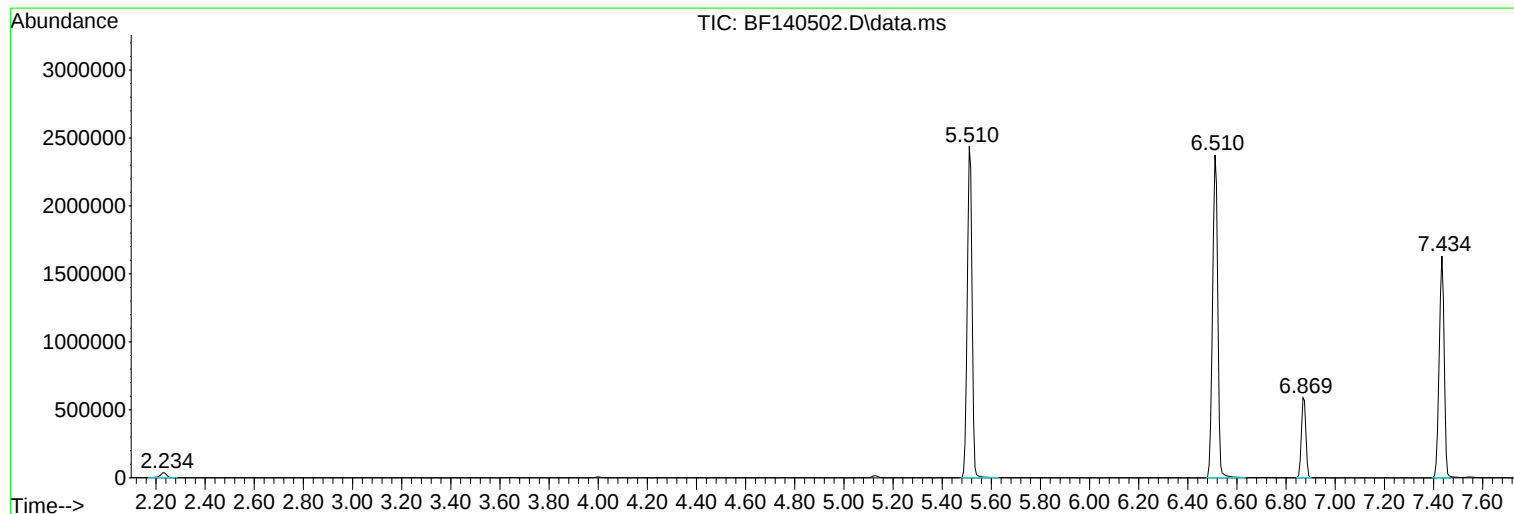

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140502.D
Acq On : 20 Nov 2024 16:25
Operator : RC/JU
Sample : PB165086BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112024\
Data File : BF140502.D
Acq On : 20 Nov 2024 16:25
Operator : RC/JU
Sample : PB165086BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------