
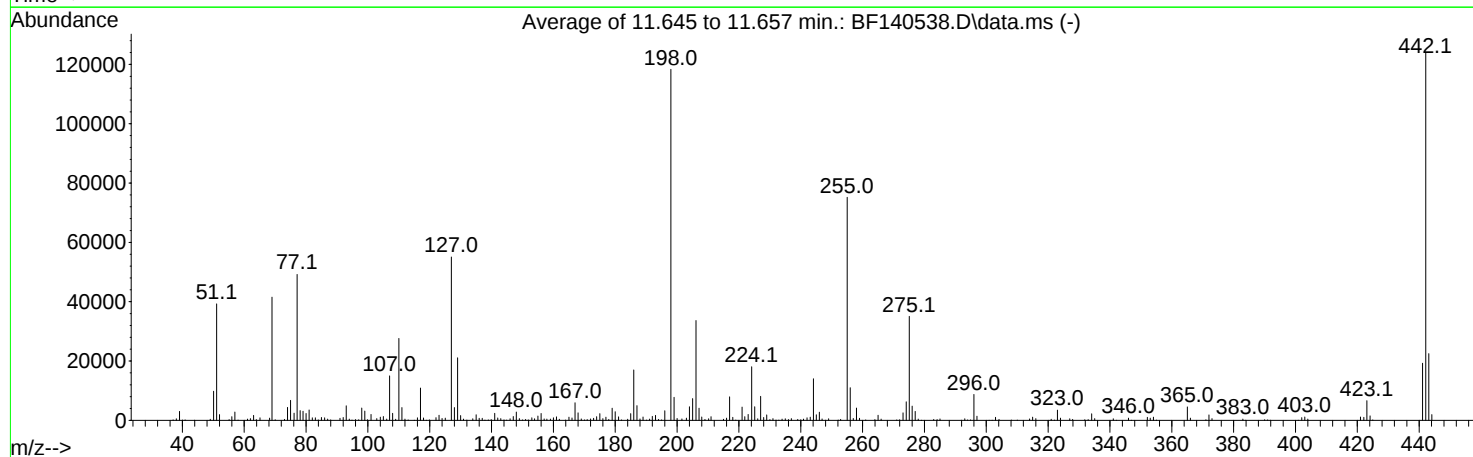


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140538.D
Acq On : 21 Nov 2024 16:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

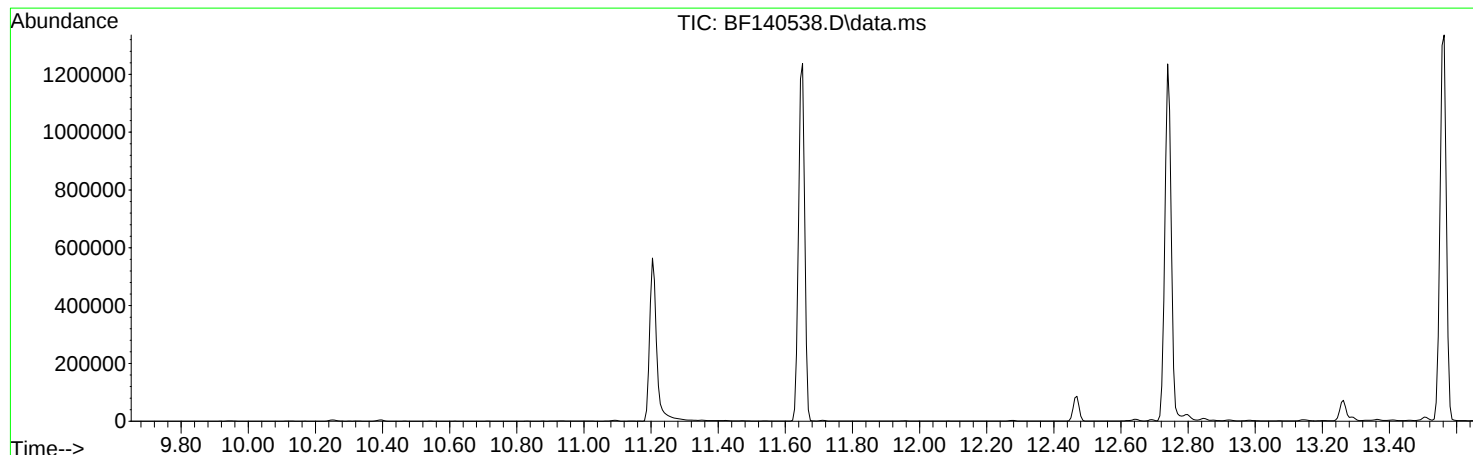

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	39277	PASS
68	69	0.00	2	1.9	779	PASS
69	198	0.00	100	35.1	41536	PASS
70	69	0.00	2	0.6	240	PASS
127	198	10	80	46.5	55053	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118333	PASS
199	198	5	9	6.6	7774	PASS
275	198	10	60	29.6	35048	PASS
365	198	1	100	3.8	4545	PASS
441	198	0.01	100	16.3	19261	PASS
442	442	50	100	100.0	124011	PASS
443	442	15	24	18.1	22475	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/21/2024	BNA_F	<u>BF140536.D</u>
Compound Name	Response	Retention Time
DDT	345993	13.563
DDD	23422	13.263
DDE	1044	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24466	370459	6.60

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140538.D
Acq On : 21 Nov 2024 16:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 21 16:59:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

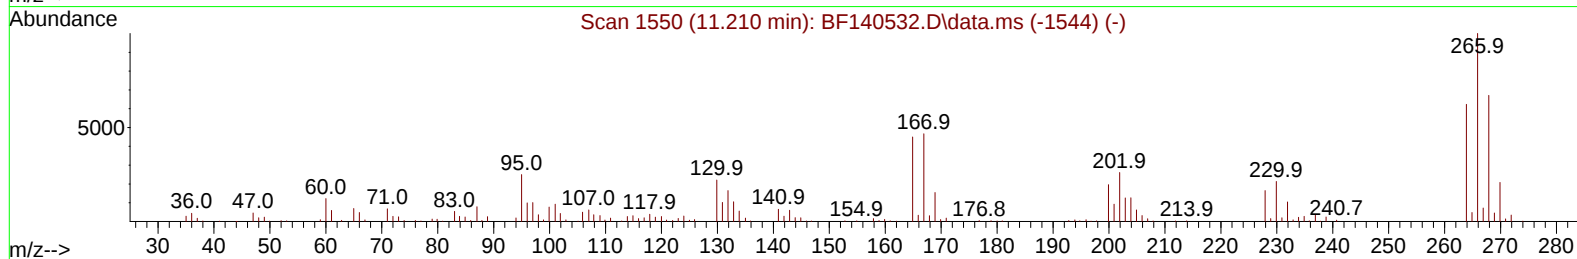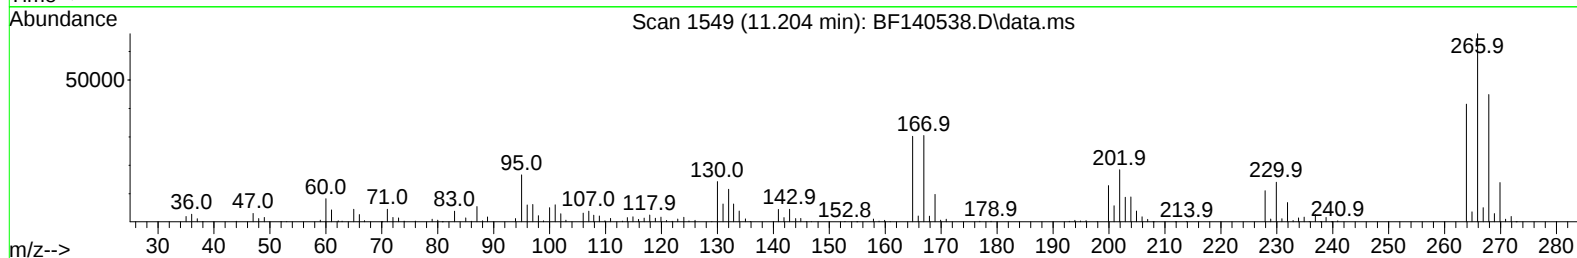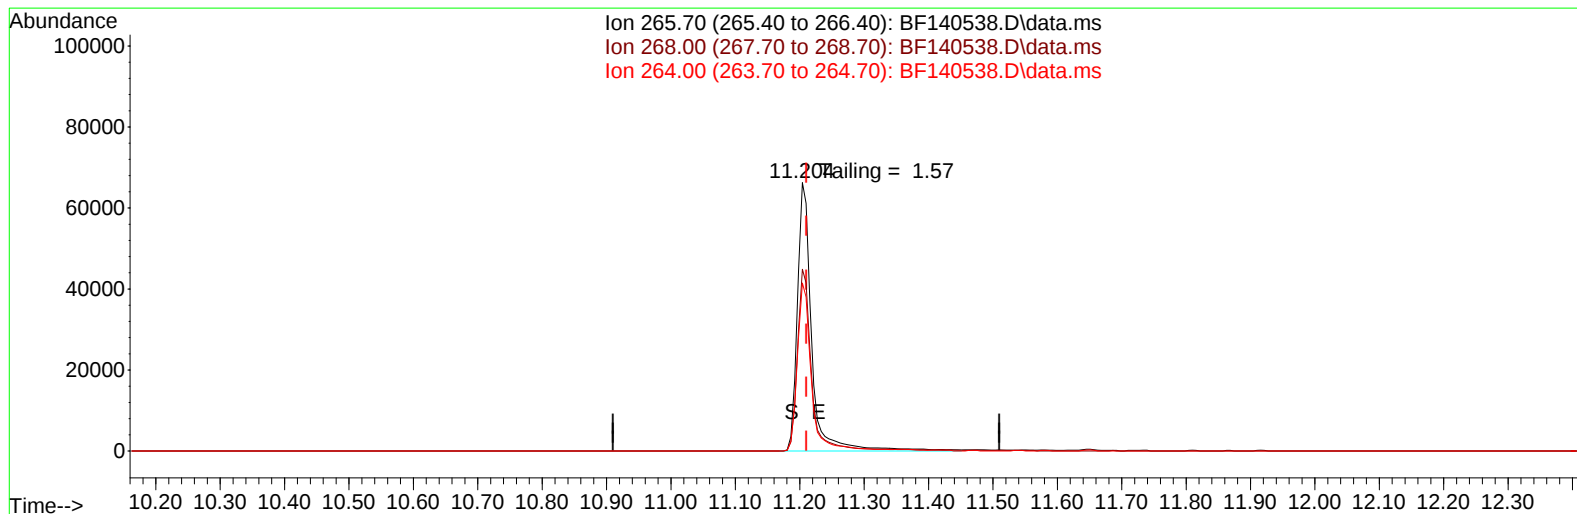

TIC: BF140538.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 29910.91 ng




response 102823

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	67.75
264.00	62.30	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140538.D
Acq On : 21 Nov 2024 16:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 21 16:59:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

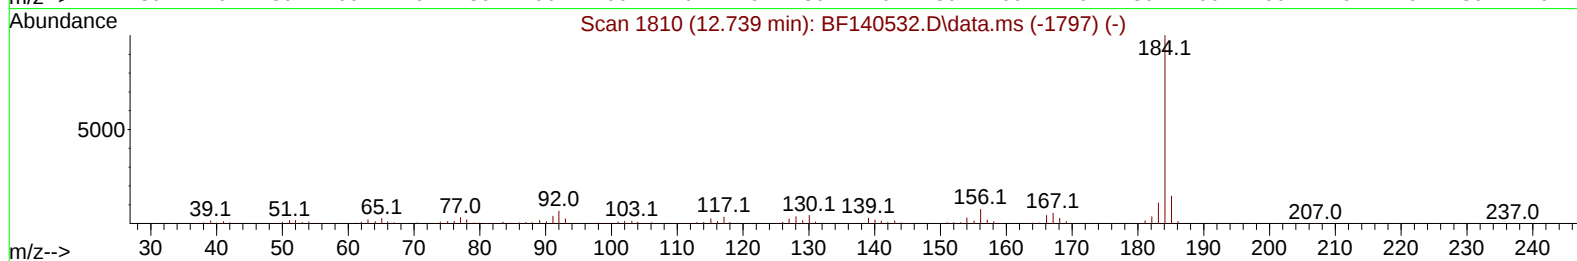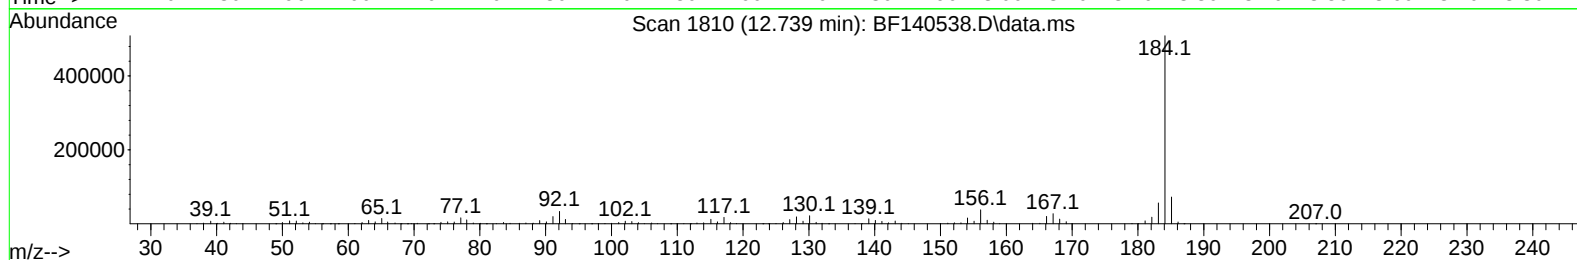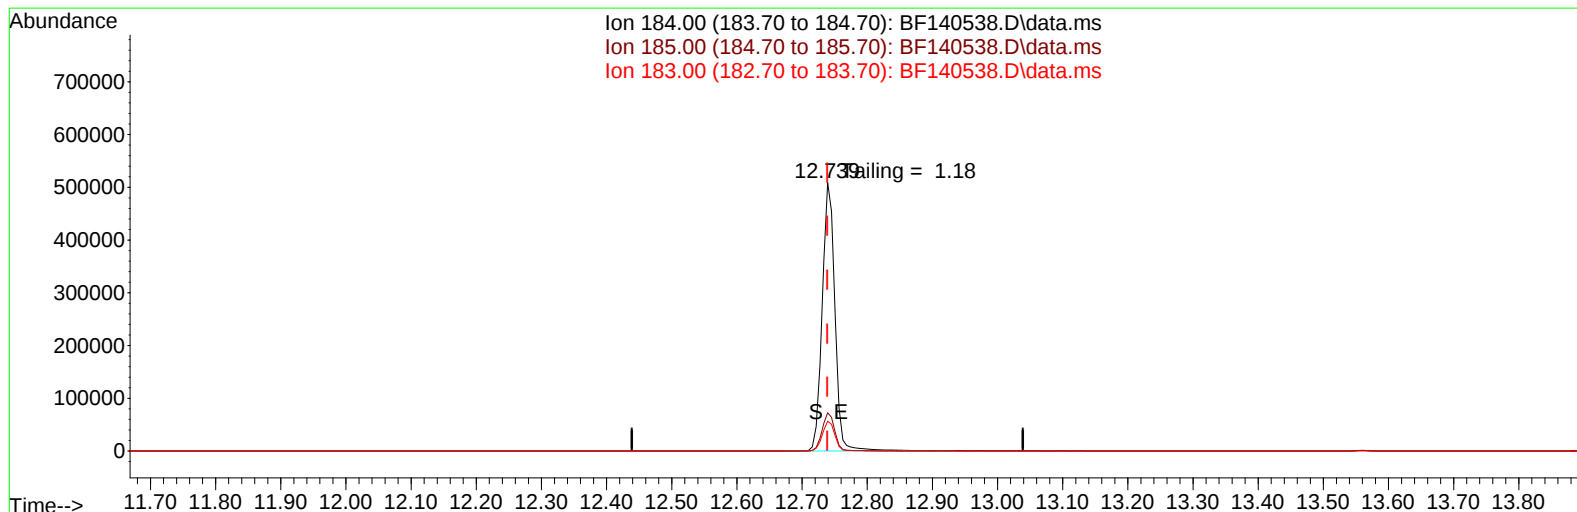

TIC: BF140538.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 64322.88 ng

response 691956

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.28
183.00	11.00	11.13
0.00	0.00	0.00