

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112124\
 Data File : PL093202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 12:08
 Operator : AR\AJ
 Sample : P4921-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-11-A-202411

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :Ankita Jodhani 11/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 23:37:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.772	50138356	55159163	20.463	20.270m
28) SA Decachlor...	9.056	7.914	33551265	52824317	17.433	19.355

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112124\
Data File : PL093202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 12:08
Operator : AR\AJ
Sample : P4921-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-11-A-202411


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :Ankita Jodhani 11/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 23:37:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

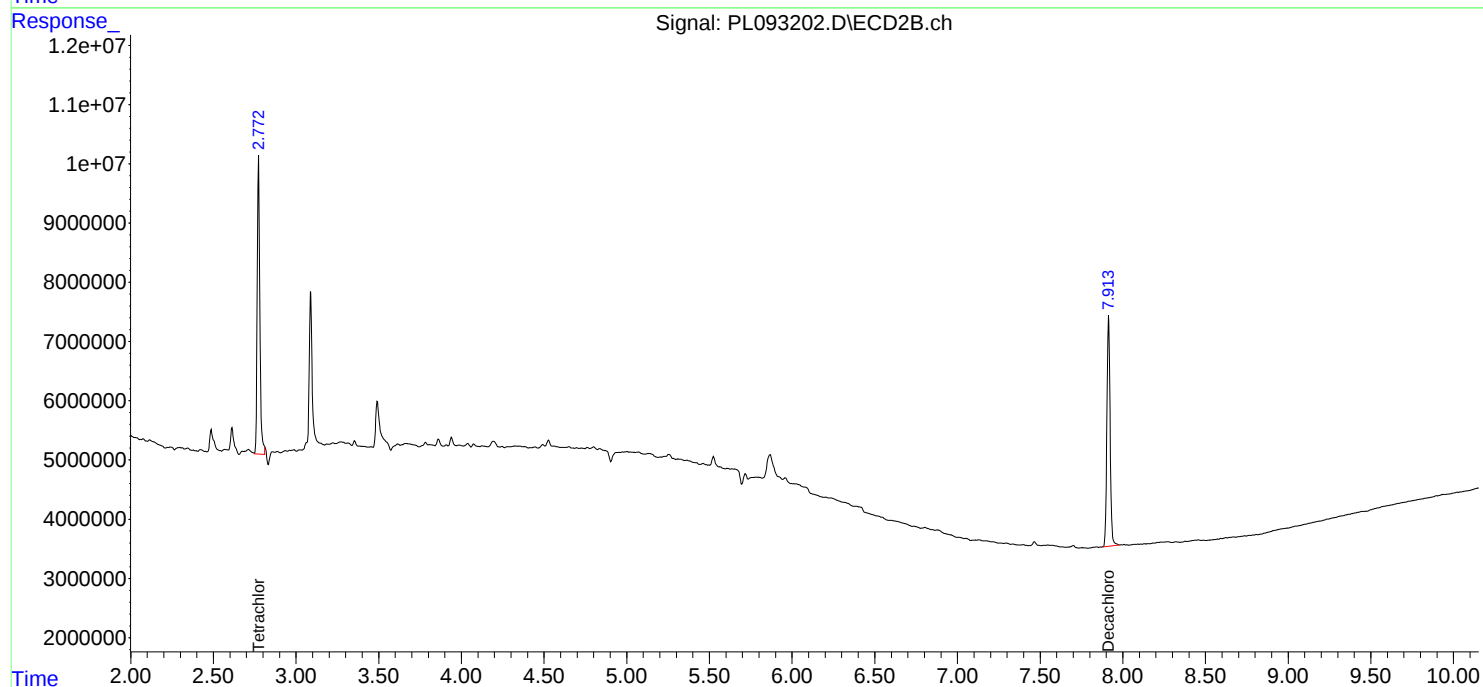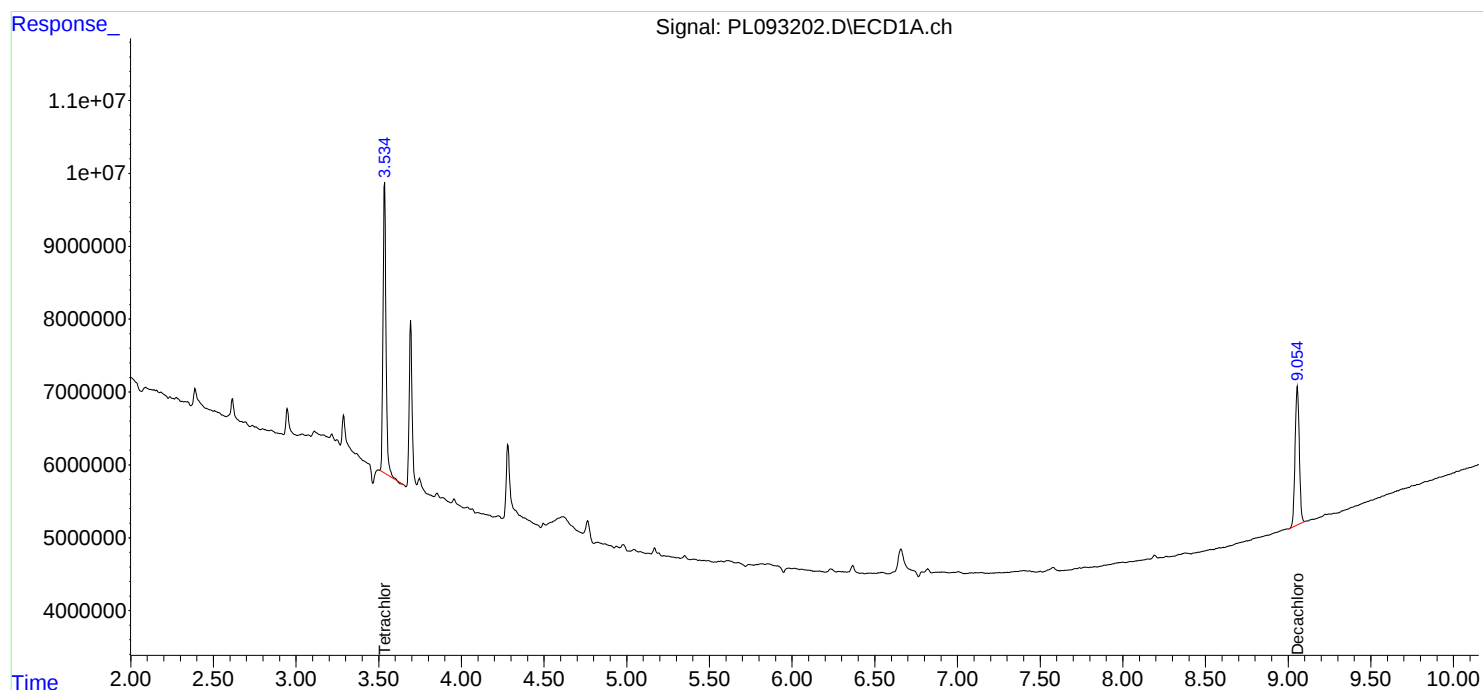

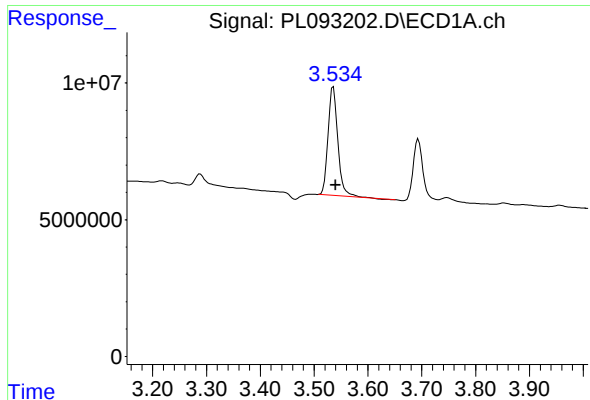


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.004 min
Response: 50138356
Conc: 20.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-11-A-202411


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :Ankita Jodhani 11/22/2024

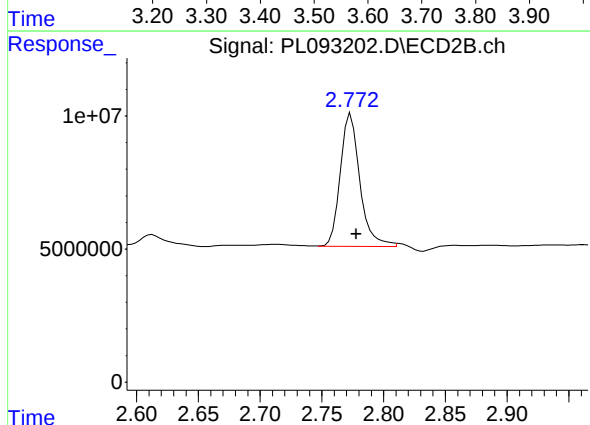


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.006 min
Response: 55159163
Conc: 20.27 ng/ml

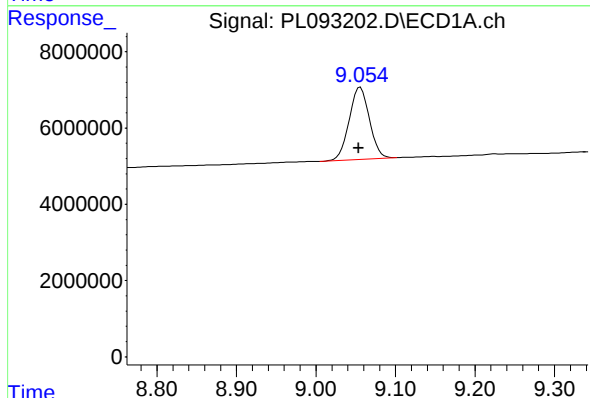

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.002 min
Response: 33551265
Conc: 17.43 ng/ml

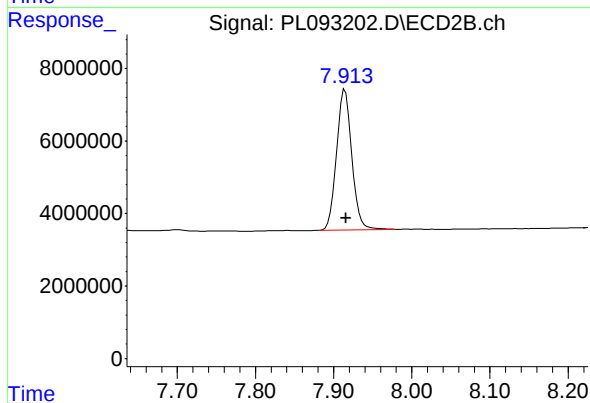

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: -0.001 min
Response: 52824317
Conc: 19.35 ng/ml