
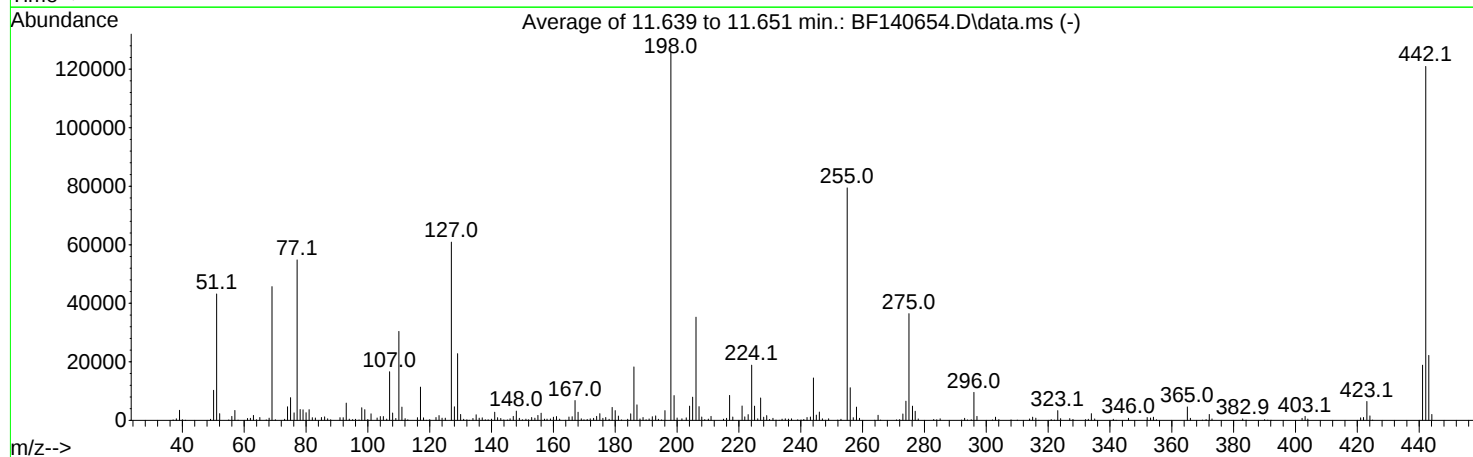


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112724\
Data File : BF140654.D
Acq On : 27 Nov 2024 08:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

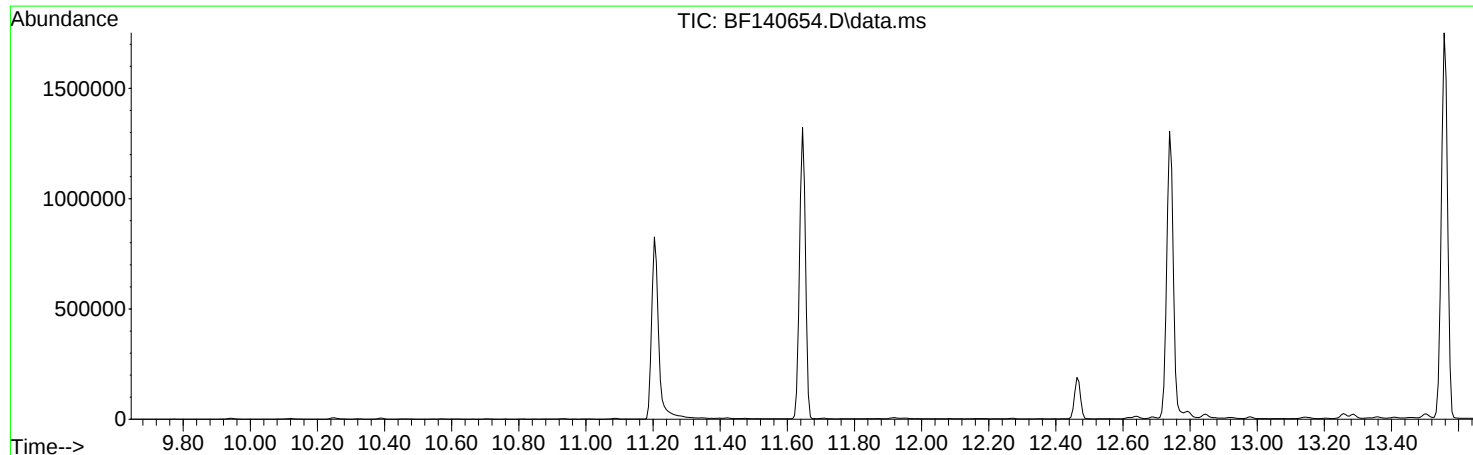

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	43184	PASS
68	69	0.00	2	1.6	746	PASS
69	198	0.00	100	36.3	45685	PASS
70	69	0.00	2	0.5	244	PASS
127	198	10	80	48.4	60880	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125693	PASS
199	198	5	9	6.7	8459	PASS
275	198	10	60	29.0	36451	PASS
365	198	1	100	3.6	4587	PASS
441	198	0.01	100	15.0	18852	PASS
442	442	50	100	100.0	120963	PASS
443	442	15	24	18.4	22197	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/27/2024	BNA_F	<u>BF140654.D</u>
Compound Name	Response	Retention Time
DDT	443642	13.557
DDD	11651	13.257
DDE	1547	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13198	456840	2.89

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112724\
Data File : BF140654.D
Acq On : 27 Nov 2024 08:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 27 10:02:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

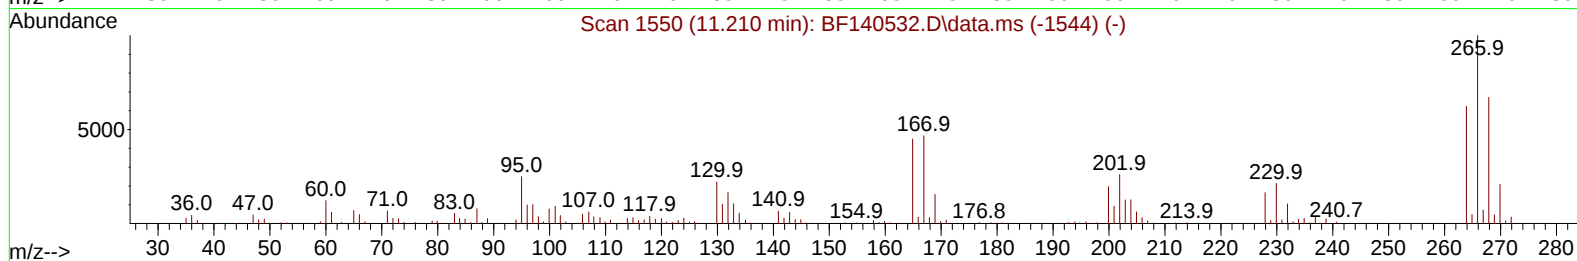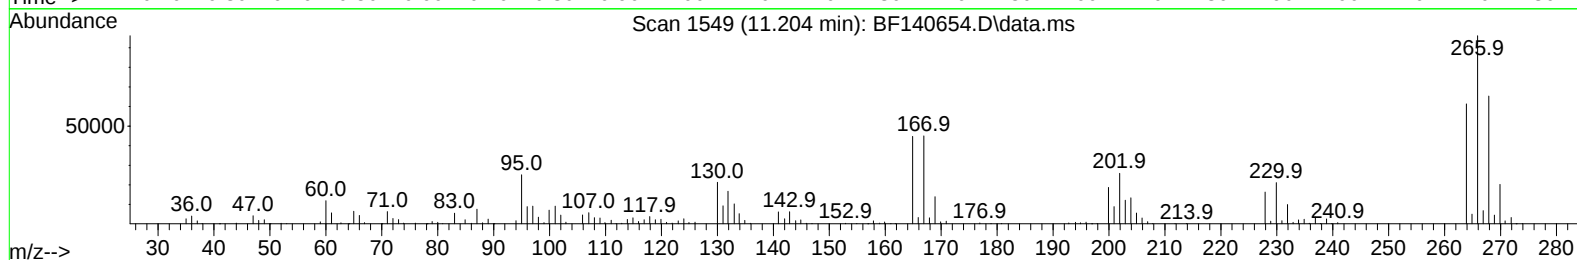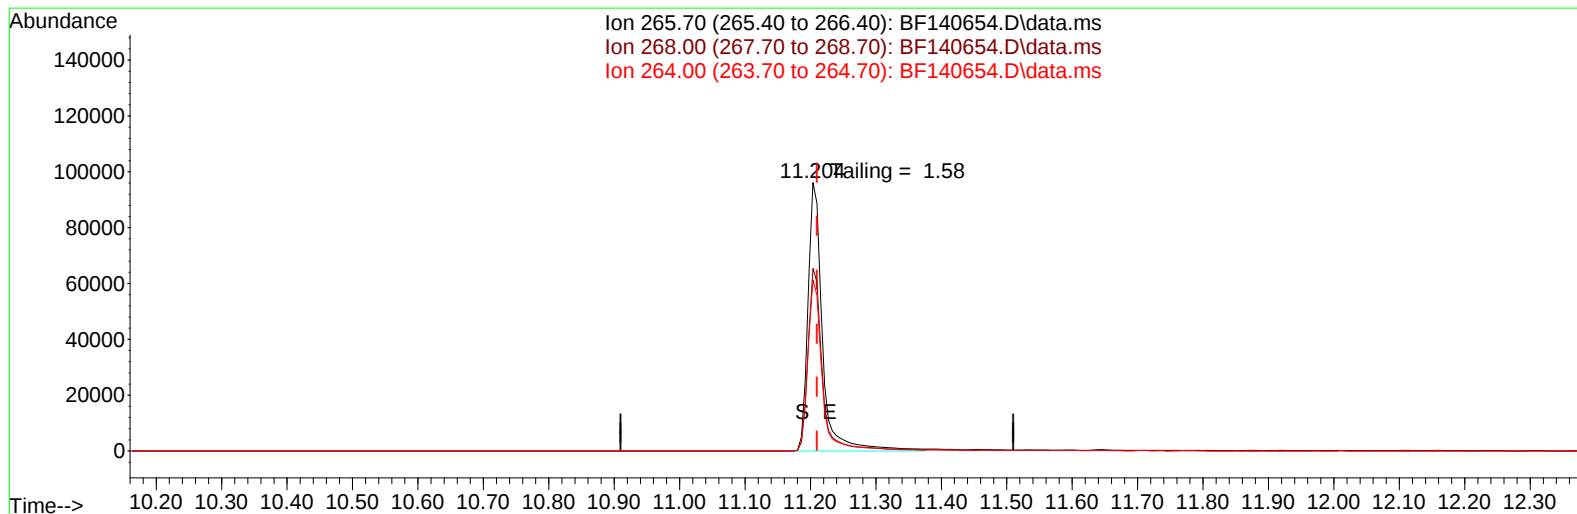

TIC: BF140654.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 18220.94 ng




response 148512

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	67.98
264.00	62.30	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112724\
Data File : BF140654.D
Acq On : 27 Nov 2024 08:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 27 10:02:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

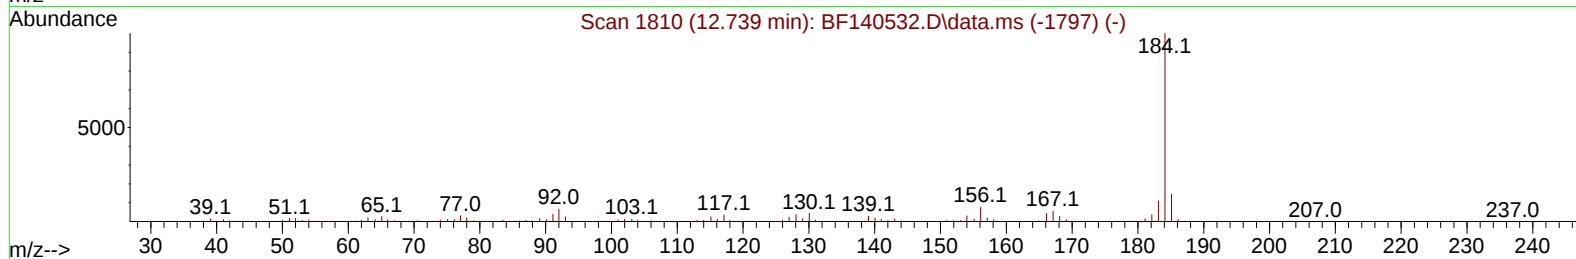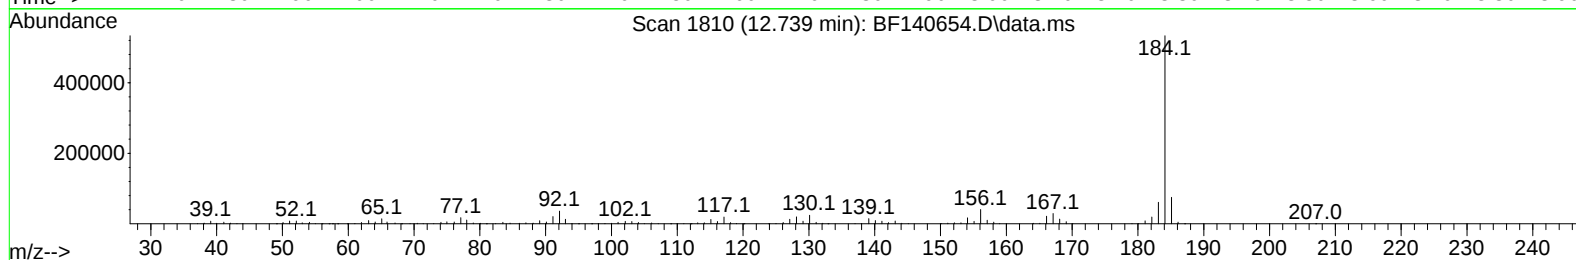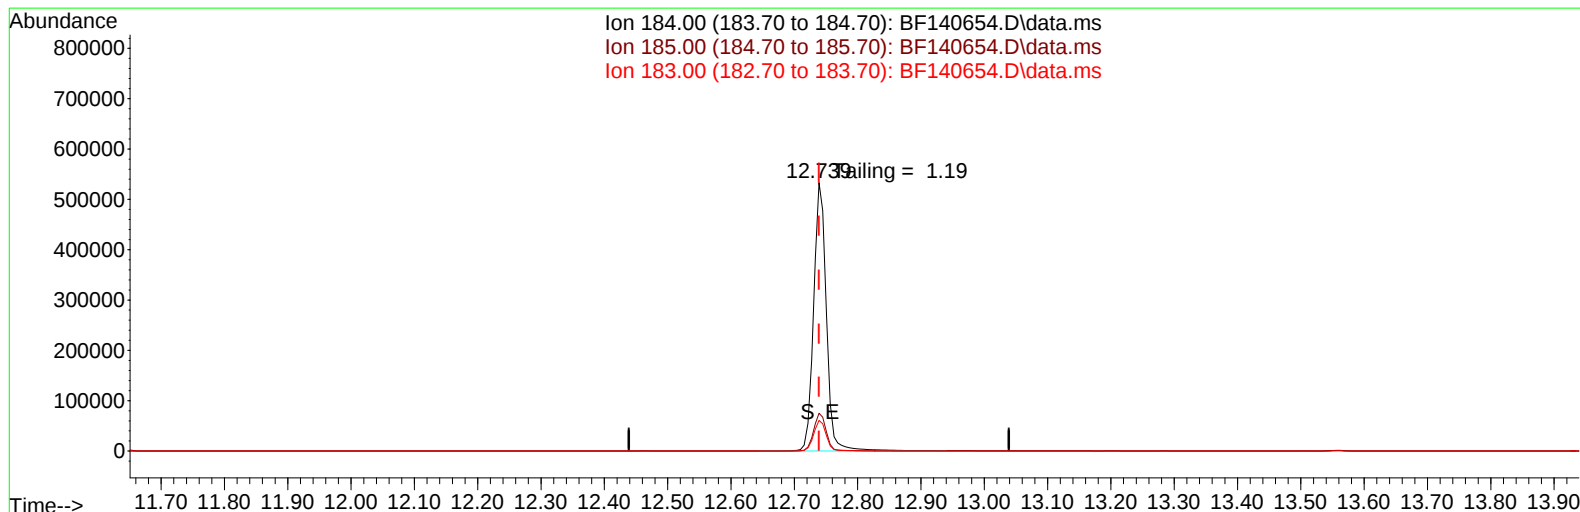

TIC: BF140654.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 21492.30 ng

response 752976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.09
183.00	11.00	11.40
0.00	0.00	0.00