
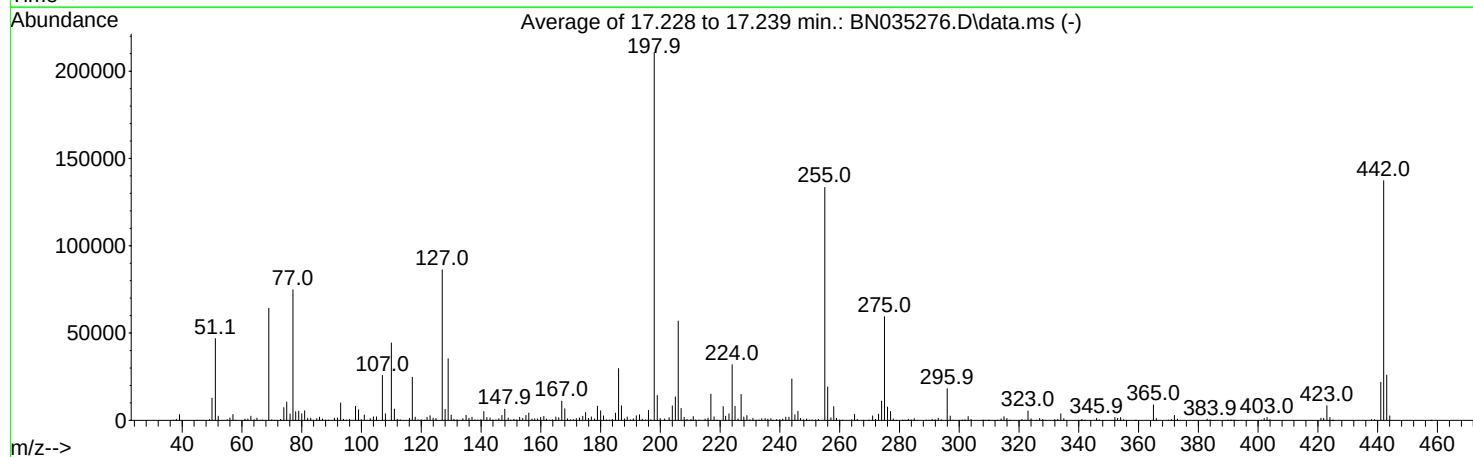


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035276.D
Acq On : 25 Nov 2024 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 26 02:36:08 2024

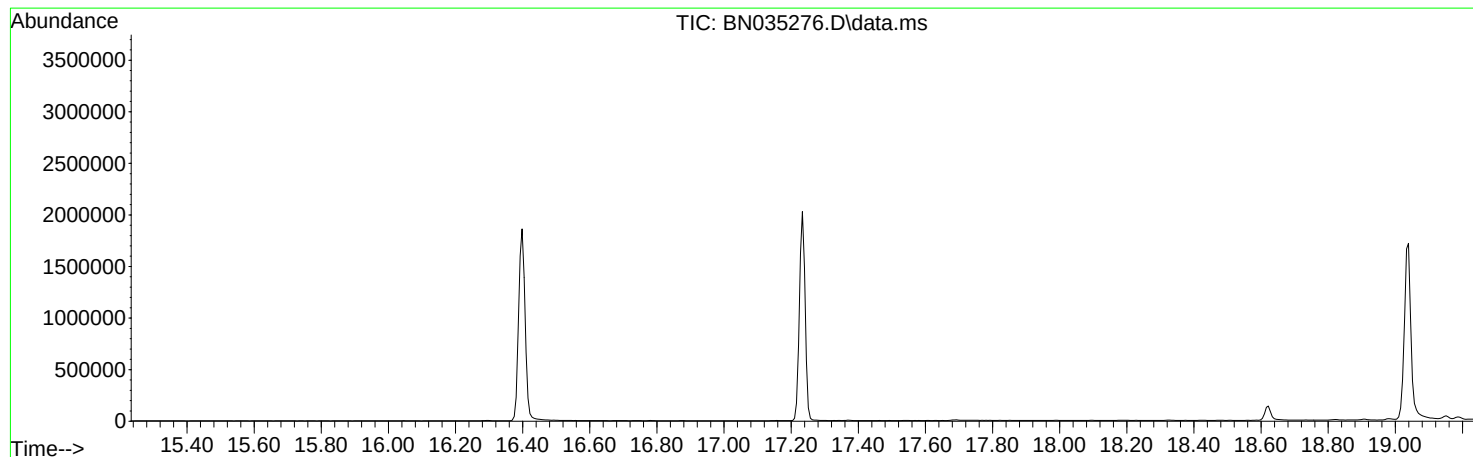

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	46795	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.5	64280	PASS
70	69	0.00	2	0.5	352	PASS
127	198	10	80	40.9	86240	PASS
197	198	0.00	2	0.2	340	PASS
198	198	100	100	100.0	210688	PASS
199	198	5	9	6.7	14182	PASS
275	198	10	60	28.2	59405	PASS
365	198	1	100	4.2	8892	PASS
441	198	0.01	100	10.4	21850	PASS
442	442	50	100	100.0	137299	PASS
443	442	15	24	18.9	25952	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/25/2024	BNA_N	<u>BN035276.D</u>
Compound Name	Response	Retention Time
DDT	703573	20.292
DDD	32612	19.845
DDE	1098	19.333
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33710	737283	4.57

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035276.D
Acq On : 25 Nov 2024 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 26 05:17:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:17:50 2024
Response via : Initial Calibration

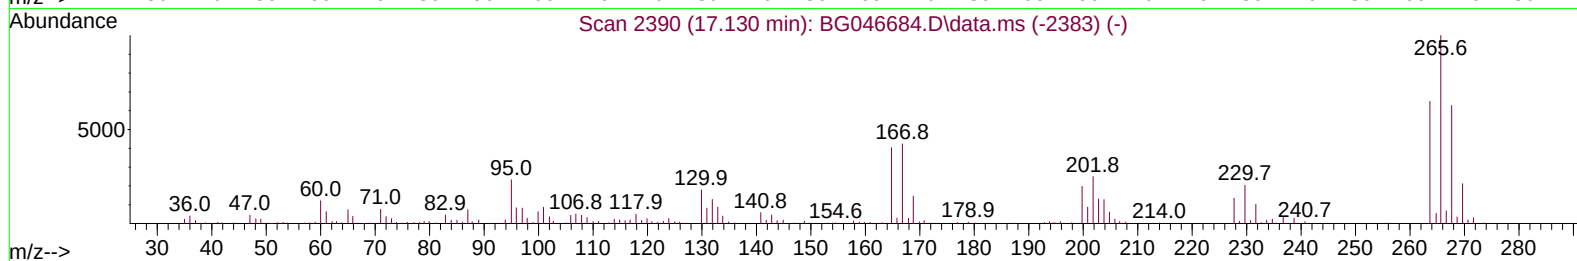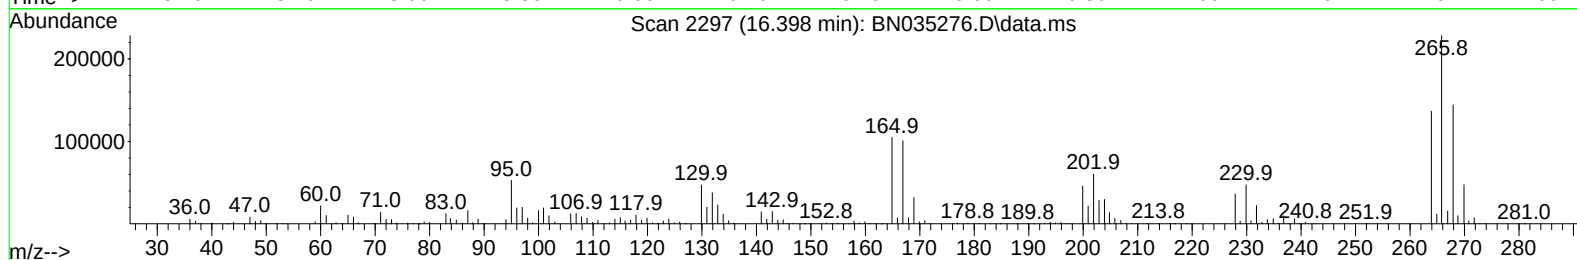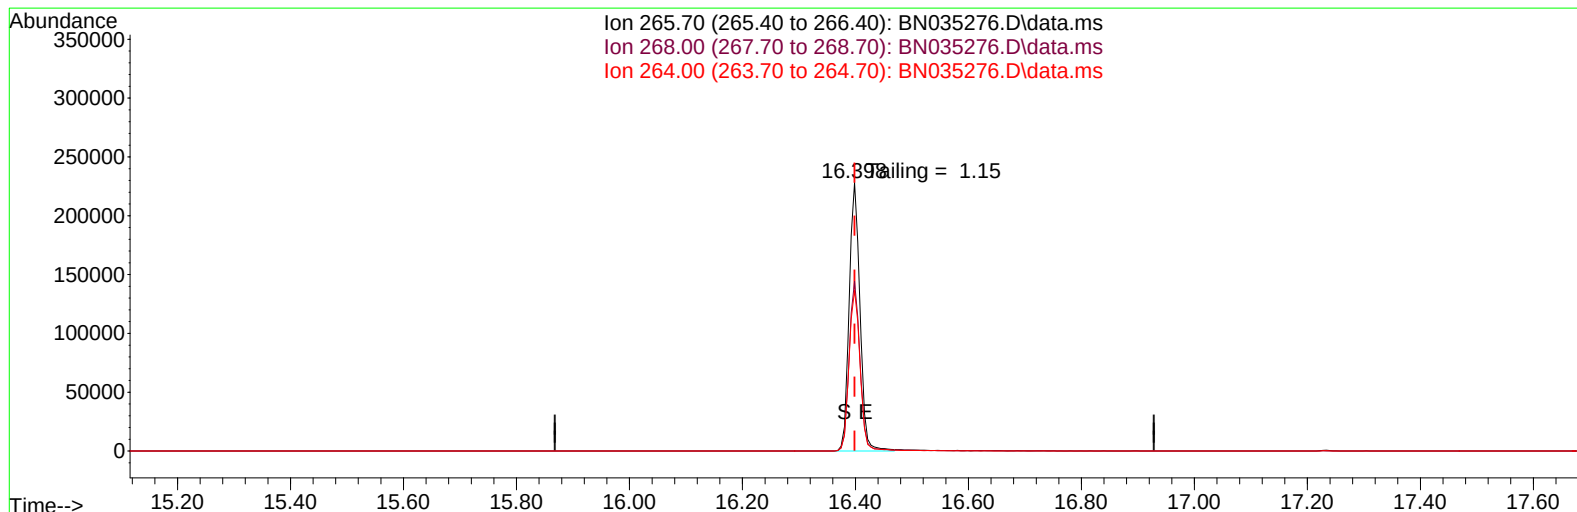

TIC: BN035276.D\data.ms

(70) Pentachlorophenol (C)

16.398min (0.000) 33730.33 ng




response 307325

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.17
264.00	61.60	59.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035276.D
Acq On : 25 Nov 2024 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 26 05:17:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:17:50 2024
Response via : Initial Calibration

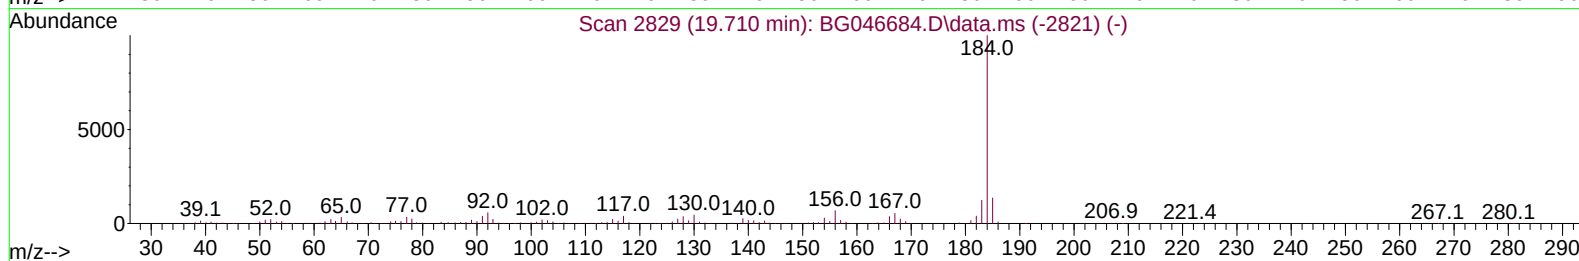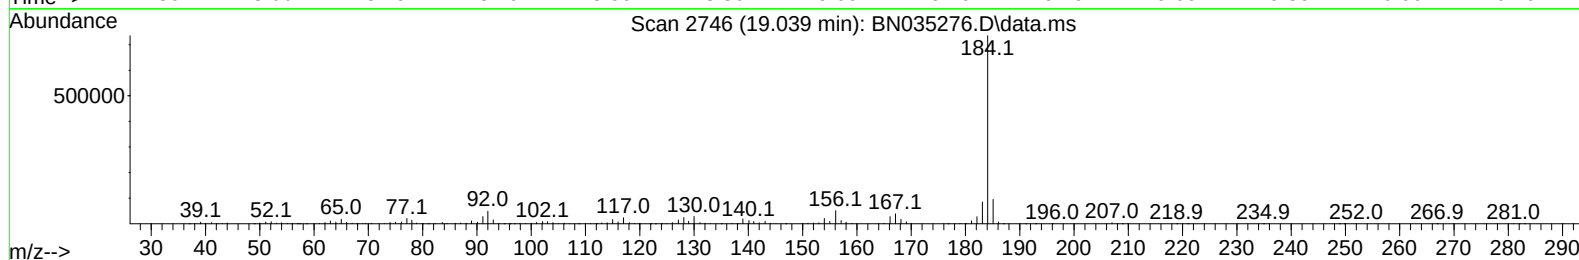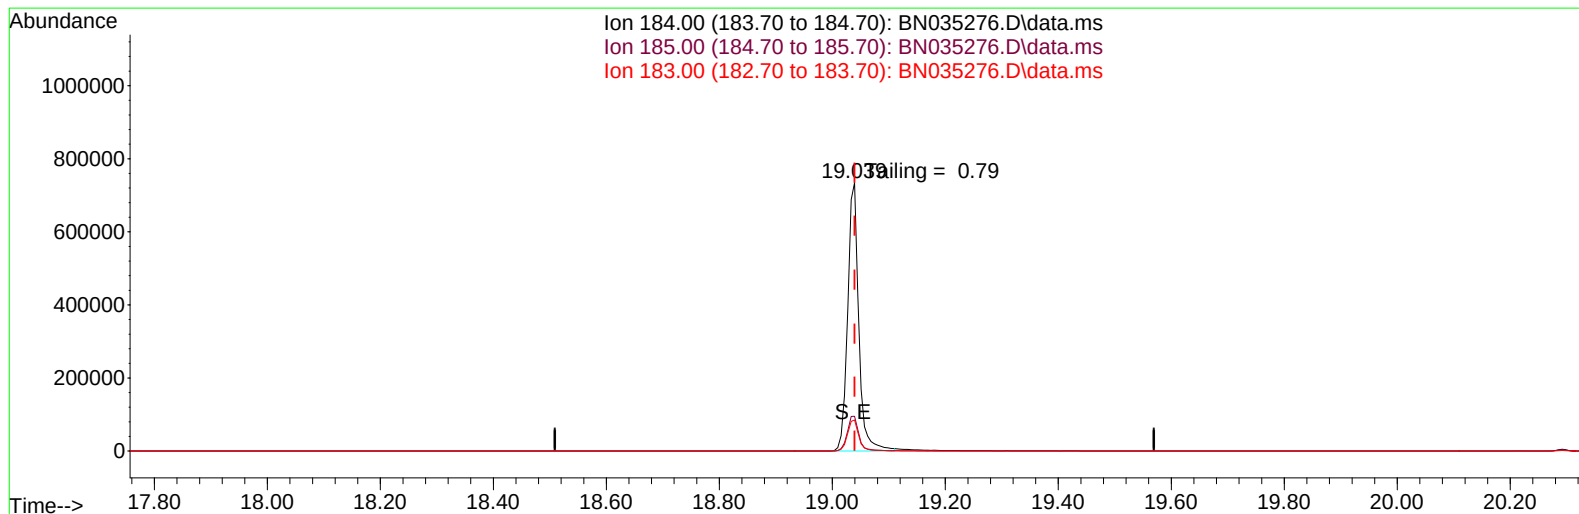

TIC: BN035276.D\data.ms

(77) Benzidine

19.039min (0.000) 0.00 ng

response 1018750

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.97
183.00	13.20	11.60
0.00	0.00	0.00