


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035292.D
Acq On : 25 Nov 2024 20:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 26 02:36:08 2024

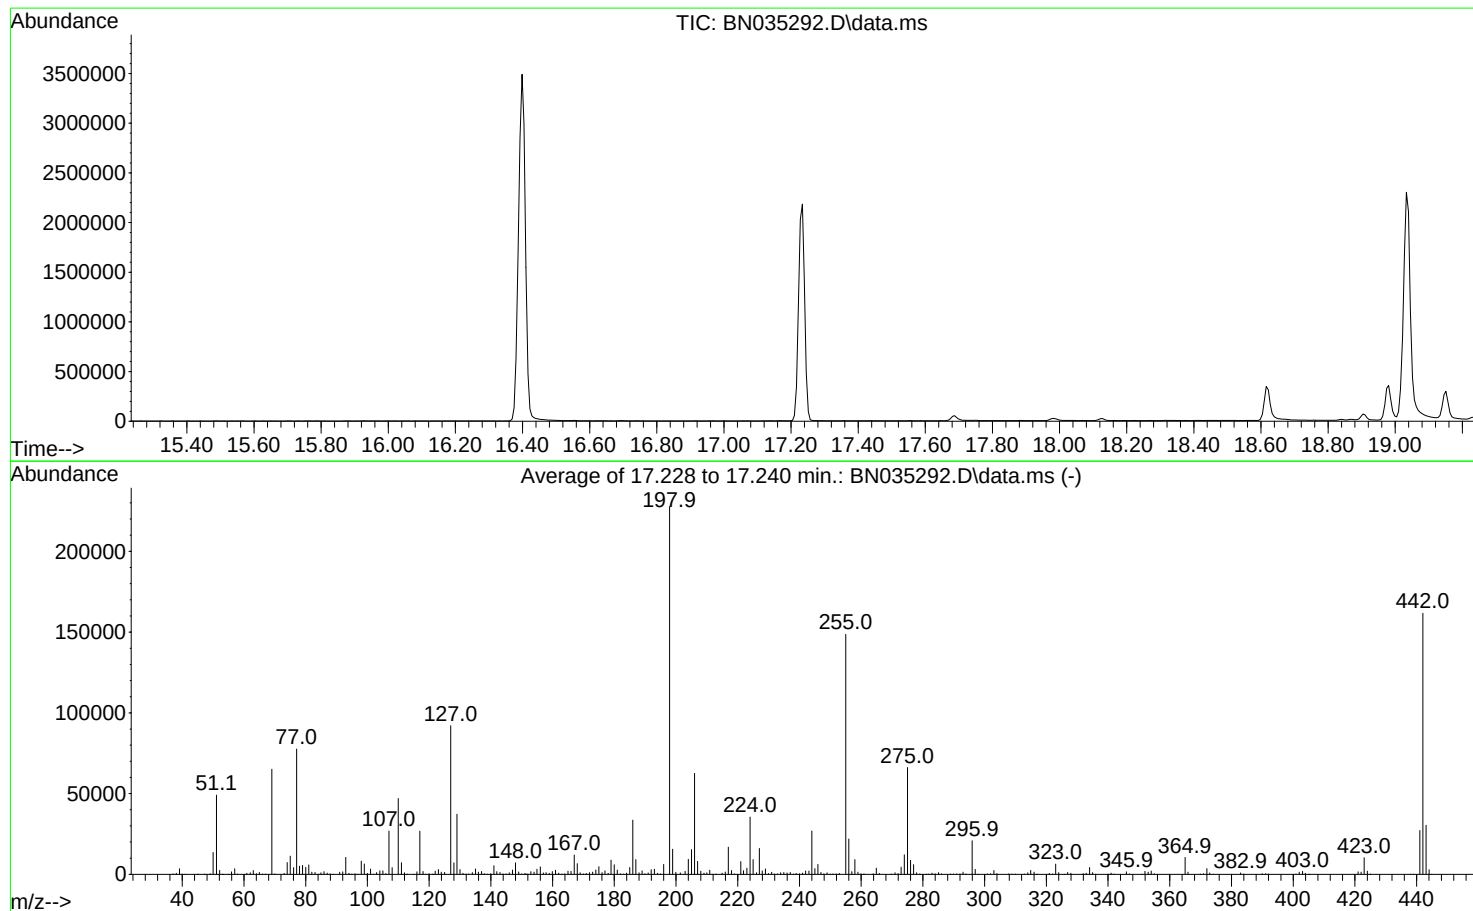

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.5	49032	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.6	65139	PASS
70	69	0.00	2	0.5	305	PASS
127	198	10	80	40.4	92040	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	227755	PASS
199	198	5	9	6.8	15559	PASS
275	198	10	60	29.0	66160	PASS
365	198	1	100	4.6	10457	PASS
441	198	0.01	100	11.9	27155	PASS
442	442	50	100	100.0	161664	PASS
443	442	15	24	18.8	30456	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/25/2024	BNA_N	<u>BN035292.D</u>
Compound Name	Response	Retention Time
DDT	727744	20.292
DDD	34008	19.845
DDE	982	19.328
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34990	762734	4.59

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035292.D
Acq On : 25 Nov 2024 20:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 26 05:22:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:21:56 2024
Response via : Initial Calibration

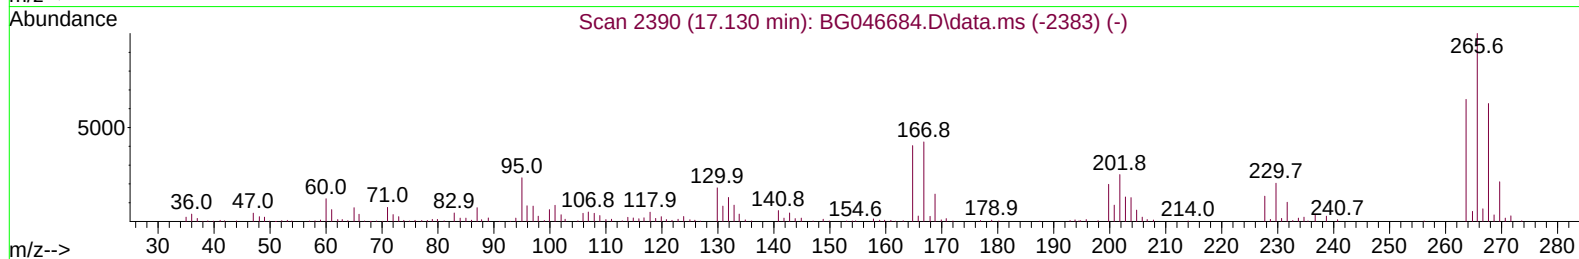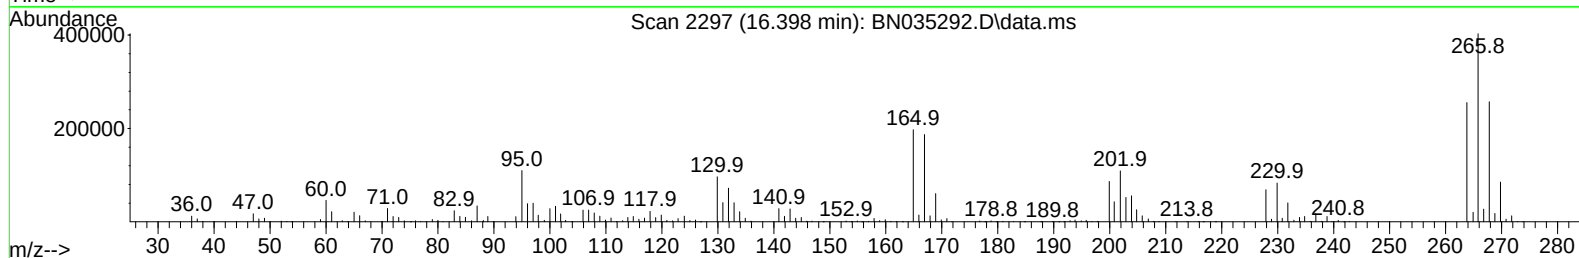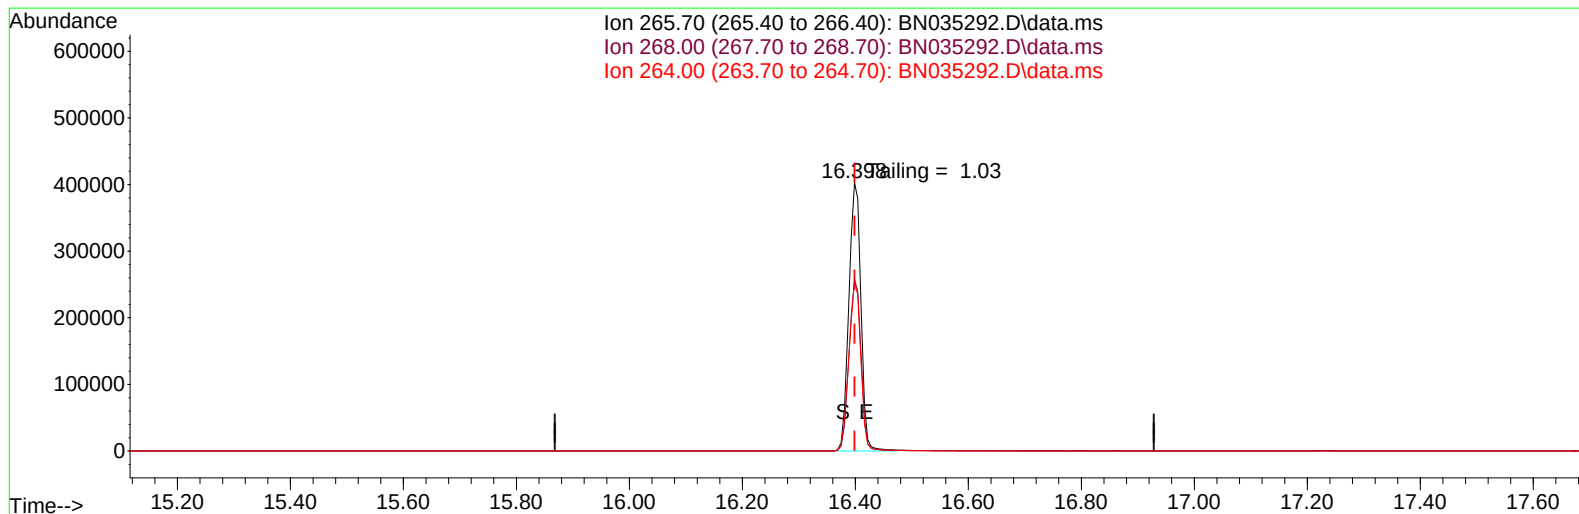

TIC: BN035292.D\data.ms

(70) Pentachlorophenol (C)

16.398min (0.000) 1275879.78 ng




response 600767

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.86
264.00	61.60	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035292.D
Acq On : 25 Nov 2024 20:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 26 05:22:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:21:56 2024
Response via : Initial Calibration

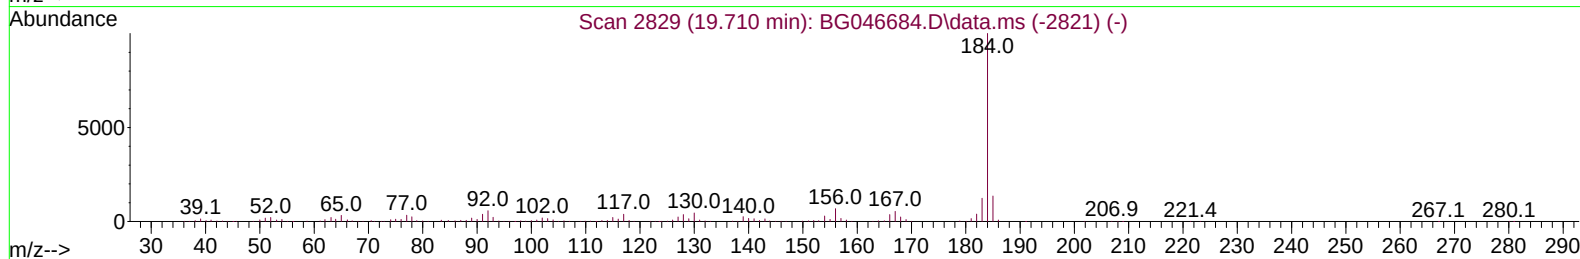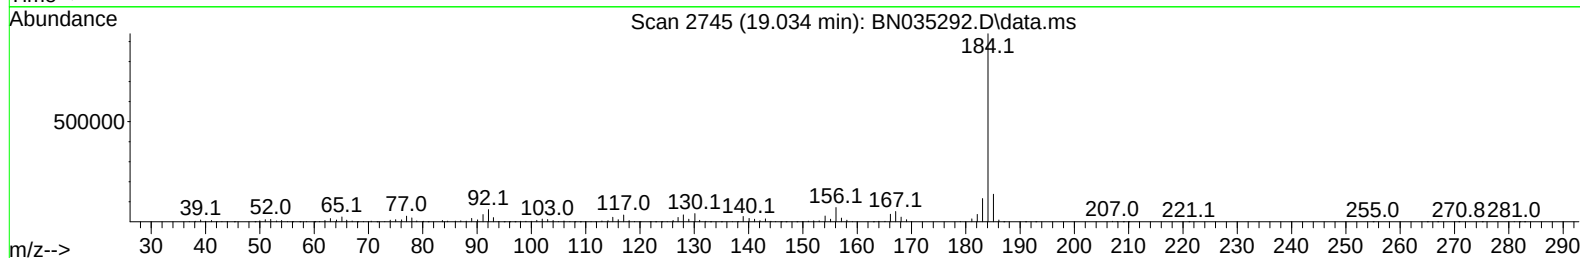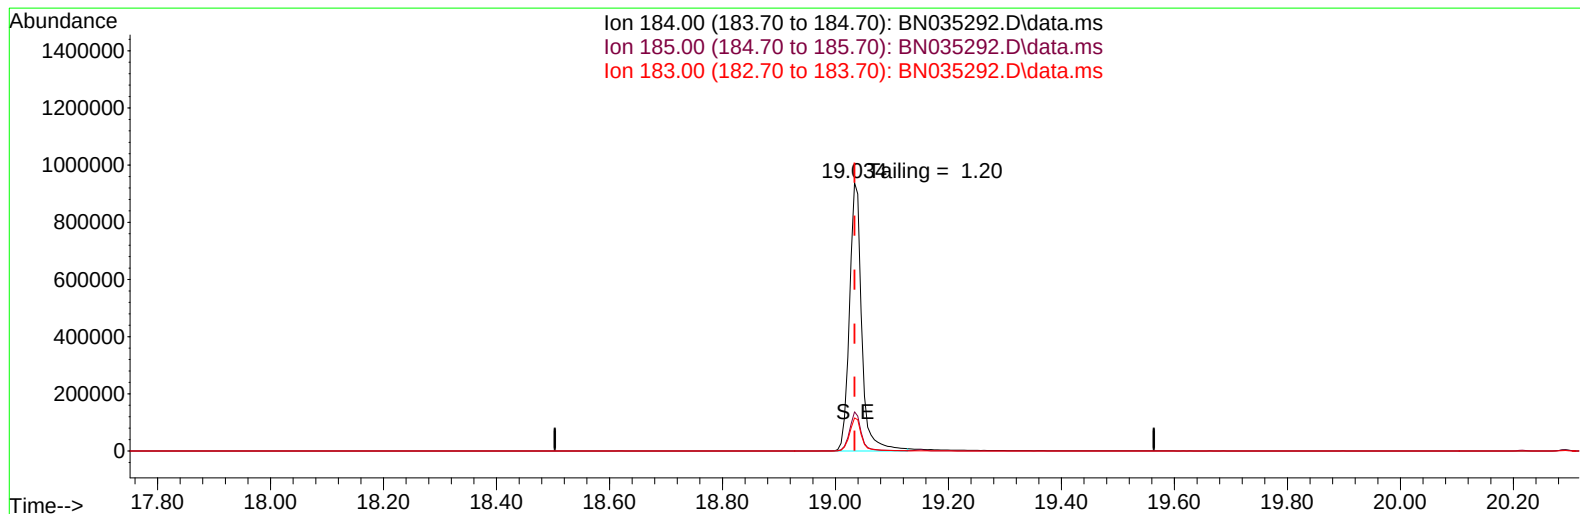

TIC: BN035292.D\data.ms

(77) Benzidine

19.034min (0.000) 201606.82 ng

response 1448003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.64
183.00	13.20	12.37
0.00	0.00	0.00