
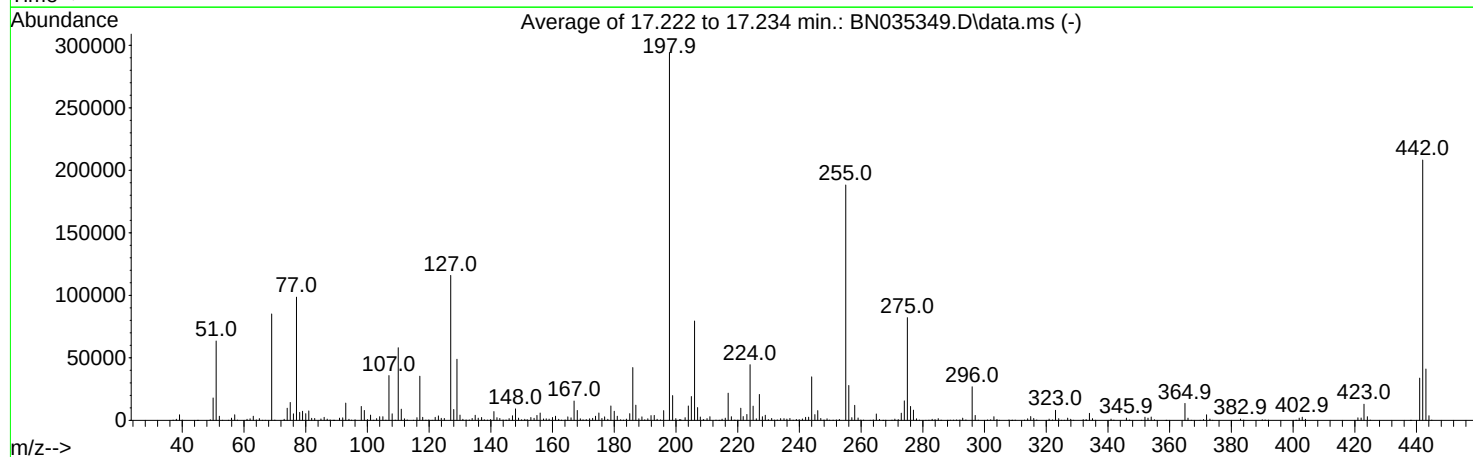


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN112724\  
Data File : BN035349.D  
Acq On : 27 Nov 2024 14:55  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN112724.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Nov 27 23:03:24 2024

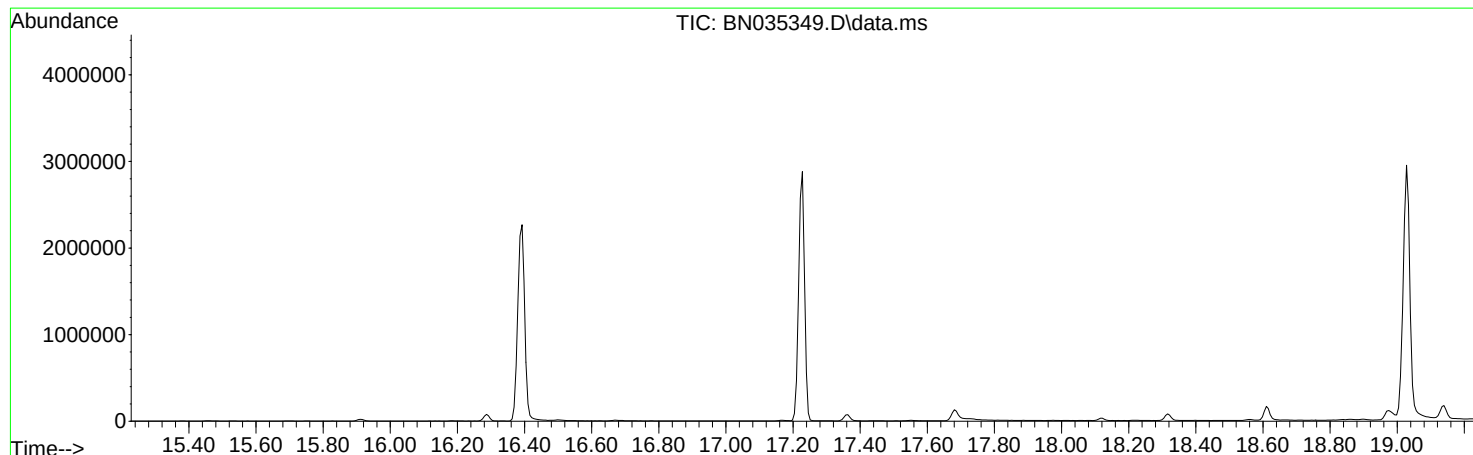

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2430

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 21.6         | 63480      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 28.9         | 85062      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 303        | PASS                |
| 127            | 198             | 10              | 80              | 39.4         | 115899     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 294229     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 19826      | PASS                |
| 275            | 198             | 10              | 60              | 27.9         | 82149      | PASS                |
| 365            | 198             | 1               | 100             | 4.6          | 13565      | PASS                |
| 441            | 198             | 0.01            | 100             | 11.5         | 33811      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 208235     | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 41045      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/27/2024    | BNA_N            | <u>BN035349.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 985457           | 20.286             |
| DDD           | 27636            | 19.839             |
| DDE           | 578              | 19.322             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 28214         | 1013671          | 2.78               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN112724\  
Data File : BN035349.D  
Acq On : 27 Nov 2024 14:55  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Nov 28 04:07:39 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 28 04:07:30 2024  
Response via : Initial Calibration

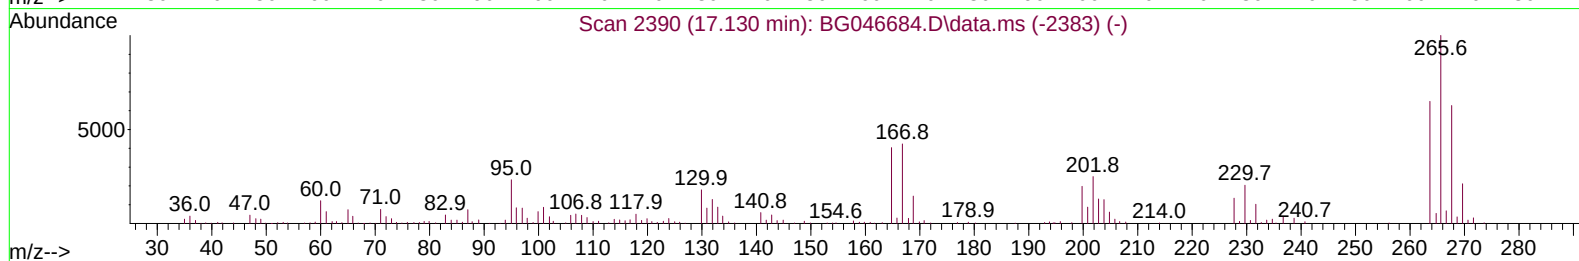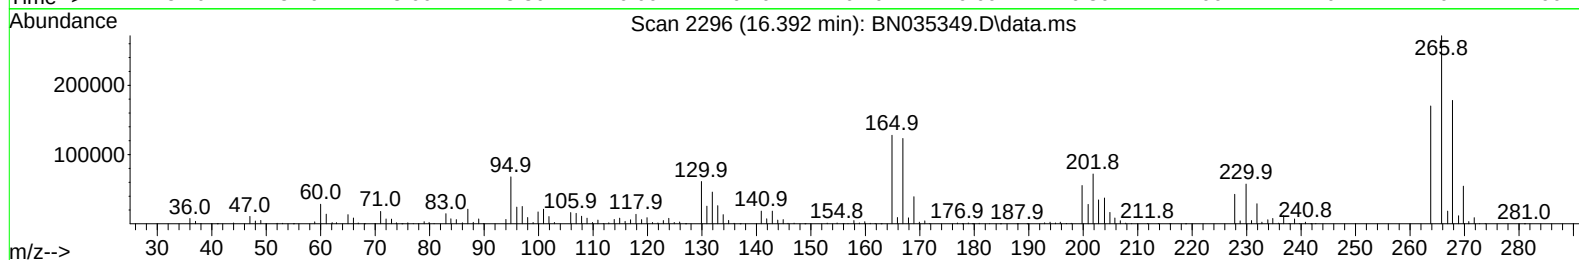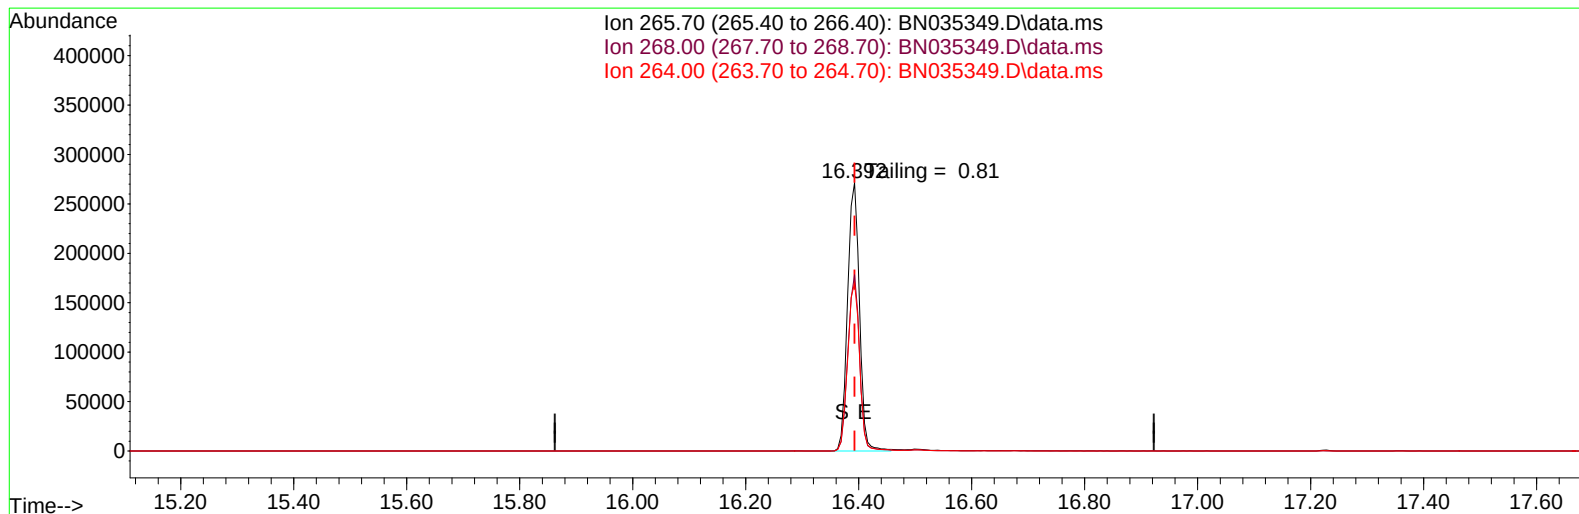

TIC: BN035349.D\data.ms

**(70) Pentachlorophenol (C)**

**16.392min ( 0.000) 27794.31 ng**




**response 398074**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 65.68  |
| 264.00 | 61.60  | 62.66  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN112724\  
Data File : BN035349.D  
Acq On : 27 Nov 2024 14:55  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Nov 28 04:07:39 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 28 04:07:30 2024  
Response via : Initial Calibration

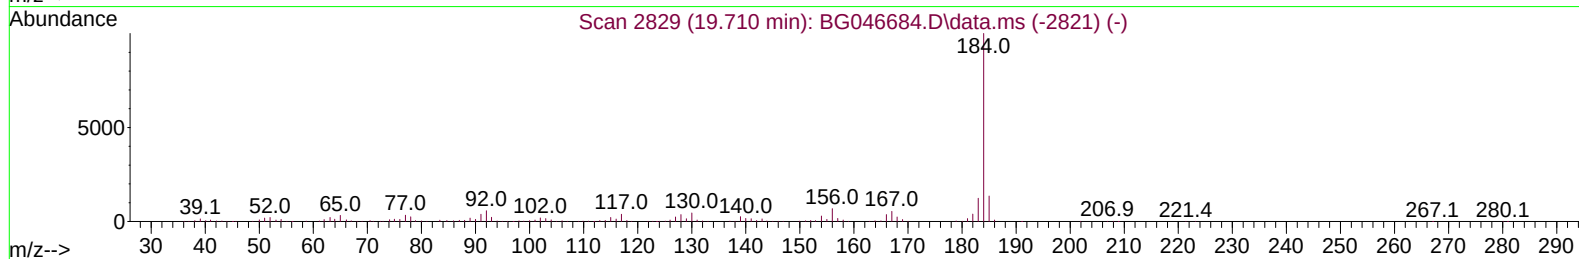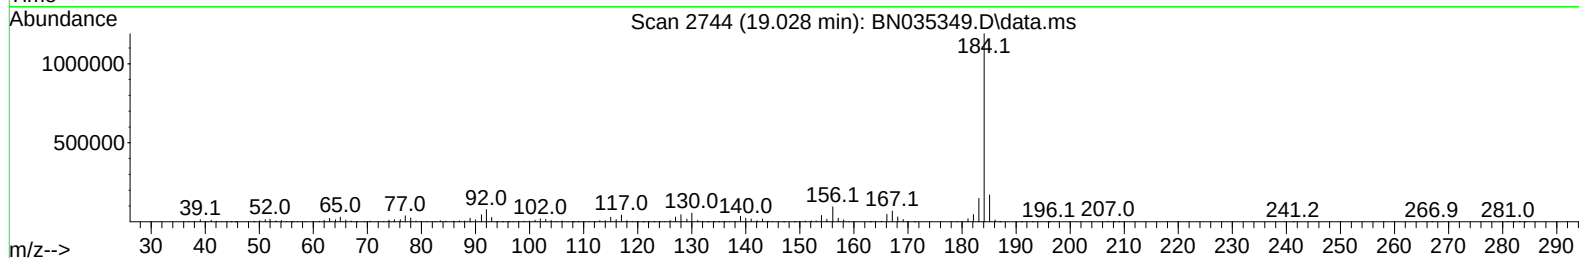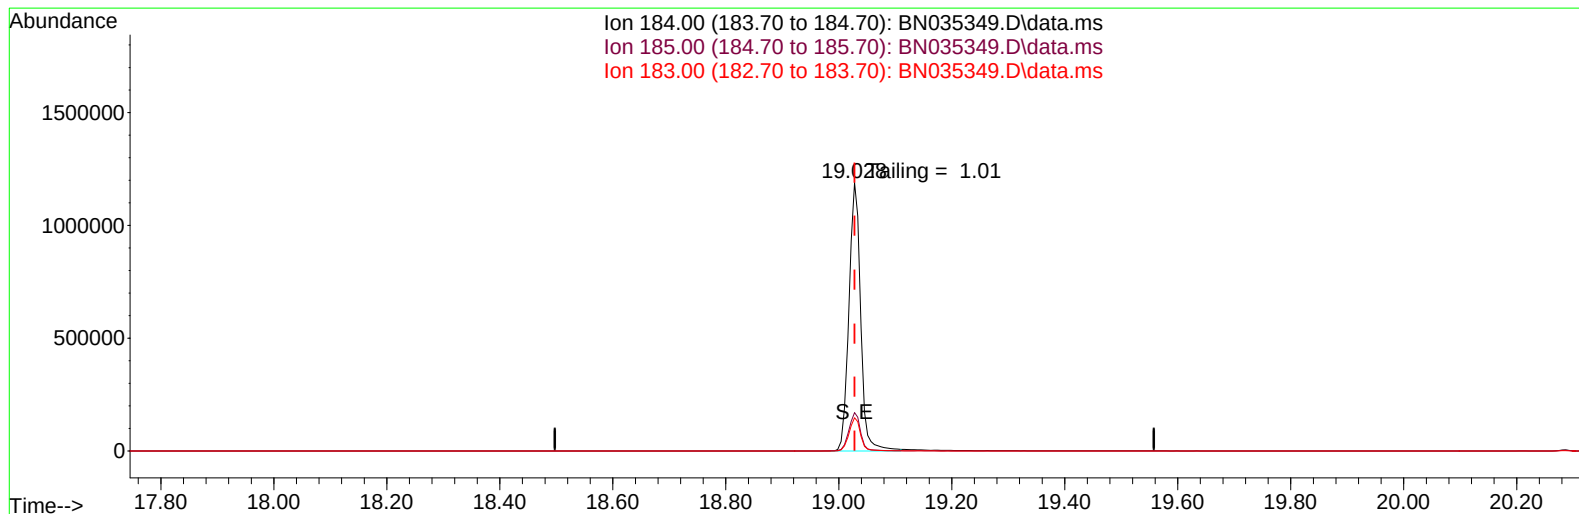

TIC: BN035349.D\data.ms

**(77) Benzidine**

19.028min ( 0.000) 0.00 ng

response 1733630

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.34  |
| 183.00 | 13.20  | 12.42  |
| 0.00   | 0.00   | 0.00   |