


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035349.D
Acq On : 27 Nov 2024 14:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 27 23:03:24 2024

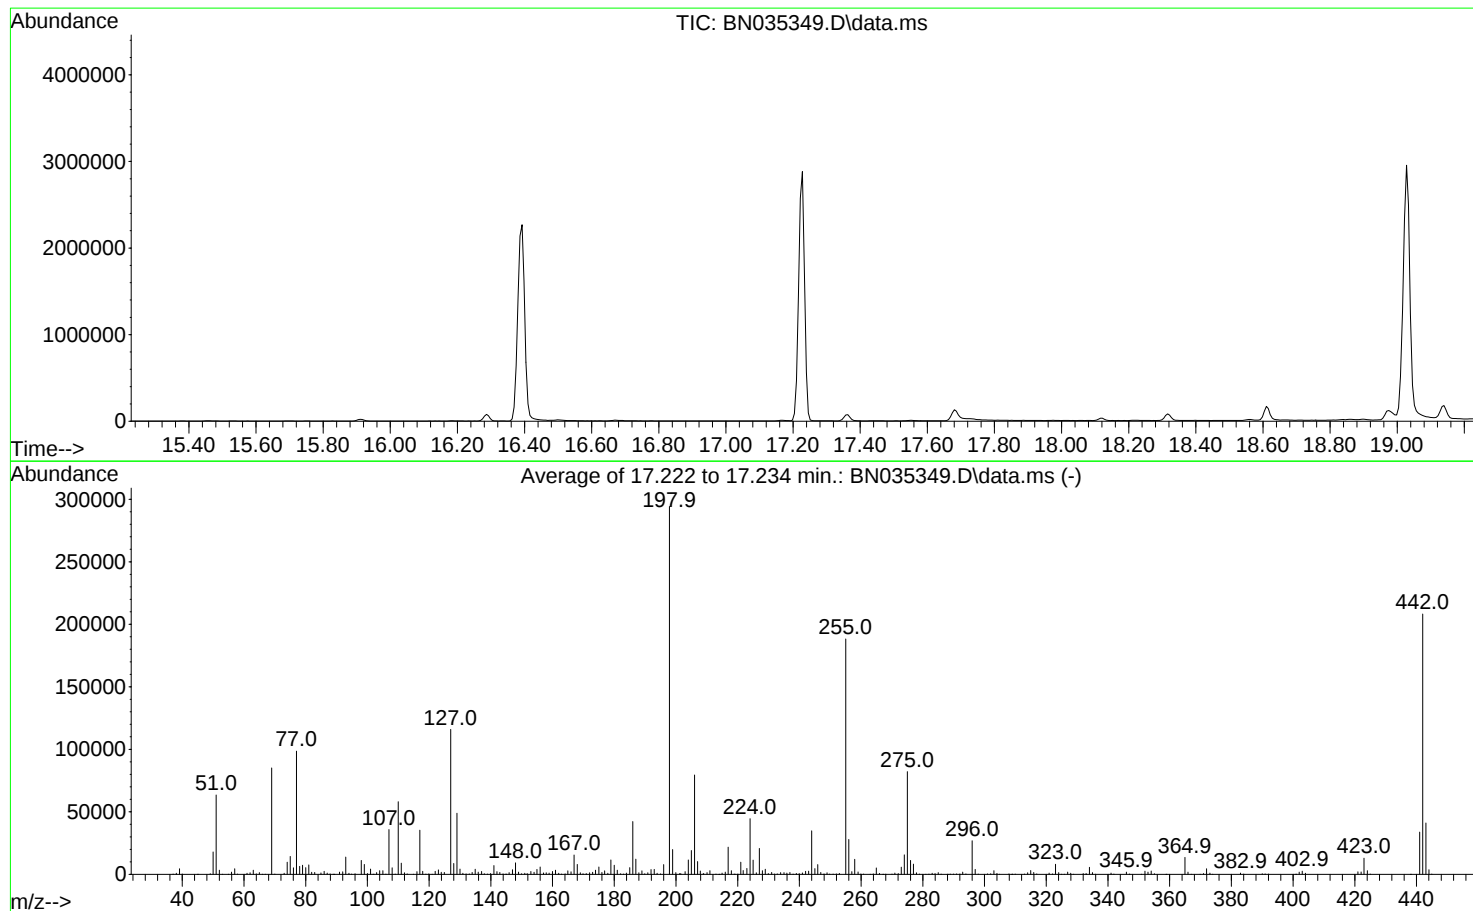

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2430

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.6	63480	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.9	85062	PASS
70	69	0.00	2	0.4	303	PASS
127	198	10	80	39.4	115899	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	294229	PASS
199	198	5	9	6.7	19826	PASS
275	198	10	60	27.9	82149	PASS
365	198	1	100	4.6	13565	PASS
441	198	0.01	100	11.5	33811	PASS
442	442	50	100	100.0	208235	PASS
443	442	15	24	19.7	41045	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/27/2024	BNA_N	<u>BN035349.D</u>
Compound Name	Response	Retention Time
DDT	985457	20.286
DDD	27636	19.839
DDE	578	19.322
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28214	1013671	2.78

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035349.D
Acq On : 27 Nov 2024 14:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 28 04:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 28 04:07:30 2024
Response via : Initial Calibration

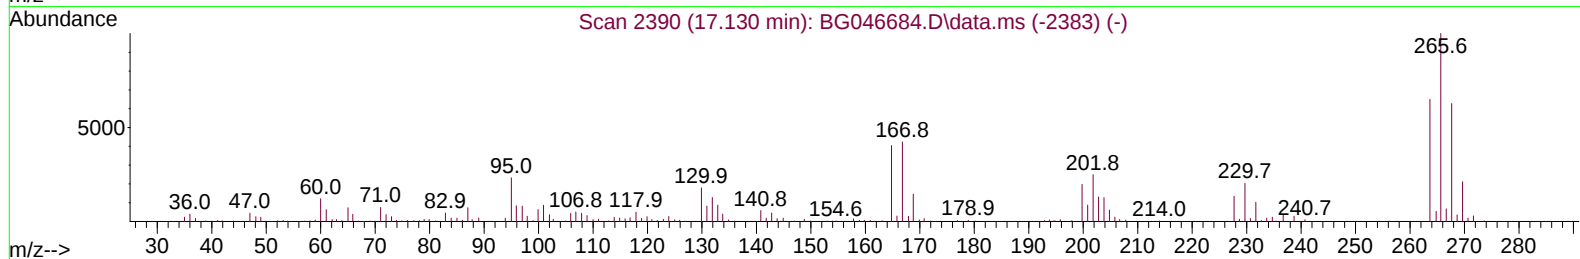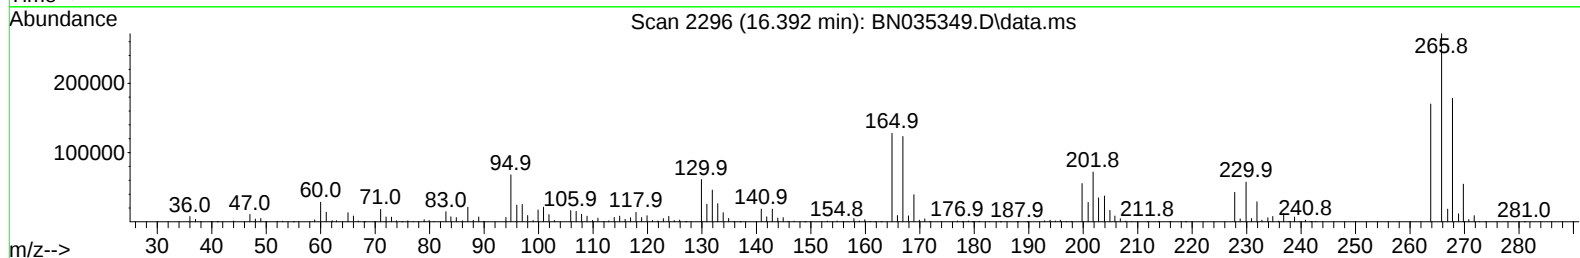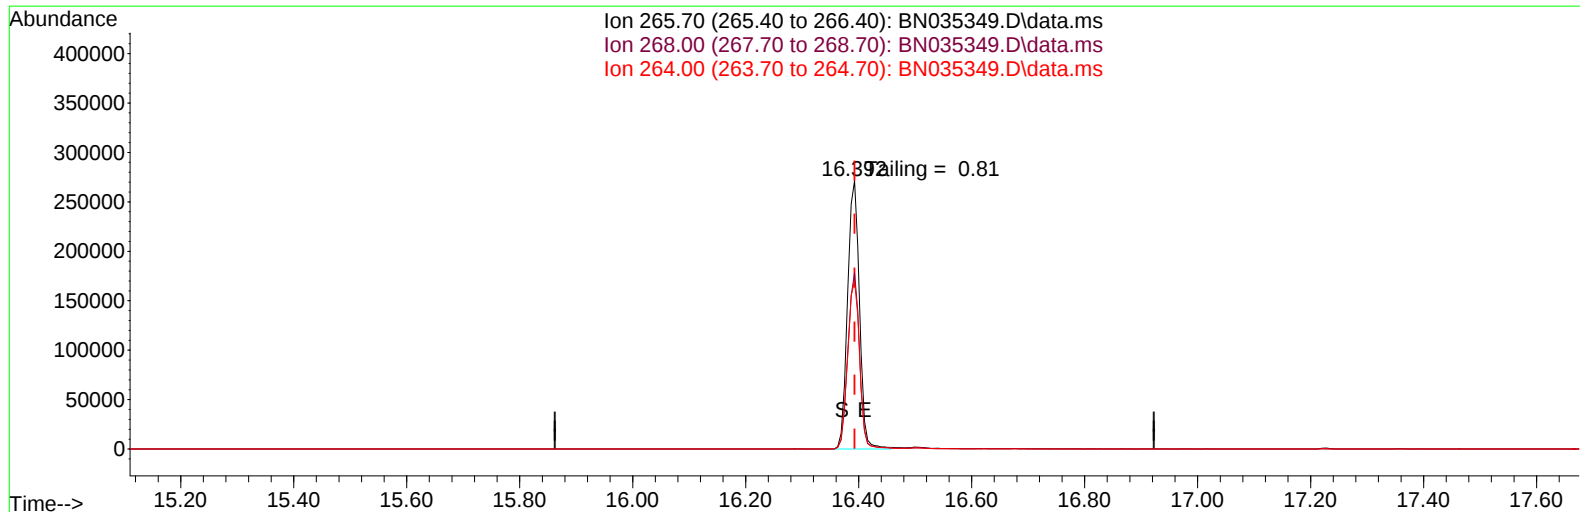

TIC: BN035349.D\data.ms

(70) Pentachlorophenol (C)

16.392min (0.000) 27794.31 ng




response 398074

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.68
264.00	61.60	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035349.D
Acq On : 27 Nov 2024 14:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 28 04:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 28 04:07:30 2024
Response via : Initial Calibration

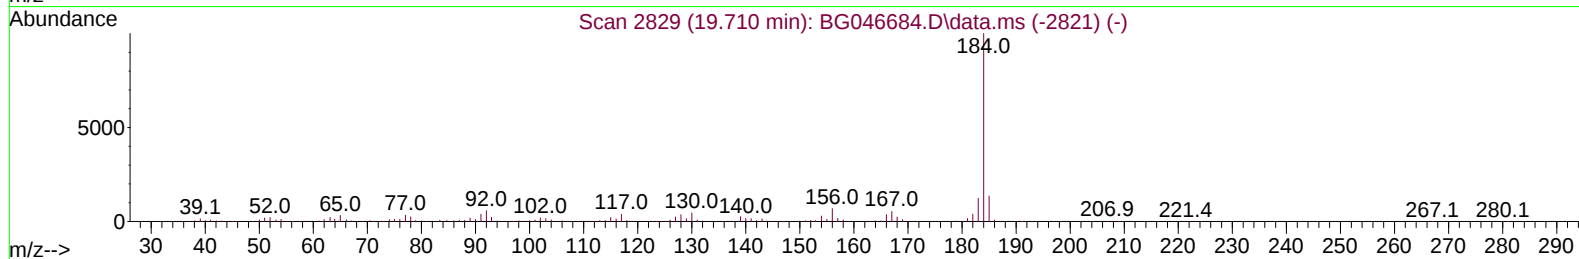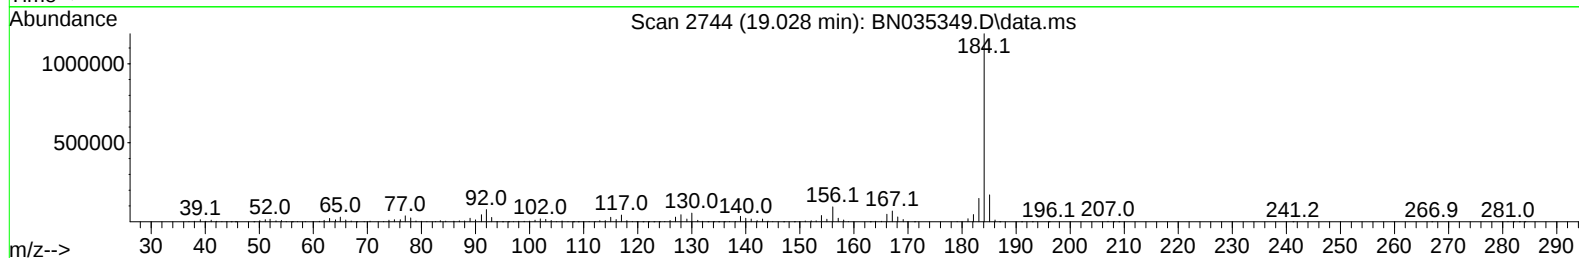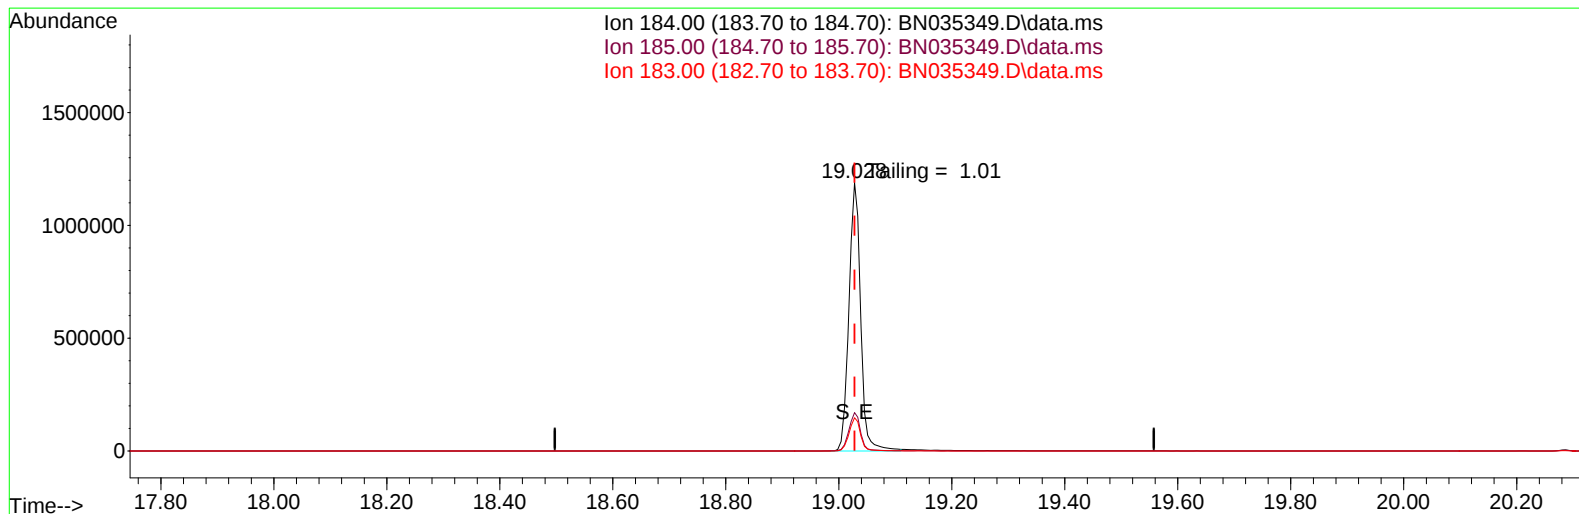

TIC: BN035349.D\data.ms

(77) Benzidine

19.028min (0.000) 0.00 ng

response 1733630

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	12.42
0.00	0.00	0.00