

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
 Data File : BN035297.D
 Acq On : 26 Nov 2024 01:26
 Operator : RC/JU
 Sample : P4959-01
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RW5-SP100-20241121

Quant Time: Nov 26 02:54:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 02:36:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.315	152	3474	0.400	ng	0.00
7) Naphthalene-d8	10.063	136	8594	0.400	ng	# 0.00
13) Acenaphthene-d10	13.973	164	5314	0.400	ng	# 0.00
19) Phenanthrene-d10	16.741	188	12516	0.400	ng	# 0.00
29) Chrysene-d12	21.006	240	912	0.400	ng	# 0.00
35) Perylene-d12	23.078	264	6981	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.968	112	1086	0.165	ng	0.00
5) Phenol-d6	6.521	99	751	0.082	ng	0.00
8) Nitrobenzene-d5	8.451	82	1834	0.263	ng	0.00
11) 2-Methylnaphthalene-d10	11.663	152	5726	0.476	ng	0.00
14) 2,4,6-Tribromophenol	15.480	330	885	0.326	ng	0.00
15) 2-Fluorobiphenyl	12.604	172	1025	0.349	ng	0.00
27) Fluoranthene-d10	18.790	212	16757	0.500	ng	0.00
31) Terphenyl-d14	19.417	244	12231	0.726	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.003	88	28516	11.419	ng	# 70
6) bis(2-Chloroethyl)ether	6.766	93	518	0.067	ng	96
20) 4,6-Dinitro-2-methylph...	15.170	198	6	0.193	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.015	149	531	0.304	ng	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035297.D
Acq On : 26 Nov 2024 01:26
Operator : RC/JU
Sample : P4959-01
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RW5-SP100-20241121


Quant Time: Nov 26 02:54:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 02:36:08 2024
Response via : Initial Calibration

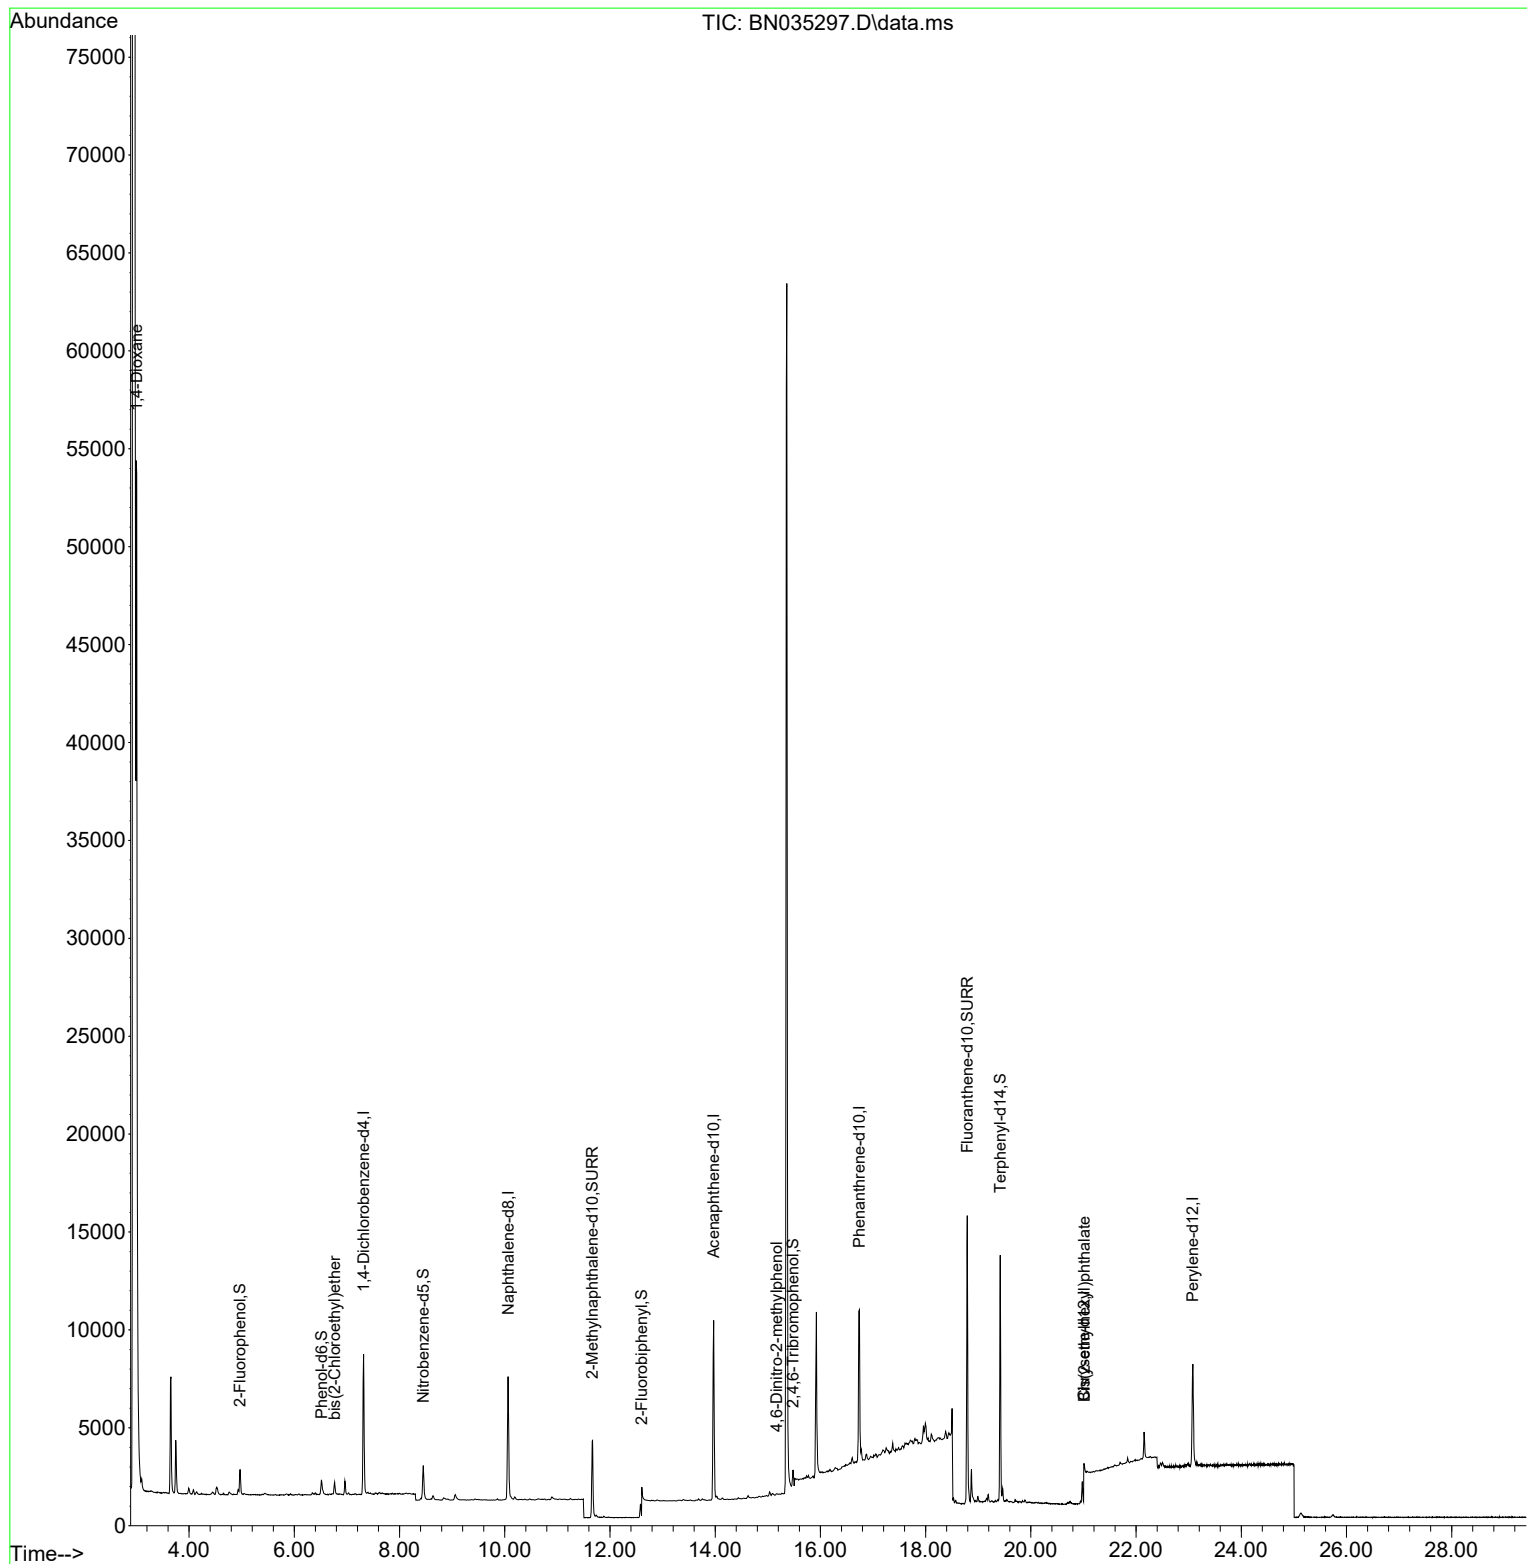






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.315 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN035297.D
 Acq: 26 Nov 2024 01:26

Instrument :
 BNA_N
 ClientSampleId :
 RW5-SP100-20241121



Tgt Ion:152 Resp: 3474




Ion	Ratio	Lower	Upper
152	100		
150	152.5	124.5	186.7
115	58.3	47.8	71.8

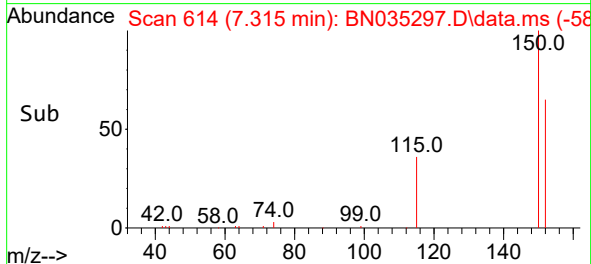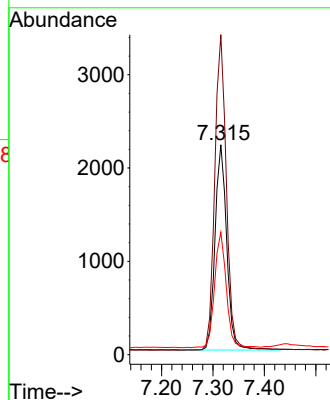


#2
 1,4-Dioxane
 Concen: 11.419 ng
 RT: 3.003 min Scan# 17
 Delta R.T. 0.000 min
 Lab File: BN035297.D
 Acq: 26 Nov 2024 01:26

Tgt Ion: 88 Resp: 28516

Ion	Ratio	Lower	Upper
88	100		
43	19.7	48.1	72.1#
58	53.5	46.9	70.3


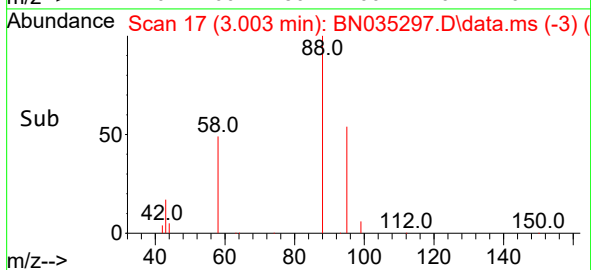
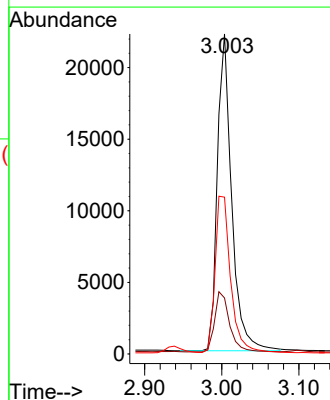
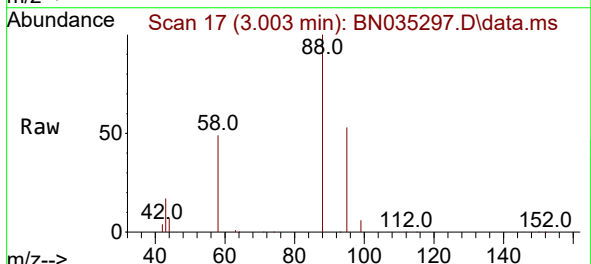




#4
2-Fluorophenol
Concen: 0.165 ng
RT: 4.968 min Scan# 289
Delta R.T. 0.000 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26




Instrument :
BNA_N
ClientSampleId :
RW5-SP100-20241121


Tgt Ion:112 Resp: 1086
Ion Ratio Lower Upper
112 100
64 48.4 40.4 60.6
63 27.0 23.8 35.8

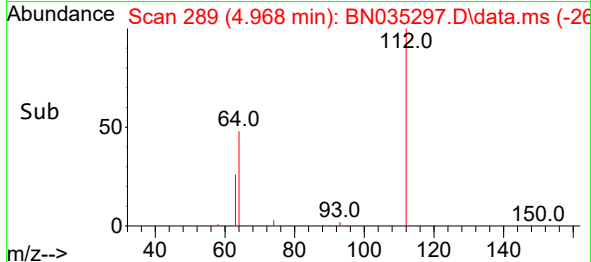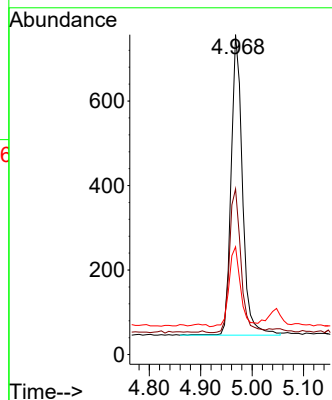

#5
Phenol-d6
Concen: 0.082 ng
RT: 6.521 min Scan# 504
Delta R.T. 0.000 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26

Tgt Ion: 99 Resp: 751
Ion Ratio Lower Upper
99 100
42 16.2 12.8 19.2
71 45.0 31.4 47.2


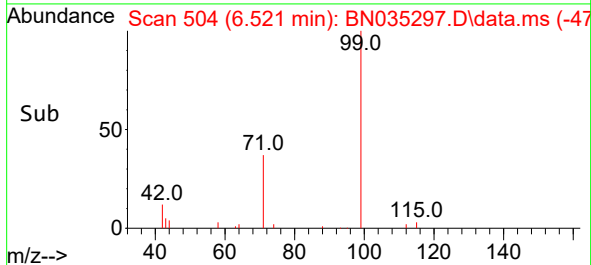
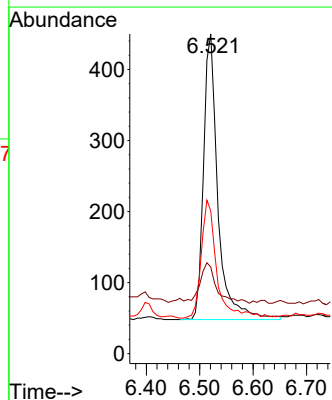
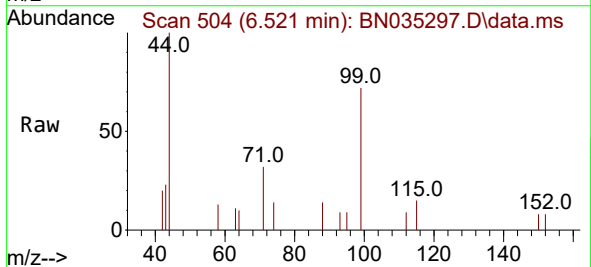




#6
bis(2-Chloroethyl)ether
Concen: 0.067 ng
RT: 6.766 min Scan# 518
Delta R.T. 0.000 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26




Instrument :
BNA_N
ClientSampleId :
RW5-SP100-20241121


Tgt Ion:	93	Resp:	518
Ion	Ratio	Lower	Upper
93	100		
63	60.4	52.3	78.5
95	31.5	25.5	38.3

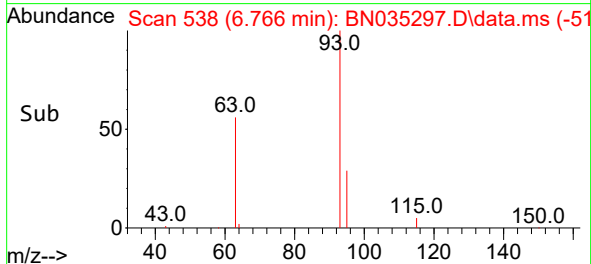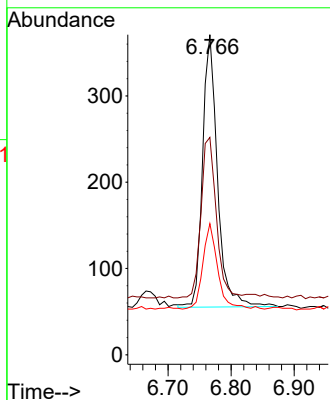

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.063 min Scan# 916
Delta R.T. 0.000 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26

Tgt Ion:	136	Resp:	8594
Ion	Ratio	Lower	Upper
136	100		
137	11.6	9.7	14.5
54	5.1	5.3	7.9#
68	5.7	5.9	8.9#


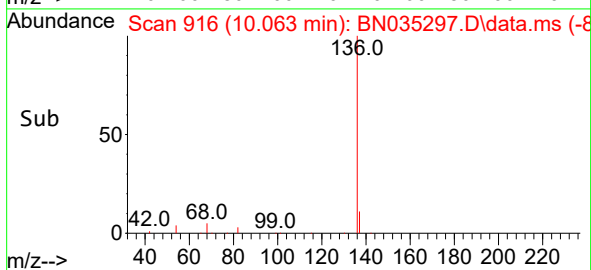
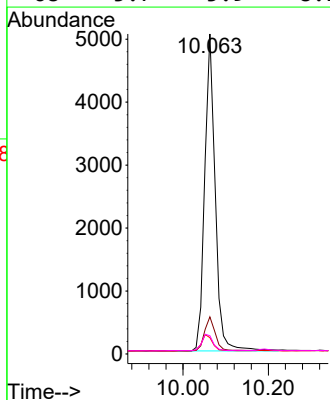
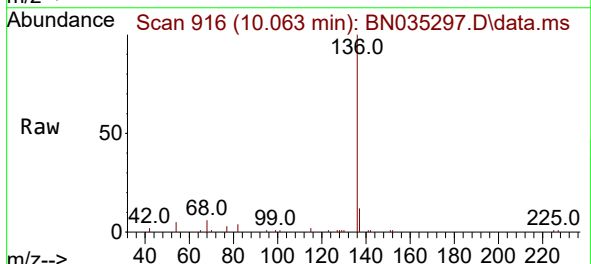




#8
 Nitrobenzene-d5
 Concen: 0.263 ng
 RT: 8.451 min Scan# 765
 Delta R.T. 0.000 min
 Lab File: BN035297.D
 Acq: 26 Nov 2024 01:26




Instrument :
 BNA_N
 ClientSampleId :
 RW5-SP100-20241121


Tgt Ion: 82 Resp: 1834
 Ion Ratio Lower Upper
 82 100
 128 45.9 33.0 49.4
 54 38.0 33.3 49.9

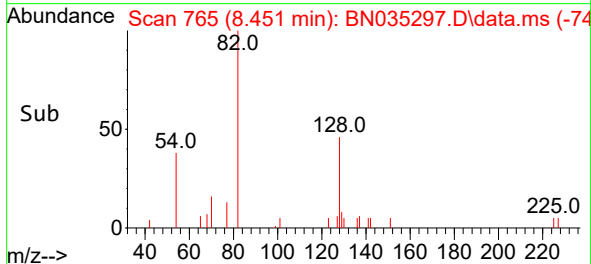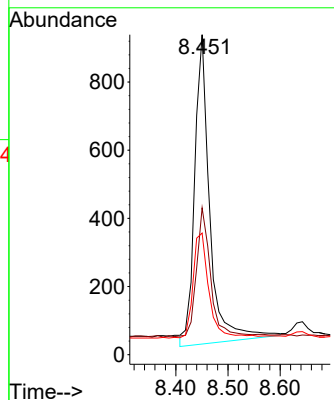

#11
 2-Methylnaphthalene-d10
 Concen: 0.476 ng
 RT: 11.663 min Scan# 1093
 Delta R.T. -0.004 min
 Lab File: BN035297.D
 Acq: 26 Nov 2024 01:26

Tgt Ion: 152 Resp: 5726
 Ion Ratio Lower Upper
 152 100
 151 20.5 17.2 25.8


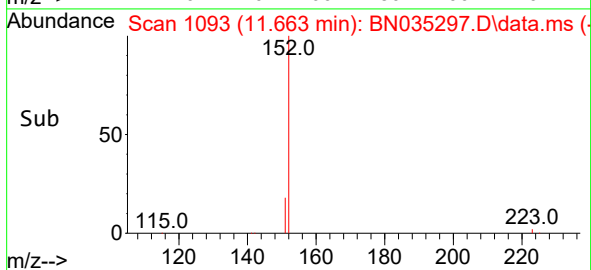
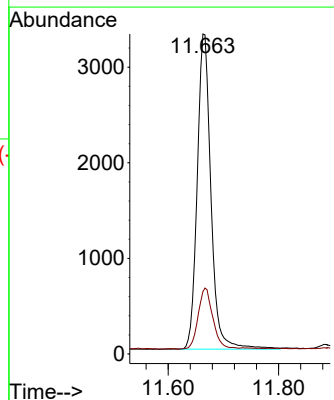
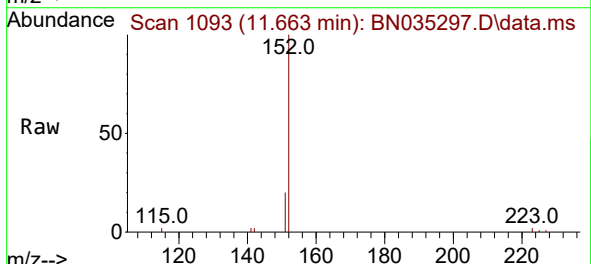




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 13.973 min Scan# 1470
Delta R.T. -0.004 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26




Instrument :
BNA_N
ClientSampleId :
RW5-SP100-20241121


Tgt Ion:164 Resp: 5314
Ion Ratio Lower Upper
164 100
162 103.9 82.0 123.0
160 53.6 63.0 94.4#

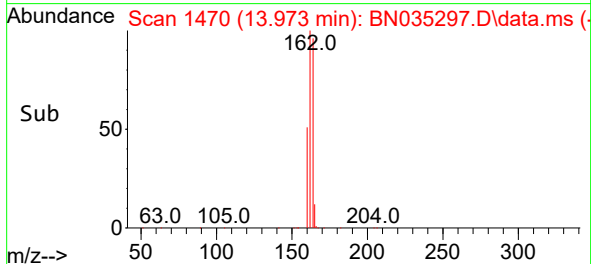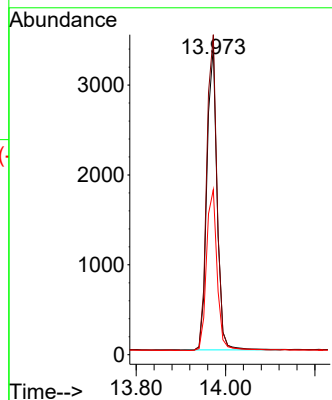

#14
2,4,6-Tribromophenol
Concen: 0.326 ng
RT: 15.480 min Scan# 1611
Delta R.T. -0.004 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26

Tgt Ion:330 Resp: 885
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.4 32.4 48.6


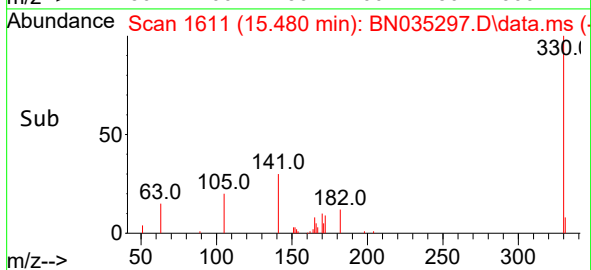
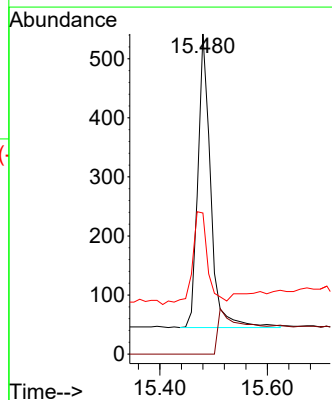
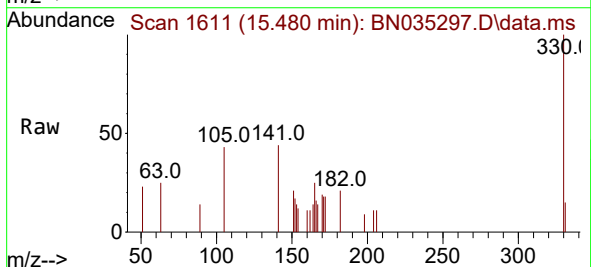




#15
2-Fluorobiphenyl
Concen: 0.349 ng
RT: 12.604 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26




Instrument :
BNA_N
ClientSampleId :
RW5-SP100-20241121


Tgt Ion:172 Resp: 1025
Ion Ratio Lower Upper
172 100
171 39.4 36.6 55.0
170 28.8 29.7 44.5#

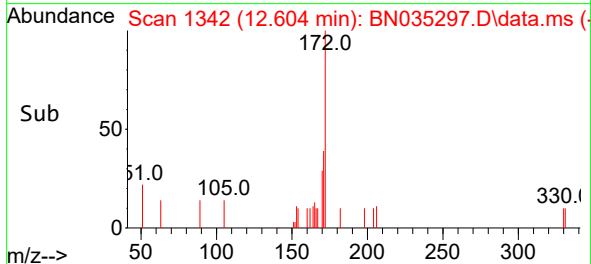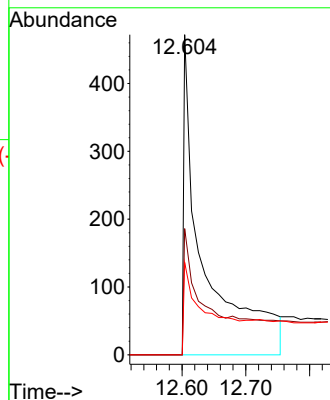

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.741 min Scan# 1713
Delta R.T. 0.007 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26

Tgt Ion:188 Resp: 12516
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.8 8.9 13.3#


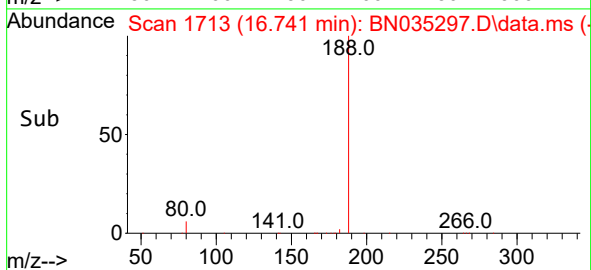
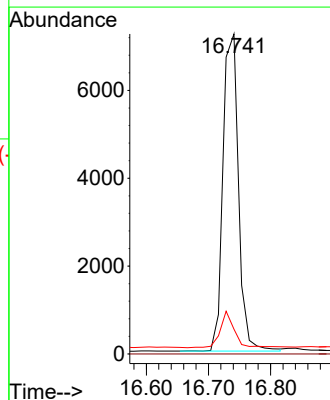
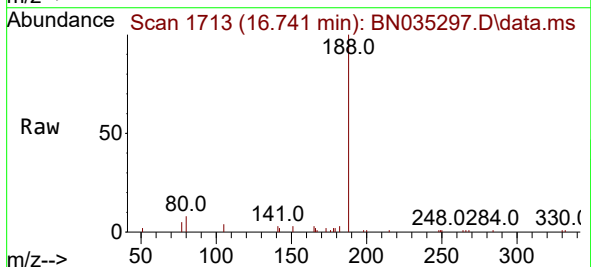




#20
4,6-Dinitro-2-methylphenol
Concen: 0.193 ng
RT: 15.170 min Scan# 1582
Delta R.T. 0.039 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26




Instrument :
BNA_N
ClientSampleId :
RW5-SP100-20241121


Tgt Ion:198 Resp: 6
Ion Ratio Lower Upper
198 100
51 214.0 53.6 80.4#
105 252.0 47.4 71.2#

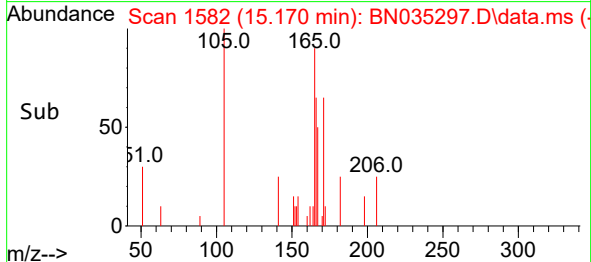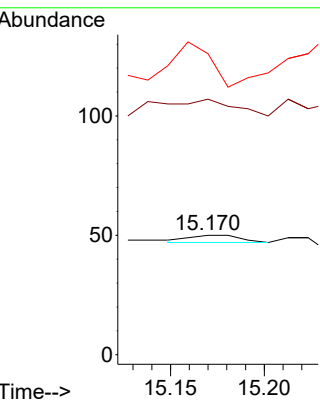

#27
Fluoranthene-d10
Concen: 0.500 ng
RT: 18.790 min Scan# 1915
Delta R.T. -0.002 min
Lab File: BN035297.D
Acq: 26 Nov 2024 01:26

Tgt Ion:212 Resp: 16757
Ion Ratio Lower Upper
212 100
106 11.8 9.8 14.8
104 6.4 5.6 8.4

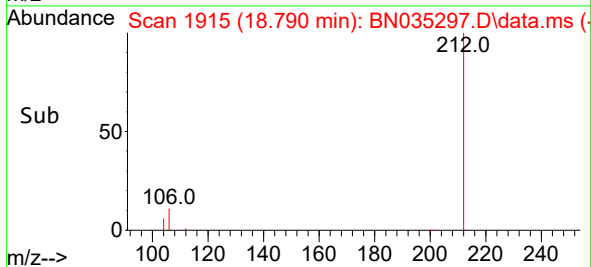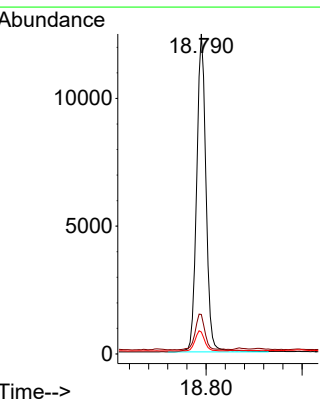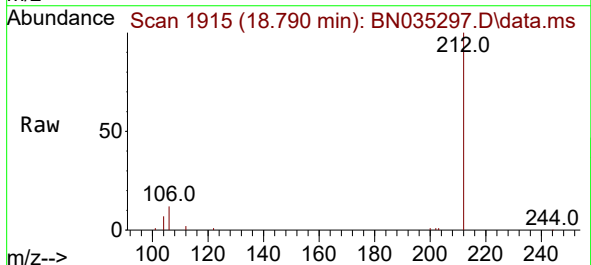

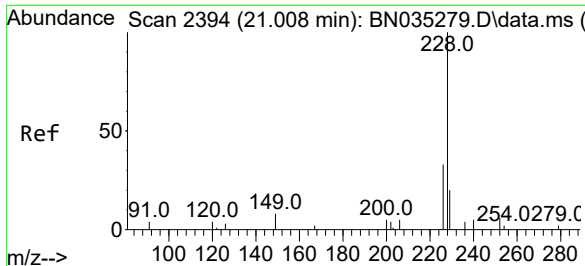

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.006 min Scan# 21

Delta R.T. -0.002 min

Lab File: BN035297.D

Acq: 26 Nov 2024 01:26

Instrument :

BNA_N

ClientSampleId :

RW5-SP100-20241121





Tgt Ion:240 Resp: 912

Ion Ratio Lower Upper

240 100

120 65.6 54.9 82.3

236 50.7 54.0 81.0#

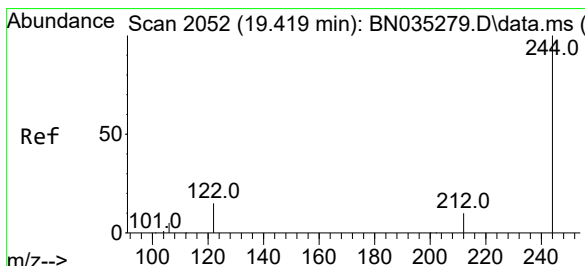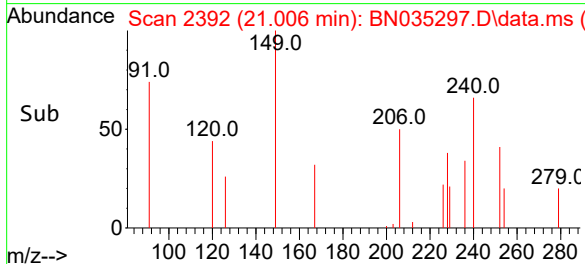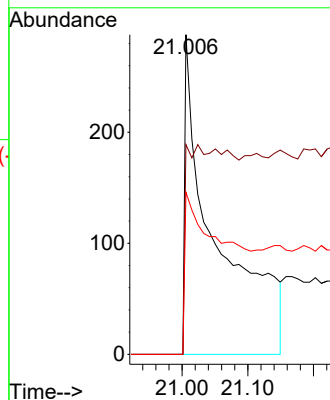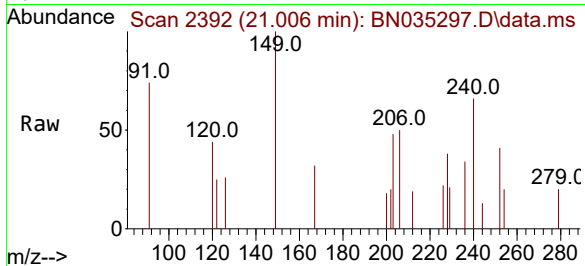

#31

Terphenyl-d14

Concen: 0.726 ng

RT: 19.417 min Scan# 2050

Delta R.T. -0.002 min

Lab File: BN035297.D

Acq: 26 Nov 2024 01:26




Tgt Ion:244 Resp: 12231


Ion Ratio Lower Upper

244 100

212 10.0 9.4 14.0

122 13.7 13.0 19.4


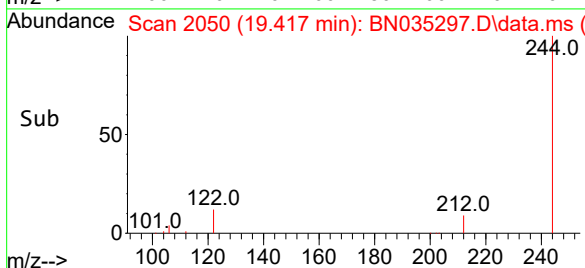
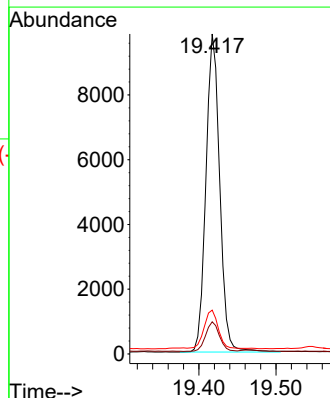
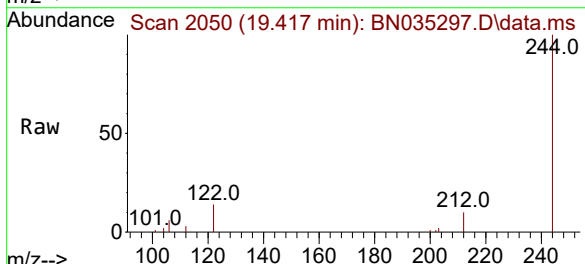


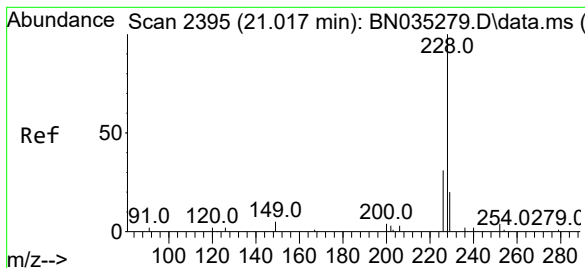

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.304 ng
 RT: 21.015 min Scan# 2100
 Delta R.T. -0.002 min
 Lab File: BN035297.D
 Acq: 26 Nov 2024 01:26

Instrument :
 BNA_N
 ClientSampleId :
 RW5-SP100-20241121

Tgt Ion:149 Resp: 531
 Ion Ratio Lower Upper
 149 100
 167 56.5 0.0 0.0#
 279 0.0 13.0 19.6#

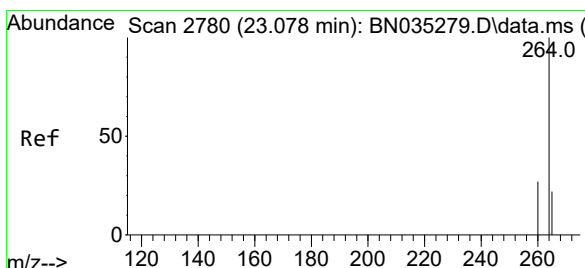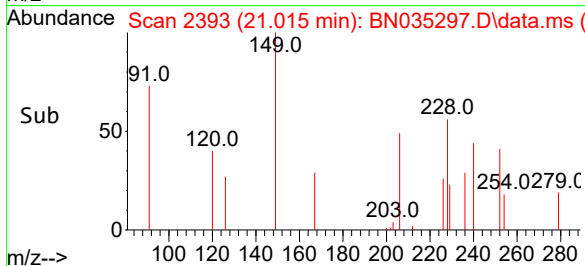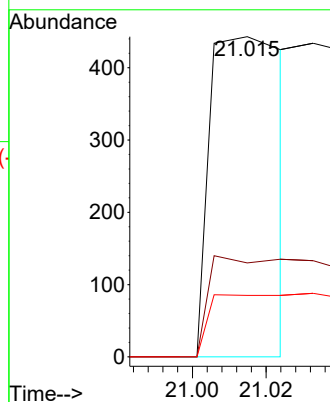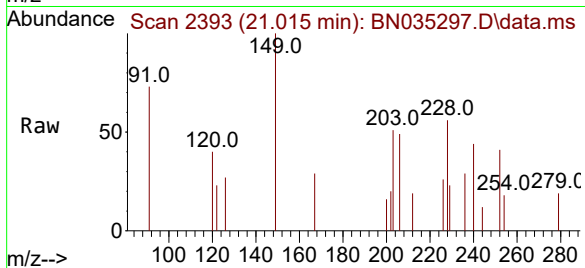

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.078 min Scan# 2779
 Delta R.T. 0.001 min
 Lab File: BN035297.D
 Acq: 26 Nov 2024 01:26

Tgt Ion:264 Resp: 6981
 Ion Ratio Lower Upper
 264 100
 260 27.5 22.3 33.5
 265 73.4 68.6 103.0

