				Reviewed By: On: Inst Id :Konelab 20 LB 133703
Test results		Aquakem 7	.2AQ1	Page:
		CHEMTECH 284 Sheff	CONSULTING Gield Street,	ROUP INC Mountainside, NJ 07092
12/3/2024 10:0	)5	Reviewed	by : <u>RM</u>	Instrument ID : Konelab
Test: TKN-NH3				
Sample Id	Result	Dil. 1 +	Response	Errors
ICV1 ICB1 CCV1 CCB1 RL CHECK PB165319BL PB165319BS P5006-18 CCV2 CCB2	4.693 -0.056 5.047 -0.054 0.427 -0.065 4.635 0.898 4.886 -0.058	0.0 0.0 0.0 0.0 0.0 0.0 0.0	0.609 0.032 0.651 0.032 0.091 0.031 0.601 0.148 0.632 0.032	85% (Sc-150) 12/03/2024 RM
N Mean SD CV%	10 2.035 2.4137 118.59			

Aquakem v. 7.2AQ1


Results from time period: Tue Dec 03 09:08:33 2024

Tue Dec 03 10:04:15 2024

Sample Id	Sam/Ctr/	c/Test short	r Test type	Result	Result unit	Result date and time	Stat
0.0PPM	А	TKN-NH3	Ρ	-0.054		12/3/2024 9:08:33	
0.5PPM	А	TKN-NH3	Р	0.4668	-	12/3/2024 9:08:34	
1.0PPM	А	TKN-NH3	Р	0.9924	mg/l	12/3/2024 9:08:35	
2.5PPM	А	TKN-NH3	Ρ	2.493		12/3/2024 9:08:36	
5.0PPM	А	TKN-NH3	Ρ	5.0483	mg/l	12/3/2024 9:08:37	
6.7PPM	А	TKN-NH3	Р	6.887	mg/l	12/3/2024 9:08:38	
10.0PPM	А	TKN-NH3	Р	9.8331	mg/l	12/3/2024 9:08:39	
ICV1	S	TKN-NH3	Р	4.6933	mg/l	12/3/2024 9:54:33	
ICB1	S	TKN-NH3	Ρ	-0.0559	mg/l	12/3/2024 9:54:35	
CCV1	S	TKN-NH3	Р	5.0467	mg/l	12/3/2024 9:54:37	
CCB1	S	TKN-NH3	Р	-0.0538	mg/l	12/3/2024 9:54:38	
RL CHECK	S	TKN-NH3	Р	0.4273	mg/l	12/3/2024 9:54:41	
PB165319BL	S	TKN-NH3	Р	-0.0654	ng/l	12/3/2024 9:54:42	
PB165319BS	S	TKN-NH3	Р	4.6351 r	ng/l	12/3/2024 10:04:07	
	S	TKN-NH3	Р	0.8983 r	ng/l	12/3/2024 10:04:08	
	S	TKN-NH3	Р	4.8863 r	ng/l	12/3/2024 10:04:10	
CCB2	S	TKN-NH3	Р	-0.0582 r	ng/l	12/3/2024 10:04:13	

			Reviewed By: On: Inst Id :Konelab 20 ====================================
Calibration result	IS	Aquakem 7.2AQ1	Page:
		CHEMTECH CONSULTING GROUP INC 284 Sheffield Street, Mountains:	ide, NJ 07092
12/3/2024 9:15		Reviewed by : <u><u><u>R</u>M</u> Instrum</u>	ment ID : Konelab
Test TKN-NH3			
Accepted	12/3/20	24 9:15	
Factor Bias	8.241 0.039		
Coeff. of det.	0.999001	1	

Errors

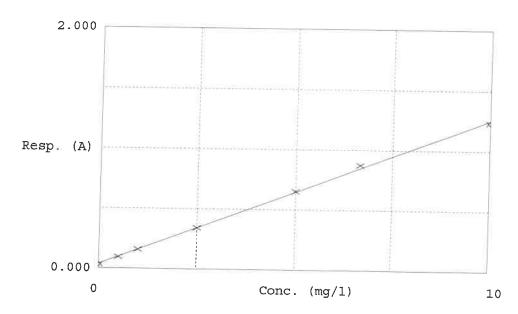

	Calibrator	Response	Calc. con.	Conc.	Lé Errors
1 2 3 4 5 6 7	0.00PPM TKN-10 TKN-10 TKN-10 TKN-10 TKN-10 TKN-10	0.032 0.096 0.159 0.342 0.652 0.875 1.232	-0.0540 0.4668 0.9924 2.4930 5.0483 6.8870 9.8331	0.0000 0.5000 1.0000 2.5000 5.0000 6.6667 10.0000	-6.6 -0.8 -0.3 1.0 2.8 -1.7

12/03/2024 RM